

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
 Data File : PS010098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2020 16:29
 Operator : DD\AJ
 Sample : PB128626BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 17:28:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.238	6.920	287.8E6	265.8E6	476.569	536.608
Target Compounds							
2) T	3,5-DICHL...	0.000	6.072	0	754491	N.D.	1.016
5) T	DICAMBA	0.000	7.088	0	1300817	N.D.	<MDL
6) T	MCP	0.000	7.204	0	798227	N.D.	<MDL
10) T	Pentachlo...	0.000	8.441	0	1905234	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.802	0	2096747	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	2417824	N.D.	<MDL
14) T	DINOSEB	0.000	10.024	0	1093147	N.D.	<MDL
15) T	Picloram	11.037	11.005	50226417	63017885	16.212	18.528
16) T	DCPA	0.000	10.951	0	6990306	N.D.	2.085



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
Data File : PS010098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2020 16:29
Operator : DD\AJ
Sample : PB128626BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 17:28:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

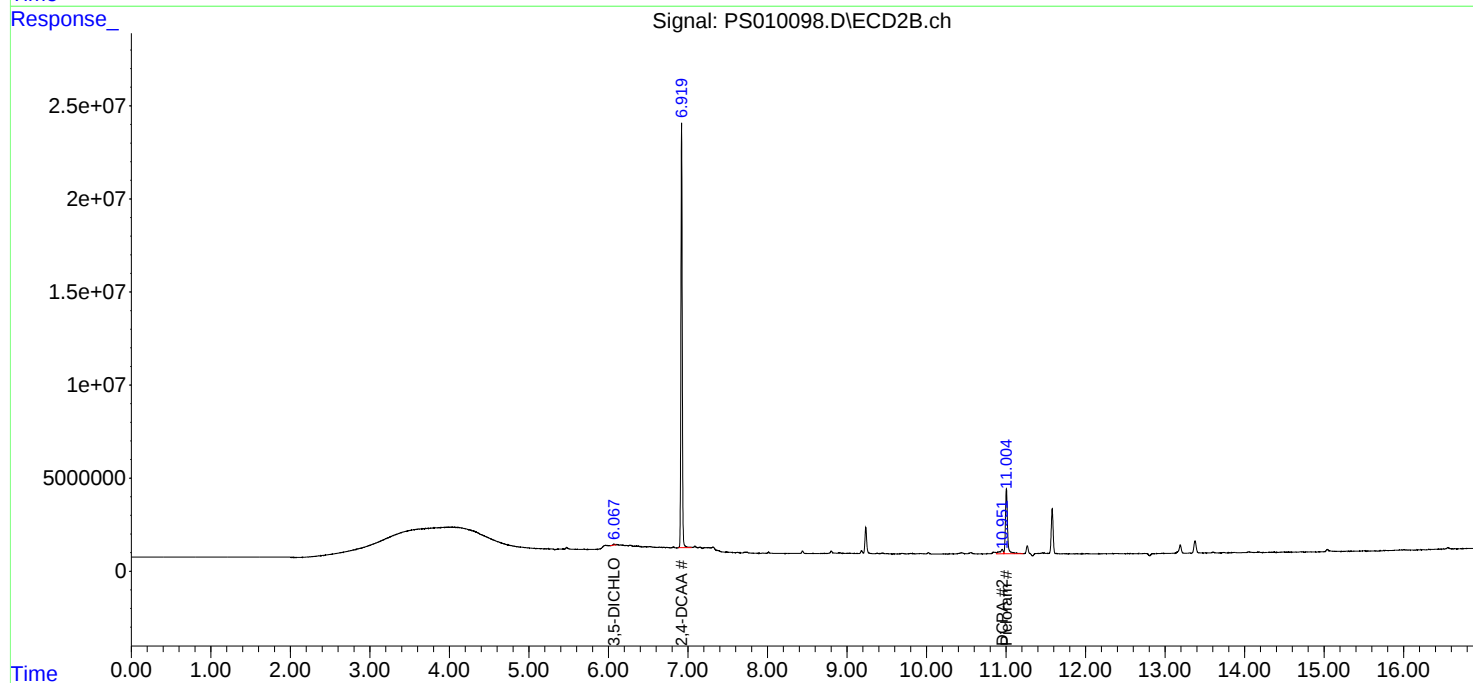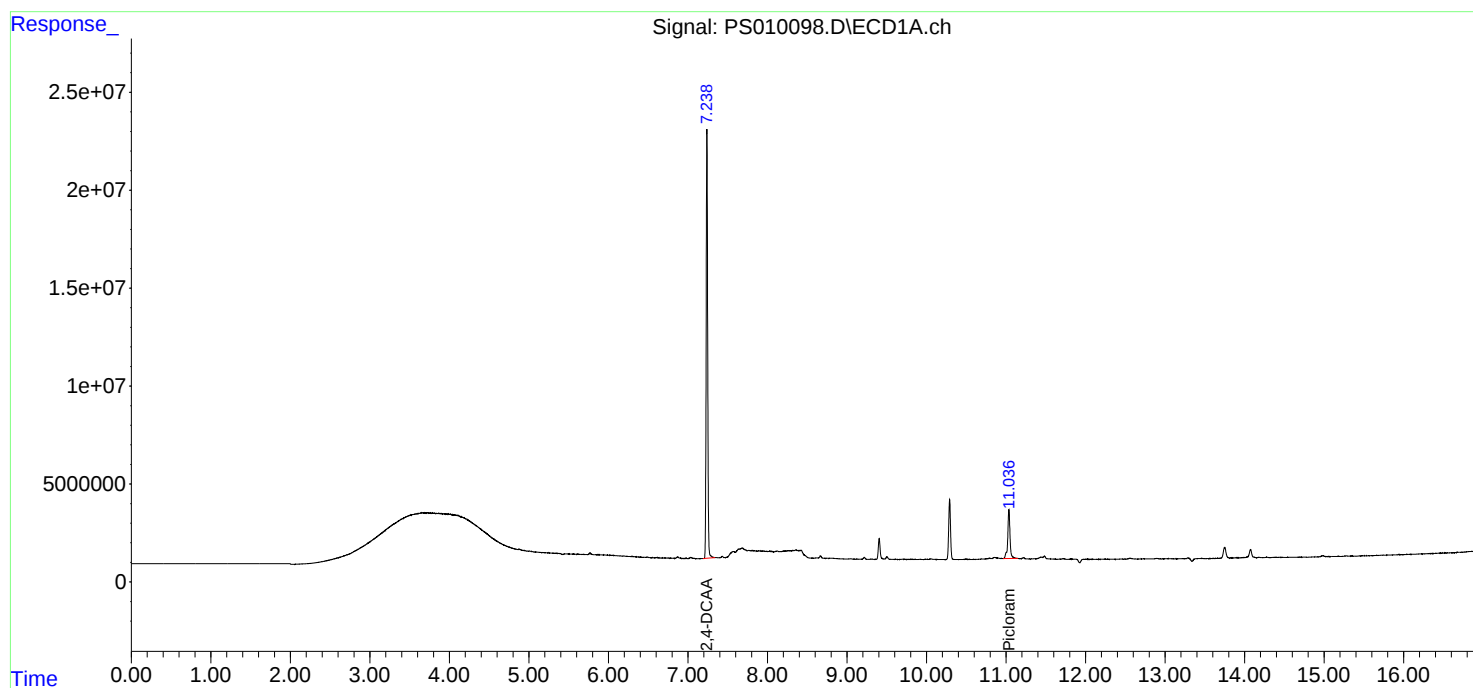


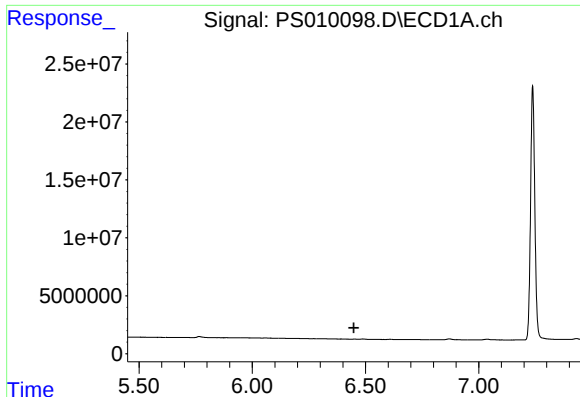

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

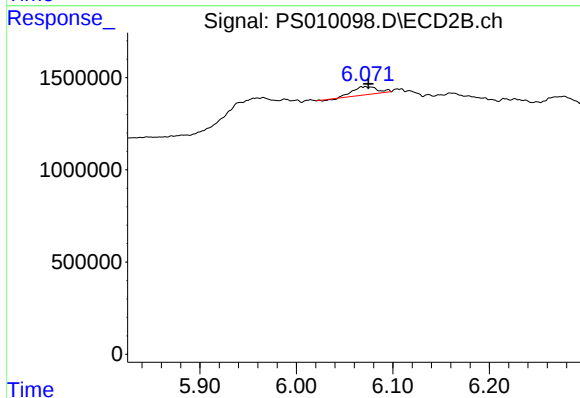


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.072 min
Delta R.T.: -0.003 min
Response: 754491
Conc: 1.02 ng/ml

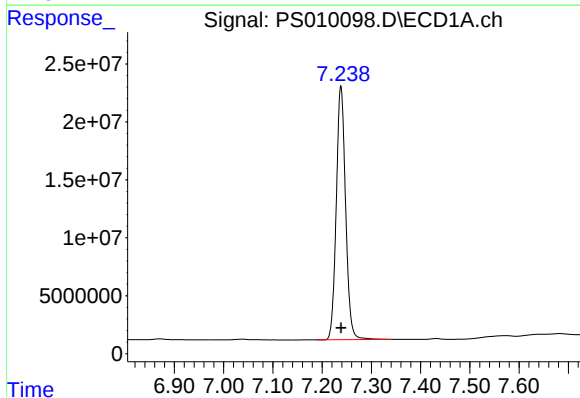


#4 2,4-DCAA

R.T.: 7.238 min
Delta R.T.: 0.000 min
Response: 287759472
Conc: 476.57 ng/ml

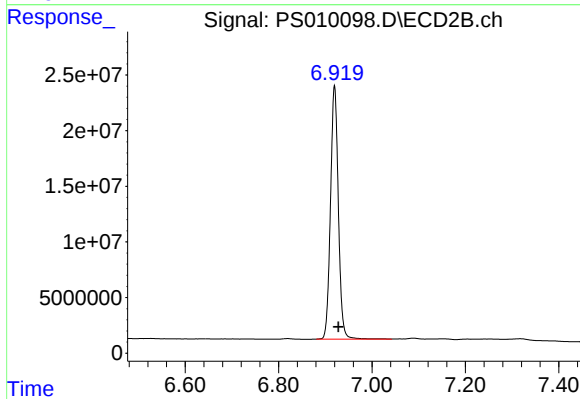

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.008 min
Response: 265755082
Conc: 536.61 ng/ml

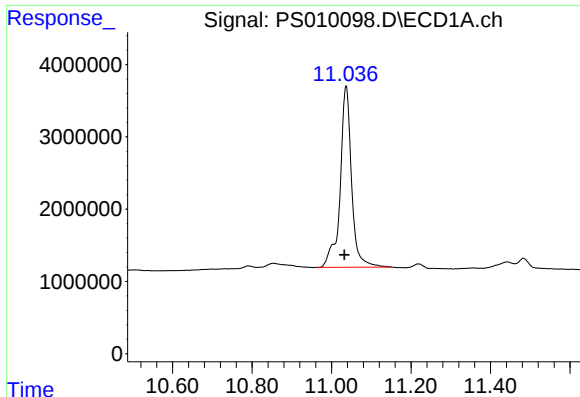

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.004 min
Response: 50226417
Conc: 16.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

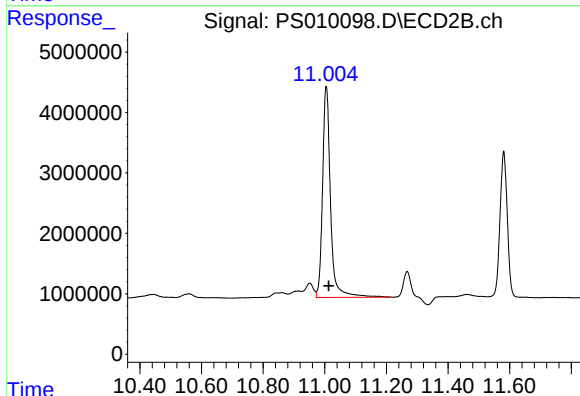


#15 Picloram

R.T.: 11.005 min
Delta R.T.: -0.008 min
Response: 63017885
Conc: 18.53 ng/ml

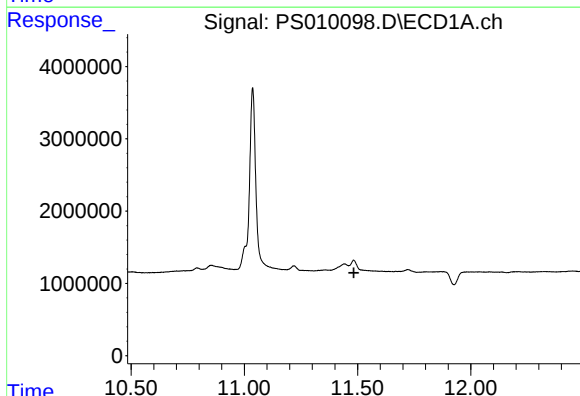

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.484 min
Response: 0
Conc: N.D.

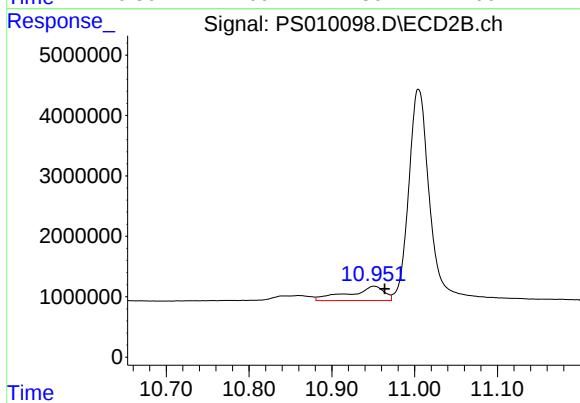

#16 DCPA

R.T.: 10.951 min
Delta R.T.: -0.013 min
Response: 6990306
Conc: 2.08 ng/ml