

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
 Data File : PS010120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2020 00:55
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 03:49:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.921	294.1E6	275.9E6	487.024	557.030
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	1157227	N.D.	<MDL
6) T	MCP	0.000	7.154	0	1162458	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.743	0	2096188	N.D.	4.165
10) T	Pentachlo...	0.000	8.442	0	1607736	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	1611019	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	1812552	N.D.	<MDL
14) T	DINOSEB	0.000	10.023	0	765644	N.D.	<MDL
15) T	Picloram	0.000	11.008	0	5288030	N.D.	1.555
16) T	DCPA	0.000	10.952	0	2469254	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
Data File : PS010120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2020 00:55
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 03:49:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

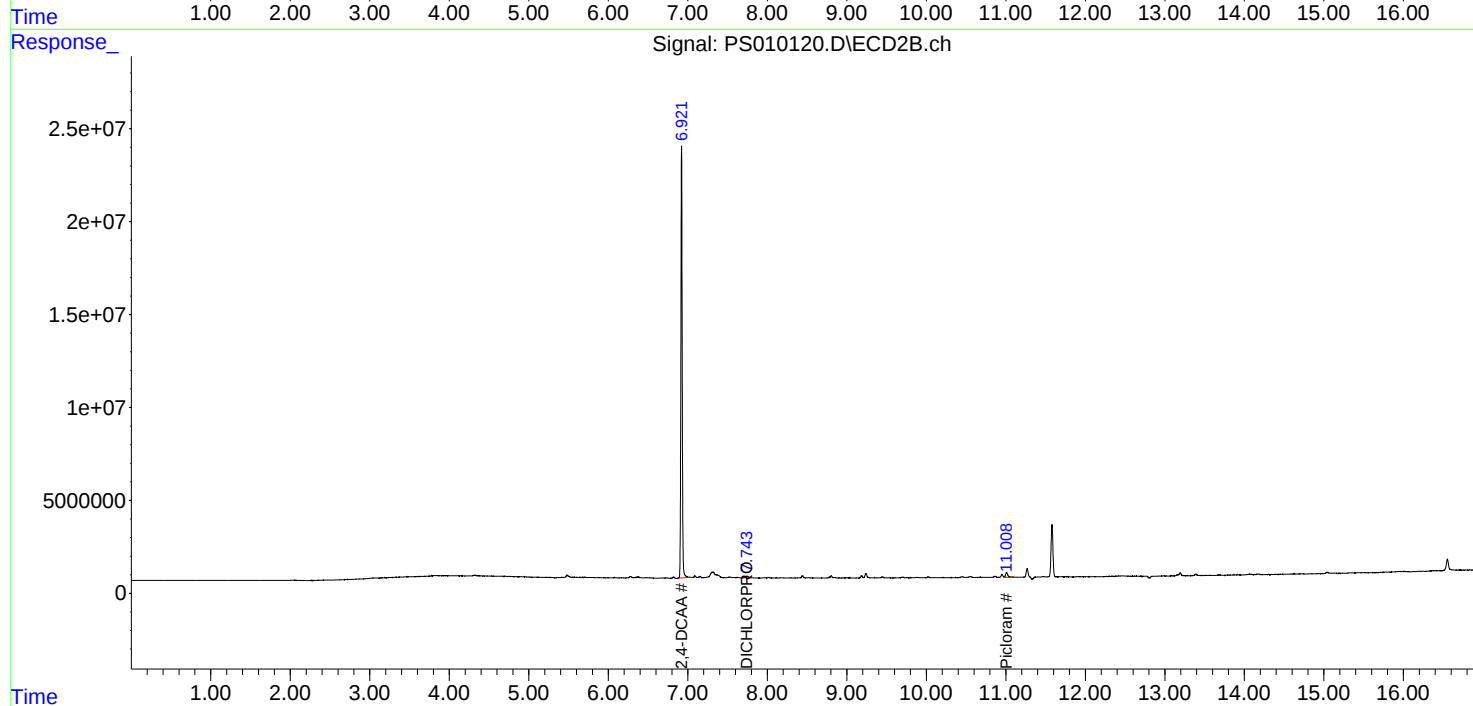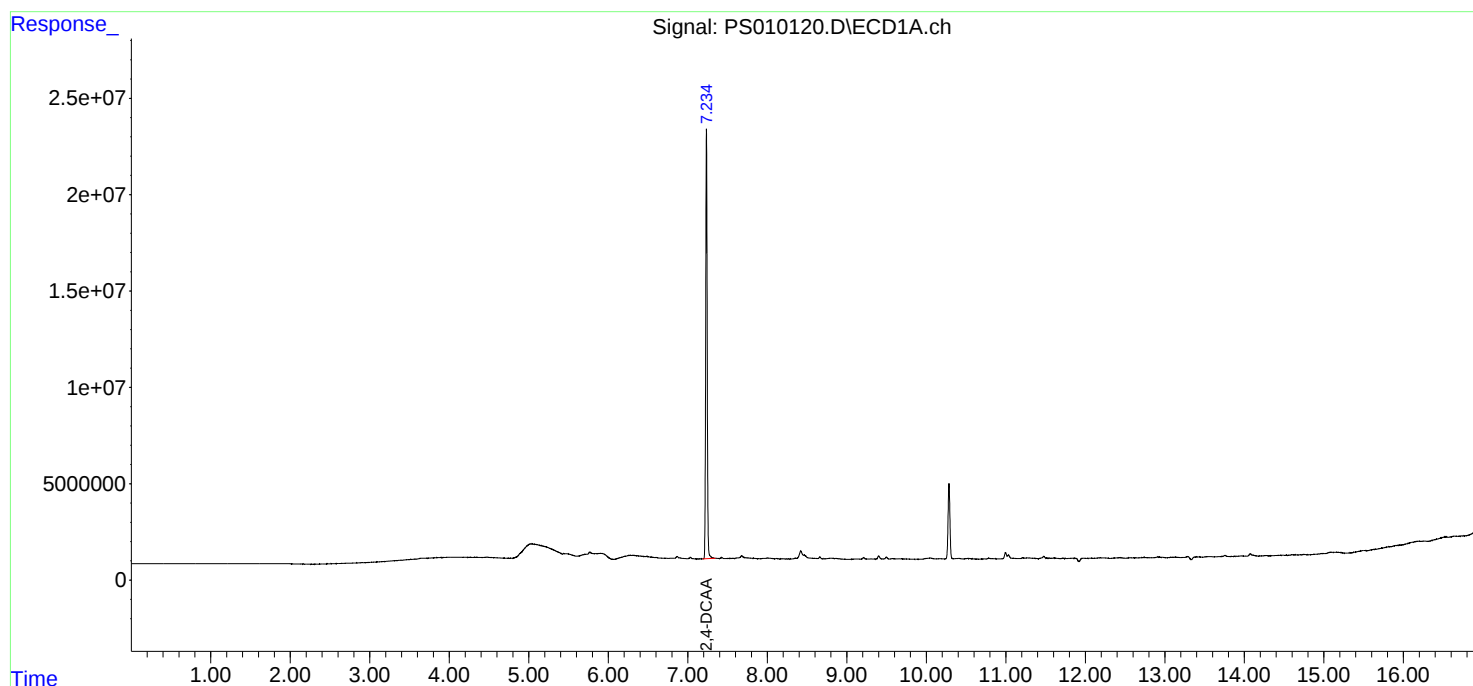


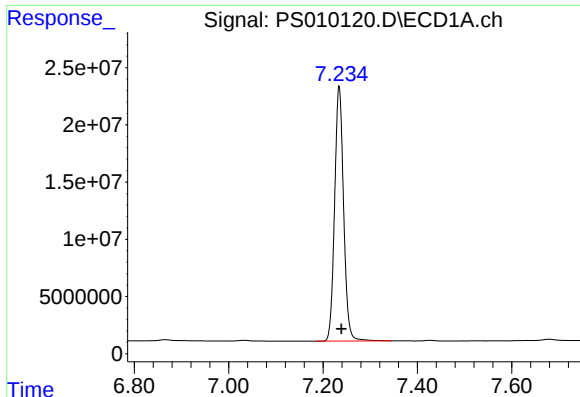

#4 2,4-DCAA


R.T.: 7.234 min
Delta R.T.: -0.005 min
Response: 294072727
Conc: 487.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

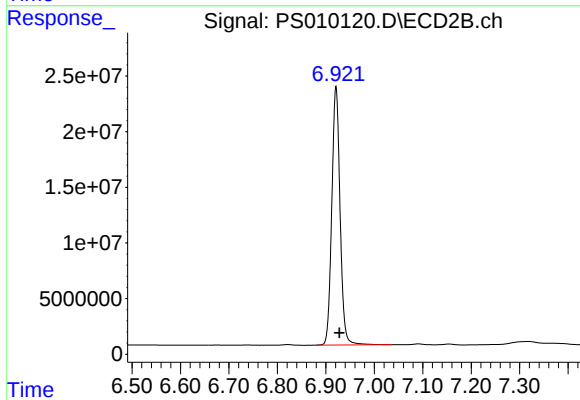


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.007 min
Response: 275869220
Conc: 557.03 ng/ml

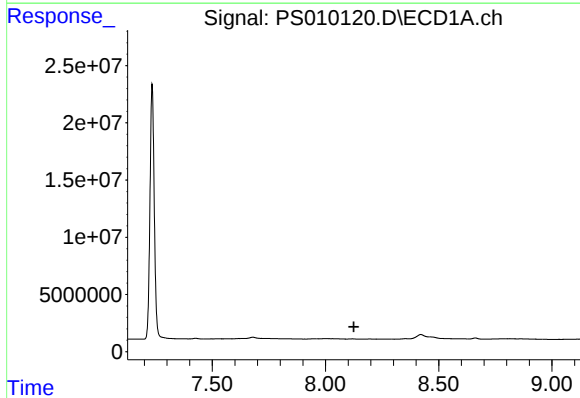


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

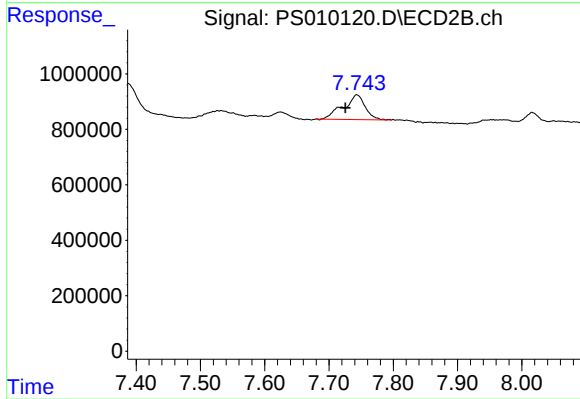

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.018 min
Response: 2096188
Conc: 4.16 ng/ml

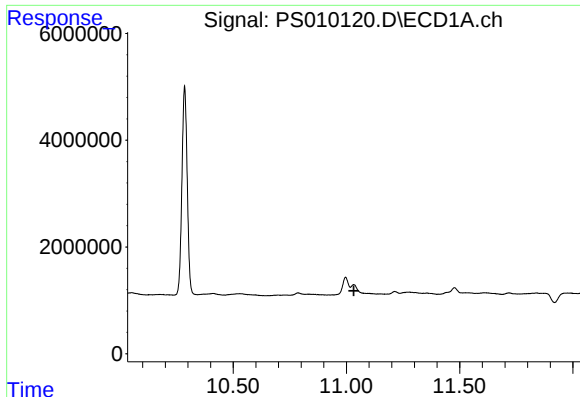

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

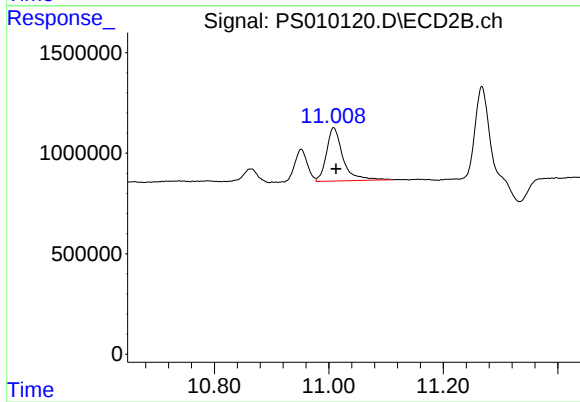

#15 Picloram

R.T.: 11.008 min
Delta R.T.: -0.005 min
Response: 5288030
Conc: 1.55 ng/ml