

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
 Data File : PS010093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2020 11:17
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 12:31:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.922	479.3E6	392.7E6	793.755	793.033
Target Compounds							
1) T	Dalapon	3.044	2.625	464.4E6	439.3E6	612.946	613.607
2) T	3,5-DICHL...	6.446	6.071	605.9E6	545.8E6	736.757	734.635
3) T	4-Nitroph...	7.065	6.526	200.9E6	217.2E6	722.161	715.068
5) T	DICAMBA	7.427	7.092	1726.8E6	1498.4E6	766.606	753.364
6) T	MCPD	7.597	7.190	134.4E6	124.7E6	75.294	75.782
7) T	MCPA	7.747	7.405	191.2E6	177.9E6	74.167	74.576
8) T	DICHLORPROP	8.121	7.718	409.9E6	378.8E6	738.571	752.512
9) T	2,4-D	8.350	8.012	418.5E6	451.3E6	728.836	753.157
10) T	Pentachlo...	8.662	8.443	5730.5E6	4768.9E6	771.181	764.254
11) T	2,4,5-TP ...	9.212	8.804	2307.8E6	2027.5E6	779.821	775.284
12) T	2,4,5-T	9.497	9.182	2151.2E6	1990.5E6	775.863	762.751
13) T	2,4-DB	10.049	9.690	278.3E6	260.7E6	734.748	735.318
14) T	DINOSEB	11.214	10.024	1633.5E6	1492.2E6	730.010	757.755
15) T	Picloram	11.028	11.003	2030.0E6	2178.1E6	655.261	640.402
16) T	DCPA	11.478	10.953	2817.4E6	2576.0E6	756.617	768.272



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
Data File : PS010093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2020 11:17
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 12:31:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

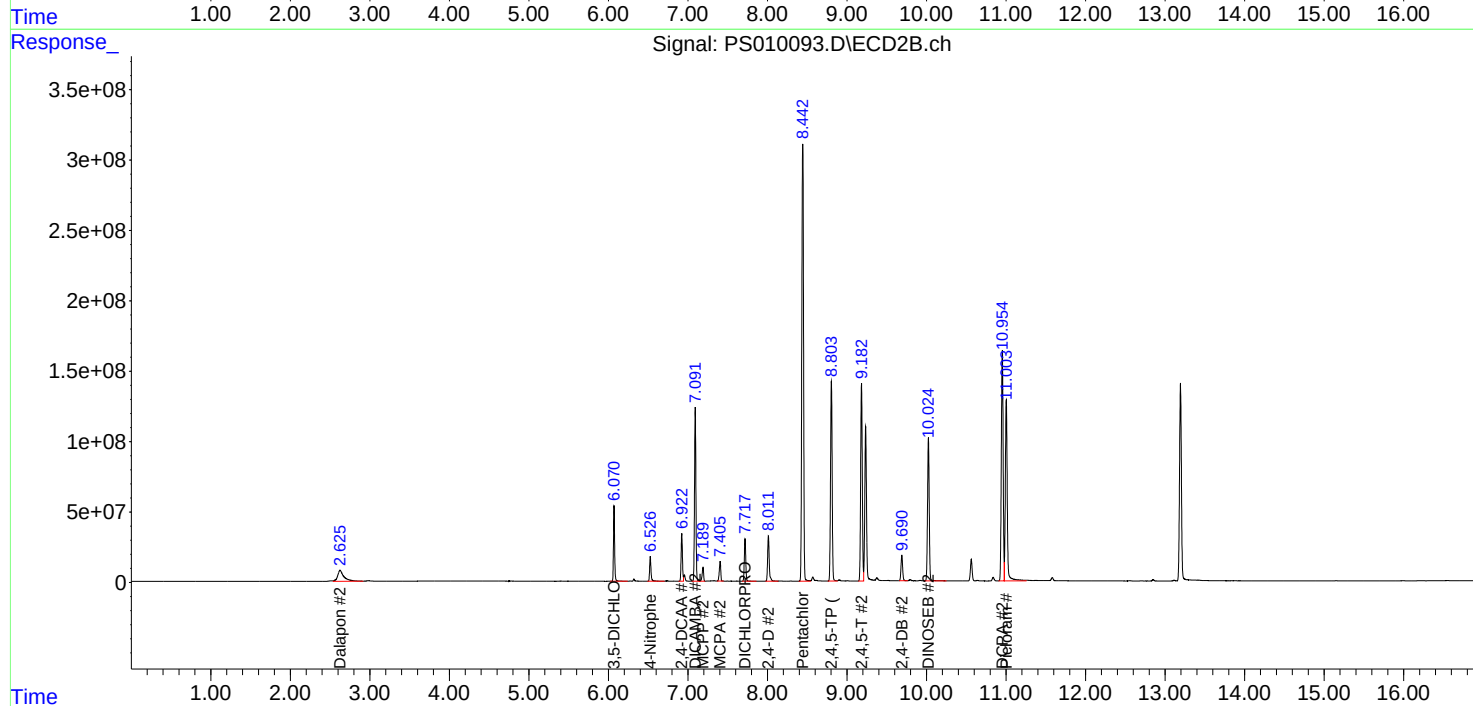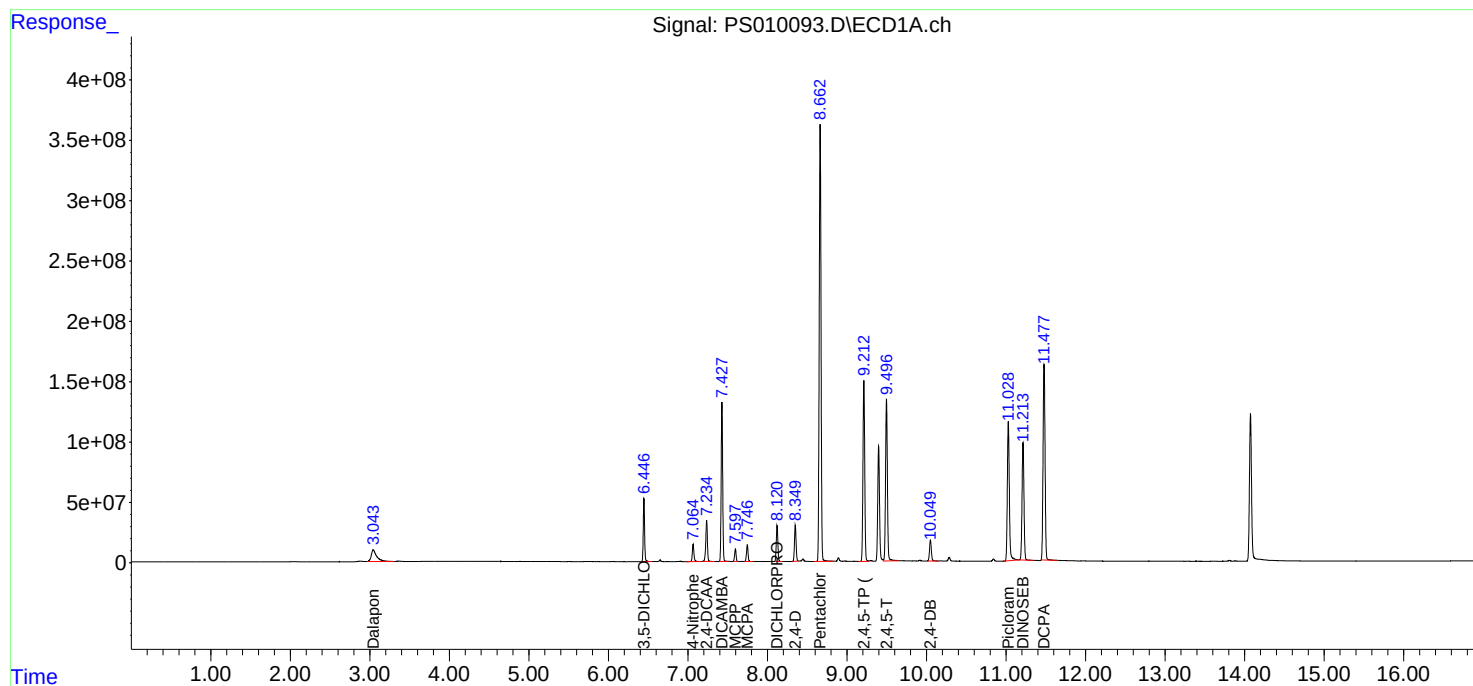


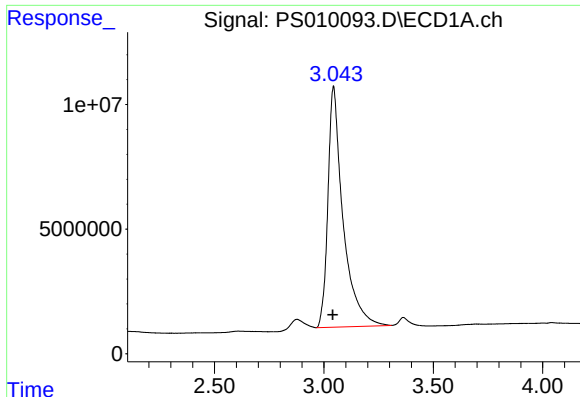

#1 Dalapon


R.T.: 3.044 min
Delta R.T.: 0.004 min
Response: 464371306
Conc: 612.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

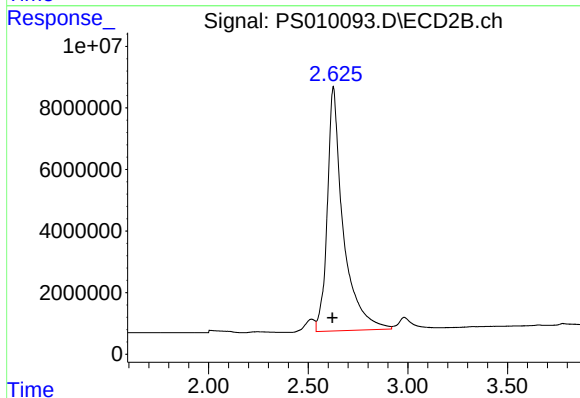


#1 Dalapon

R.T.: 2.625 min
Delta R.T.: 0.004 min
Response: 439276035
Conc: 613.61 ng/ml

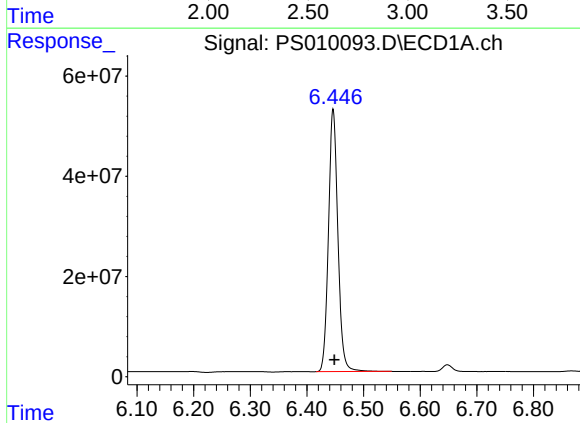


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.446 min
Delta R.T.: -0.002 min
Response: 605855178
Conc: 736.76 ng/ml

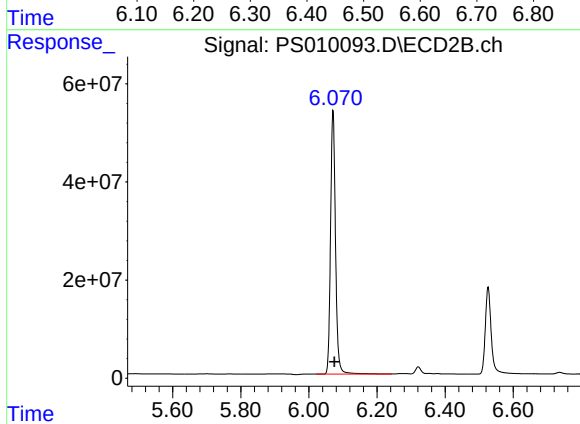

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.071 min
Delta R.T.: -0.004 min
Response: 545764931
Conc: 734.63 ng/ml

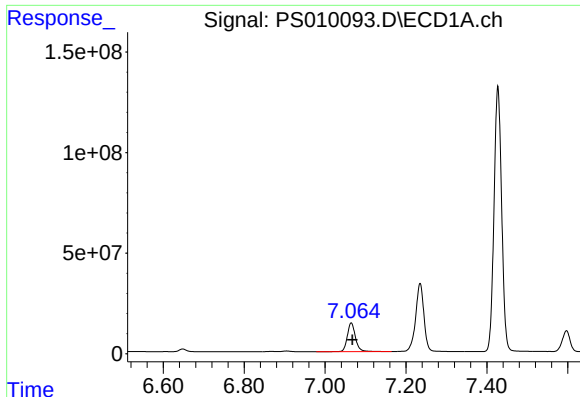

#3 4-Nitrophenol


R.T.: 7.065 min
Delta R.T.: -0.003 min
Response: 200902636
Conc: 722.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

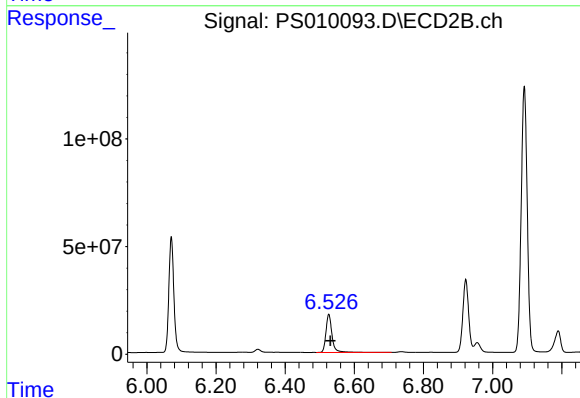


#3 4-Nitrophenol

R.T.: 6.526 min
Delta R.T.: -0.004 min
Response: 217152887
Conc: 715.07 ng/ml

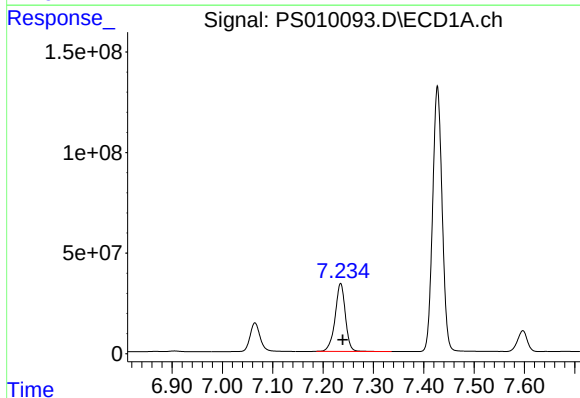


#4 2,4-DCAA

R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 479281611
Conc: 793.76 ng/ml

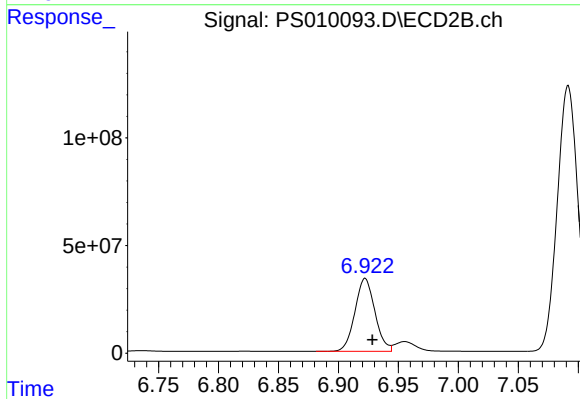

#4 2,4-DCAA


R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 392749524
Conc: 793.03 ng/ml

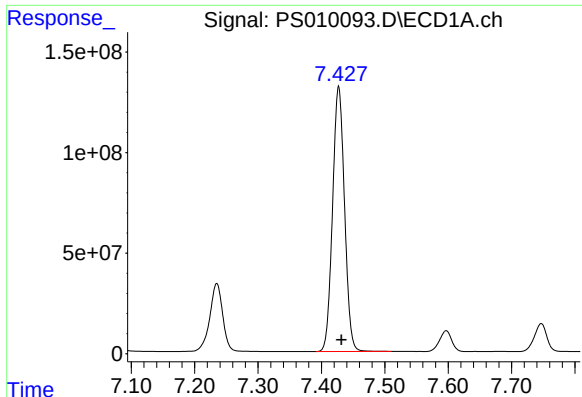

#5 DICAMBA


R.T.: 7.427 min
Delta R.T.: -0.005 min
Response: 1726832157
Conc: 766.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

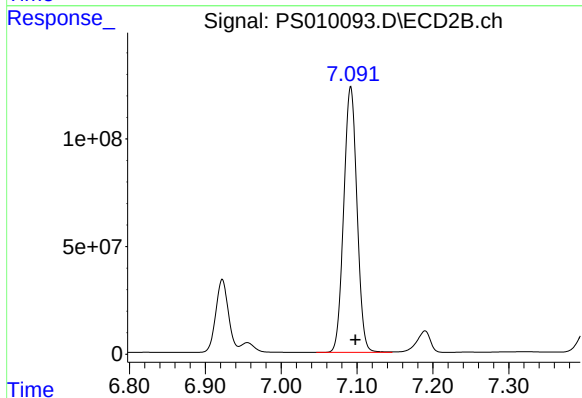


#5 DICAMBA

R.T.: 7.092 min
Delta R.T.: -0.006 min
Response: 1498435315
Conc: 753.36 ng/ml

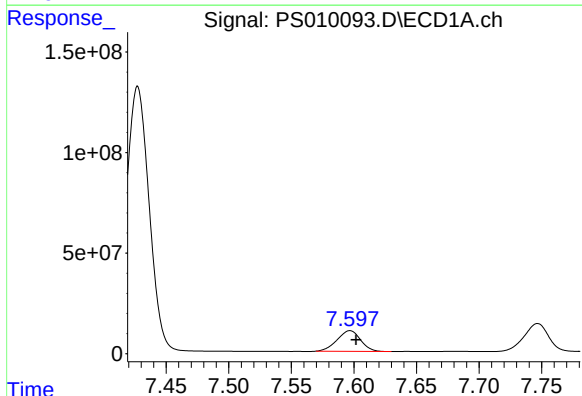


#6 MCP

R.T.: 7.597 min
Delta R.T.: -0.005 min
Response: 134441137
Conc: 75.29 ug/ml

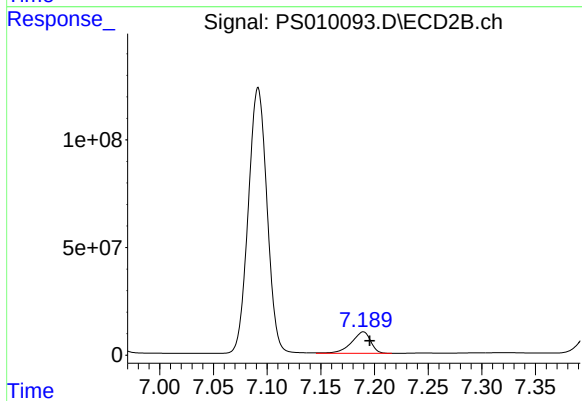

#6 MCP


R.T.: 7.190 min
Delta R.T.: -0.006 min
Response: 124735508
Conc: 75.78 ug/ml

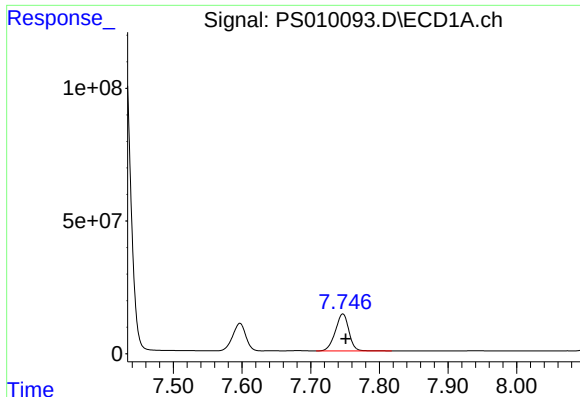

#7 MCPA


R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 191174993
Conc: 74.17 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

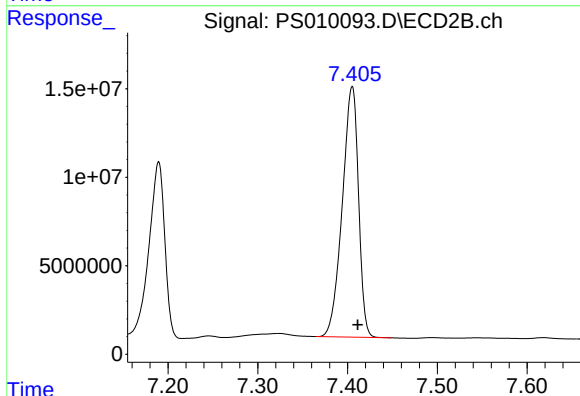


#7 MCPA

R.T.: 7.405 min
Delta R.T.: -0.006 min
Response: 177884536
Conc: 74.58 ug/ml

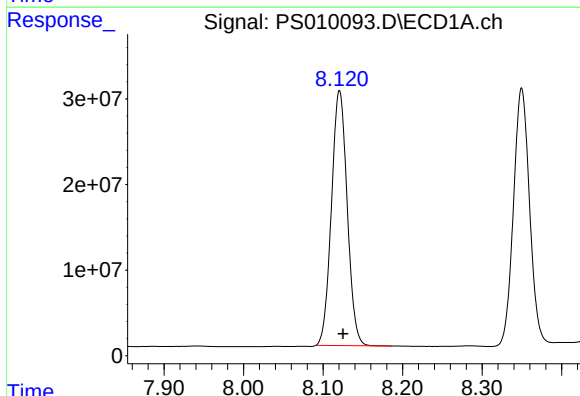


#8 DICHLORPROP

R.T.: 8.121 min
Delta R.T.: -0.005 min
Response: 409896066
Conc: 738.57 ng/ml

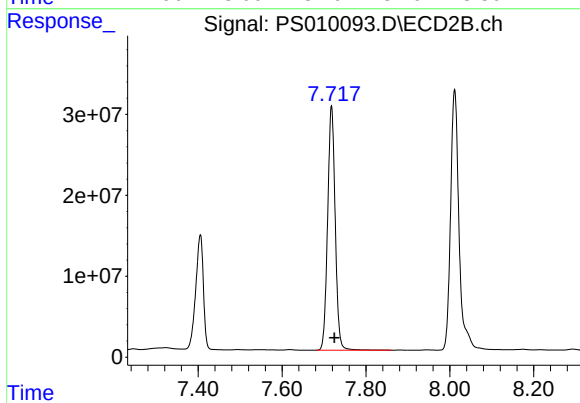

#8 DICHLORPROP


R.T.: 7.718 min
Delta R.T.: -0.007 min
Response: 378751715
Conc: 752.51 ng/ml

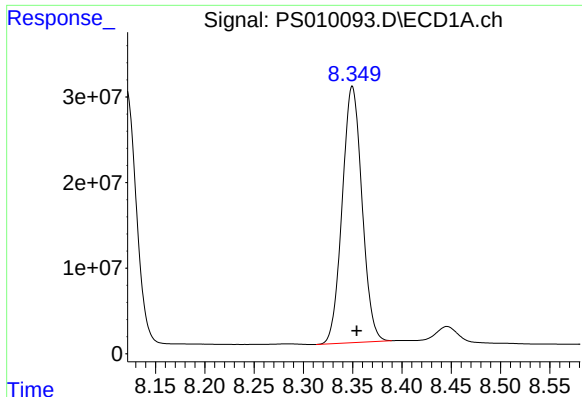

#9 2,4-D


R.T.: 8.350 min
Delta R.T.: -0.004 min
Response: 418486552
Conc: 728.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

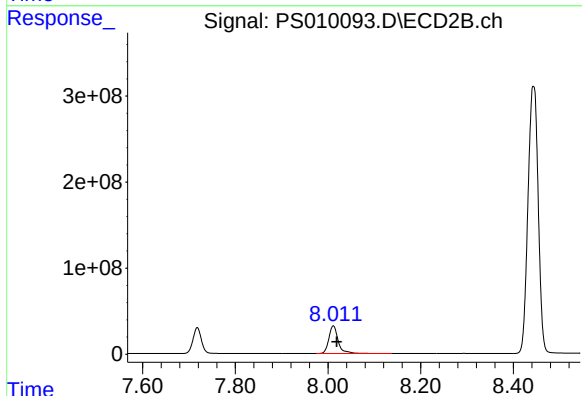


#9 2,4-D

R.T.: 8.012 min
Delta R.T.: -0.007 min
Response: 451299208
Conc: 753.16 ng/ml

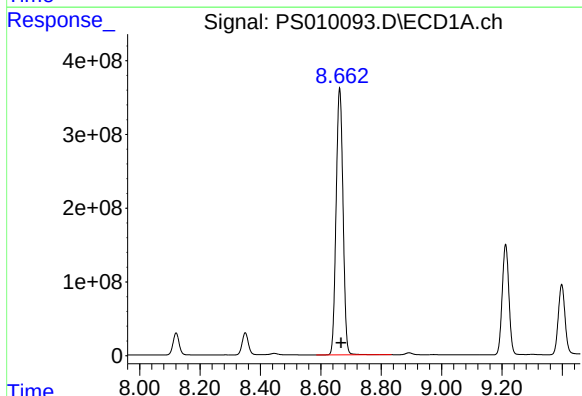


#10 Pentachlorophenol

R.T.: 8.662 min
Delta R.T.: -0.005 min
Response: 5730504254
Conc: 771.18 ng/ml

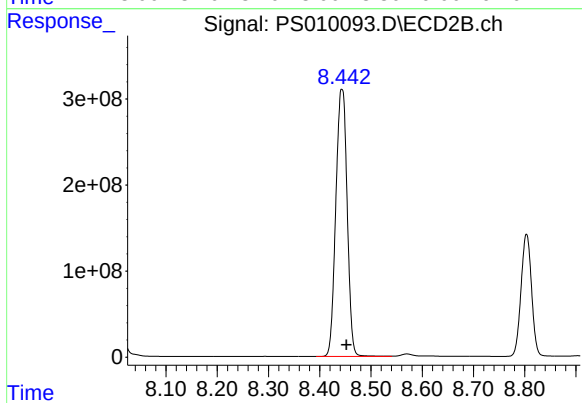

#10 Pentachlorophenol


R.T.: 8.443 min
Delta R.T.: -0.009 min
Response: 4768935347
Conc: 764.25 ng/ml

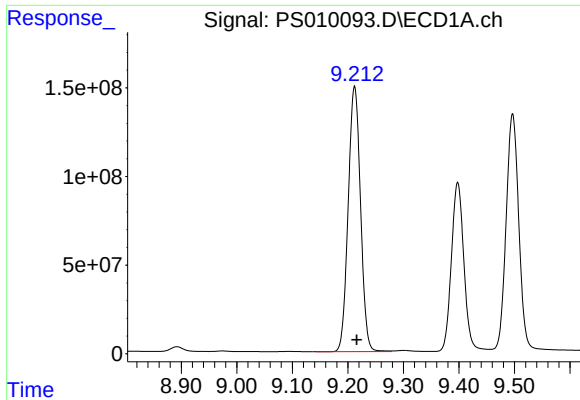

#11 2,4,5-TP (SILVEX)


R.T.: 9.212 min
Delta R.T.: -0.004 min
Response: 2307825151
Conc: 779.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

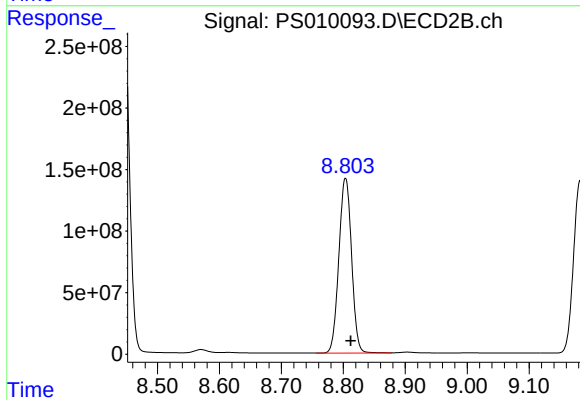


#11 2,4,5-TP (SILVEX)

R.T.: 8.804 min
Delta R.T.: -0.008 min
Response: 2027542475
Conc: 775.28 ng/ml

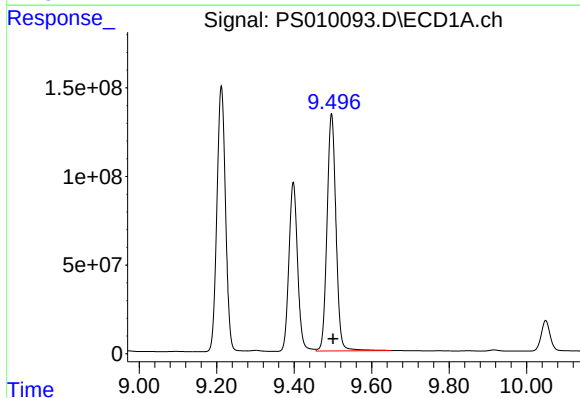


#12 2,4,5-T

R.T.: 9.497 min
Delta R.T.: -0.004 min
Response: 2151216110
Conc: 775.86 ng/ml

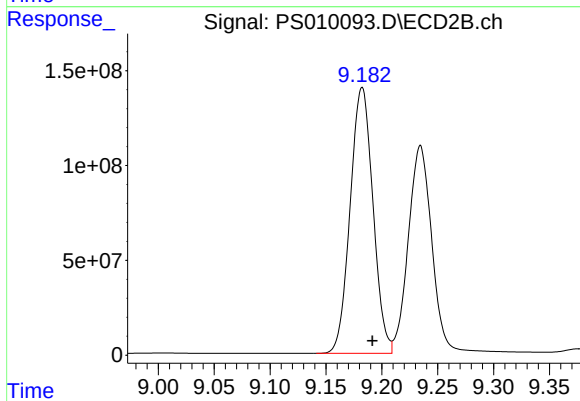

#12 2,4,5-T


R.T.: 9.182 min
Delta R.T.: -0.009 min
Response: 1990453322
Conc: 762.75 ng/ml

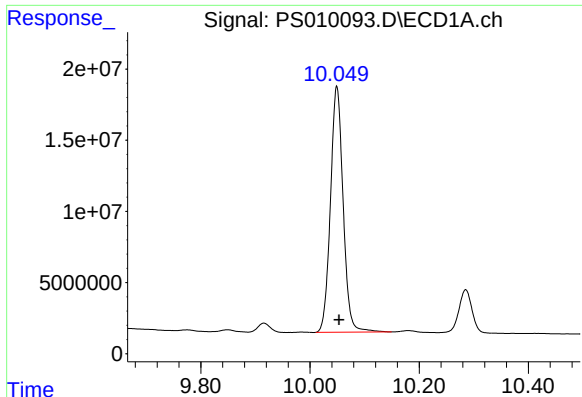

#13 2,4-DB


R.T.: 10.049 min
Delta R.T.: -0.004 min
Response: 278327142
Conc: 734.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

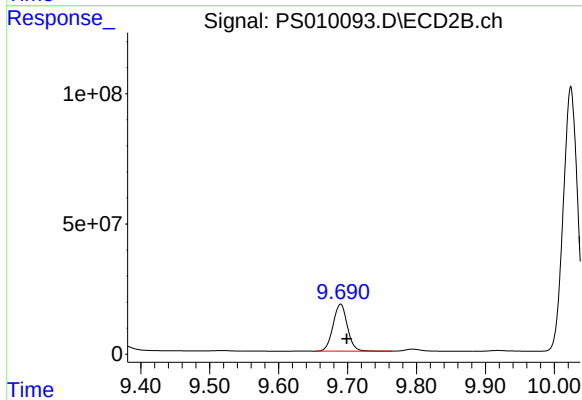


#13 2,4-DB

R.T.: 9.690 min
Delta R.T.: -0.009 min
Response: 260720004
Conc: 735.32 ng/ml

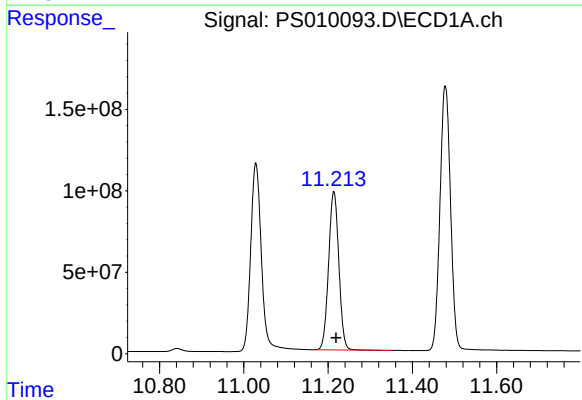


#14 DINOSEB

R.T.: 11.214 min
Delta R.T.: -0.005 min
Response: 1633500142
Conc: 730.01 ng/ml

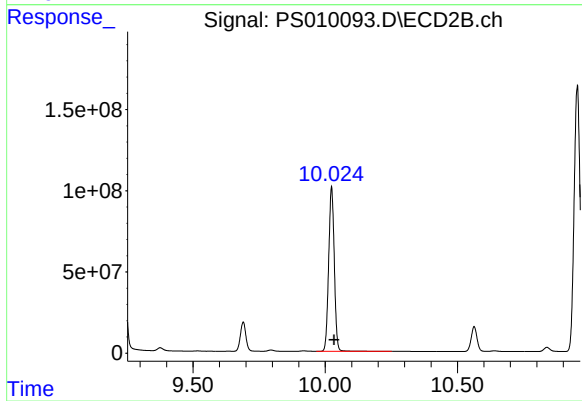

#14 DINOSEB


R.T.: 10.024 min
Delta R.T.: -0.010 min
Response: 1492214172
Conc: 757.76 ng/ml

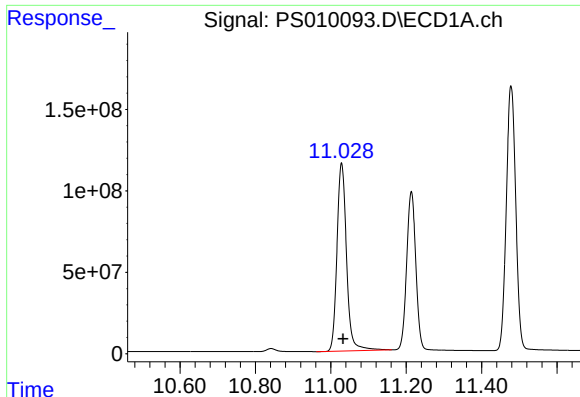

#15 Picloram


R.T.: 11.028 min
Delta R.T.: -0.004 min
Response: 2030041409
Conc: 655.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

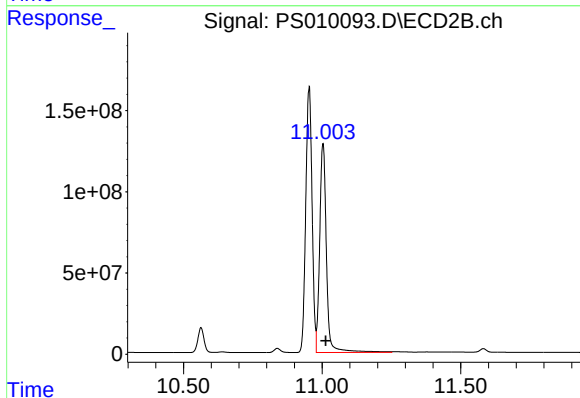


#15 Picloram

R.T.: 11.003 min
Delta R.T.: -0.010 min
Response: 2178138430
Conc: 640.40 ng/ml

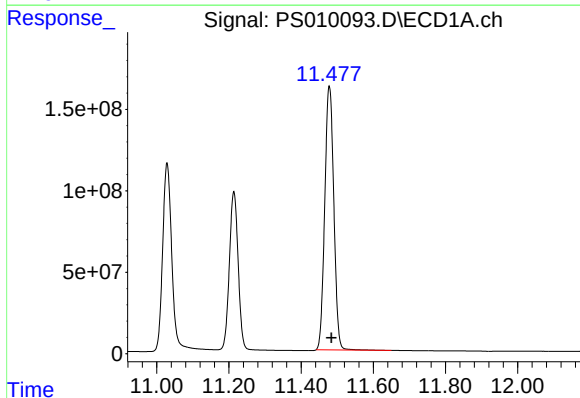

#16 DCPA

R.T.: 11.478 min
Delta R.T.: -0.006 min
Response: 2817396647
Conc: 756.62 ng/ml

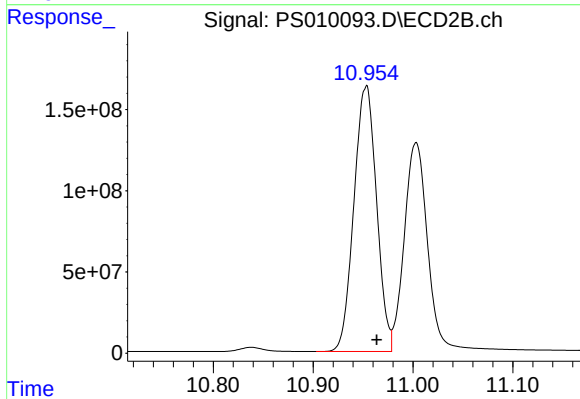

#16 DCPA

R.T.: 10.953 min
Delta R.T.: -0.010 min
Response: 2576043726
Conc: 768.27 ng/ml