

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
 Data File : PS004407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 07:48
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 13:29:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.003	5.696	348.8E6	258.9E6	554.087	536.748
Target Compounds							
9) T	2,4-D	7.088	0.000	67682114	0	118.960	N.D. #
15) T	Picloram	0.000	9.539	0	10028870	N.D.	2.742
16) T	DCPA	0.000	9.539	0	10028870	N.D.	3.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
Data File : PS004407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 07:48
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 13:29:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

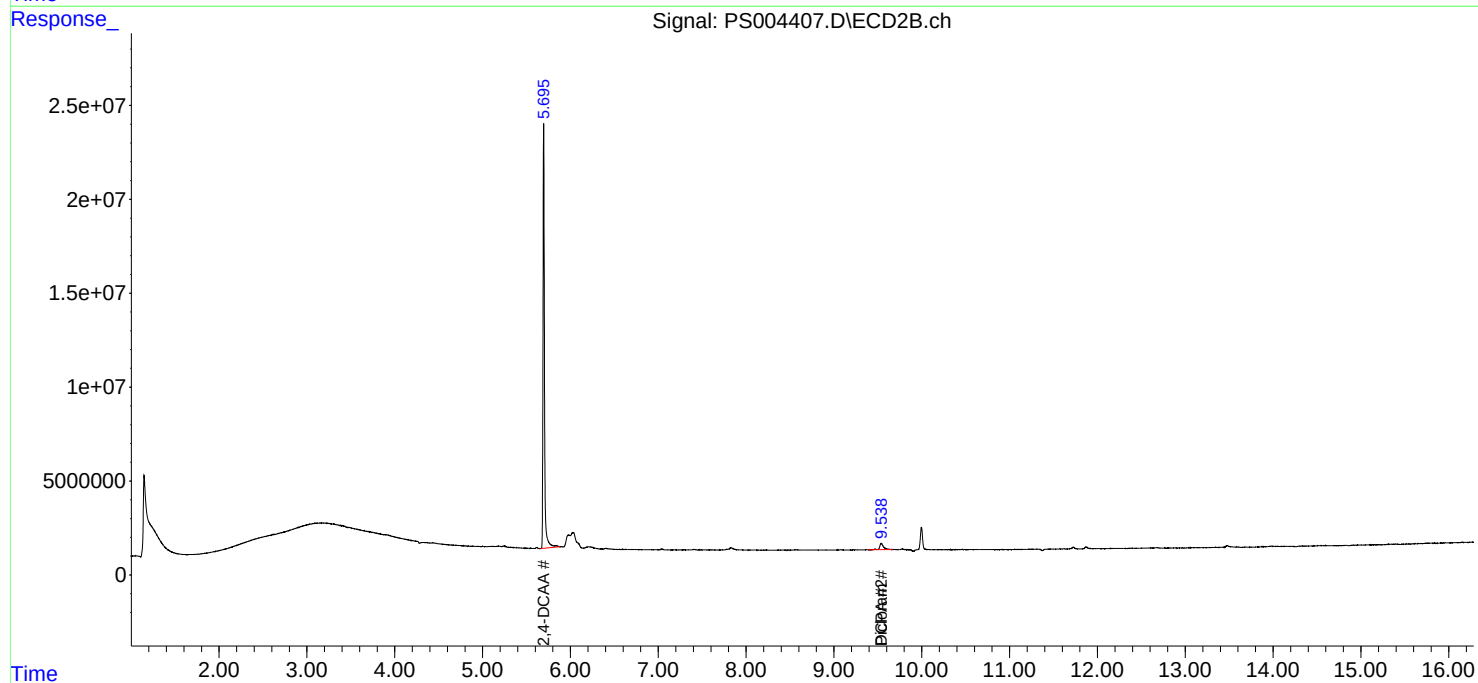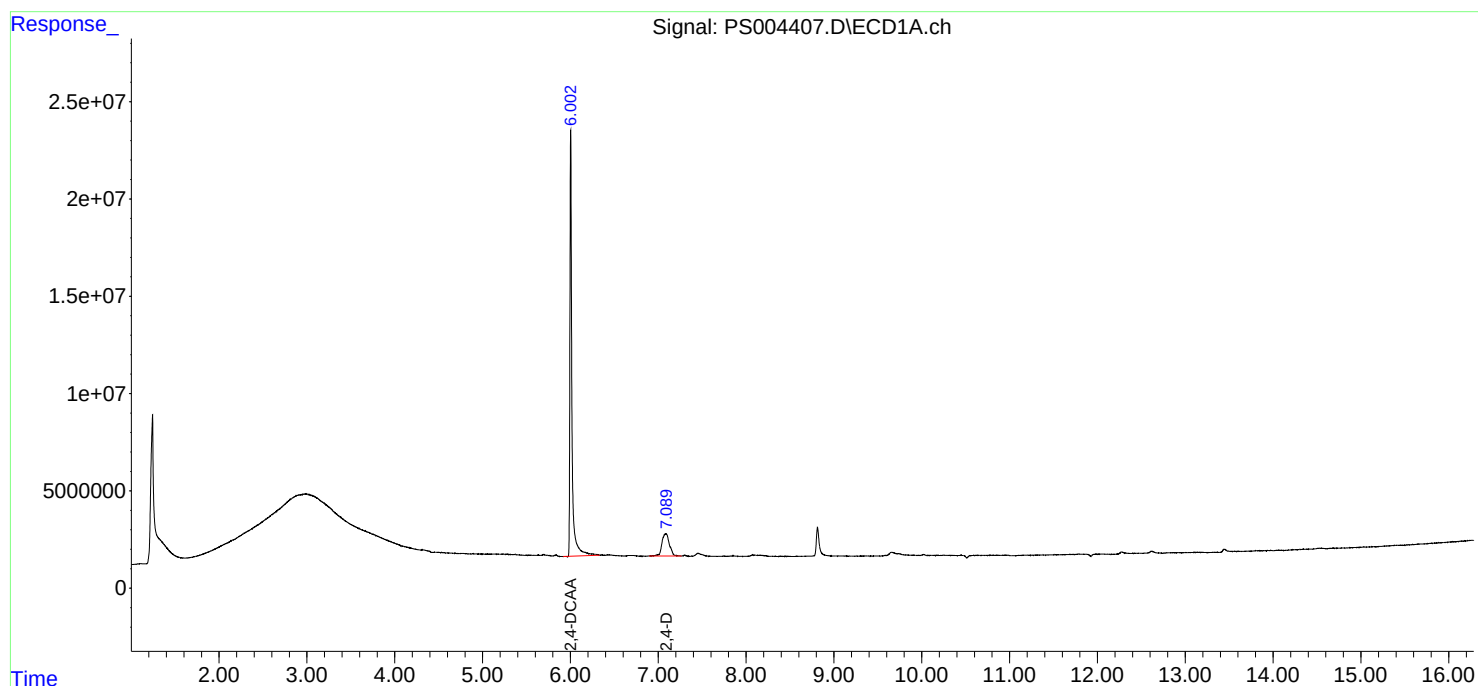


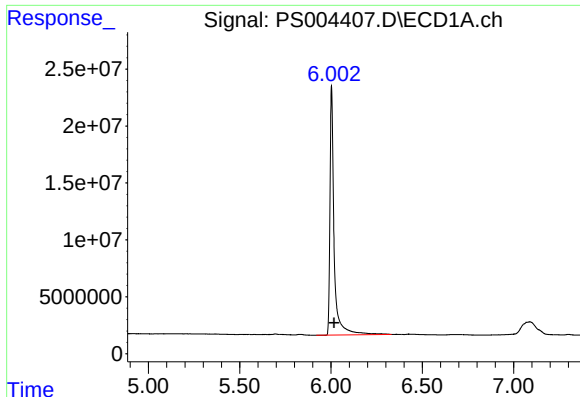

#4 2,4-DCAA


R.T.: 6.003 min
Delta R.T.: -0.015 min
Response: 348774002
Conc: 554.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

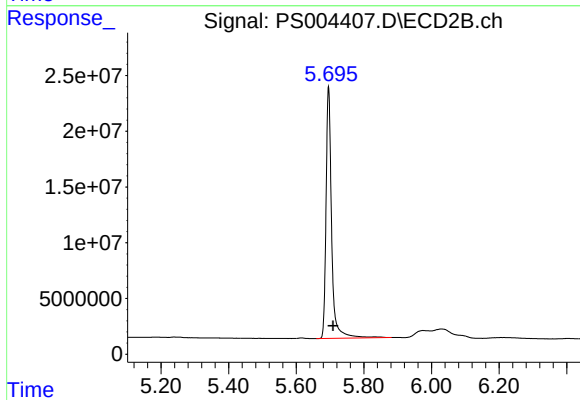


#4 2,4-DCAA

R.T.: 5.696 min
Delta R.T.: -0.013 min
Response: 258864518
Conc: 536.75 ng/ml

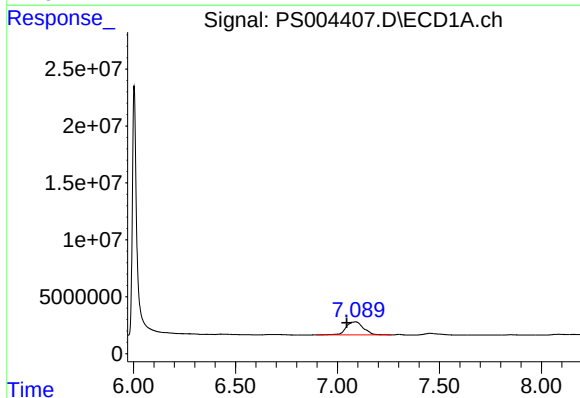


#9 2,4-D

R.T.: 7.088 min
Delta R.T.: 0.043 min
Response: 67682114
Conc: 118.96 ng/ml

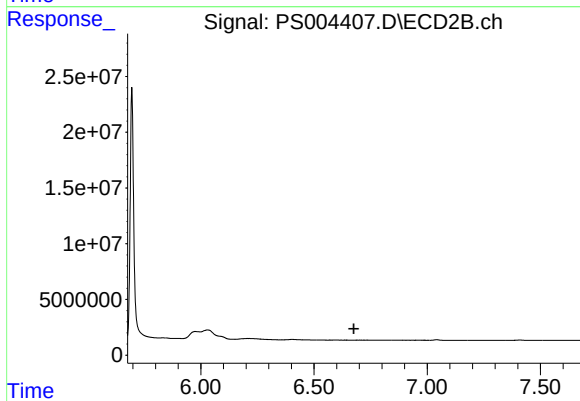

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.676 min
Response: 0
Conc: N.D.

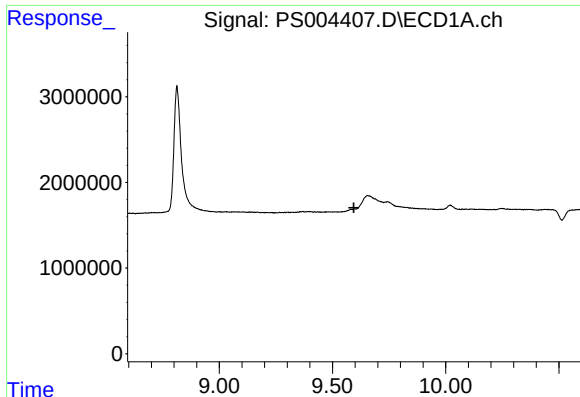

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

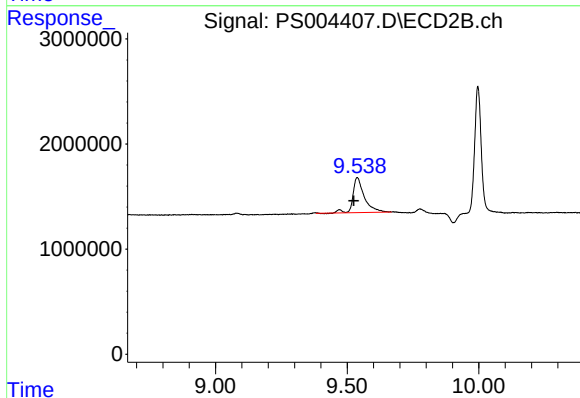


#15 Picloram

R.T.: 9.539 min
Delta R.T.: 0.013 min
Response: 10028870
Conc: 2.74 ng/ml

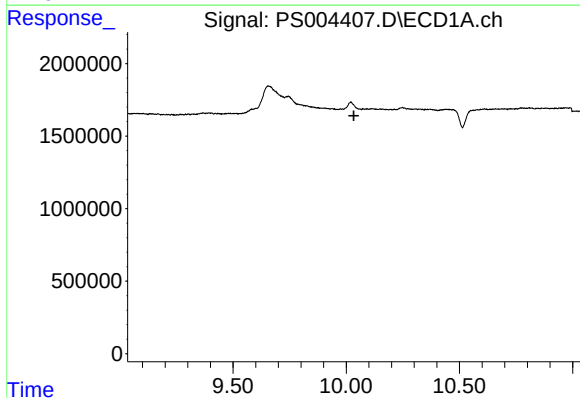

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.034 min
Response: 0
Conc: N.D.

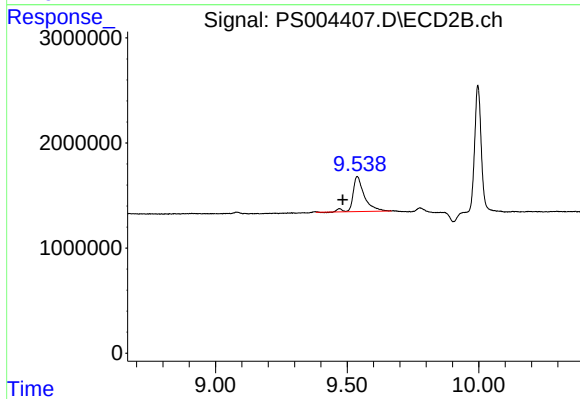

#16 DCPA

R.T.: 9.539 min
Delta R.T.: 0.055 min
Response: 10028870
Conc: 3.05 ng/ml