

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
 Data File : PS004411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 11:56
 Operator : EI\SJ
 Sample : K2194-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 JC-03-042919-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 13:30:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.017	5.710	138.4E6	114.2E6	219.837	236.740
Target Compounds							
1) T	Dalapon	2.381	2.042	28597056	55508962	36.393	82.950 #
2) T	3,5-DICHL...	0.000	4.981	0	5589051	N.D.	9.092
3) T	4-Nitroph...	5.803	0.000	3792905	0	15.178	N.D. #
5) T	DICAMBA	6.115	5.818	11219695	6572710	4.718	3.512 #
6) T	MCPD	6.375	0.000	2969022	0	1.718	N.D. #
7) T	MCPA	6.500	6.174	40856425	287.8E6	15.858	144.878 #
8) T	DICHLORPROP	0.000	6.403	0	7682828	N.D.	16.326
9) T	2,4-D	7.107	0.000	25999824	0	45.698	N.D. #
11) T	2,4,5-TP ...	0.000	7.369	0	54795014	N.D.	20.855



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
Data File : PS004411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 11:56
Operator : EI\SJ
Sample : K2194-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
JC-03-042919-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 13:30:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

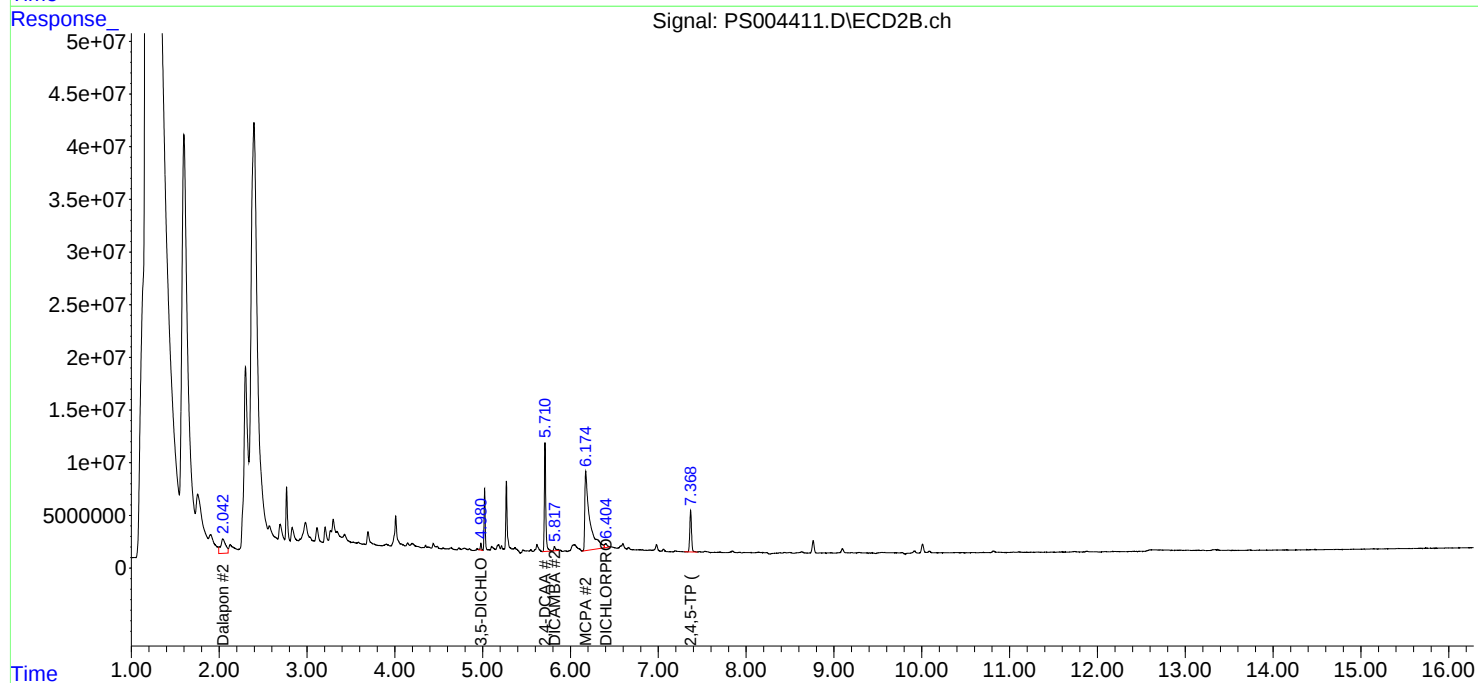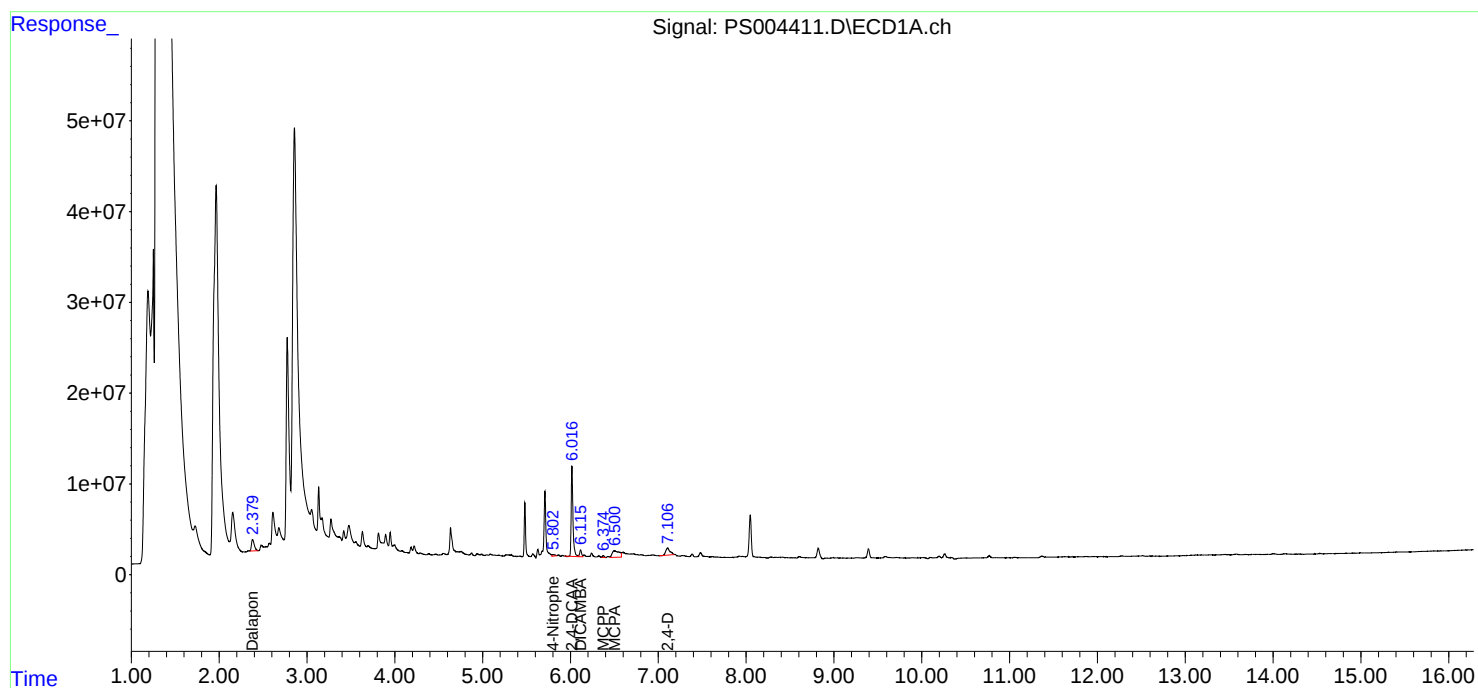


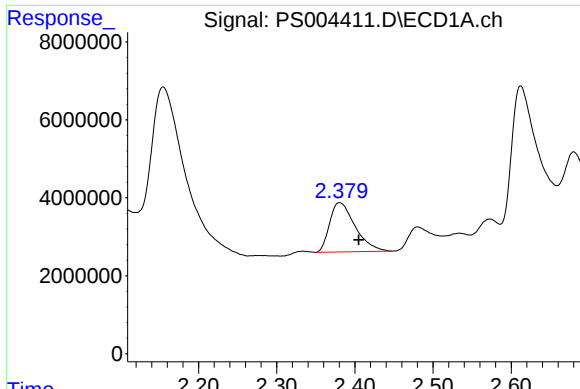

#1 Dalapon


R.T.: 2.381 min
Delta R.T.: -0.024 min
Response: 28597056
Conc: 36.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-042919-A

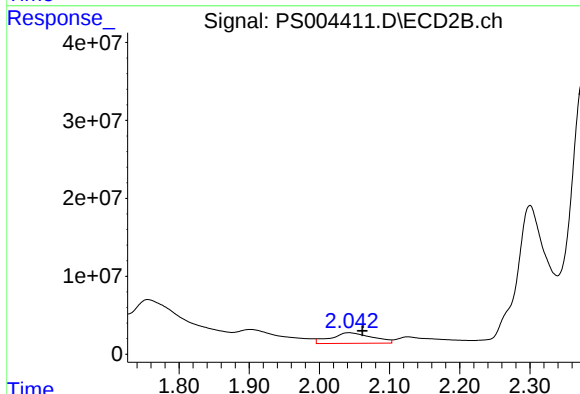


#1 Dalapon

R.T.: 2.042 min
Delta R.T.: -0.019 min
Response: 55508962
Conc: 82.95 ng/ml

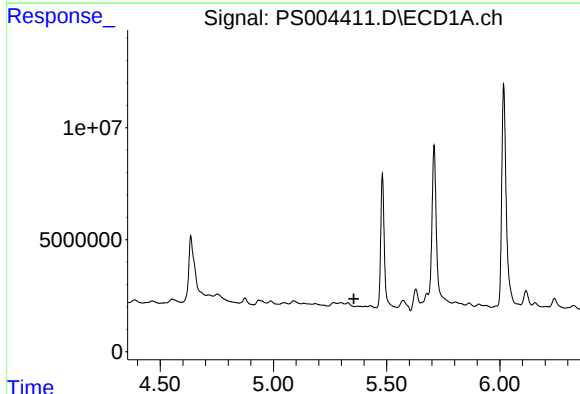


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

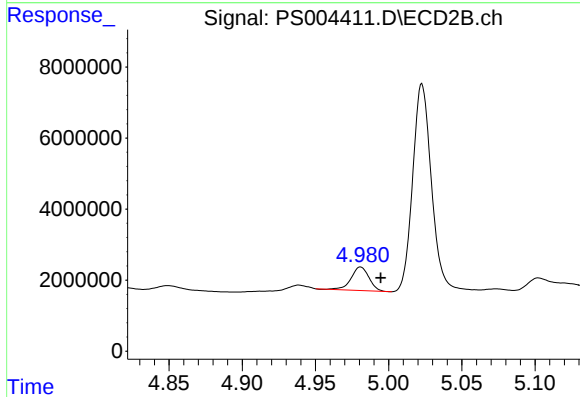

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.981 min
Delta R.T.: -0.014 min
Response: 5589051
Conc: 9.09 ng/ml

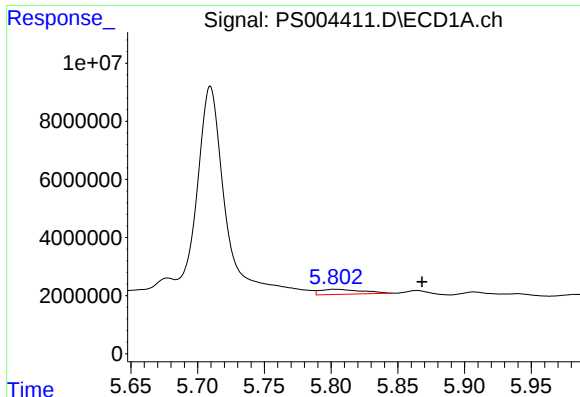

#3 4-Nitrophenol


R.T.: 5.803 min
Delta R.T.: -0.065 min
Response: 3792905
Conc: 15.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-042919-A

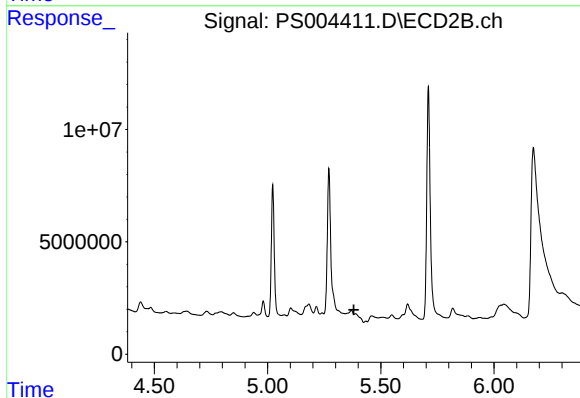


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.381 min
Response: 0
Conc: N.D.

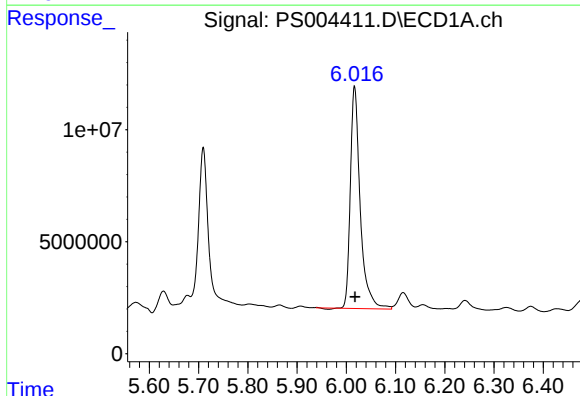


#4 2,4-DCAA

R.T.: 6.017 min
Delta R.T.: -0.001 min
Response: 138377640
Conc: 219.84 ng/ml

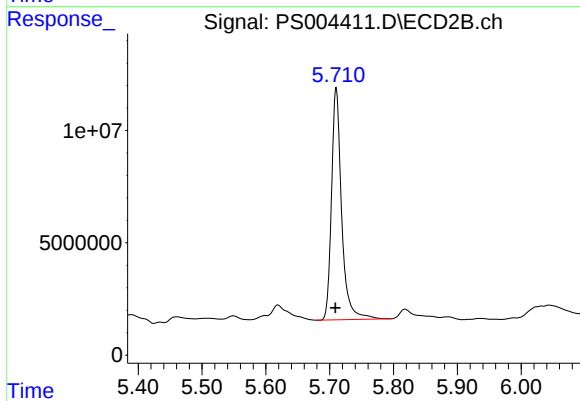

#4 2,4-DCAA


R.T.: 5.710 min
Delta R.T.: 0.001 min
Response: 114175630
Conc: 236.74 ng/ml

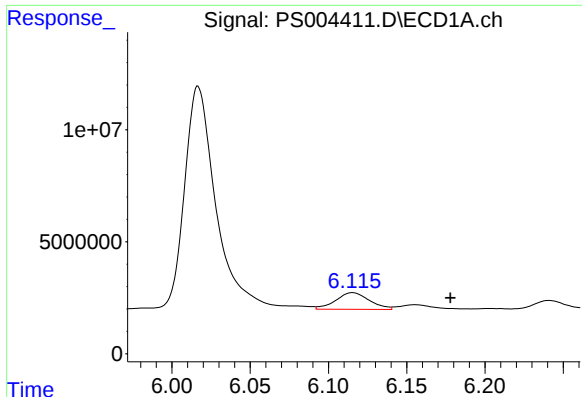

#5 DICAMBA


R.T.: 6.115 min
Delta R.T.: -0.062 min
Response: 11219695
Conc: 4.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-042919-A

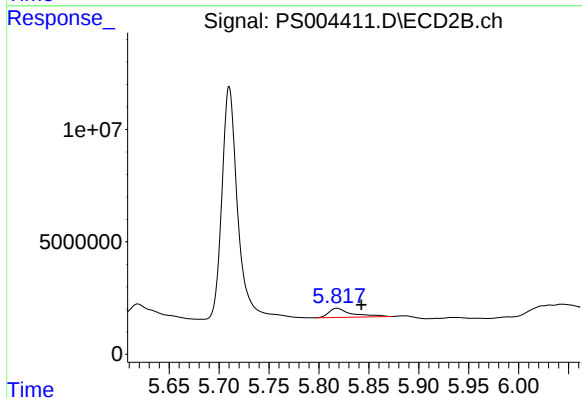


#5 DICAMBA

R.T.: 5.818 min
Delta R.T.: -0.024 min
Response: 6572710
Conc: 3.51 ng/ml

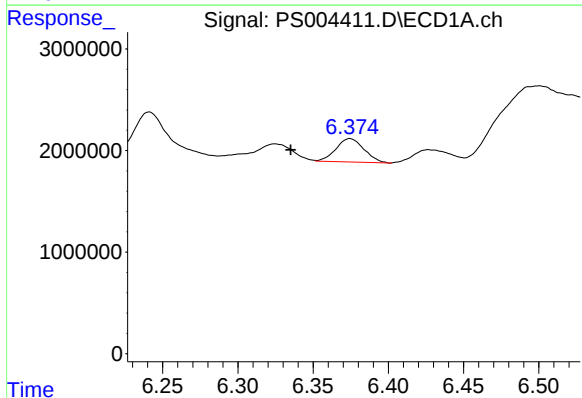


#6 MCP

R.T.: 6.375 min
Delta R.T.: 0.039 min
Response: 2969022
Conc: 1.72 ug/ml

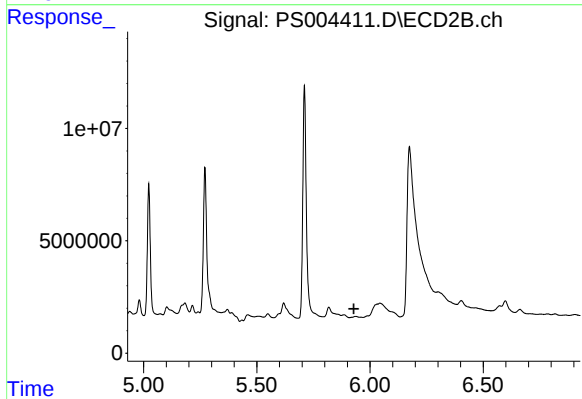

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

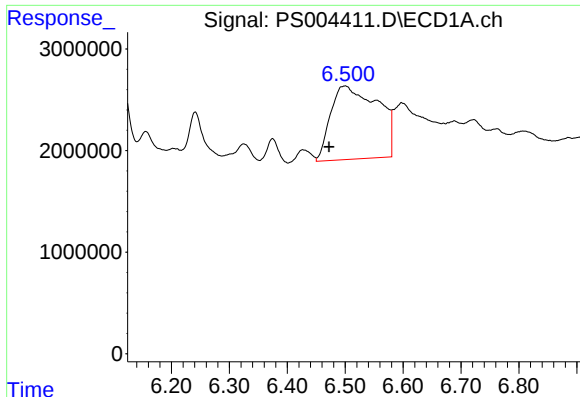

#7 MCPA


R.T.: 6.500 min
Delta R.T.: 0.027 min
Response: 40856425
Conc: 15.86 ug/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-042919-A

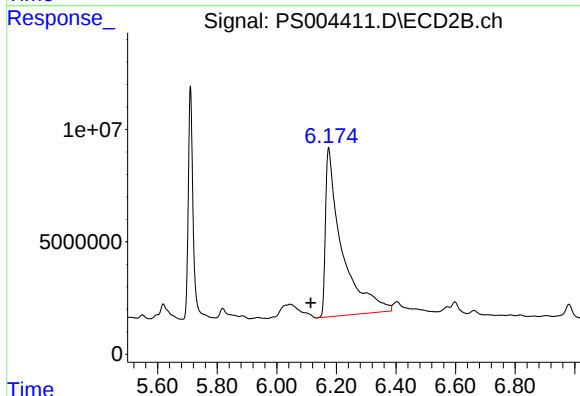


#7 MCPA

R.T.: 6.174 min
Delta R.T.: 0.061 min
Response: 287803375
Conc: 144.88 ug/ml

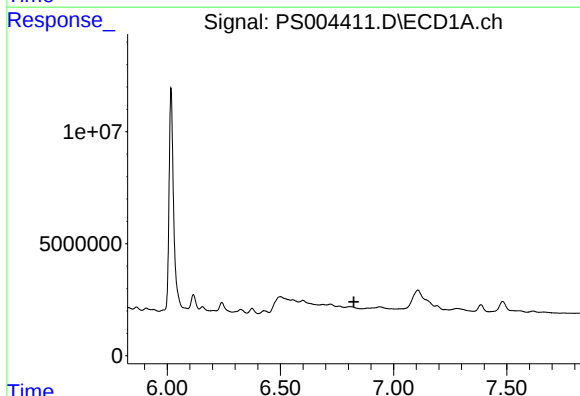


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.825 min
Response: 0
Conc: N.D.

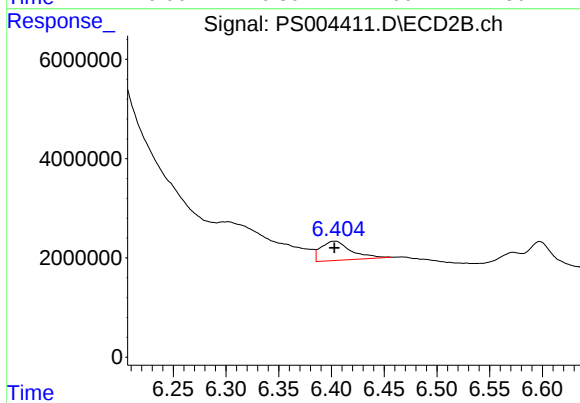

#8 DICHLORPROP


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 7682828
Conc: 16.33 ng/ml

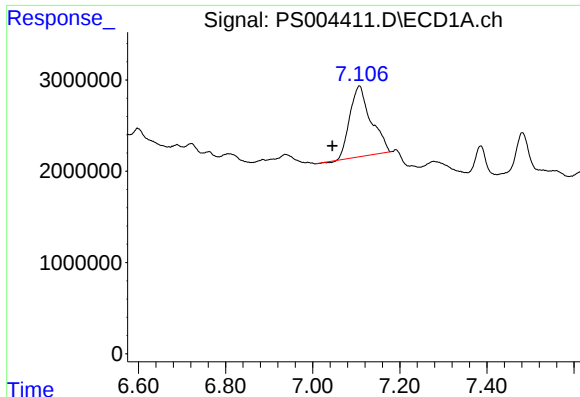

#9 2,4-D


R.T.: 7.107 min
Delta R.T.: 0.062 min
Response: 25999824
Conc: 45.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-042919-A

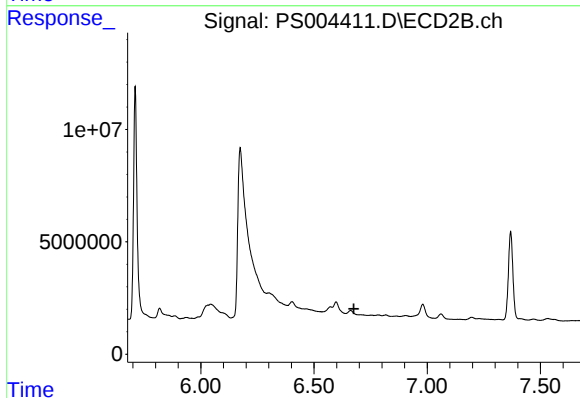


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

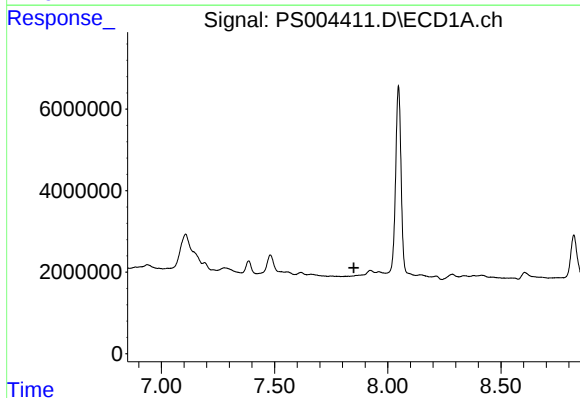

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

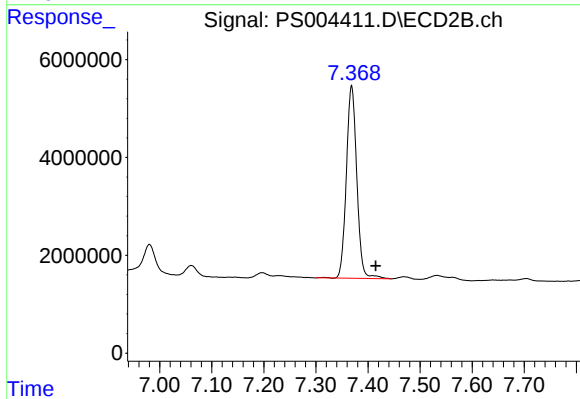

#11 2,4,5-TP (SILVEX)

R.T.: 7.369 min
Delta R.T.: -0.046 min
Response: 54795014
Conc: 20.85 ng/ml