

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
 Data File : PS004418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 15:48
 Operator : EI\SJ
 Sample : PB119406TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB119406TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:01:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.013	5.707	268.8E6	206.6E6	427.109	428.399
Target Compounds							
1) T	Dalapon	2.379	2.041	43548307	105.7E6	55.420	157.991 #
2) T	3,5-DICHL...	5.325	5.020	3260745	156.1E6	4.128	253.889 #
3) T	4-Nitroph...	5.862	5.386	6901456	6457364	27.617	26.105
5) T	DICAMBA	6.152	5.815	6771400	21046600	2.848	11.244 #
6) T	MCPD	6.371	0.000	6465527	0	3.742	N.D. #
7) T	MCPA	0.000	6.049	0	37381508	N.D.	18.818
8) T	DICHLORPROP	0.000	6.404	0	10141511	N.D.	21.551
9) T	2,4-D	7.098	0.000	40613011	0	71.383	N.D. #
10) T	Pentachlo...	7.308	7.054	4728978	6261047	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	7.366	0	110.0E6	N.D.	41.852



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
Data File : PS004418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 15:48
Operator : EI\SJ
Sample : PB119406TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
PB119406TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:01:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

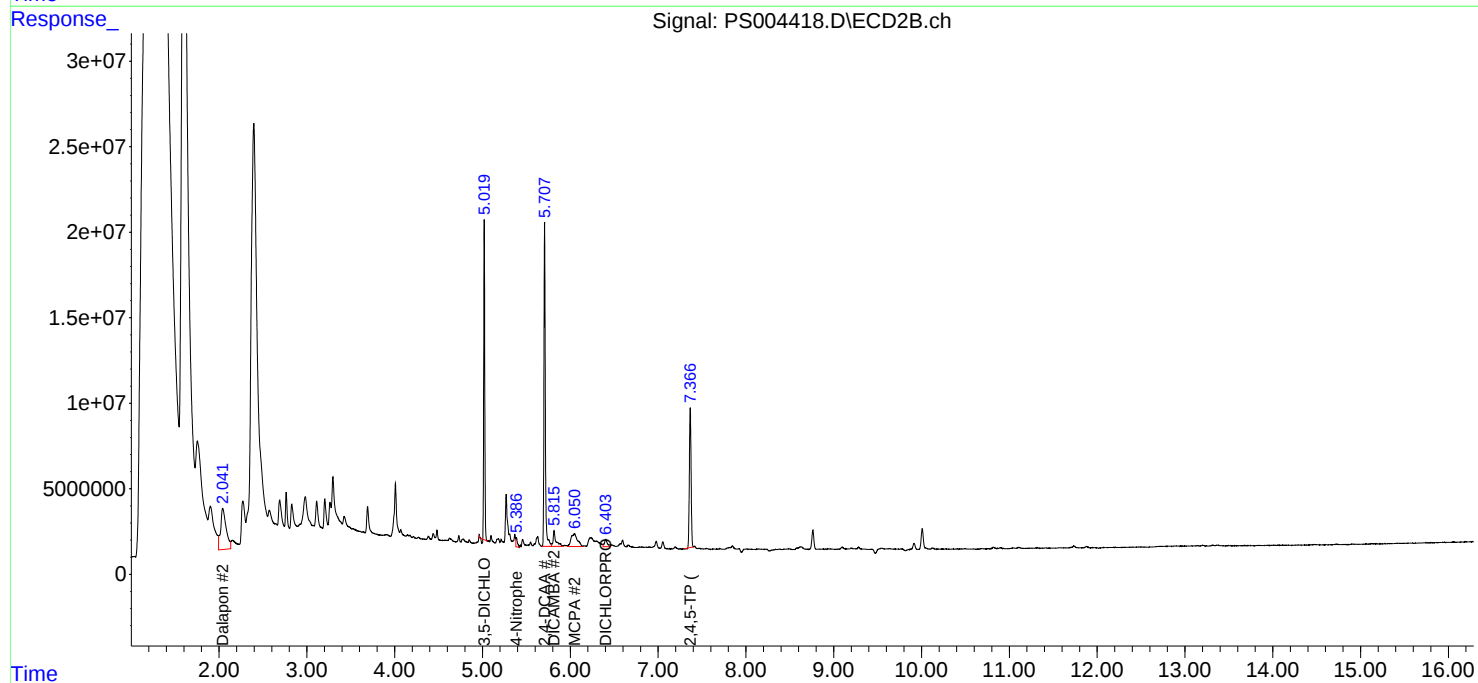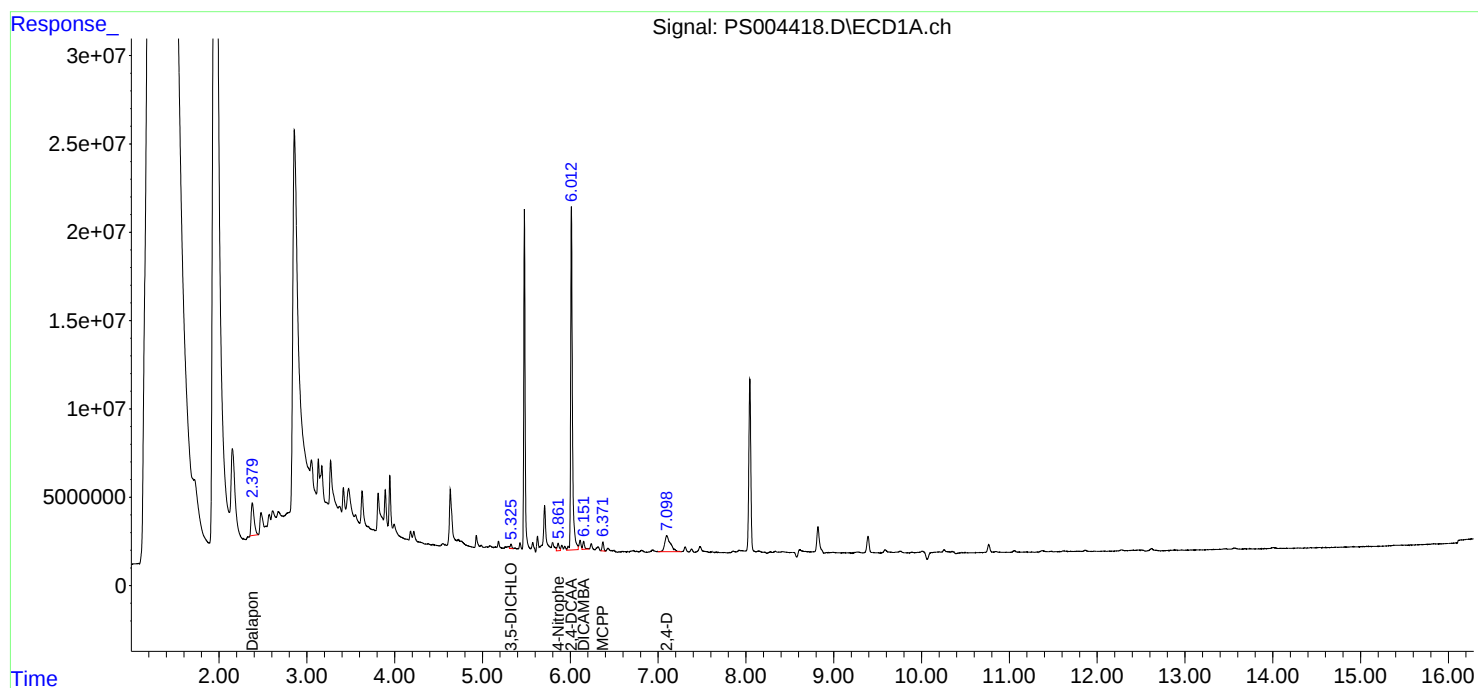


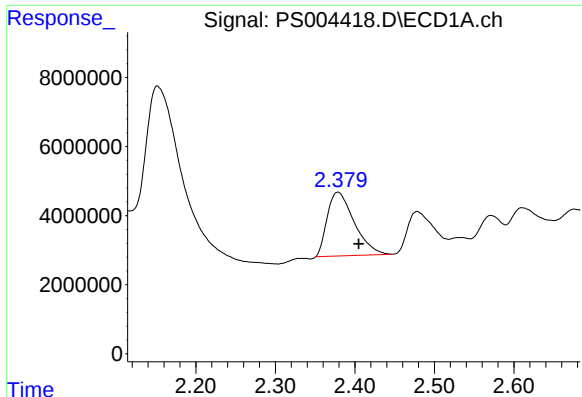

#1 Dalapon


R.T.: 2.379 min
Delta R.T.: -0.026 min
Response: 43548307
Conc: 55.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119406TB

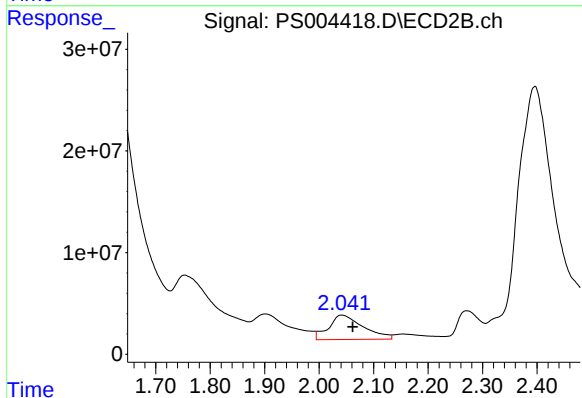


#1 Dalapon

R.T.: 2.041 min
Delta R.T.: -0.020 min
Response: 105725209
Conc: 157.99 ng/ml

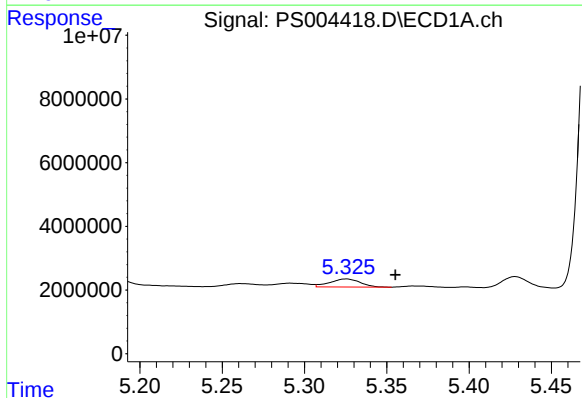


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.325 min
Delta R.T.: -0.030 min
Response: 3260745
Conc: 4.13 ng/ml

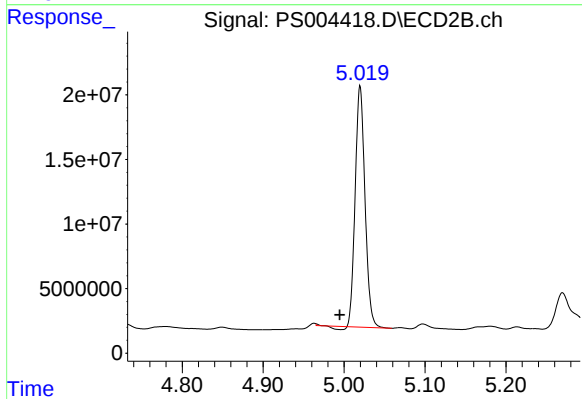

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.020 min
Delta R.T.: 0.025 min
Response: 156073065
Conc: 253.89 ng/ml

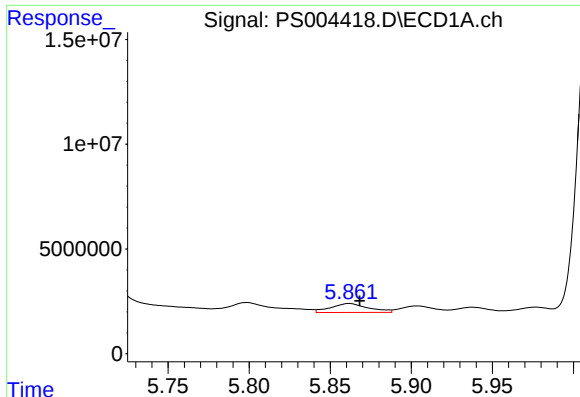

#3 4-Nitrophenol


R.T.: 5.862 min
Delta R.T.: -0.006 min
Response: 6901456
Conc: 27.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119406TB

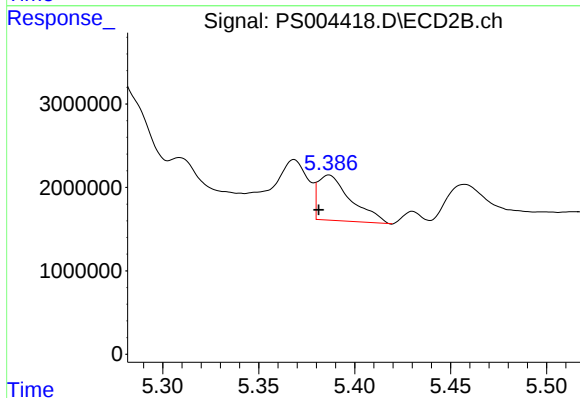


#3 4-Nitrophenol

R.T.: 5.386 min
Delta R.T.: 0.005 min
Response: 6457364
Conc: 26.11 ng/ml

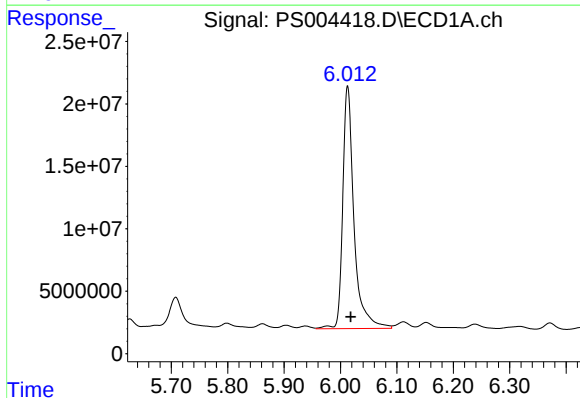


#4 2,4-DCAA

R.T.: 6.013 min
Delta R.T.: -0.005 min
Response: 268846866
Conc: 427.11 ng/ml

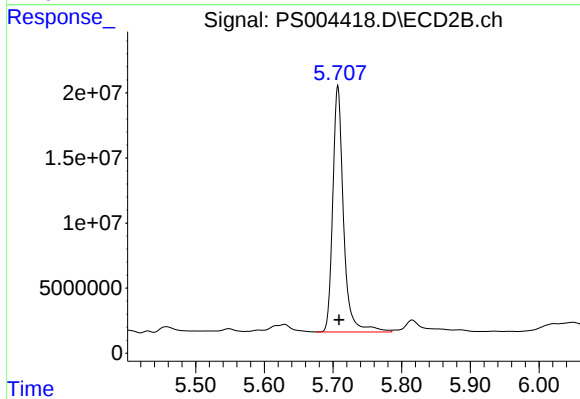

#4 2,4-DCAA


R.T.: 5.707 min
Delta R.T.: -0.002 min
Response: 206609828
Conc: 428.40 ng/ml

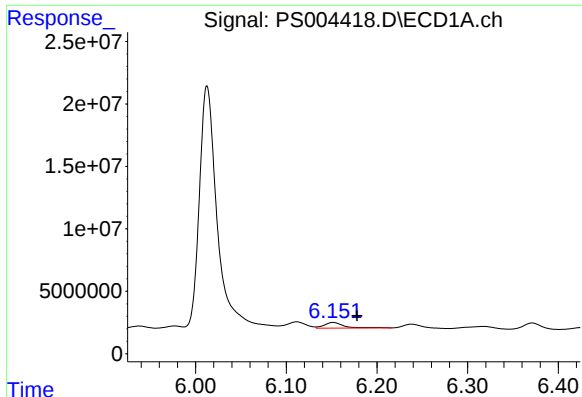

#5 DICAMBA


R.T.: 6.152 min
Delta R.T.: -0.026 min
Response: 6771400
Conc: 2.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119406TB

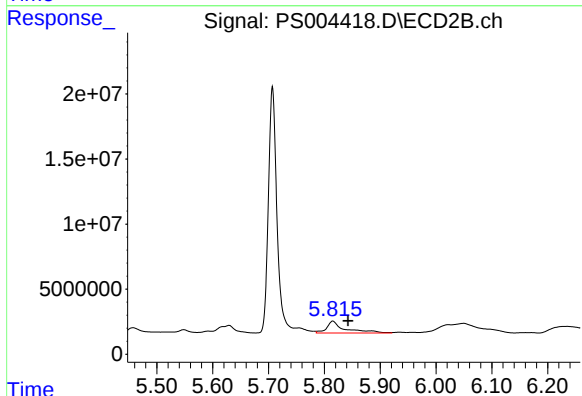


#5 DICAMBA

R.T.: 5.815 min
Delta R.T.: -0.027 min
Response: 21046600
Conc: 11.24 ng/ml

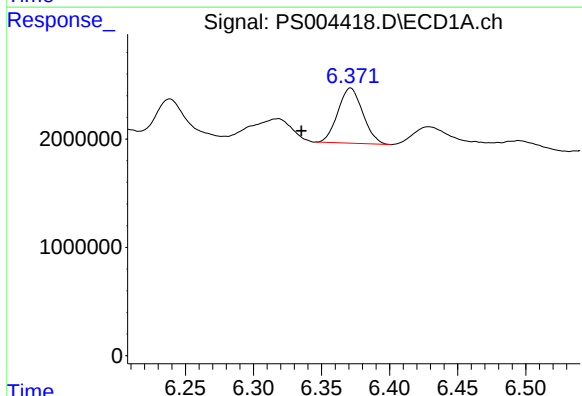


#6 MCPP

R.T.: 6.371 min
Delta R.T.: 0.036 min
Response: 6465527
Conc: 3.74 ug/ml

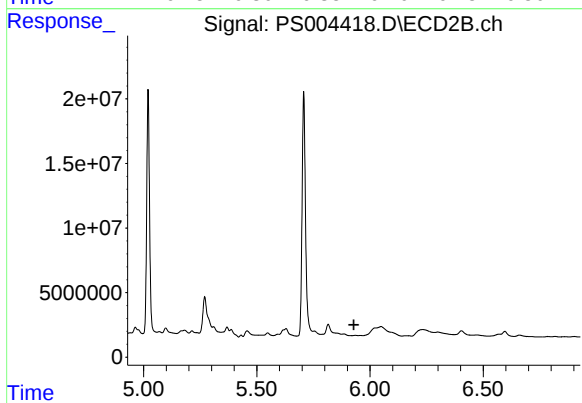

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

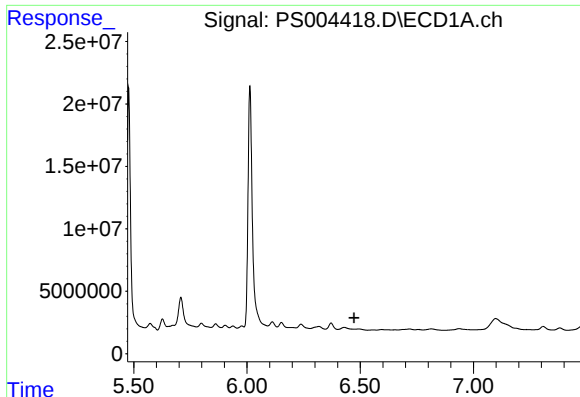

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB119406TB

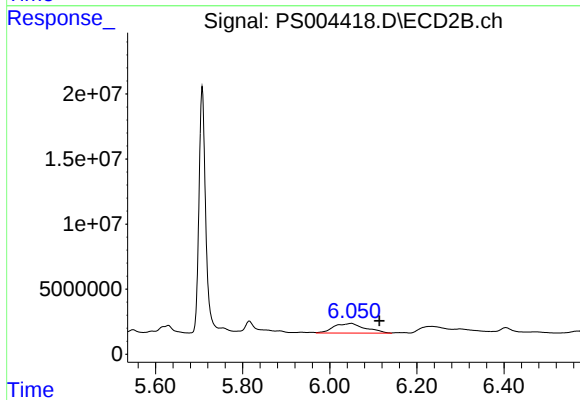


#7 MCPA

R.T.: 6.049 min
Delta R.T.: -0.065 min
Response: 37381508
Conc: 18.82 ug/ml

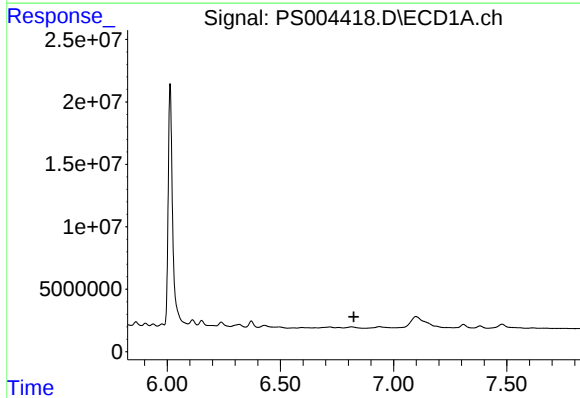


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

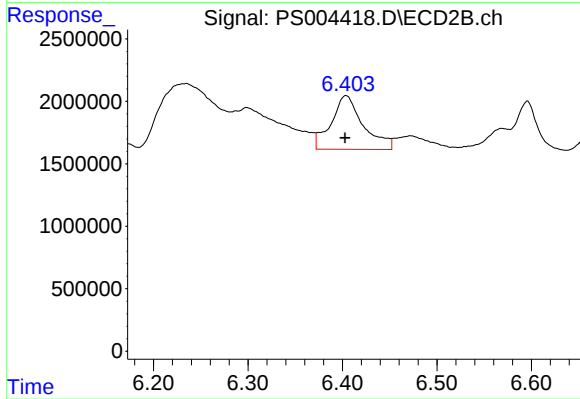

#8 DICHLORPROP


R.T.: 6.404 min
Delta R.T.: 0.001 min
Response: 10141511
Conc: 21.55 ng/ml

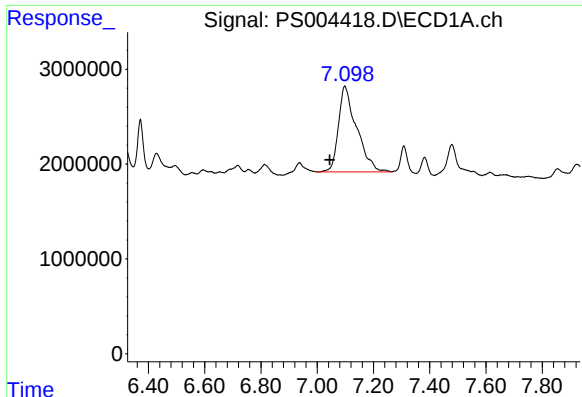

#9 2,4-D


R.T.: 7.098 min
Delta R.T.: 0.053 min
Response: 40613011
Conc: 71.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119406TB

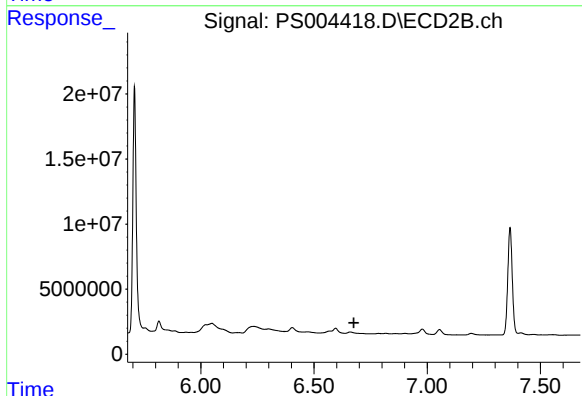


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

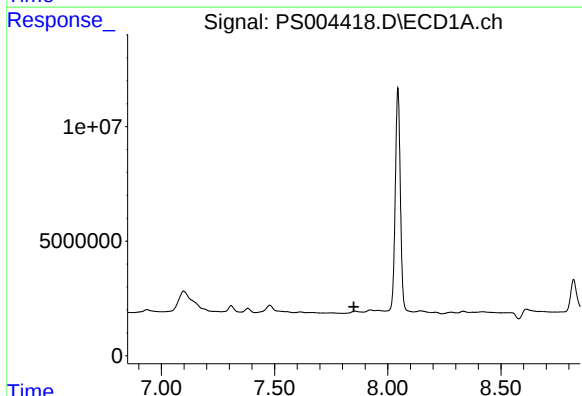

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

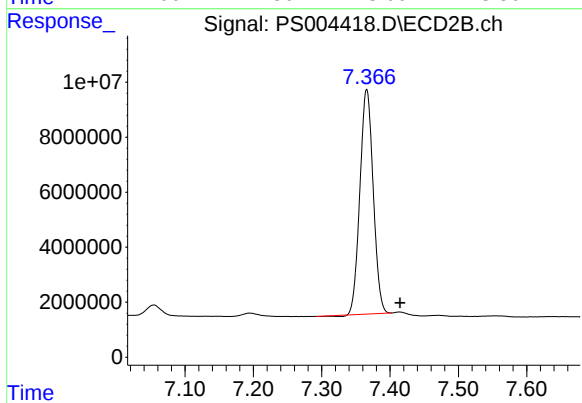

#11 2,4,5-TP (SILVEX)

R.T.: 7.366 min
Delta R.T.: -0.049 min
Response: 109964537
Conc: 41.85 ng/ml