

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
 Data File : PS004424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 18:49
 Operator : EI\SJ
 Sample : K2627-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:02:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.010	5.705	271.0E6	202.8E6	430.595	420.574
Target Compounds							
1) T	Dalapon	2.378	2.041	62233396	198.4E6	79.199	296.458 #
2) T	3,5-DICHL...	5.425	4.976	6337289	8589870	8.022	13.973 #
3) T	4-Nitroph...	5.859	5.367	10110221	17544276	40.457	70.927 #
5) T	DICAMBA	6.149	5.813	7141809	9962031	3.003	5.322 #
6) T	MCPD	6.368	0.000	6088068	0	3.523	N.D. #
7) T	MCPA	0.000	6.046	0	34409373	N.D.	17.321
8) T	DICHLORPROP	0.000	6.400	0	16468600	N.D.	34.997
9) T	2,4-D	7.097	0.000	42227238	0	74.220	N.D. #
10) T	Pentachlo...	7.378	7.055	4110389	3620150	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	7.364	0	122.6E6	N.D.	46.650
12) T	2,4,5-T	0.000	7.841	0	5432502	N.D.	2.415
15) T	Picloram	0.000	9.541	0	9699311	N.D.	2.652
16) T	DCPA	0.000	9.541	0	9699311	N.D.	2.949



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050219\
Data File : PS004424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 18:49
Operator : EI\SJ
Sample : K2627-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
WC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:02:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

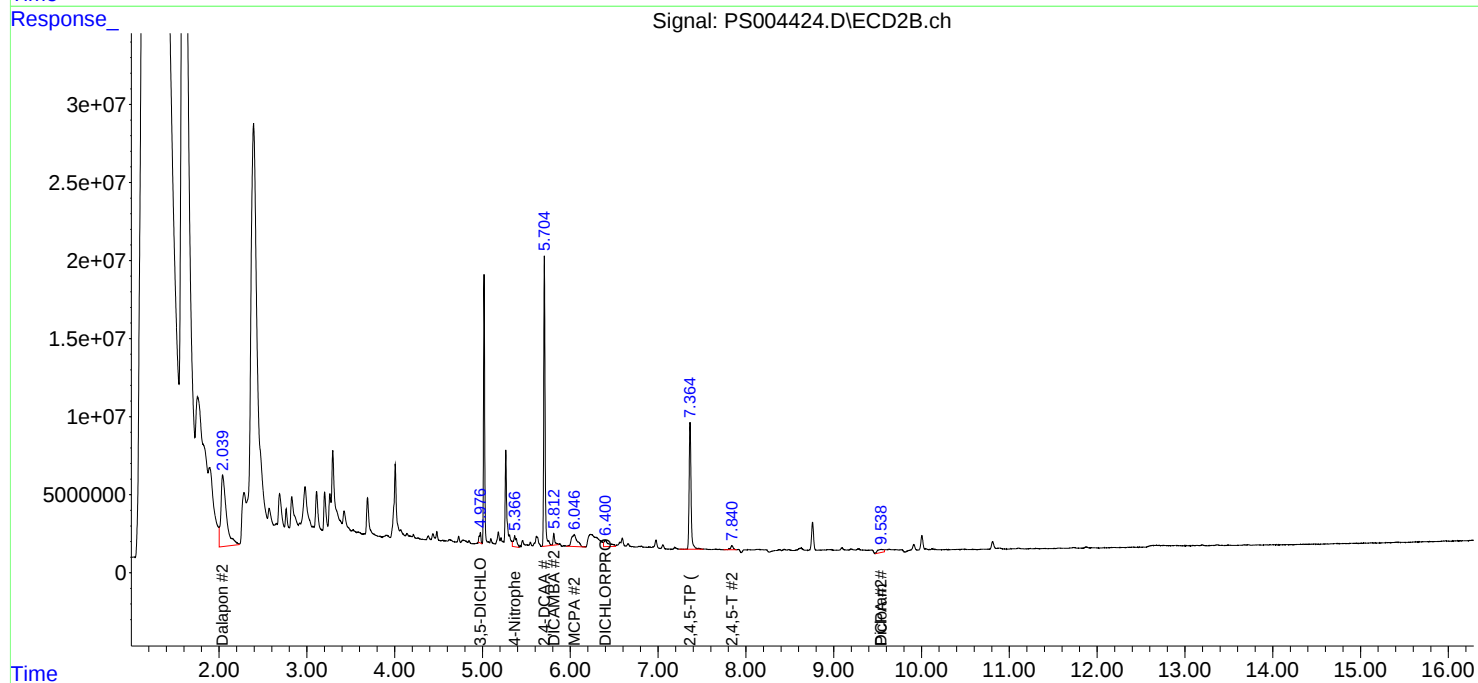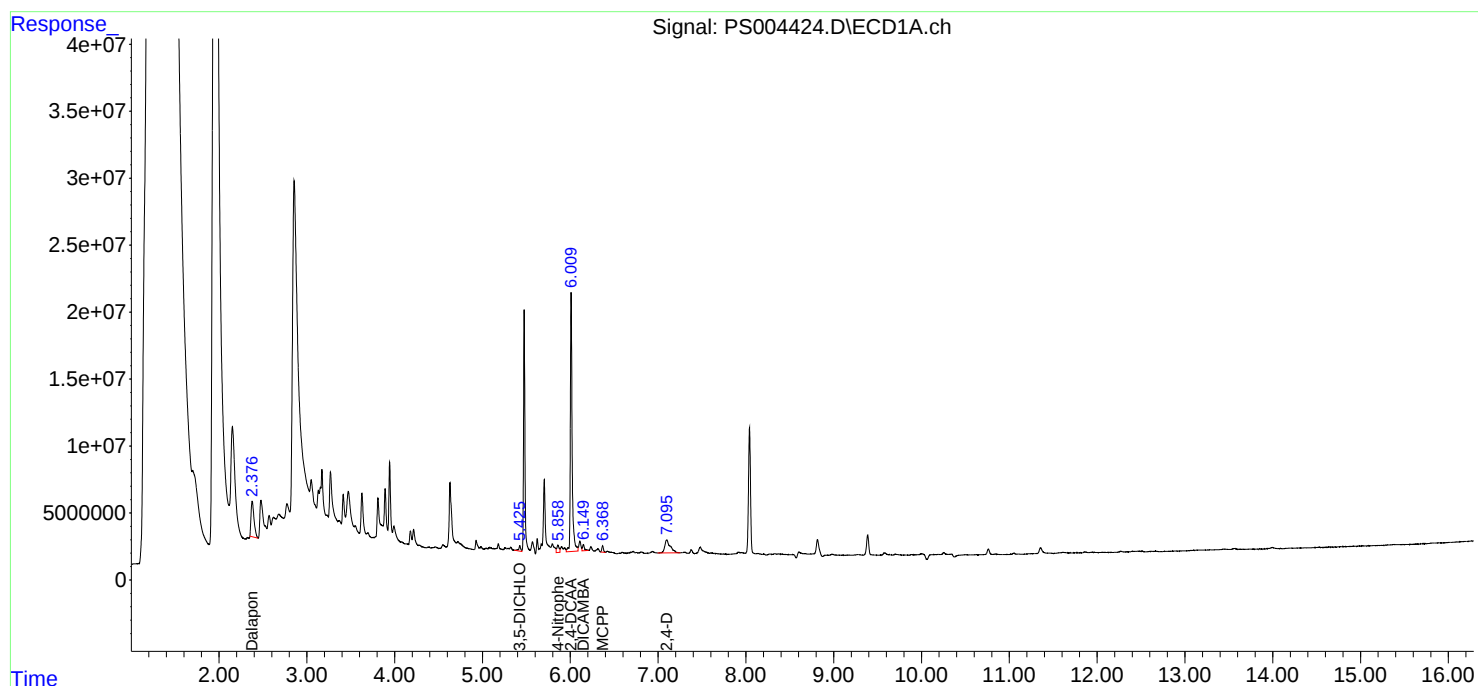


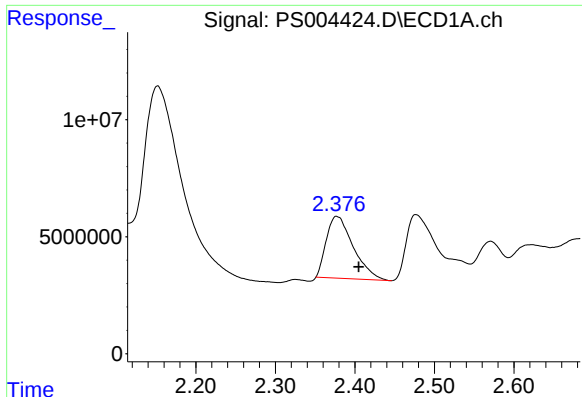

#1 Dalapon


R.T.: 2.378 min
Delta R.T.: -0.027 min
Response: 62233396
Conc: 79.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-1

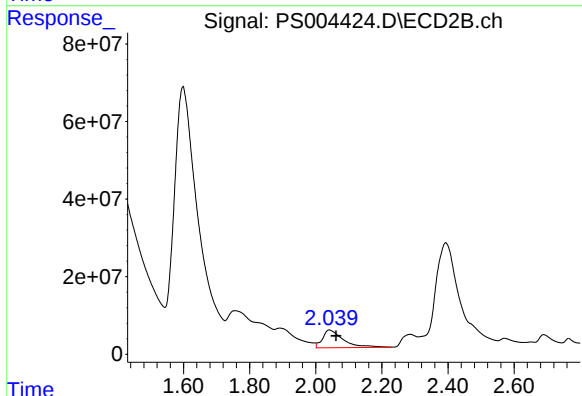


#1 Dalapon

R.T.: 2.041 min
Delta R.T.: -0.021 min
Response: 198385606
Conc: 296.46 ng/ml

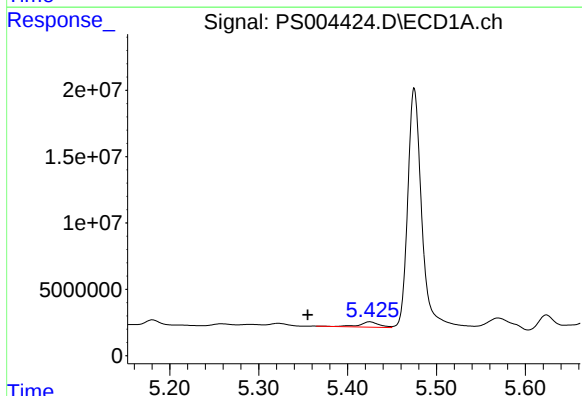


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.425 min
Delta R.T.: 0.070 min
Response: 6337289
Conc: 8.02 ng/ml

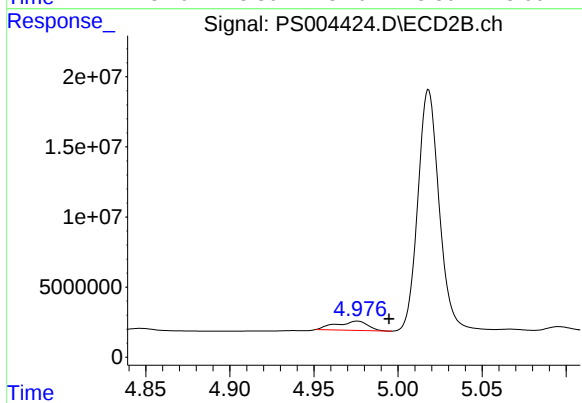

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.976 min
Delta R.T.: -0.019 min
Response: 8589870
Conc: 13.97 ng/ml

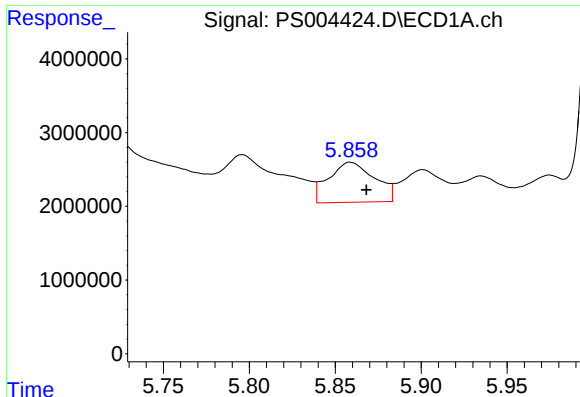

#3 4-Nitrophenol


R.T.: 5.859 min
Delta R.T.: -0.009 min
Response: 10110221
Conc: 40.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-1

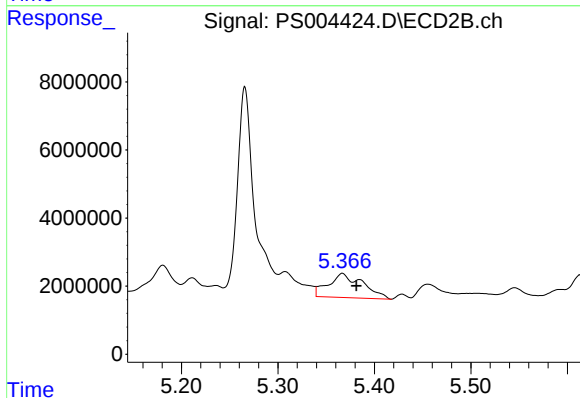


#3 4-Nitrophenol

R.T.: 5.367 min
Delta R.T.: -0.015 min
Response: 17544276
Conc: 70.93 ng/ml

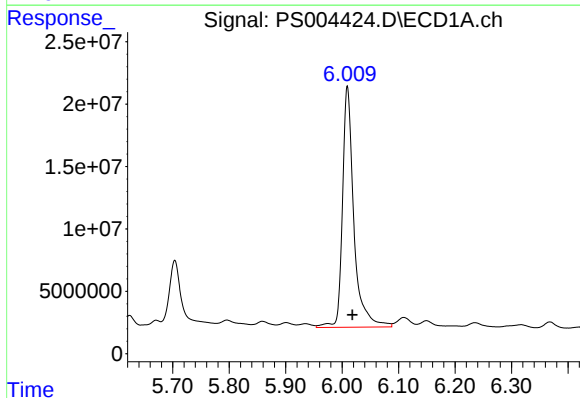


#4 2,4-DCAA

R.T.: 6.010 min
Delta R.T.: -0.009 min
Response: 271041278
Conc: 430.60 ng/ml

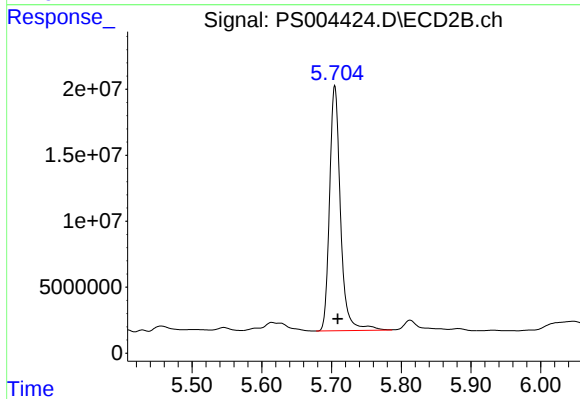

#4 2,4-DCAA


R.T.: 5.705 min
Delta R.T.: -0.004 min
Response: 202835536
Conc: 420.57 ng/ml

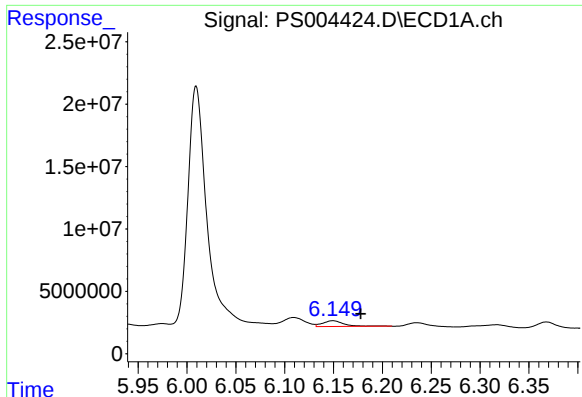

#5 DICAMBA


R.T.: 6.149 min
Delta R.T.: -0.029 min
Response: 7141809
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-1

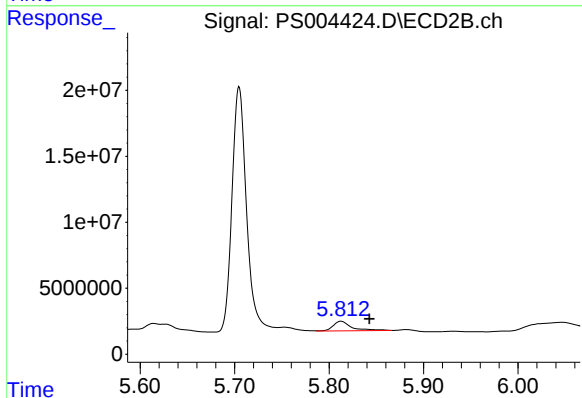


#5 DICAMBA

R.T.: 5.813 min
Delta R.T.: -0.030 min
Response: 9962031
Conc: 5.32 ng/ml

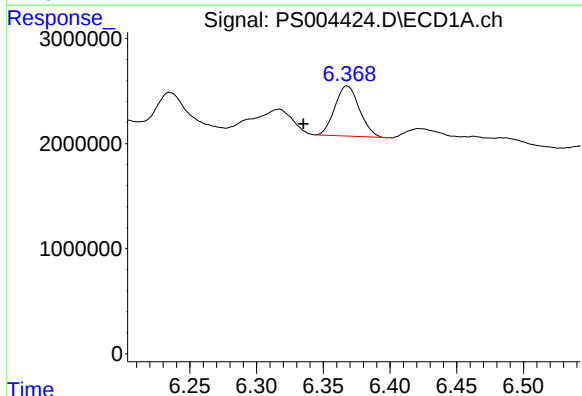


#6 MCP

R.T.: 6.368 min
Delta R.T.: 0.033 min
Response: 6088068
Conc: 3.52 ug/ml

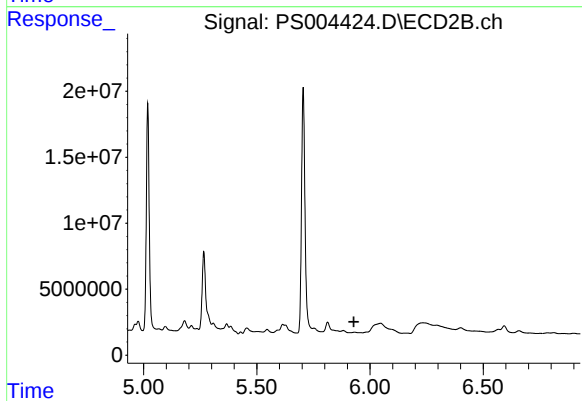

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

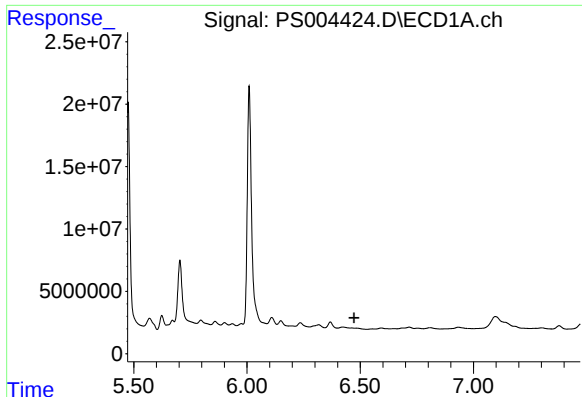

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-1

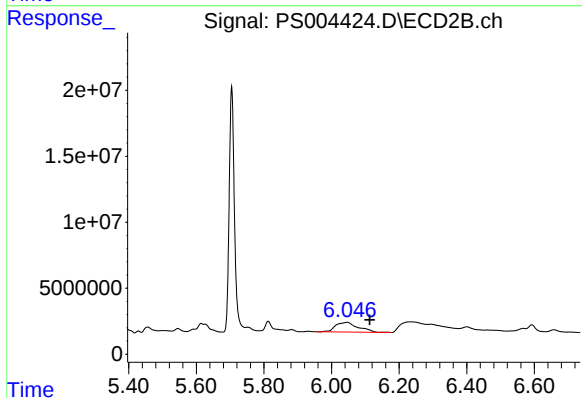


#7 MCPA

R.T.: 6.046 min
Delta R.T.: -0.068 min
Response: 34409373
Conc: 17.32 ug/ml

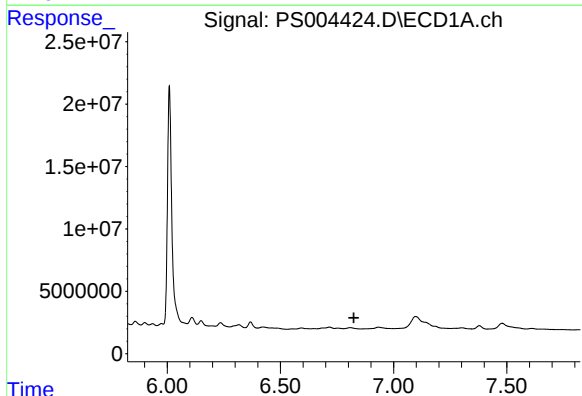


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

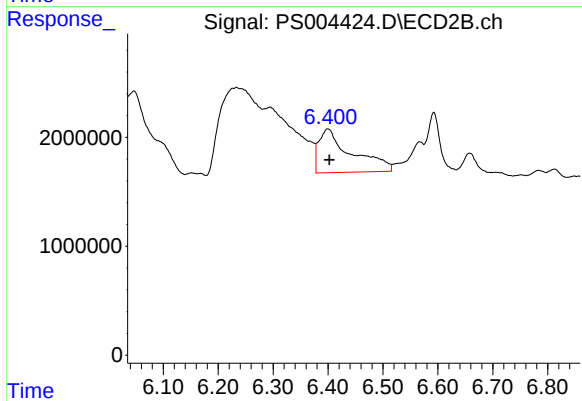

#8 DICHLORPROP


R.T.: 6.400 min
Delta R.T.: -0.003 min
Response: 16468600
Conc: 35.00 ng/ml

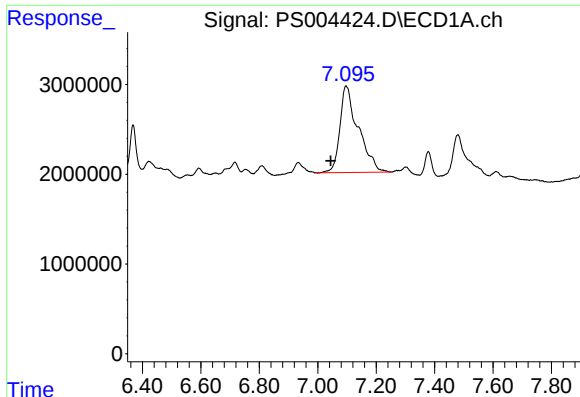

#9 2,4-D


R.T.: 7.097 min
Delta R.T.: 0.052 min
Response: 42227238
Conc: 74.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-1

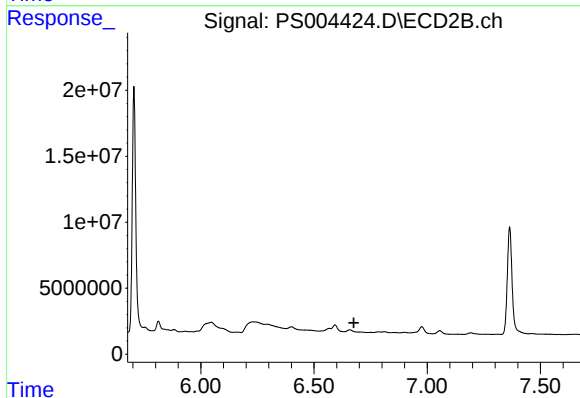


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

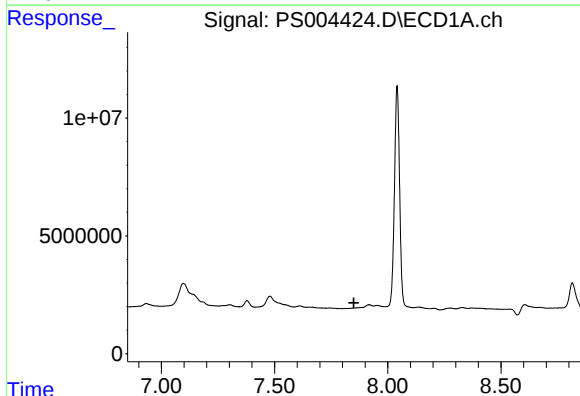


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

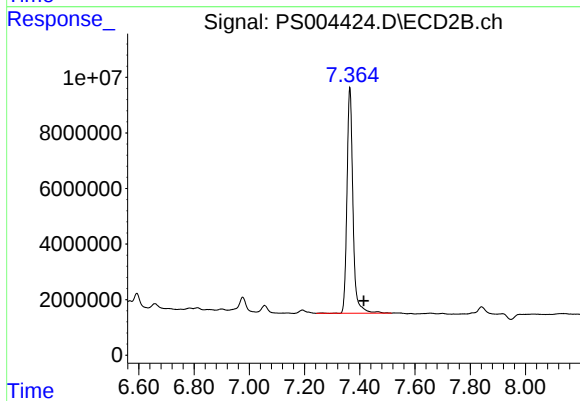

#11 2,4,5-TP (SILVEX)


R.T.: 7.364 min
Delta R.T.: -0.051 min
Response: 122569494
Conc: 46.65 ng/ml

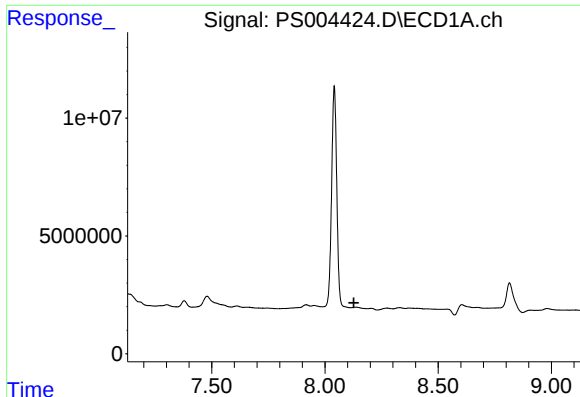

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-1

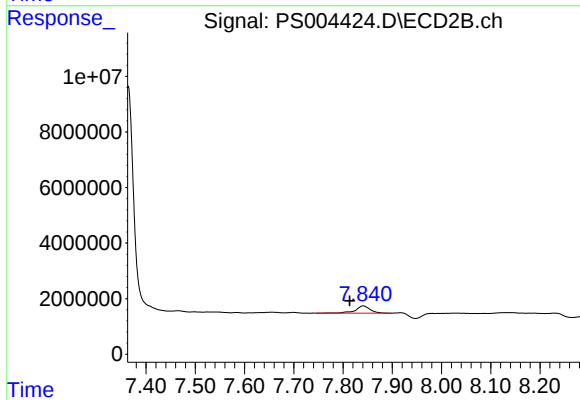


#12 2,4,5-T

R.T.: 7.841 min
Delta R.T.: 0.027 min
Response: 5432502
Conc: 2.42 ng/ml

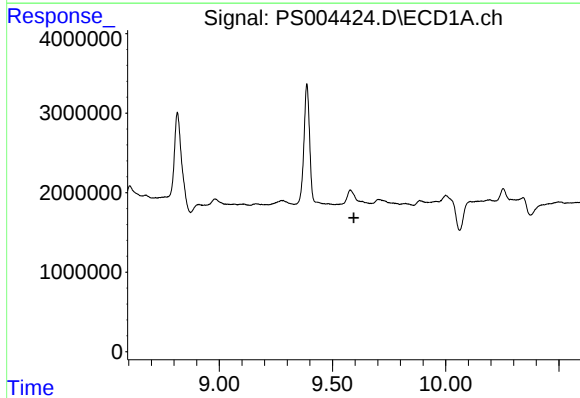


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.595 min
Response: 0
Conc: N.D.

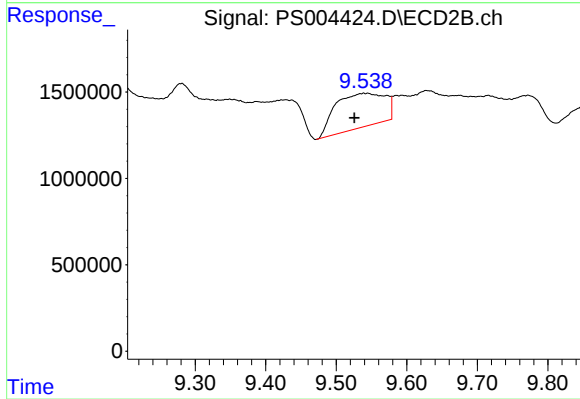

#15 Picloram


R.T.: 9.541 min
Delta R.T.: 0.015 min
Response: 9699311
Conc: 2.65 ng/ml

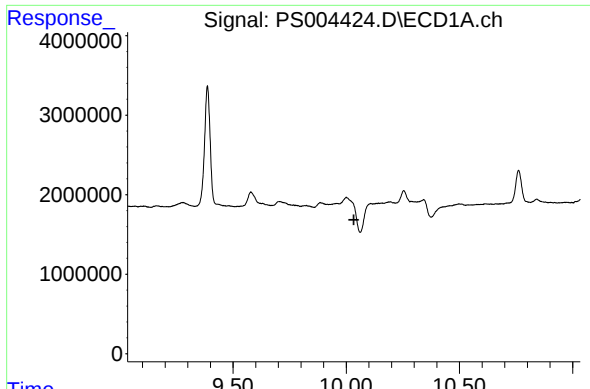

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-1

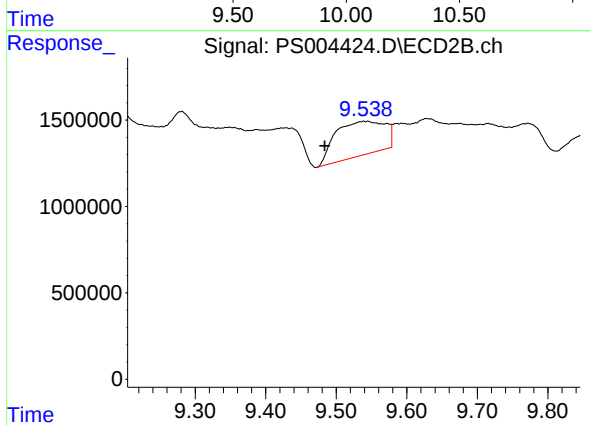

#16 DCPA

R.T.: 9.541 min
Delta R.T.: 0.057 min
Response: 9699311
Conc: 2.95 ng/ml