

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050319\
 Data File : PS004434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2019 13:59
 Operator : EI\SJ
 Sample : PB119177BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB119177BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 15:03:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.016	5.709	174.8E6	118.8E6	277.648	246.372
Target Compounds							
1) T	Dalapon	2.380	2.041	39543561	68338074	50.323	102.121 #
2) T	3,5-DICHL...	5.327	4.979	7428433	10130827	9.403	16.480 #
3) T	4-Nitroph...	5.862	5.370	13293228	13228630	53.194	53.480
5) T	DICAMBA	6.154	5.816	13358469	12506422	5.618	6.682
6) T	MCPD	6.372	0.000	10041006	0	5.811	N.D. #
7) T	MCPA	6.429	0.000	12275881	0	4.765	N.D. #
8) T	DICHLORPROP	6.759	6.406	5200209	8933435	9.086	18.984 #
9) T	2,4-D	7.103	0.000	43131278	0	67.283	N.D. #
11) T	2,4,5-TP ...	0.000	7.368	0	111.9E6	N.D.	42.571
12) T	2,4,5-T	0.000	7.842	0	6012334	N.D.	2.673
15) T	Picloram	9.635	9.542	12028092	9230747	2.841	2.524
16) T	DCPA	0.000	9.542	0	9230747	N.D.	2.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050319\
Data File : PS004434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2019 13:59
Operator : EI\SJ
Sample : PB119177BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB119177BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 15:03:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

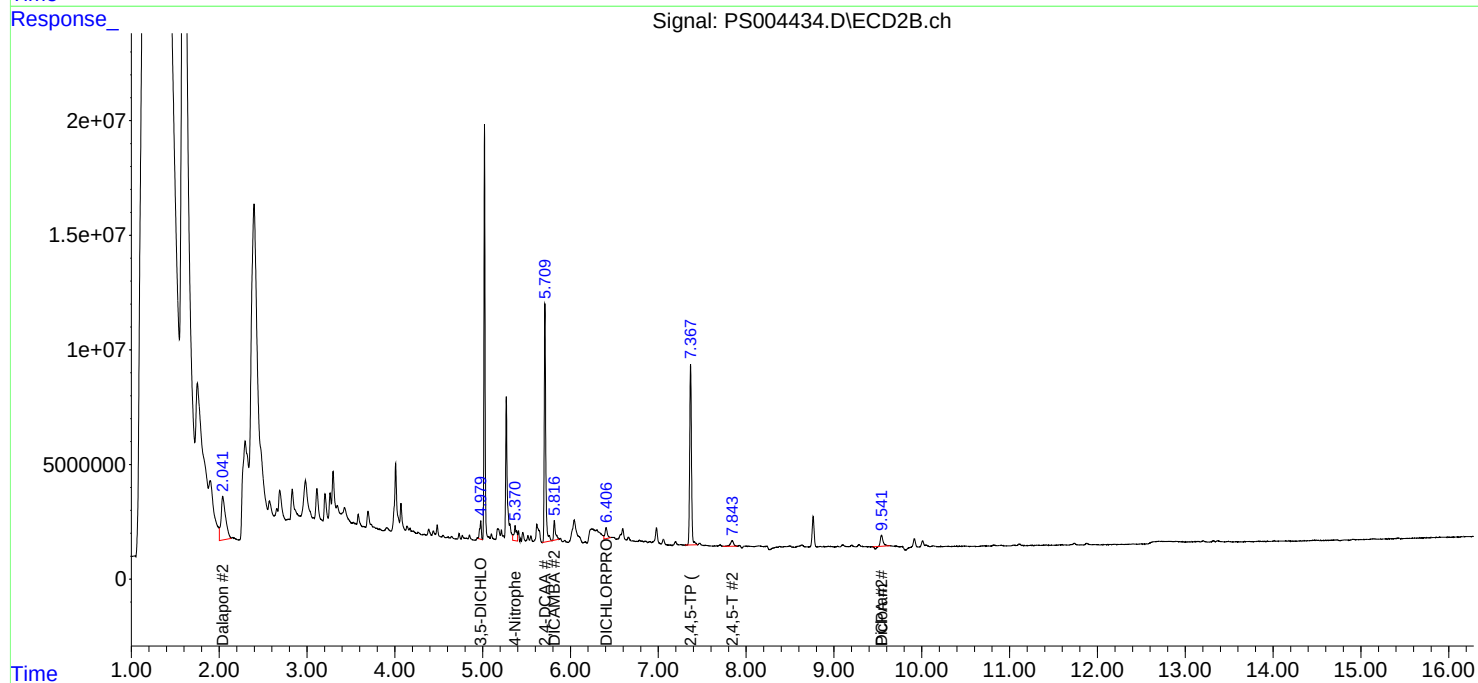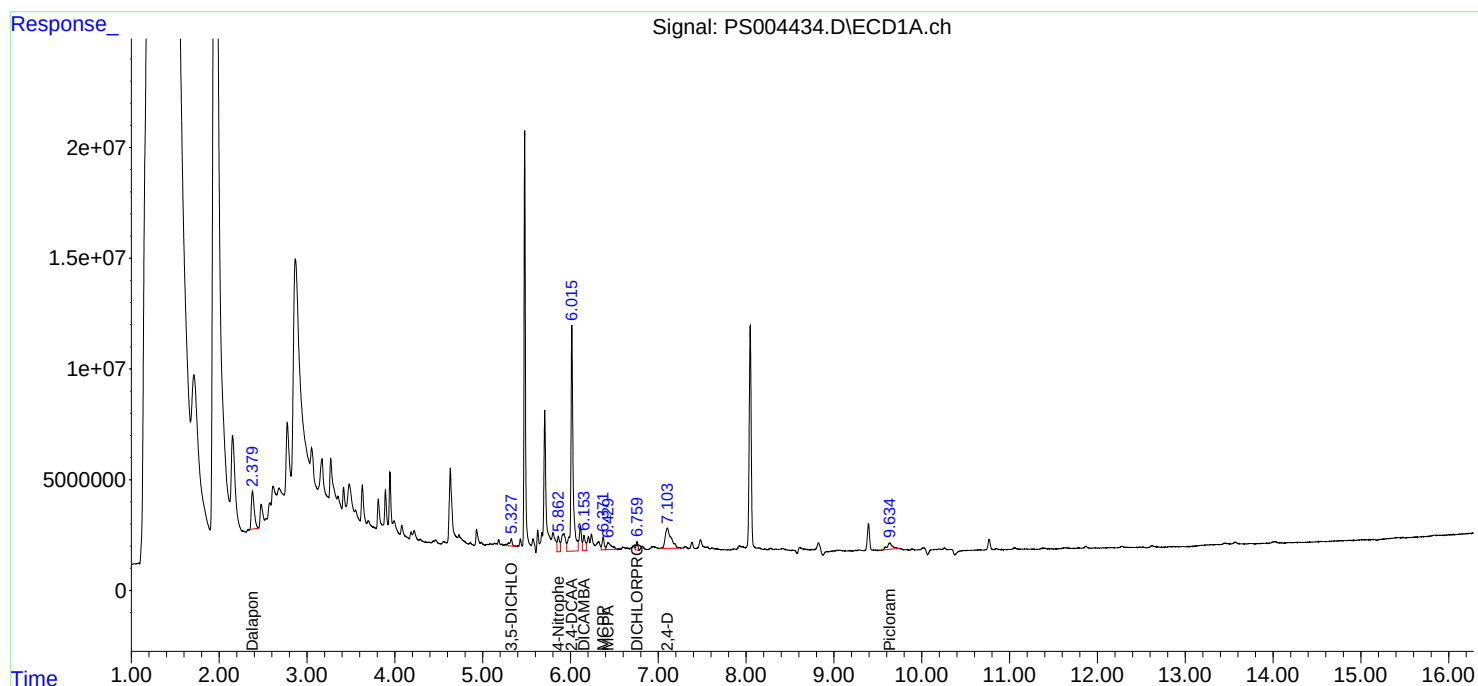


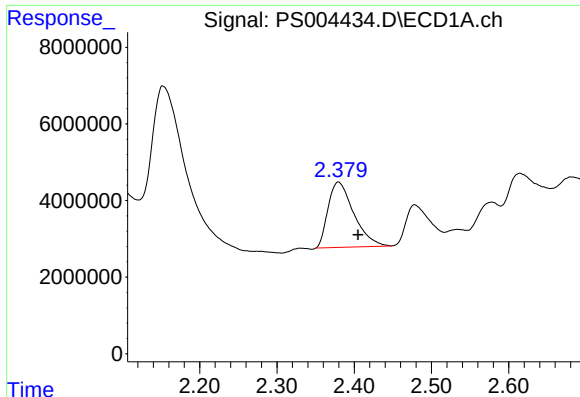

#1 Dalapon


R.T.: 2.380 min
Delta R.T.: -0.025 min
Response: 39543561
Conc: 50.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119177BL

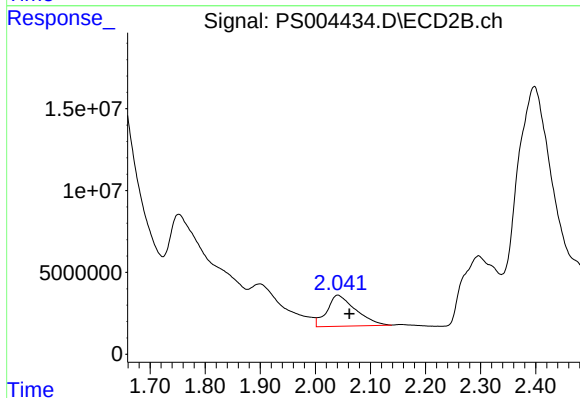


#1 Dalapon

R.T.: 2.041 min
Delta R.T.: -0.021 min
Response: 68338074
Conc: 102.12 ng/ml

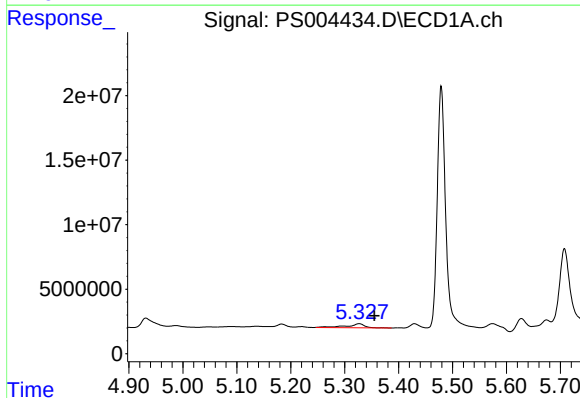


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.327 min
Delta R.T.: -0.028 min
Response: 7428433
Conc: 9.40 ng/ml

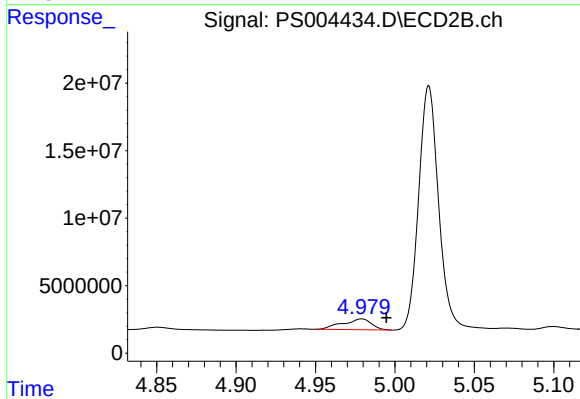

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.979 min
Delta R.T.: -0.016 min
Response: 10130827
Conc: 16.48 ng/ml

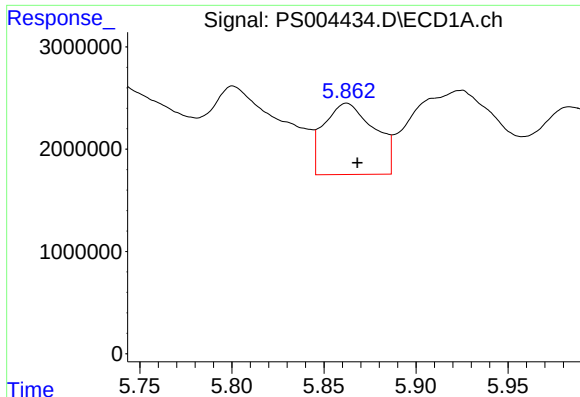

#3 4-Nitrophenol


R.T.: 5.862 min
Delta R.T.: -0.006 min
Response: 13293228
Conc: 53.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119177BL

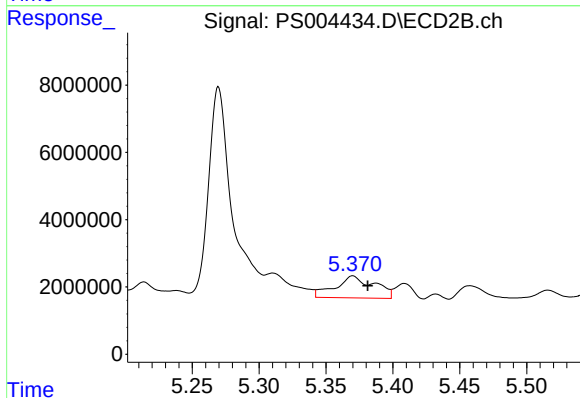


#3 4-Nitrophenol

R.T.: 5.370 min
Delta R.T.: -0.011 min
Response: 13228630
Conc: 53.48 ng/ml

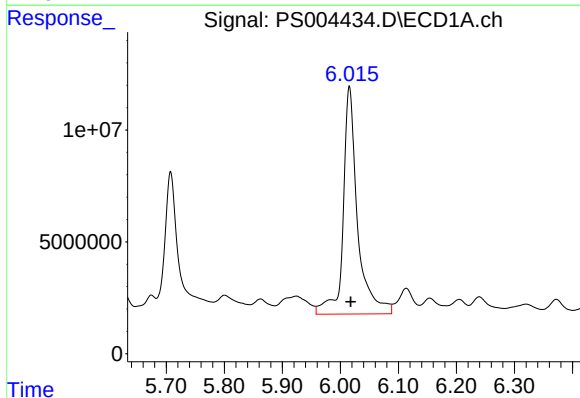


#4 2,4-DCAA

R.T.: 6.016 min
Delta R.T.: -0.002 min
Response: 174767695
Conc: 277.65 ng/ml

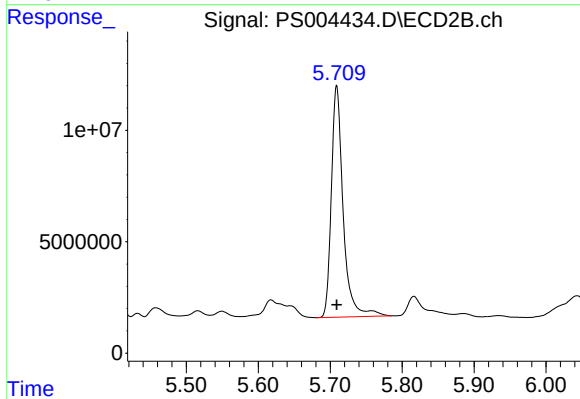

#4 2,4-DCAA


R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 118820836
Conc: 246.37 ng/ml

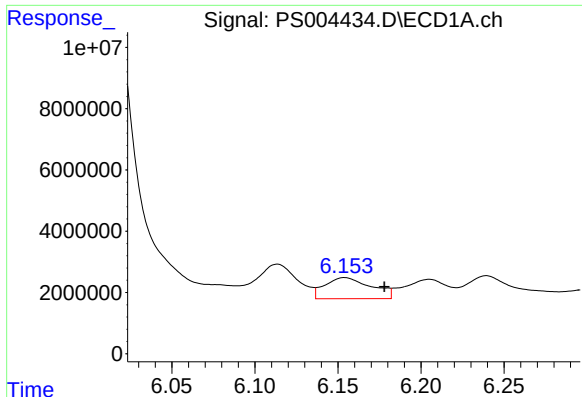

#5 DICAMBA


R.T.: 6.154 min
Delta R.T.: -0.024 min
Response: 13358469
Conc: 5.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119177BL

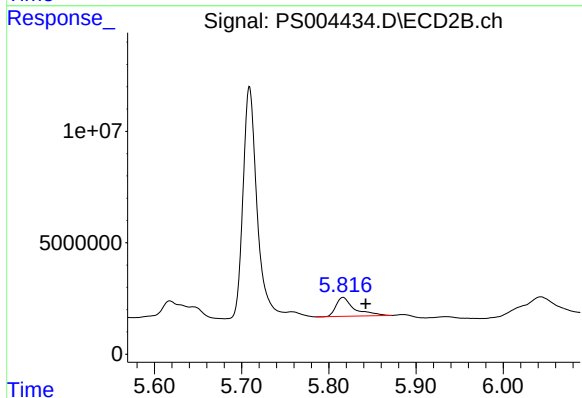


#5 DICAMBA

R.T.: 5.816 min
Delta R.T.: -0.026 min
Response: 12506422
Conc: 6.68 ng/ml

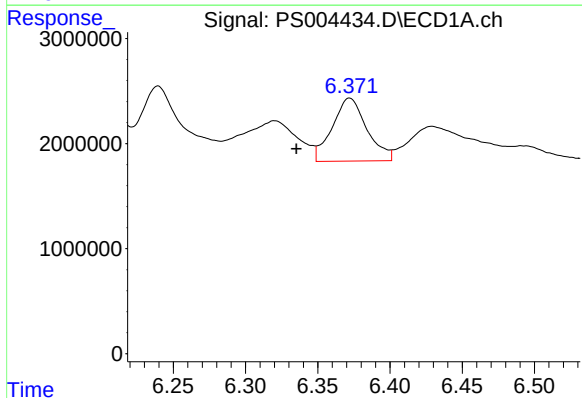


#6 MCP

R.T.: 6.372 min
Delta R.T.: 0.037 min
Response: 10041006
Conc: 5.81 ug/ml

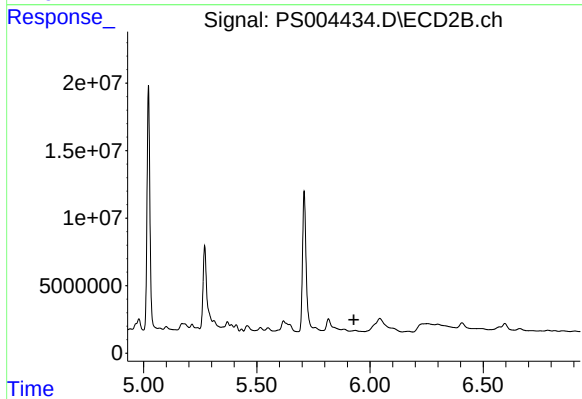

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

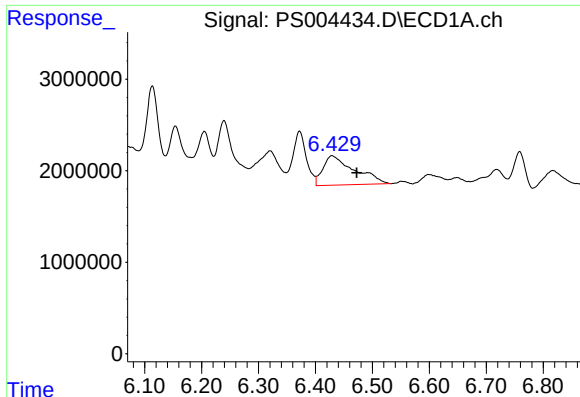

#7 MCPA


R.T.: 6.429 min
Delta R.T.: -0.043 min
Response: 12275881
Conc: 4.76 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB119177BL

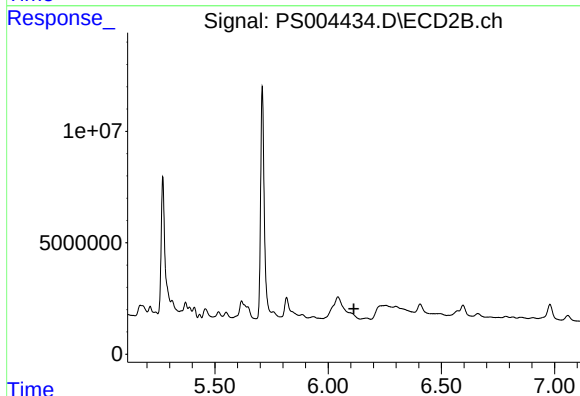


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.114 min
Response: 0
Conc: N.D.

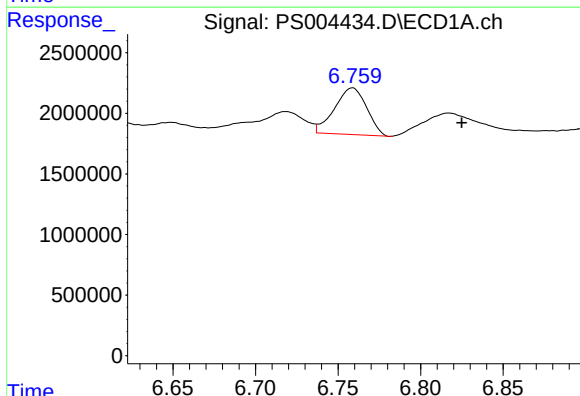


#8 DICHLORPROP

R.T.: 6.759 min
Delta R.T.: -0.066 min
Response: 5200209
Conc: 9.09 ng/ml

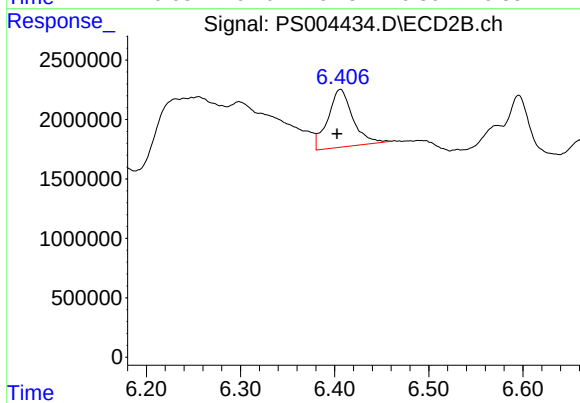

#8 DICHLORPROP


R.T.: 6.406 min
Delta R.T.: 0.003 min
Response: 8933435
Conc: 18.98 ng/ml

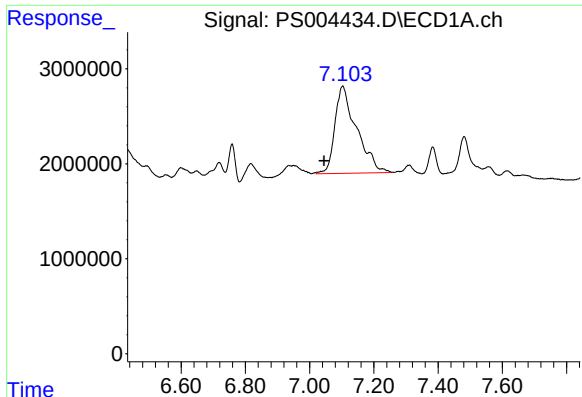

#9 2,4-D


R.T.: 7.103 min
Delta R.T.: 0.058 min
Response: 43131278
Conc: 67.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119177BL

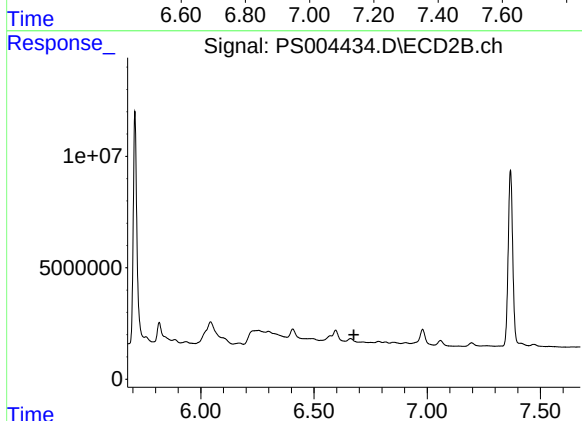


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

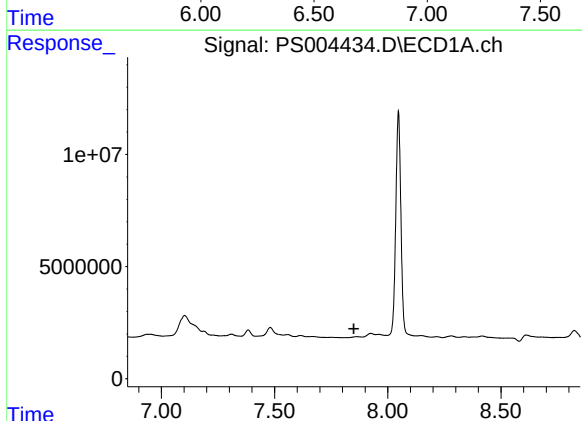


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

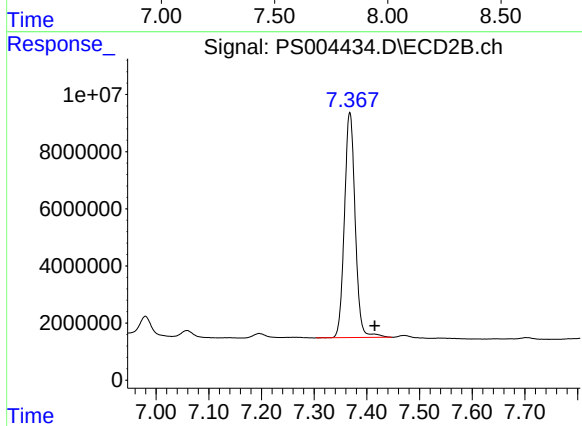

#11 2,4,5-TP (SILVEX)


R.T.: 7.368 min
Delta R.T.: -0.047 min
Response: 111853066
Conc: 42.57 ng/ml

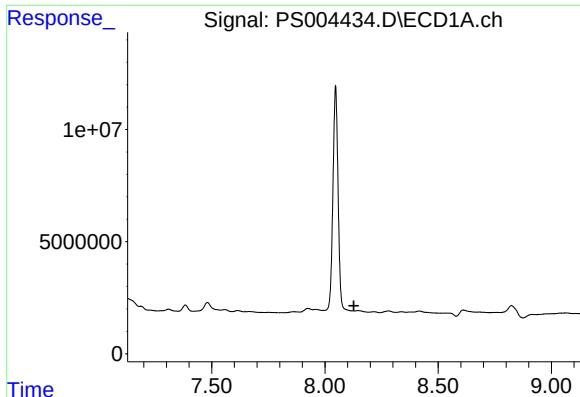

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB119177BL

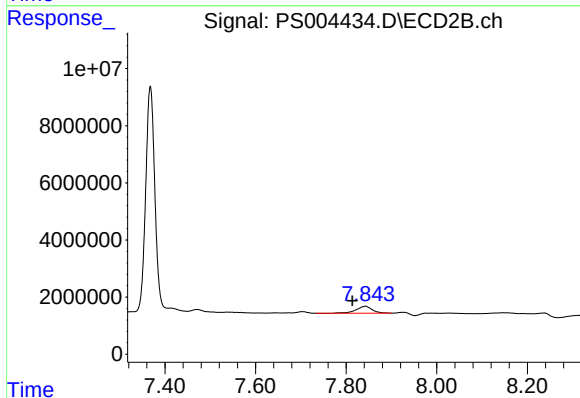


#12 2,4,5-T

R.T.: 7.842 min
Delta R.T.: 0.028 min
Response: 6012334
Conc: 2.67 ng/ml

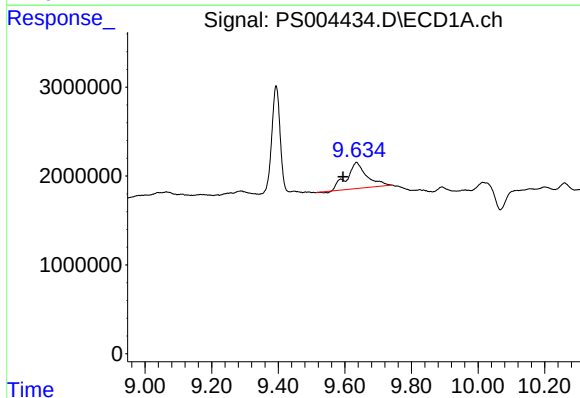


#15 Picloram

R.T.: 9.635 min
Delta R.T.: 0.040 min
Response: 12028092
Conc: 2.84 ng/ml

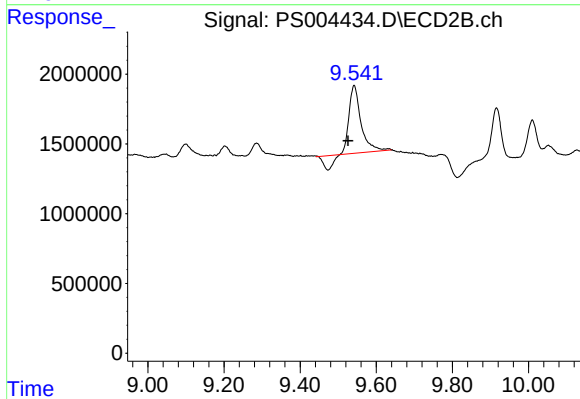

#15 Picloram


R.T.: 9.542 min
Delta R.T.: 0.016 min
Response: 9230747
Conc: 2.52 ng/ml

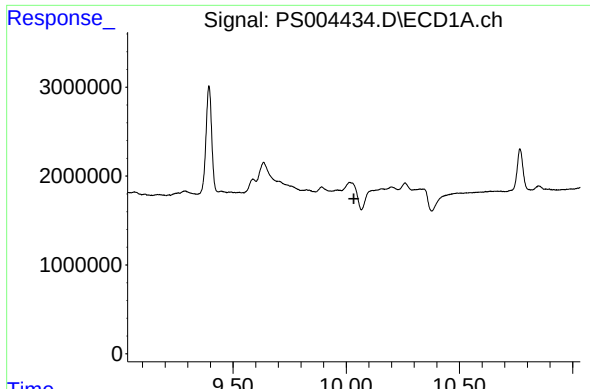

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB119177BL

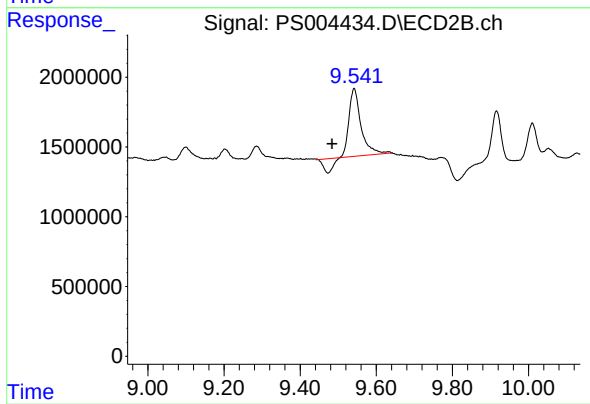

#16 DCPA

R.T.: 9.542 min
Delta R.T.: 0.058 min
Response: 9230747
Conc: 2.81 ng/ml