

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050319\
 Data File : PS004436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2019 14:59
 Operator : EI\SJ
 Sample : PB119280BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB119280BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 15:18:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.014	5.707	172.4E6	120.4E6	273.959	249.699
Target Compounds							
1) T	Dalapon	2.378	2.041	38693272	71896877	49.241	107.439 #
2) T	3,5-DICHL...	5.325	4.978	8225079	11023539	10.411	17.932 #
3) T	4-Nitroph...	5.861	5.369	14266921	14372335	57.091	58.103
5) T	DICAMBA	6.203	5.814	9486893	13880420	3.989	7.416 #
6) T	MCPD	6.370	0.000	9445258	0	5.466	N.D. #
7) T	MCPA	6.427	0.000	12448132	0	4.832	N.D. #
8) T	DICHLORPROP	6.758	6.404	4079603	9739241	7.128	20.696 #
9) T	2,4-D	7.101	0.000	38325017	0	59.786	N.D. #
11) T	2,4,5-TP ...	0.000	7.366	0	108.0E6	N.D.	41.090



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050319\
Data File : PS004436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2019 14:59
Operator : EI\SJ
Sample : PB119280BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB119280BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 15:18:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

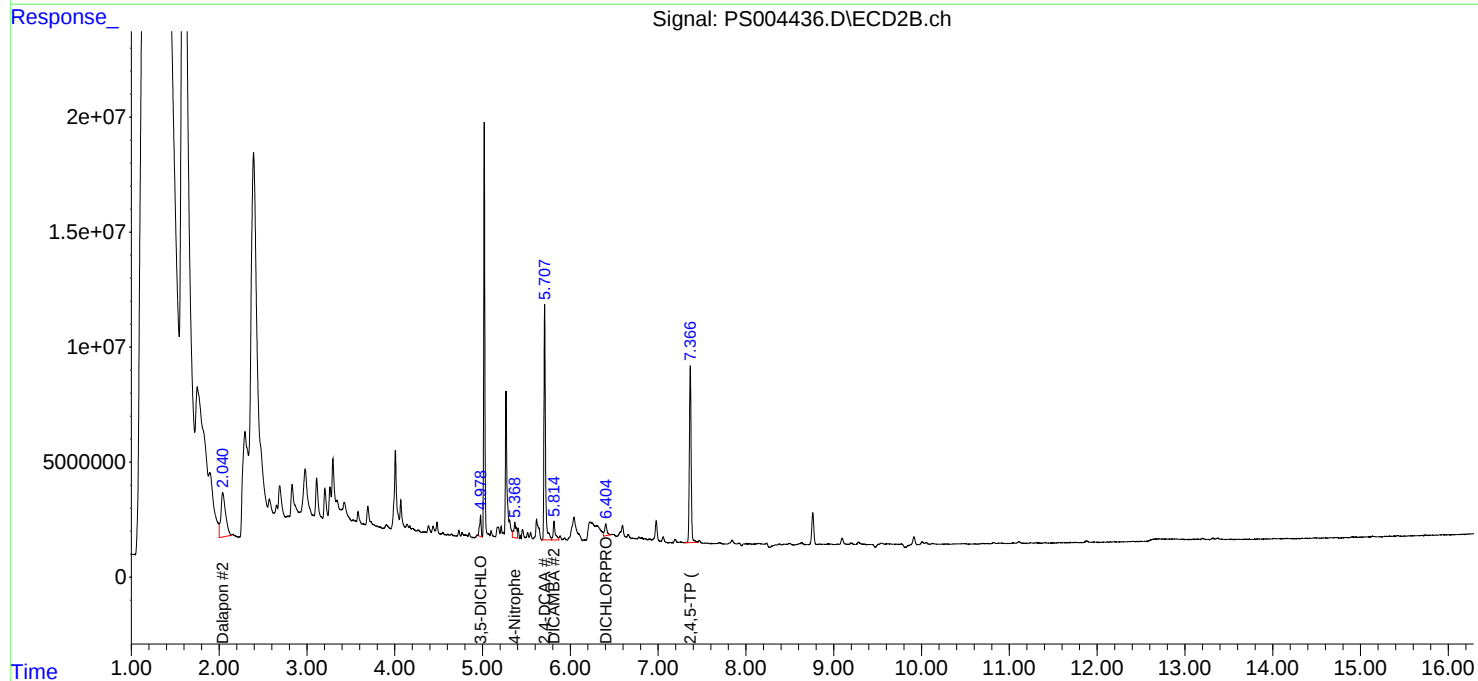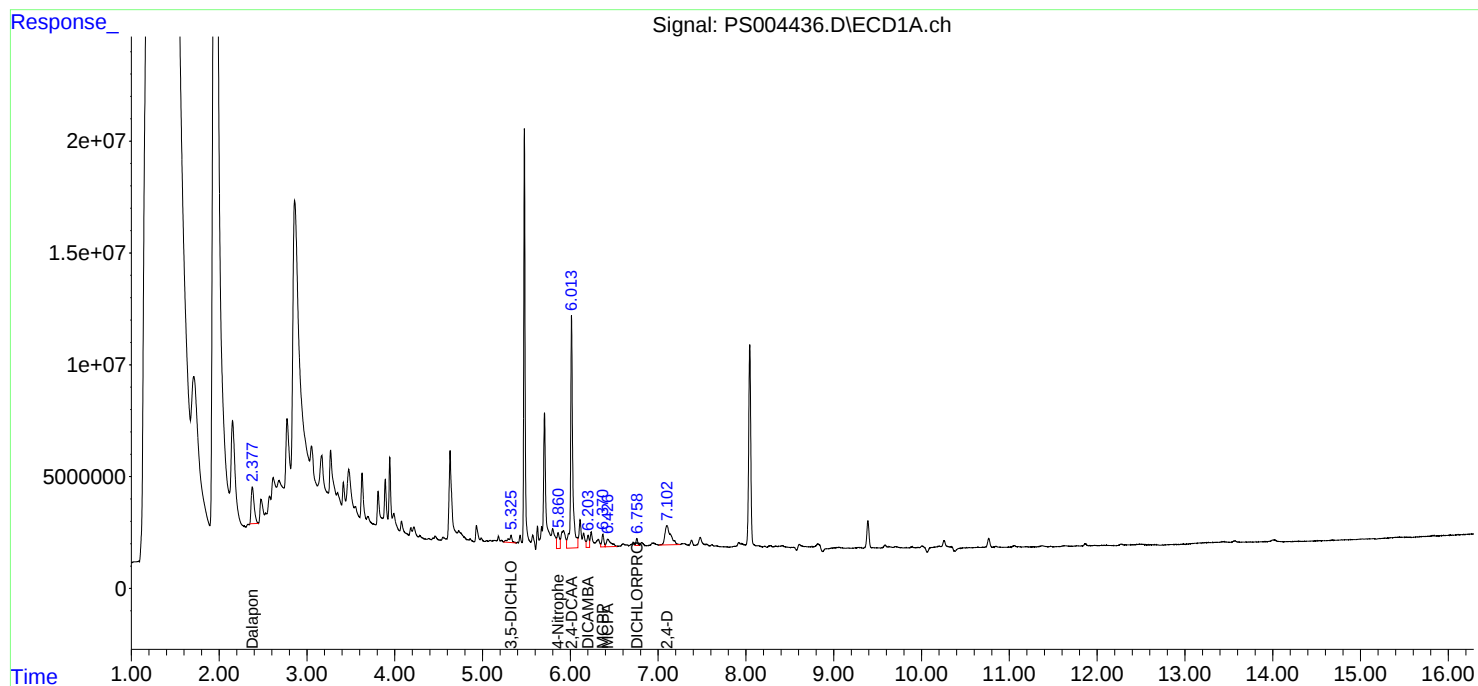


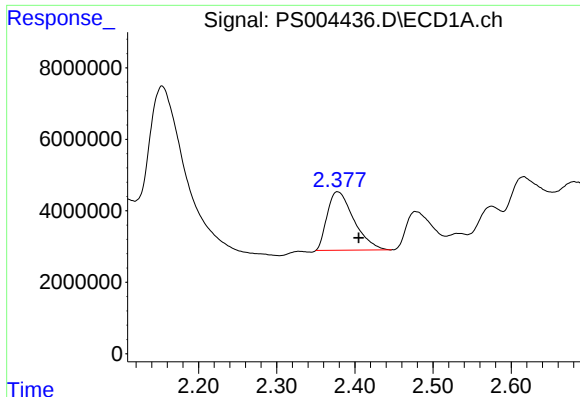

#1 Dalapon


R.T.: 2.378 min
Delta R.T.: -0.027 min
Response: 38693272
Conc: 49.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119280BL

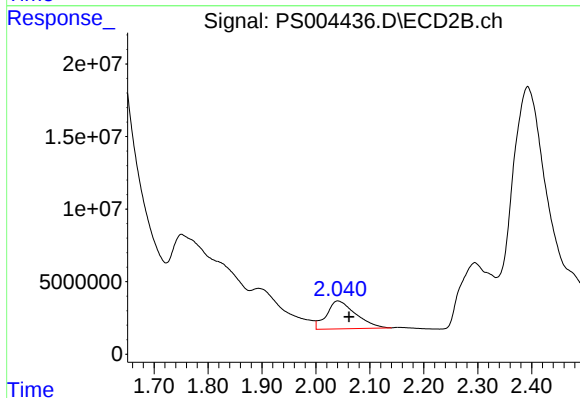


#1 Dalapon

R.T.: 2.041 min
Delta R.T.: -0.021 min
Response: 71896877
Conc: 107.44 ng/ml

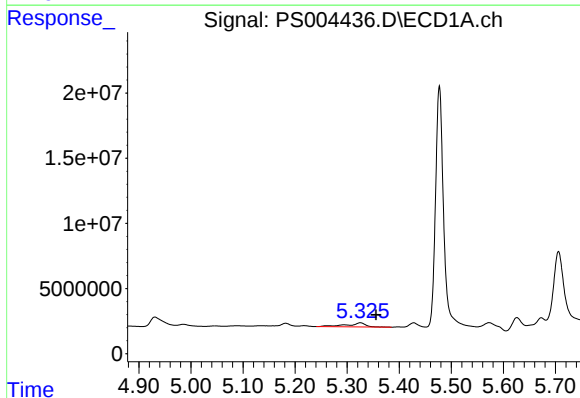


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.325 min
Delta R.T.: -0.030 min
Response: 8225079
Conc: 10.41 ng/ml

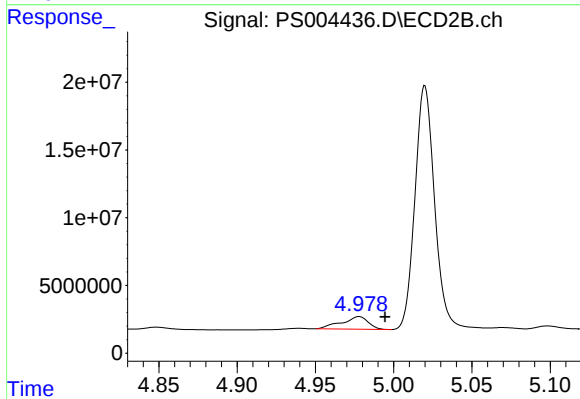

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.978 min
Delta R.T.: -0.017 min
Response: 11023539
Conc: 17.93 ng/ml

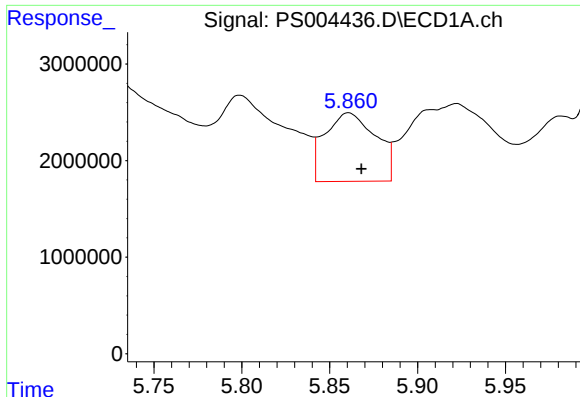

#3 4-Nitrophenol


R.T.: 5.861 min
Delta R.T.: -0.007 min
Response: 14266921
Conc: 57.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119280BL

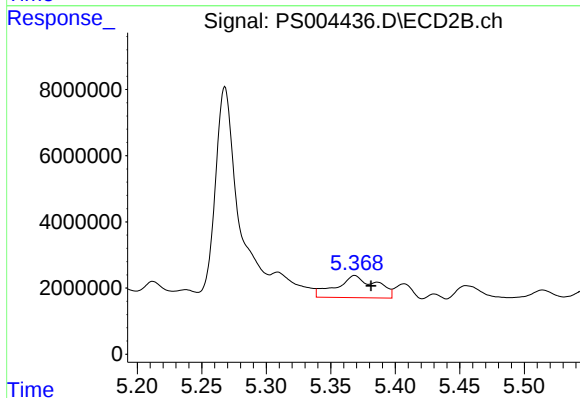


#3 4-Nitrophenol

R.T.: 5.369 min
Delta R.T.: -0.013 min
Response: 14372335
Conc: 58.10 ng/ml

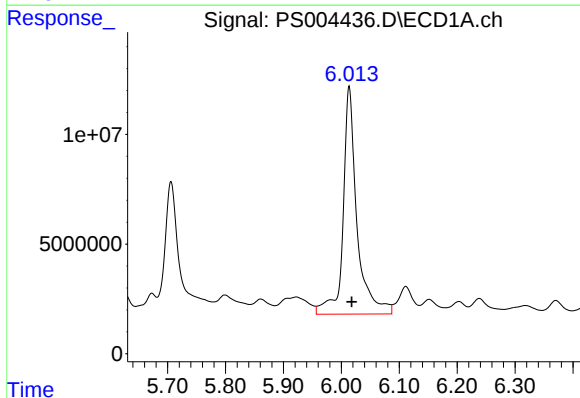


#4 2,4-DCAA

R.T.: 6.014 min
Delta R.T.: -0.004 min
Response: 172445317
Conc: 273.96 ng/ml

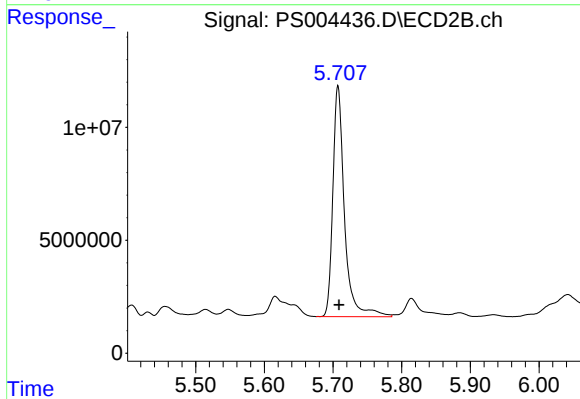

#4 2,4-DCAA


R.T.: 5.707 min
Delta R.T.: -0.001 min
Response: 120425465
Conc: 249.70 ng/ml

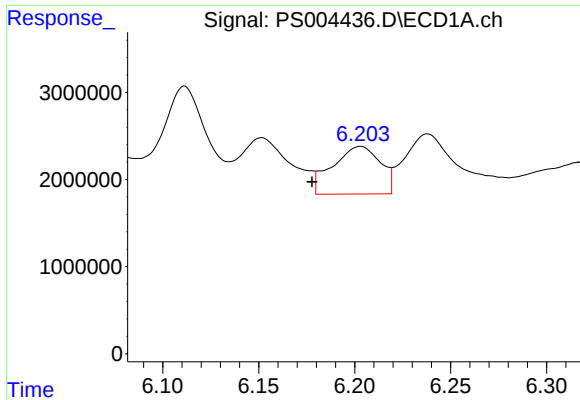

#5 DICAMBA


R.T.: 6.203 min
Delta R.T.: 0.025 min
Response: 9486893
Conc: 3.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119280BL

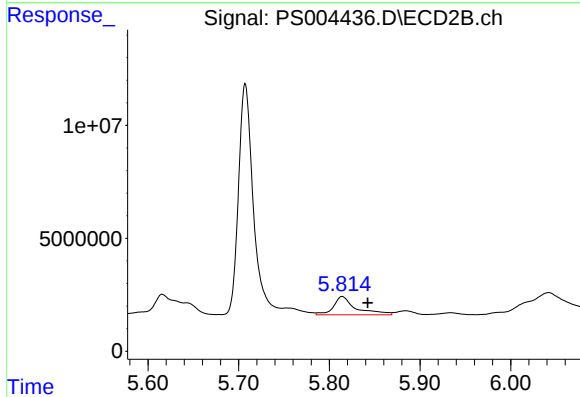


#5 DICAMBA

R.T.: 5.814 min
Delta R.T.: -0.028 min
Response: 13880420
Conc: 7.42 ng/ml

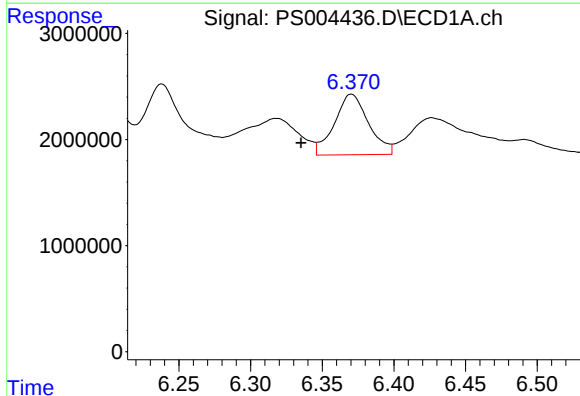


#6 MCP

R.T.: 6.370 min
Delta R.T.: 0.035 min
Response: 9445258
Conc: 5.47 ug/ml

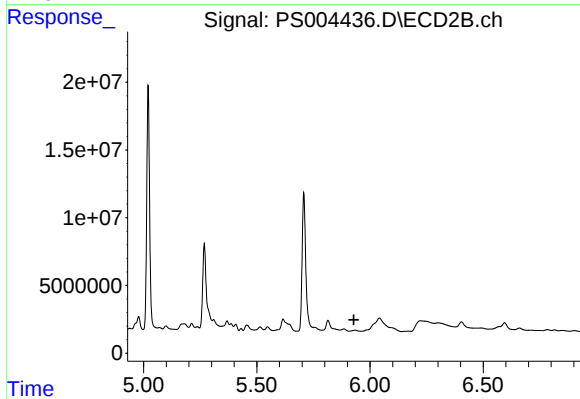

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

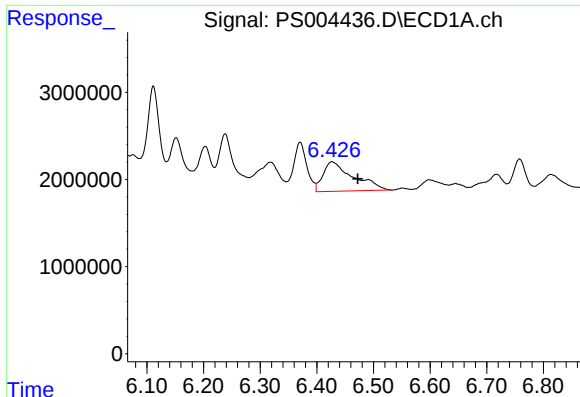

#7 MCPA


R.T.: 6.427 min
Delta R.T.: -0.046 min
Response: 12448132
Conc: 4.83 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB119280BL

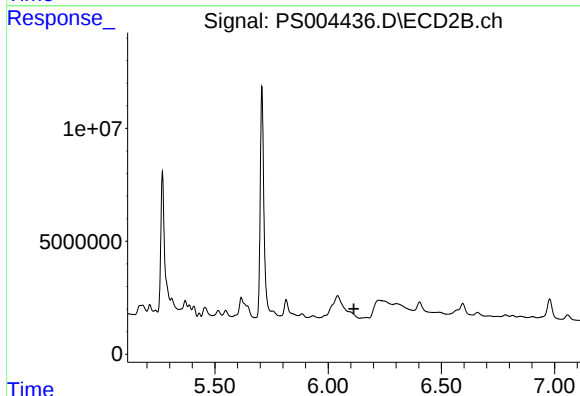


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.114 min
Response: 0
Conc: N.D.

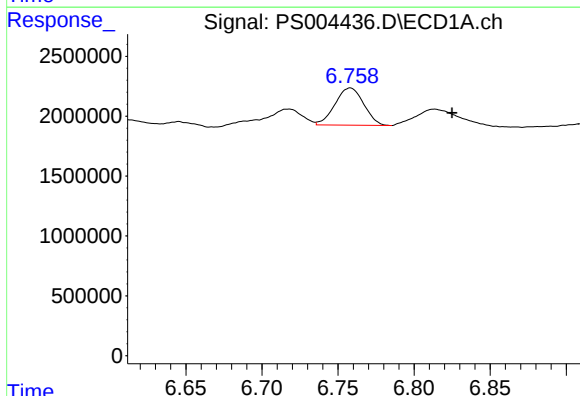


#8 DICHLORPROP

R.T.: 6.758 min
Delta R.T.: -0.067 min
Response: 4079603
Conc: 7.13 ng/ml

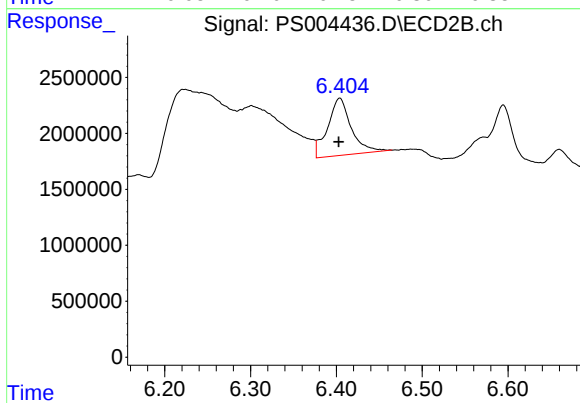

#8 DICHLORPROP


R.T.: 6.404 min
Delta R.T.: 0.001 min
Response: 9739241
Conc: 20.70 ng/ml

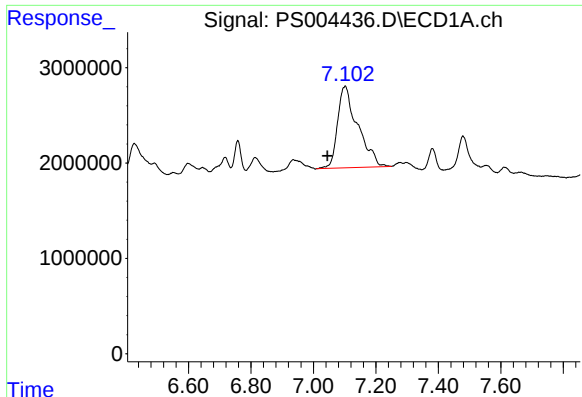

#9 2,4-D


R.T.: 7.101 min
Delta R.T.: 0.056 min
Response: 38325017
Conc: 59.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119280BL

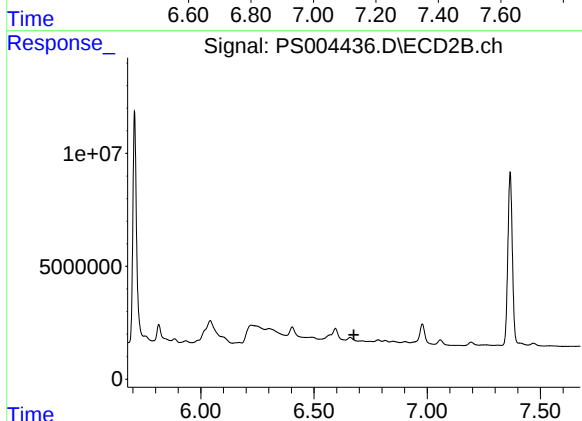


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

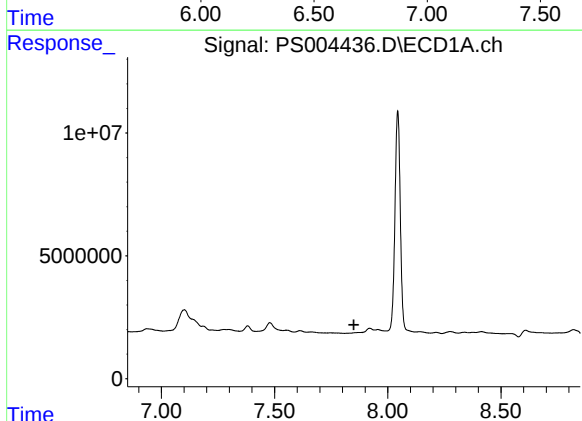

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

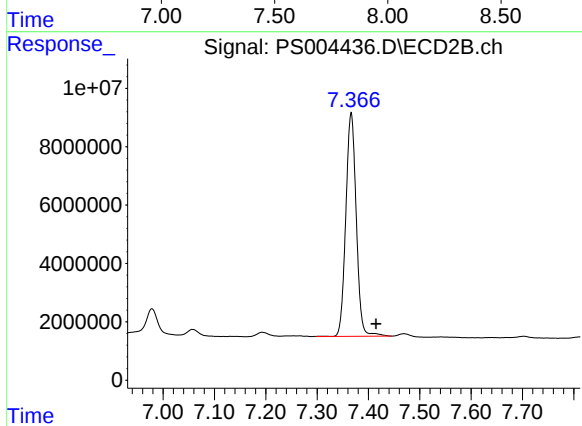

#11 2,4,5-TP (SILVEX)

R.T.: 7.366 min
Delta R.T.: -0.049 min
Response: 107963092
Conc: 41.09 ng/ml