

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050321\
 Data File : PS014881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2021 08:28
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 14:17:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
7) T	MCPA	7.617f	0.000	3134448	0	<MDL	N.D. #
10) T	Pentachlo...	8.564	8.395	4683759	1851904	<MDL	<MDL #
11) T	2,4,5-TP ...	9.110	8.756	3702933	1927298	<MDL	<MDL #
12) T	2,4,5-T	9.404	9.146	6920897	1878947	<MDL	<MDL #
14) T	DINOSEB	11.091	0.000	4012693	0	<MDL	N.D. #
15) T	Picloram	10.936	10.970	68010334	28249876	6.079	7.533
16) T	DCPA	11.356	10.897	8102118	3634285	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050321\
Data File : PS014881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2021 08:28
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 14:17:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

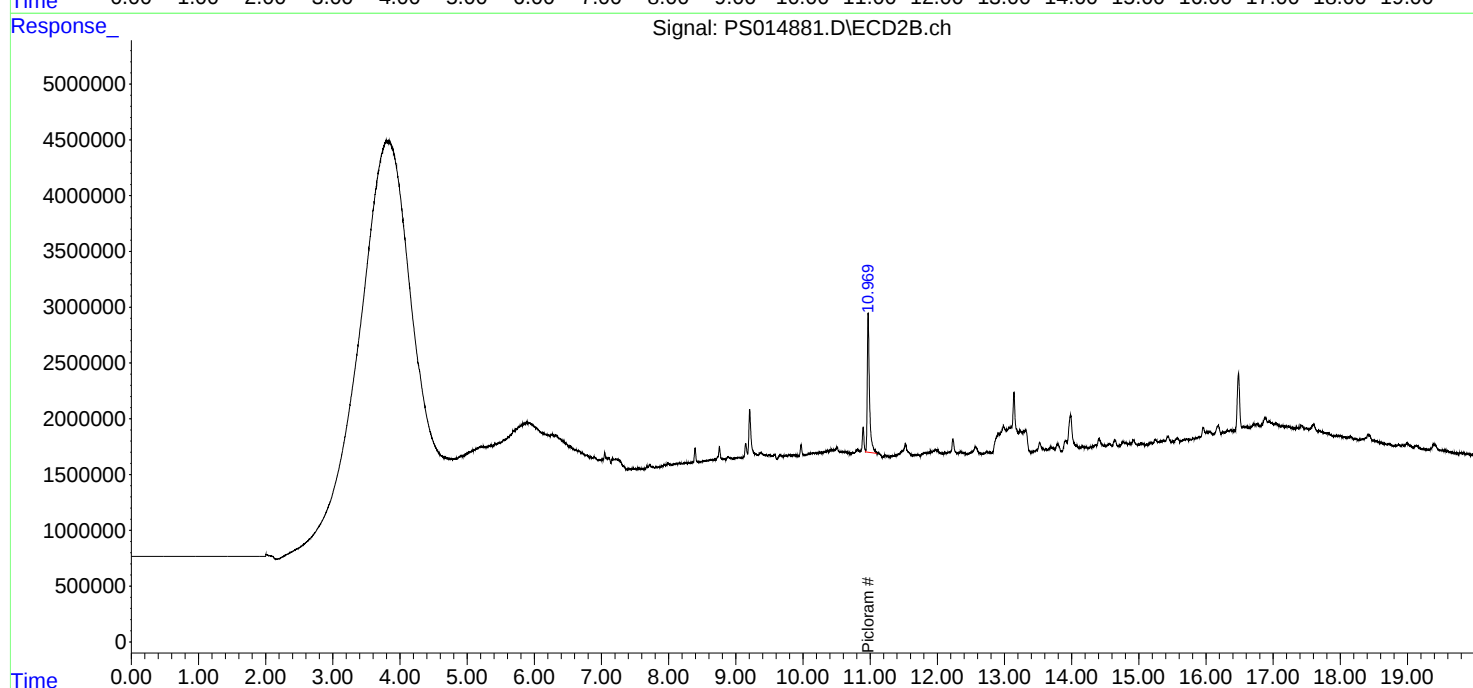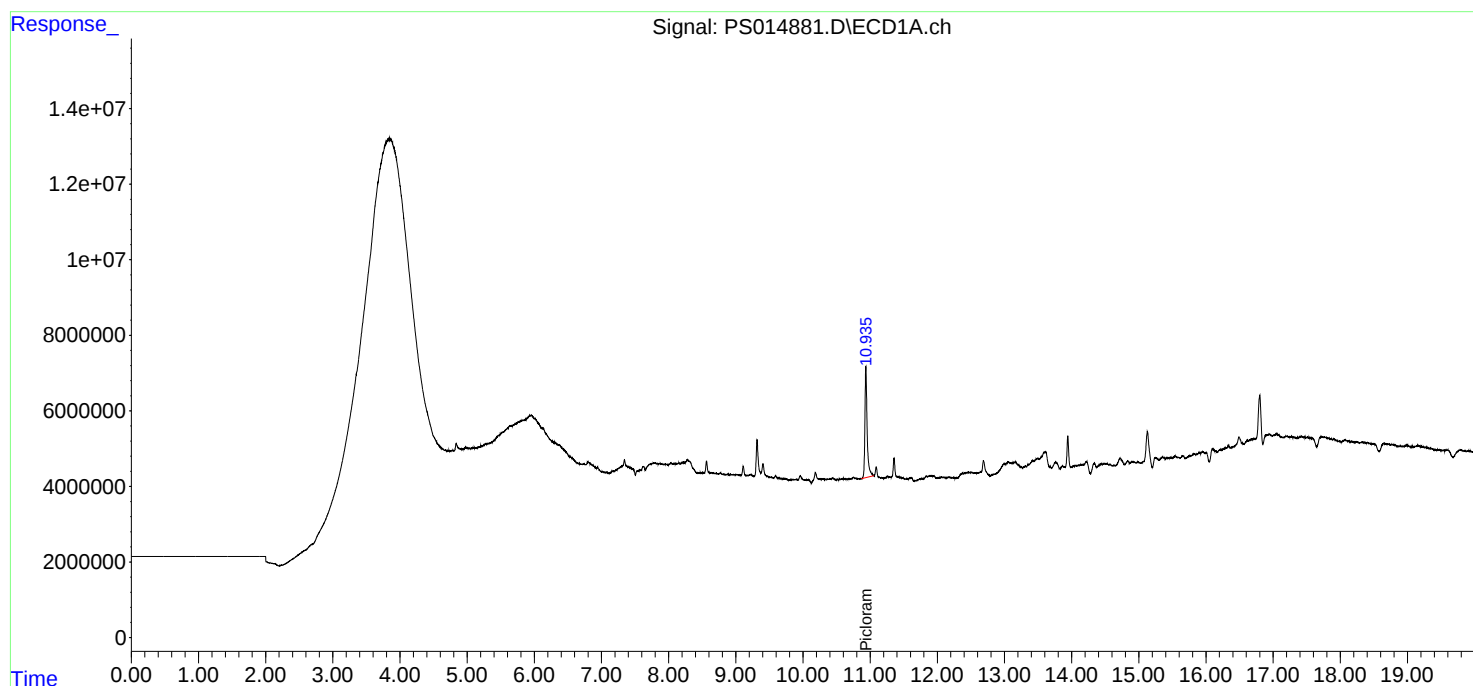


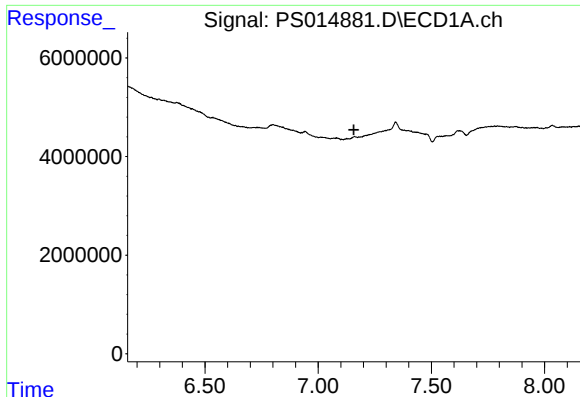

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

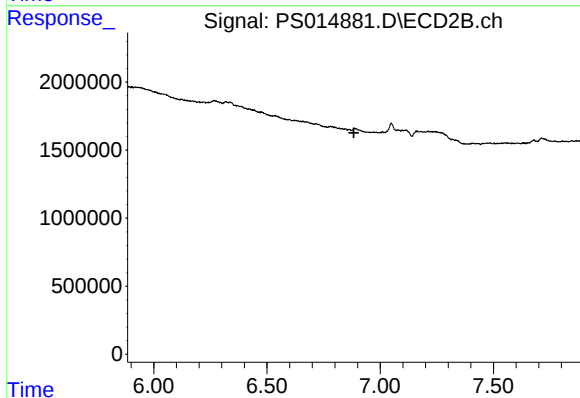


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

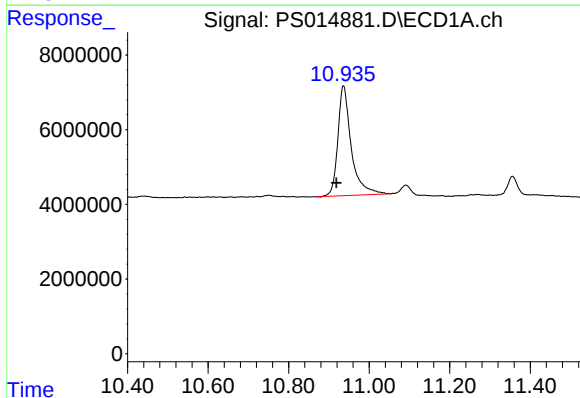

#15 Picloram

R.T.: 10.936 min
Delta R.T.: 0.017 min
Response: 68010334
Conc: 6.08 ng/ml

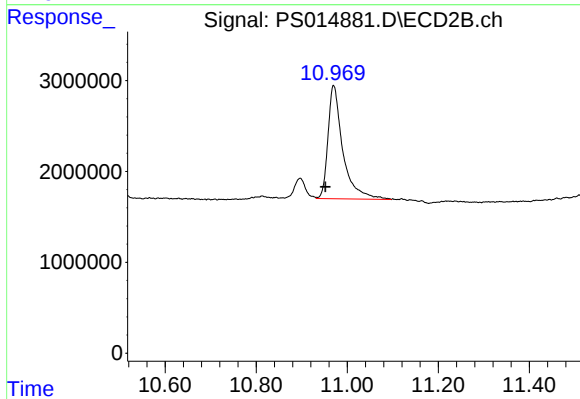

#15 Picloram

R.T.: 10.970 min
Delta R.T.: 0.017 min
Response: 28249876
Conc: 7.53 ng/ml