

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050321\  
 Data File : PS014882.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 May 2021 08:54  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 03 14:18:00 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040821.M  
 Quant Title : 8080.M  
 QLast Update : Thu Apr 08 14:34:06 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1   | RT#2    | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|---------|---------|---------|---------|---------|
| -----                       |          |        |         |         |         |         |         |
| System Monitoring Compounds |          |        |         |         |         |         |         |
| 4) S                        | 2,4-DCAA | 7.159  | 6.888   | 728.5E6 | 227.6E6 | 478.911 | 488.946 |
| Target Compounds            |          |        |         |         |         |         |         |
| 9) T                        | 2,4-D    | 8.325f | 0.000   | 3727241 | 0       | 2.344   | N.D. #  |
| 15) T                       | Picloram | 0.000  | 11.022f | 0       | 8256679 | N.D.    | 2.202   |
| -----                       |          |        |         |         |         |         |         |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050321\  
Data File : PS014882.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 May 2021 08:54  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 03 14:18:00 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040821.M  
Quant Title : 8080.M  
QLast Update : Thu Apr 08 14:34:06 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

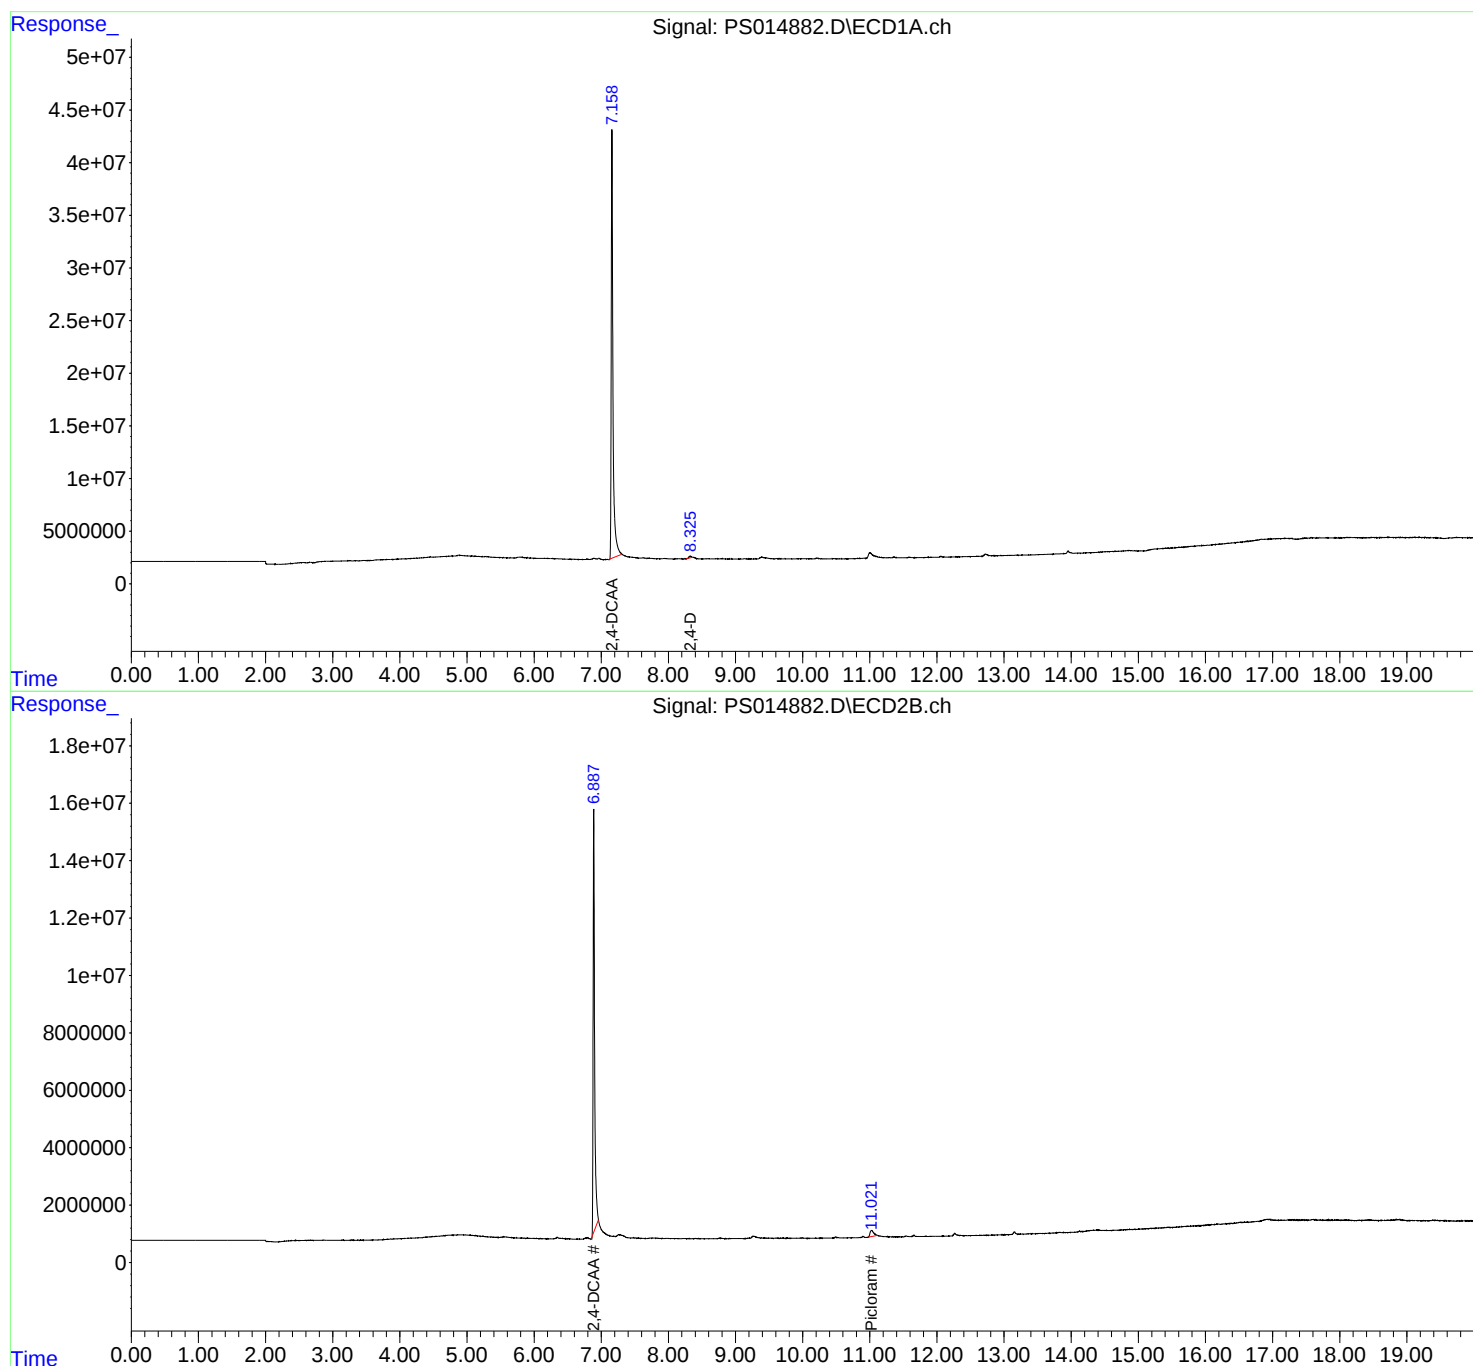


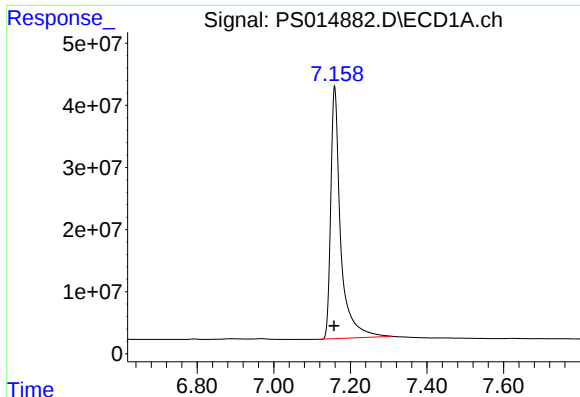

#4 2,4-DCAA


R.T.: 7.159 min  
Delta R.T.: 0.000 min  
Response: 728516854  
Conc: 478.91 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

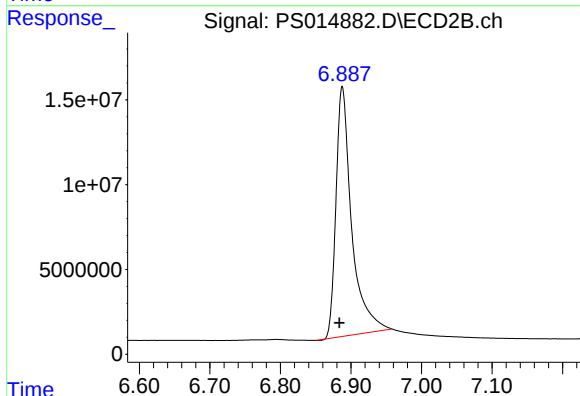


#4 2,4-DCAA

R.T.: 6.888 min  
Delta R.T.: 0.004 min  
Response: 227582443  
Conc: 488.95 ng/ml

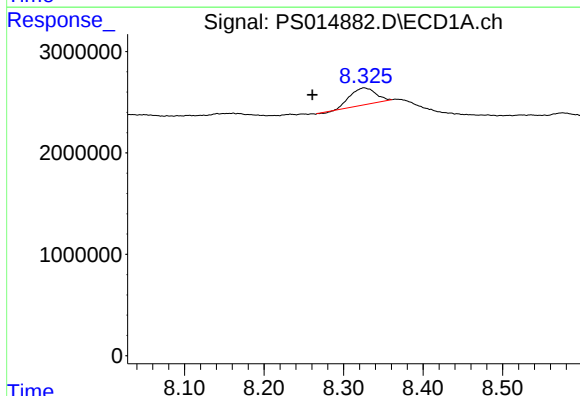


#9 2,4-D

R.T.: 8.325 min  
Delta R.T.: 0.065 min  
Response: 3727241  
Conc: 2.34 ng/ml

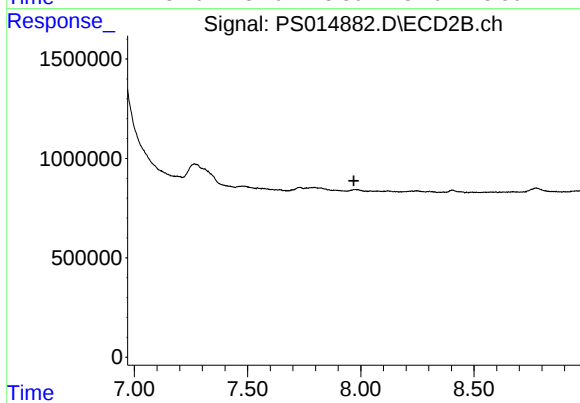

#9 2,4-D


R.T.: 0.000 min  
Exp R.T. : 7.970 min  
Response: 0  
Conc: N.D.

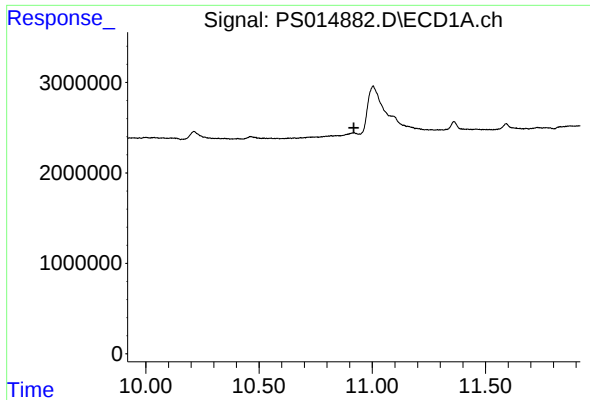

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 10.919 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

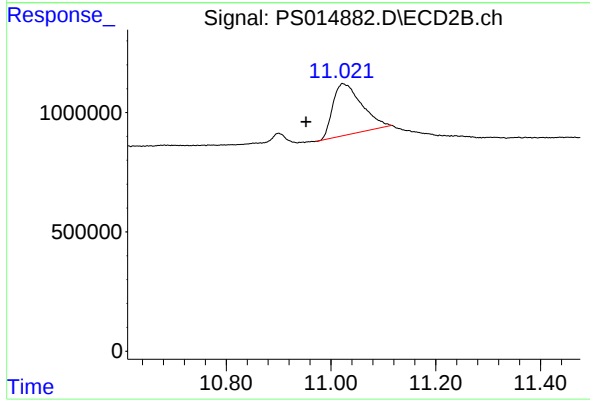

#15 Picloram

R.T.: 11.022 min  
Delta R.T.: 0.069 min  
Response: 8256679  
Conc: 2.20 ng/ml