

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050321\
 Data File : PS014887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2021 12:08
 Operator : DD\AJ
 Sample : M2217-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HTRCV2-GRAB-CF02-02

Manual Integrations
 APPROVED

Ankita
 5/4/2021 2:30:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 15:40:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.153	6.883	430.4E6	158.8E6	282.943m	341.245

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050321\
Data File : PS014887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2021 12:08
Operator : DD\AJ
Sample : M2217-18
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
HTCRV2-GRAB-CF02-02


Manual Integrations
APPROVED

Ankita
5/4/2021 2:30:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 15:40:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

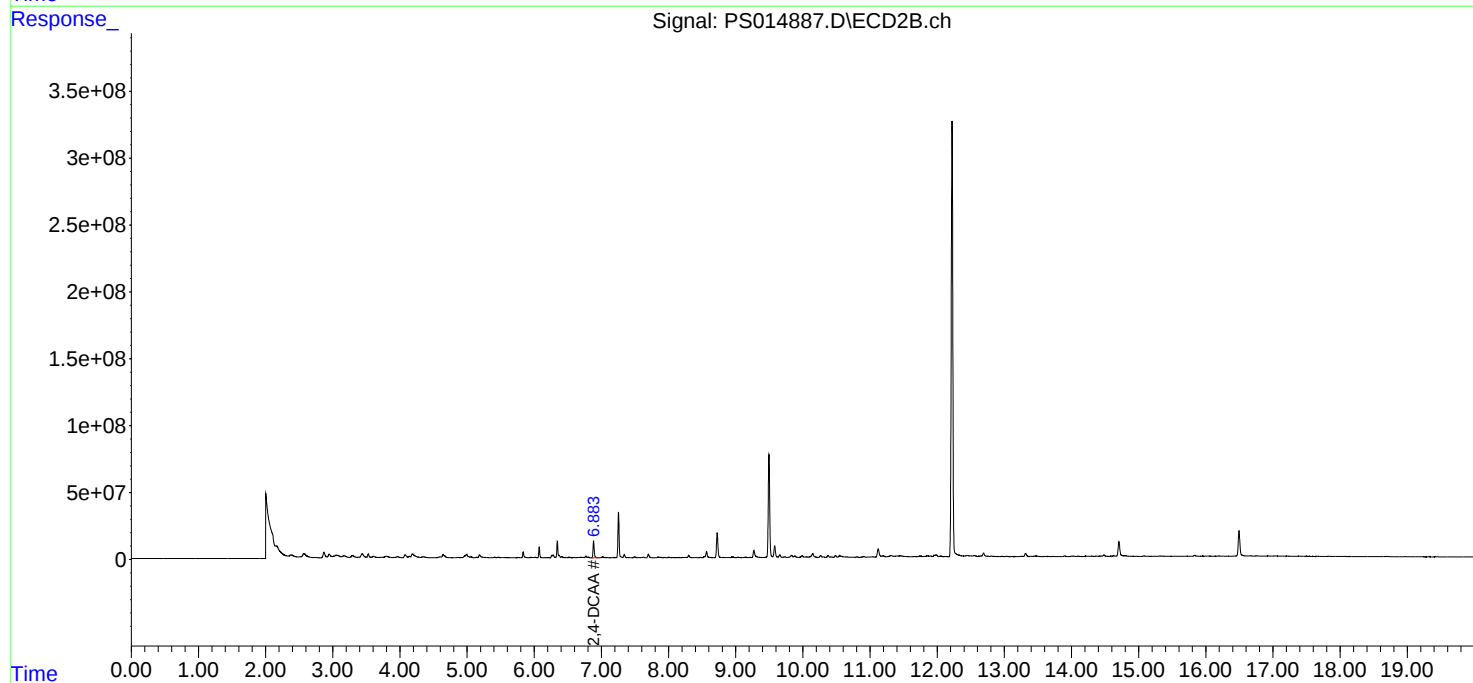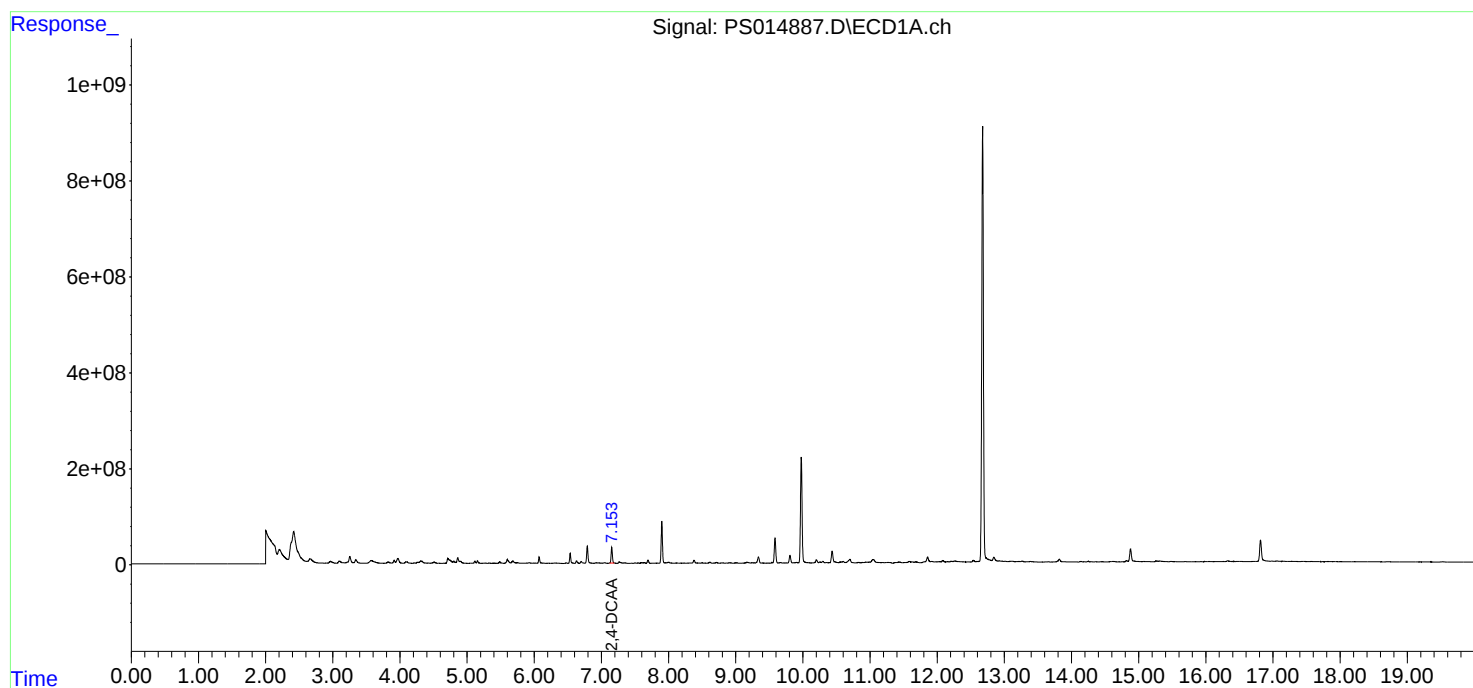

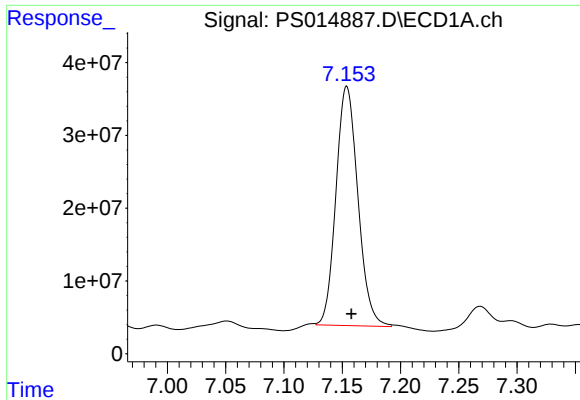


#4 2,4-DCAA

R.T.: 7.153 min
Delta R.T.: -0.004 min
Response: 430412170
Conc: 282.94 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HTCRV2-GRAB-CF02-02

Manual Integrations
APPROVED

Ankita
5/4/2021 2:30:25 PM

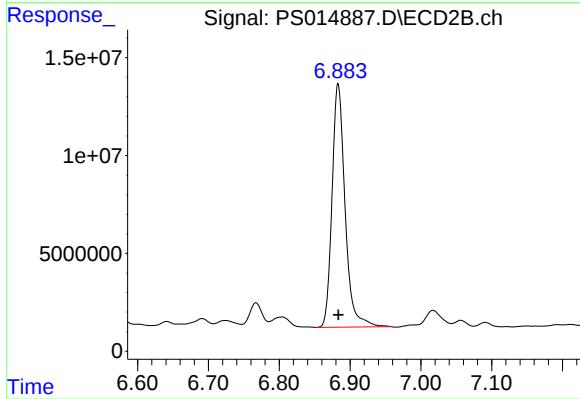

#4 2,4-DCAA

R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 158833885
Conc: 341.24 ng/ml