

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050422\
 Data File : PS019261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 14:33
 Operator : AJ\MA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 16:04:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:02:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	2044.5E6	553.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.027	2.533	3248.2E6	596.5E6	682.500	682.500
2) T	3,5-DICHL...	6.431	5.975	2451.0E6	808.7E6	697.500	697.500
3) T	4-Nitroph...	7.055	6.417	659.6E6	239.8E6	682.500	682.500
5) T	DICAMBA	7.410	6.964	7809.9E6	2369.4E6	705.000	705.000
6) T	MCPD	7.580	7.062	641.2E6	187.3E6	70.500	70.500
7) T	MCPA	7.730	7.276	882.7E6	257.6E6	69.750	69.750
8) T	DICHLORPROP	8.104	7.586	1955.5E6	597.2E6	705.000	705.000
9) T	2,4-D	8.336	7.880	2256.3E6	699.1E6	705.000	705.000
10) T	Pentachlo...	8.643	8.306	28337.9E6	7931.8E6	712.500	712.500
11) T	2,4,5-TP ...	9.195	8.668	12824.4E6	3432.5E6	712.500	712.500
12) T	2,4,5-T	9.481	9.046	14863.9E6	3111.3E6	712.500	712.500
13) T	2,4-DB	10.036	9.552	3071.6E6	405.6E6	712.500	712.500
14) T	DINOSEB	11.190	9.879	11224.5E6	2014.1E6	705.000	705.000
15) T	Picloram	11.025	10.867	21797.5E6	4194.4E6	712.500	712.500
16) T	DCPA	11.457	10.808	18526.3E6	4193.6E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050422\
Data File : PS019261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 14:33
Operator : AJ\MA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 16:04:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:02:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

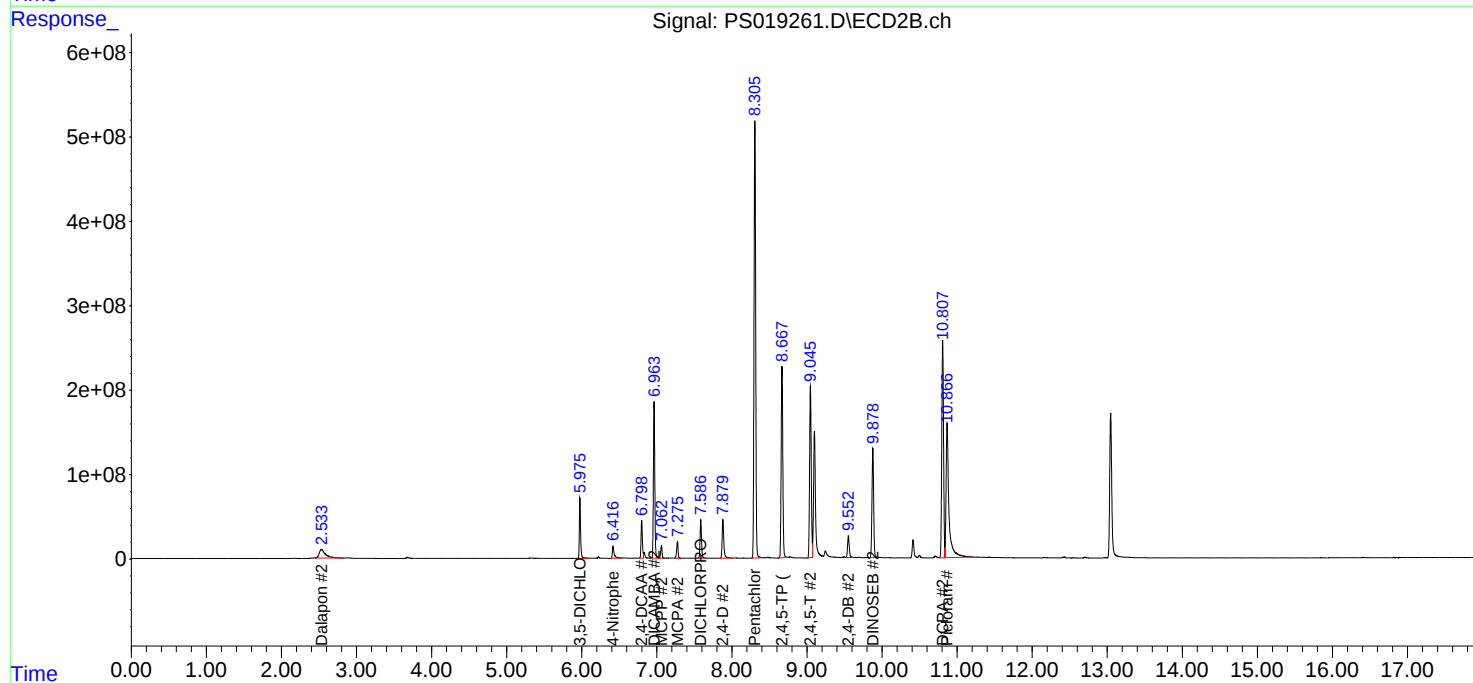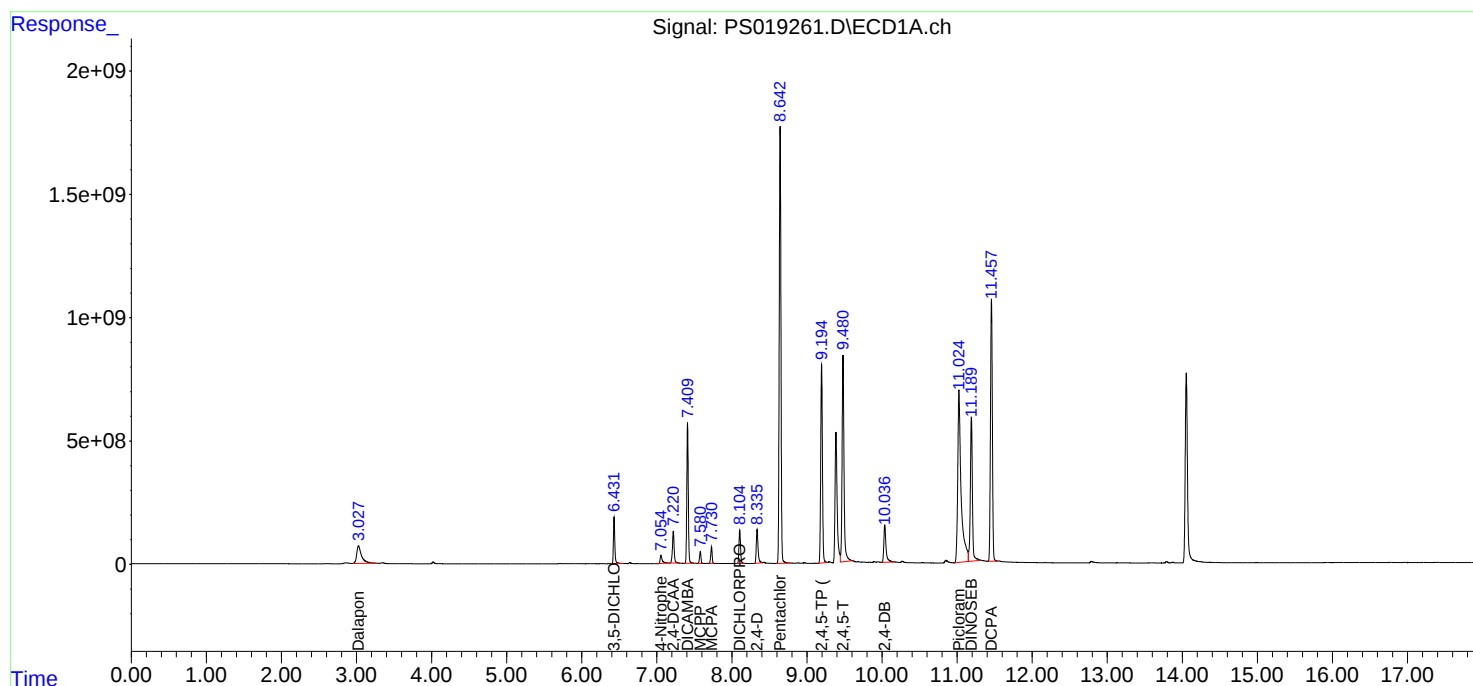


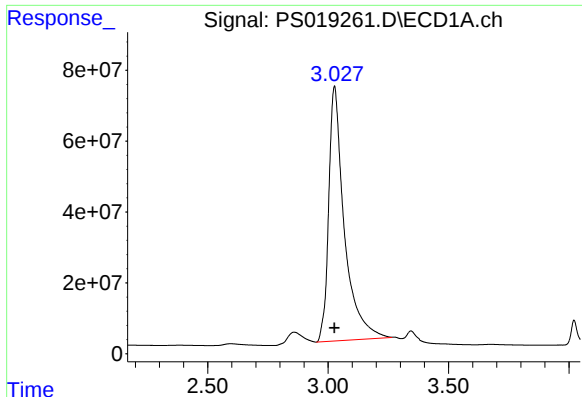

#1 Dalapon


R.T.: 3.027 min
Delta R.T.: 0.000 min
Response: 3248216634
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

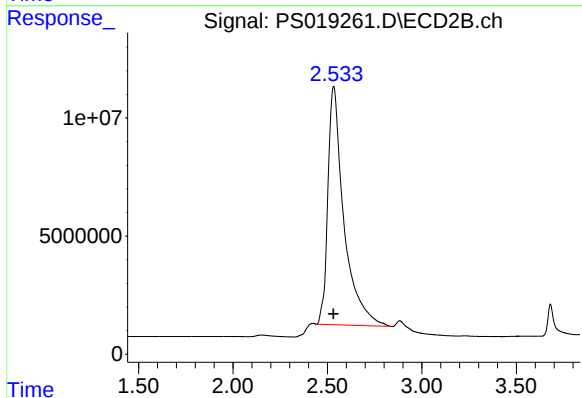


#1 Dalapon

R.T.: 2.533 min
Delta R.T.: 0.000 min
Response: 596506696
Conc: 682.50 ng/ml

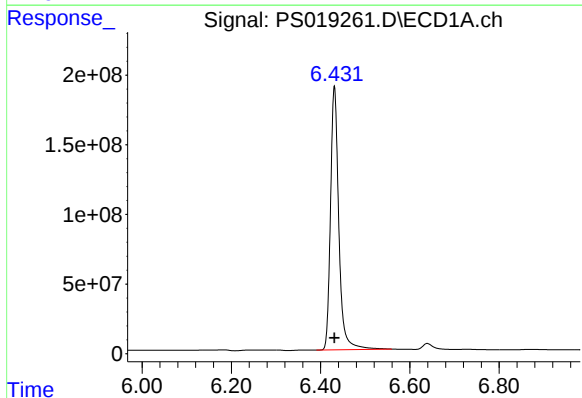


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 2450952720
Conc: 697.50 ng/ml

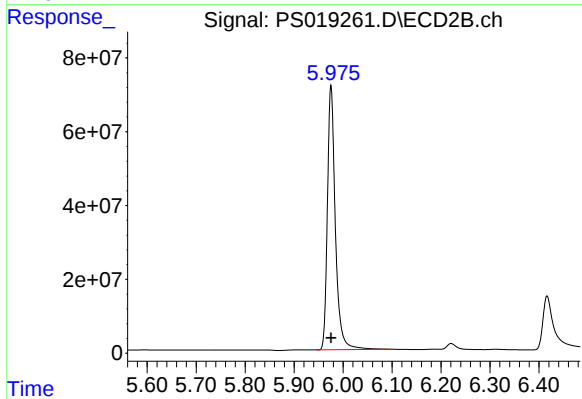

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 808705729
Conc: 697.50 ng/ml

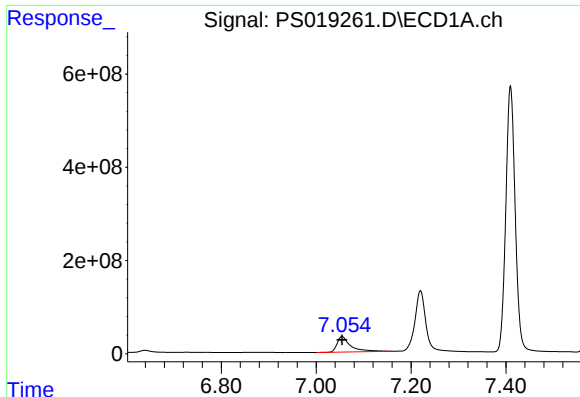

#3 4-Nitrophenol


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 659618537
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

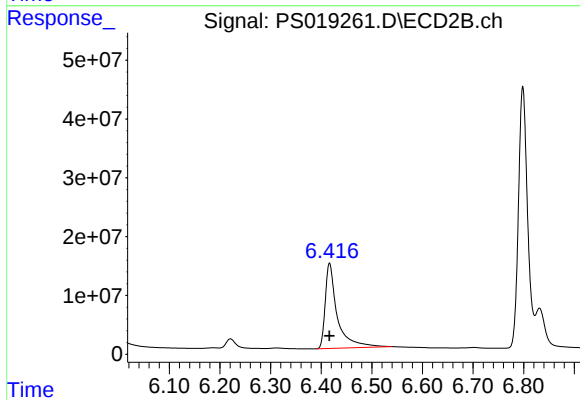


#3 4-Nitrophenol

R.T.: 6.417 min
Delta R.T.: 0.000 min
Response: 239764848
Conc: 682.50 ng/ml

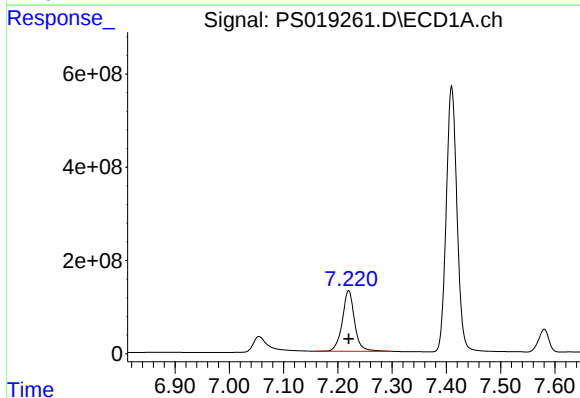


#4 2,4-DCAA

R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 2044510063
Conc: 750.00 ng/ml

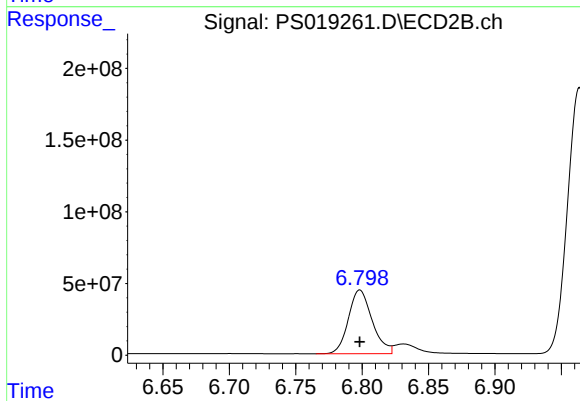

#4 2,4-DCAA


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 553676796
Conc: 750.00 ng/ml

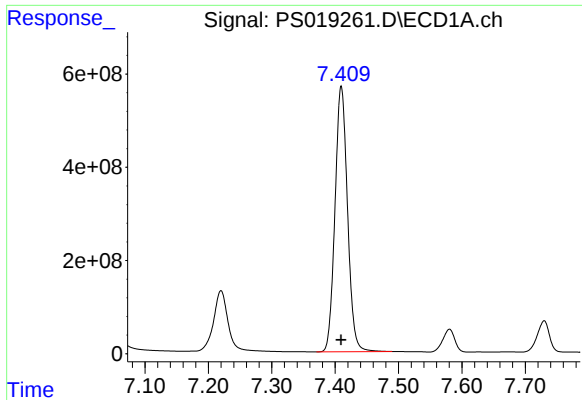

#5 DICAMBA


R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 7809896154
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

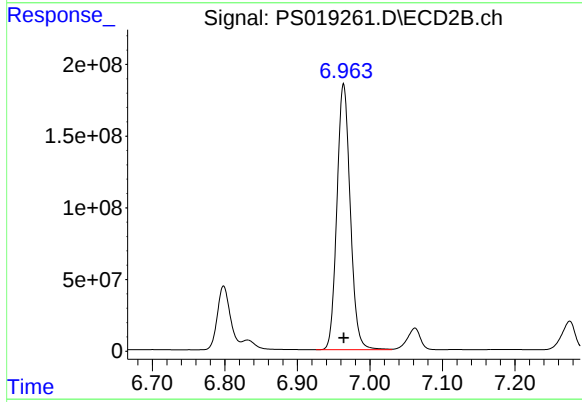


#5 DICAMBA

R.T.: 6.964 min
Delta R.T.: 0.000 min
Response: 2369353699
Conc: 705.00 ng/ml

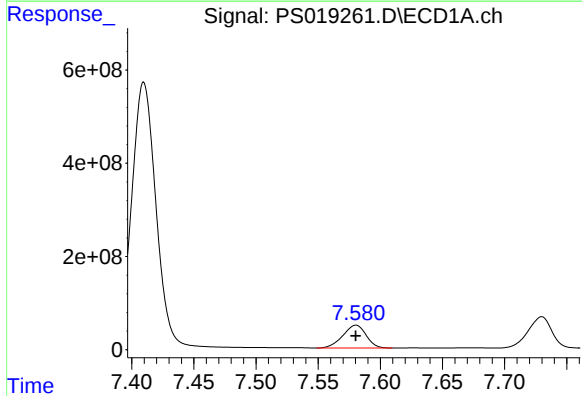


#6 MCP

R.T.: 7.580 min
Delta R.T.: 0.000 min
Response: 641189396
Conc: 70.50 ug/ml

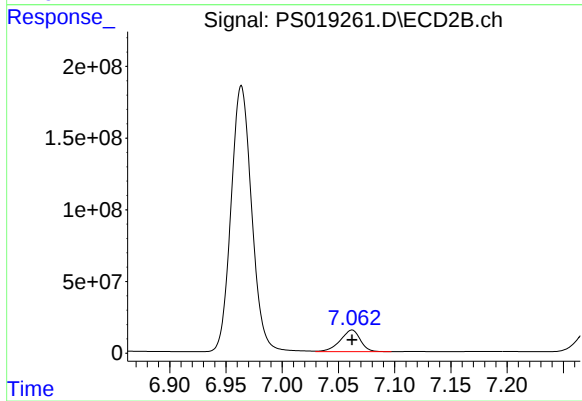

#6 MCP


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 187288689
Conc: 70.50 ug/ml

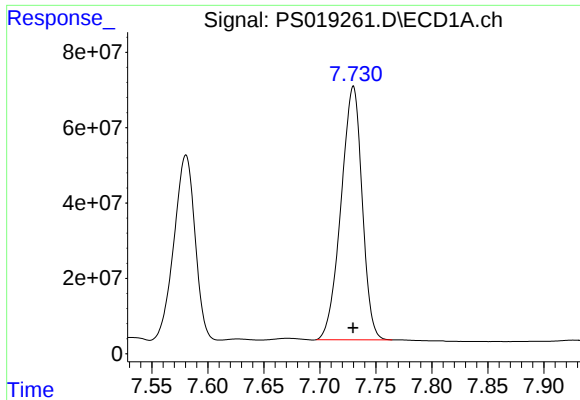

#7 MCPA


R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 882716397
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :

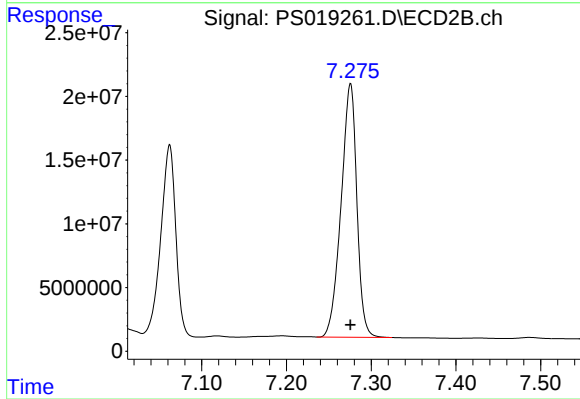


#7 MCPA

R.T.: 7.276 min
Delta R.T.: 0.000 min
Response: 257557735
Conc: 69.75 ug/ml

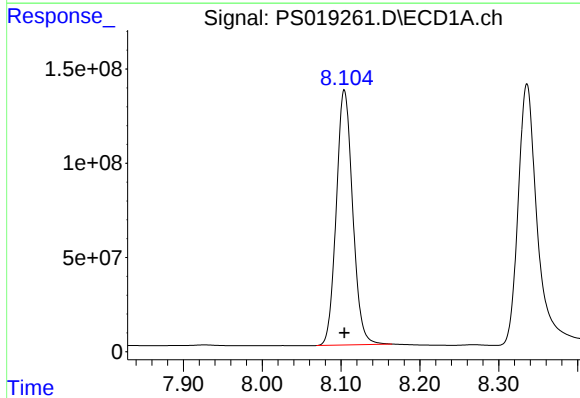


#8 DICHLORPROP

R.T.: 8.104 min
Delta R.T.: 0.000 min
Response: 1955527897
Conc: 705.00 ng/ml

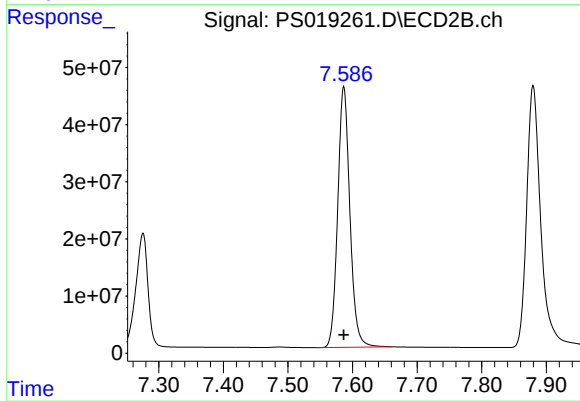

#8 DICHLORPROP


R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 597240181
Conc: 705.00 ng/ml

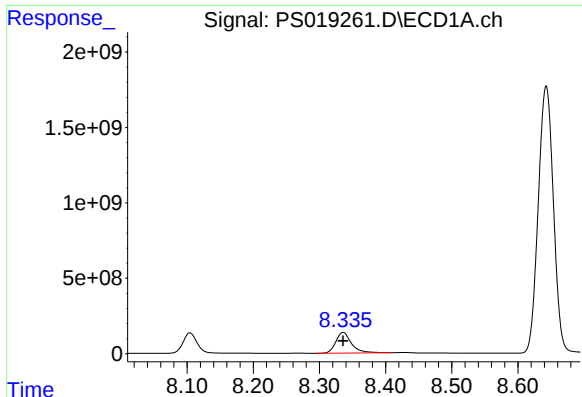

#9 2,4-D


R.T.: 8.336 min
Delta R.T.: 0.000 min
Response: 2256270723
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

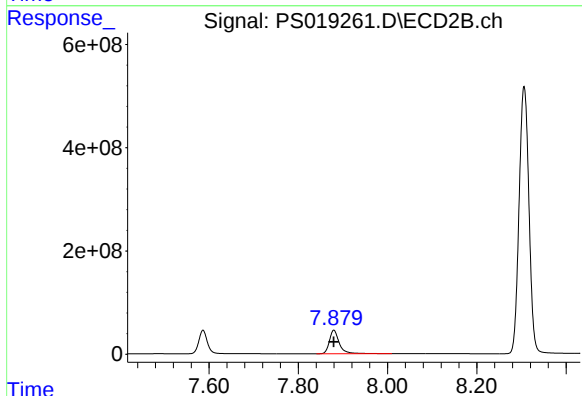


#9 2,4-D

R.T.: 7.880 min
Delta R.T.: 0.000 min
Response: 699085406
Conc: 705.00 ng/ml

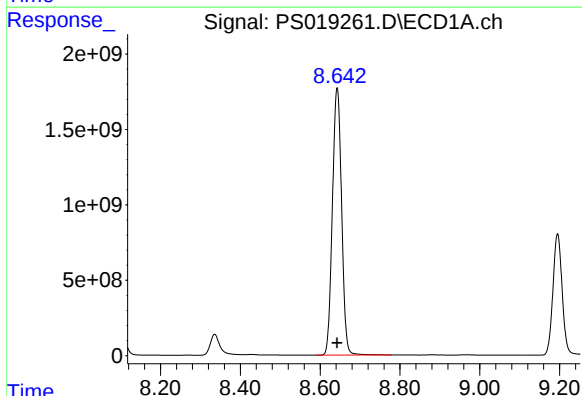


#10 Pentachlorophenol

R.T.: 8.643 min
Delta R.T.: 0.000 min
Response: 28337922866
Conc: 712.50 ng/ml

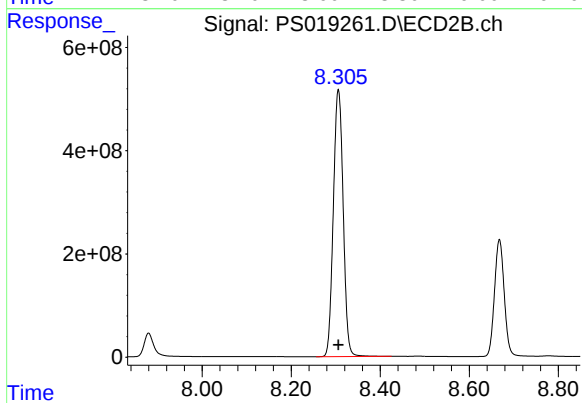

#10 Pentachlorophenol


R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 7931815167
Conc: 712.50 ng/ml

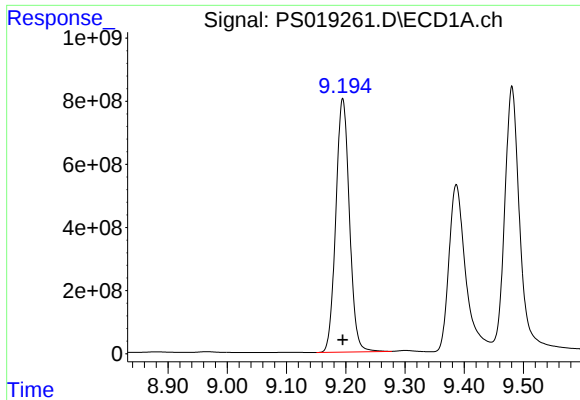

#11 2,4,5-TP (SILVEX)


R.T.: 9.195 min
Delta R.T.: 0.000 min
Response: 12824360534
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

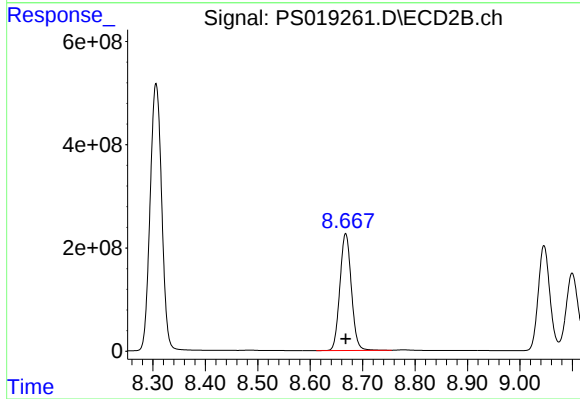


#11 2,4,5-TP (SILVEX)

R.T.: 8.668 min
Delta R.T.: 0.000 min
Response: 3432517750
Conc: 712.50 ng/ml

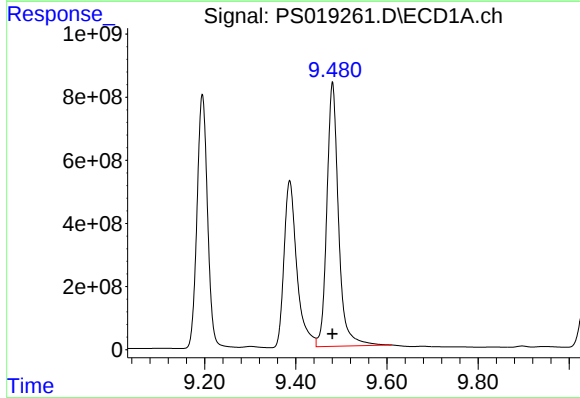


#12 2,4,5-T

R.T.: 9.481 min
Delta R.T.: 0.000 min
Response: 14863895386
Conc: 712.50 ng/ml

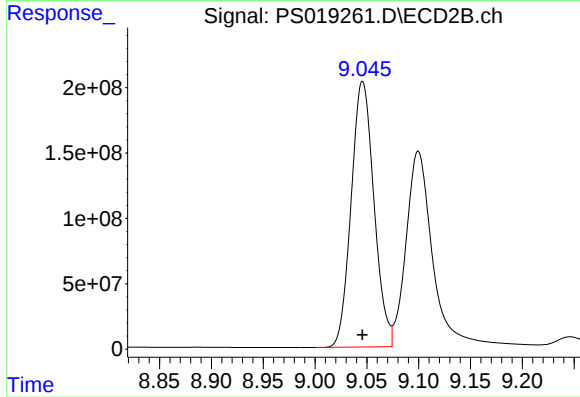

#12 2,4,5-T


R.T.: 9.046 min
Delta R.T.: 0.000 min
Response: 3111321437
Conc: 712.50 ng/ml

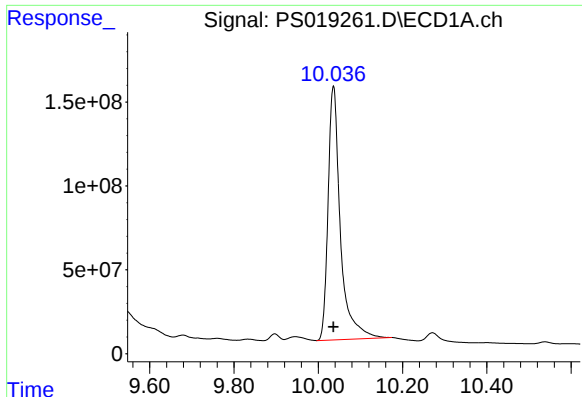

#13 2,4-DB


R.T.: 10.036 min
Delta R.T.: 0.000 min
Response: 3071616682
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

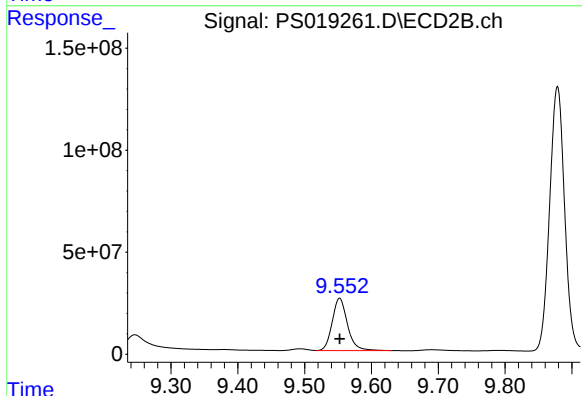


#13 2,4-DB

R.T.: 9.552 min
Delta R.T.: 0.000 min
Response: 405553854
Conc: 712.50 ng/ml

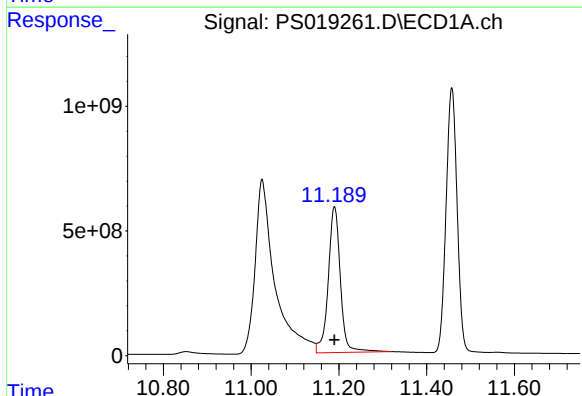


#14 DINOSEB

R.T.: 11.190 min
Delta R.T.: 0.000 min
Response: 11224471420
Conc: 705.00 ng/ml

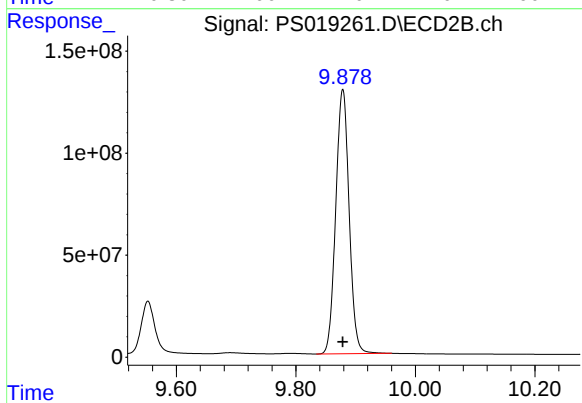

#14 DINOSEB


R.T.: 9.879 min
Delta R.T.: 0.000 min
Response: 2014093298
Conc: 705.00 ng/ml

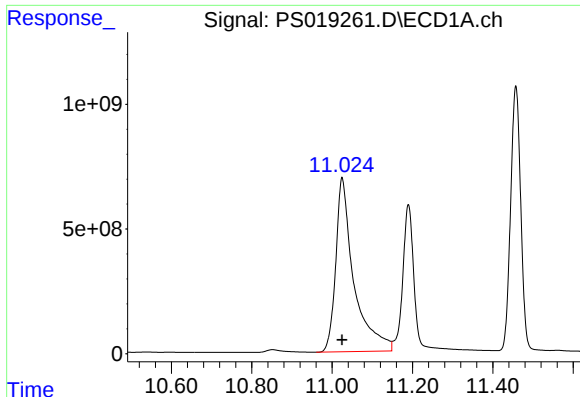

#15 Picloram


R.T.: 11.025 min
Delta R.T.: 0.000 min
Response: 21797461303
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

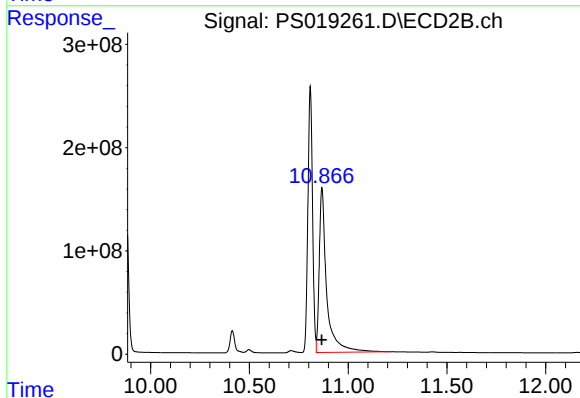


#15 Picloram

R.T.: 10.867 min
Delta R.T.: 0.000 min
Response: 4194420982
Conc: 712.50 ng/ml

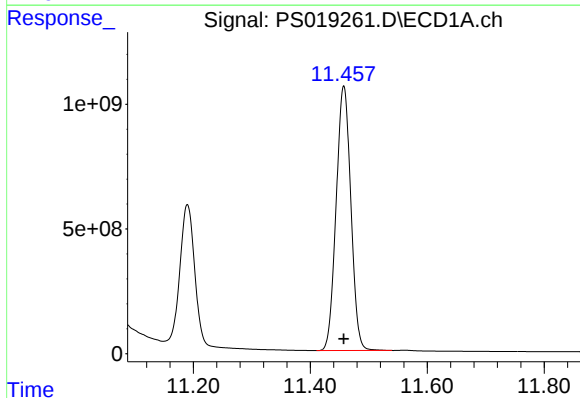

#16 DCPA

R.T.: 11.457 min
Delta R.T.: 0.000 min
Response: 18526253042
Conc: 720.00 ng/ml

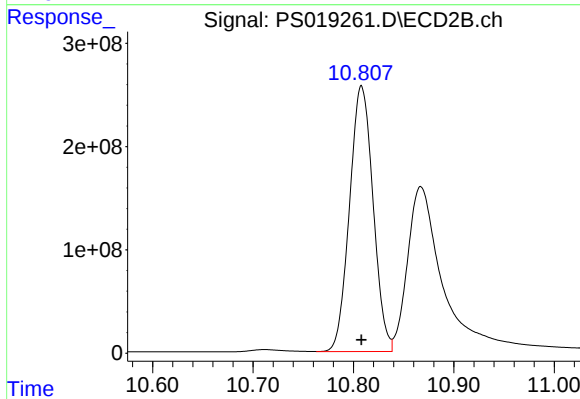

#16 DCPA

R.T.: 10.808 min
Delta R.T.: 0.000 min
Response: 4193624135
Conc: 720.00 ng/ml