

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050422\  
 Data File : PS019289.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2022 02:07  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 02:33:26 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS050422.M  
 Quant Title : 8080.M  
 QLast Update : Wed May 04 16:27:11 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2    | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|---------|----------|---------|---------|---------|
| -----                       |              |        |         |          |         |         |         |
| System Monitoring Compounds |              |        |         |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 7.221  | 6.799   | 1260.3E6 | 372.4E6 | 461.510 | 480.754 |
| Target Compounds            |              |        |         |          |         |         |         |
| 1) T                        | Dalapon      | 3.072f | 0.000   | 205654   | 0       | <MDL    | N.D. #  |
| 2) T                        | 3,5-DICHL... | 6.477f | 5.932f  | 210706   | 33209   | <MDL    | <MDL #  |
| 3) T                        | 4-Nitroph... | 7.024  | 0.000   | 2495328  | 0       | 2.575   | N.D. #  |
| 5) T                        | DICAMBA      | 0.000  | 6.964   | 0        | 3891521 | N.D.    | 1.161   |
| 7) T                        | MCPA         | 7.676f | 0.000   | 298970   | 0       | <MDL    | N.D. #  |
| 8) T                        | DICHLORPROP  | 8.111  | 7.629f  | 245518   | 736823  | <MDL    | <MDL #  |
| 9) T                        | 2,4-D        | 8.331  | 0.000   | 108989   | 0       | <MDL    | N.D. #  |
| 10) T                       | Pentachlo... | 8.645  | 8.306   | 1697203  | 1696033 | <MDL    | <MDL #  |
| 13) T                       | 2,4-DB       | 10.033 | 9.590   | 262418   | 48799   | <MDL    | <MDL #  |
| 14) T                       | DINOSEB      | 0.000  | 9.882   | 0        | 418157  | N.D.    | <MDL    |
| 15) T                       | Picloram     | 11.007 | 10.808f | 5243654  | 812515  | <MDL    | <MDL #  |
| 16) T                       | DCPA         | 11.462 | 10.808  | 1668850  | 812515  | <MDL    | <MDL #  |
| -----                       |              |        |         |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050422\  
Data File : PS019289.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 05 May 2022 02:07  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 05 02:33:26 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS050422.M  
Quant Title : 8080.M  
QLast Update : Wed May 04 16:27:11 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

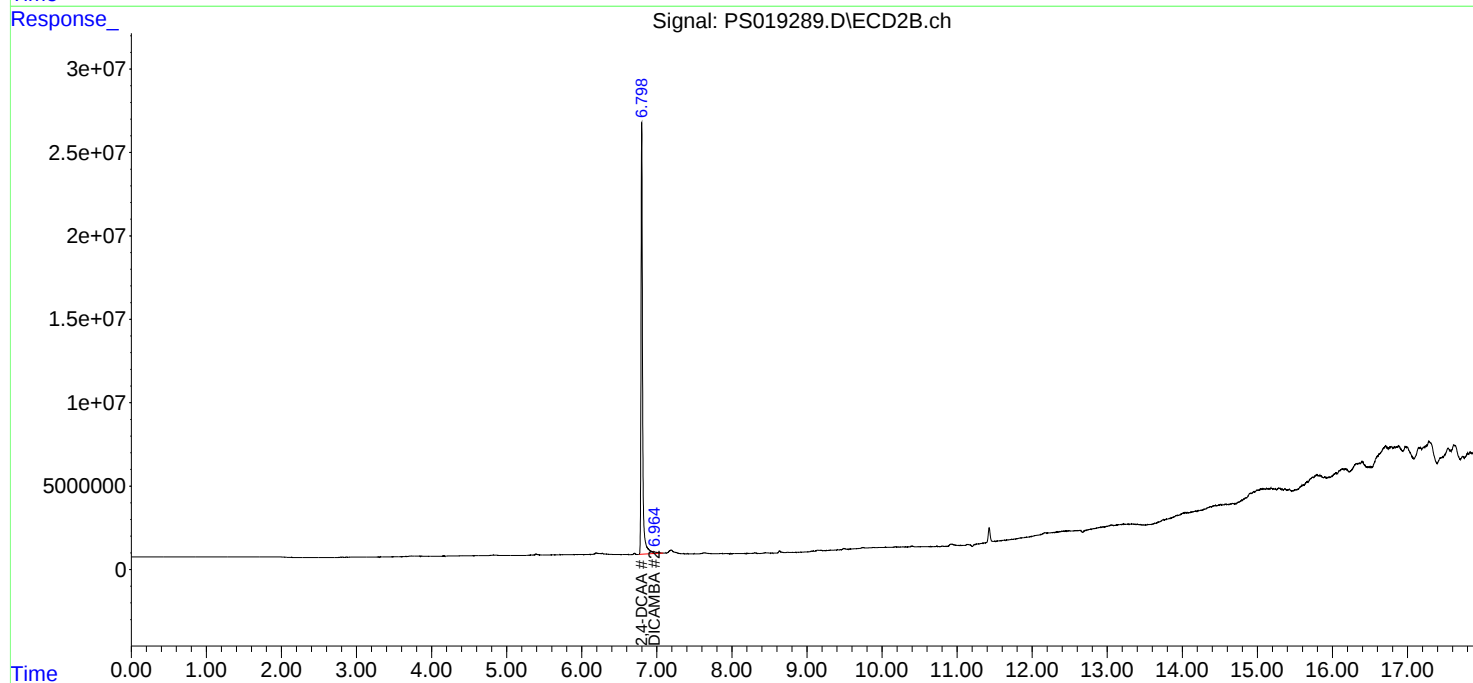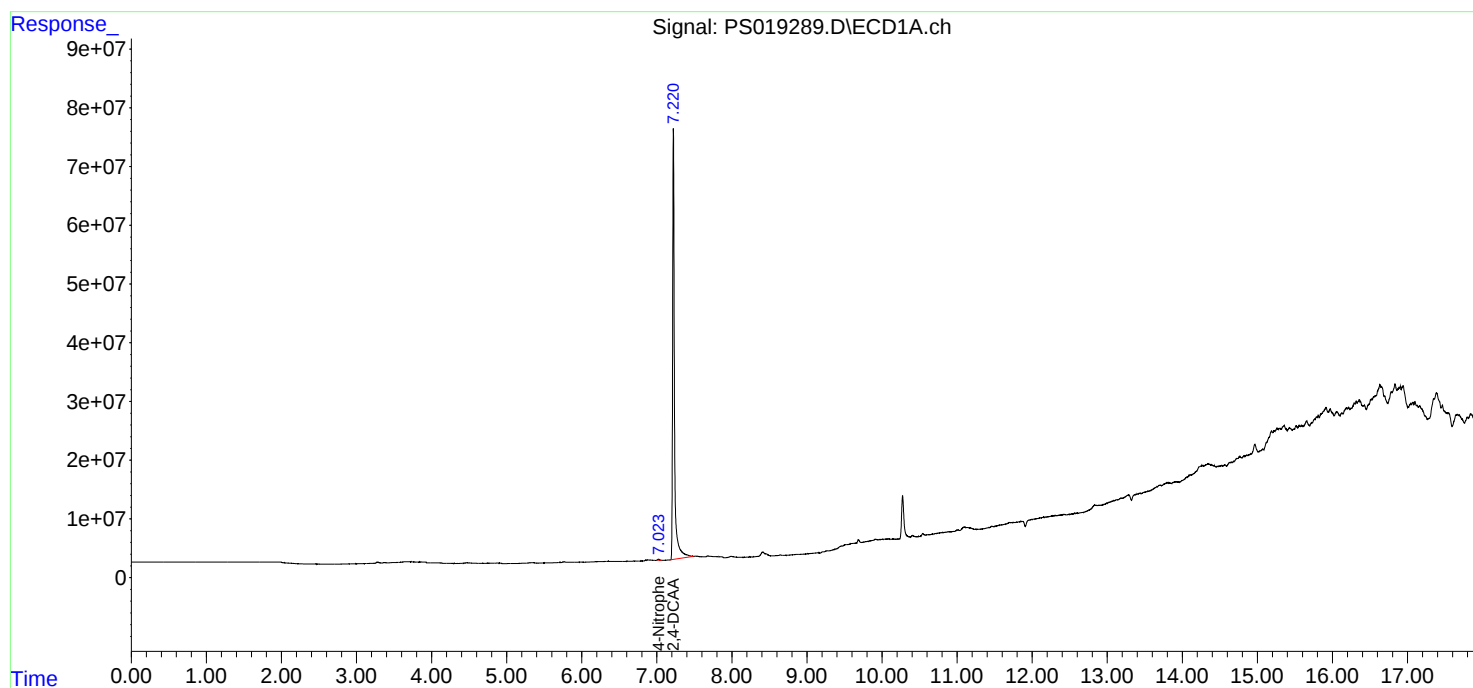


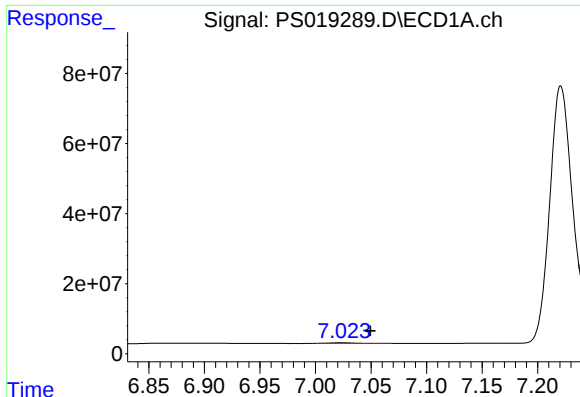

#3 4-Nitrophenol


R.T.: 7.024 min  
Delta R.T.: -0.026 min  
Response: 2495328  
Conc: 2.57 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

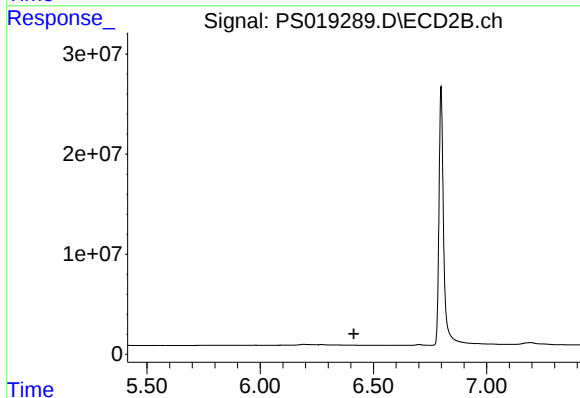


#3 4-Nitrophenol

R.T.: 0.000 min  
Exp R.T. : 6.414 min  
Response: 0  
Conc: N.D.

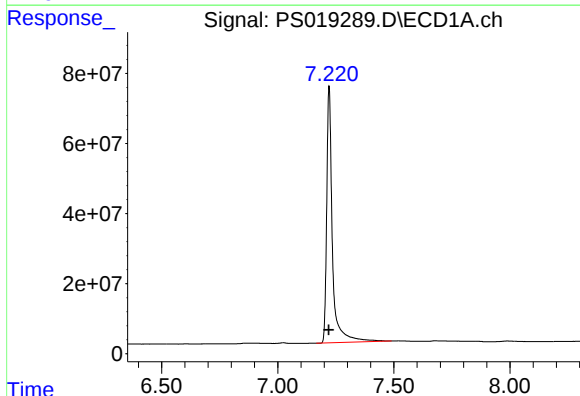


#4 2,4-DCAA

R.T.: 7.221 min  
Delta R.T.: 0.002 min  
Response: 1260326119  
Conc: 461.51 ng/ml

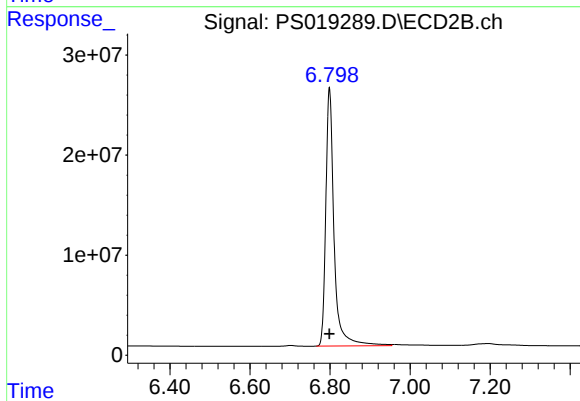

#4 2,4-DCAA


R.T.: 6.799 min  
Delta R.T.: 0.000 min  
Response: 372370662  
Conc: 480.75 ng/ml

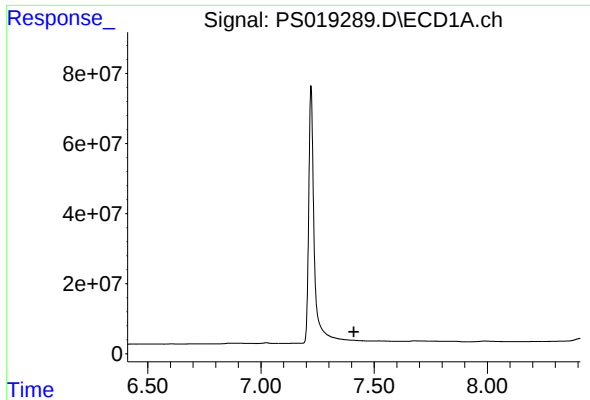

#5 DICAMBA

R.T.: 0.000 min  
Exp R.T.: 7.410 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

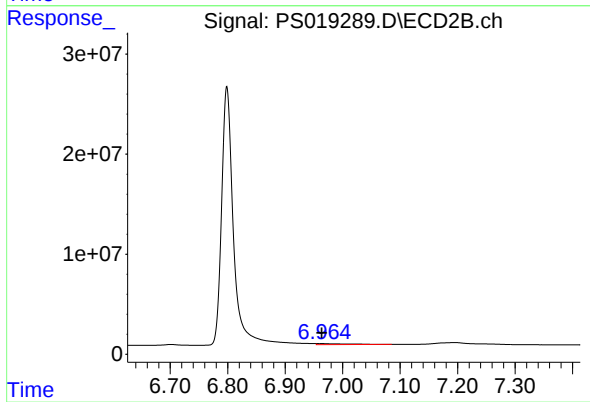

#5 DICAMBA

R.T.: 6.964 min  
Delta R.T.: 0.000 min  
Response: 3891521  
Conc: 1.16 ng/ml