

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050522\
 Data File : PS019321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2022 21:34
 Operator : AJ\MA
 Sample : N2641-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 23:58:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.797	1067.7E6	317.1E6	390.963	409.408
Target Compounds							
2) T	3,5-DICHL...	6.413	5.999	454097	30825423	<MDL	26.431 #
5) T	DICAMBA	7.400	6.955	23552761	3679385	2.133	1.098 #
6) T	MCP	7.576	7.074	17962867	1566689	2.009	<MDL #
7) T	MCPA	0.000	7.262	0	20665202	N.D.	5.548
8) T	DICHLORPROP	8.049f	7.606	5750214	5608096	2.055	6.544 #
9) T	2,4-D	8.337	7.860	26615399	8162893	8.437	8.174
10) T	Pentachlo...	8.619	8.334	28059224	3119354	<MDL	<MDL #
11) T	2,4,5-TP ...	9.257f	8.702	45132	11356132	<MDL	2.360 #
12) T	2,4,5-T	9.497	9.050	10694532	41036192	<MDL	9.477 #
13) T	2,4-DB	10.071	9.562	352.2E6	87551628	82.127	153.988 #
14) T	DINOSEB	11.156	9.882	657.2E6	109.5E6	39.804	37.796
15) T	Picloram	10.985	10.882	87775694	37722012	3.003	6.307 #
16) T	DCPA	0.000	10.810	0	25463130	N.D.	4.337



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050522\
Data File : PS019321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2022 21:34
Operator : AJ\MA
Sample : N2641-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 23:58:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

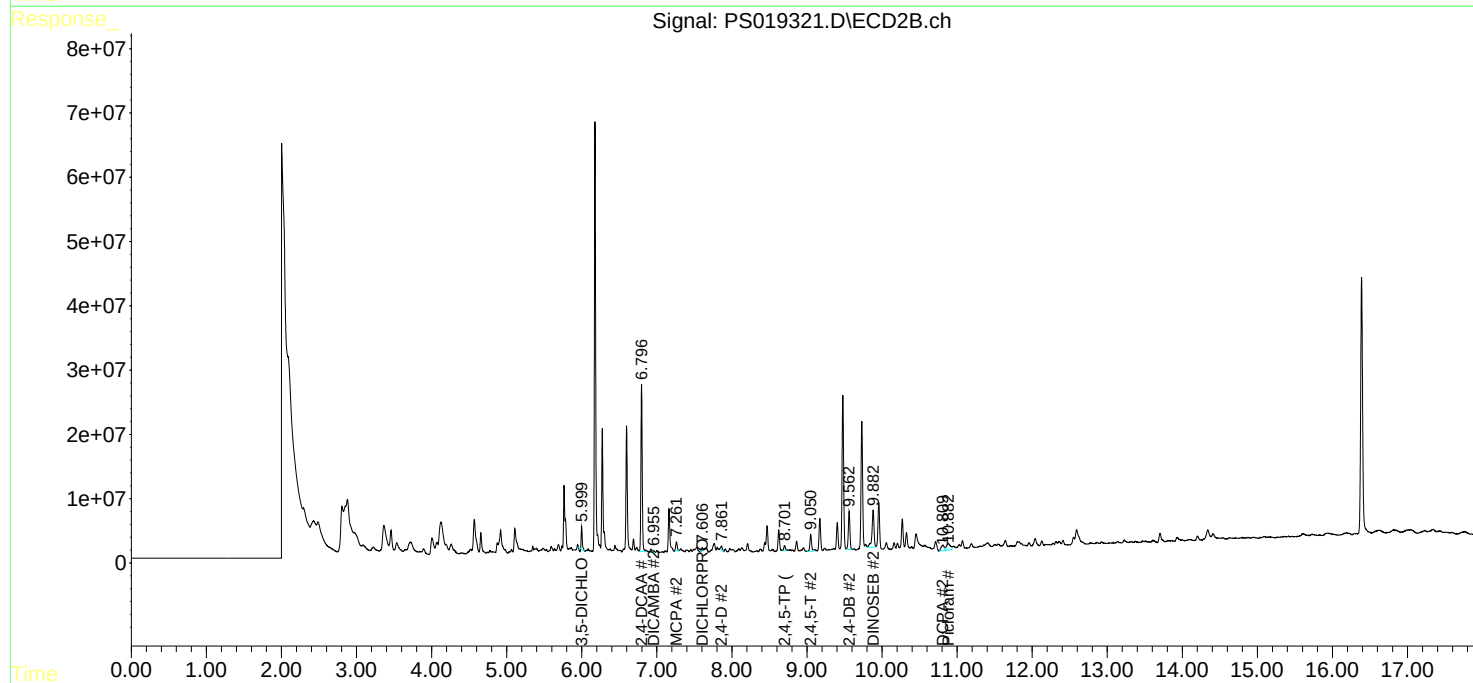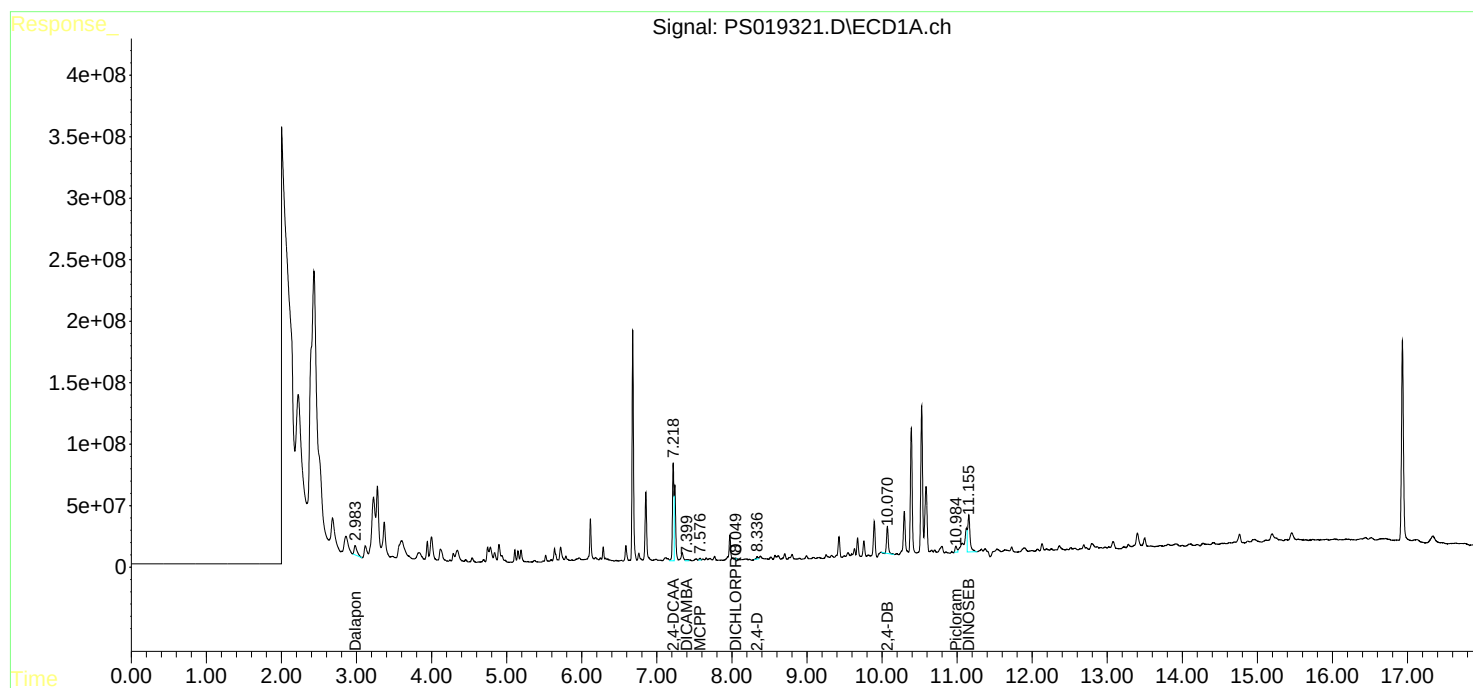


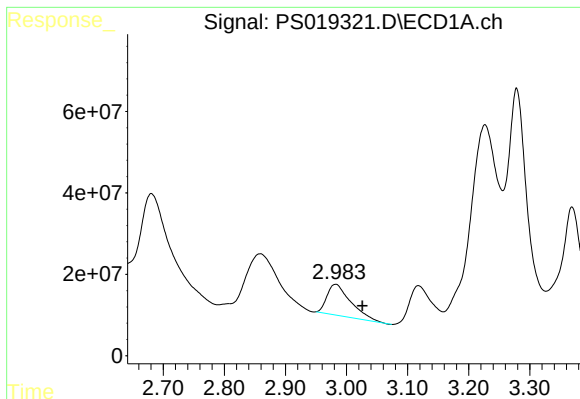

#1 Dalapon


R.T.: 2.982 min
Delta R.T.: -0.044 min
Response: 204552168
Conc: 42.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

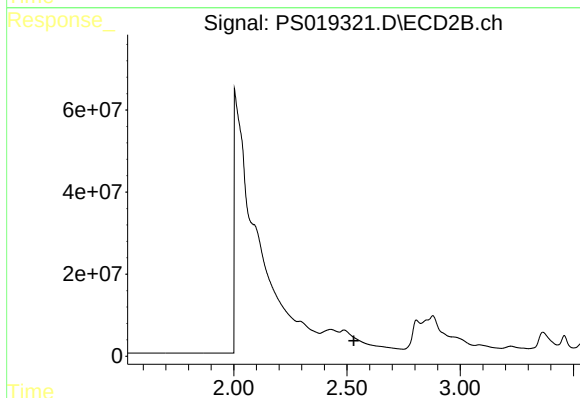


#1 Dalapon

R.T.: 2.487 min
Delta R.T.: -0.044 min
Response: -77040850
Conc: N.D.

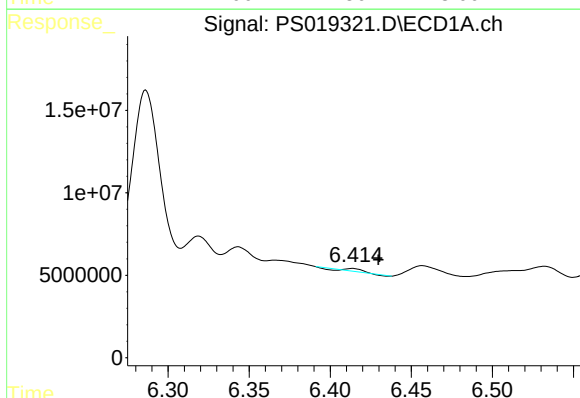


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.413 min
Delta R.T.: -0.016 min
Response: 454097
Conc: N.D.

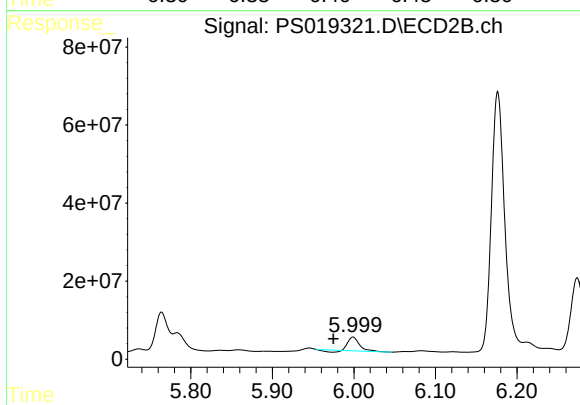

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.999 min
Delta R.T.: 0.024 min
Response: 30825423
Conc: 26.43 ng/ml

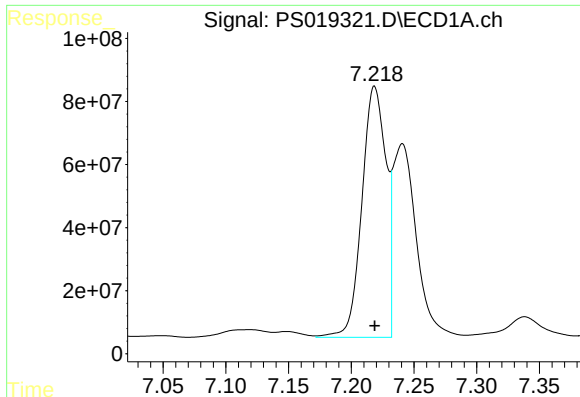

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 1067672771
Conc: 390.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

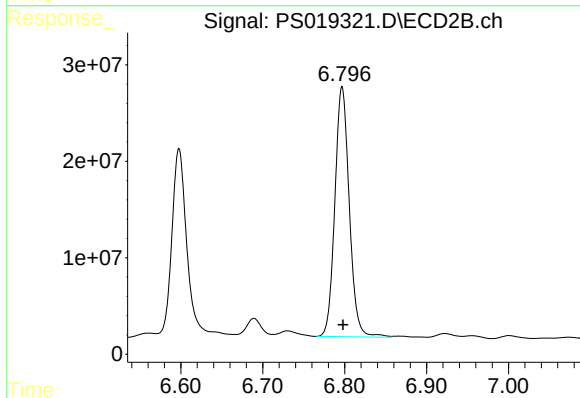


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.001 min
Response: 317109265
Conc: 409.41 ng/ml

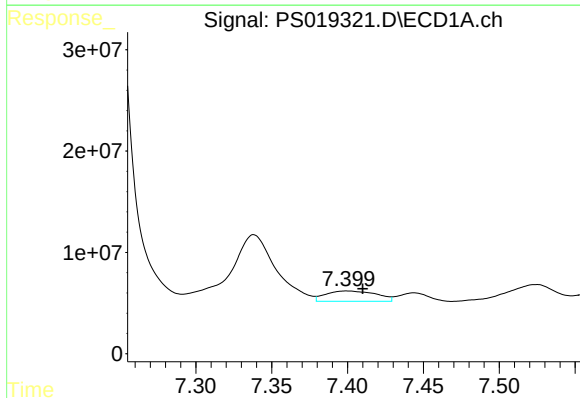


#5 DICAMBA

R.T.: 7.400 min
Delta R.T.: -0.010 min
Response: 23552761
Conc: 2.13 ng/ml

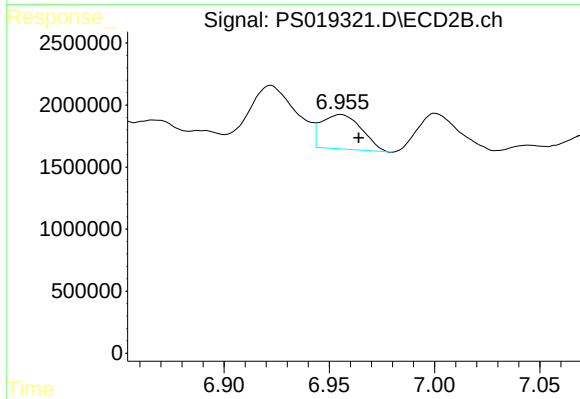

#5 DICAMBA


R.T.: 6.955 min
Delta R.T.: -0.009 min
Response: 3679385
Conc: 1.10 ng/ml

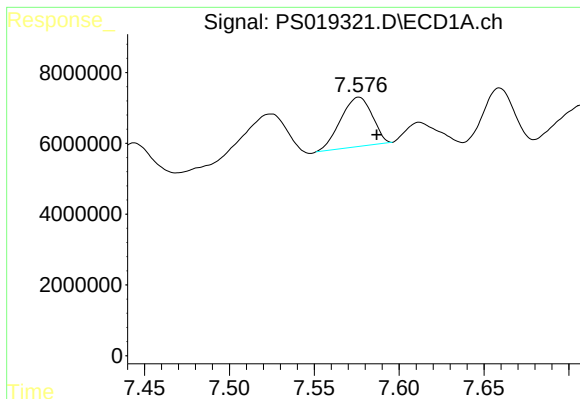

#6 MCP


R.T.: 7.576 min
Delta R.T.: -0.011 min
Response: 17962867
Conc: 2.01 ug/ml

Instrument :
ECD_S
ClientSampleId :

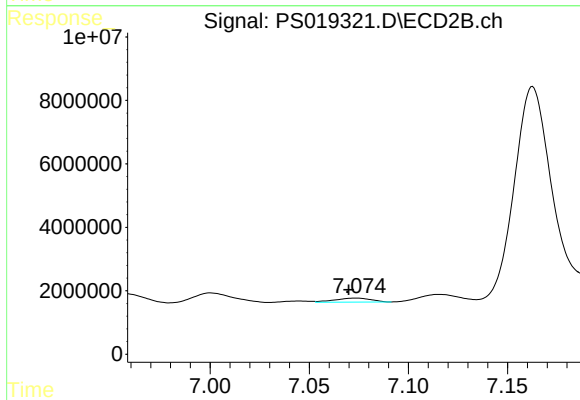


#6 MCP

R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 1566689
Conc: N.D.

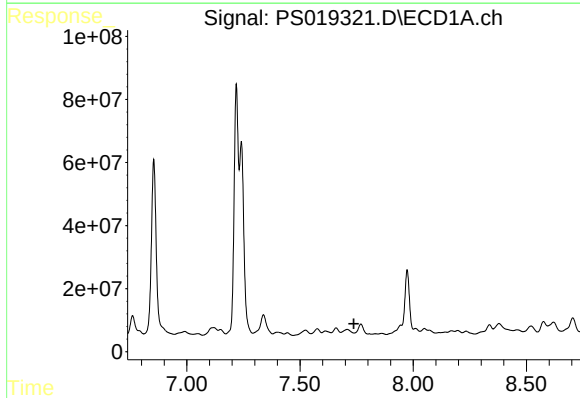


#7 MCP

R.T.: 0.000 min
Exp R.T. : 7.738 min
Response: 0
Conc: N.D.

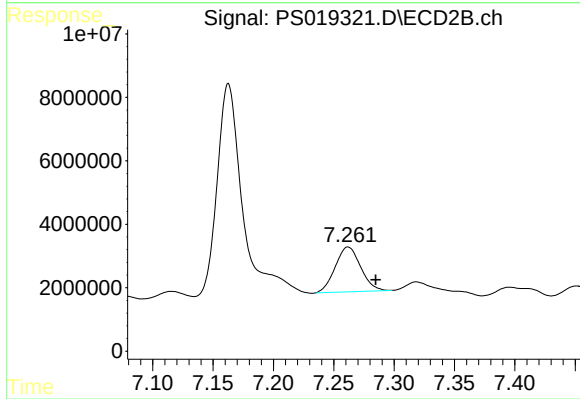

#7 MCP


R.T.: 7.262 min
Delta R.T.: -0.023 min
Response: 20665202
Conc: 5.55 ug/ml

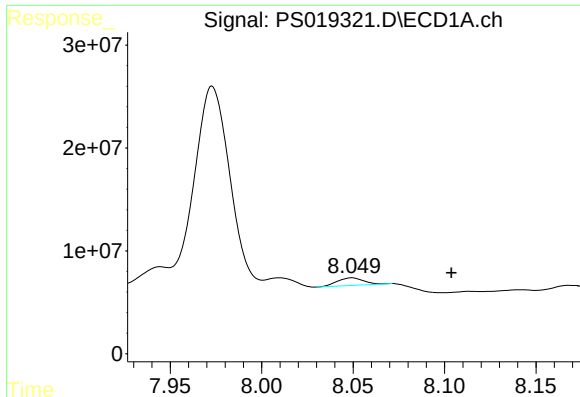

#8 DICHLORPROP


R.T.: 8.049 min
Delta R.T.: -0.054 min
Response: 5750214
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

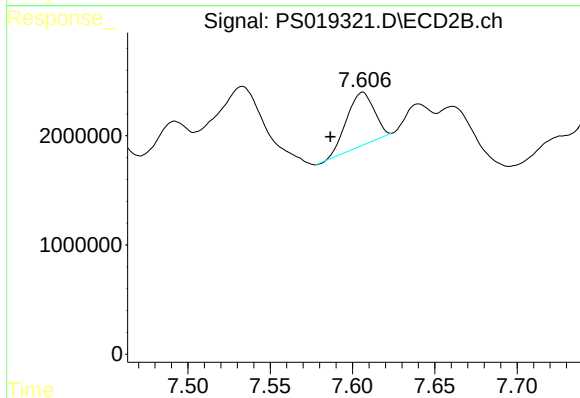


#8 DICHLORPROP

R.T.: 7.606 min
Delta R.T.: 0.020 min
Response: 5608096
Conc: 6.54 ng/ml

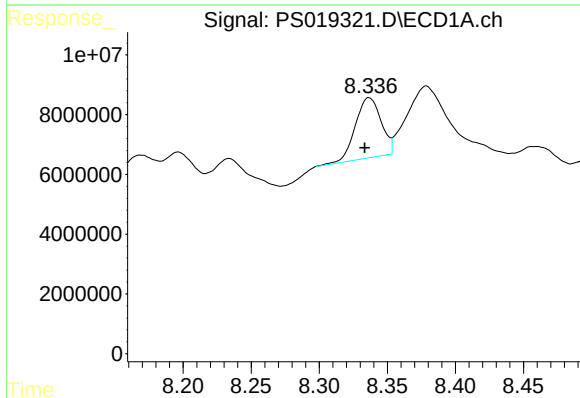


#9 2,4-D

R.T.: 8.337 min
Delta R.T.: 0.003 min
Response: 26615399
Conc: 8.44 ng/ml

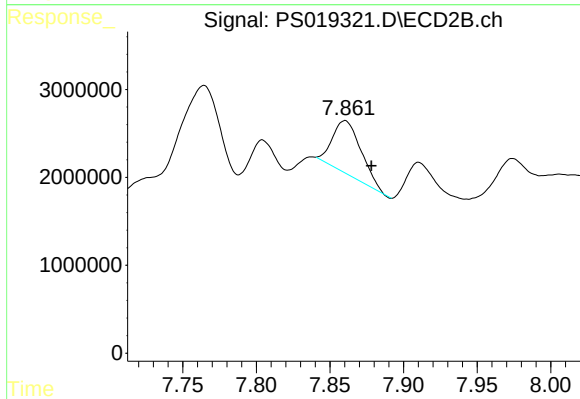

#9 2,4-D


R.T.: 7.860 min
Delta R.T.: -0.018 min
Response: 8162893
Conc: 8.17 ng/ml

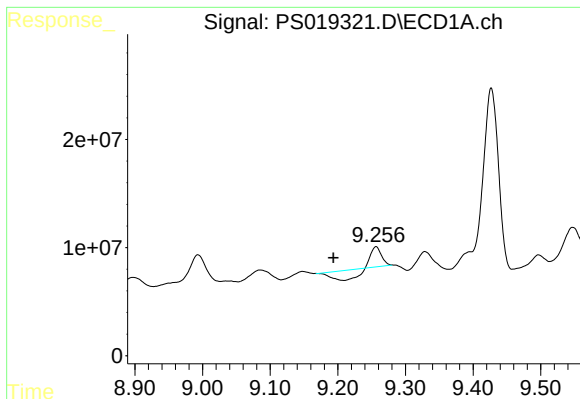

#11 2,4,5-TP (SILVEX)


R.T.: 9.257 min
Delta R.T.: 0.063 min
Response: 45132
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

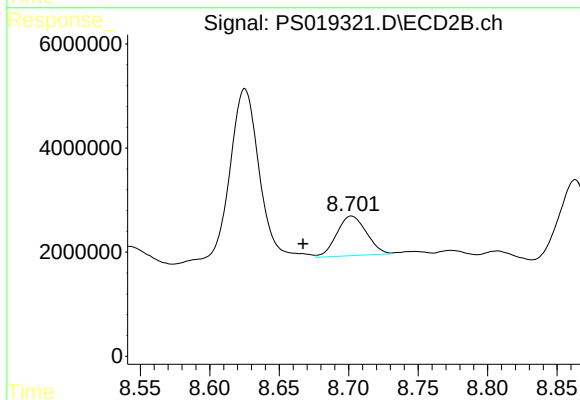


#11 2,4,5-TP (SILVEX)

R.T.: 8.702 min
Delta R.T.: 0.035 min
Response: 11356132
Conc: 2.36 ng/ml

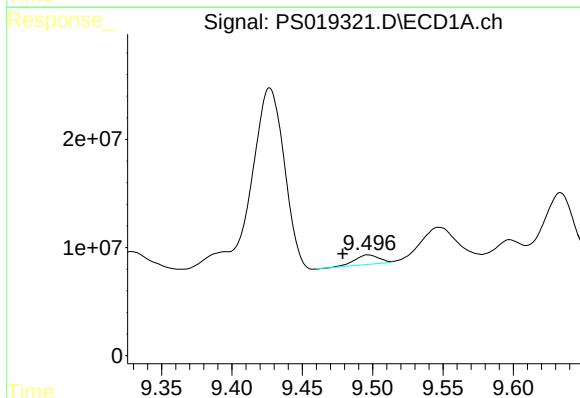


#12 2,4,5-T

R.T.: 9.497 min
Delta R.T.: 0.018 min
Response: 10694532
Conc: N.D.

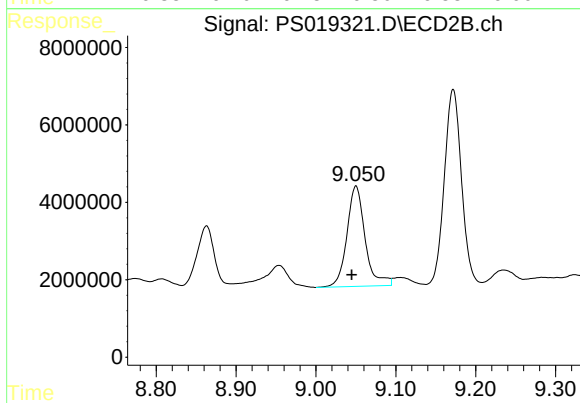

#12 2,4,5-T


R.T.: 9.050 min
Delta R.T.: 0.005 min
Response: 41036192
Conc: 9.48 ng/ml

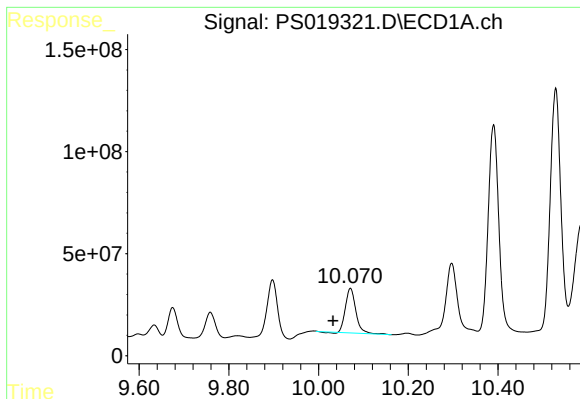

#13 2,4-DB


R.T.: 10.071 min
Delta R.T.: 0.039 min
Response: 352183725
Conc: 82.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

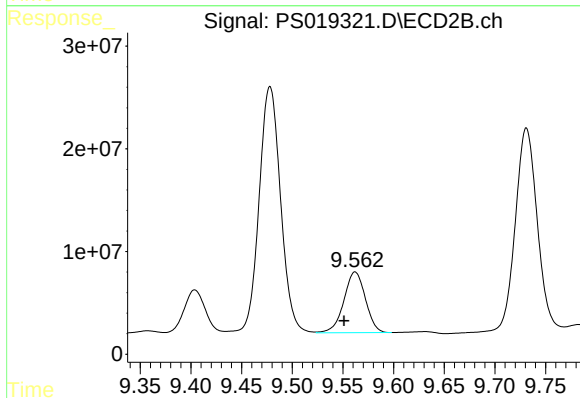


#13 2,4-DB

R.T.: 9.562 min
Delta R.T.: 0.011 min
Response: 87551628
Conc: 153.99 ng/ml

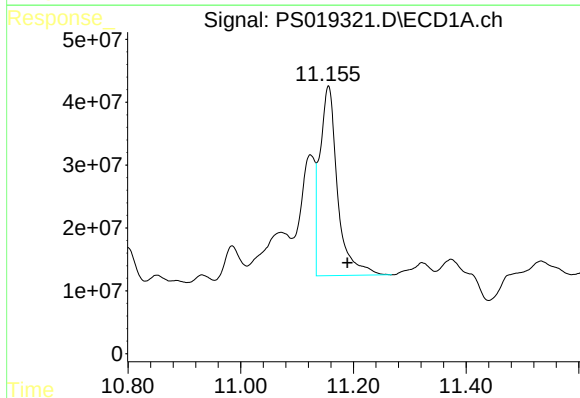


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: -0.034 min
Response: 657222915
Conc: 39.80 ng/ml

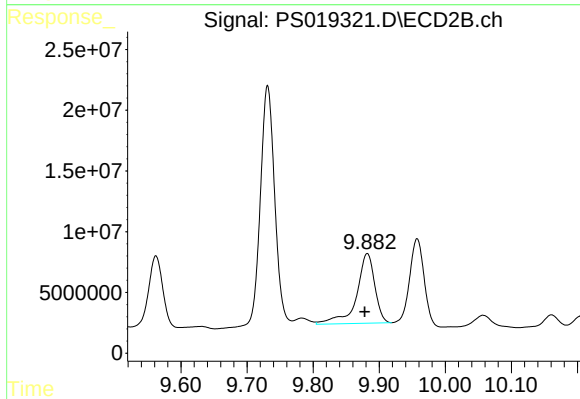

#14 DINOSEB


R.T.: 9.882 min
Delta R.T.: 0.004 min
Response: 109529349
Conc: 37.80 ng/ml

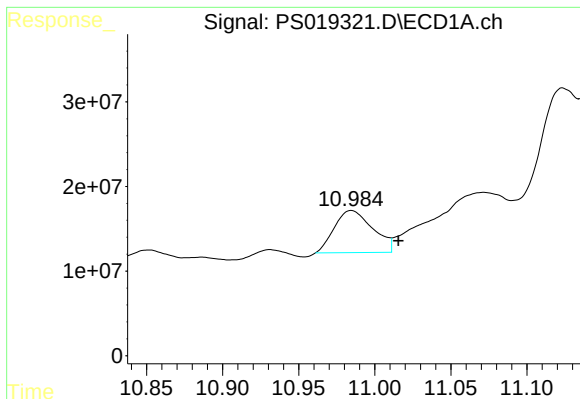

#15 Picloram


R.T.: 10.985 min
Delta R.T.: -0.031 min
Response: 87775694
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

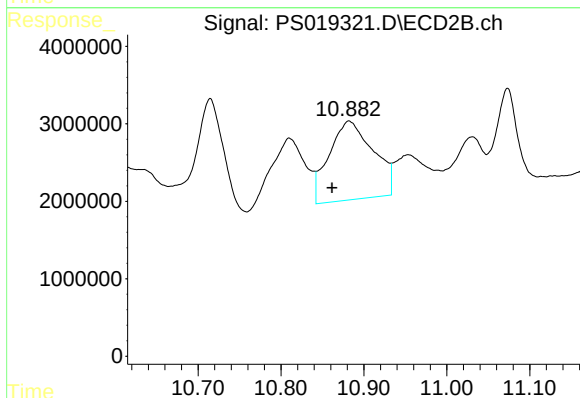


#15 Picloram

R.T.: 10.882 min
Delta R.T.: 0.021 min
Response: 37722012
Conc: 6.31 ng/ml

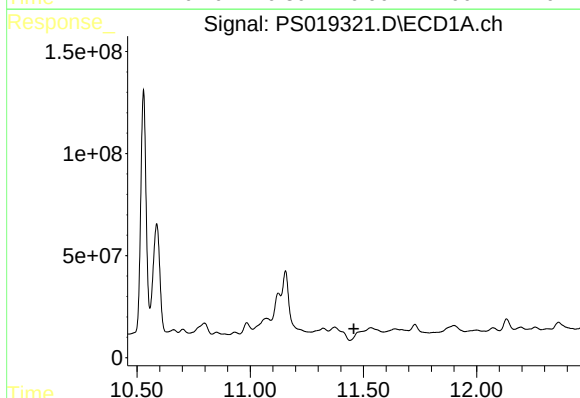

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

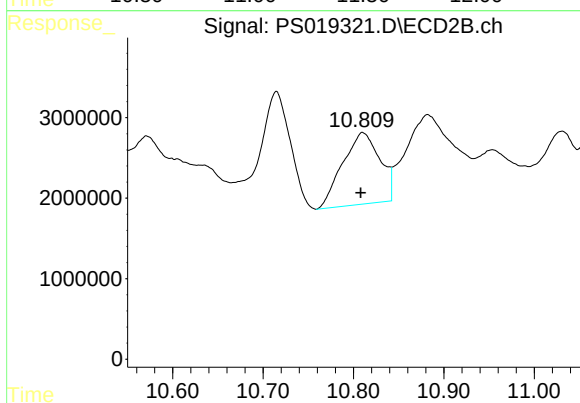

#16 DCPA

R.T.: 10.810 min
Delta R.T.: 0.002 min
Response: 25463130
Conc: 4.34 ng/ml