

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050522\
 Data File : PS019325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2022 23:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:00:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.222	6.799	1284.0E6	385.9E6	470.192	498.188
Target Compounds							
1) T	Dalapon	3.077f	0.000	1364122	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.475f	5.915f	730633	111175	<MDL	<MDL #
5) T	DICAMBA	0.000	7.023f	0	1428142	N.D.	<MDL
6) T	MCP	7.601	7.023f	-654789	1428142	N.D.	<MDL
7) T	MCPA	7.729	0.000	4694114	0	<MDL	N.D. #
10) T	Pentachlo...	8.646	8.308	1968233	1911995	<MDL	<MDL #
11) T	2,4,5-TP ...	9.212	8.640	-610755	2724620	N.D.	<MDL
12) T	2,4,5-T	9.525f	9.079	-1860001	649464	N.D.	<MDL
13) T	2,4-DB	0.000	9.592f	0	124946	N.D.	<MDL
14) T	DINOSEB	11.187	9.885	22204538	1332993	1.345	<MDL #
15) T	Picloram	11.009	10.813f	13955382	6533654	<MDL	1.092 #
16) T	DCPA	11.460	10.813	2160440	6533654	<MDL	1.113 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050522\
Data File : PS019325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2022 23:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:00:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

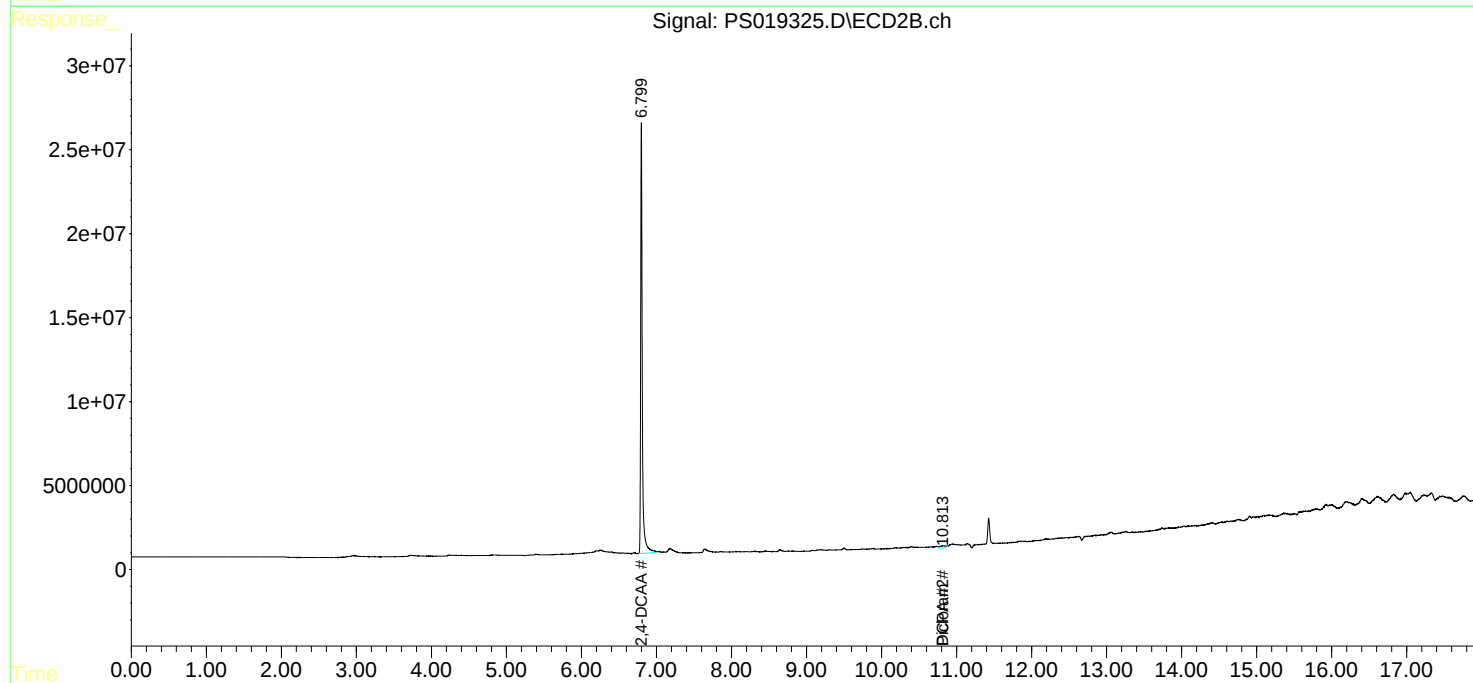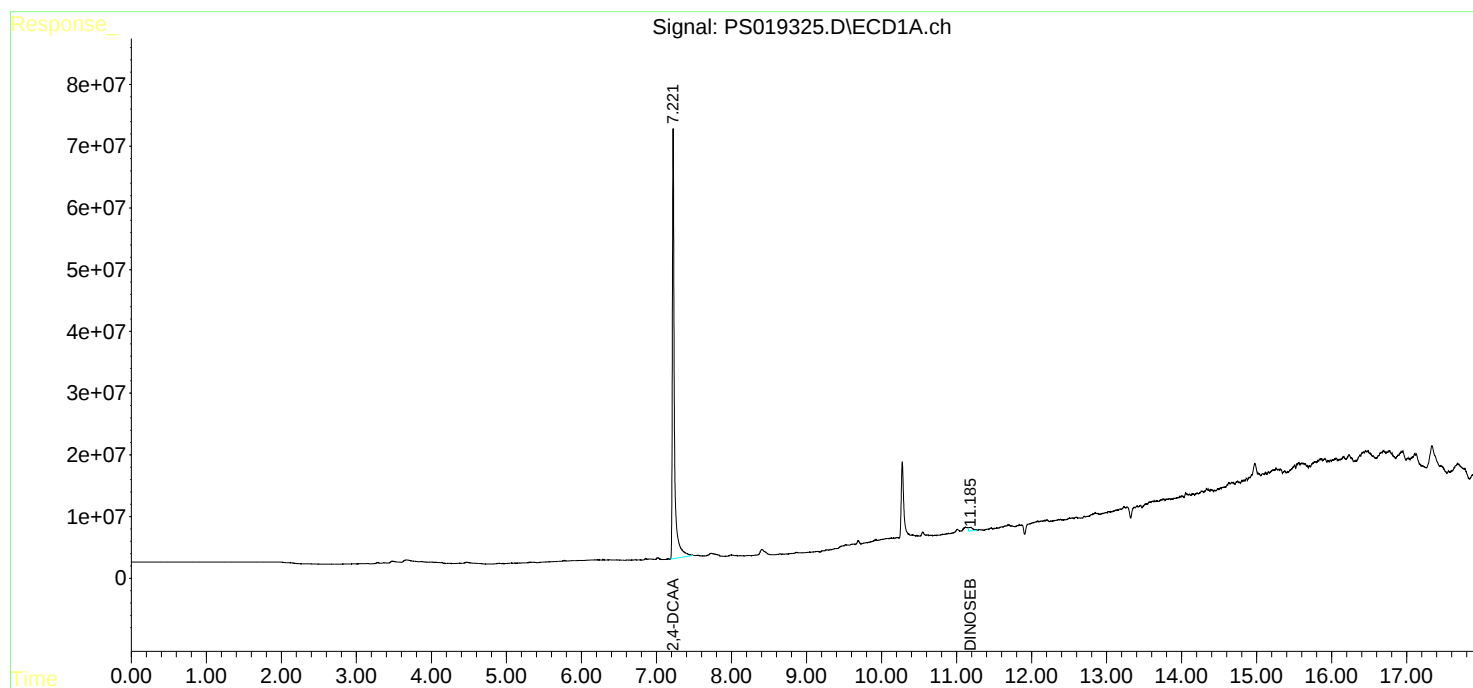


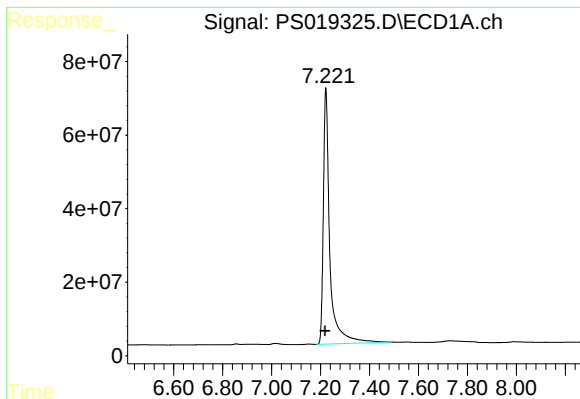

#4 2,4-DCAA


R.T.: 7.222 min
Delta R.T.: 0.003 min
Response: 1284035054
Conc: 470.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

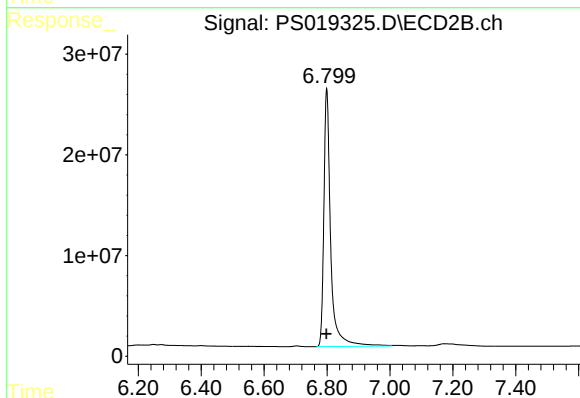


#4 2,4-DCAA

R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 385874448
Conc: 498.19 ng/ml

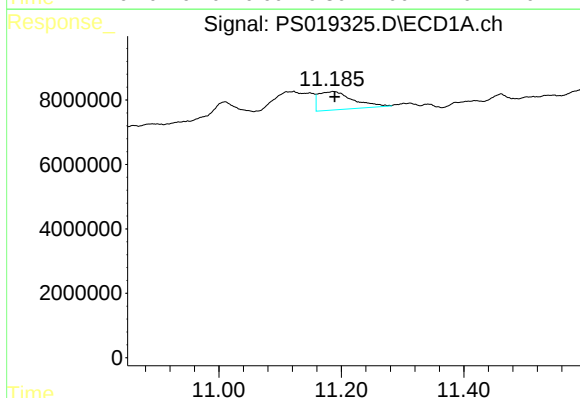


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.002 min
Response: 22204538
Conc: 1.34 ng/ml

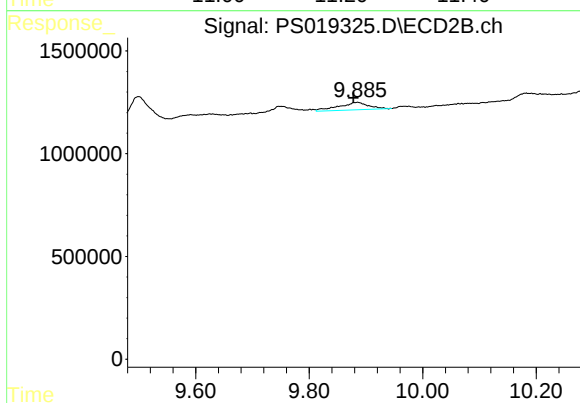

#14 DINOSEB


R.T.: 9.885 min
Delta R.T.: 0.007 min
Response: 1332993
Conc: N.D.

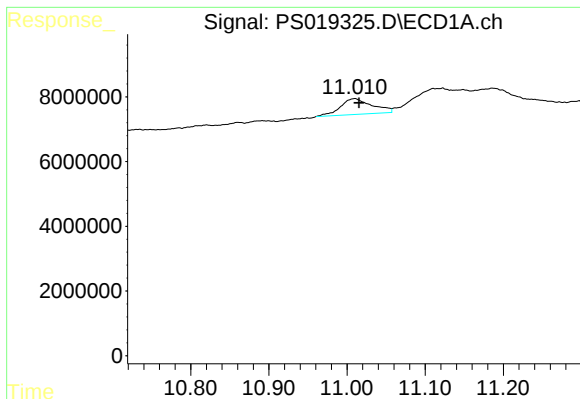

#15 Picloram


R.T.: 11.009 min
Delta R.T.: -0.006 min
Response: 13955382
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

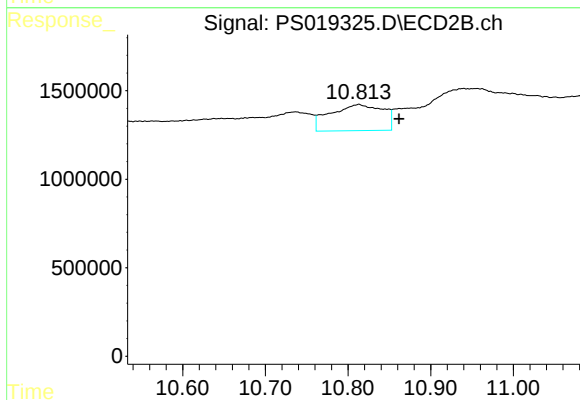


#15 Picloram

R.T.: 10.813 min
Delta R.T.: -0.048 min
Response: 6533654
Conc: 1.09 ng/ml

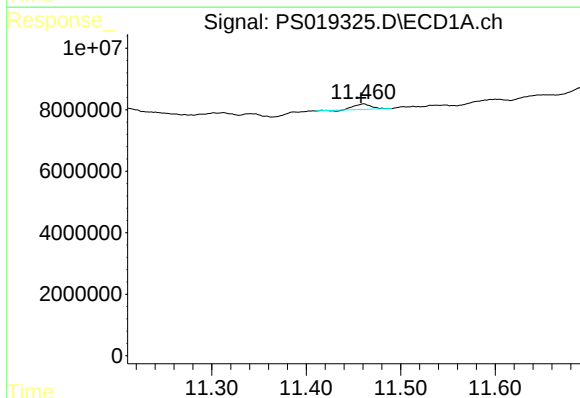

#16 DCPA

R.T.: 11.460 min
Delta R.T.: 0.002 min
Response: 2160440
Conc: N.D.

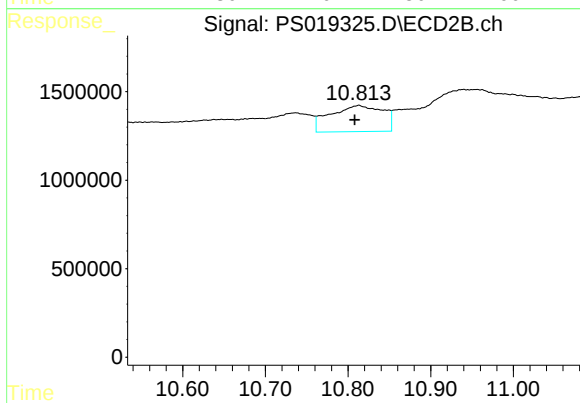

#16 DCPA

R.T.: 10.813 min
Delta R.T.: 0.005 min
Response: 6533654
Conc: 1.11 ng/ml