

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050523\
 Data File : PS022933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2023 02:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 07:23:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.481	6.858	1376.9E6	549.8E6	553.037	539.608
Target Compounds							
1) T	Dalapon	2.582	0.000	5367520	0	1.817	N.D. #
2) T	3,5-DICHL...	5.832	6.103f	708060	24306	<MDL	<MDL #
3) T	4-Nitroph...	6.317	0.000	5738307	0	3.092	N.D. #
5) T	DICAMBA	6.629	0.000	1265886	0	<MDL	N.D. #
6) T	MCP	6.815	0.000	10694966	0	1.271	N.D. #
7) T	MCPA	6.933	7.305	239785	6285079	<MDL	1.300 #
8) T	DICHLORPROP	7.242	7.665	2989185	4539405	<MDL	4.076 #
9) T	2,4-D	7.403f	0.000	15443689	0	4.171	N.D. #
10) T	Pentachlo...	7.676	8.366	4877317	3774433	<MDL	<MDL #
11) T	2,4,5-TP ...	8.212	8.727	8946797	813744	<MDL	<MDL #
12) T	2,4,5-T	8.473	9.101	5414113	1179471	<MDL	<MDL #
13) T	2,4-DB	8.929f	9.686f	21155495	1187274	4.951	1.585 #
14) T	DINOSEB	10.061	0.000	2107336	0	<MDL	N.D. #
15) T	Picloram	9.885	10.905	46665668	8383641	1.567	1.031 #
16) T	DCPA	10.330	10.905	6046343	8383641	<MDL	1.207 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050523\
Data File : PS022933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2023 02:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 07:23:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

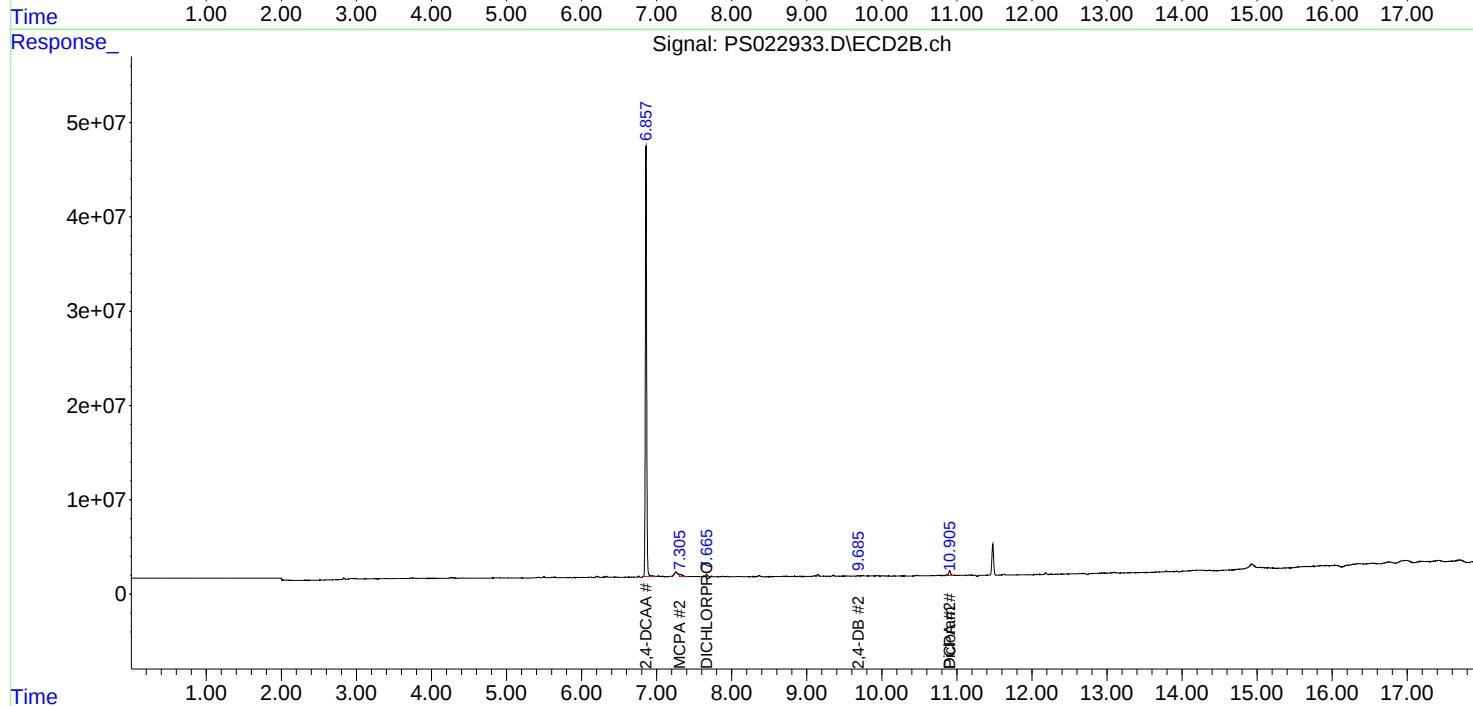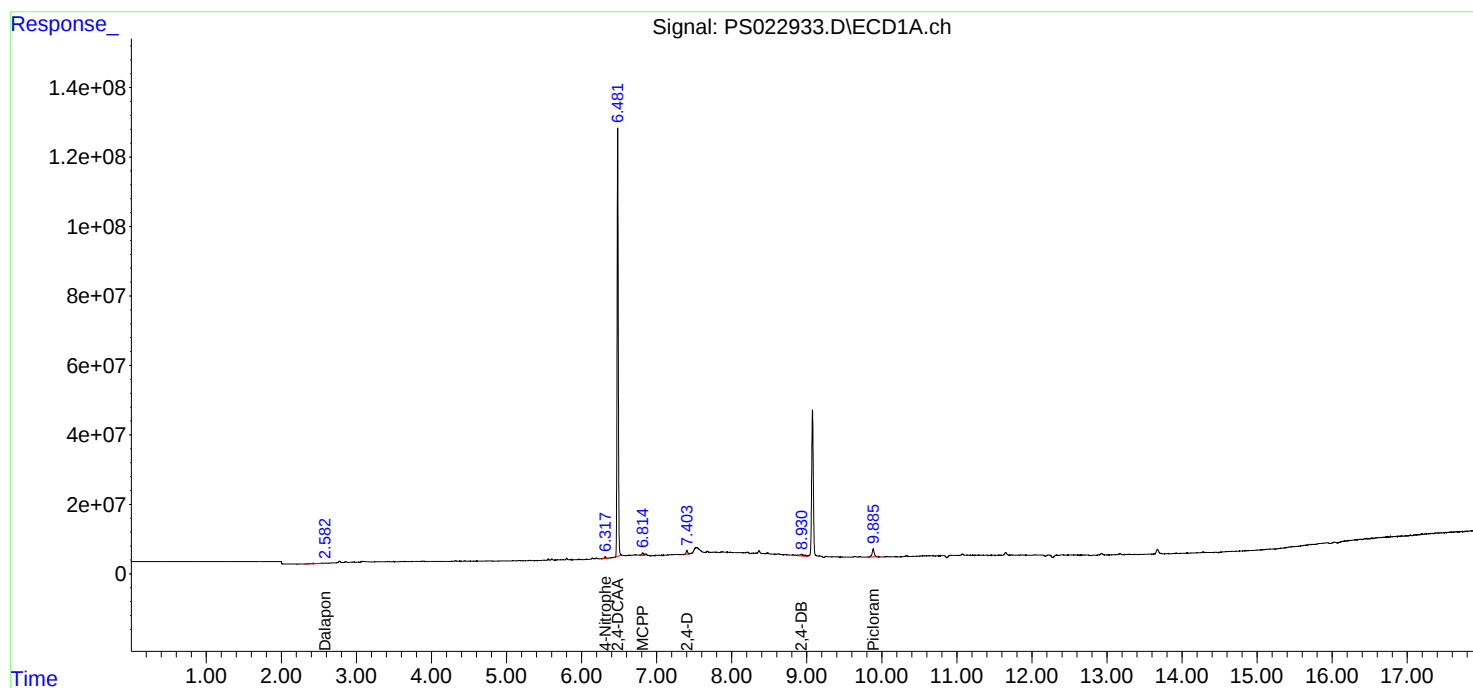


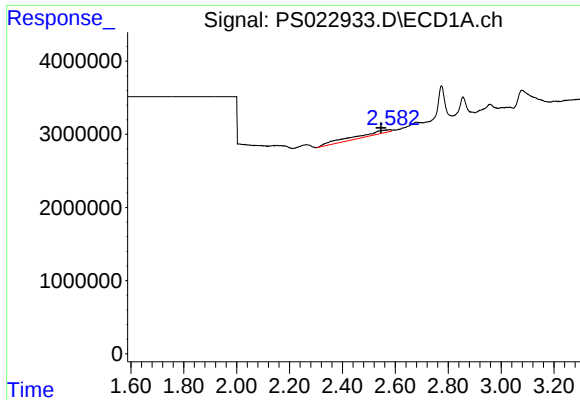

#1 Dalapon


R.T.: 2.582 min
Delta R.T.: 0.035 min
Response: 5367520
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

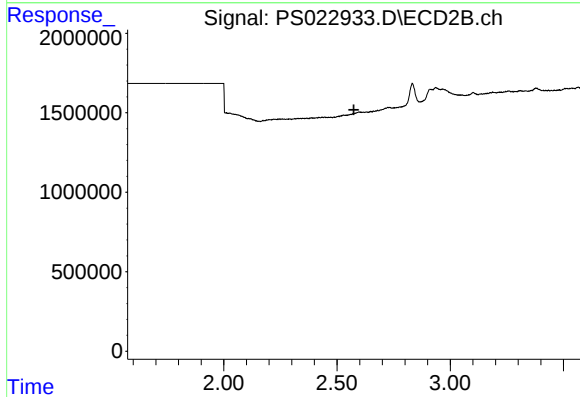


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

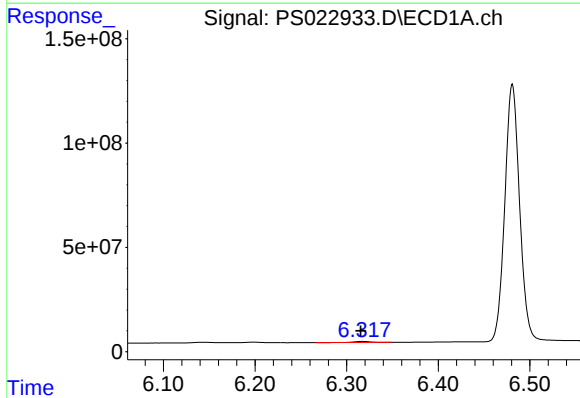


#3 4-Nitrophenol

R.T.: 6.317 min
Delta R.T.: 0.002 min
Response: 5738307
Conc: 3.09 ng/ml

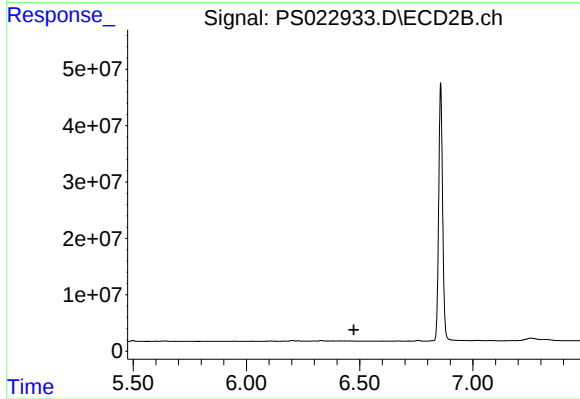

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

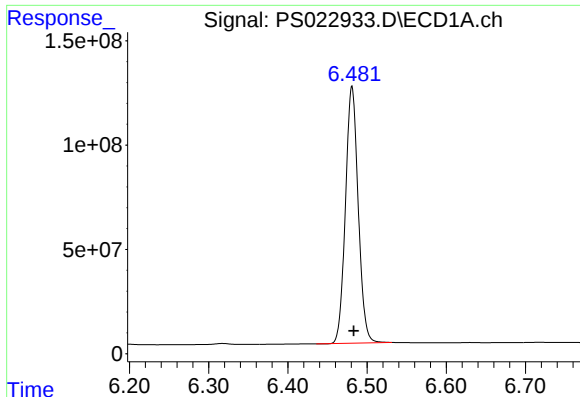

#4 2,4-DCAA


R.T.: 6.481 min
Delta R.T.: -0.002 min
Response: 1376899078
Conc: 553.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

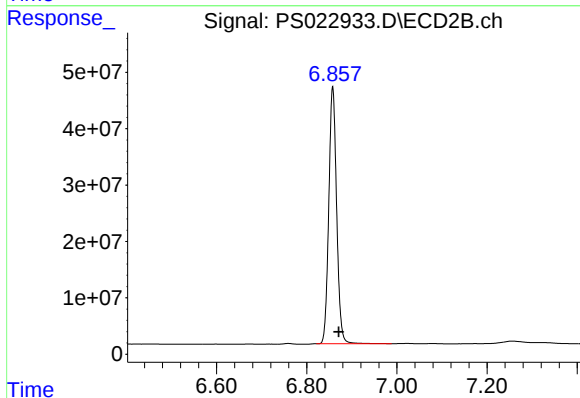


#4 2,4-DCAA

R.T.: 6.858 min
Delta R.T.: -0.013 min
Response: 549831033
Conc: 539.61 ng/ml

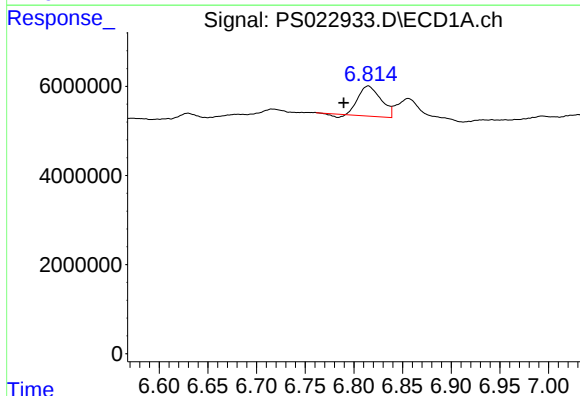


#6 MCP

R.T.: 6.815 min
Delta R.T.: 0.025 min
Response: 10694966
Conc: 1.27 ug/ml

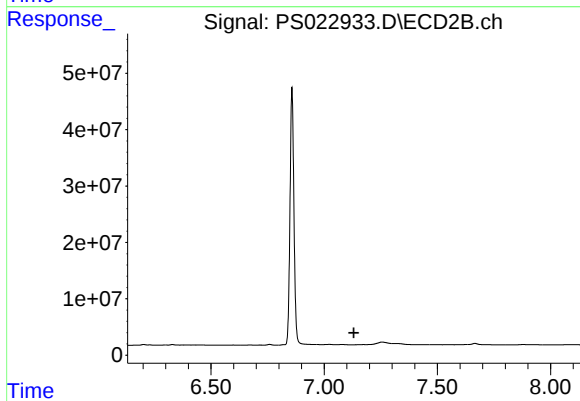

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.132 min
Response: 0
Conc: N.D.

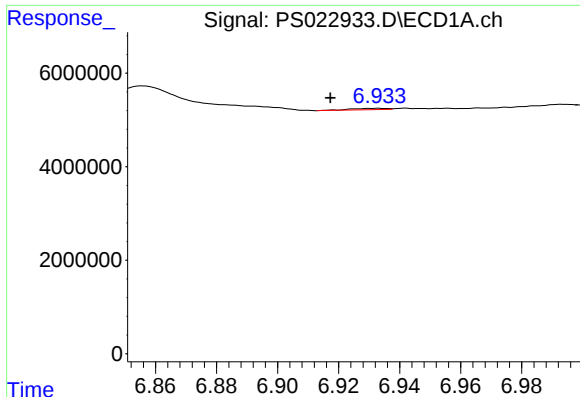

#7 MCPA


R.T.: 6.933 min
Delta R.T.: 0.015 min
Response: 239785
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

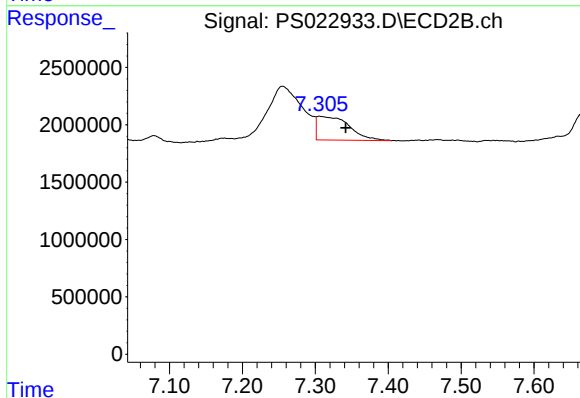


#7 MCPA

R.T.: 7.305 min
Delta R.T.: -0.037 min
Response: 6285079
Conc: 1.30 ug/ml

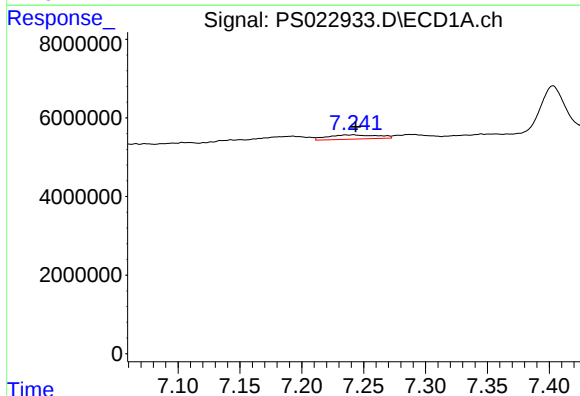


#8 DICHLORPROP

R.T.: 7.242 min
Delta R.T.: -0.002 min
Response: 2989185
Conc: N.D.

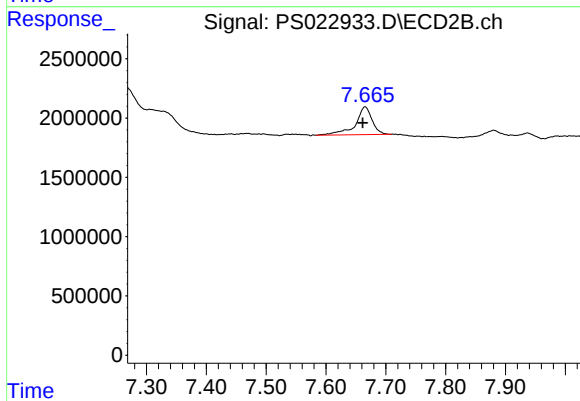

#8 DICHLORPROP


R.T.: 7.665 min
Delta R.T.: 0.004 min
Response: 4539405
Conc: 4.08 ng/ml

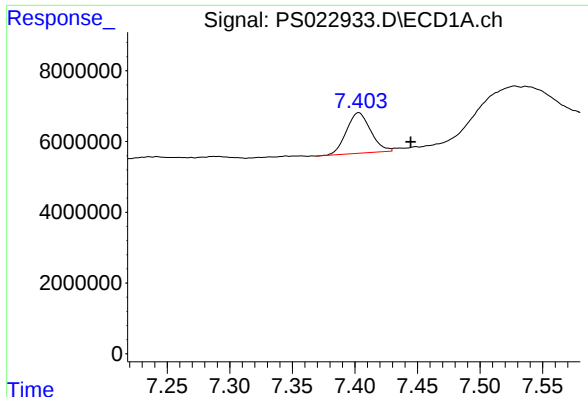

#9 2,4-D


R.T.: 7.403 min
Delta R.T.: -0.042 min
Response: 15443689
Conc: 4.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

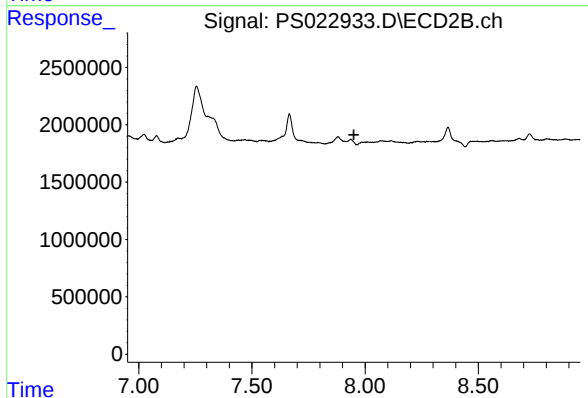


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.950 min
Response: 0
Conc: N.D.

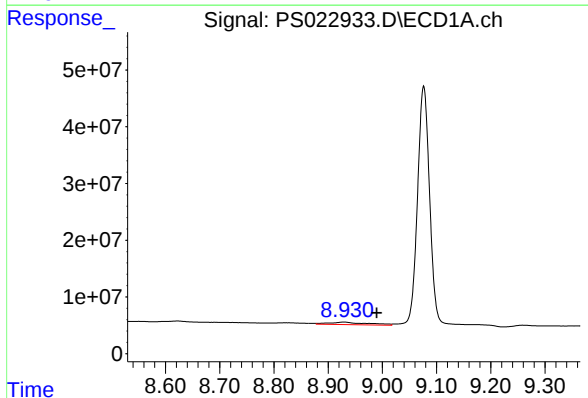


#13 2,4-DB

R.T.: 8.929 min
Delta R.T.: -0.060 min
Response: 21155495
Conc: 4.95 ng/ml

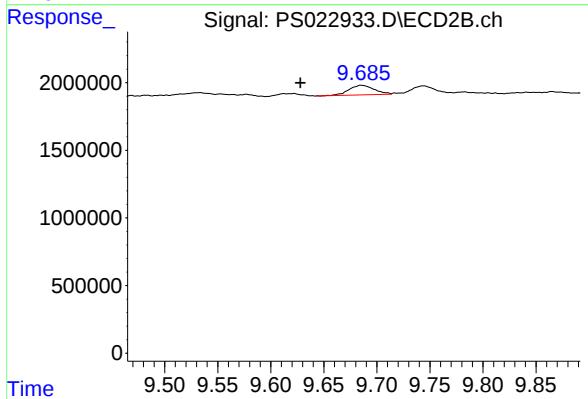

#13 2,4-DB


R.T.: 9.686 min
Delta R.T.: 0.058 min
Response: 1187274
Conc: 1.58 ng/ml

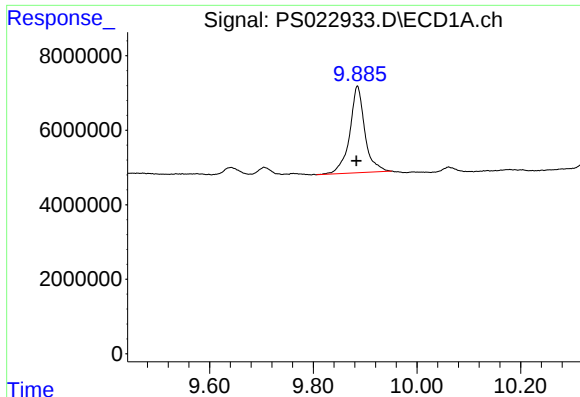

#15 Picloram


R.T.: 9.885 min
Delta R.T.: 0.002 min
Response: 46665668
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

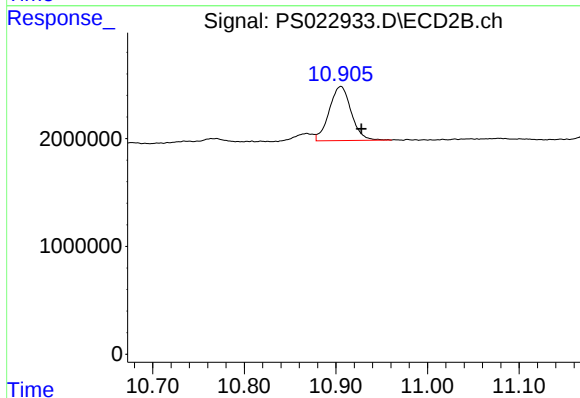


#15 Picloram

R.T.: 10.905 min
Delta R.T.: -0.023 min
Response: 8383641
Conc: 1.03 ng/ml

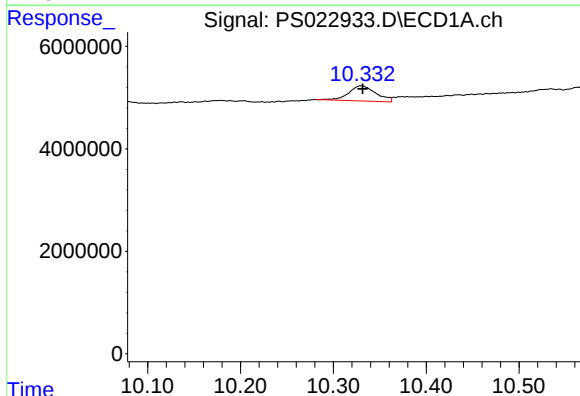

#16 DCPA

R.T.: 10.330 min
Delta R.T.: -0.001 min
Response: 6046343
Conc: N.D.

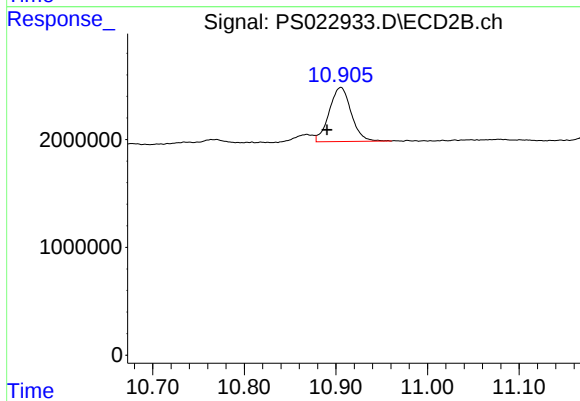

#16 DCPA

R.T.: 10.905 min
Delta R.T.: 0.015 min
Response: 8383641
Conc: 1.21 ng/ml