

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050523\
 Data File : PS022939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2023 06:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 07:26:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.481	6.858	1399.4E6	554.7E6	562.076	544.397
Target Compounds							
1) T	Dalapon	2.572	0.000	1607422	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.832	0.000	747322	0	<MDL	N.D. #
3) T	4-Nitroph...	6.317	0.000	5519676	0	2.975	N.D. #
5) T	DICAMBA	6.630	7.080f	709107	990225	<MDL	<MDL #
6) T	MCP	6.815	7.080f	8116404	990225	<MDL	<MDL #
7) T	MCPA	6.961f	7.312	245927	4015404	<MDL	<MDL #
8) T	DICHLORPROP	7.248	7.666	1437183	3534825	<MDL	3.174 #
9) T	2,4-D	7.440	0.000	661869	0	<MDL	N.D. #
10) T	Pentachlo...	7.675	8.366	3380085	2975943	<MDL	<MDL #
11) T	2,4,5-TP ...	8.211	0.000	10255427	0	<MDL	N.D. #
12) T	2,4,5-T	8.475	9.101	6734427	1110254	<MDL	<MDL #
13) T	2,4-DB	8.980	9.685f	6560722	1250592	1.535	1.669
14) T	DINOSEB	10.062	0.000	1304725	0	<MDL	N.D. #
15) T	Picloram	9.887	10.906	35268851	5847317	1.184	<MDL #
16) T	DCPA	10.331	10.906	3368977	5847317	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050523\
Data File : PS022939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2023 06:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 07:26:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

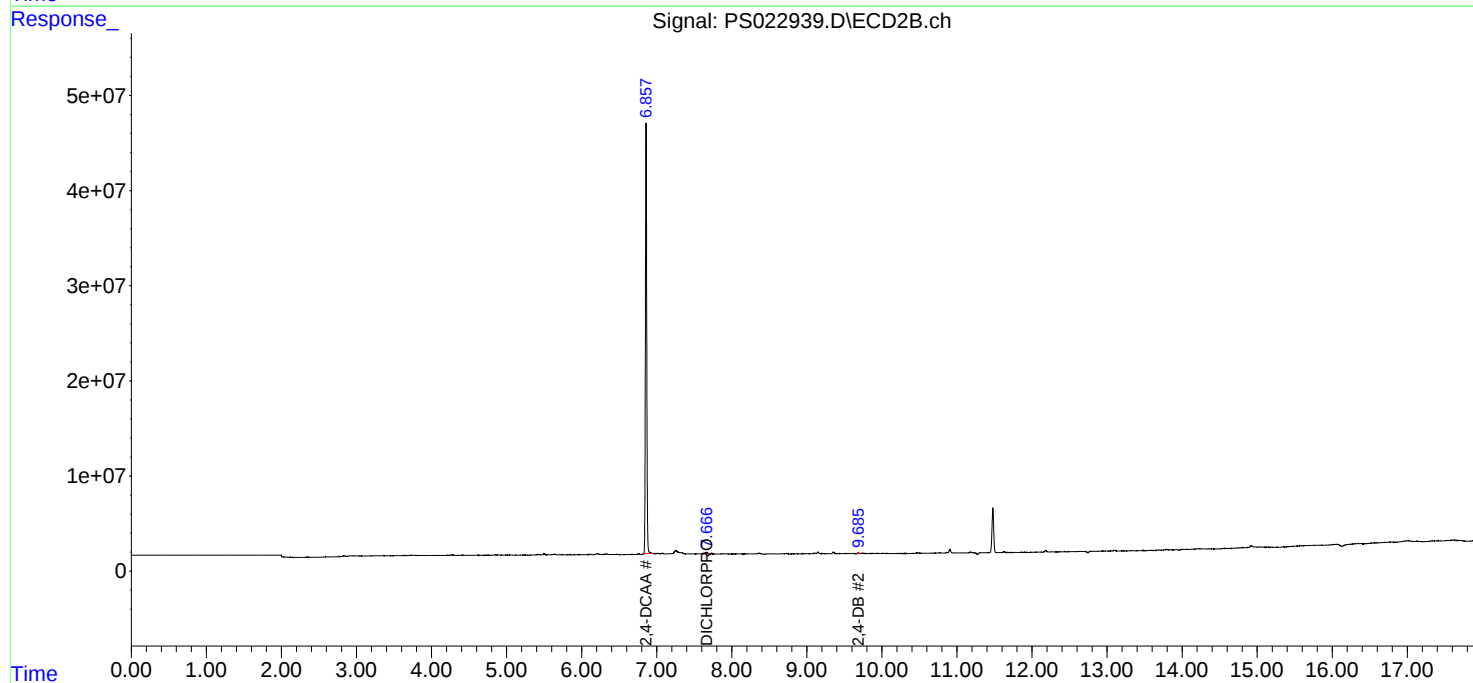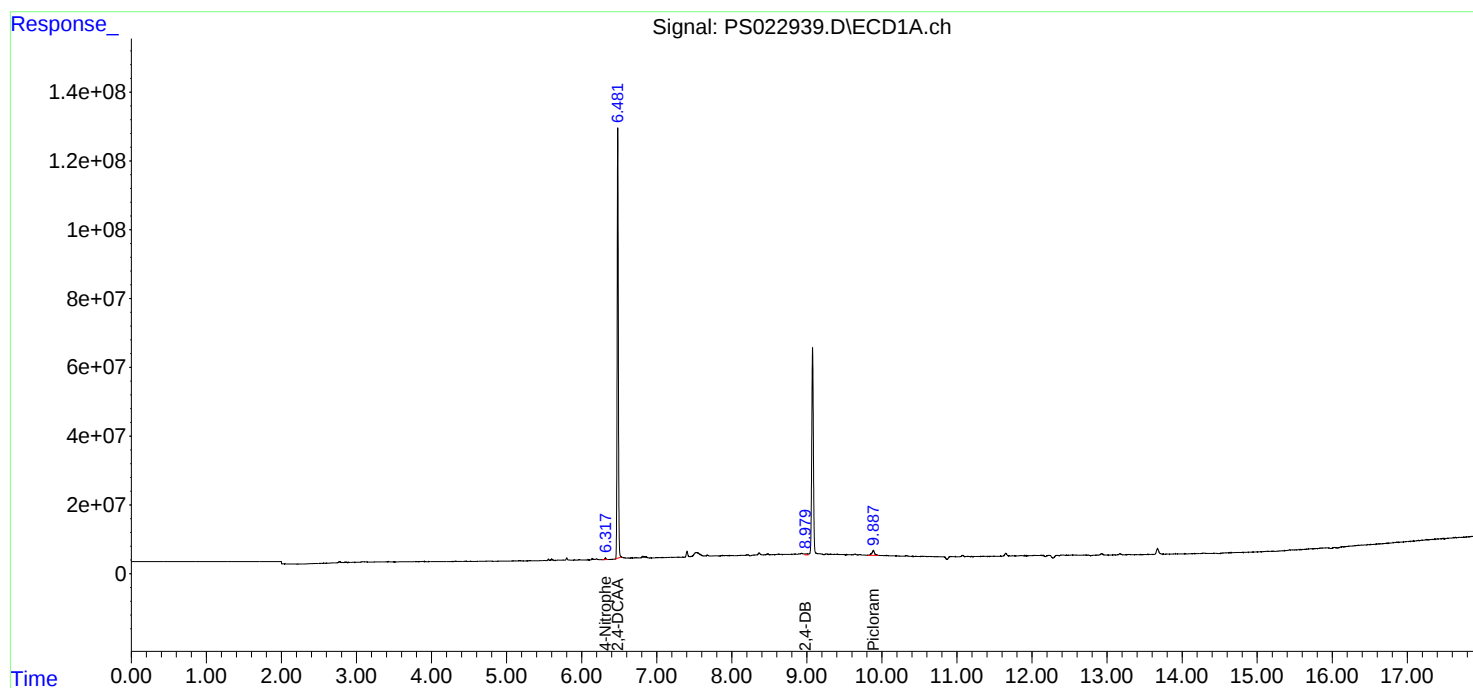


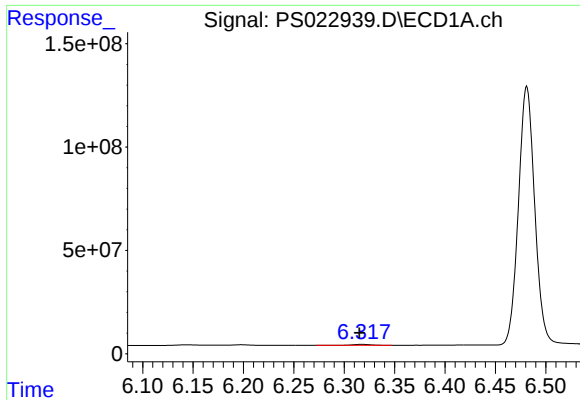

#3 4-Nitrophenol


R.T.: 6.317 min
Delta R.T.: 0.002 min
Response: 5519676
Conc: 2.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

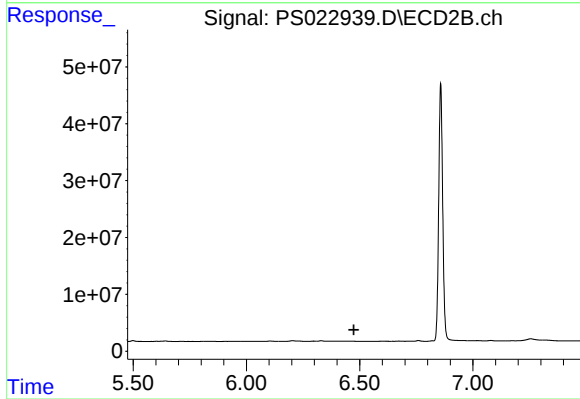


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

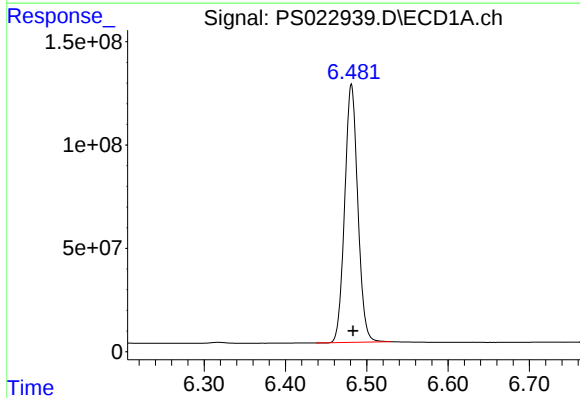


#4 2,4-DCAA

R.T.: 6.481 min
Delta R.T.: -0.002 min
Response: 1399403444
Conc: 562.08 ng/ml

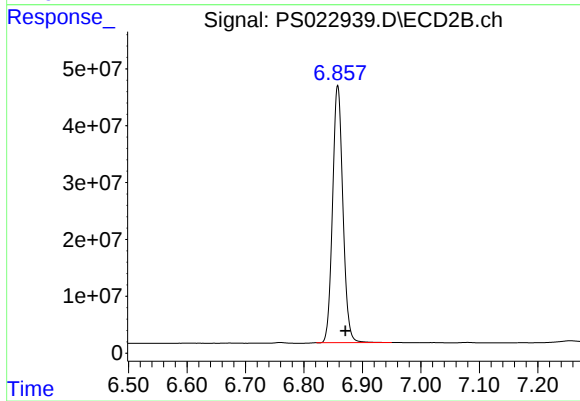

#4 2,4-DCAA


R.T.: 6.858 min
Delta R.T.: -0.013 min
Response: 554710615
Conc: 544.40 ng/ml

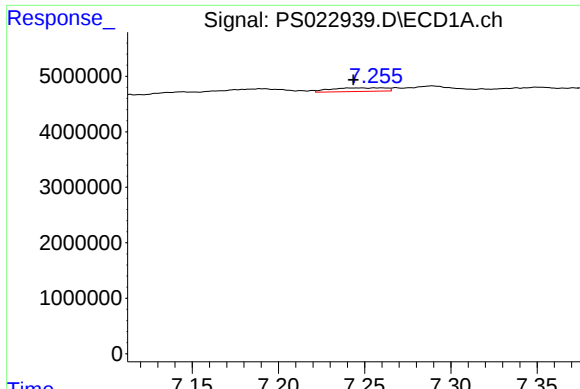

#8 DICHLORPROP


R.T.: 7.248 min
Delta R.T.: 0.005 min
Response: 1437183
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

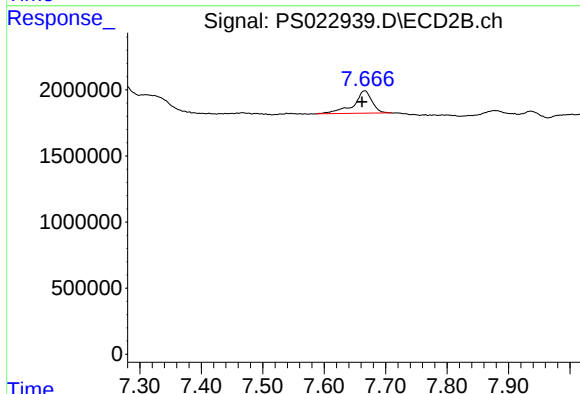


#8 DICHLORPROP

R.T.: 7.666 min
Delta R.T.: 0.005 min
Response: 3534825
Conc: 3.17 ng/ml

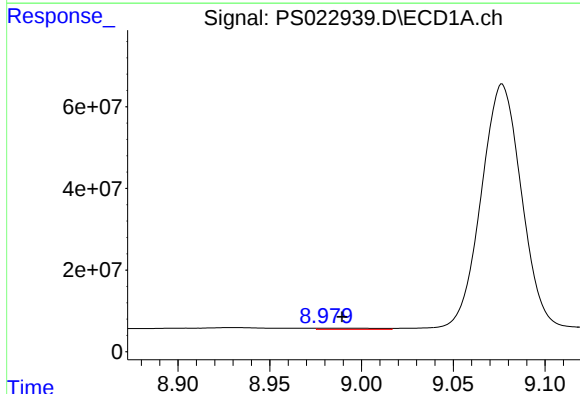


#13 2,4-DB

R.T.: 8.980 min
Delta R.T.: -0.009 min
Response: 6560722
Conc: 1.54 ng/ml

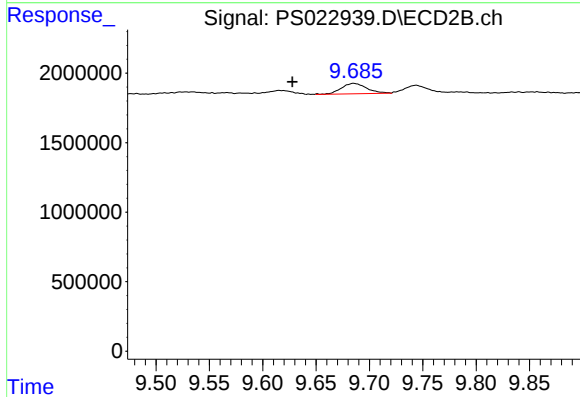

#13 2,4-DB


R.T.: 9.685 min
Delta R.T.: 0.058 min
Response: 1250592
Conc: 1.67 ng/ml

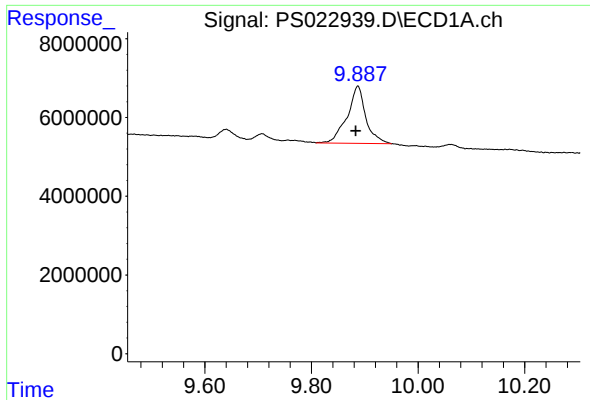

#15 Picloram

R.T.: 9.887 min
Delta R.T.: 0.004 min
Response: 35268851
Conc: 1.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

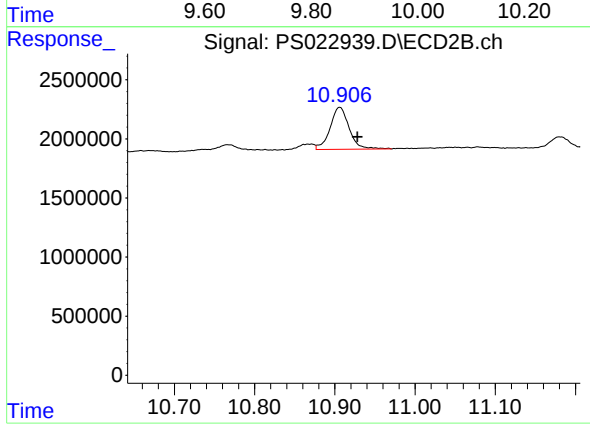

#15 Picloram

R.T.: 10.906 min
Delta R.T.: -0.022 min
Response: 5847317
Conc: N.D.