

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
 Data File : PS004446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 11:06
 Operator : EI\SJ
 Sample : K2635-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-05-050219-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 04:45:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.039	5.732	288.0E6	201.5E6	457.547	417.828
Target Compounds							
1) T	Dalapon	2.404	2.068	58951817	158.6E6	75.022	236.951 #
2) T	3,5-DICHL...	0.000	5.003	0	10979306	N.D.	17.860
3) T	4-Nitroph...	5.888	5.393	12620813	17899529	50.503	72.363 #
5) T	DICAMBA	6.179	5.840	13053254	12266759	5.489	6.554
6) T	MCPD	6.346	0.000	10233532	0	5.923	N.D. #
7) T	MCPA	6.451	6.067	12532508	38556689	4.864	19.409 #
8) T	DICHLORPROP	6.785	6.429	3660988	10482138	6.397	22.275 #
9) T	2,4-D	0.000	6.621	0	10585707	N.D.	20.132
10) T	Pentachlo...	0.000	7.083	0	3745726	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	7.392	0	118.2E6	N.D.	44.984
12) T	2,4,5-T	8.071	7.870	169.9E6	4733512	49.914	2.104 #
13) T	2,4-DB	8.641	0.000	12841598	0	38.169	N.D. #
15) T	Picloram	0.000	9.569	0	1826713	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
Data File : PS004446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 11:06
Operator : EI\SJ
Sample : K2635-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 04:45:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

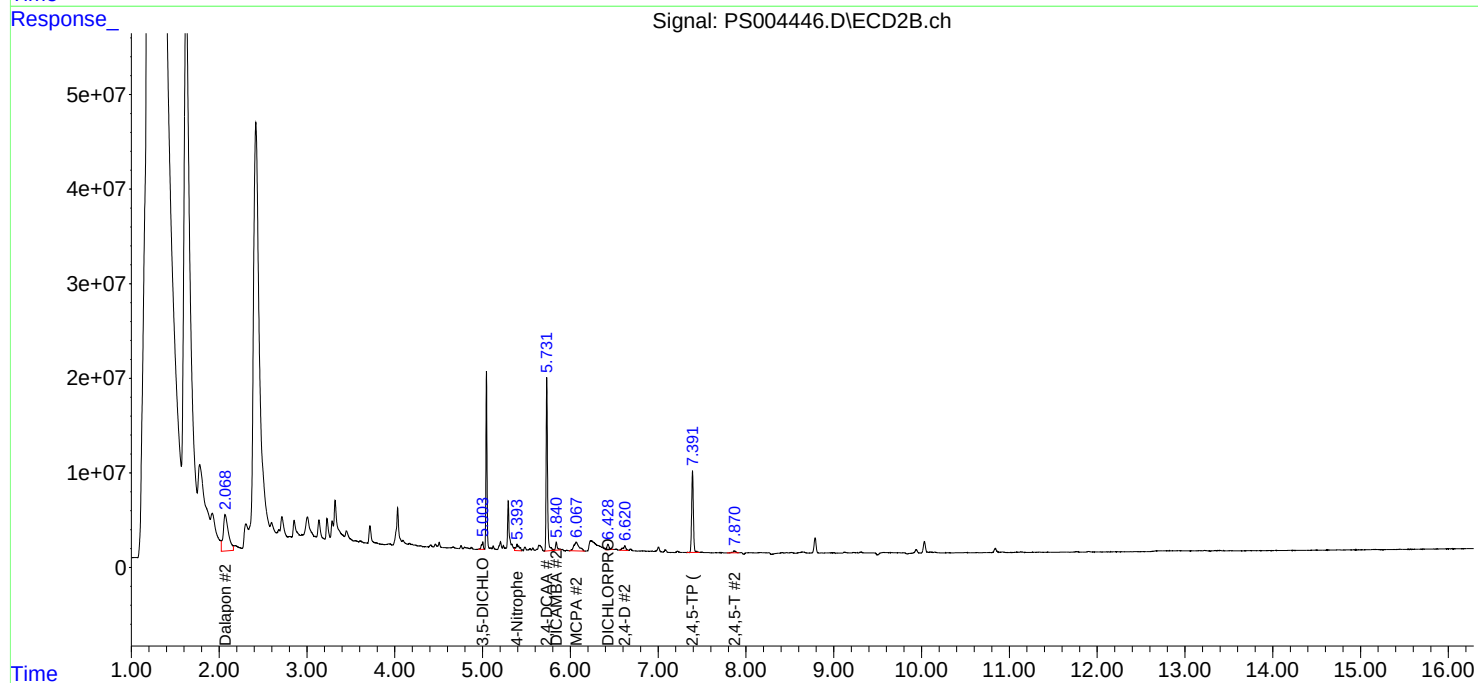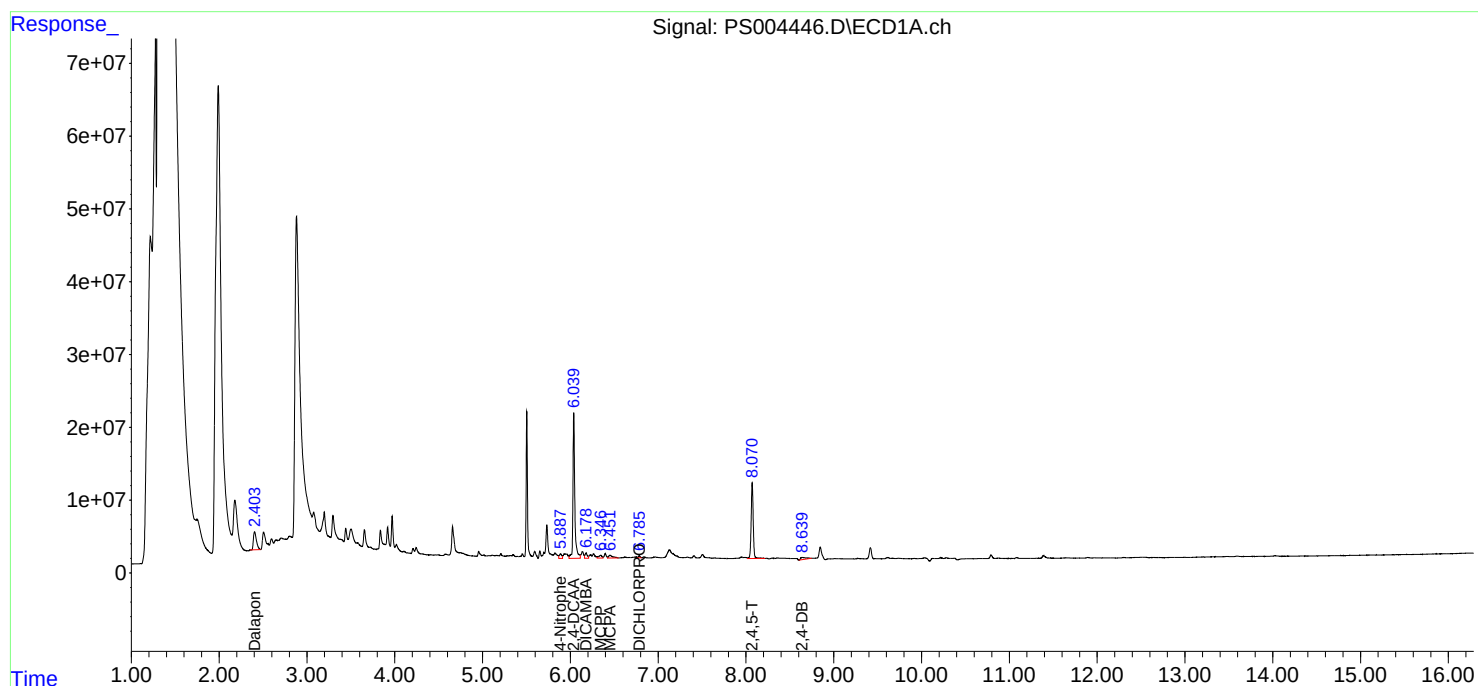


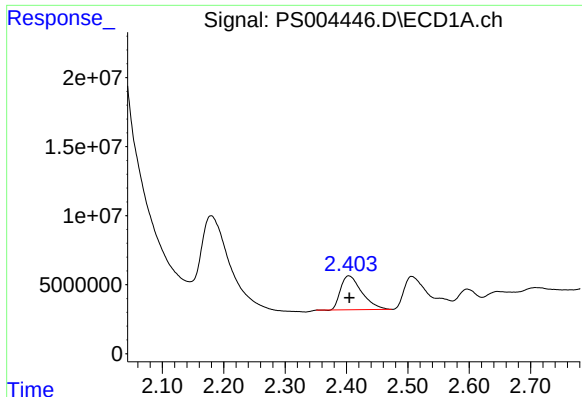

#1 Dalapon


R.T.: 2.404 min
Delta R.T.: -0.001 min
Response: 58951817
Conc: 75.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

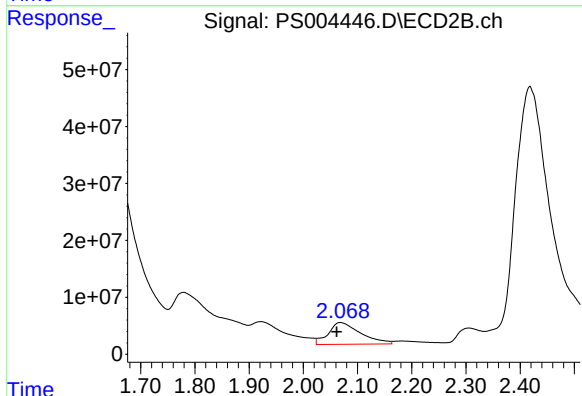


#1 Dalapon

R.T.: 2.068 min
Delta R.T.: 0.007 min
Response: 158564375
Conc: 236.95 ng/ml

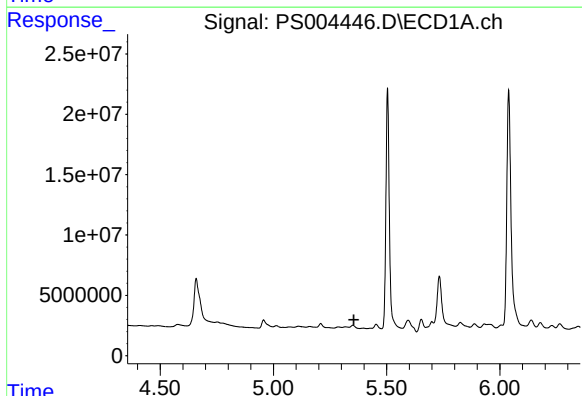


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

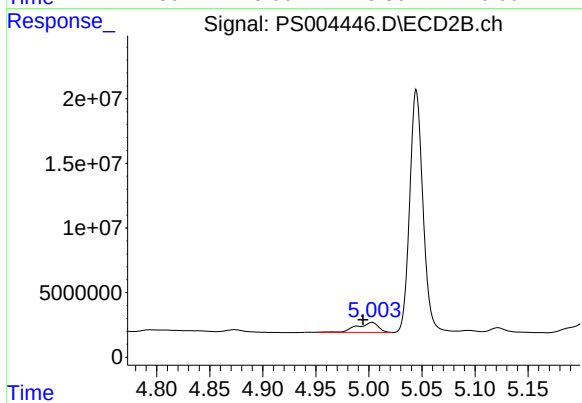

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.003 min
Delta R.T.: 0.008 min
Response: 10979306
Conc: 17.86 ng/ml

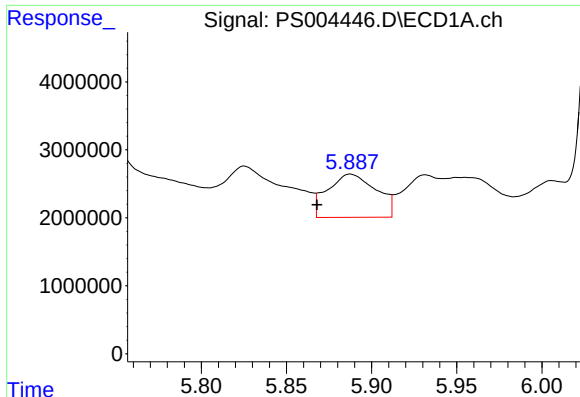

#3 4-Nitrophenol


R.T.: 5.888 min
Delta R.T.: 0.020 min
Response: 12620813
Conc: 50.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

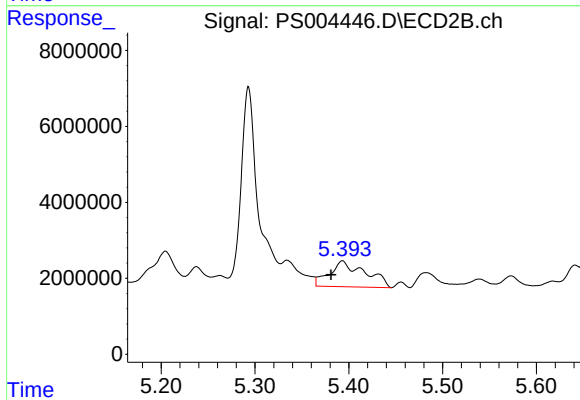


#3 4-Nitrophenol

R.T.: 5.393 min
Delta R.T.: 0.012 min
Response: 17899529
Conc: 72.36 ng/ml

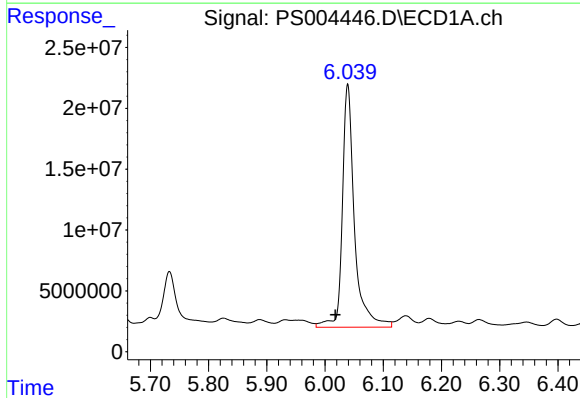


#4 2,4-DCAA

R.T.: 6.039 min
Delta R.T.: 0.021 min
Response: 288006137
Conc: 457.55 ng/ml

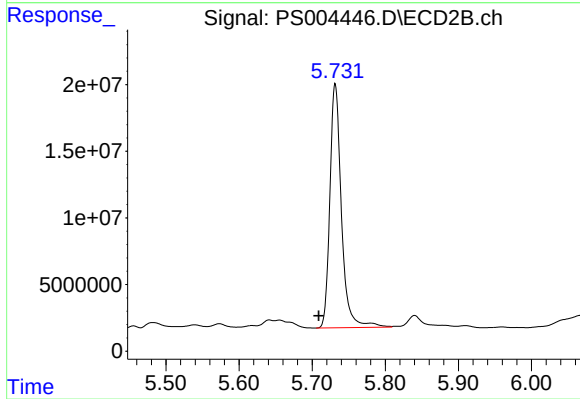

#4 2,4-DCAA


R.T.: 5.732 min
Delta R.T.: 0.023 min
Response: 201511268
Conc: 417.83 ng/ml

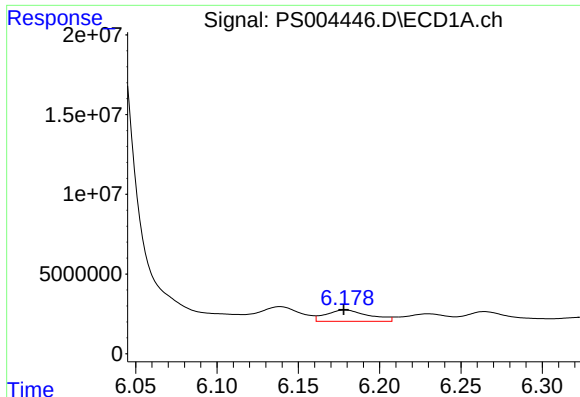

#5 DICAMBA


R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 13053254
Conc: 5.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

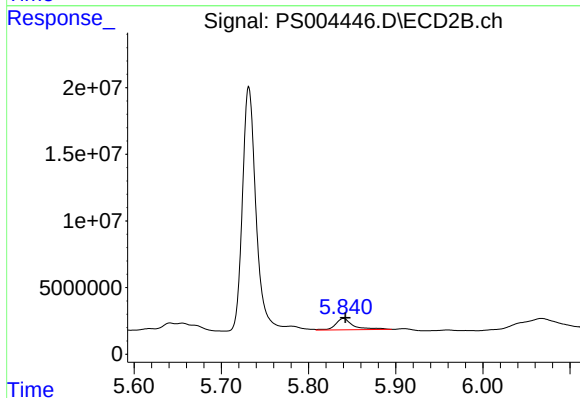


#5 DICAMBA

R.T.: 5.840 min
Delta R.T.: -0.002 min
Response: 12266759
Conc: 6.55 ng/ml

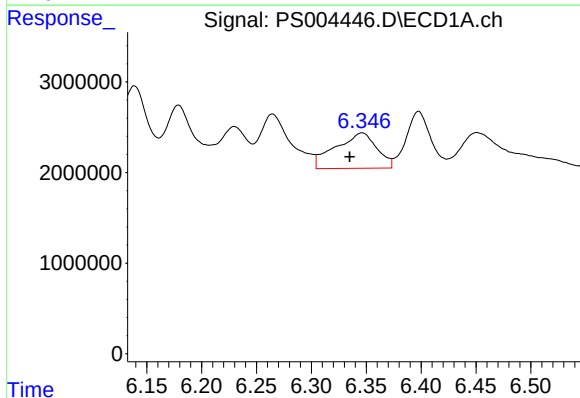


#6 MCP

R.T.: 6.346 min
Delta R.T.: 0.011 min
Response: 10233532
Conc: 5.92 ug/ml

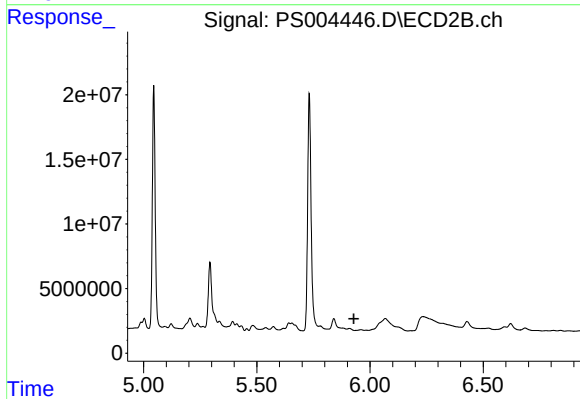

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

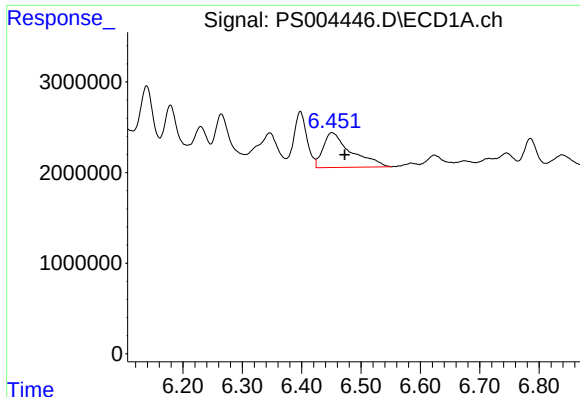

#7 MCPA


R.T.: 6.451 min
Delta R.T.: -0.021 min
Response: 12532508
Conc: 4.86 ug/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

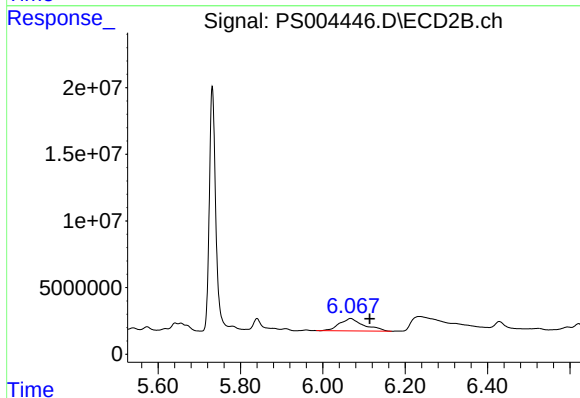


#7 MCPA

R.T.: 6.067 min
Delta R.T.: -0.046 min
Response: 38556689
Conc: 19.41 ug/ml

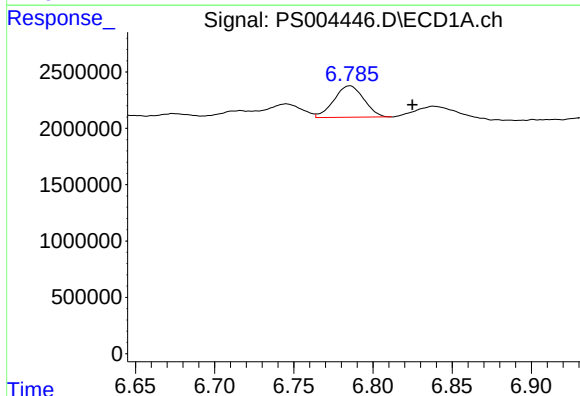


#8 DICHLORPROP

R.T.: 6.785 min
Delta R.T.: -0.040 min
Response: 3660988
Conc: 6.40 ng/ml

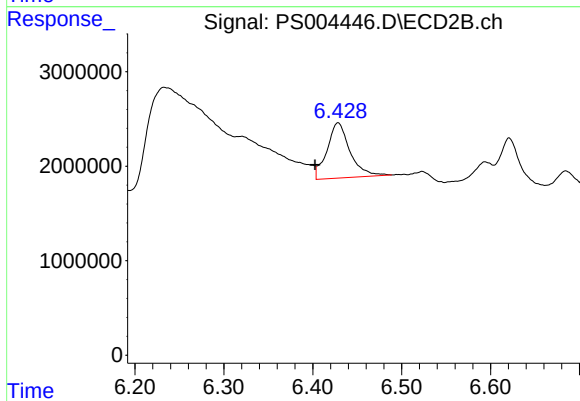

#8 DICHLORPROP


R.T.: 6.429 min
Delta R.T.: 0.026 min
Response: 10482138
Conc: 22.28 ng/ml

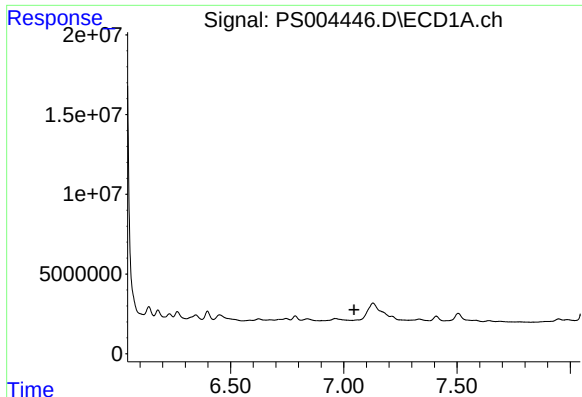

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.045 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

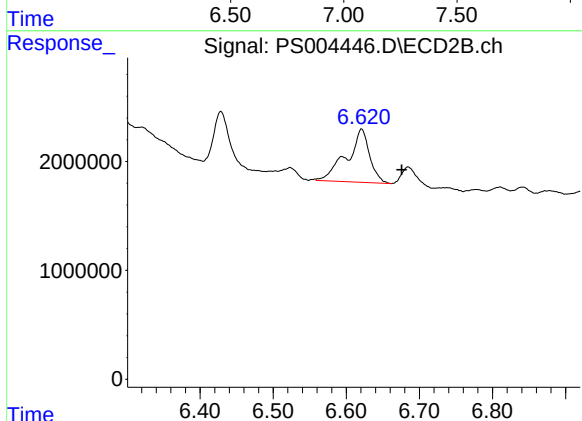


#9 2,4-D

R.T.: 6.621 min
Delta R.T.: -0.055 min
Response: 10585707
Conc: 20.13 ng/ml

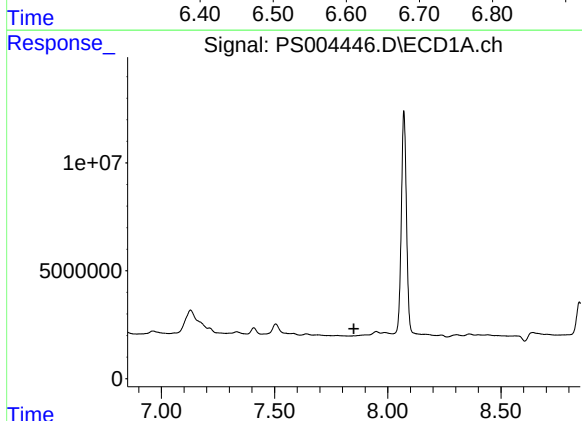


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.850 min
Response: 0
Conc: N.D.

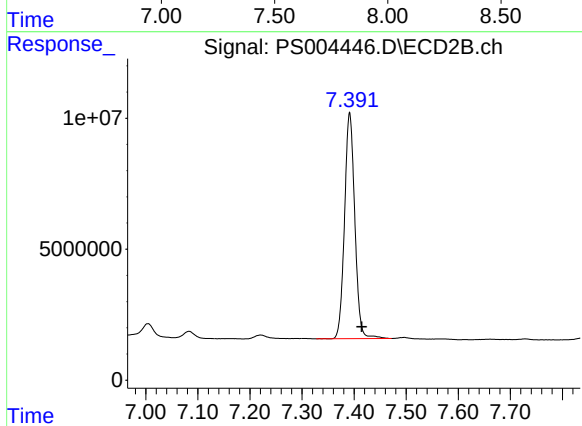

#11 2,4,5-TP (SILVEX)


R.T.: 7.392 min
Delta R.T.: -0.023 min
Response: 118193857
Conc: 44.98 ng/ml

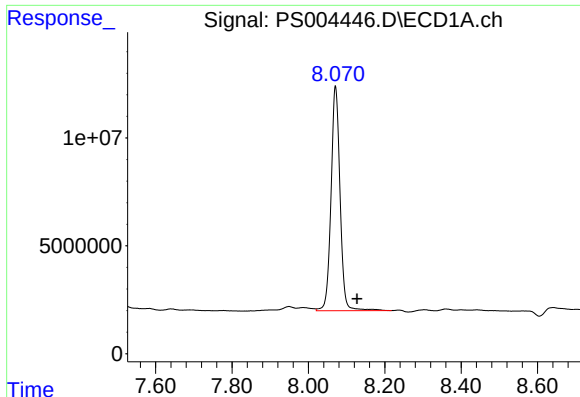

#12 2,4,5-T


R.T.: 8.071 min
Delta R.T.: -0.056 min
Response: 169942326
Conc: 49.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-A

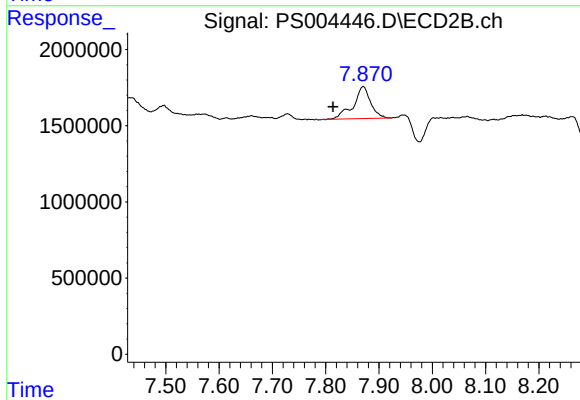


#12 2,4,5-T

R.T.: 7.870 min
Delta R.T.: 0.057 min
Response: 4733512
Conc: 2.10 ng/ml

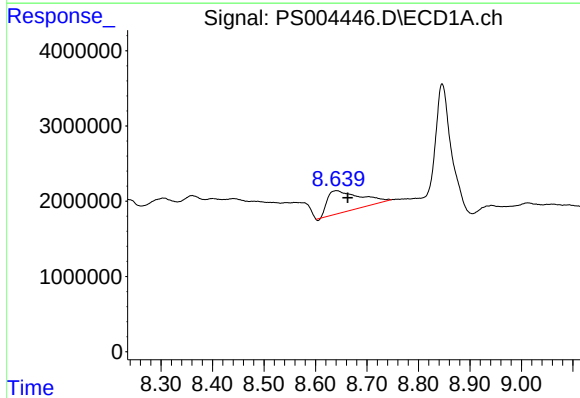

#13 2,4-DB

R.T.: 8.641 min
Delta R.T.: -0.022 min
Response: 12841598
Conc: 38.17 ng/ml

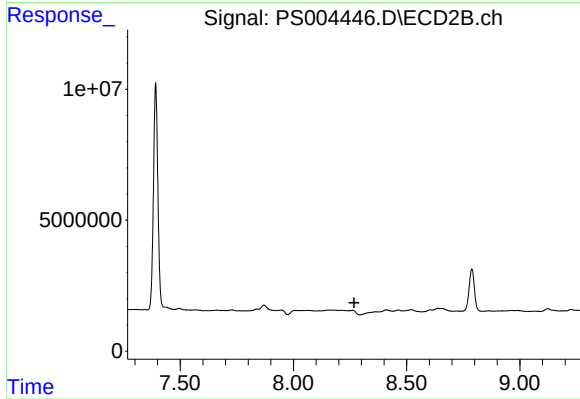

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.268 min
Response: 0
Conc: N.D.