

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
 Data File : PS004450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 13:05
 Operator : EI\SJ
 Sample : K2635-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-05-050219-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 04:46:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.021	5.716	294.1E6	211.4E6	467.304	438.411
Target Compounds							
1) T	Dalapon	2.387	2.054	64531094	184.6E6	82.123	275.868 #
2) T	3,5-DICHL...	5.334	4.987	7520532	8114647	9.520	13.200 #
3) T	4-Nitroph...	5.870	5.377	11220820	15501198	44.901	62.667 #
5) T	DICAMBA	6.160	5.824	11362197	11566212	4.778	6.179 #
6) T	MCPD	6.379	0.000	7698985	0	4.456	N.D. #
7) T	MCPA	0.000	6.053	0	36083446	N.D.	18.164
8) T	DICHLORPROP	0.000	6.412	0	6923922	N.D.	14.714
9) T	2,4-D	7.112	0.000	45773071	0	80.452	N.D. #
10) T	Pentachlo...	0.000	7.066	0	5307953	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	7.376	0	124.8E6	N.D.	47.494
15) T	Picloram	0.000	9.587	0	1002009	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
Data File : PS004450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 13:05
Operator : EI\SJ
Sample : K2635-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 04:46:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

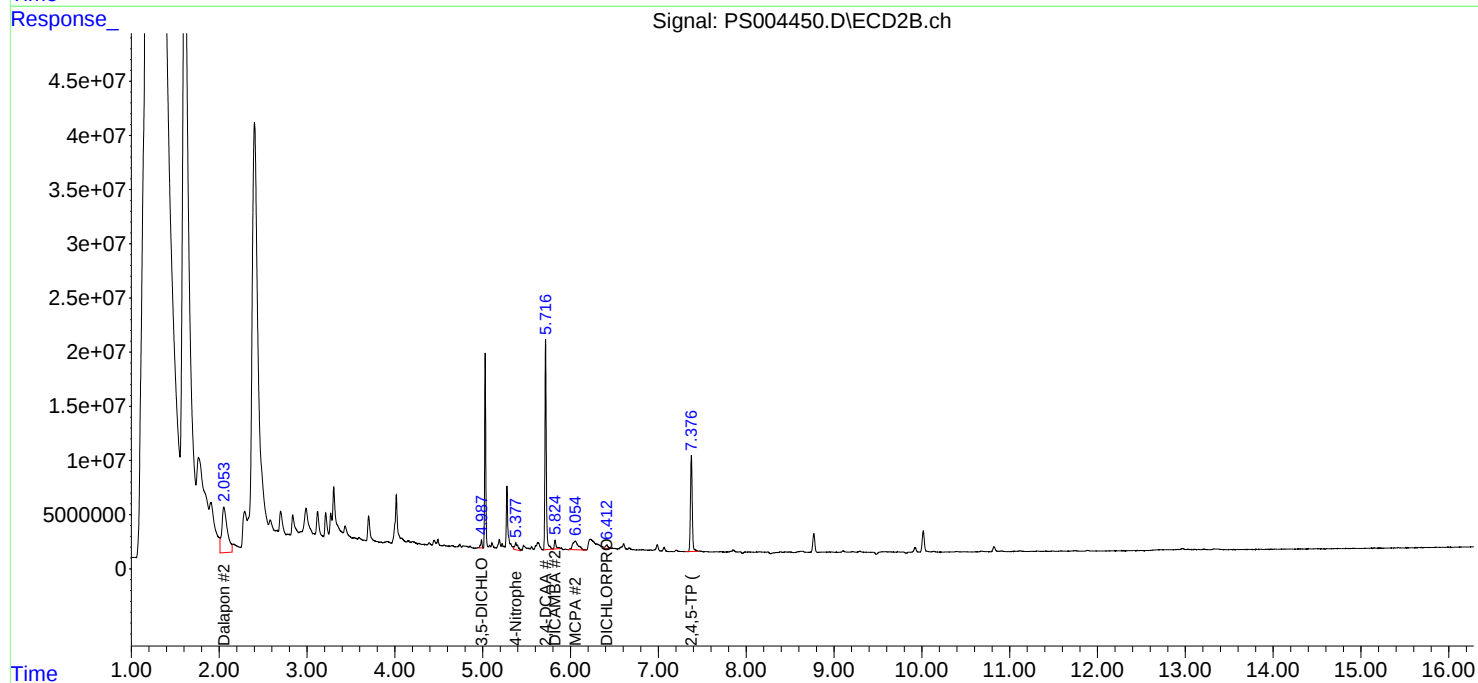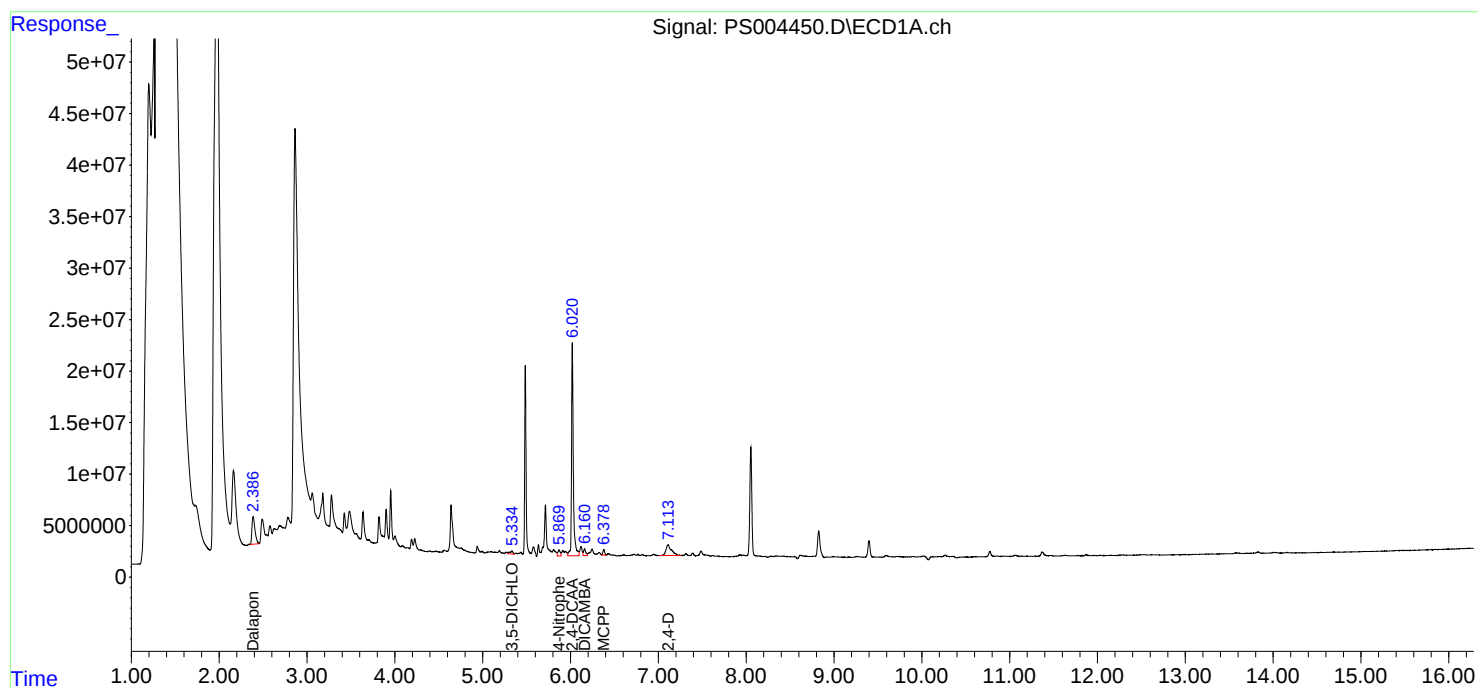


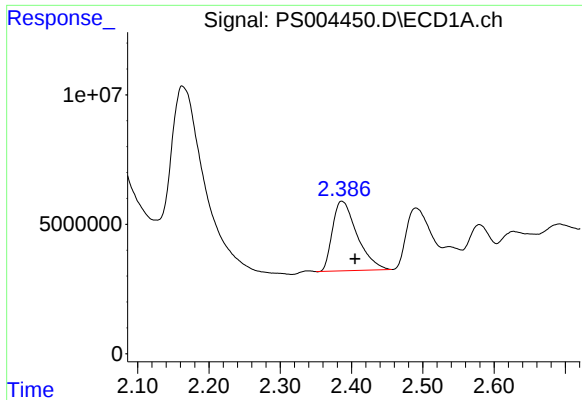

#1 Dalapon


R.T.: 2.387 min
Delta R.T.: -0.018 min
Response: 64531094
Conc: 82.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-C

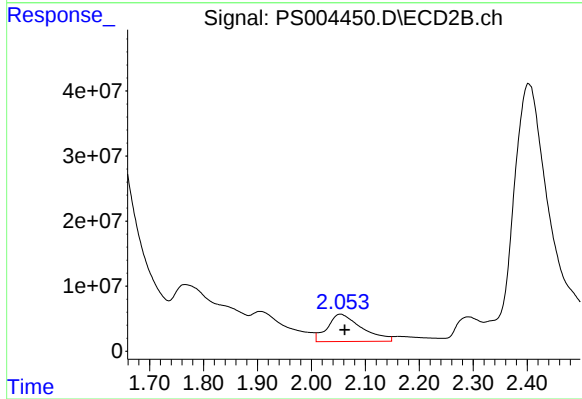


#1 Dalapon

R.T.: 2.054 min
Delta R.T.: -0.008 min
Response: 184607033
Conc: 275.87 ng/ml

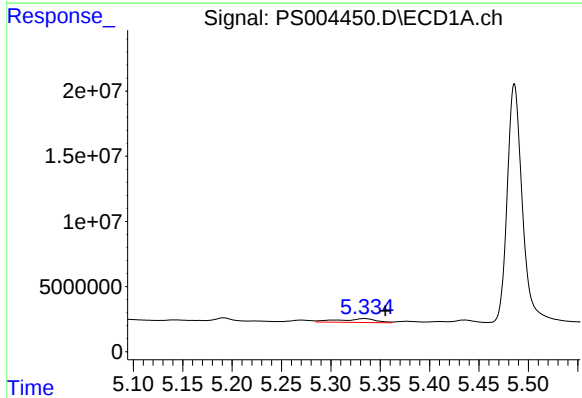


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.334 min
Delta R.T.: -0.021 min
Response: 7520532
Conc: 9.52 ng/ml

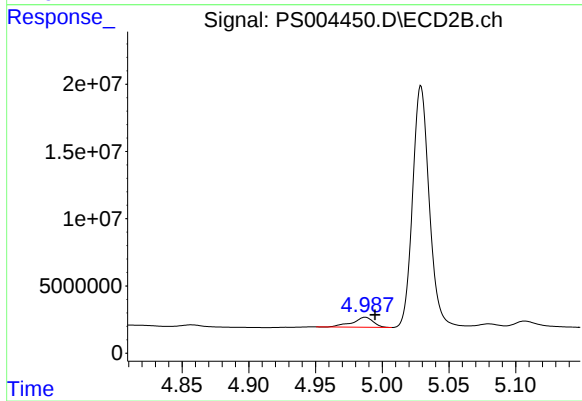

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.987 min
Delta R.T.: -0.007 min
Response: 8114647
Conc: 13.20 ng/ml

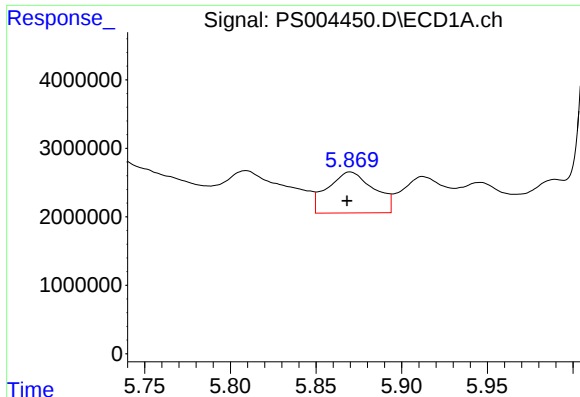

#3 4-Nitrophenol


R.T.: 5.870 min
Delta R.T.: 0.002 min
Response: 11220820
Conc: 44.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-C

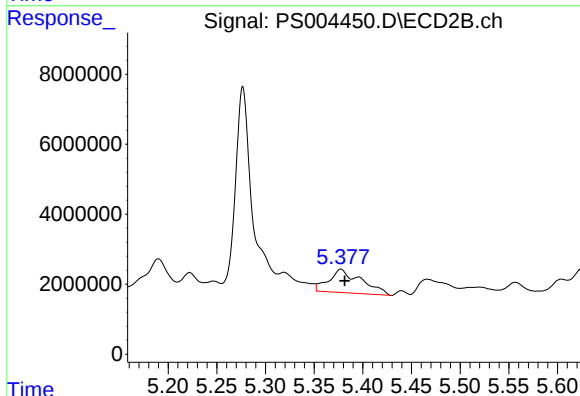


#3 4-Nitrophenol

R.T.: 5.377 min
Delta R.T.: -0.004 min
Response: 15501198
Conc: 62.67 ng/ml

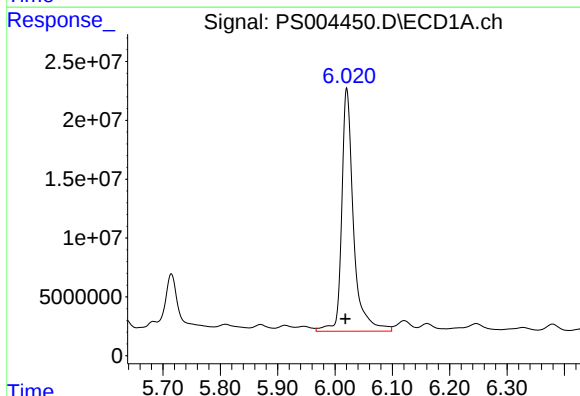


#4 2,4-DCAA

R.T.: 6.021 min
Delta R.T.: 0.003 min
Response: 294147454
Conc: 467.30 ng/ml

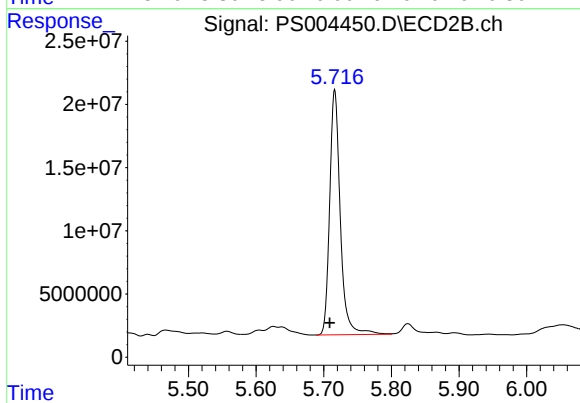

#4 2,4-DCAA


R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 211438227
Conc: 438.41 ng/ml

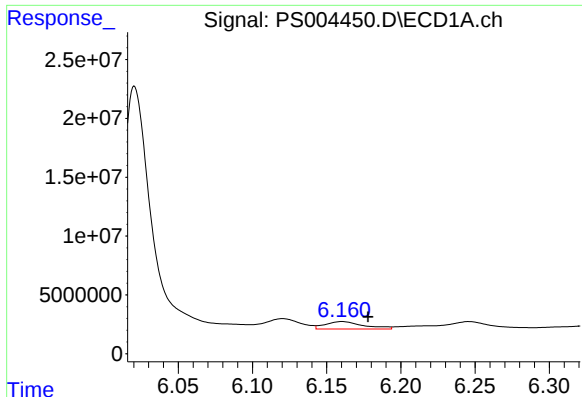

#5 DICAMBA


R.T.: 6.160 min
Delta R.T.: -0.017 min
Response: 11362197
Conc: 4.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-C

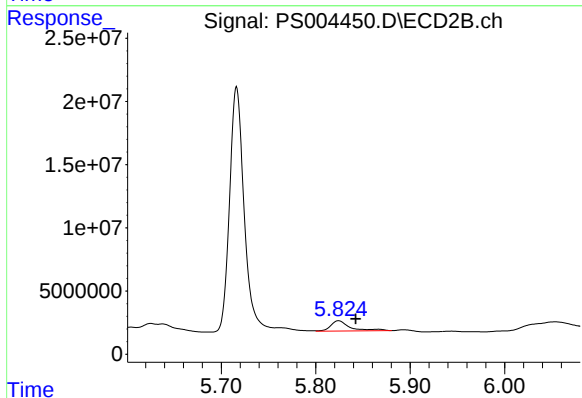


#5 DICAMBA

R.T.: 5.824 min
Delta R.T.: -0.018 min
Response: 11566212
Conc: 6.18 ng/ml

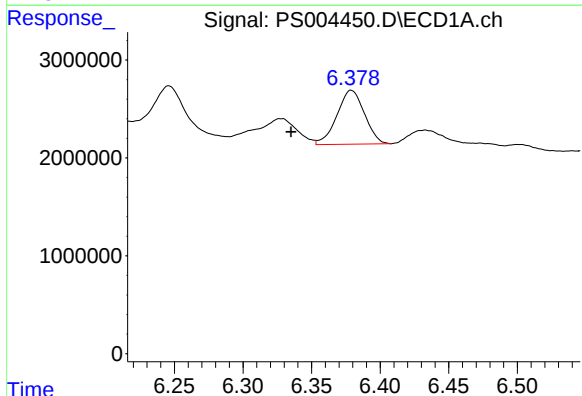


#6 MCP

R.T.: 6.379 min
Delta R.T.: 0.044 min
Response: 7698985
Conc: 4.46 ug/ml

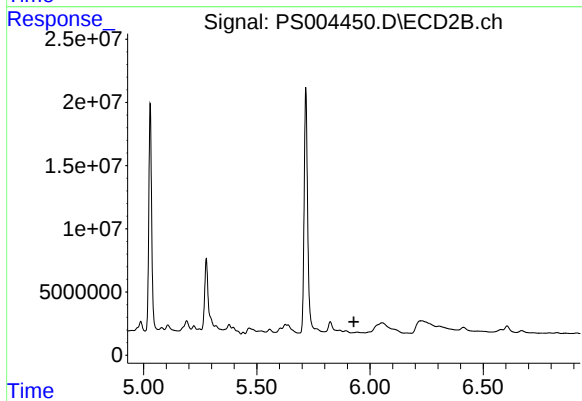

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

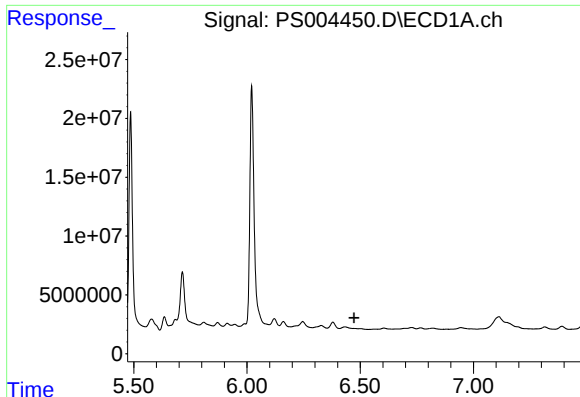

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-C

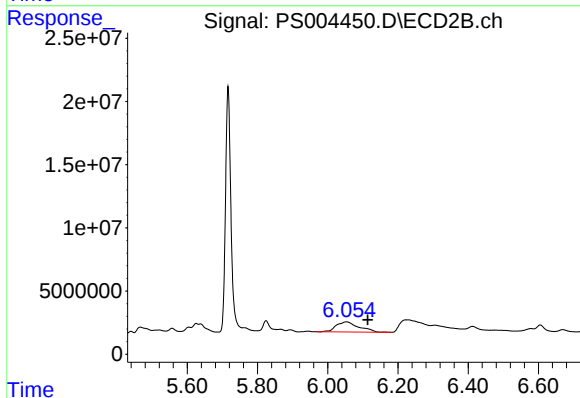


#7 MCPA

R.T.: 6.053 min
Delta R.T.: -0.061 min
Response: 36083446
Conc: 18.16 ug/ml

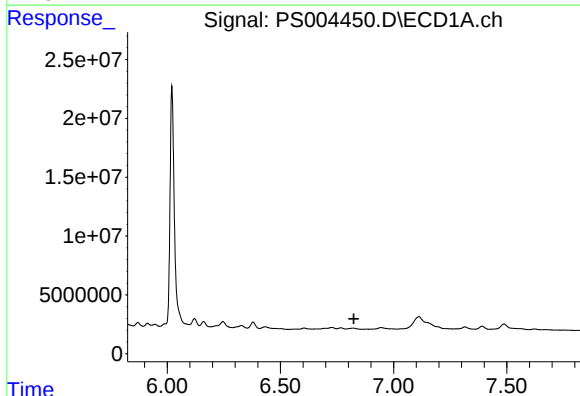


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

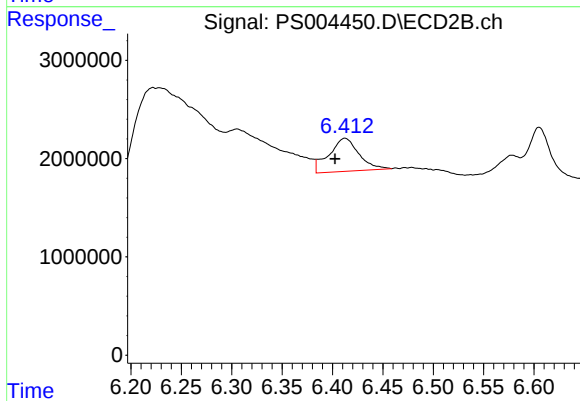

#8 DICHLORPROP


R.T.: 6.412 min
Delta R.T.: 0.010 min
Response: 6923922
Conc: 14.71 ng/ml

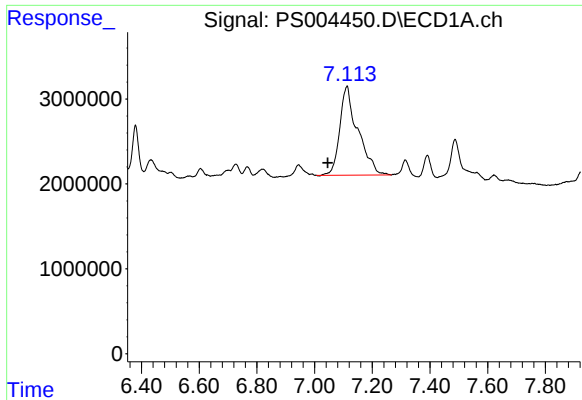

#9 2,4-D


R.T.: 7.112 min
Delta R.T.: 0.067 min
Response: 45773071
Conc: 80.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-050219-C

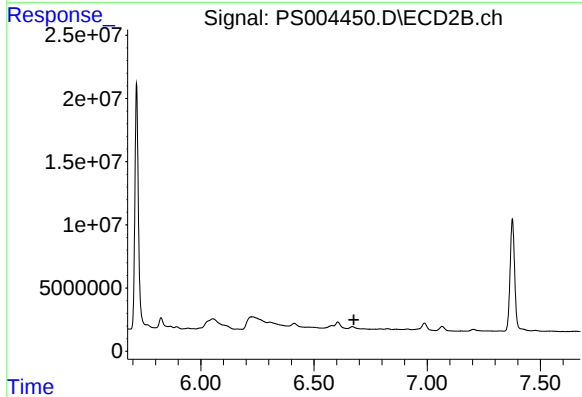


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

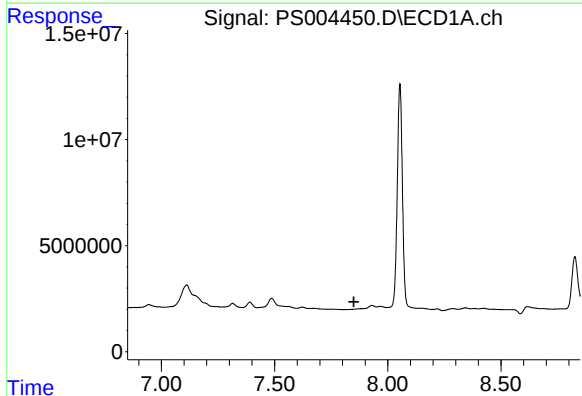

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

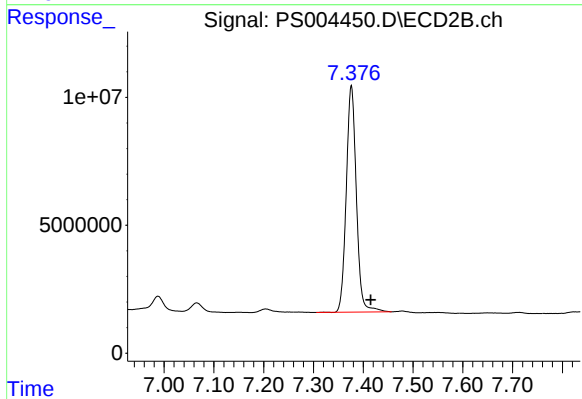

#11 2,4,5-TP (SILVEX)

R.T.: 7.376 min
Delta R.T.: -0.039 min
Response: 124786997
Conc: 47.49 ng/ml