

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
 Data File : PS004458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 17:13
 Operator : EI\SJ
 Sample : K2668-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 04:48:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.016	5.711	253.6E6	197.4E6	402.904	409.298
Target Compounds							
1) T	Dalapon	2.383	2.047	53185324	136.1E6	67.684	203.360 #
2) T	3,5-DICHL...	5.373	4.982	6798779	6937197	8.606	11.285 #
3) T	4-Nitroph...	5.865	5.372	8540474	16844683	34.176	68.098 #
5) T	DICAMBA	6.155	5.863	6805561	9542179	2.862	5.098 #
6) T	MCPD	6.374	5.863	5739293	9542179	3.322	7.095 #
7) T	MCPA	0.000	6.048	0	42387523	N.D.	21.338
8) T	DICHLORPROP	0.000	6.408	0	7394355	N.D.	15.713
9) T	2,4-D	7.102	0.000	50054090	0	87.977	N.D. #
10) T	Pentachlo...	0.000	6.982	0	8152451	N.D.	1.222
11) T	2,4,5-TP ...	0.000	7.370	0	110.7E6	N.D.	42.143



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
Data File : PS004458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 17:13
Operator : EI\SJ
Sample : K2668-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 04:48:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

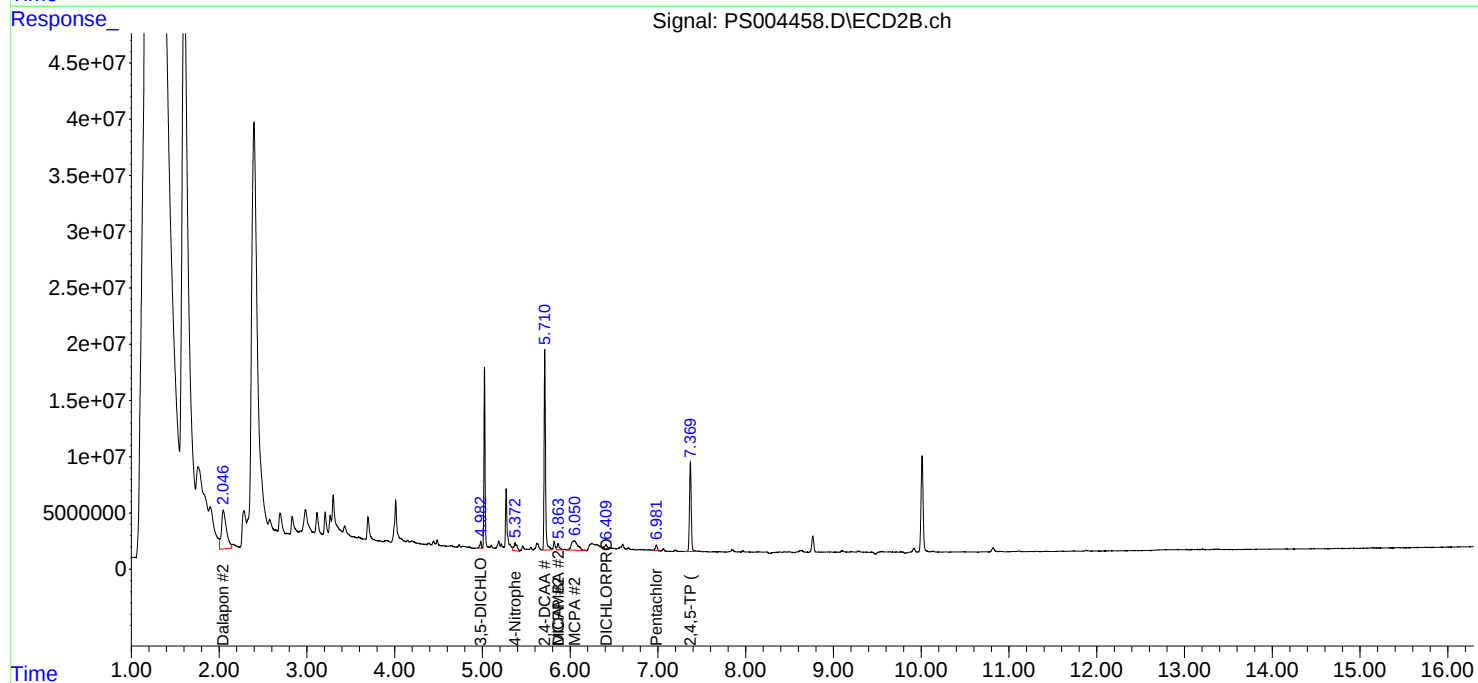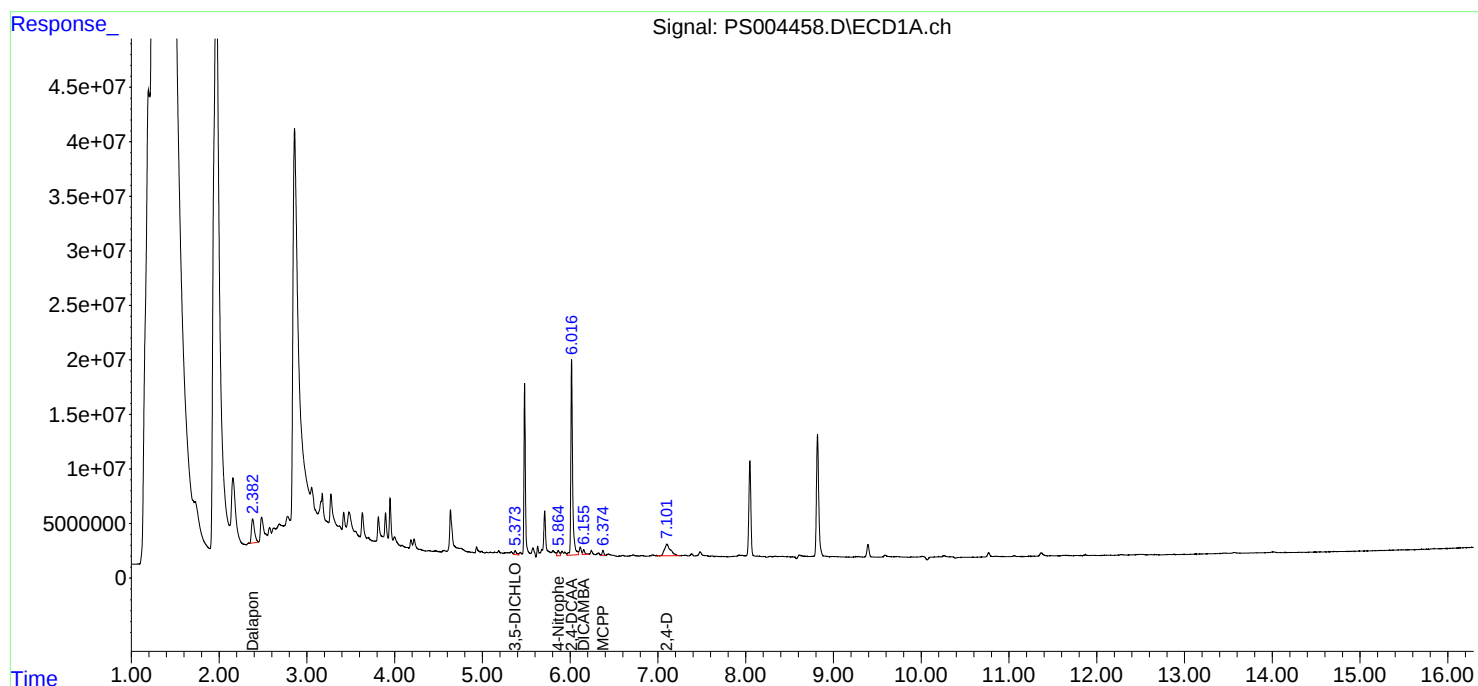


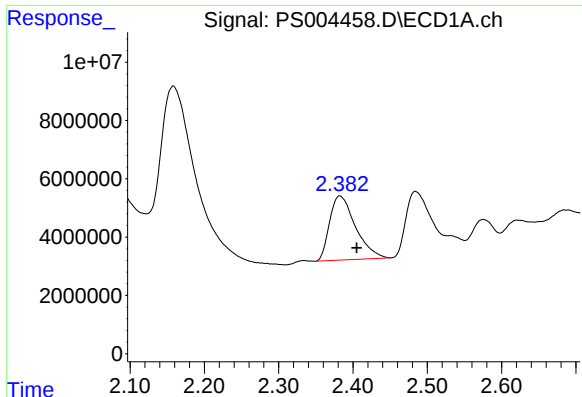

#1 Dalapon


R.T.: 2.383 min
Delta R.T.: -0.022 min
Response: 53185324
Conc: 67.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

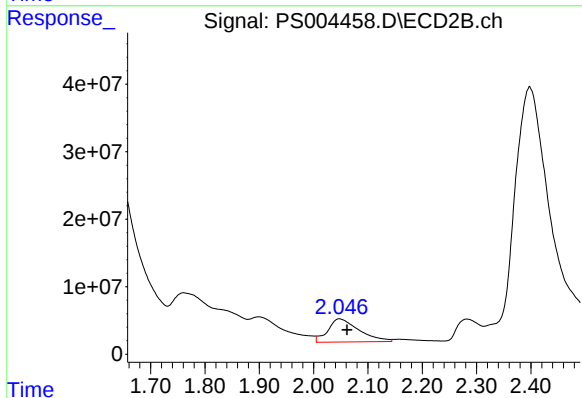


#1 Dalapon

R.T.: 2.047 min
Delta R.T.: -0.014 min
Response: 136085791
Conc: 203.36 ng/ml

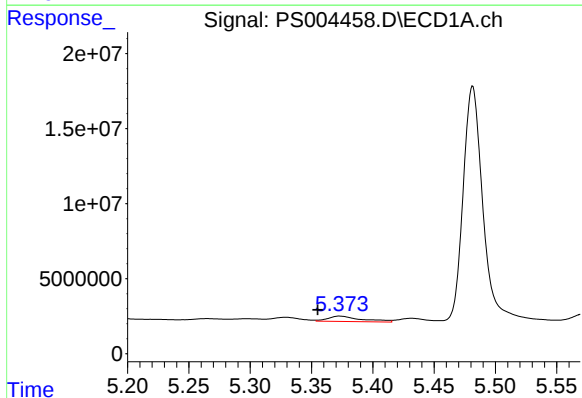


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.373 min
Delta R.T.: 0.018 min
Response: 6798779
Conc: 8.61 ng/ml

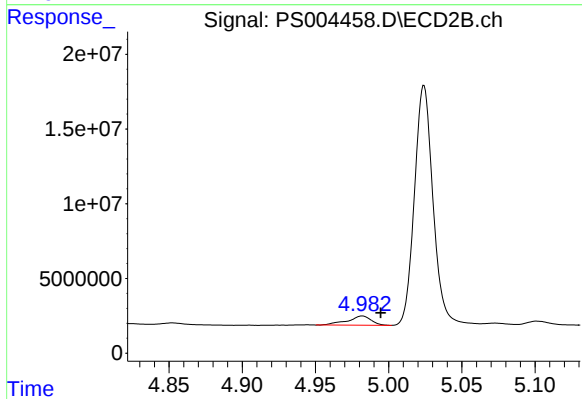

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.982 min
Delta R.T.: -0.013 min
Response: 6937197
Conc: 11.28 ng/ml

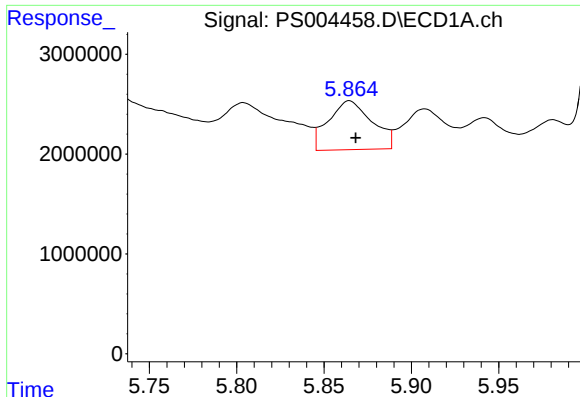

#3 4-Nitrophenol


R.T.: 5.865 min
Delta R.T.: -0.003 min
Response: 8540474
Conc: 34.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

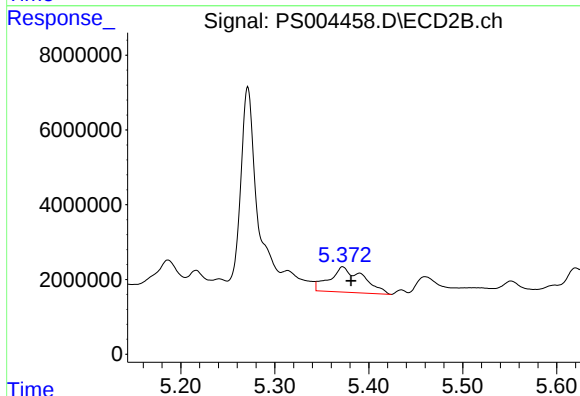


#3 4-Nitrophenol

R.T.: 5.372 min
Delta R.T.: -0.009 min
Response: 16844683
Conc: 68.10 ng/ml

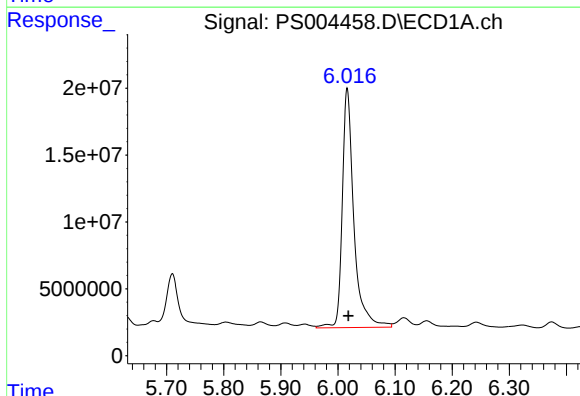


#4 2,4-DCAA

R.T.: 6.016 min
Delta R.T.: -0.002 min
Response: 253610969
Conc: 402.90 ng/ml

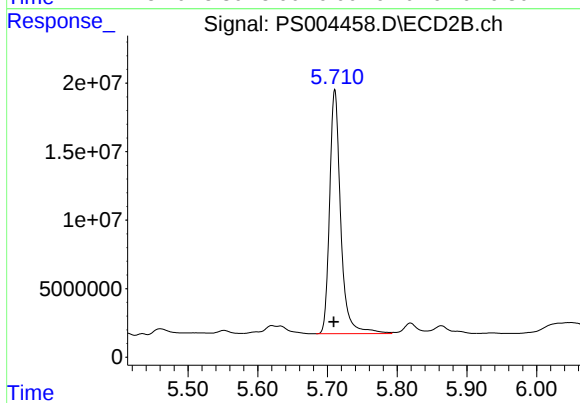

#4 2,4-DCAA


R.T.: 5.711 min
Delta R.T.: 0.002 min
Response: 197397513
Conc: 409.30 ng/ml

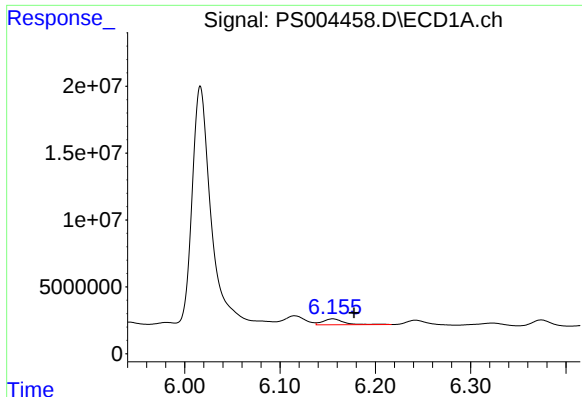

#5 DICAMBA


R.T.: 6.155 min
Delta R.T.: -0.023 min
Response: 6805561
Conc: 2.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

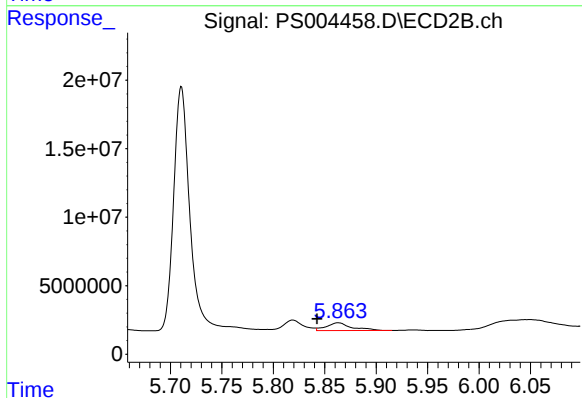


#5 DICAMBA

R.T.: 5.863 min
Delta R.T.: 0.021 min
Response: 9542179
Conc: 5.10 ng/ml

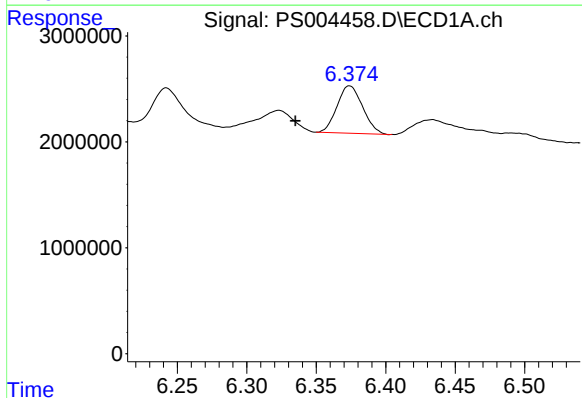


#6 MCP

R.T.: 6.374 min
Delta R.T.: 0.039 min
Response: 5739293
Conc: 3.32 ug/ml

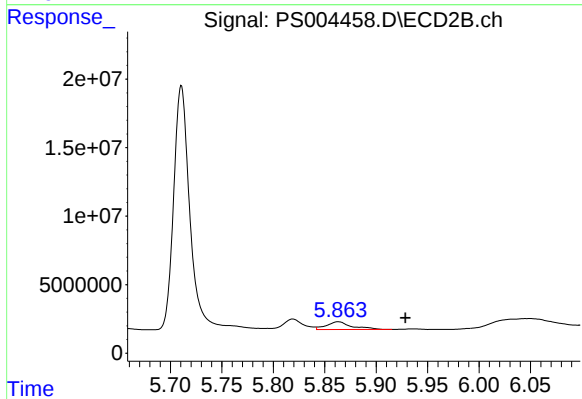

#6 MCP


R.T.: 5.863 min
Delta R.T.: -0.066 min
Response: 9542179
Conc: 7.10 ug/ml

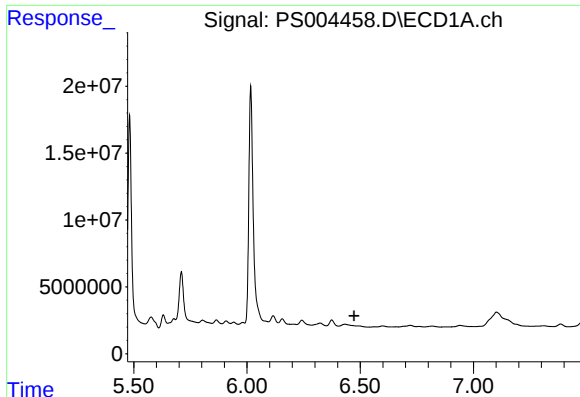

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

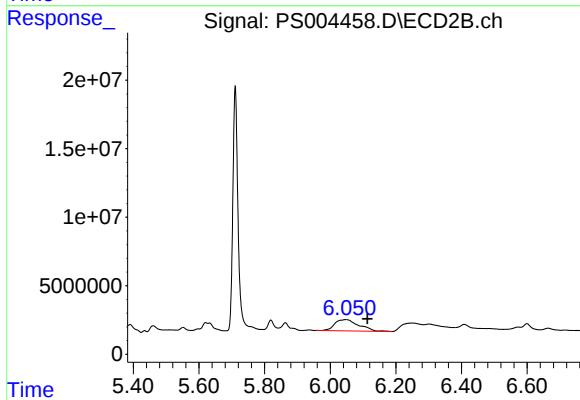


#7 MCPA

R.T.: 6.048 min
Delta R.T.: -0.066 min
Response: 42387523
Conc: 21.34 ug/ml

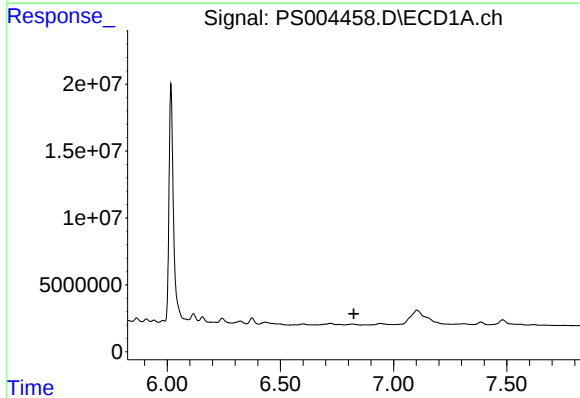


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

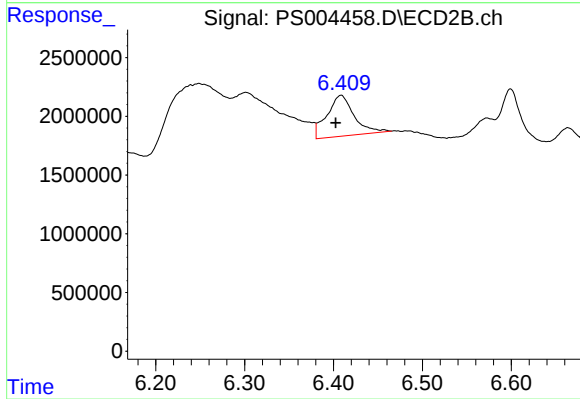

#8 DICHLORPROP


R.T.: 6.408 min
Delta R.T.: 0.006 min
Response: 7394355
Conc: 15.71 ng/ml

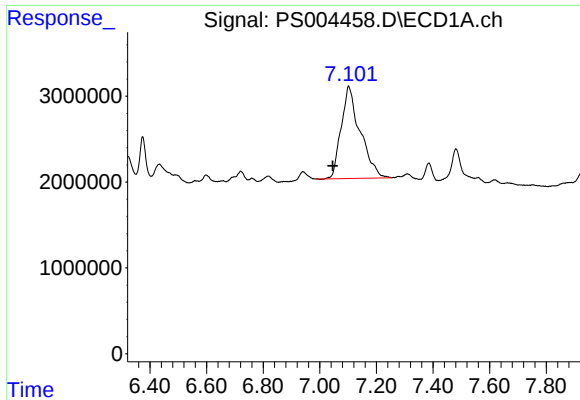

#9 2,4-D


R.T.: 7.102 min
Delta R.T.: 0.057 min
Response: 50054090
Conc: 87.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

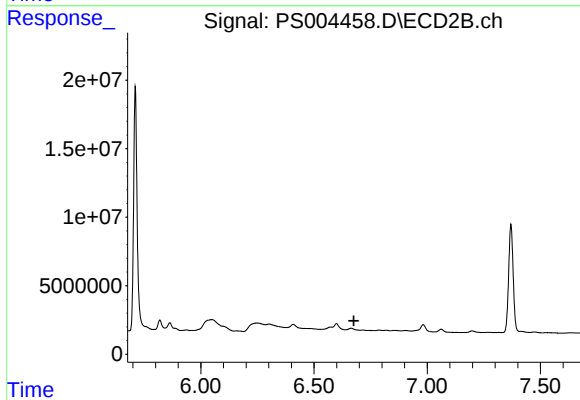


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

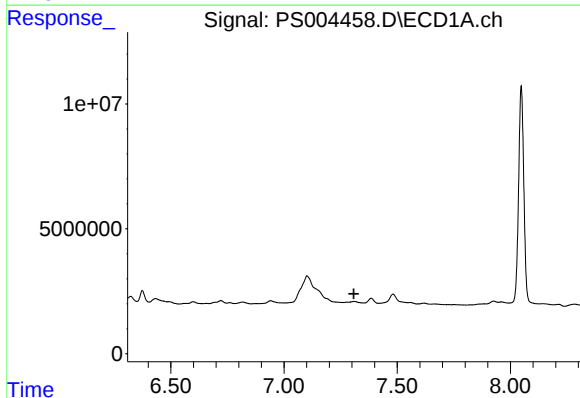


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.309 min
Response: 0
Conc: N.D.

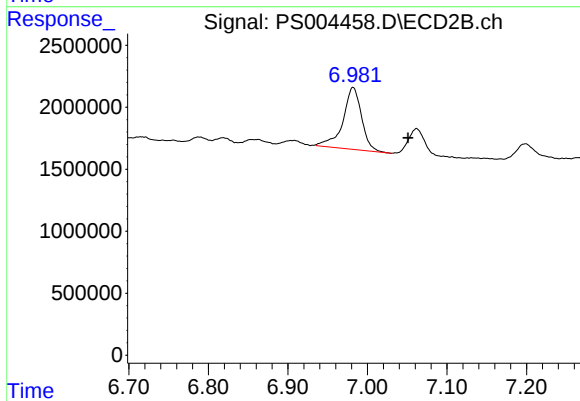

#10 Pentachlorophenol


R.T.: 6.982 min
Delta R.T.: -0.069 min
Response: 8152451
Conc: 1.22 ng/ml

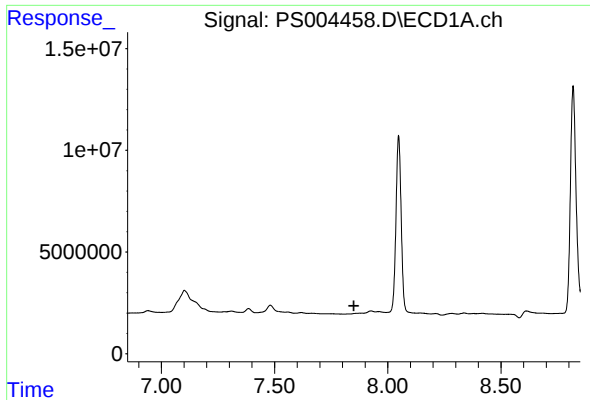

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.850 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

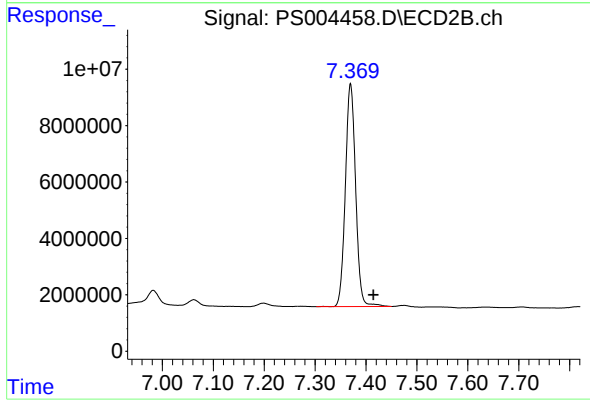

#11 2,4,5-TP (SILVEX)

R.T.: 7.370 min
Delta R.T.: -0.045 min
Response: 110728133
Conc: 42.14 ng/ml