

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
 Data File : PS004459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 17:43
 Operator : EI\SJ
 Sample : K2674-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FILTERBAG-RO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 04:49:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.998	5.692	276.7E6	206.5E6	439.508	428.135
Target Compounds							
1) T	Dalapon	2.464	2.027	17115215	150.5E6	21.781	224.919 #
2) T	3,5-DICHL...	5.355	5.005	6433459	166.7E6	8.144	271.171 #
3) T	4-Nitroph...	5.890	5.354	8773995	18471279	35.110	74.674 #
5) T	DICAMBA	6.138	5.845	11285800	9108191	4.746	4.866
6) T	MCP	6.357	0.000	7584579	0	4.390	N.D. #
8) T	DICHLORPROP	0.000	6.391	0	6891634	N.D.	14.645
9) T	2,4-D	7.082	0.000	50592004	0	88.922	N.D. #
11) T	2,4,5-TP ...	0.000	7.352	0	132.9E6	N.D.	50.590



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
Data File : PS004459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 17:43
Operator : EI\SJ
Sample : K2674-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 04:49:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

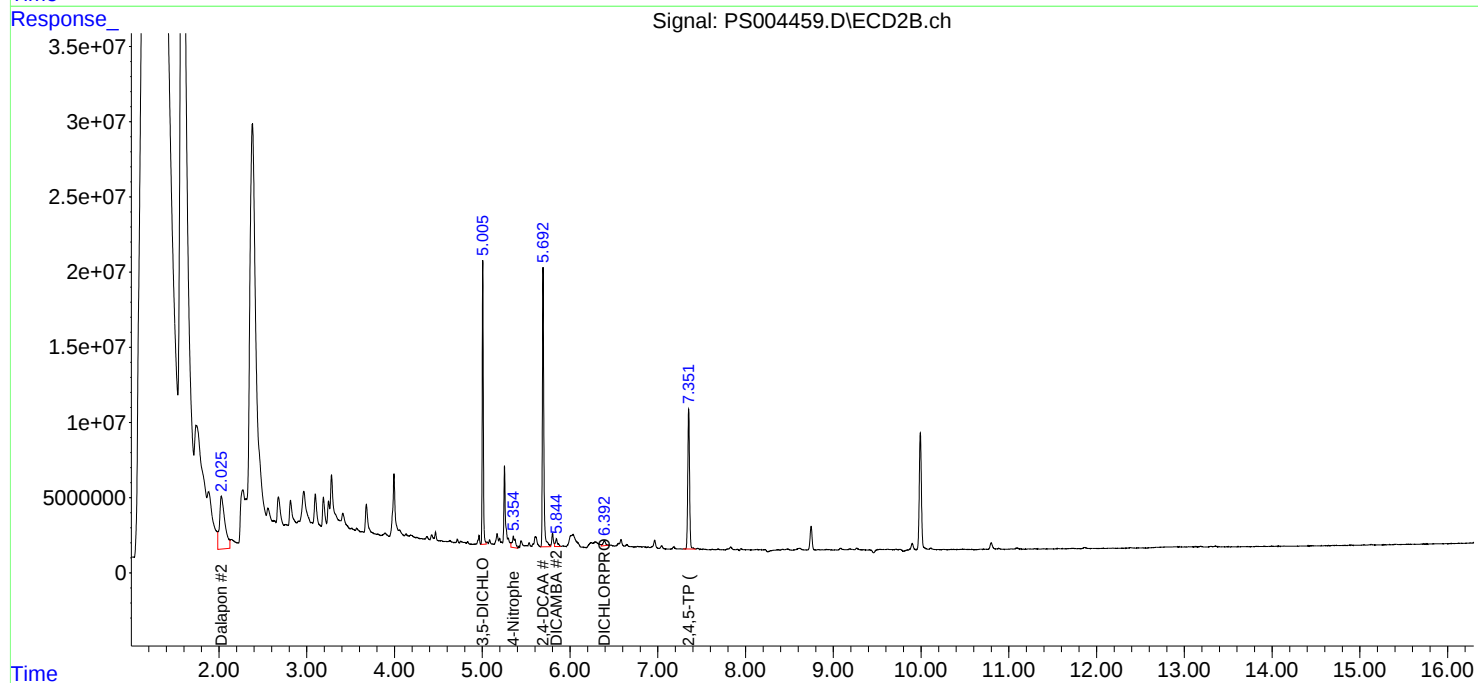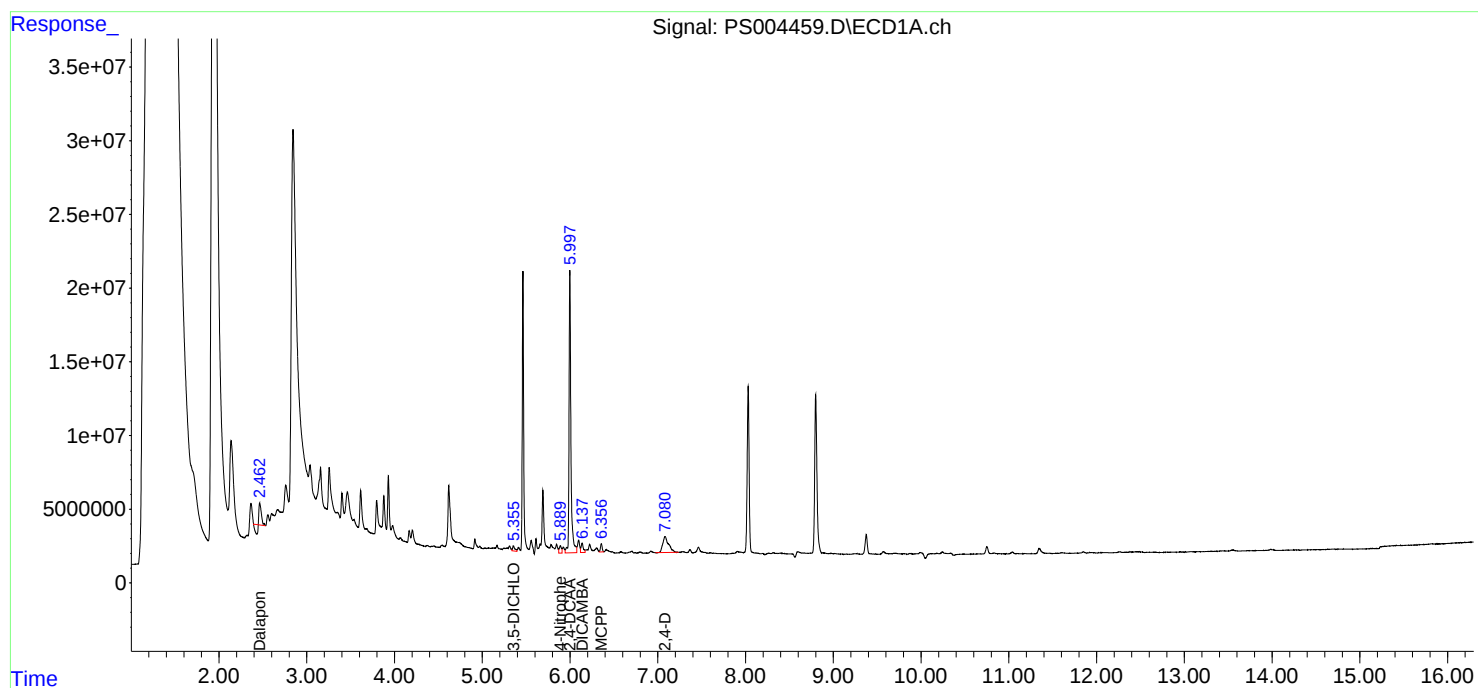


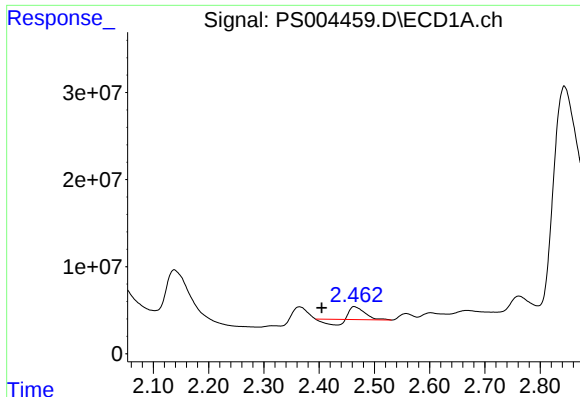

#1 Dalapon


R.T.: 2.464 min
Delta R.T.: 0.059 min
Response: 17115215
Conc: 21.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

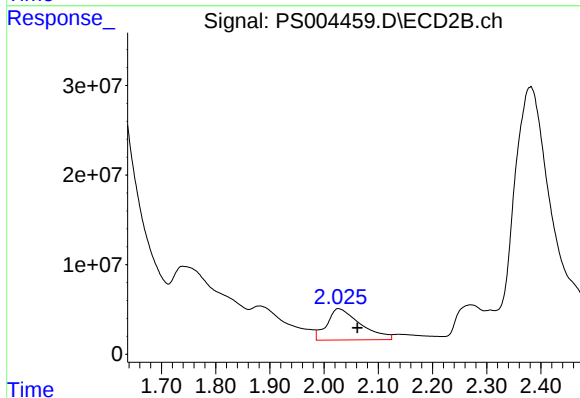


#1 Dalapon

R.T.: 2.027 min
Delta R.T.: -0.035 min
Response: 150512784
Conc: 224.92 ng/ml

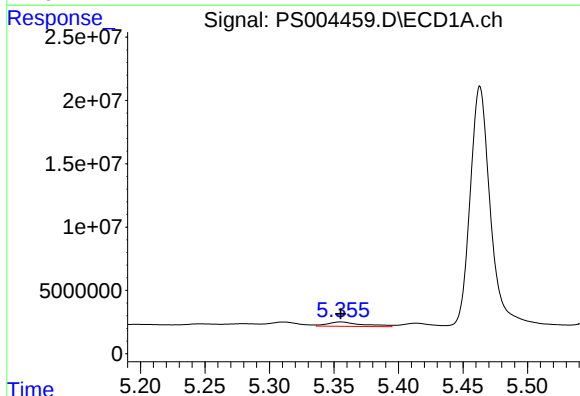


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 6433459
Conc: 8.14 ng/ml

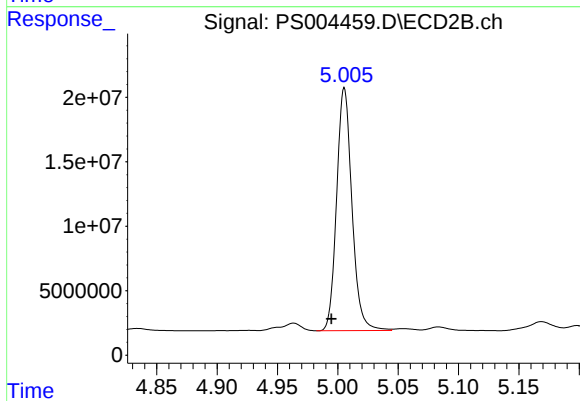

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.005 min
Delta R.T.: 0.011 min
Response: 166697083
Conc: 271.17 ng/ml

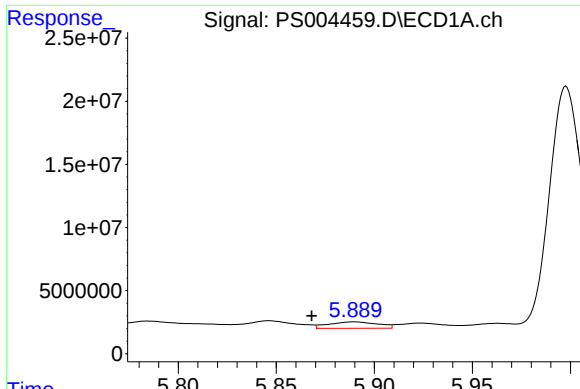

#3 4-Nitrophenol


R.T.: 5.890 min
Delta R.T.: 0.021 min
Response: 8773995
Conc: 35.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

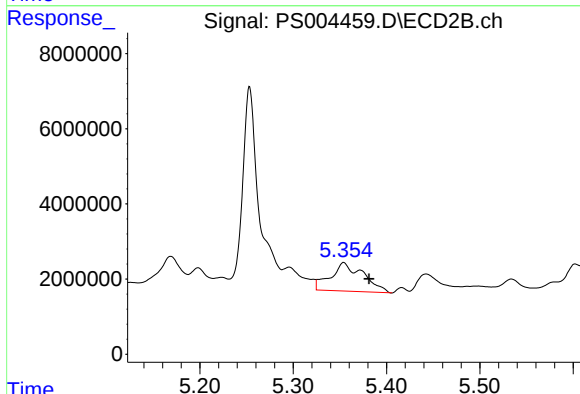


#3 4-Nitrophenol

R.T.: 5.354 min
Delta R.T.: -0.027 min
Response: 18471279
Conc: 74.67 ng/ml

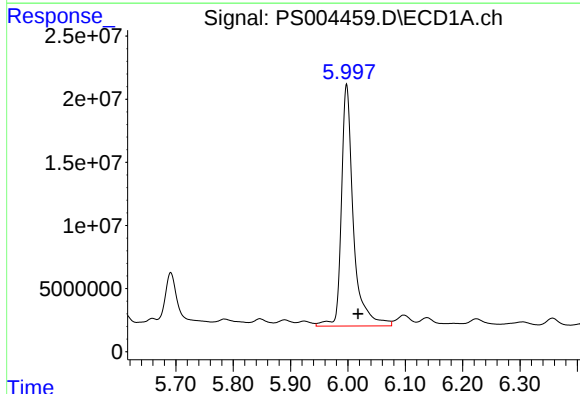


#4 2,4-DCAA

R.T.: 5.998 min
Delta R.T.: -0.020 min
Response: 276651591
Conc: 439.51 ng/ml

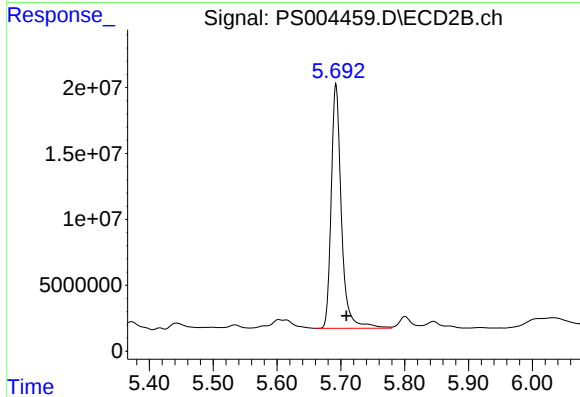

#4 2,4-DCAA


R.T.: 5.692 min
Delta R.T.: -0.016 min
Response: 206482268
Conc: 428.13 ng/ml

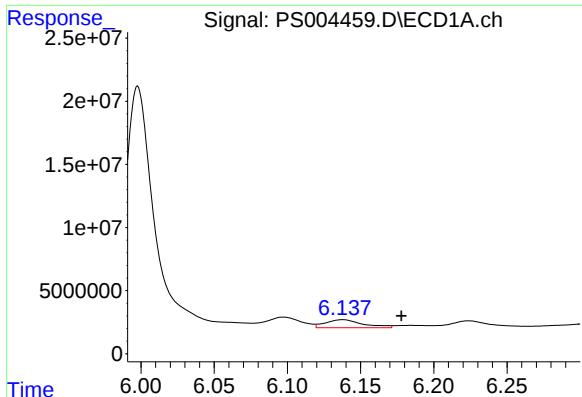

#5 DICAMBA


R.T.: 6.138 min
Delta R.T.: -0.040 min
Response: 11285800
Conc: 4.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

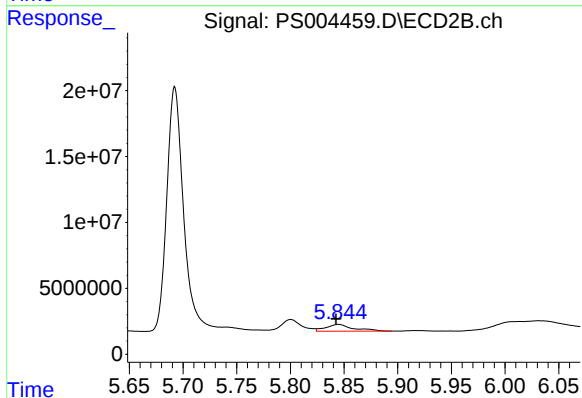


#5 DICAMBA

R.T.: 5.845 min
Delta R.T.: 0.002 min
Response: 9108191
Conc: 4.87 ng/ml

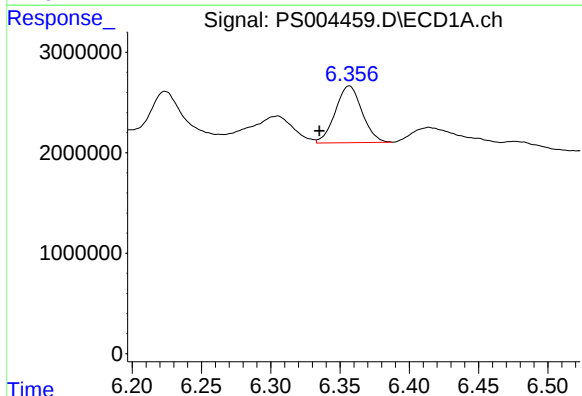


#6 MCP

R.T.: 6.357 min
Delta R.T.: 0.022 min
Response: 7584579
Conc: 4.39 ug/ml

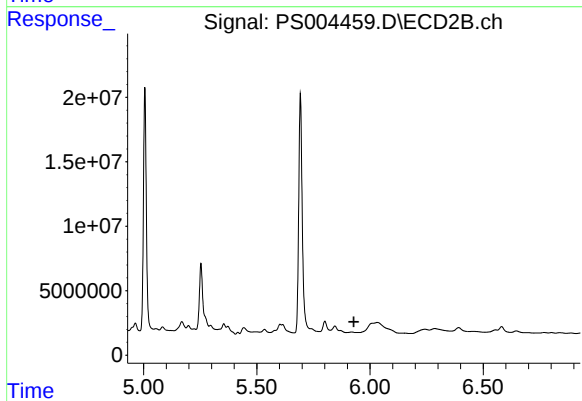

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

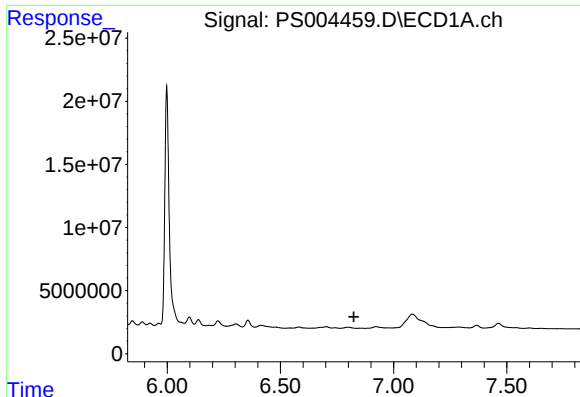

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

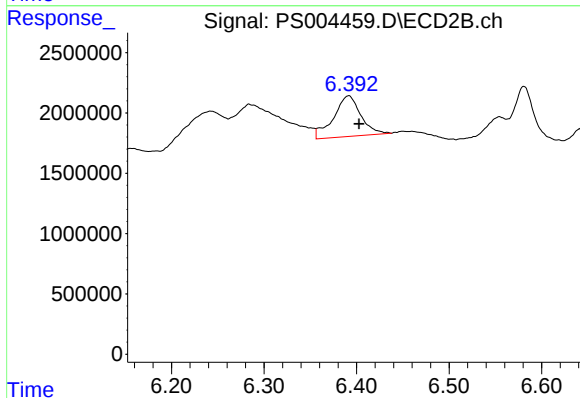


#8 DICHLORPROP

R.T.: 6.391 min
Delta R.T.: -0.011 min
Response: 6891634
Conc: 14.65 ng/ml

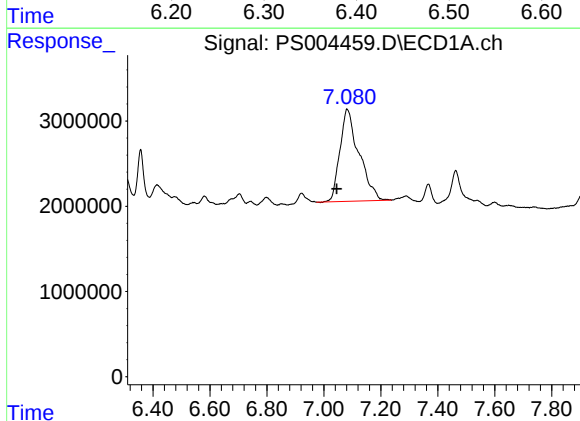


#9 2,4-D

R.T.: 7.082 min
Delta R.T.: 0.037 min
Response: 50592004
Conc: 88.92 ng/ml

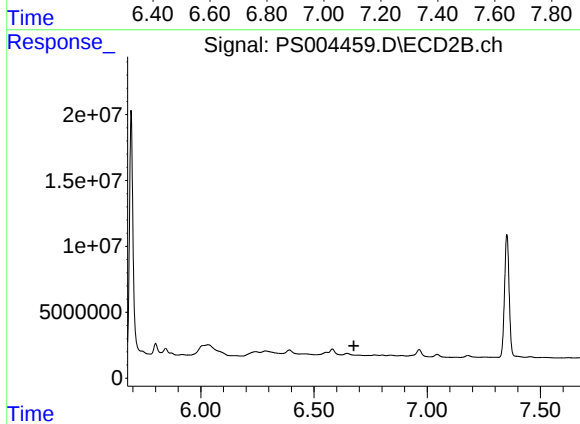

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.676 min
Response: 0
Conc: N.D.

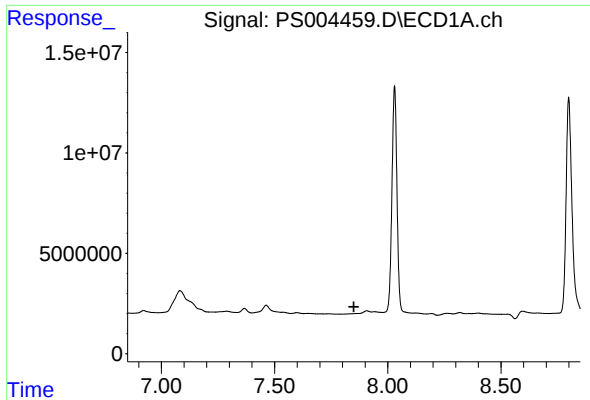

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min

Exp R.T.: 7.850 min

Response: 0

Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

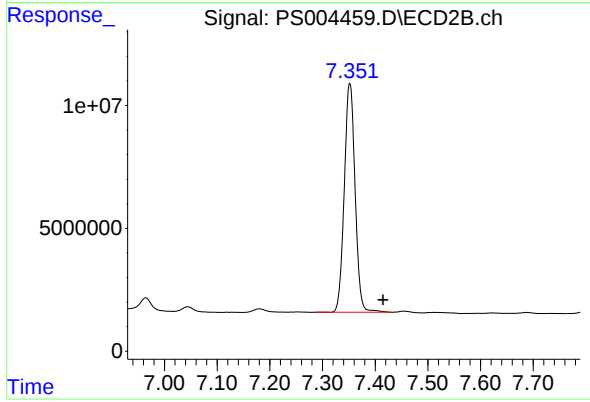

#11 2,4,5-TP (SILVEX)

R.T.: 7.352 min

Delta R.T.: -0.063 min

Response: 132923717

Conc: 50.59 ng/ml