

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
 Data File : PS004460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 18:13
 Operator : EI\SJ
 Sample : K2674-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FILTERBAG-RO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 04:49:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.014	5.708	292.5E6	214.8E6	464.706	445.421
Target Compounds							
1) T	Dalapon	2.383	2.046	55786798	162.8E6	70.995	243.341 #
2) T	3,5-DICHL...	5.372	4.980	6419483	7560669	8.126	12.299 #
3) T	4-Nitroph...	5.862	5.370	11227344	17708862	44.927	71.592 #
5) T	DICAMBA	6.153	5.860	11322026	9127753	4.761	4.877
6) T	MCPD	6.372	5.860	6871982	9127753	3.977	6.787 #
7) T	MCPA	0.000	6.047	0	41812200	N.D.	21.048
8) T	DICHLORPROP	0.000	6.406	0	7315175	N.D.	15.545
9) T	2,4-D	7.101	0.000	50928691	0	89.514	N.D. #
11) T	2,4,5-TP ...	0.000	7.367	0	117.9E6	N.D.	44.869
12) T	2,4,5-T	0.000	7.846	0	4830764	N.D.	2.148
15) T	Picloram	9.588	0.000	5646221	0	1.334	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050619\
Data File : PS004460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 18:13
Operator : EI\SJ
Sample : K2674-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 04:49:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

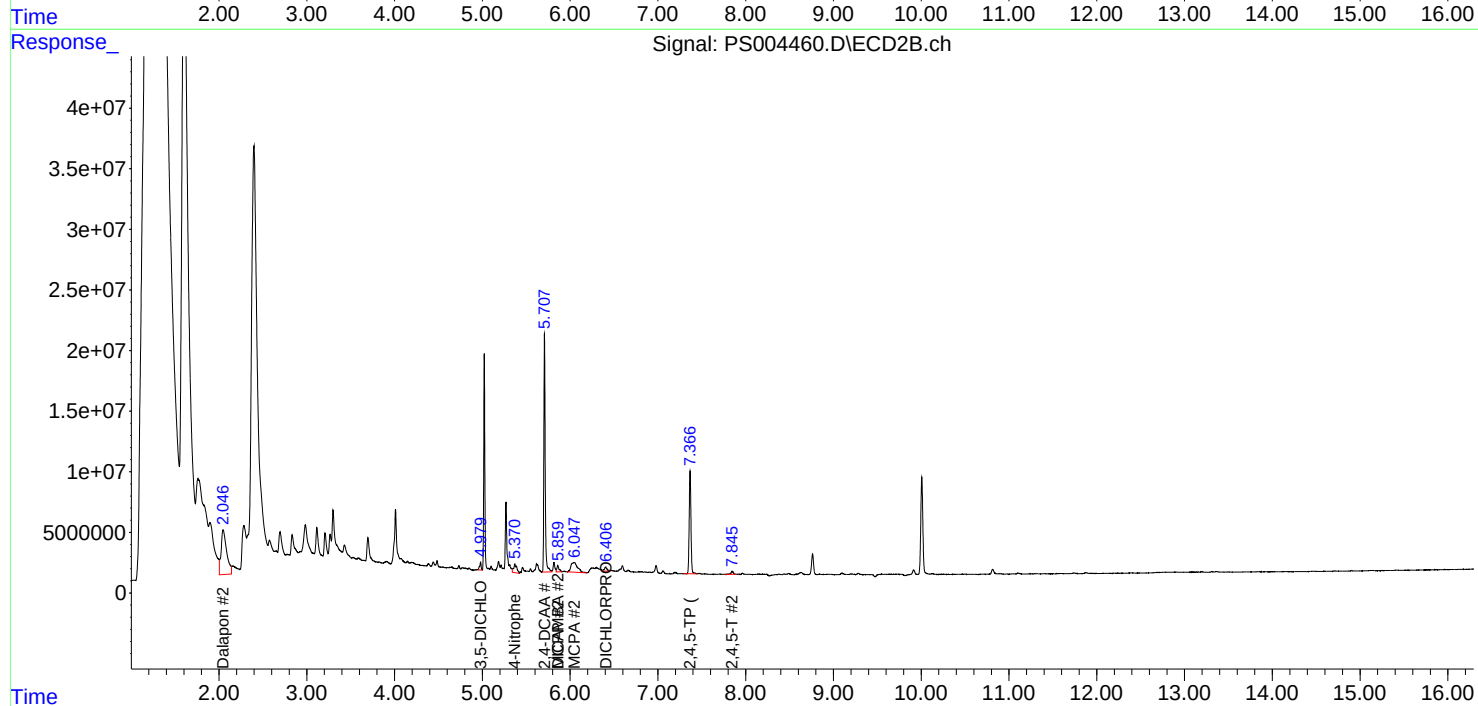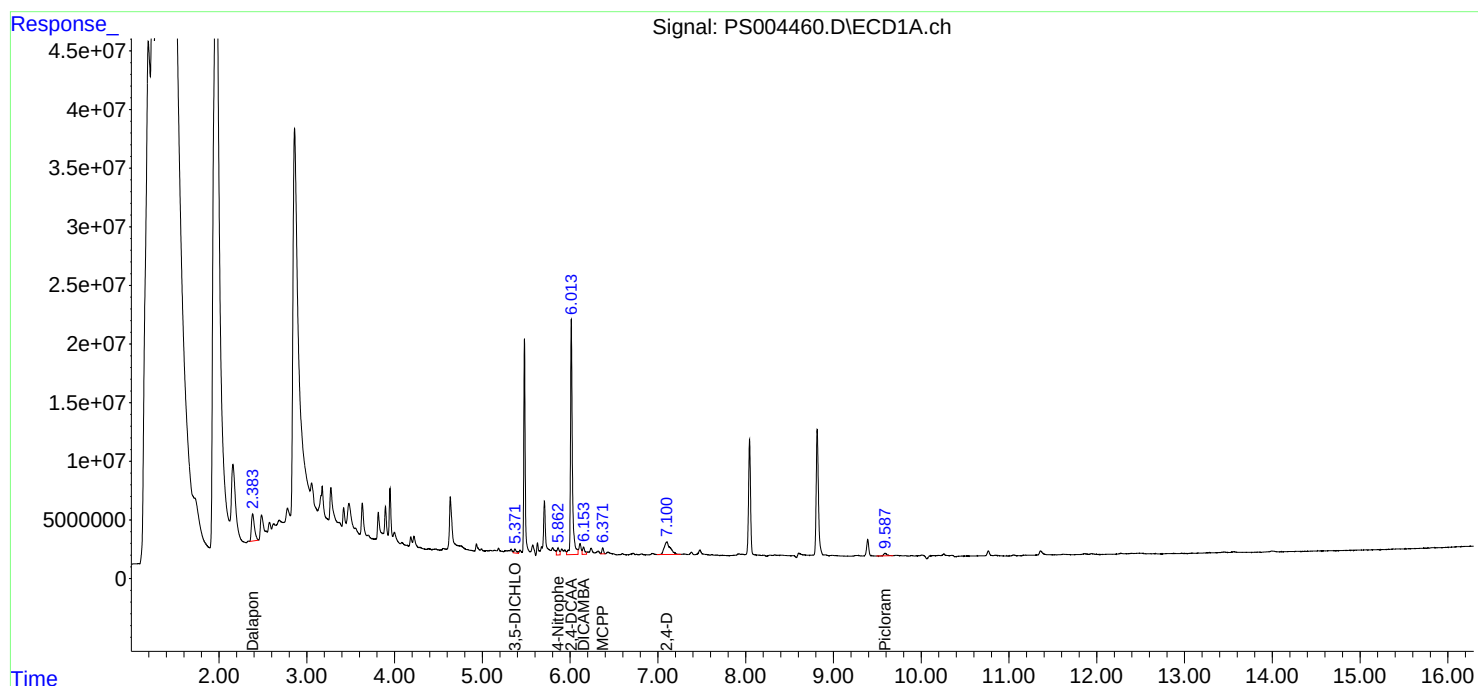


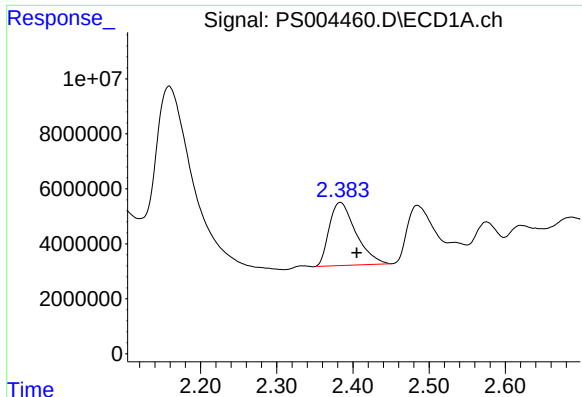

#1 Dalapon


R.T.: 2.383 min
Delta R.T.: -0.022 min
Response: 55786798
Conc: 70.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

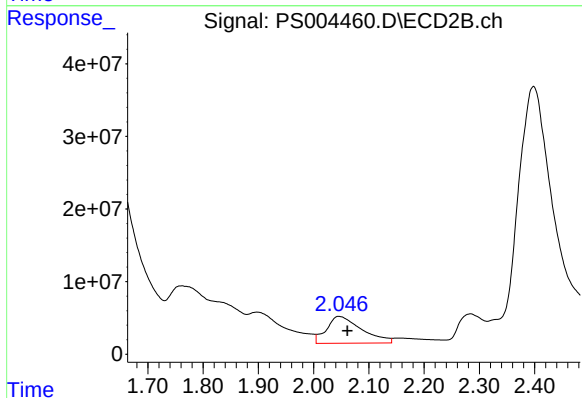


#1 Dalapon

R.T.: 2.046 min
Delta R.T.: -0.016 min
Response: 162840367
Conc: 243.34 ng/ml

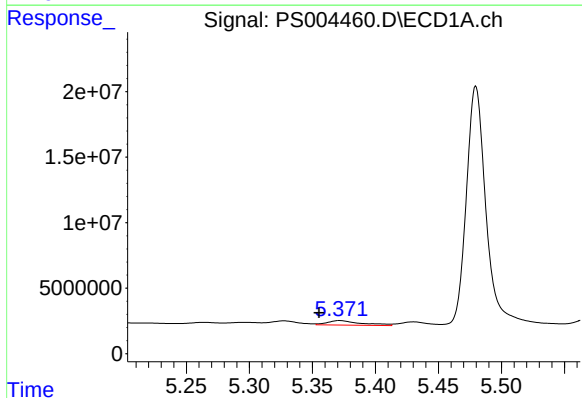


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.372 min
Delta R.T.: 0.016 min
Response: 6419483
Conc: 8.13 ng/ml

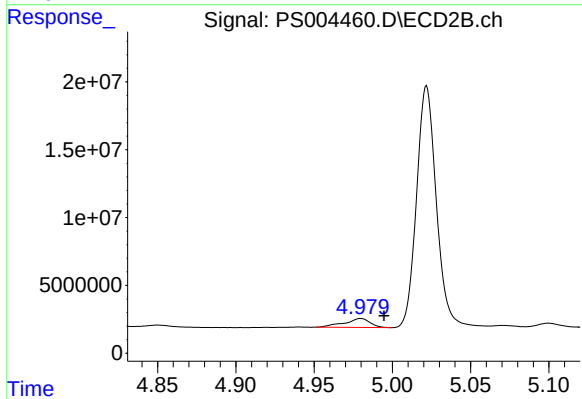

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.980 min
Delta R.T.: -0.015 min
Response: 7560669
Conc: 12.30 ng/ml

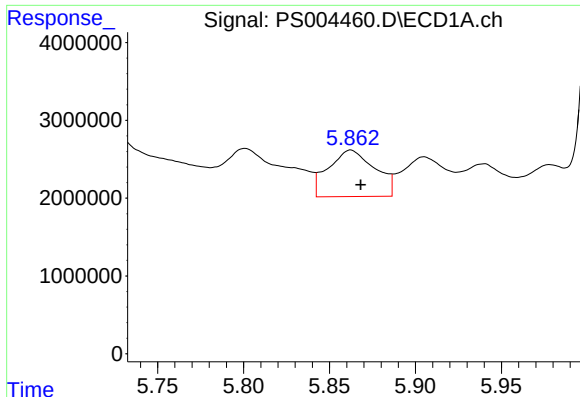

#3 4-Nitrophenol


R.T.: 5.862 min
Delta R.T.: -0.006 min
Response: 11227344
Conc: 44.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

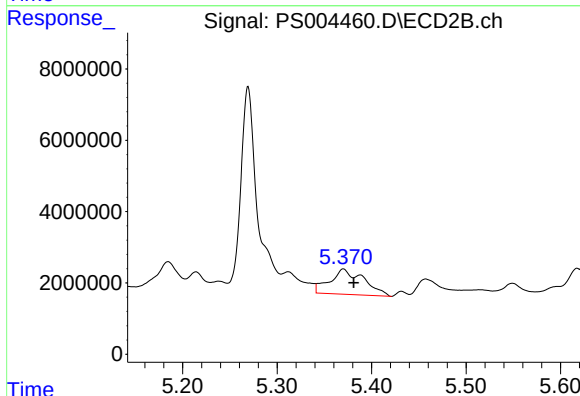


#3 4-Nitrophenol

R.T.: 5.370 min
Delta R.T.: -0.011 min
Response: 17708862
Conc: 71.59 ng/ml

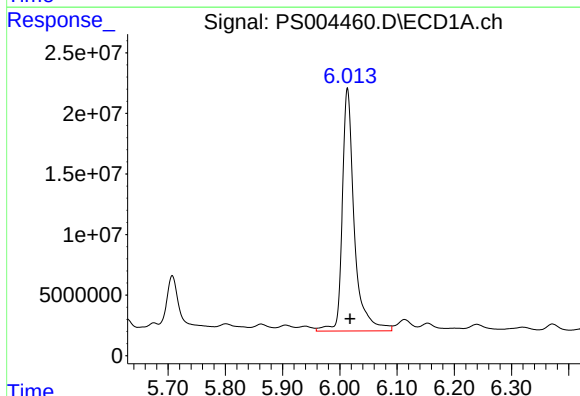


#4 2,4-DCAA

R.T.: 6.014 min
Delta R.T.: -0.004 min
Response: 292512122
Conc: 464.71 ng/ml

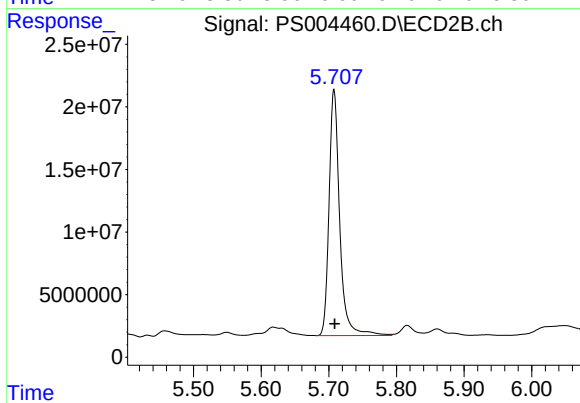

#4 2,4-DCAA


R.T.: 5.708 min
Delta R.T.: -0.001 min
Response: 214819074
Conc: 445.42 ng/ml

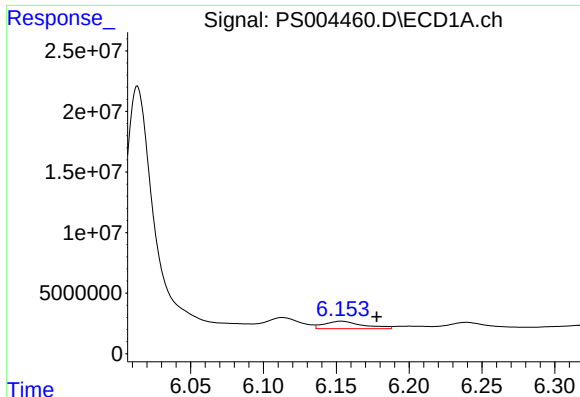

#5 DICAMBA


R.T.: 6.153 min
Delta R.T.: -0.024 min
Response: 11322026
Conc: 4.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

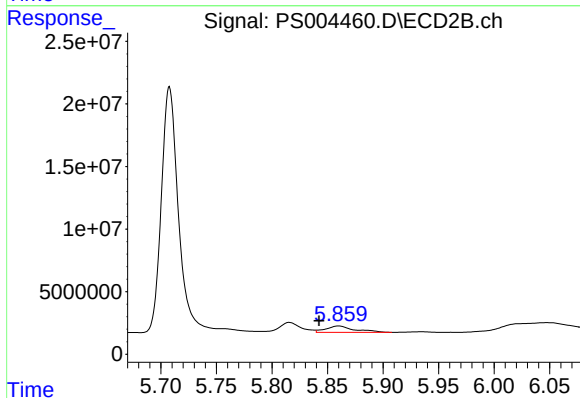


#5 DICAMBA

R.T.: 5.860 min
Delta R.T.: 0.018 min
Response: 9127753
Conc: 4.88 ng/ml

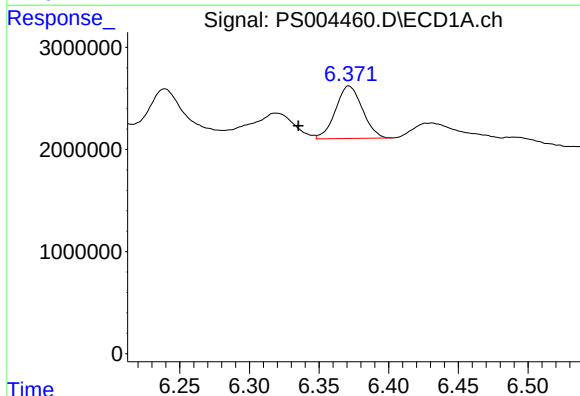


#6 MCP

R.T.: 6.372 min
Delta R.T.: 0.037 min
Response: 6871982
Conc: 3.98 ug/ml

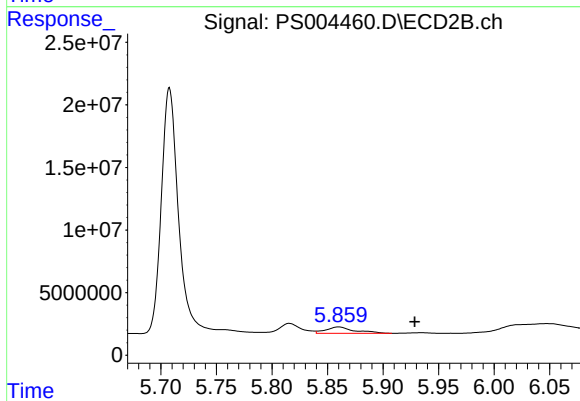

#6 MCP


R.T.: 5.860 min
Delta R.T.: -0.069 min
Response: 9127753
Conc: 6.79 ug/ml

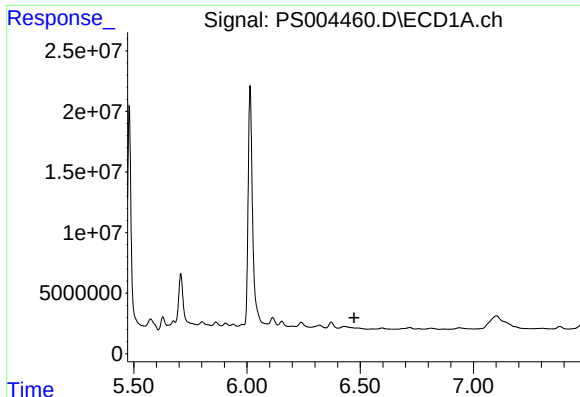

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

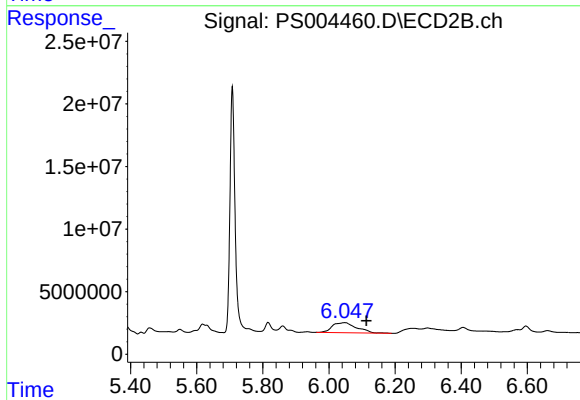


#7 MCPA

R.T.: 6.047 min
Delta R.T.: -0.066 min
Response: 41812200
Conc: 21.05 ug/ml

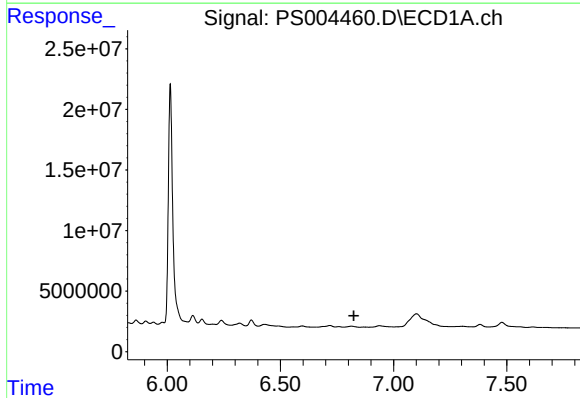


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.825 min
Response: 0
Conc: N.D.

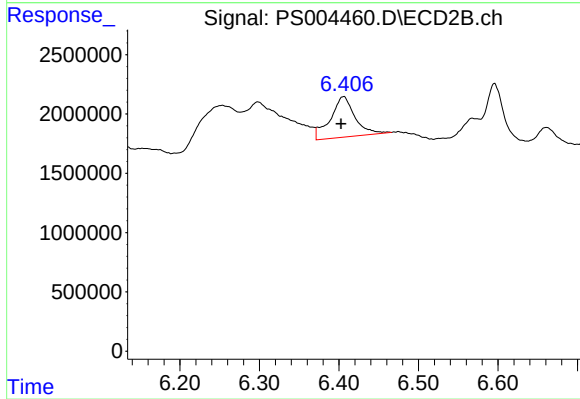

#8 DICHLORPROP


R.T.: 6.406 min
Delta R.T.: 0.003 min
Response: 7315175
Conc: 15.55 ng/ml

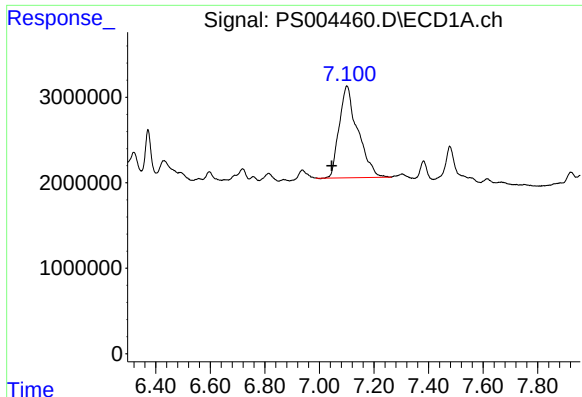

#9 2,4-D


R.T.: 7.101 min
Delta R.T.: 0.056 min
Response: 50928691
Conc: 89.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

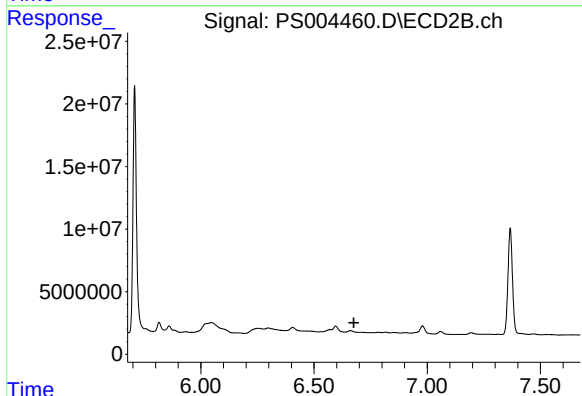


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

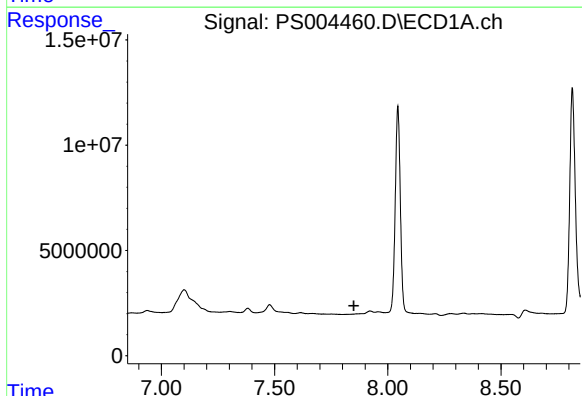


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

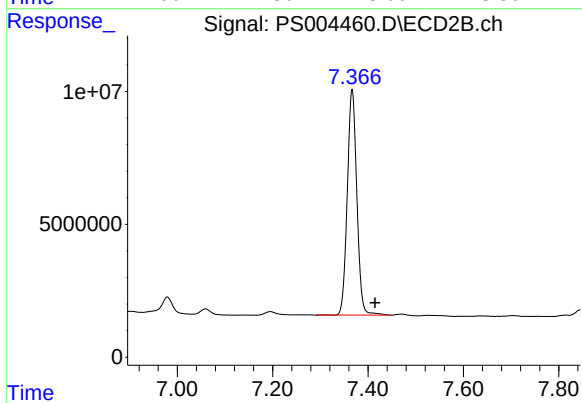

#11 2,4,5-TP (SILVEX)


R.T.: 7.367 min
Delta R.T.: -0.048 min
Response: 117890146
Conc: 44.87 ng/ml

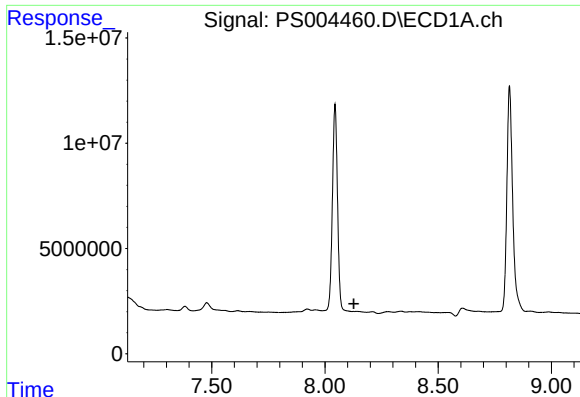

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FILTERBAG-RO

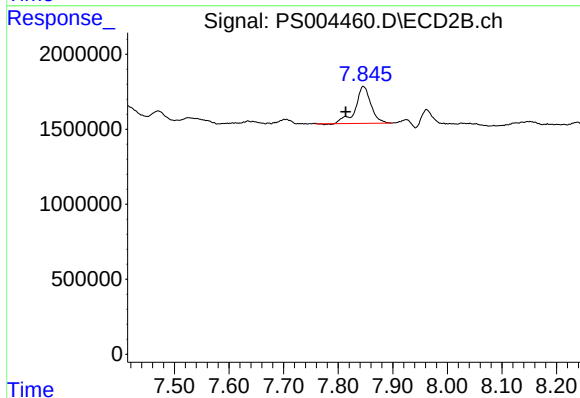


#12 2,4,5-T

R.T.: 7.846 min
Delta R.T.: 0.033 min
Response: 4830764
Conc: 2.15 ng/ml

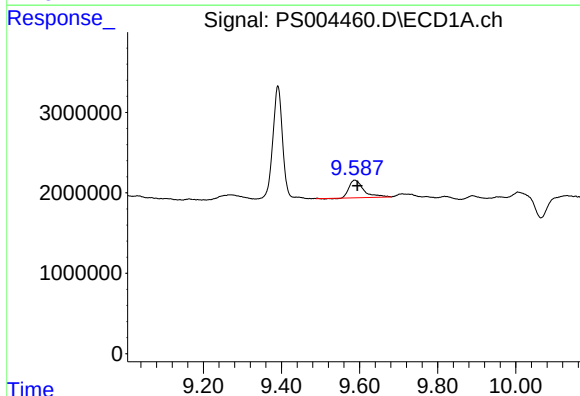

#15 Picloram

R.T.: 9.588 min
Delta R.T.: -0.006 min
Response: 5646221
Conc: 1.33 ng/ml

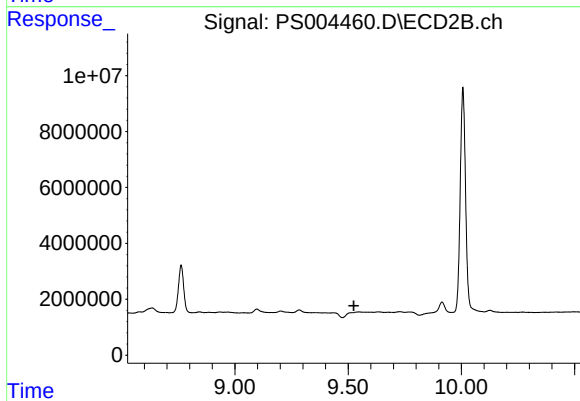

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.526 min
Response: 0
Conc: N.D.