

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050621\
 Data File : PS014927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2021 19:14
 Operator : DD\AJ
 Sample : M2277-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-A3-A3A-B3-B3A

Manual Integrations
 APPROVED

Ankita
 5/7/2021 11:34:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 03:51:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.154	6.884	524.4E6	180.7E6	344.751m	388.225

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050621\
Data File : PS014927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2021 19:14
Operator : DD\AJ
Sample : M2277-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3A


Manual Integrations
APPROVED

Ankita
5/7/2021 11:34:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 03:51:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

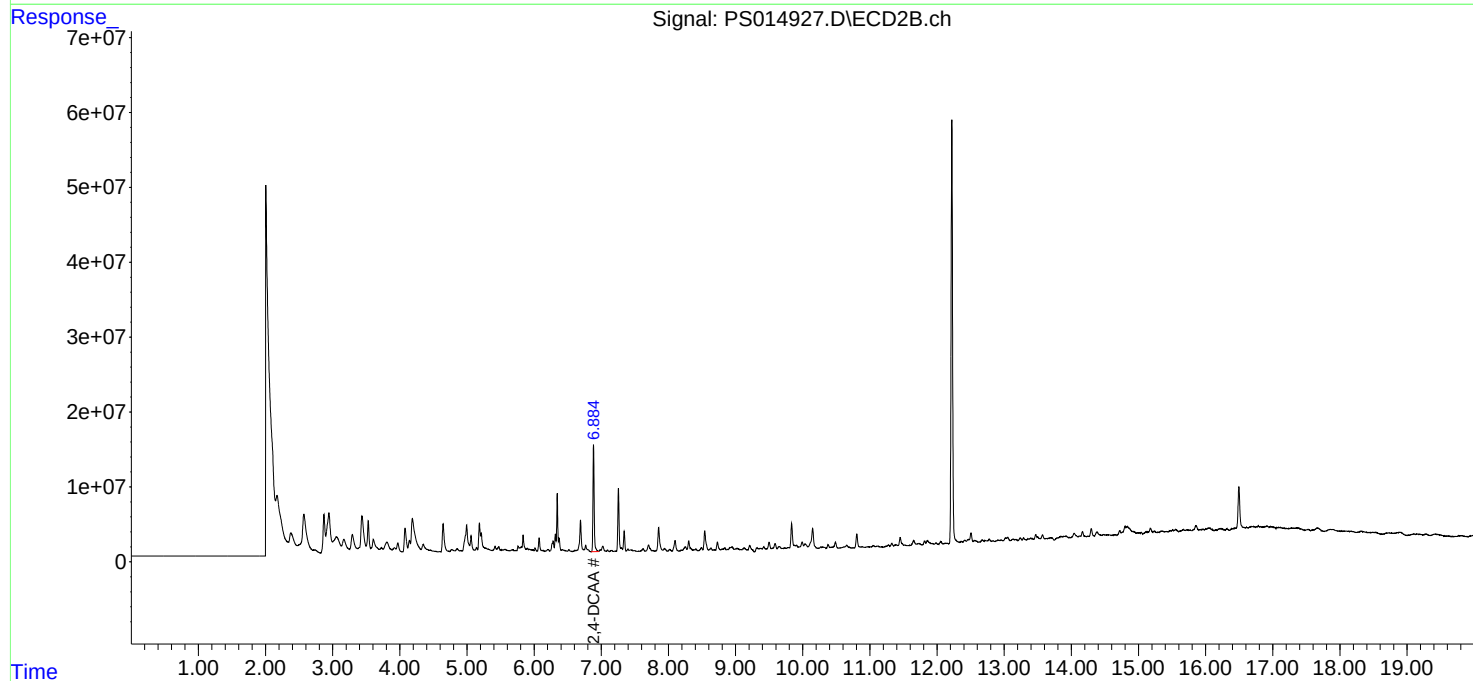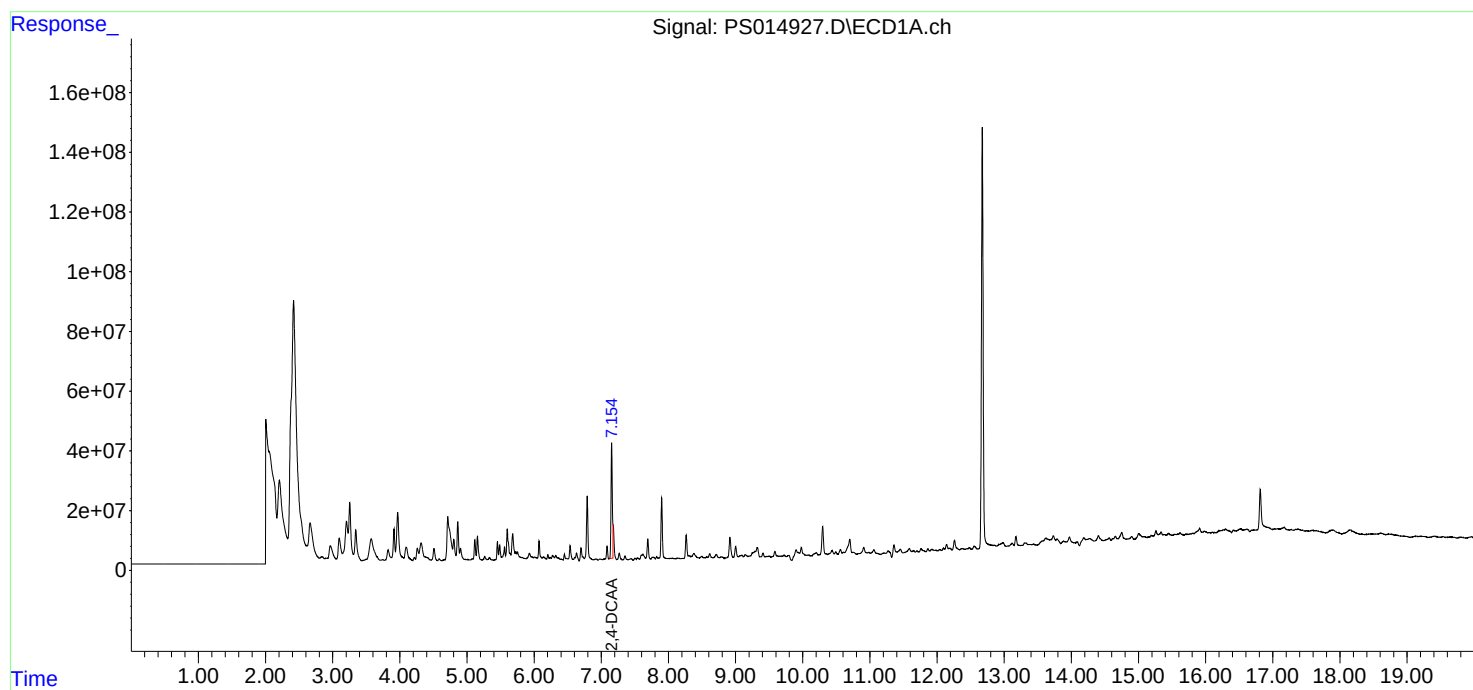

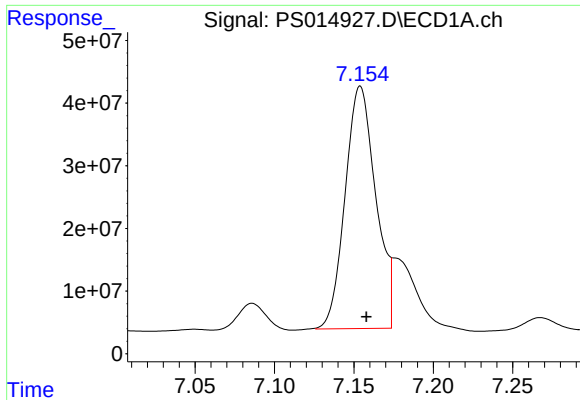


#4 2,4-DCAA

R.T.: 7.154 min
Delta R.T.: -0.004 min
Response: 524434293
Conc: 344.75 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3A

Manual Integrations
APPROVED

Ankita
5/7/2021 11:34:07 AM

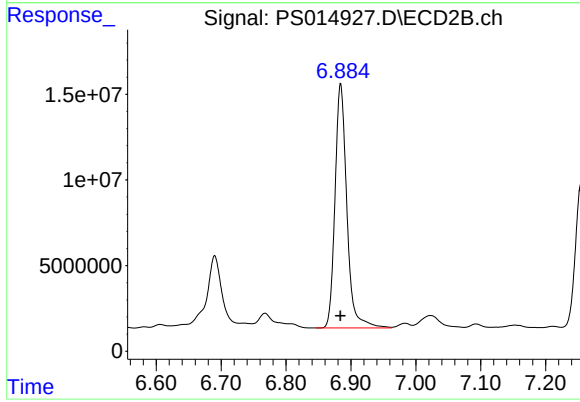

#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 180701282
Conc: 388.23 ng/ml