

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050624\
 Data File : PS026669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2024 22:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:21:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
 Quant Title : 8080.M
 QLast Update : Mon May 06 13:55:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.275	7.782	1319.8E6	902.4E6	530.710	541.221
Target Compounds							
1) T	Dalapon	2.700f	2.746f	24333261	20658007	6.653	7.046
2) T	3,5-DICHL...	6.424	0.000	9016949	0	2.622	N.D. #
3) T	4-Nitroph...	7.068	7.282f	13400017	3833209	8.317	3.371 #
5) T	DICAMBA	7.468	7.976	122304	1254166	<MDL	<MDL #
6) T	MCP	7.608f	8.089	108544	2224013	<MDL	<MDL #
7) T	MCPA	7.817	8.312	1429944	6294117	<MDL	<MDL #
8) T	DICHLORPROP	8.137f	0.000	12766572	0	4.260	N.D. #
9) T	2,4-D	8.421	0.000	10579867	0	3.214	N.D. #
10) T	Pentachlo...	8.698	9.561	1889949	1882695	<MDL	<MDL #
11) T	2,4,5-TP ...	9.277	9.904f	3700758	11125905	<MDL	1.008 #
12) T	2,4,5-T	9.527f	10.355	1065744	1397847	<MDL	<MDL #
14) T	DINOSEB	11.319f	11.300	8730646	317373	<MDL	<MDL #
16) T	DCPA	11.688f	0.000	245.0E6	0	13.016	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050624\
Data File : PS026669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2024 22:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:21:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
Quant Title : 8080.M
QLast Update : Mon May 06 13:55:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

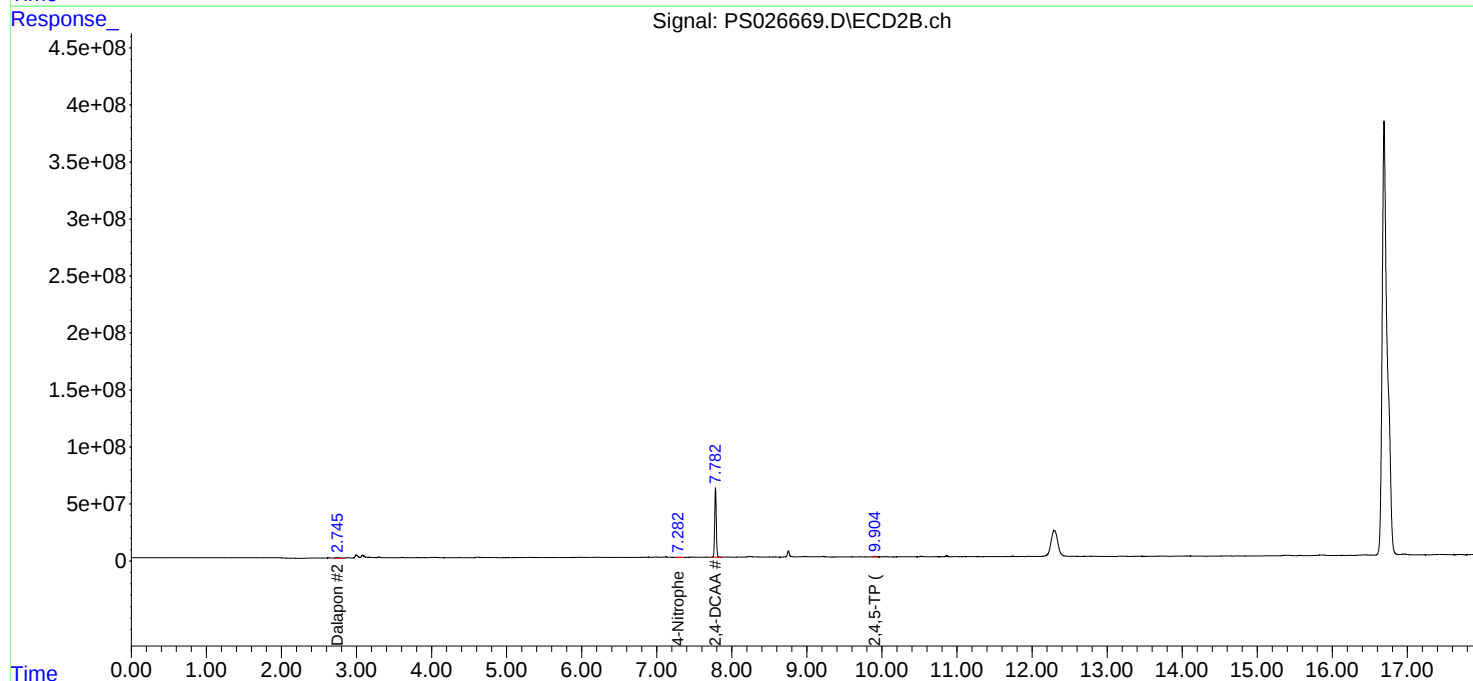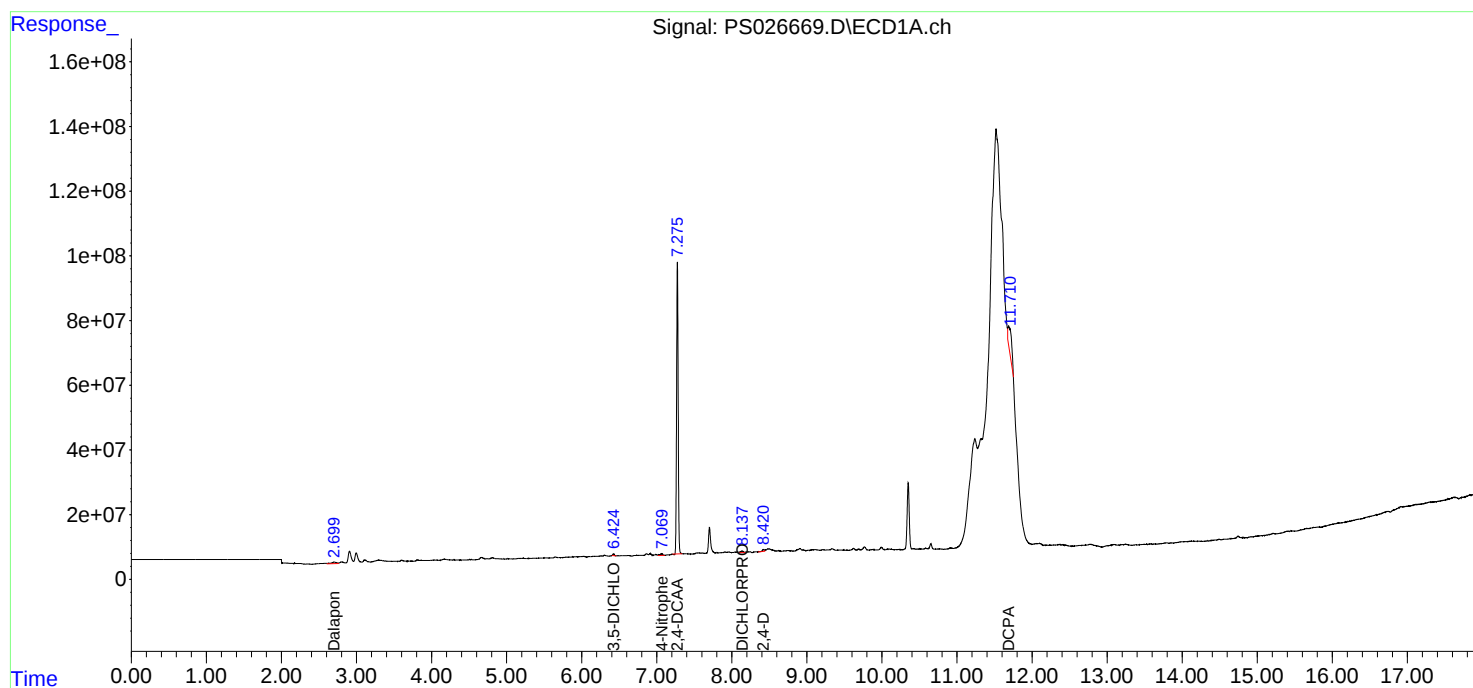


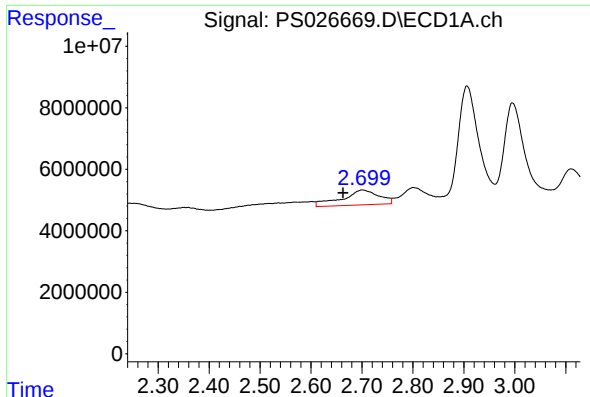

#1 Dalapon


R.T.: 2.700 min
Delta R.T.: 0.037 min
Response: 24333261
Conc: 6.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

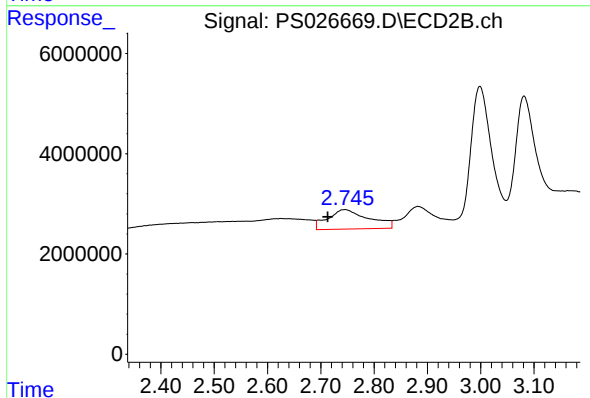


#1 Dalapon

R.T.: 2.746 min
Delta R.T.: 0.033 min
Response: 20658007
Conc: 7.05 ng/ml

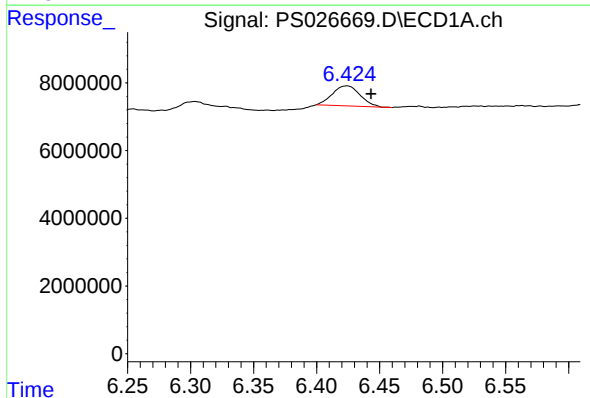


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.424 min
Delta R.T.: -0.019 min
Response: 9016949
Conc: 2.62 ng/ml

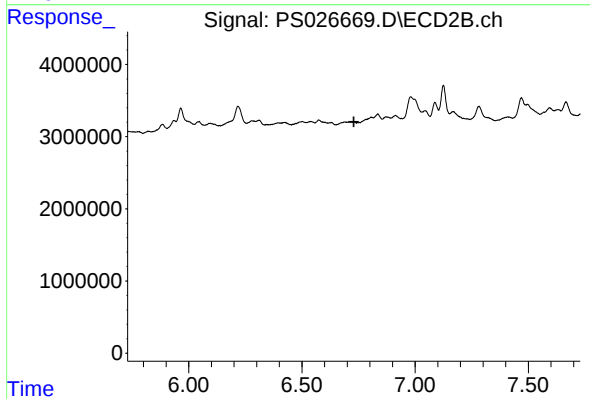

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.730 min
Response: 0
Conc: N.D.

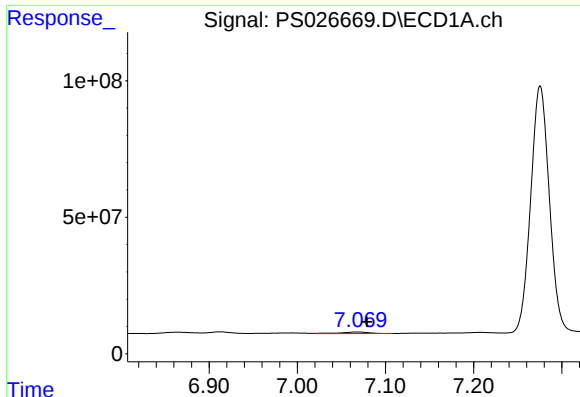

#3 4-Nitrophenol


R.T.: 7.068 min
Delta R.T.: -0.011 min
Response: 13400017
Conc: 8.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

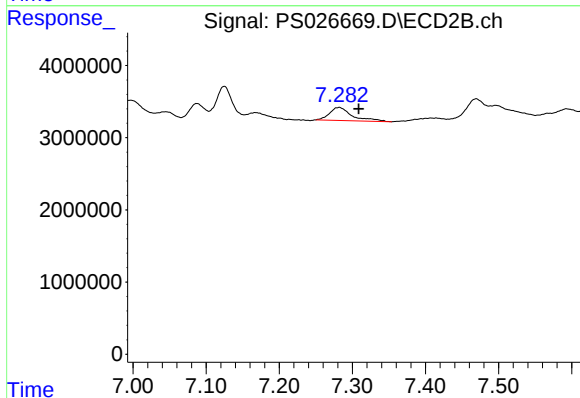


#3 4-Nitrophenol

R.T.: 7.282 min
Delta R.T.: -0.027 min
Response: 3833209
Conc: 3.37 ng/ml

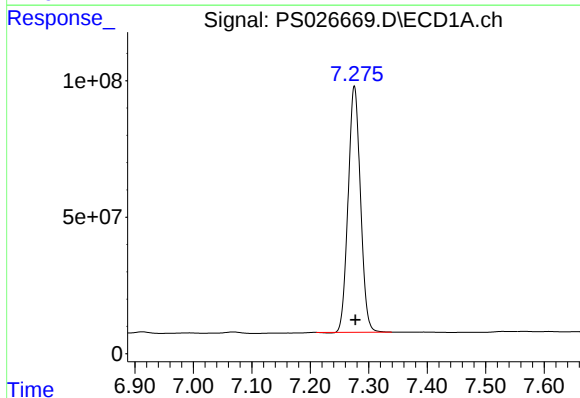


#4 2,4-DCAA

R.T.: 7.275 min
Delta R.T.: -0.002 min
Response: 1319799542
Conc: 530.71 ng/ml

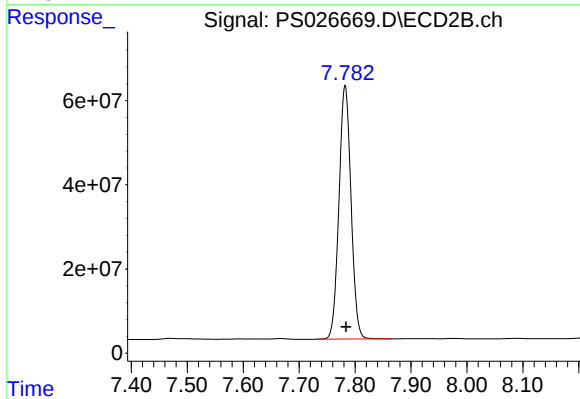

#4 2,4-DCAA


R.T.: 7.782 min
Delta R.T.: -0.002 min
Response: 902439545
Conc: 541.22 ng/ml

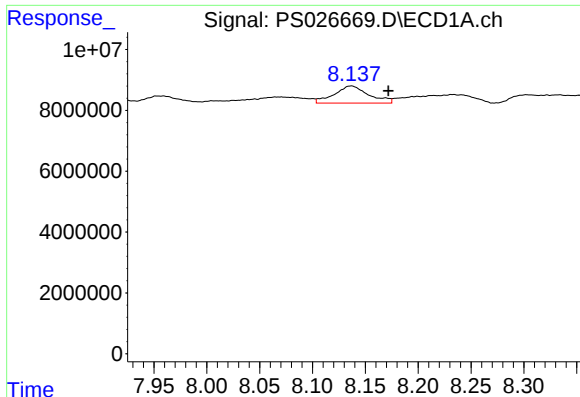

#8 DICHLORPROP


R.T.: 8.137 min
Delta R.T.: -0.035 min
Response: 12766572
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

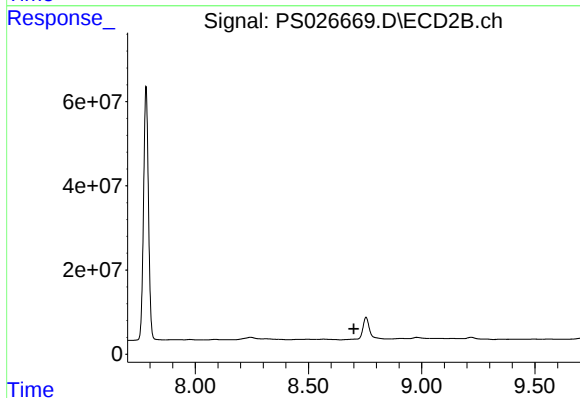


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.701 min
Response: 0
Conc: N.D.

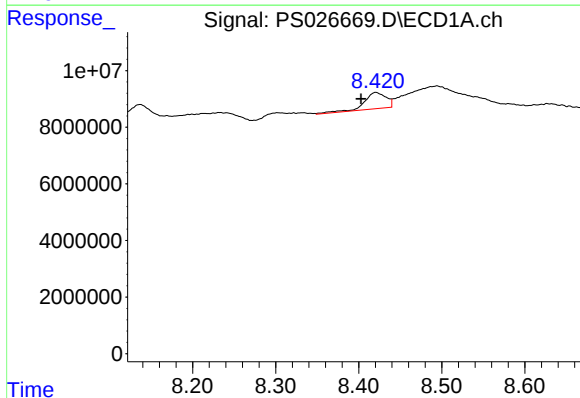


#9 2,4-D

R.T.: 8.421 min
Delta R.T.: 0.018 min
Response: 10579867
Conc: 3.21 ng/ml

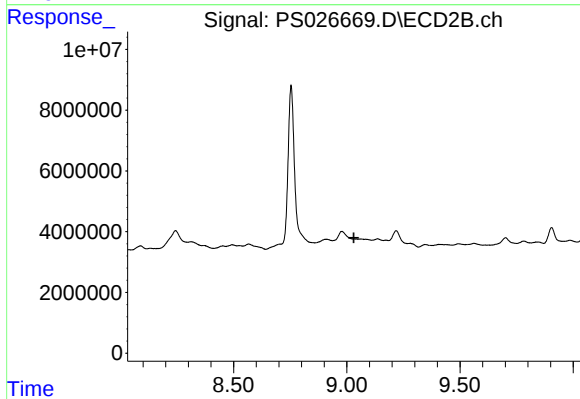

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

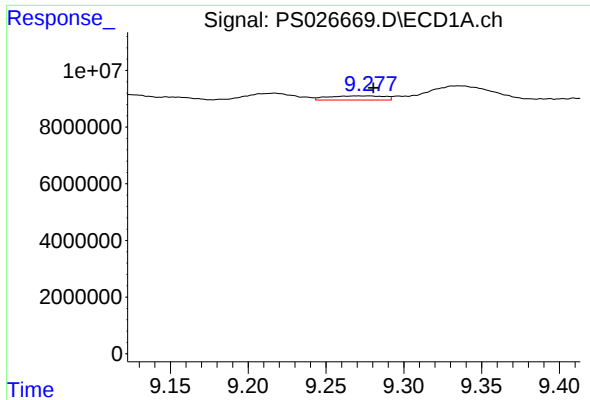

#11 2,4,5-TP (SILVEX)


R.T.: 9.277 min
Delta R.T.: -0.003 min
Response: 3700758
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

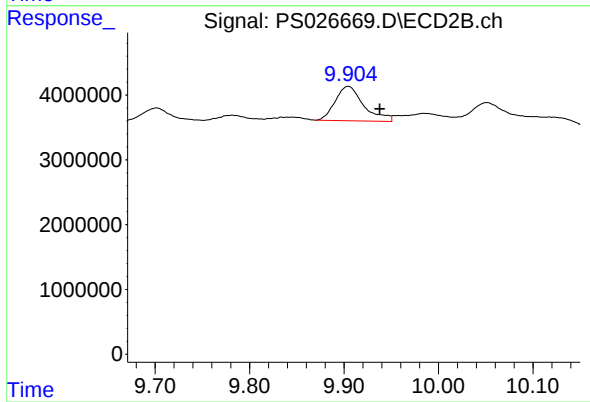


#11 2,4,5-TP (SILVEX)

R.T.: 9.904 min
Delta R.T.: -0.033 min
Response: 11125905
Conc: 1.01 ng/ml

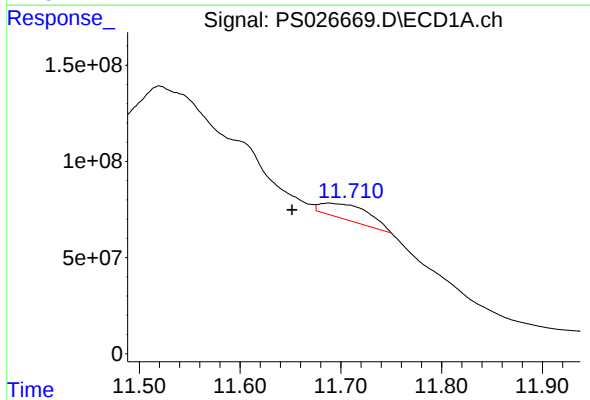

#16 DCPA

R.T.: 11.688 min
Delta R.T.: 0.036 min
Response: 245047331
Conc: 13.02 ng/ml

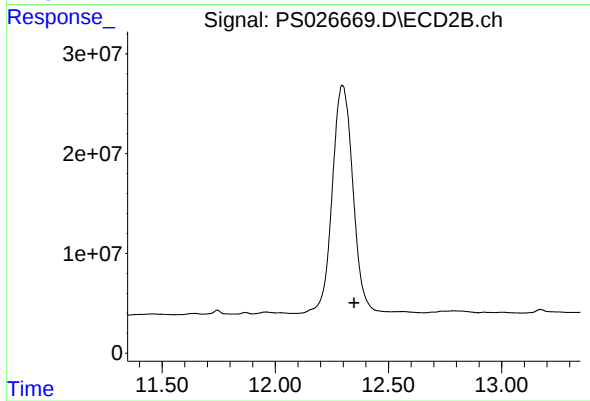

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 12.347 min
Response: 0
Conc: N.D.