

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050624\
 Data File : PS026653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2024 15:11
 Operator : AR\AJ
 Sample : PB160701BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB160701BL

Manual Integrations
 APPROVED

Reviewed By :Abdul
 Mirza
 05/07/2024

Supervised By :Ankita
 Jodhani
 05/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:02:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
 Quant Title : 8080.M
 QLast Update : Mon May 06 13:55:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.276	7.783	1396.8E6	882.2E6	561.673m	529.095

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050624\
Data File : PS026653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2024 15:11
Operator : AR\AJ
Sample : PB160701BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB160701BL

Manual Integrations
APPROVED

Reviewed By :Abdul

Mirza

05/07/2024



Supervised By :Ankita


Jodhani

05/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:02:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
Quant Title : 8080.M
QLast Update : Mon May 06 13:55:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

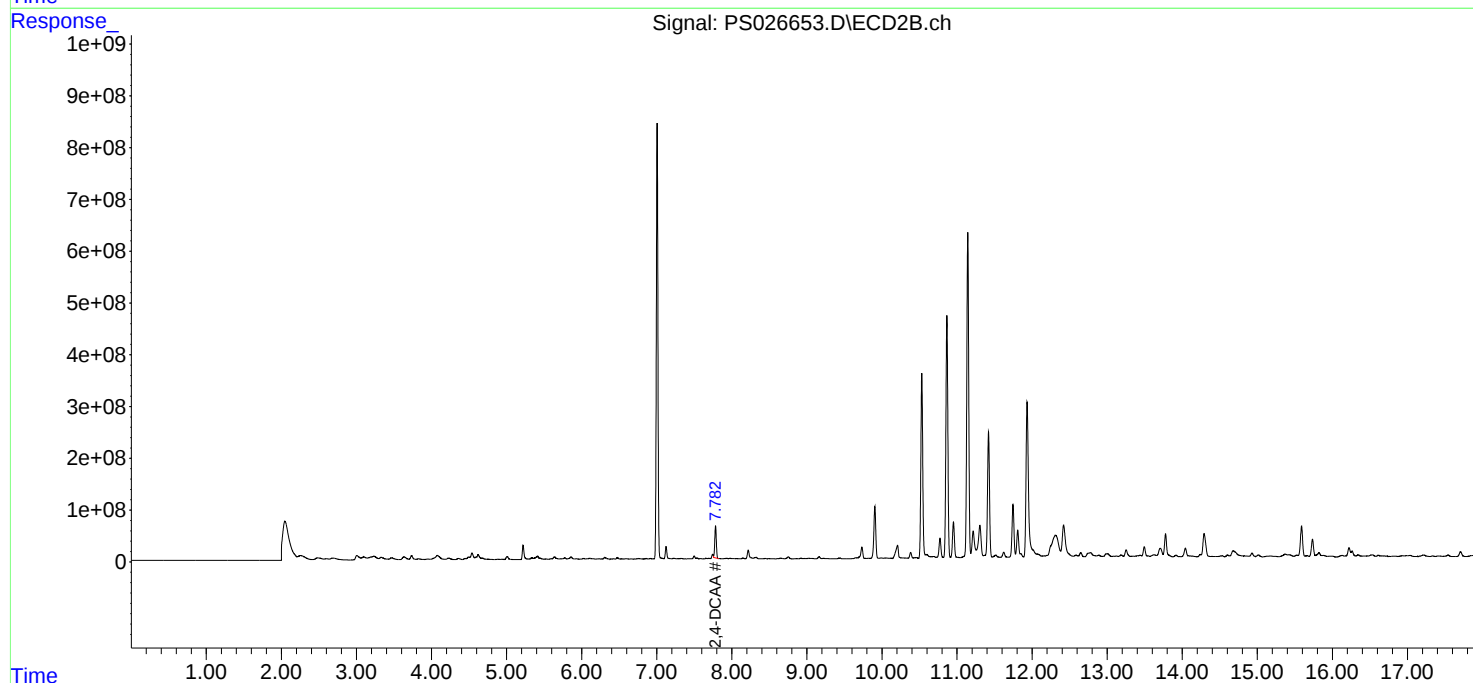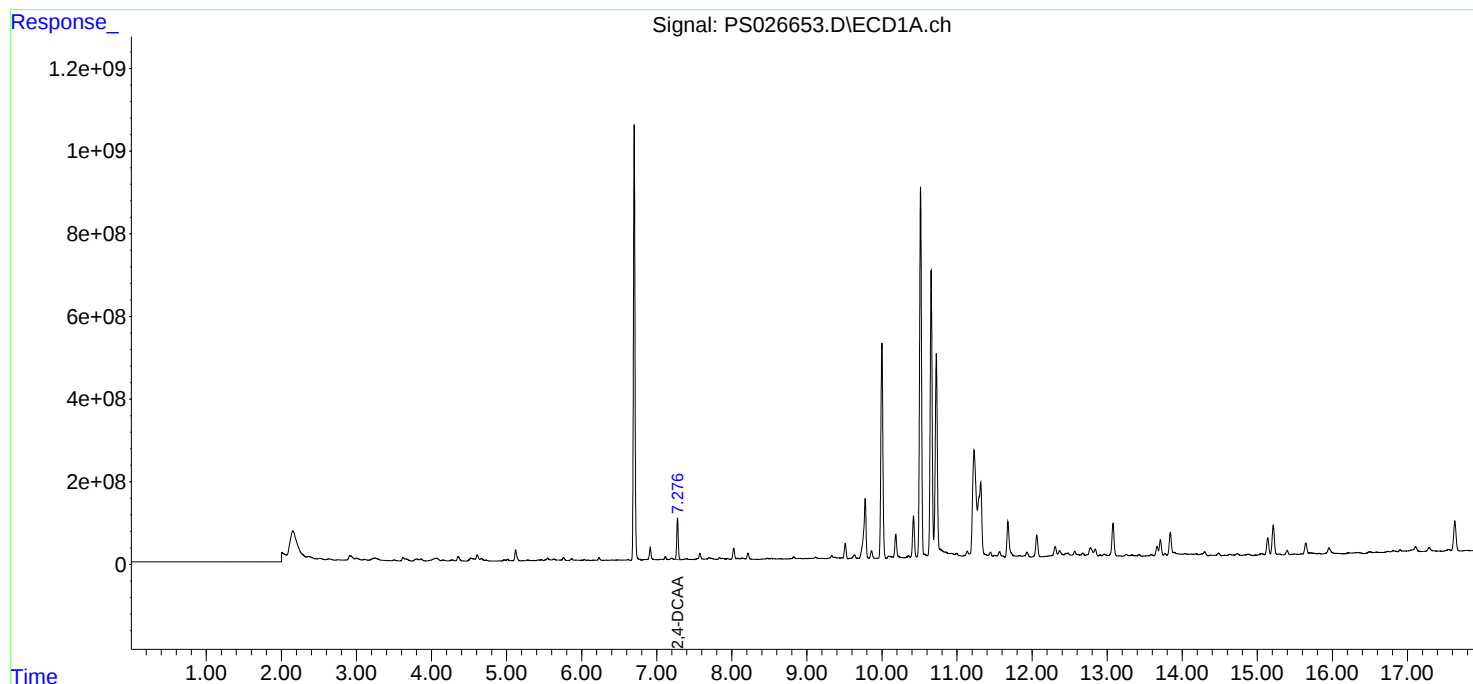

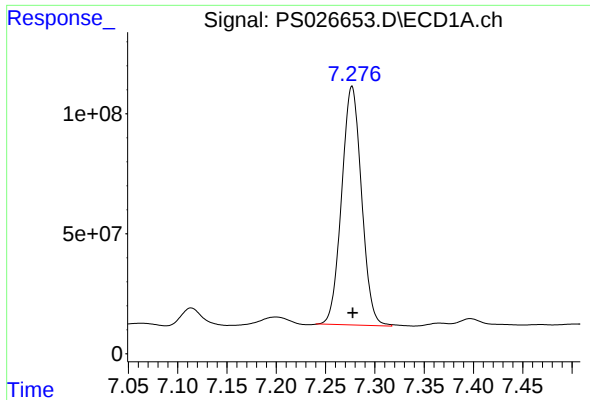

#4 2,4-DCAA


R.T.: 7.276 min
Delta R.T.: 0.000 min
Response: 1396800478
Conc: 561.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB160701BL

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza
05/07/2024

Supervised By :Ankita
Jodhani
05/07/2024

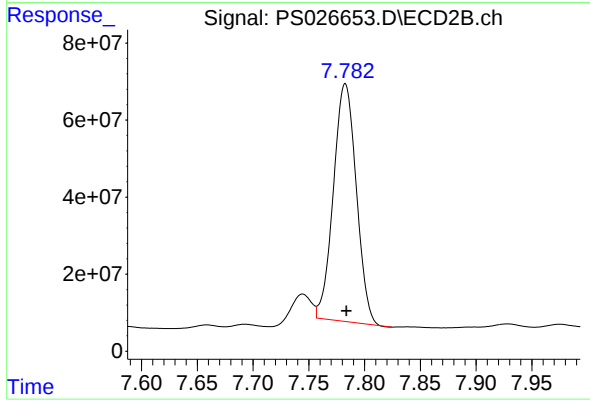

#4 2,4-DCAA

R.T.: 7.783 min
Delta R.T.: -0.001 min
Response: 882221411
Conc: 529.10 ng/ml