

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050719\
 Data File : PS004492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2019 23:08
 Operator : EI\SJ
 Sample : K2680-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SSSI-0502-S-TCLP-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 01:13:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.011	5.706	308.8E6	240.7E6	490.600	499.186
Target Compounds							
1) T	Dalapon	2.379	2.041	54838954	123.0E6	69.788	183.870 #
2) T	3,5-DICHL...	0.000	4.976	0	12949557	N.D.	21.065
3) T	4-Nitroph...	5.860	5.368	33307180	23716701	133.282	95.880 #
5) T	DICAMBA	6.202	5.856	16616912	17937746	6.988	9.584 #
6) T	MCPD	6.316	0.000	23159336	0	13.403	N.D. #
7) T	MCPA	6.419	0.000	23233242	0	9.018	N.D. #
8) T	DICHLORPROP	6.756	6.401	2661020	16260903	4.650	34.555 #
9) T	2,4-D	7.097	0.000	79326463	0	139.427	N.D. #
10) T	Pentachlo...	7.277	7.057	8216800	3796275	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	7.365	0	118.2E6	N.D.	45.004
12) T	2,4,5-T	0.000	7.842	0	83964069	N.D.	37.329
15) T	Picloram	0.000	9.545	0	30165303	N.D.	8.248
16) T	DCPA	0.000	9.545	0	30165303	N.D.	9.171



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050719\
Data File : PS004492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2019 23:08
Operator : EI\SJ
Sample : K2680-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 01:13:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

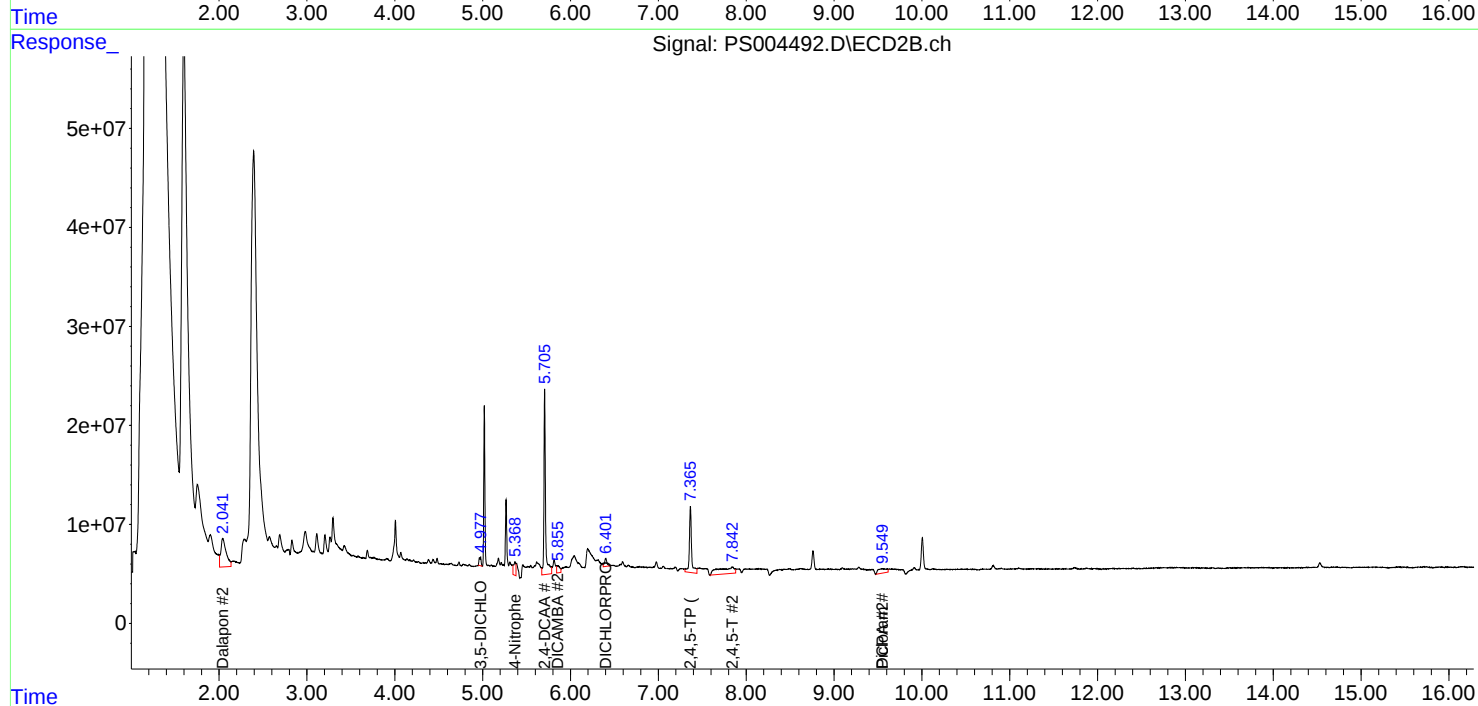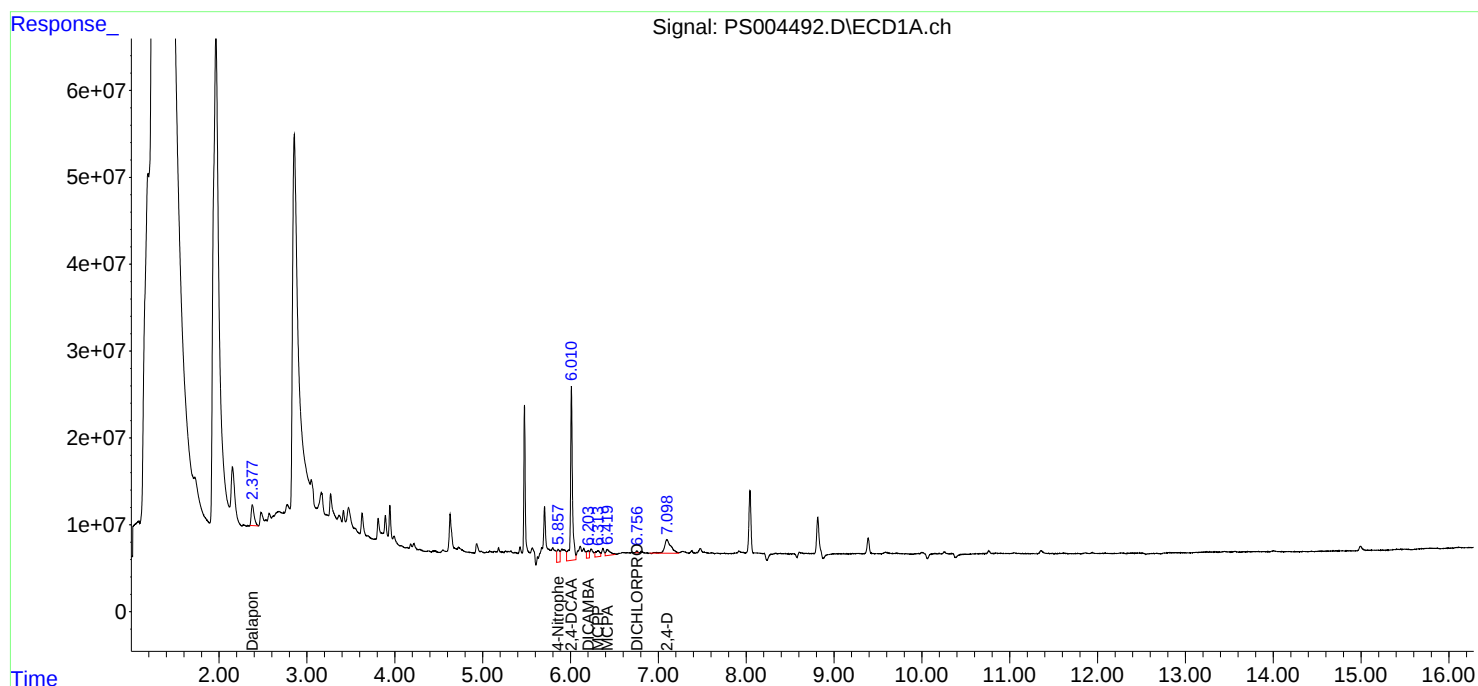


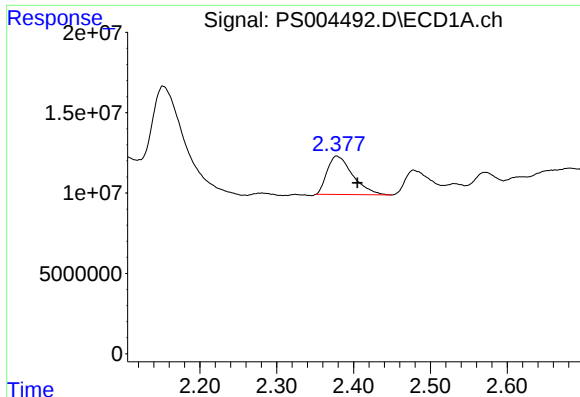

#1 Dalapon


R.T.: 2.379 min
Delta R.T.: -0.026 min
Response: 54838954
Conc: 69.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

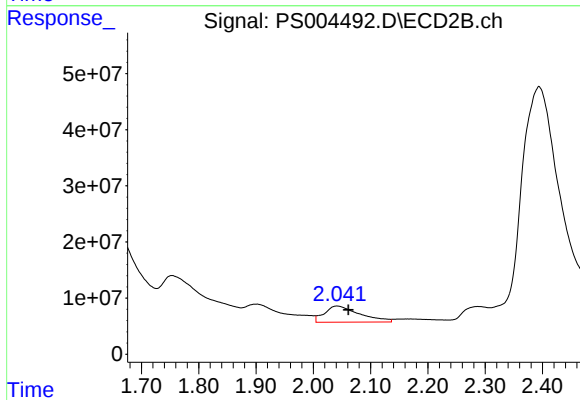


#1 Dalapon

R.T.: 2.041 min
Delta R.T.: -0.020 min
Response: 123043145
Conc: 183.87 ng/ml

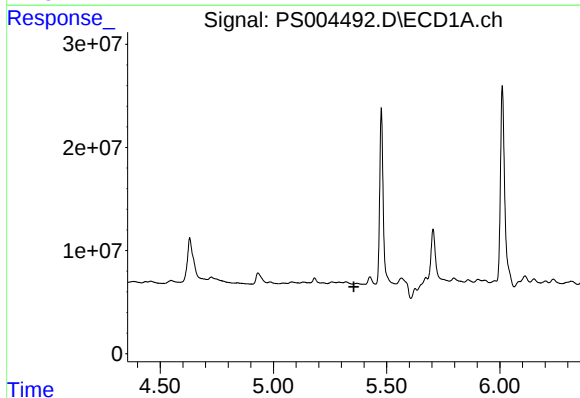


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

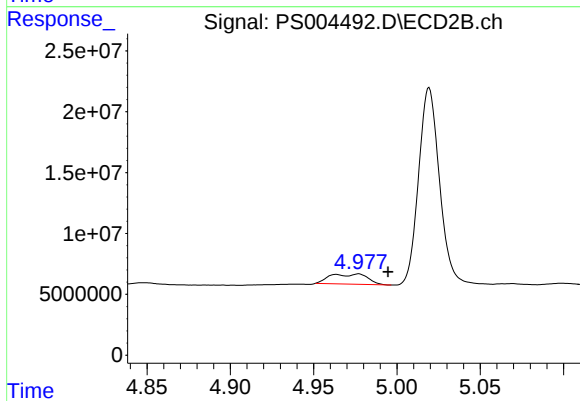

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.976 min
Delta R.T.: -0.018 min
Response: 12949557
Conc: 21.07 ng/ml

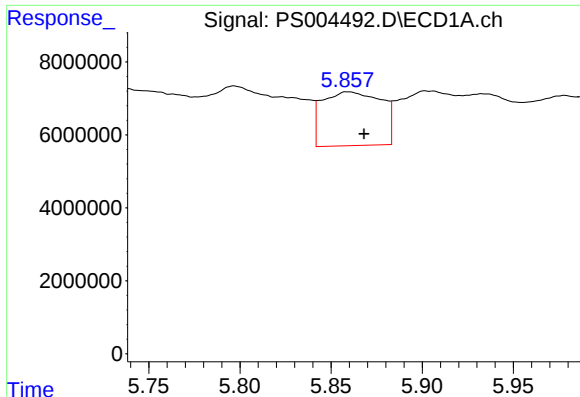

#3 4-Nitrophenol


R.T.: 5.860 min
Delta R.T.: -0.008 min
Response: 33307180
Conc: 133.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

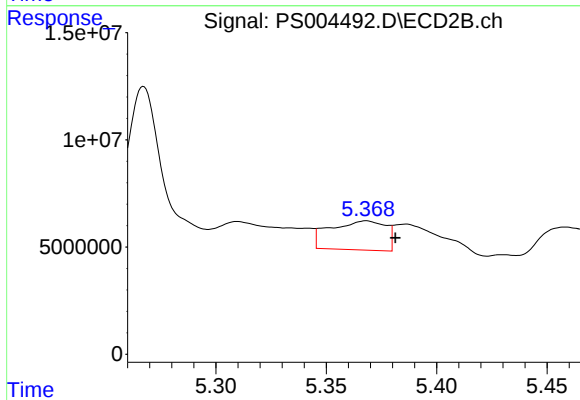


#3 4-Nitrophenol

R.T.: 5.368 min
Delta R.T.: -0.013 min
Response: 23716701
Conc: 95.88 ng/ml

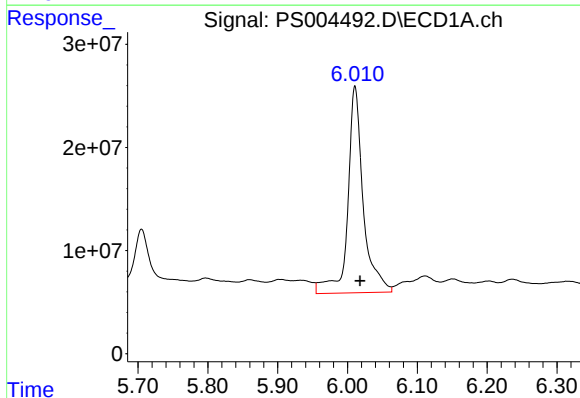


#4 2,4-DCAA

R.T.: 6.011 min
Delta R.T.: -0.007 min
Response: 308811885
Conc: 490.60 ng/ml

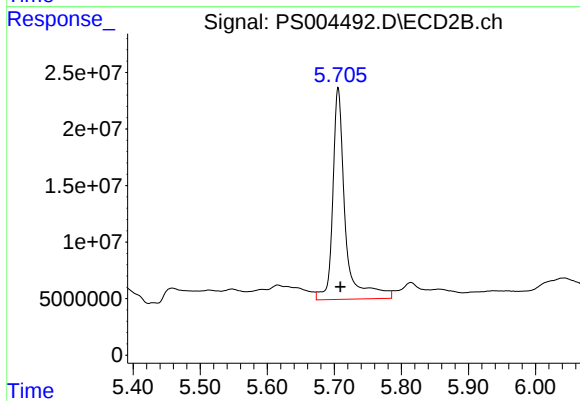

#4 2,4-DCAA


R.T.: 5.706 min
Delta R.T.: -0.003 min
Response: 240749100
Conc: 499.19 ng/ml

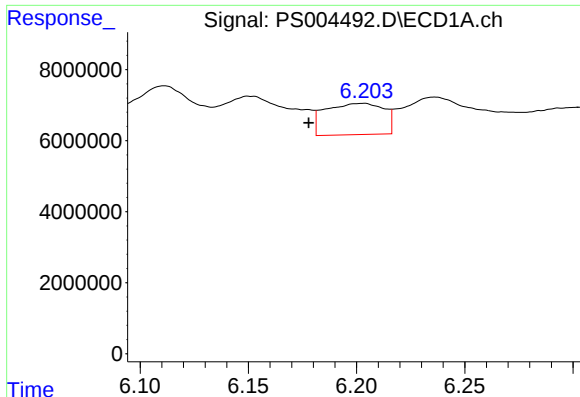

#5 DICAMBA


R.T.: 6.202 min
Delta R.T.: 0.024 min
Response: 16616912
Conc: 6.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

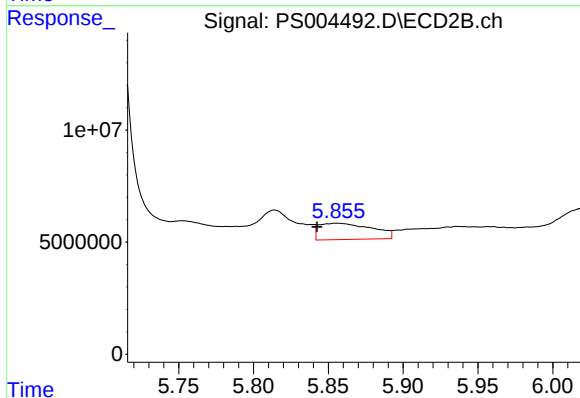


#5 DICAMBA

R.T.: 5.856 min
Delta R.T.: 0.014 min
Response: 17937746
Conc: 9.58 ng/ml

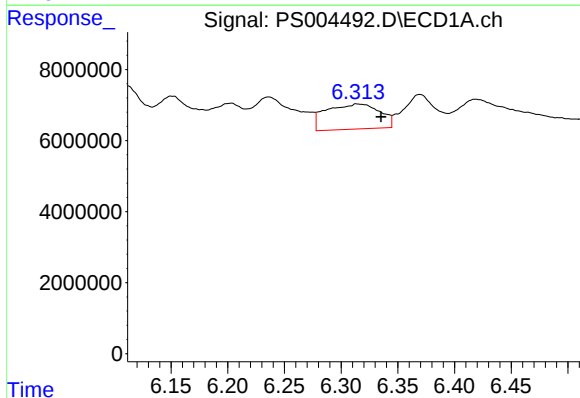


#6 MCP

R.T.: 6.316 min
Delta R.T.: -0.019 min
Response: 23159336
Conc: 13.40 ug/ml

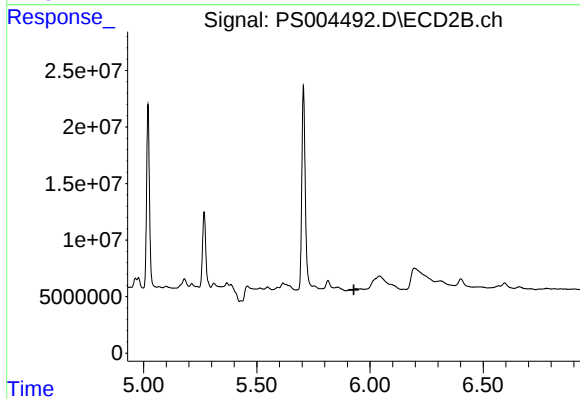

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

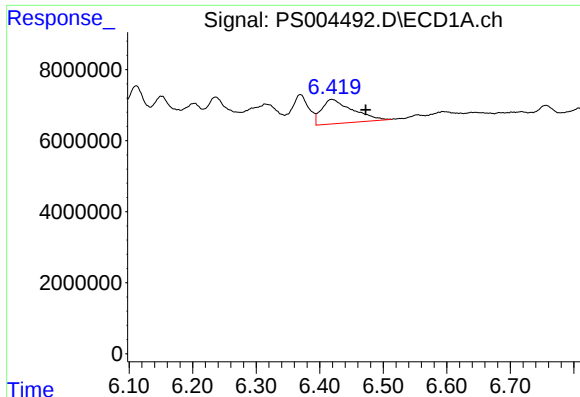

#7 MCPA


R.T.: 6.419 min
Delta R.T.: -0.053 min
Response: 23233242
Conc: 9.02 ug/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

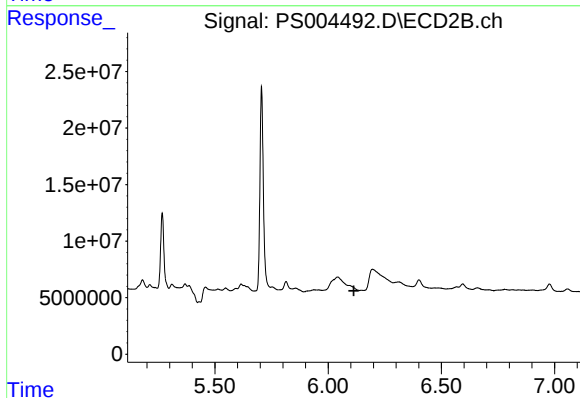


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.114 min
Response: 0
Conc: N.D.

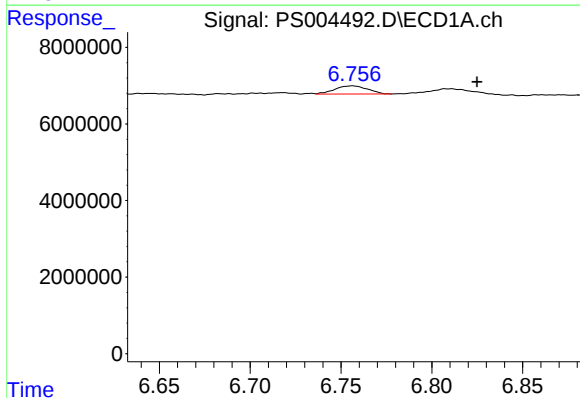


#8 DICHLORPROP

R.T.: 6.756 min
Delta R.T.: -0.069 min
Response: 2661020
Conc: 4.65 ng/ml

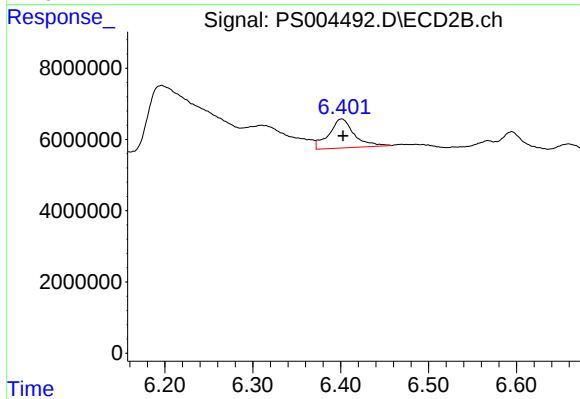

#8 DICHLORPROP


R.T.: 6.401 min
Delta R.T.: -0.002 min
Response: 16260903
Conc: 34.56 ng/ml

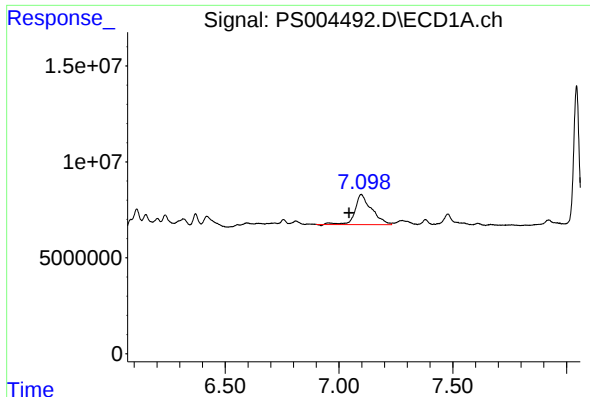

#9 2,4-D


R.T.: 7.097 min
Delta R.T.: 0.052 min
Response: 79326463
Conc: 139.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

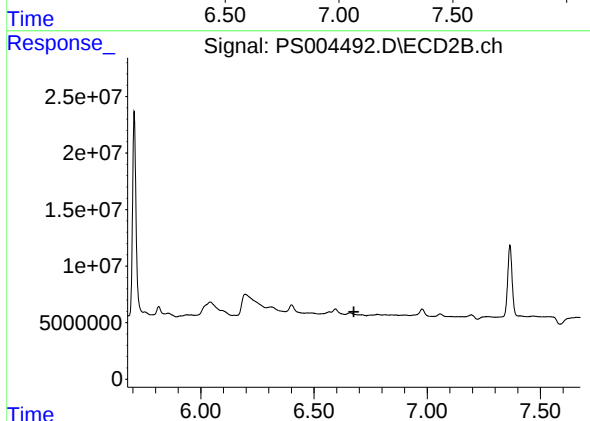


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

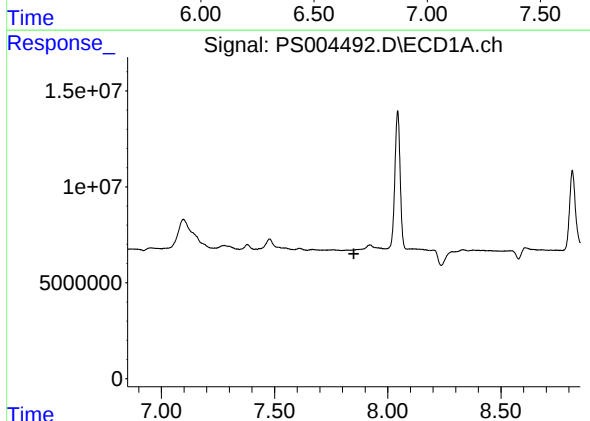


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

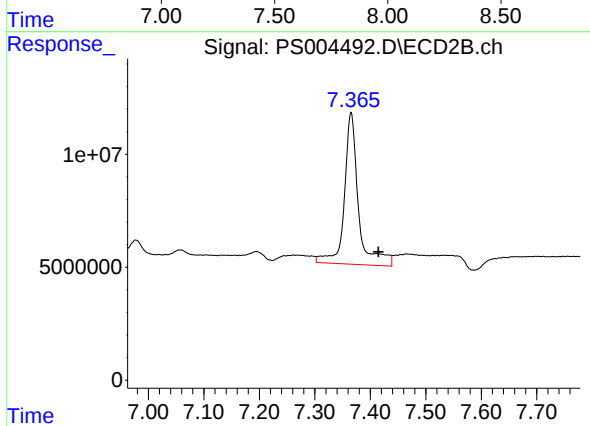

#11 2,4,5-TP (SILVEX)


R.T.: 7.365 min
Delta R.T.: -0.049 min
Response: 118246506
Conc: 45.00 ng/ml

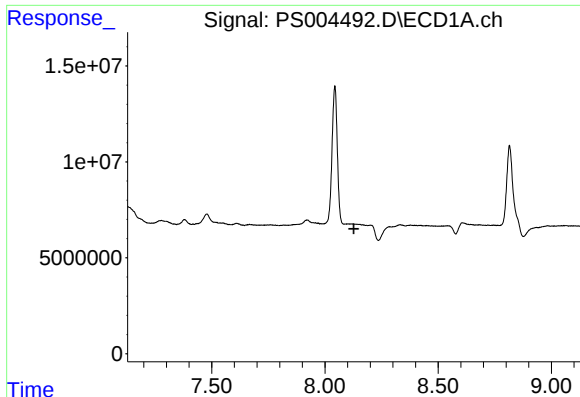

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

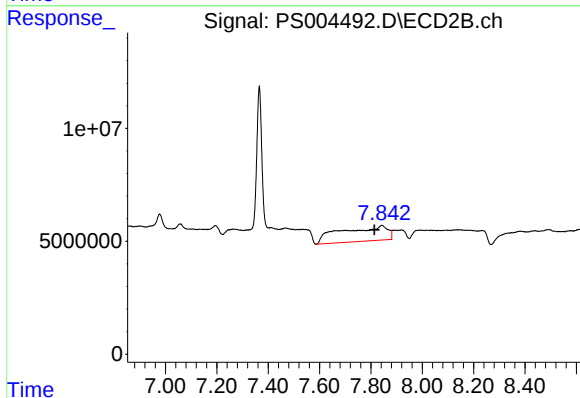


#12 2,4,5-T

R.T.: 7.842 min
Delta R.T.: 0.029 min
Response: 83964069
Conc: 37.33 ng/ml

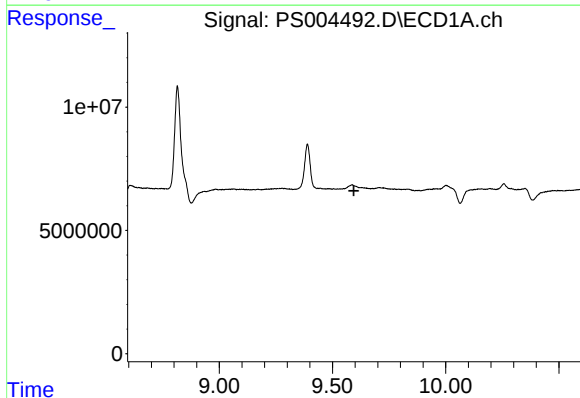


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.595 min
Response: 0
Conc: N.D.

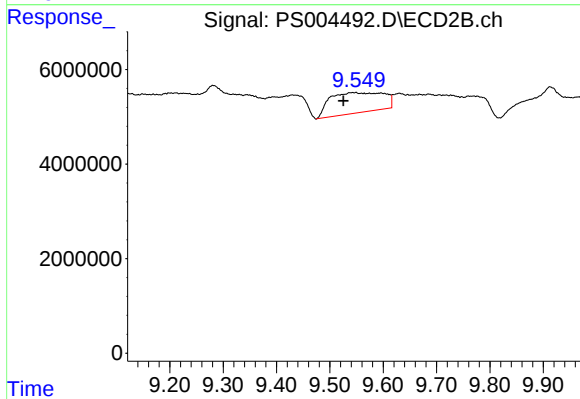

#15 Picloram


R.T.: 9.545 min
Delta R.T.: 0.020 min
Response: 30165303
Conc: 8.25 ng/ml

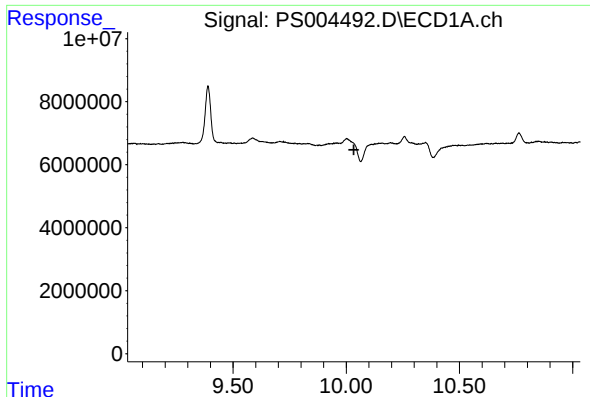

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SSSI-0502-S-TCLP-9

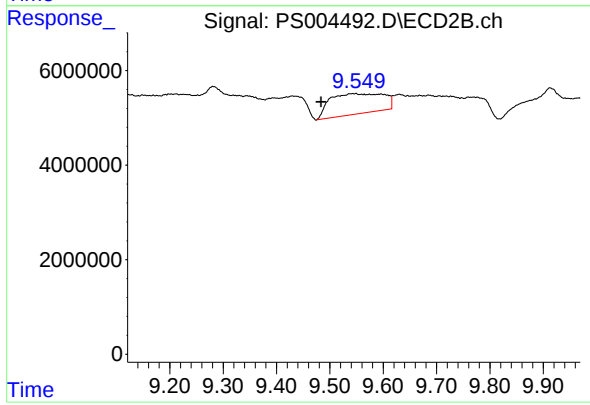

#16 DCPA

R.T.: 9.545 min
Delta R.T.: 0.062 min
Response: 30165303
Conc: 9.17 ng/ml