

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050719\
 Data File : PS004495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2019 00:44
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 01:14:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.998	5.692	313.3E6	237.5E6	497.786	492.379
Target Compounds							
9) T	2,4-D	7.080	0.000	79605384	0	139.917	N.D. #
15) T	Picloram	0.000	9.540	0	9001320	N.D.	2.461
16) T	DCPA	0.000	9.540	0	9001320	N.D.	2.737



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050719\
Data File : PS004495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2019 00:44
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 01:14:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

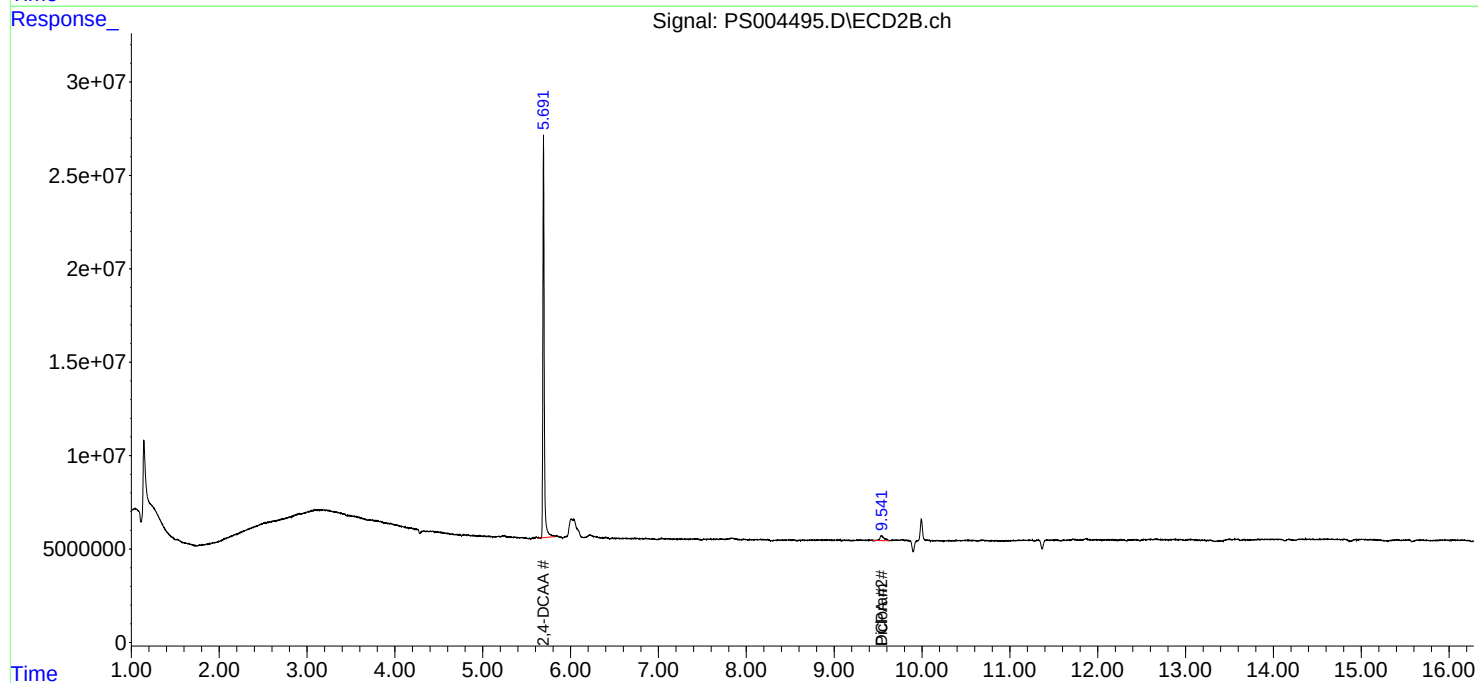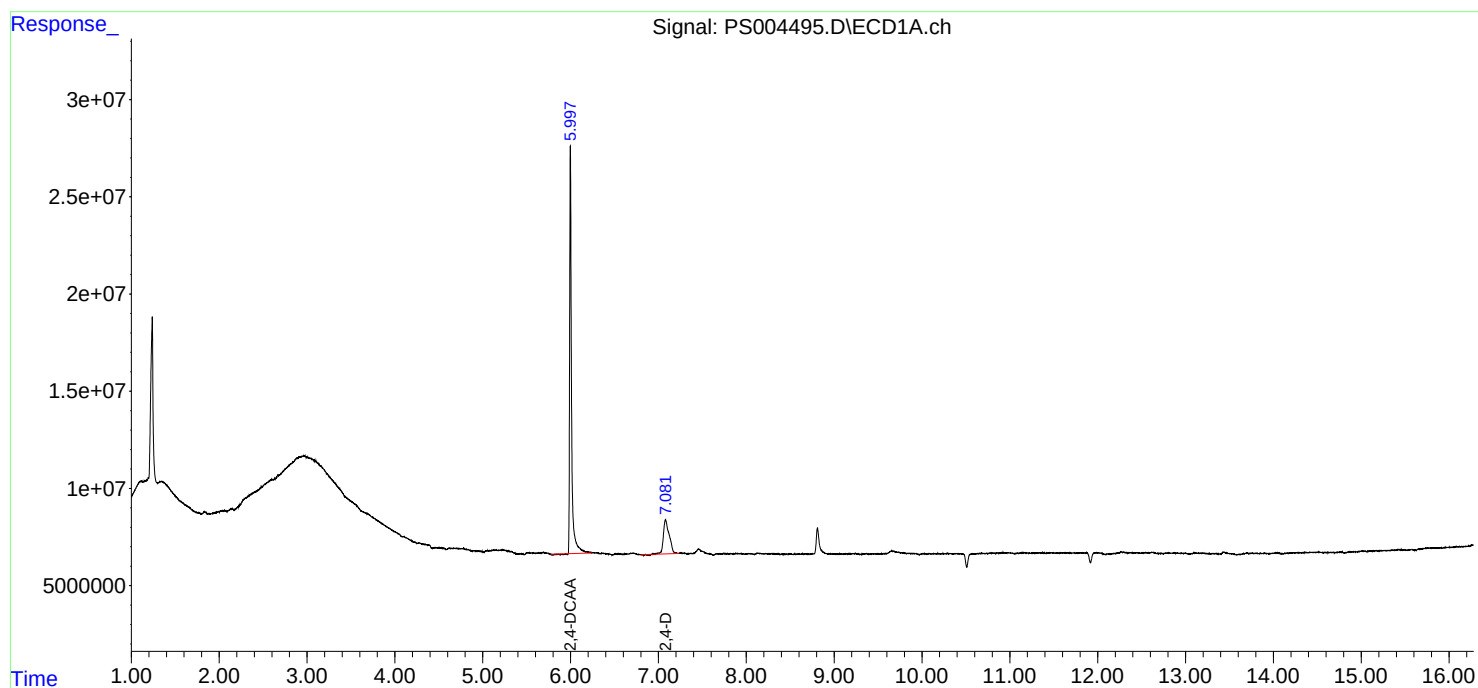


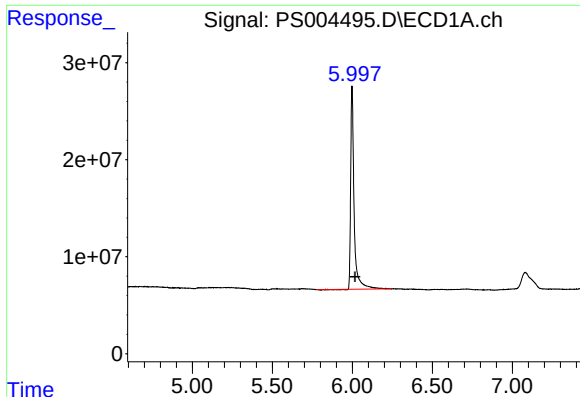

#4 2,4-DCAA


R.T.: 5.998 min
Delta R.T.: -0.020 min
Response: 313334889
Conc: 497.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

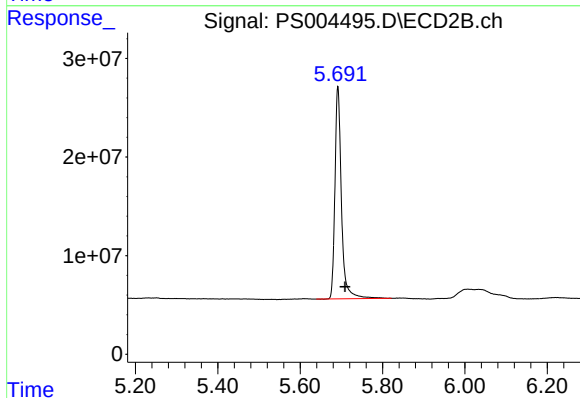


#4 2,4-DCAA

R.T.: 5.692 min
Delta R.T.: -0.017 min
Response: 237466036
Conc: 492.38 ng/ml

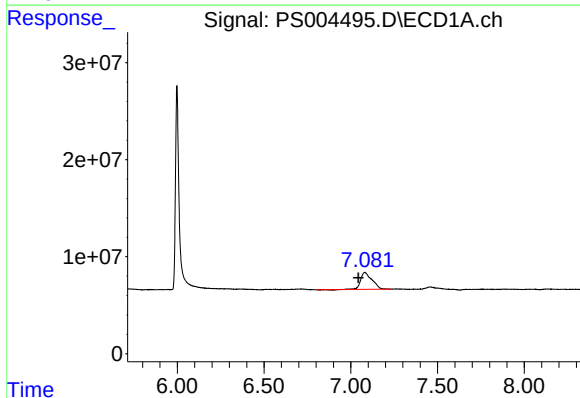


#9 2,4-D

R.T.: 7.080 min
Delta R.T.: 0.035 min
Response: 79605384
Conc: 139.92 ng/ml

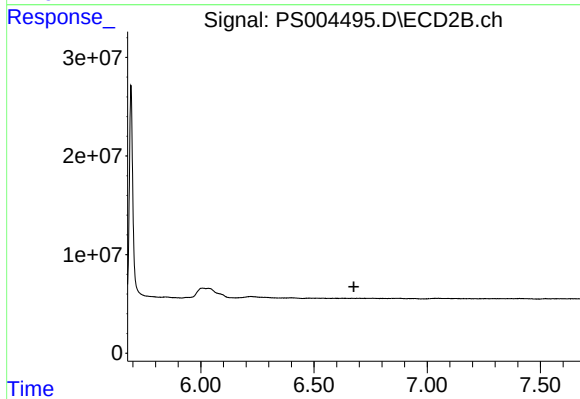

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.676 min
Response: 0
Conc: N.D.

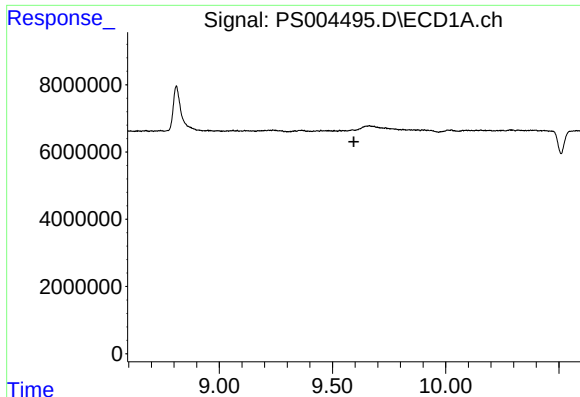

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

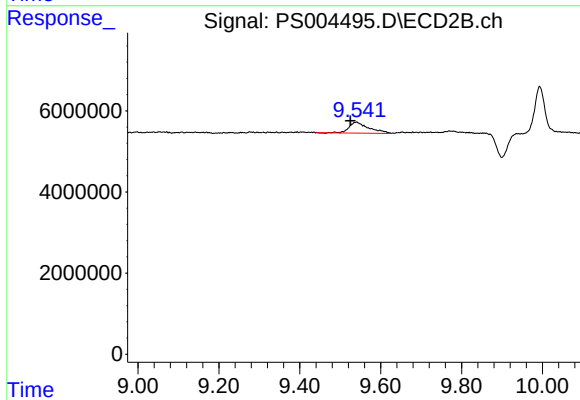


#15 Picloram

R.T.: 9.540 min
Delta R.T.: 0.014 min
Response: 9001320
Conc: 2.46 ng/ml

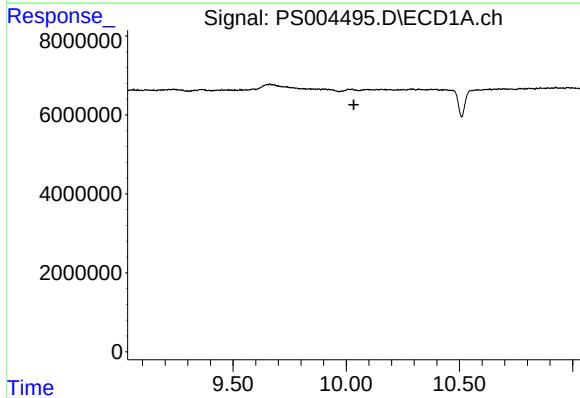

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.034 min
Response: 0
Conc: N.D.

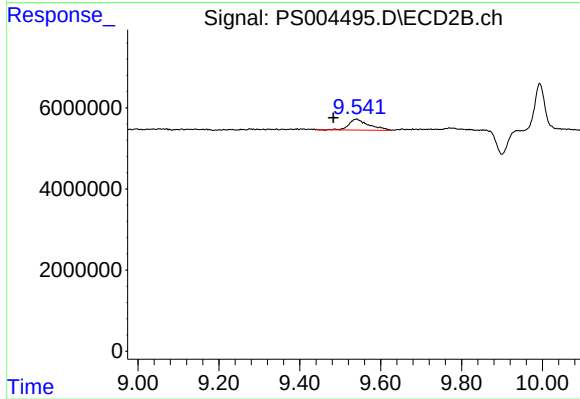

#16 DCPA

R.T.: 9.540 min
Delta R.T.: 0.056 min
Response: 9001320
Conc: 2.74 ng/ml