

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050719\
 Data File : PS004485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2019 19:29
 Operator : EI\SJ
 Sample : K2639-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NB-08-050319-A

Manual Integrations
 APPROVED

Ankita
 5/8/2019 2:32:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 01:11:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.014	5.709	285.3E6	204.5E6	453.188m	424.096m
------	----------	-------	-------	---------	---------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050719\
Data File : PS004485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2019 19:29
Operator : EI\SJ
Sample : K2639-02
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
NB-08-050319-A


Manual Integrations
APPROVED

Ankita
5/8/2019 2:32:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 01:11:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

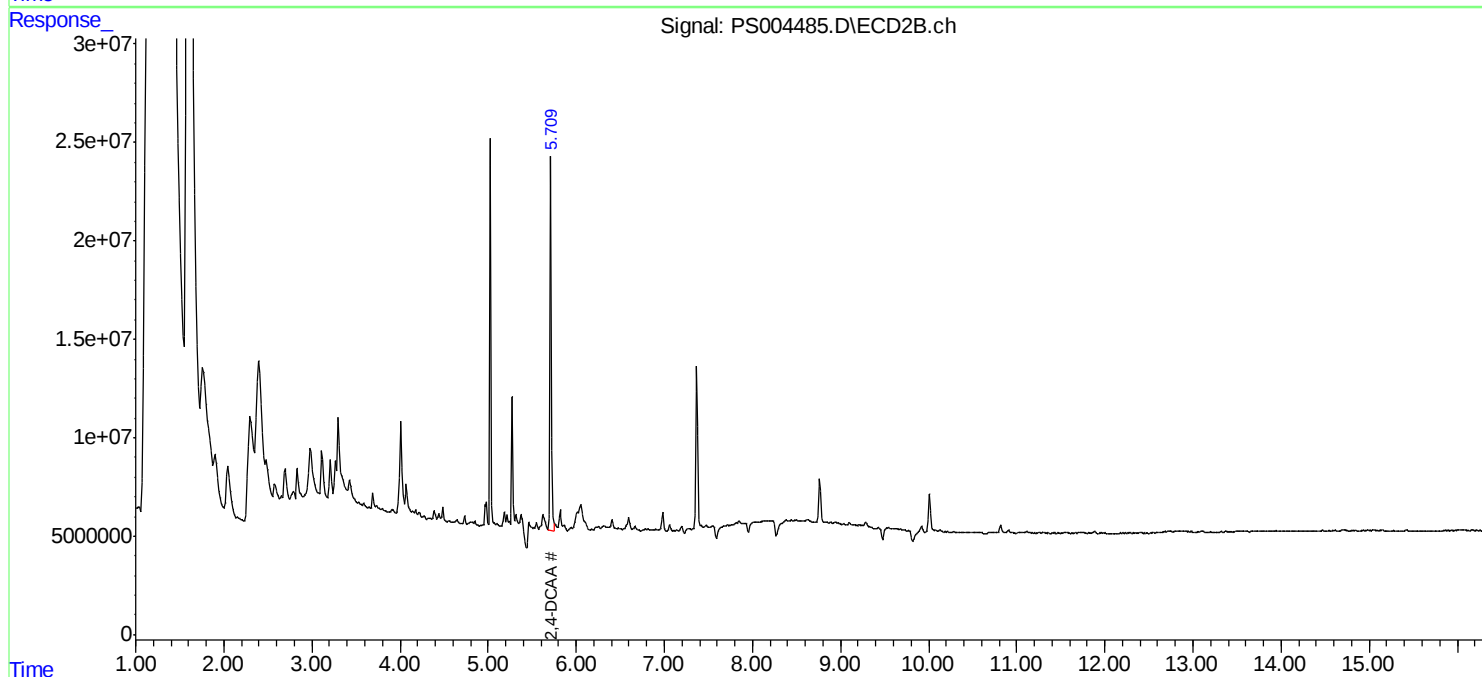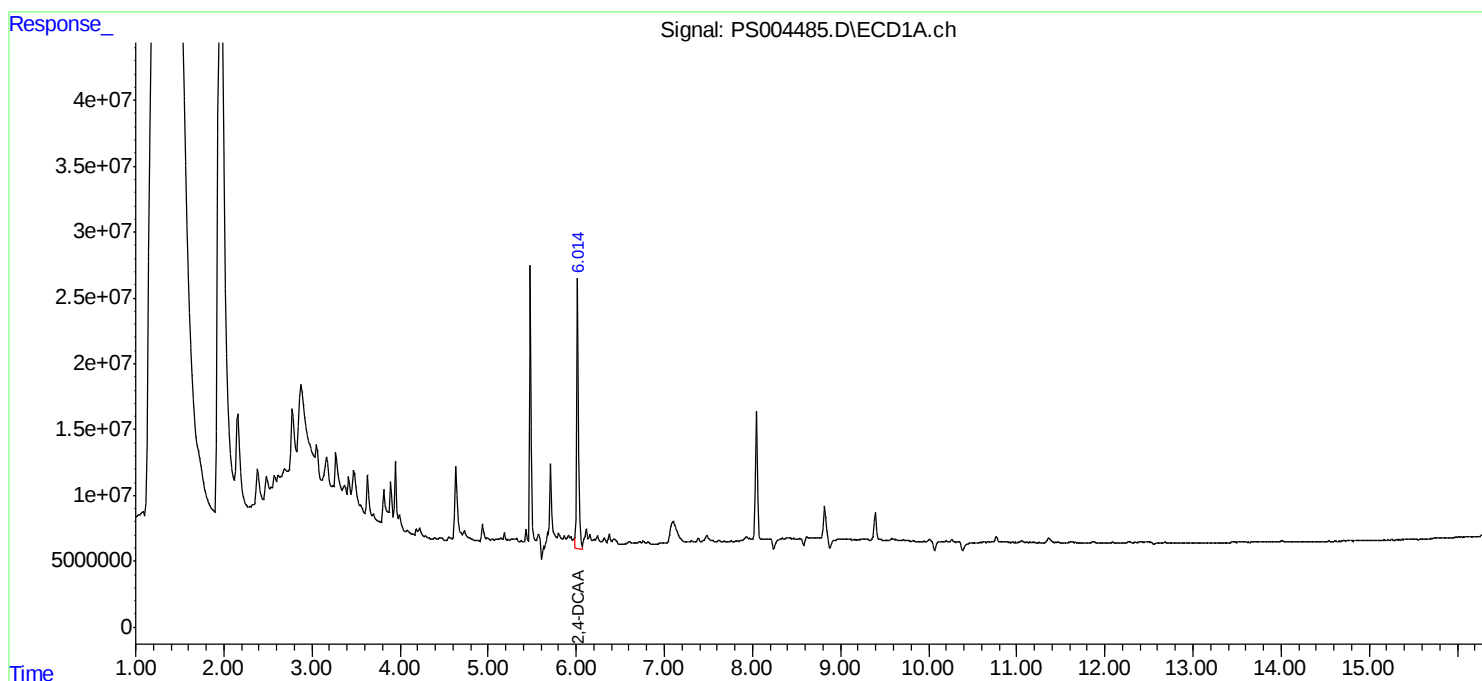

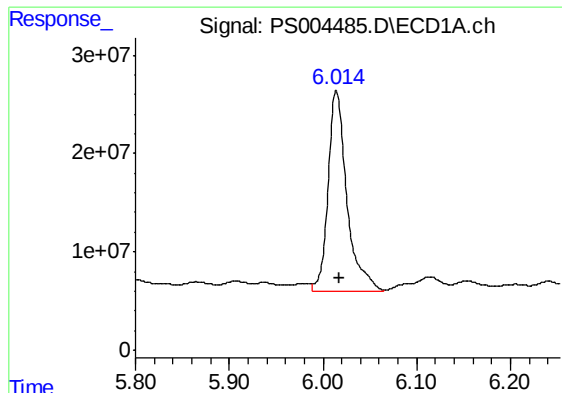


#4 2,4-DCAA

R.T.: 6.014 min
Delta R.T.: -0.004 min
Response: 285262504
Conc: 453.19 ng/ml m

Instrument :
ECD_S
ClientSampleId :
NB-08-050319-A

Manual Integrations
APPROVED

Ankita
5/8/2019 2:32:24 PM

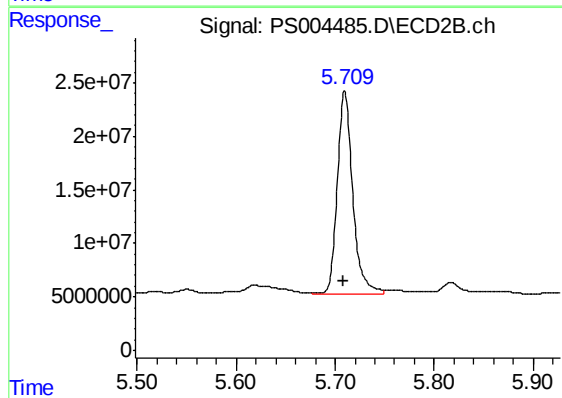

#4 2,4-DCAA

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 204534569
Conc: 424.10 ng/ml m