

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050721\
 Data File : PS014944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 13:25
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 16:03:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.888	752.6E6	270.1E6	494.762	580.288
Target Compounds							
5) T	DICAMBA	0.000	7.056	0	4700903	N.D.	2.324
9) T	2,4-D	8.319f	0.000	5476570	0	3.444	N.D. #
10) T	Pentachlo...	8.580	8.408	8261070	3160522	<MDL	<MDL #
12) T	2,4,5-T	9.408	0.000	14812268	0	1.801	N.D. #
14) T	DINOSEB	11.095	0.000	16006029	0	2.484	N.D. #
15) T	Picloram	0.000	10.901f	0	3666569	N.D.	<MDL
16) T	DCPA	11.362	10.901	8755312	3666569	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050721\
Data File : PS014944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 13:25
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 16:03:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

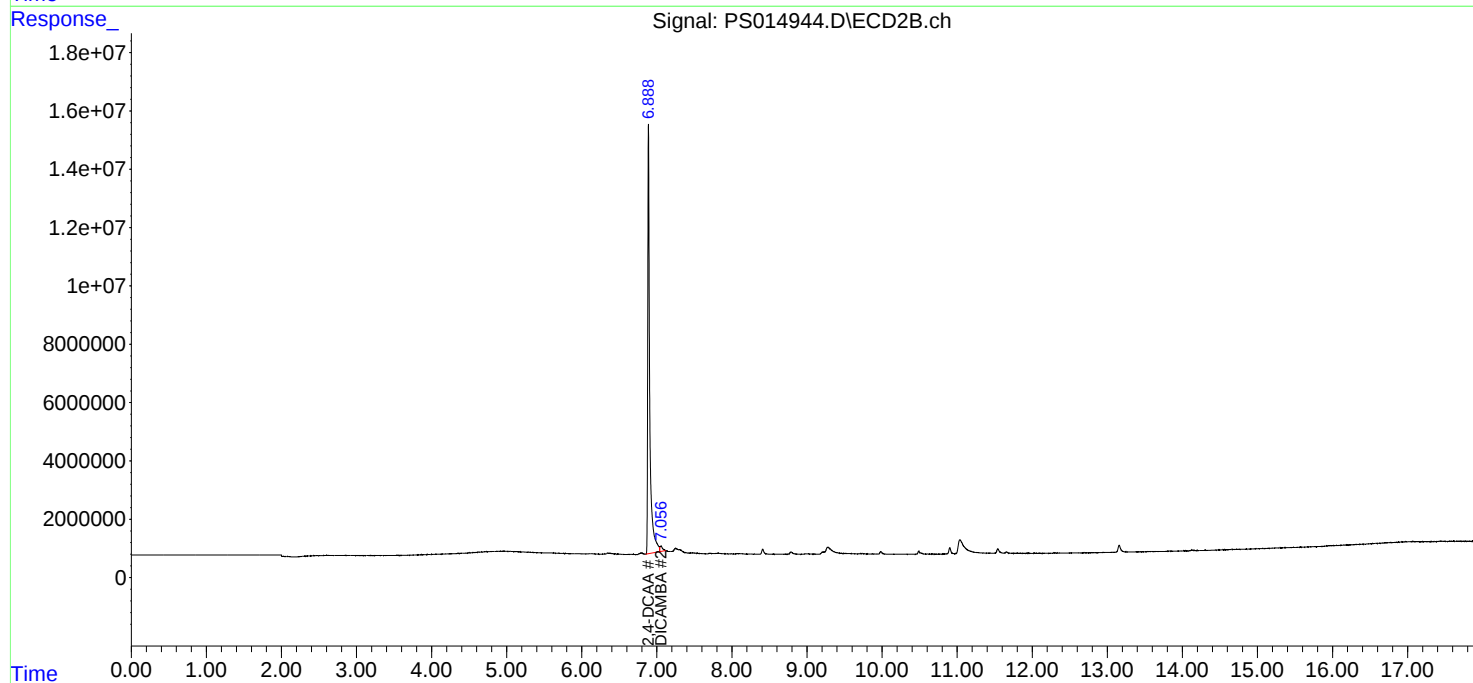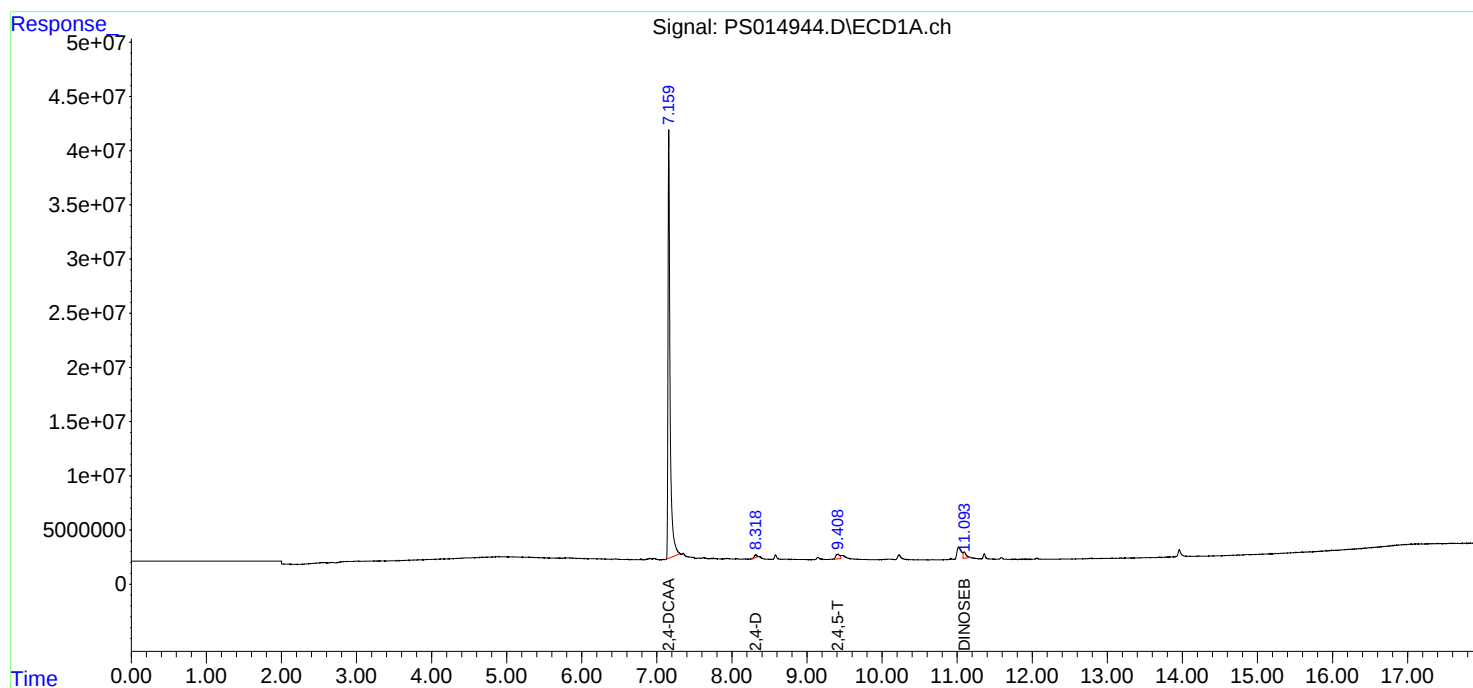


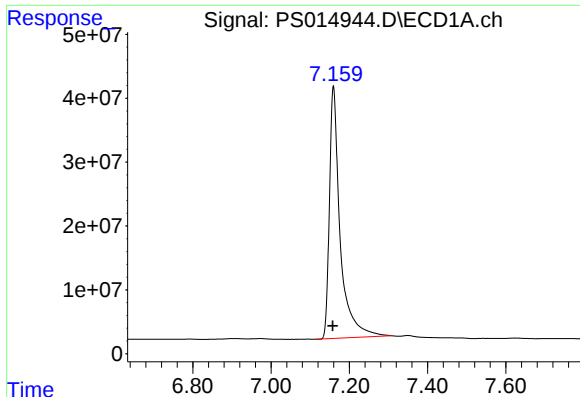

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.002 min
Response: 752629146
Conc: 494.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

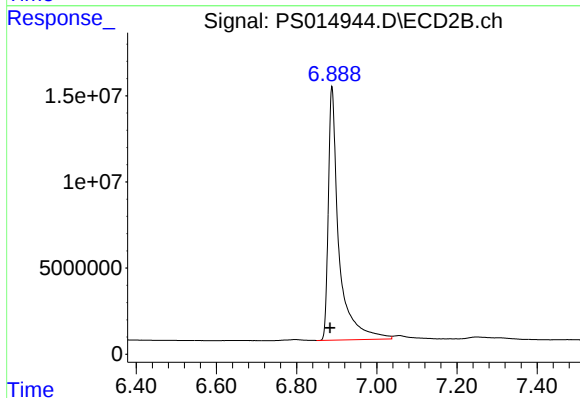


#4 2,4-DCAA

R.T.: 6.888 min
Delta R.T.: 0.005 min
Response: 270097954
Conc: 580.29 ng/ml

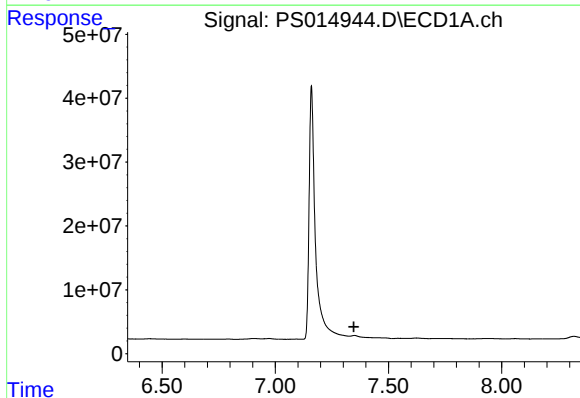


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.347 min
Response: 0
Conc: N.D.

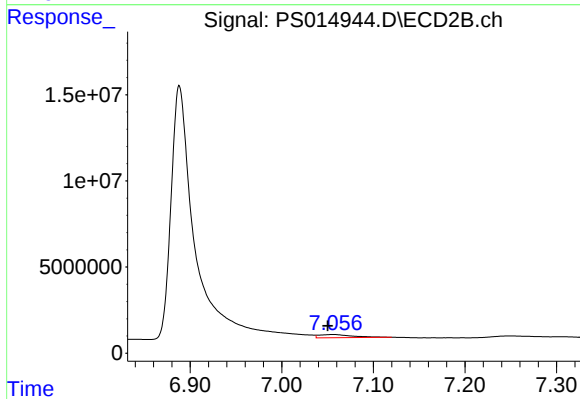

#5 DICAMBA


R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 4700903
Conc: 2.32 ng/ml

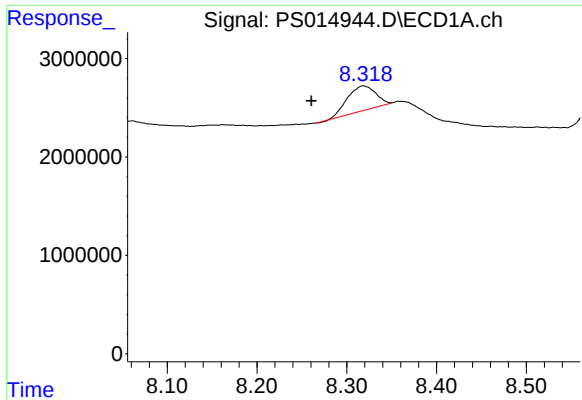

#9 2,4-D


R.T.: 8.319 min
Delta R.T.: 0.058 min
Response: 5476570
Conc: 3.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

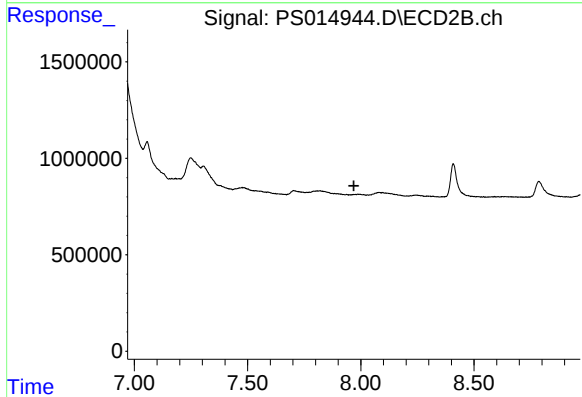


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.970 min
Response: 0
Conc: N.D.

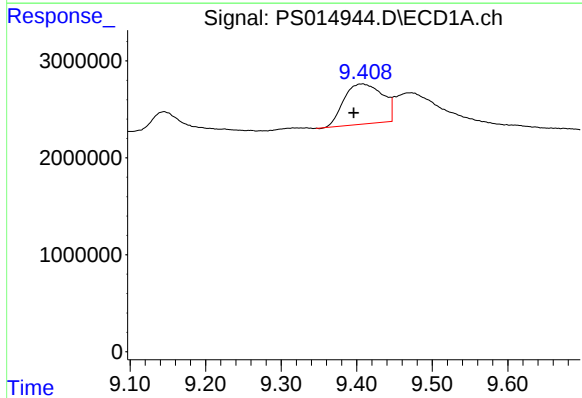


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: 0.012 min
Response: 14812268
Conc: 1.80 ng/ml

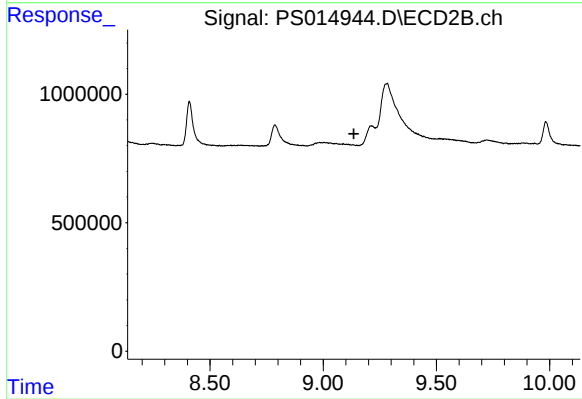

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.135 min
Response: 0
Conc: N.D.

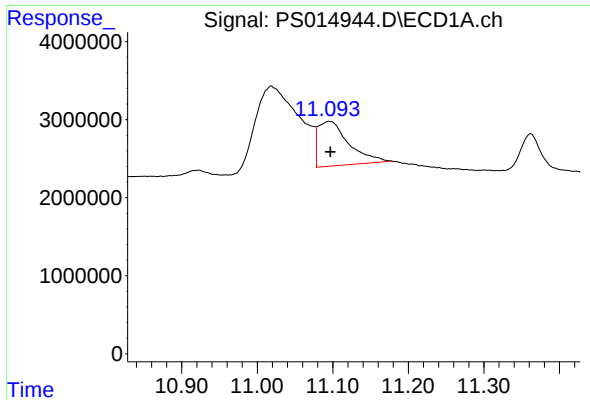

#14 DINOSEB

R.T.: 11.095 min
Delta R.T.: -0.002 min
Response: 16006029
Conc: 2.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

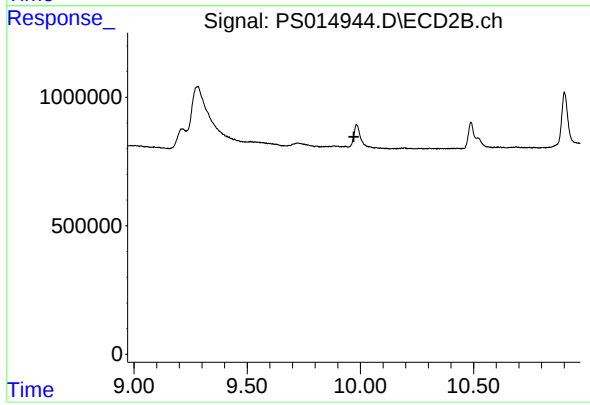

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.