

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050823\
 Data File : PS022945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2023 12:01
 Operator : AR\AJ
 Sample : 02588-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ZONE-A-0-3-05022023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/09/2023
 Supervised By :Ankita Jodhani 05/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 15:38:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.483	6.857	952.3E6	338.0E6	382.494	331.762m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050823\
Data File : PS022945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2023 12:01
Operator : AR\AJ
Sample : 02588-07
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
ZONE-A-0-3-05022023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/09/2023
Supervised By : Ankita Jodhani 05/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 15:38:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

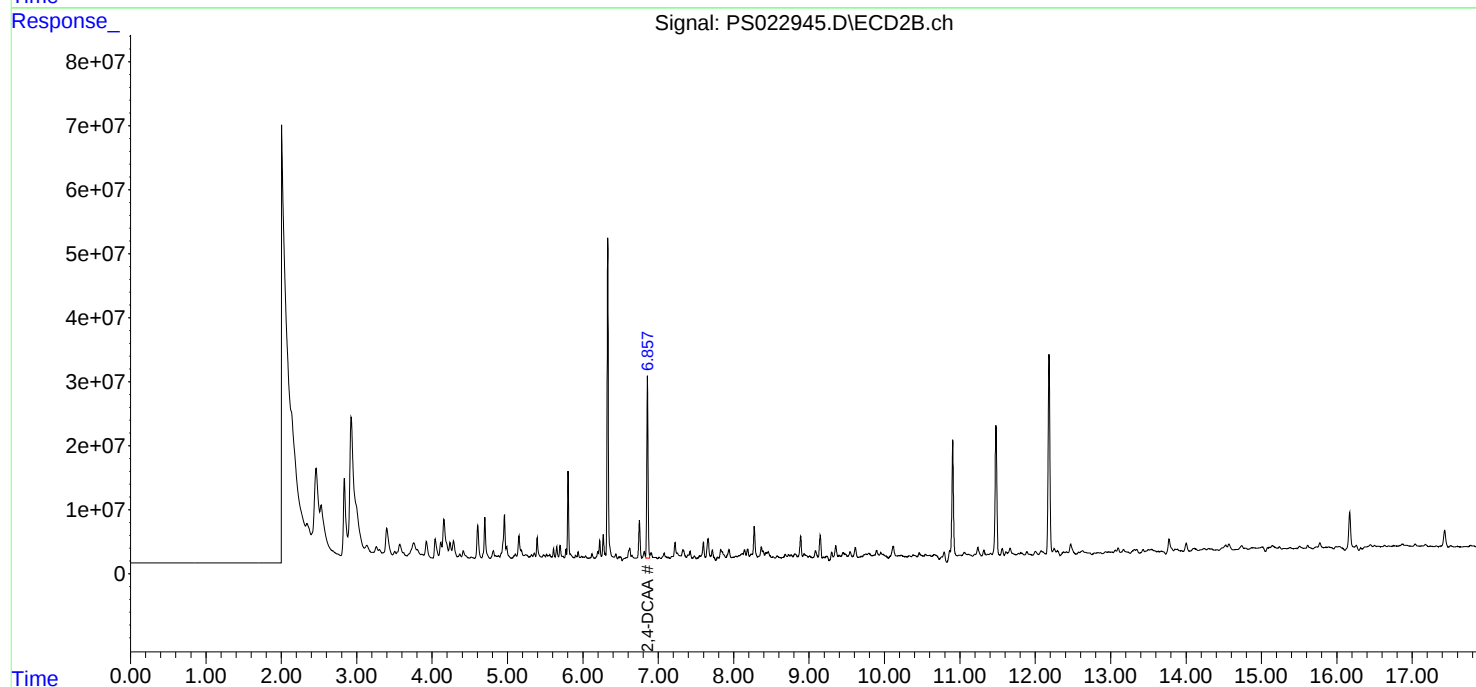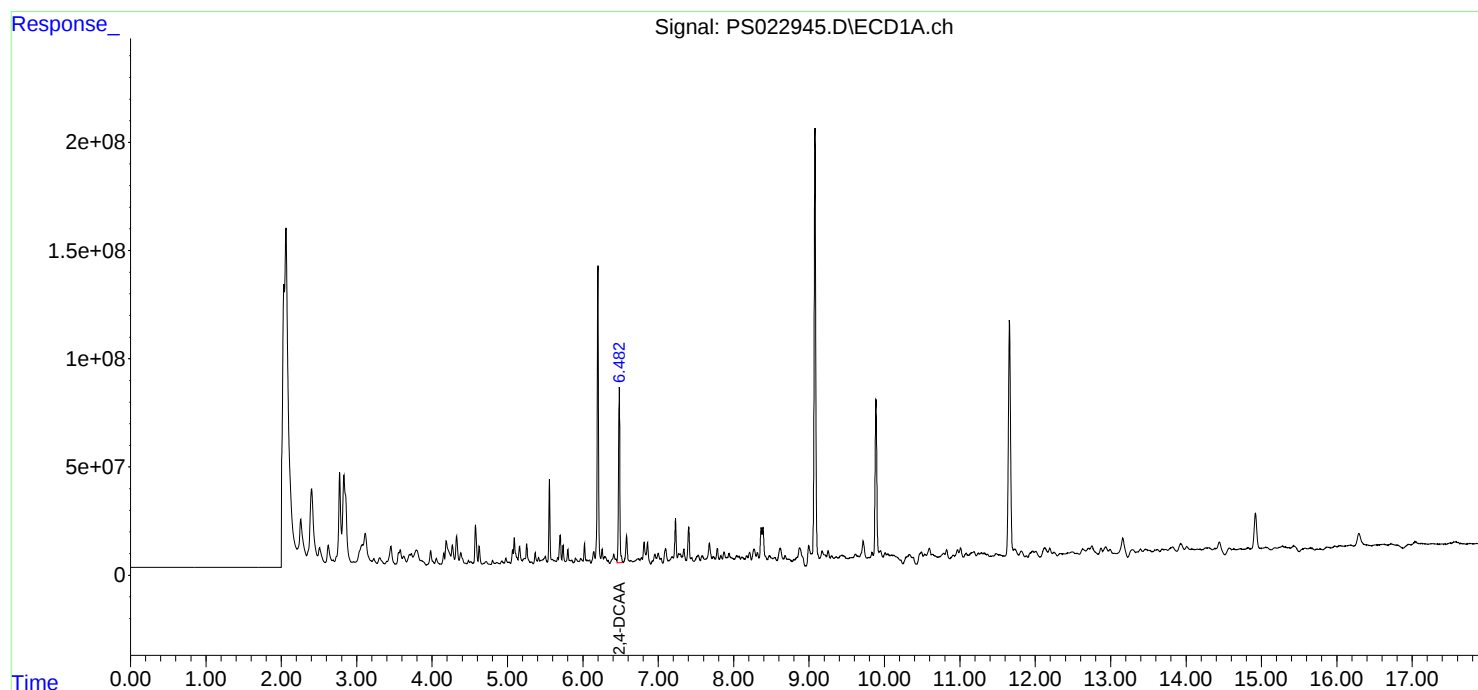

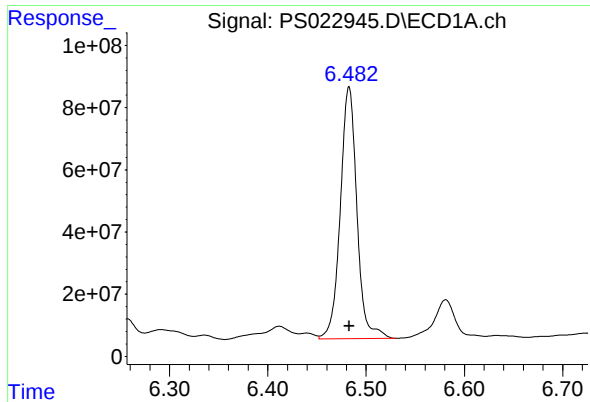


#4 2,4-DCAA

R.T.: 6.483 min
Delta R.T.: 0.000 min
Response: 952296138
Conc: 382.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
ZONE-A-0-3-05022023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/09/2023
Supervised By :Ankita Jodhani 05/09/2023

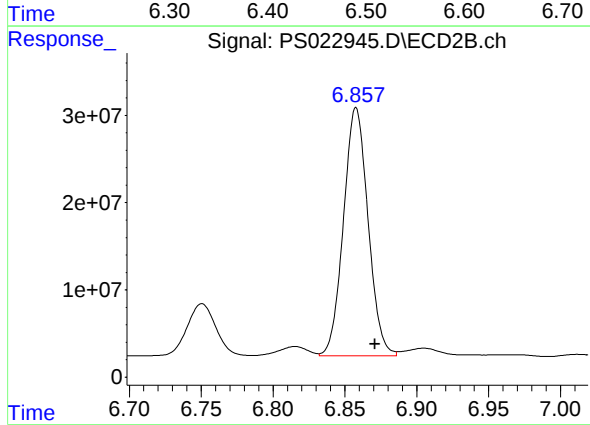

#4 2,4-DCAA

R.T.: 6.857 min
Delta R.T.: -0.014 min
Response: 338047020
Conc: 331.76 ng/ml m