

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050920\
 Data File : PS010195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2020 14:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 00:57:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050520.M
 Quant Title : 8080.M
 QLast Update : Tue May 05 13:43:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.921	297.8E6	263.1E6	440.337	510.250
Target Compounds							
8) T	DICHLORPROP	0.000	7.745	0	2223936	N.D.	4.225



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050920\
Data File : PS010195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2020 14:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 00:57:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050520.M
Quant Title : 8080.M
QLast Update : Tue May 05 13:43:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

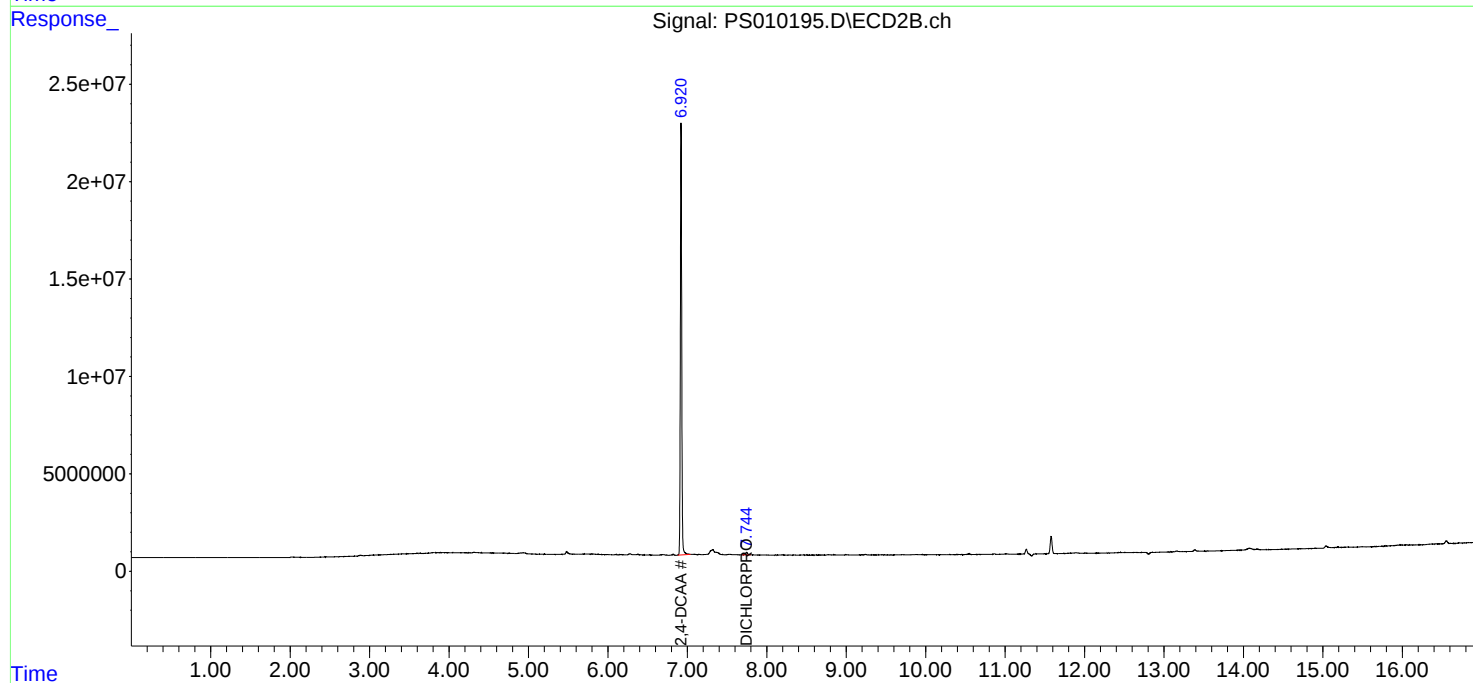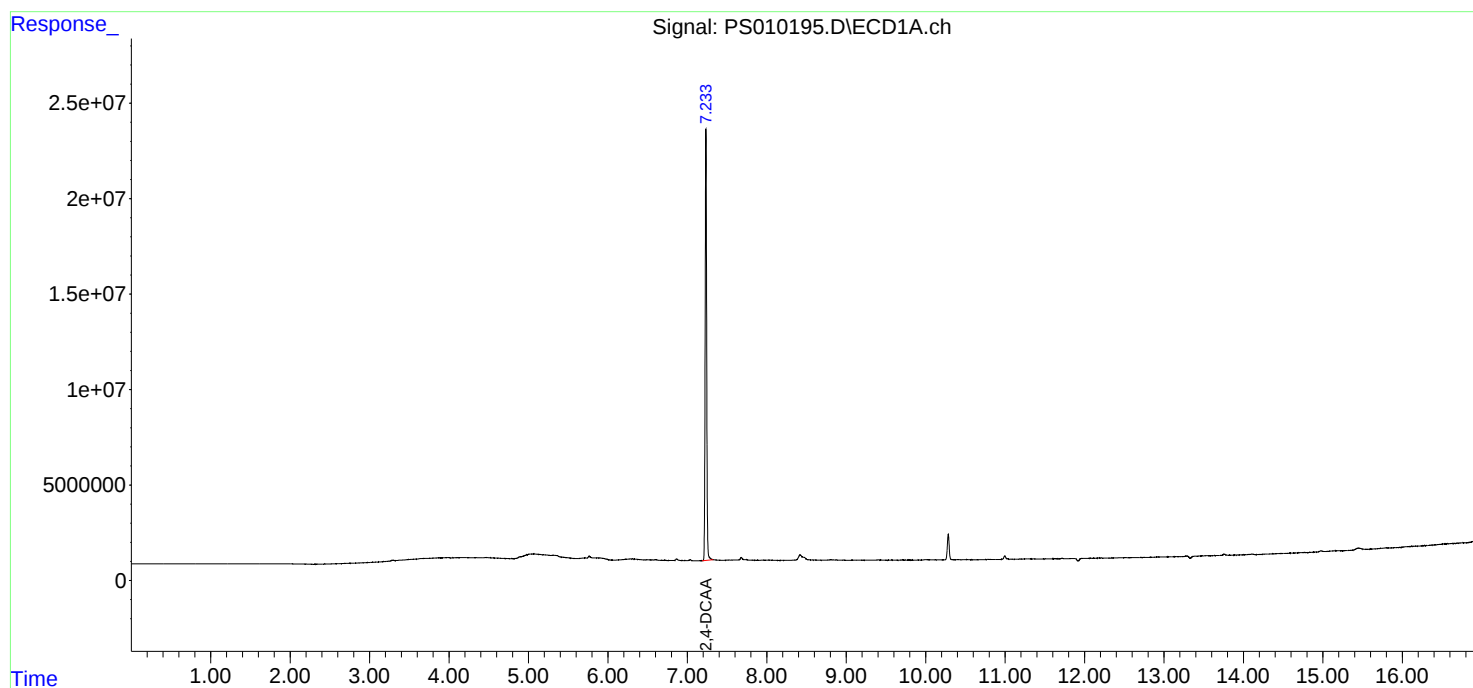


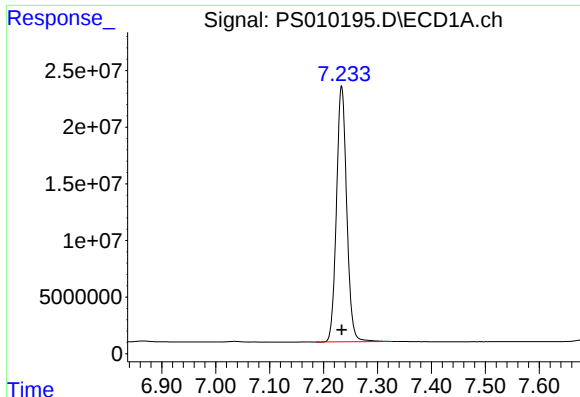

#4 2,4-DCAA


R.T.: 7.233 min
Delta R.T.: 0.000 min
Response: 297838273
Conc: 440.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

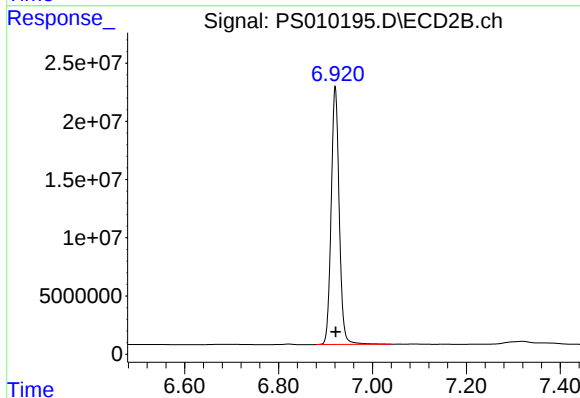


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 263081371
Conc: 510.25 ng/ml

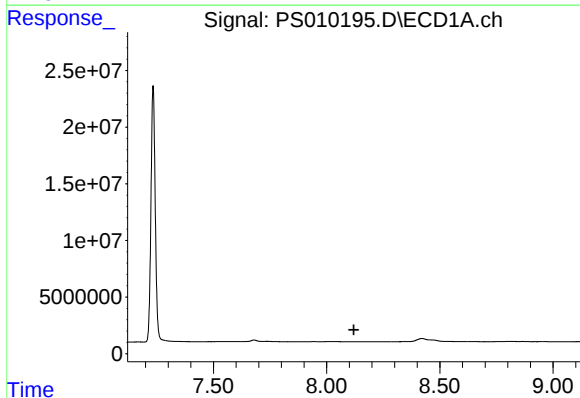

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.120 min
Response: 0
Conc: N.D.

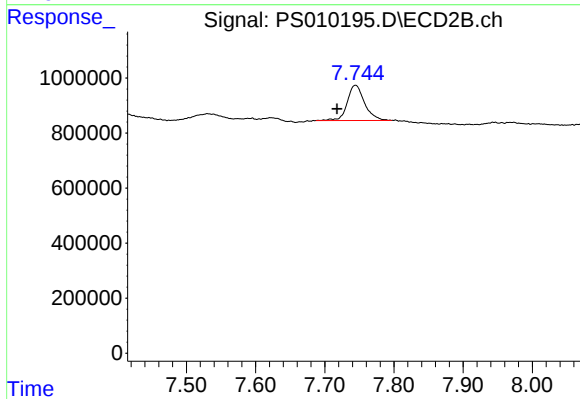

#8 DICHLORPROP

R.T.: 7.745 min
Delta R.T.: 0.027 min
Response: 2223936
Conc: 4.23 ng/ml