

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050922\
 Data File : PS019349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2022 16:34
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:09:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.226	6.797	2771357	698477	1.015	<MDL	#
Target Compounds								
1) T	Dalapon	3.076f	0.000	17487	0	<MDL	N.D.	#
2) T	3,5-DICHL...	6.434	5.977	649358	518068	<MDL	<MDL	#
5) T	DICAMBA	7.414	6.962	2748087	1014337	<MDL	<MDL	#
6) T	MCP	0.000	7.023f	0	2463337	N.D.	<MDL	#
8) T	DICHLORPROP	8.111	7.611	520761	5138418	<MDL	5.996	#
10) T	Pentachlo...	8.651	8.306	6298682	1558779	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.204	8.668	3167856	1389357	<MDL	<MDL	#
12) T	2,4,5-T	9.494	9.051	7757676	1683083	<MDL	<MDL	#
13) T	2,4-DB	10.074f	9.569	2391706	531071	<MDL	<MDL	#
14) T	DINOSEB	11.199	9.879	4450055	913808	<MDL	<MDL	#
15) T	Picloram	11.039	10.876	82748481	52021110	2.831	8.698	#
16) T	DCPA	11.466	10.812	6334017	19613978	<MDL	3.341	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050922\
Data File : PS019349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2022 16:34
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:09:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

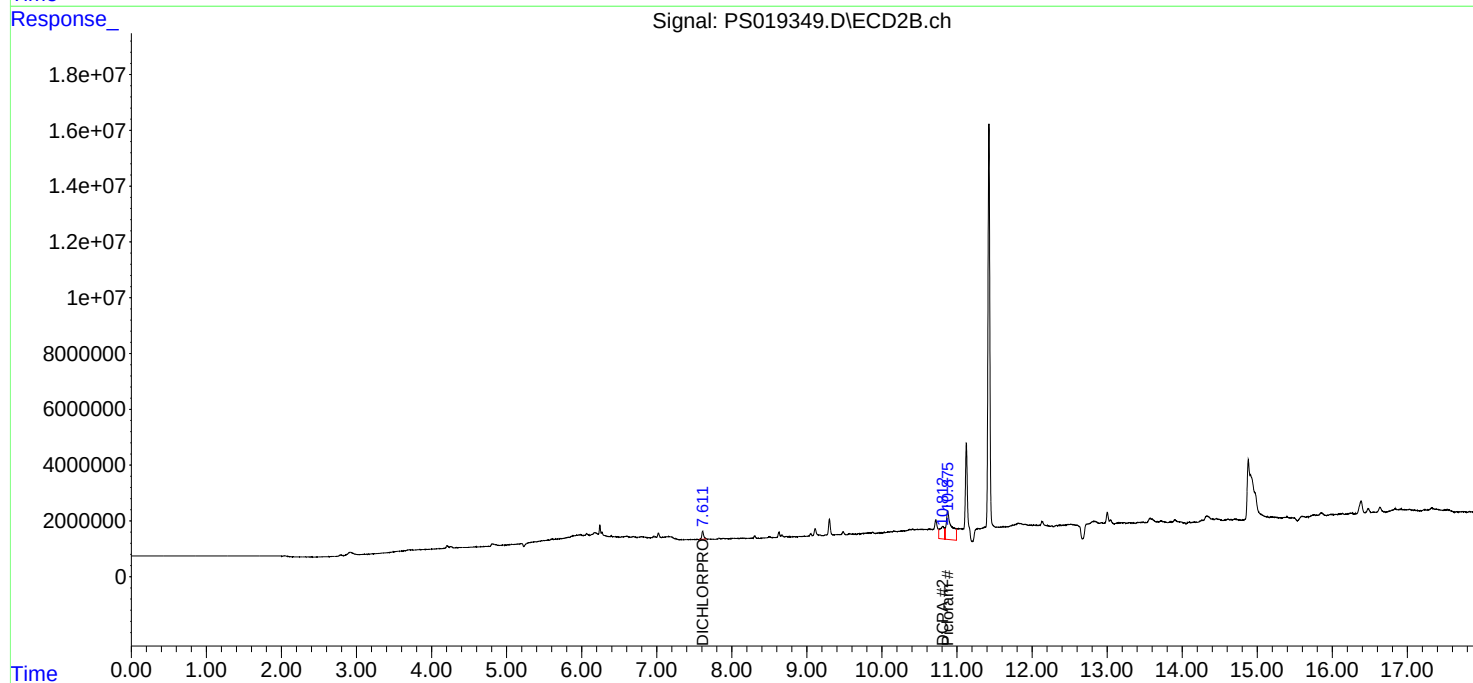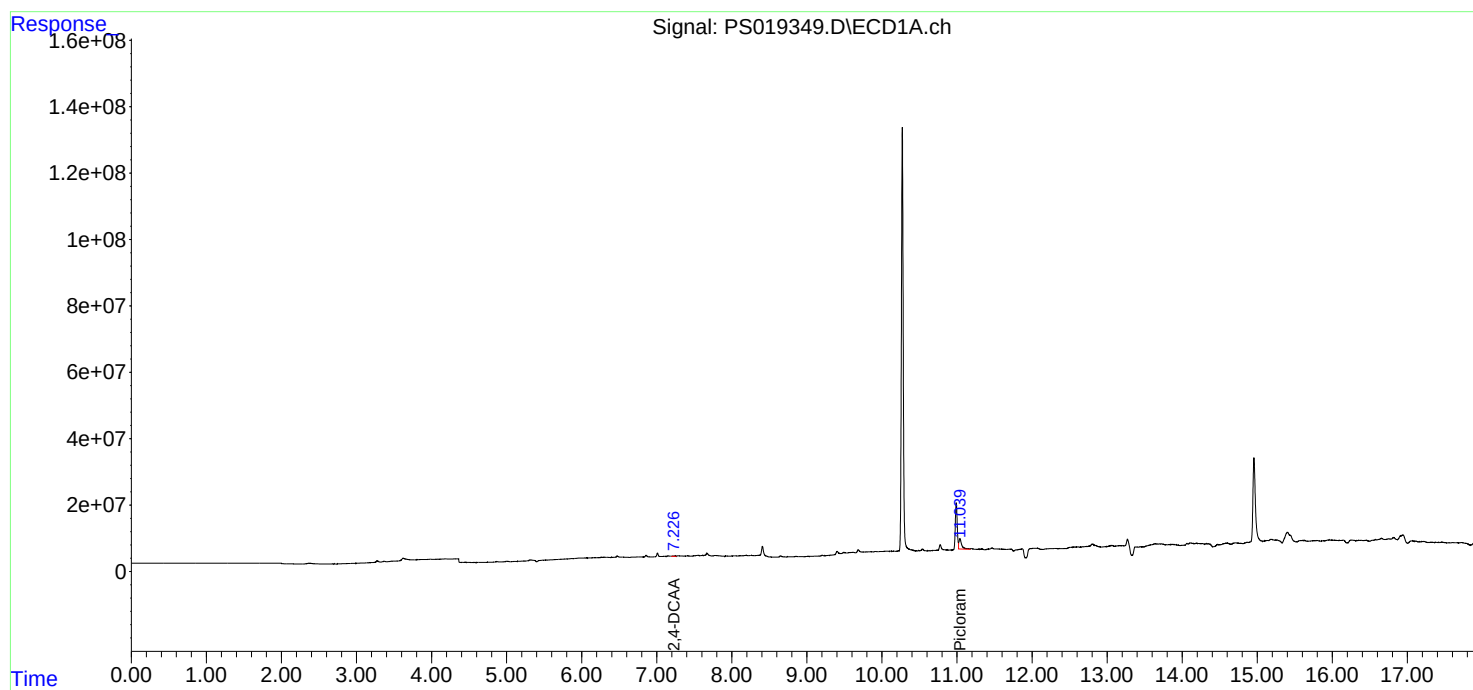


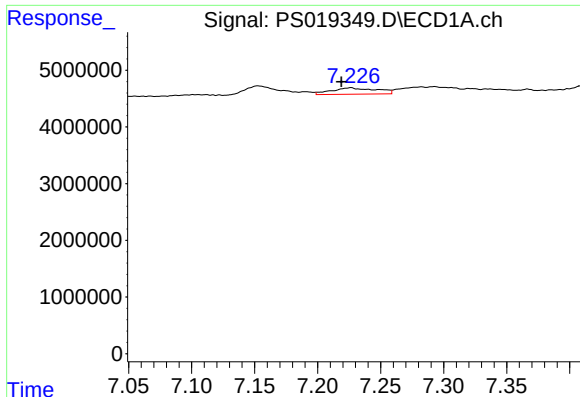

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.007 min
Response: 2771357
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

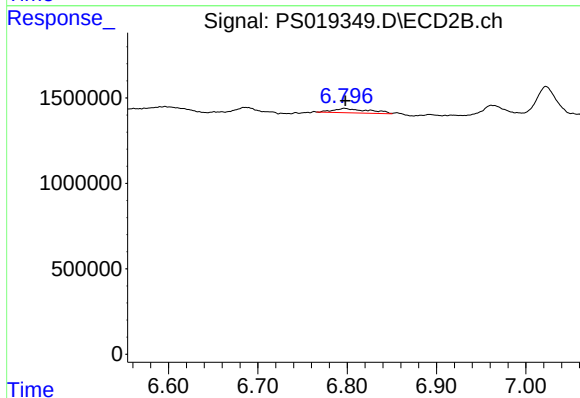


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.001 min
Response: 698477
Conc: N.D.

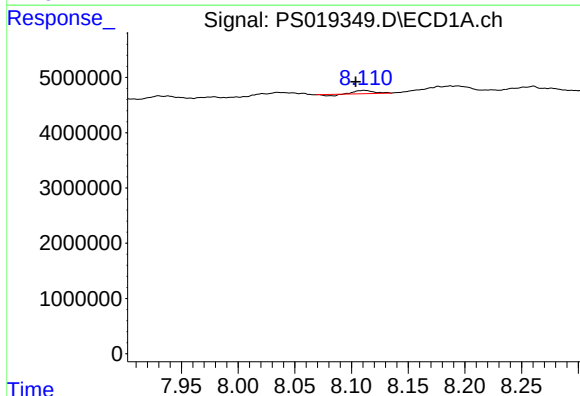


#8 DICHLORPROP

R.T.: 8.111 min
Delta R.T.: 0.007 min
Response: 520761
Conc: N.D.

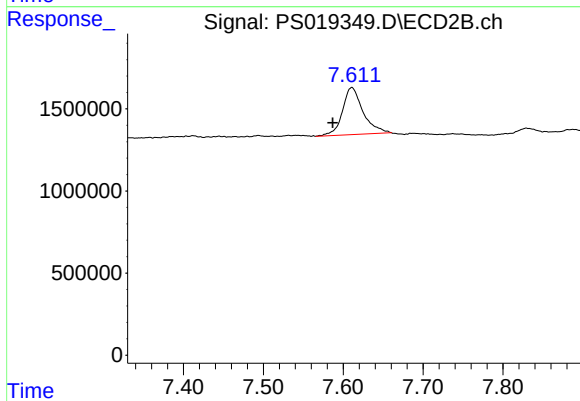

#8 DICHLORPROP


R.T.: 7.611 min
Delta R.T.: 0.024 min
Response: 5138418
Conc: 6.00 ng/ml

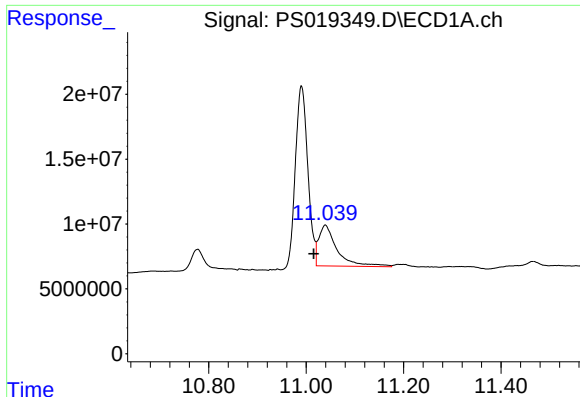

#15 Picloram


R.T.: 11.039 min
Delta R.T.: 0.024 min
Response: 82748481
Conc: 2.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

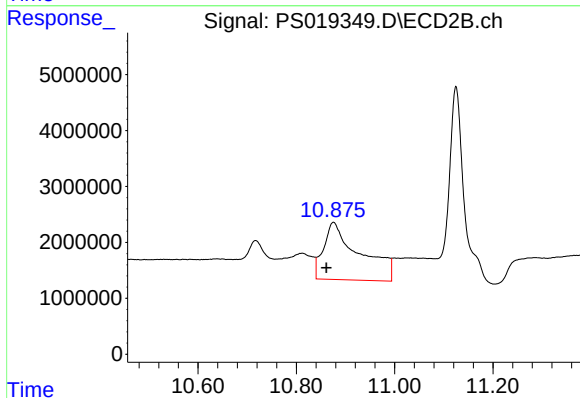


#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.014 min
Response: 52021110
Conc: 8.70 ng/ml

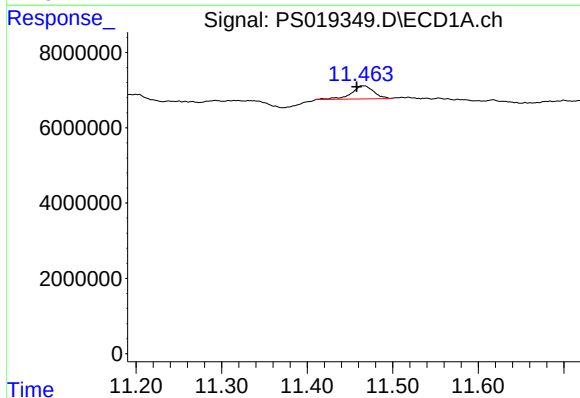

#16 DCPA

R.T.: 11.466 min
Delta R.T.: 0.008 min
Response: 6334017
Conc: N.D.

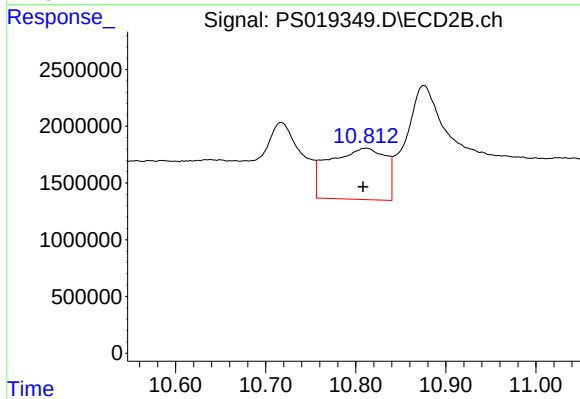

#16 DCPA

R.T.: 10.812 min
Delta R.T.: 0.004 min
Response: 19613978
Conc: 3.34 ng/ml