

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050922\
 Data File : PS019362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2022 22:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:13:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.800	1180.8E6	379.7E6	432.383	490.180
Target Compounds							
1) T	Dalapon	3.024	0.000	142381	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.368f	0.000	413499	0	<MDL	N.D. #
3) T	4-Nitroph...	7.029	0.000	2203831	0	2.274	N.D. #
10) T	Pentachlo...	8.650	8.311	1613739	1743550	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.653	0	1925993	N.D.	<MDL
12) T	2,4,5-T	9.532f	9.086f	8574932	-609246	<MDL	N.D. #
13) T	2,4-DB	10.079f	9.505f	234022	2292429	<MDL	4.032 #
14) T	DINOSEB	11.187	9.890	33189744	645943	2.010	<MDL #
15) T	Picloram	11.033	10.812f	1350808	1141633	<MDL	<MDL #
16) T	DCPA	11.463	10.812	2478439	1141633	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050922\
Data File : PS019362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2022 22:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:13:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

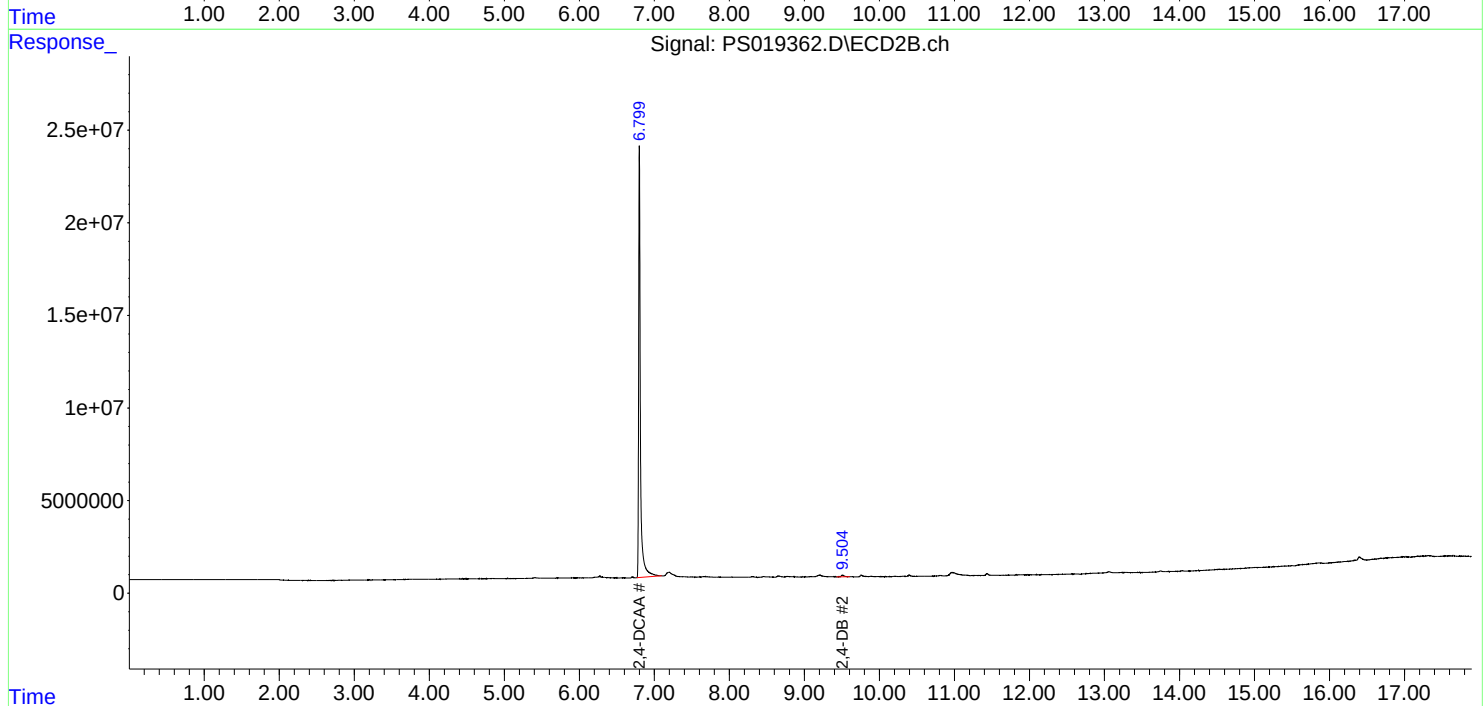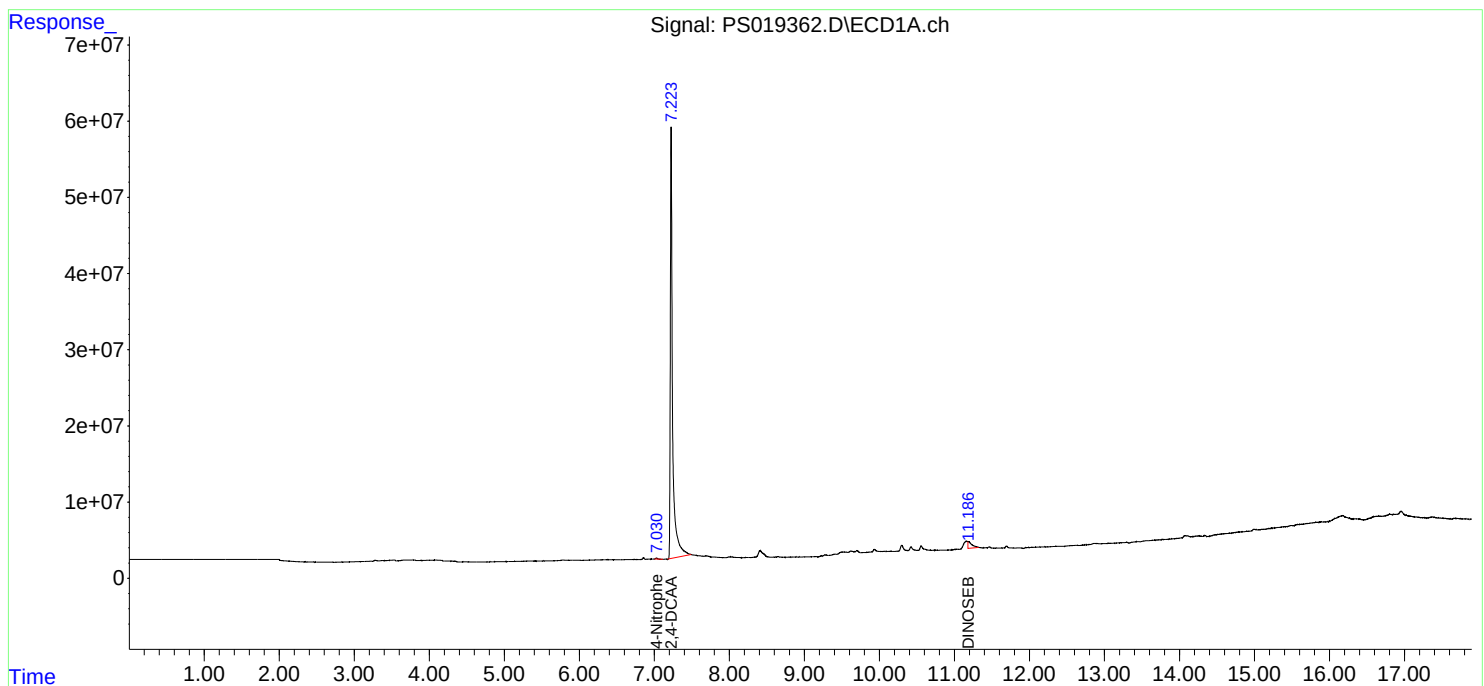


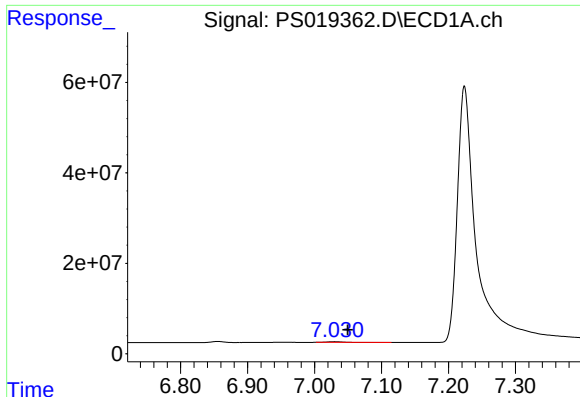

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.020 min
Response: 2203831
Conc: 2.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

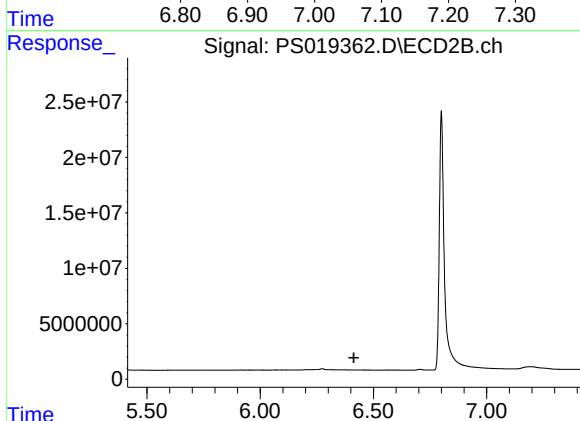


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

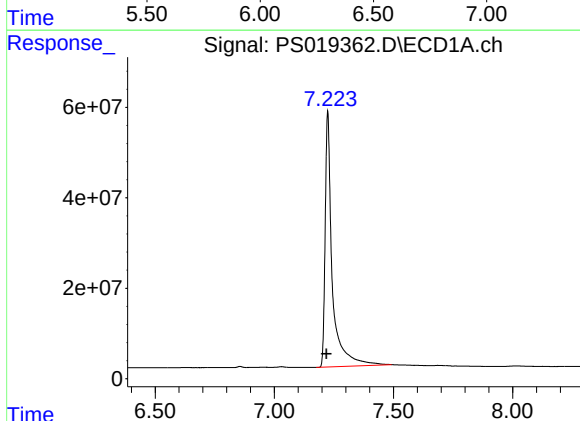


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: 0.005 min
Response: 1180784114
Conc: 432.38 ng/ml

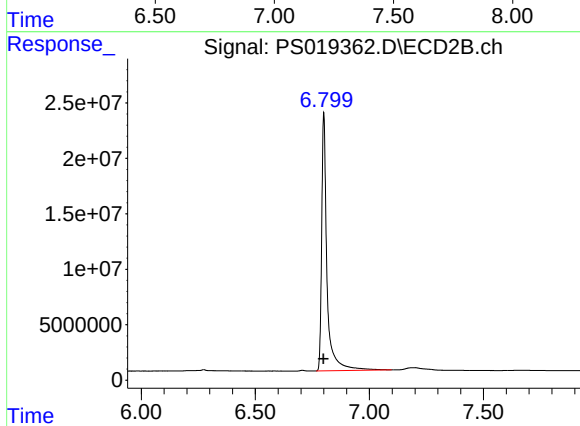

#4 2,4-DCAA


R.T.: 6.800 min
Delta R.T.: 0.002 min
Response: 379671905
Conc: 490.18 ng/ml

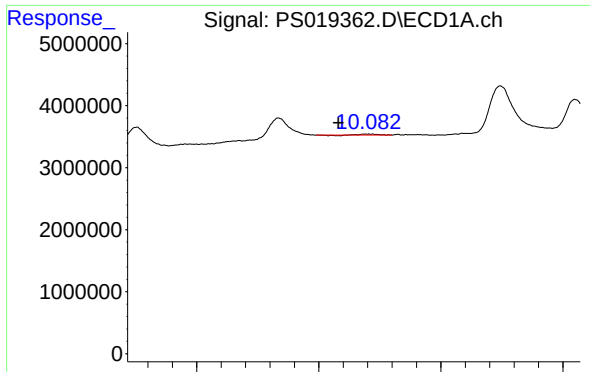

#13 2,4-DB


R.T.: 10.079 min
Delta R.T.: 0.047 min
Response: 234022
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

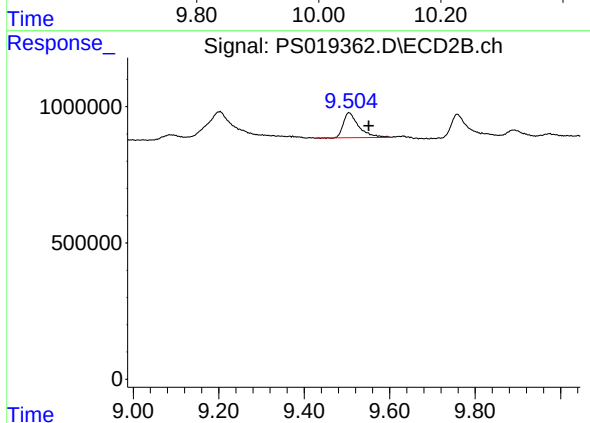


#13 2,4-DB

R.T.: 9.505 min
Delta R.T.: -0.046 min
Response: 2292429
Conc: 4.03 ng/ml

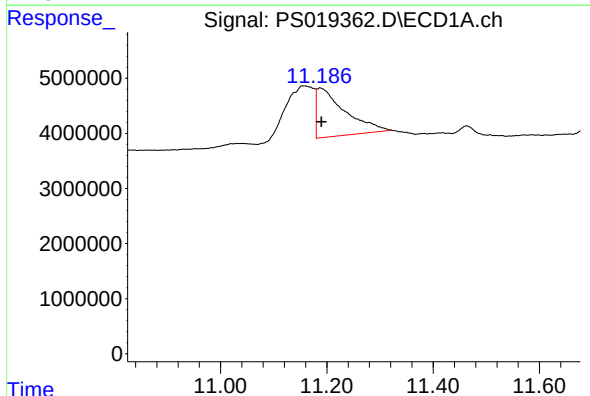

#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.002 min
Response: 33189744
Conc: 2.01 ng/ml

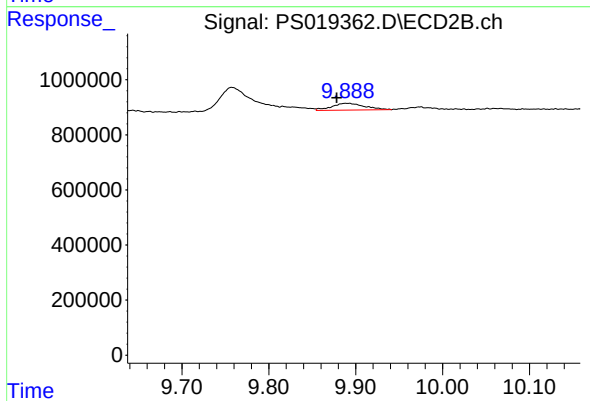

#14 DINOSEB

R.T.: 9.890 min
Delta R.T.: 0.012 min
Response: 645943
Conc: N.D.