

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050922\
 Data File : PS019363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2022 22:56
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:13:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	2122.4E6	577.4E6	777.178	745.499
Target Compounds							
1) T	Dalapon	3.027	2.534	3230.8E6	635.6E6	669.221	715.004
2) T	3,5-DICHL...	6.430	5.975	2411.0E6	836.6E6	682.097	717.380
3) T	4-Nitroph...	7.054	6.416	801.9E6	262.8E6	827.471	744.742
5) T	DICAMBA	7.410	6.964	7541.1E6	2454.5E6	682.804	732.501
6) T	MCPD	7.581	7.062	616.9E6	194.3E6	69.013	73.076
7) T	MCPA	7.730	7.276	849.5E6	270.2E6	68.160	72.543
8) T	DICHLORPROP	8.103	7.586	1887.3E6	621.7E6	674.621	725.470
9) T	2,4-D	8.334	7.879	2223.8E6	739.5E6	704.883	740.555
10) T	Pentachlo...	8.642	8.306	26914.5E6	8159.3E6	685.080	725.824
11) T	2,4,5-TP ...	9.193	8.667	12076.6E6	3570.9E6	668.132	741.990
12) T	2,4,5-T	9.480	9.046	14172.9E6	3298.1E6	670.079	761.679
13) T	2,4-DB	10.034	9.552	2966.5E6	425.0E6	691.781	747.413
14) T	DINOSEB	11.188	9.878	11156.1E6	2303.4E6	675.664	794.846
15) T	Picloram	11.024	10.867	21036.4E6	4497.5E6	719.683	751.989
16) T	DCPA	11.457	10.808	17436.4E6	4337.6E6	666.248	738.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050922\
Data File : PS019363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2022 22:56
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:13:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

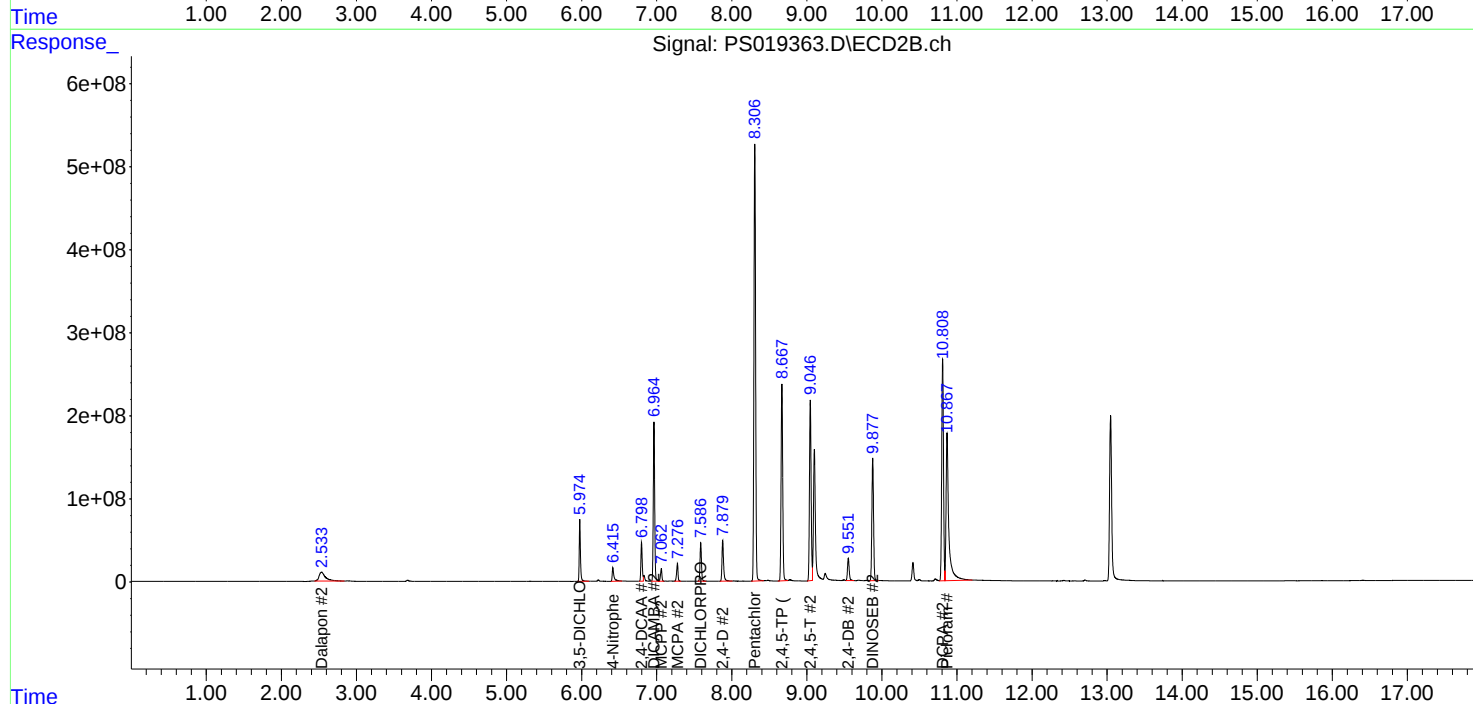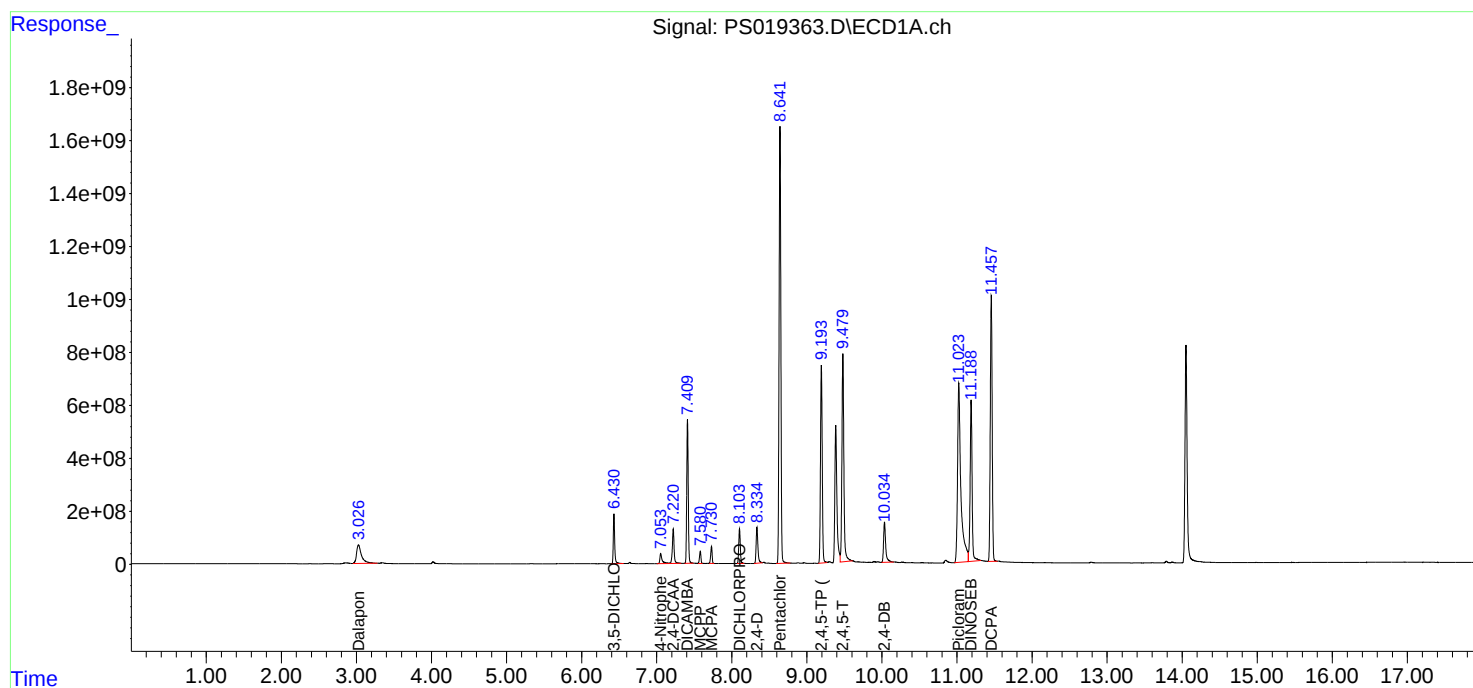


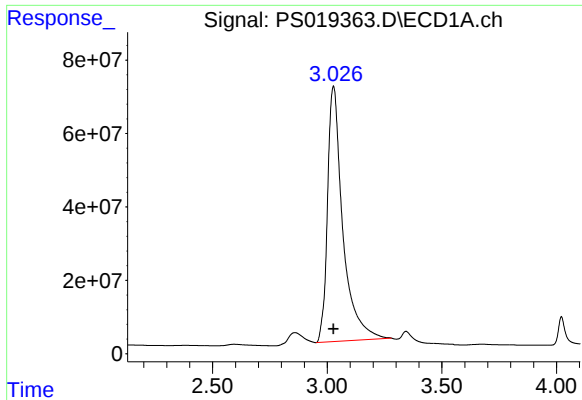

#1 Dalapon


R.T.: 3.027 min
Delta R.T.: 0.000 min
Response: 3230795897
Conc: 669.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

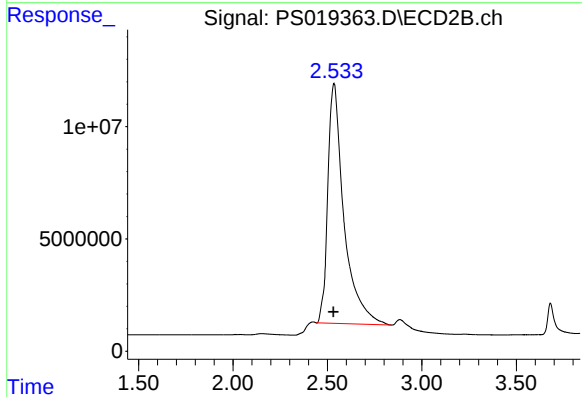


#1 Dalapon

R.T.: 2.534 min
Delta R.T.: 0.003 min
Response: 635582049
Conc: 715.00 ng/ml

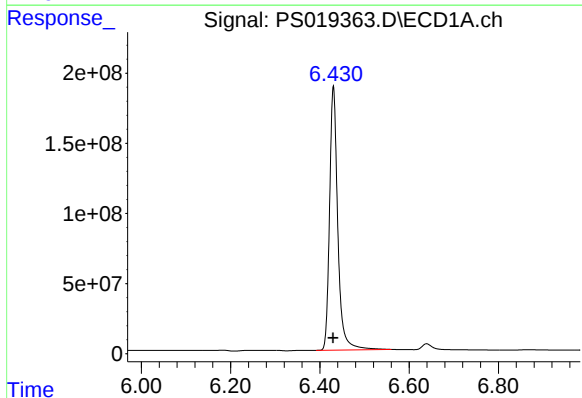


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.430 min
Delta R.T.: 0.000 min
Response: 2410995180
Conc: 682.10 ng/ml

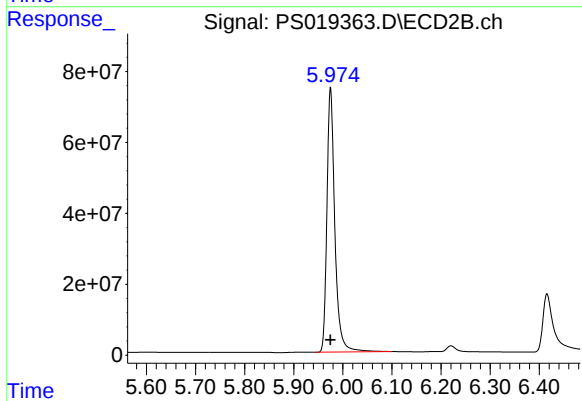

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 836640380
Conc: 717.38 ng/ml

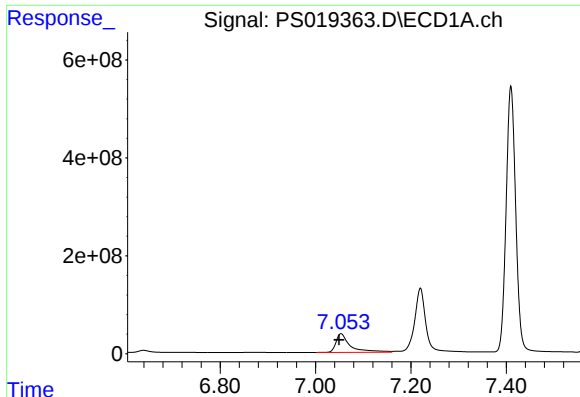

#3 4-Nitrophenol


R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 801893129
Conc: 827.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

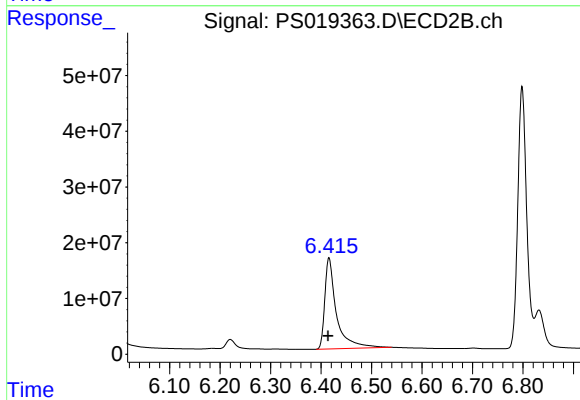


#3 4-Nitrophenol

R.T.: 6.416 min
Delta R.T.: 0.002 min
Response: 262769757
Conc: 744.74 ng/ml

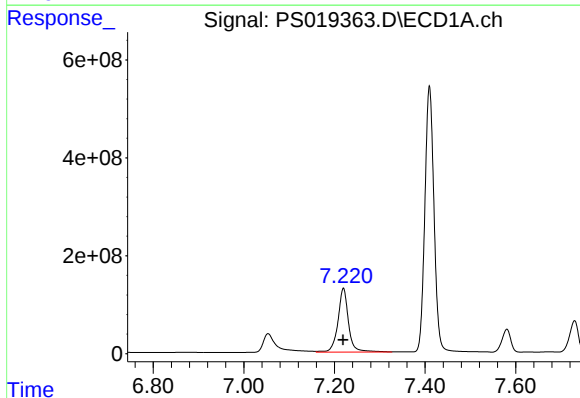


#4 2,4-DCAA

R.T.: 7.220 min
Delta R.T.: 0.001 min
Response: 2122376099
Conc: 777.18 ng/ml

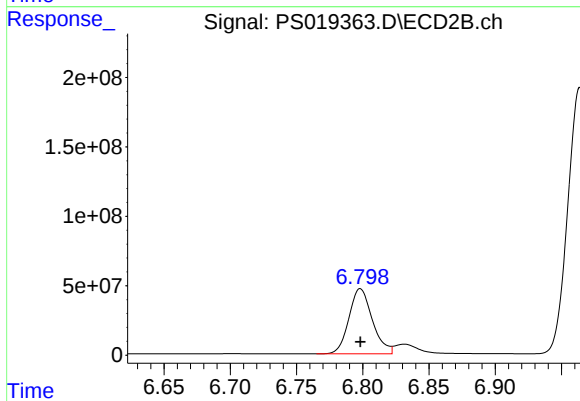

#4 2,4-DCAA


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 577430464
Conc: 745.50 ng/ml

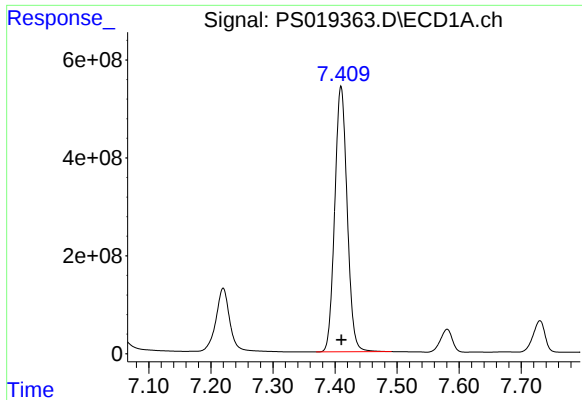

#5 DICAMBA


R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 7541093478
Conc: 682.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

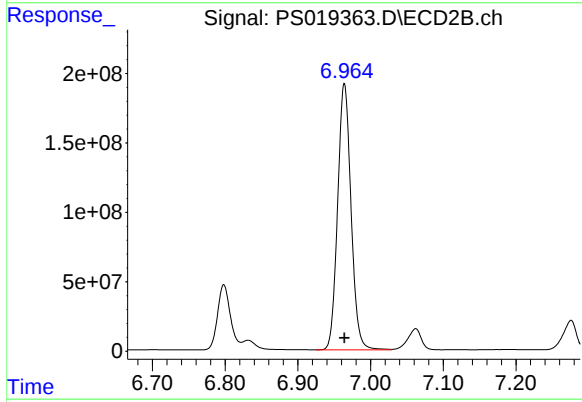


#5 DICAMBA

R.T.: 6.964 min
Delta R.T.: 0.000 min
Response: 2454475831
Conc: 732.50 ng/ml

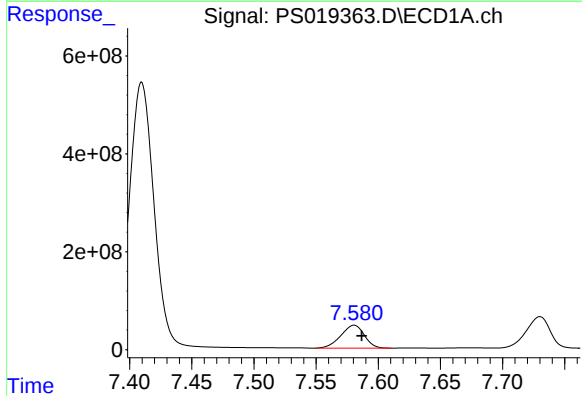


#6 MCP

R.T.: 7.581 min
Delta R.T.: -0.006 min
Response: 616923563
Conc: 69.01 ug/ml

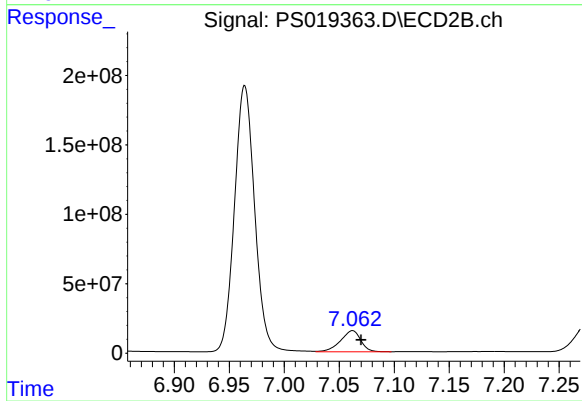

#6 MCP


R.T.: 7.062 min
Delta R.T.: -0.008 min
Response: 194334340
Conc: 73.08 ug/ml

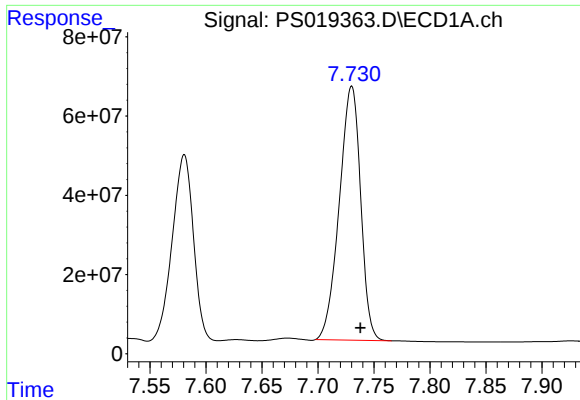

#7 MCPA


R.T.: 7.730 min
Delta R.T.: -0.008 min
Response: 849485132
Conc: 68.16 ug/ml

Instrument :
ECD_S
ClientSampleId :

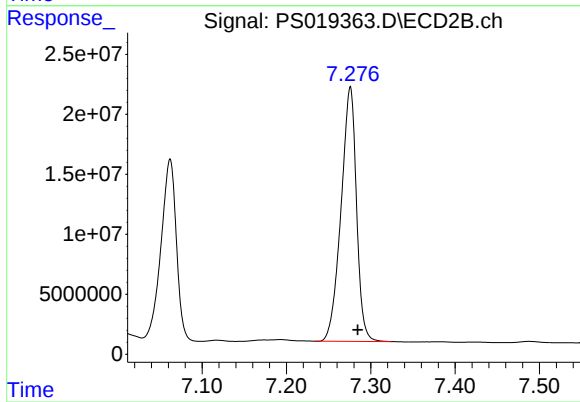


#7 MCPA

R.T.: 7.276 min
Delta R.T.: -0.009 min
Response: 270195144
Conc: 72.54 ug/ml

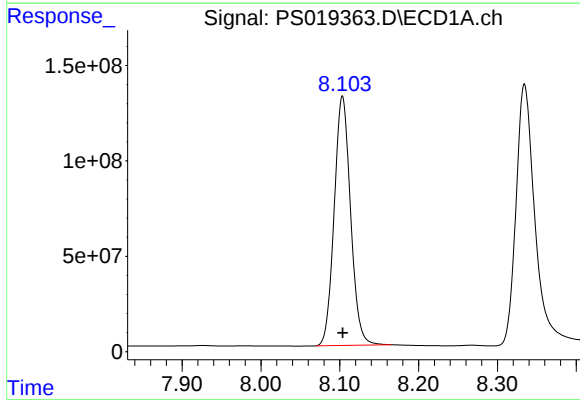


#8 DICHLORPROP

R.T.: 8.103 min
Delta R.T.: 0.000 min
Response: 1887305098
Conc: 674.62 ng/ml

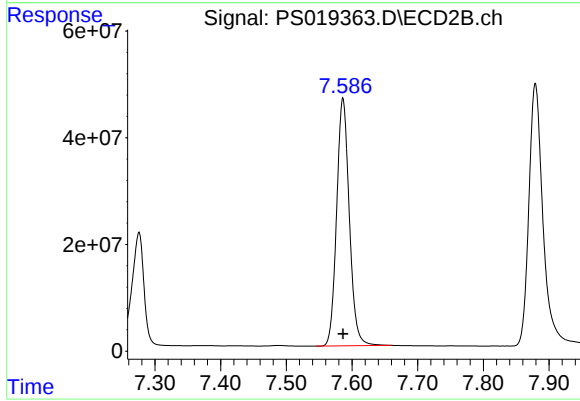

#8 DICHLORPROP


R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 621726320
Conc: 725.47 ng/ml

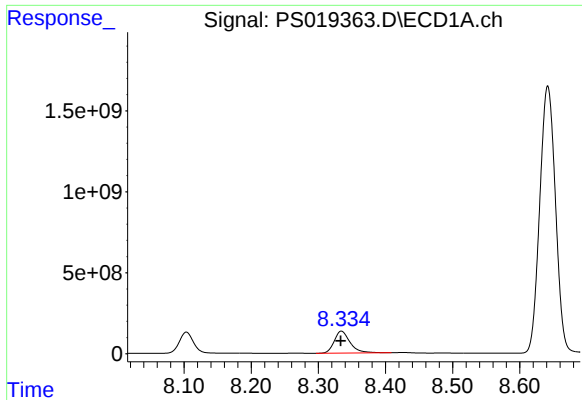

#9 2,4-D


R.T.: 8.334 min
Delta R.T.: 0.000 min
Response: 2223756321
Conc: 704.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

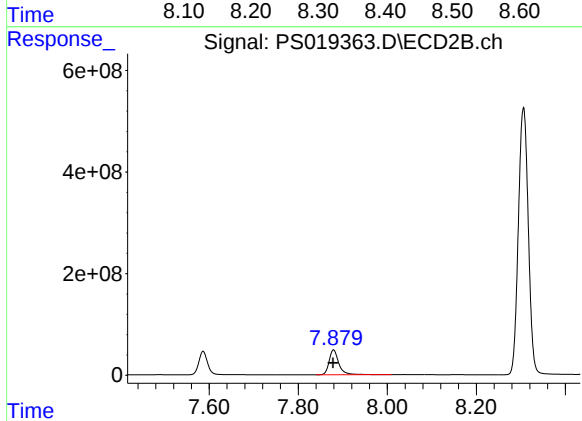


#9 2,4-D

R.T.: 7.879 min
Delta R.T.: 0.001 min
Response: 739542422
Conc: 740.56 ng/ml

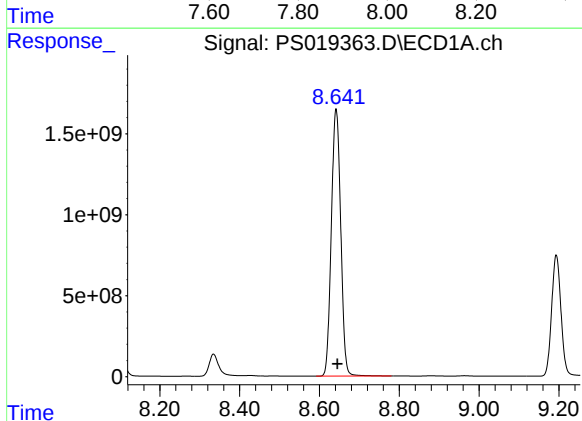


#10 Pentachlorophenol

R.T.: 8.642 min
Delta R.T.: -0.003 min
Response: 26914466033
Conc: 685.08 ng/ml

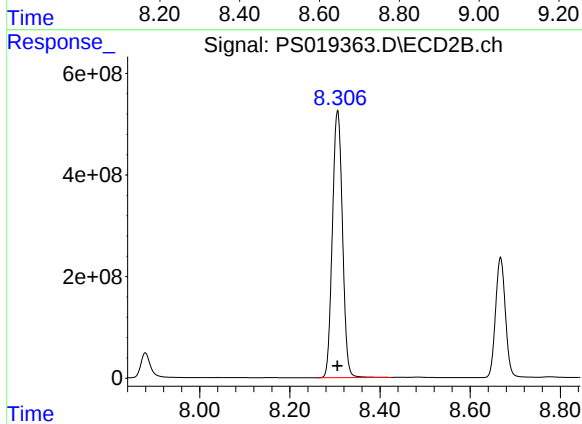

#10 Pentachlorophenol


R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 8159314567
Conc: 725.82 ng/ml

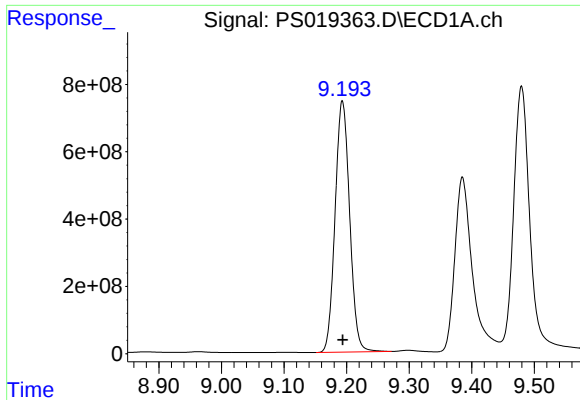

#11 2,4,5-TP (SILVEX)


R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 12076562051
Conc: 668.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

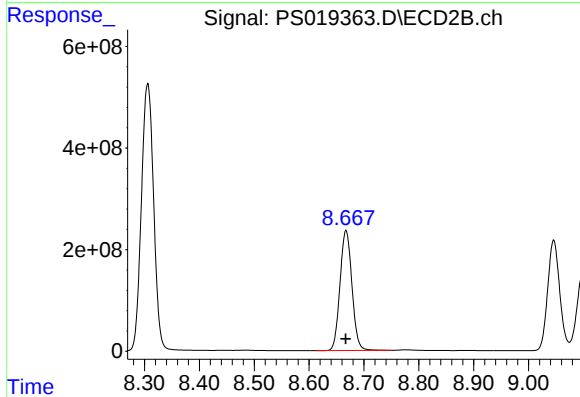


#11 2,4,5-TP (SILVEX)

R.T.: 8.667 min
Delta R.T.: 0.000 min
Response: 3570859859
Conc: 741.99 ng/ml

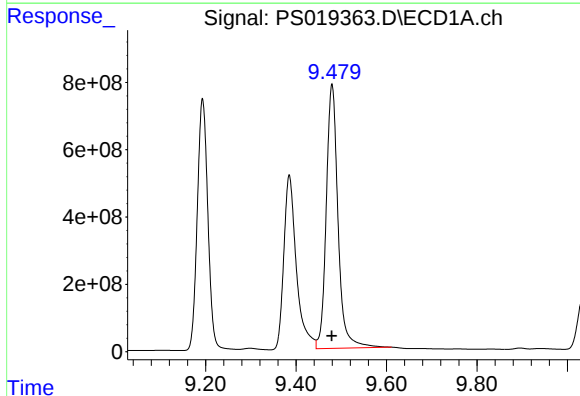


#12 2,4,5-T

R.T.: 9.480 min
Delta R.T.: 0.000 min
Response: 14172887482
Conc: 670.08 ng/ml

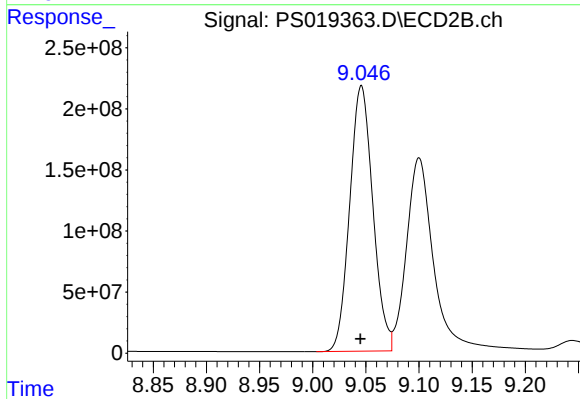

#12 2,4,5-T


R.T.: 9.046 min
Delta R.T.: 0.000 min
Response: 3298116493
Conc: 761.68 ng/ml

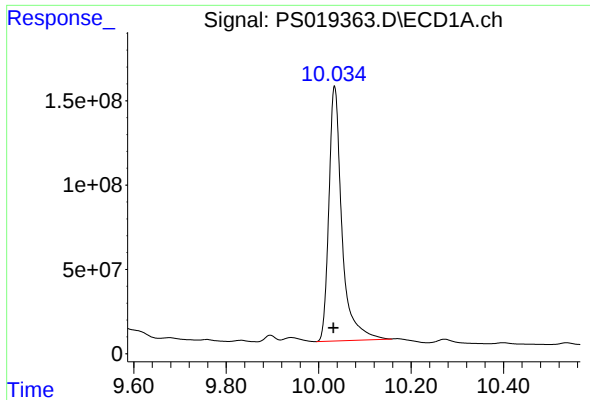

#13 2,4-DB


R.T.: 10.034 min
Delta R.T.: 0.002 min
Response: 2966536322
Conc: 691.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

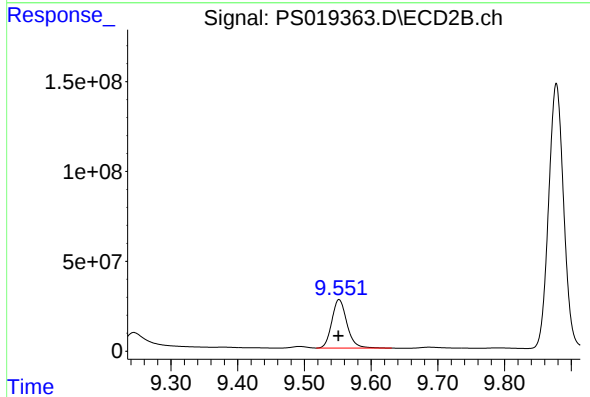


#13 2,4-DB

R.T.: 9.552 min
Delta R.T.: 0.000 min
Response: 424950840
Conc: 747.41 ng/ml

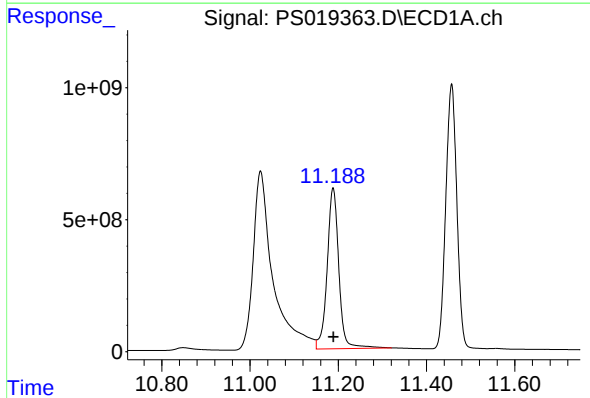


#14 DINOSEB

R.T.: 11.188 min
Delta R.T.: -0.001 min
Response: 11156118071
Conc: 675.66 ng/ml

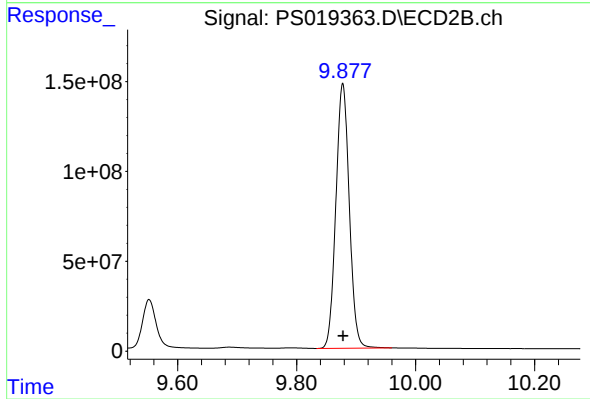

#14 DINOSEB


R.T.: 9.878 min
Delta R.T.: 0.000 min
Response: 2303368454
Conc: 794.85 ng/ml

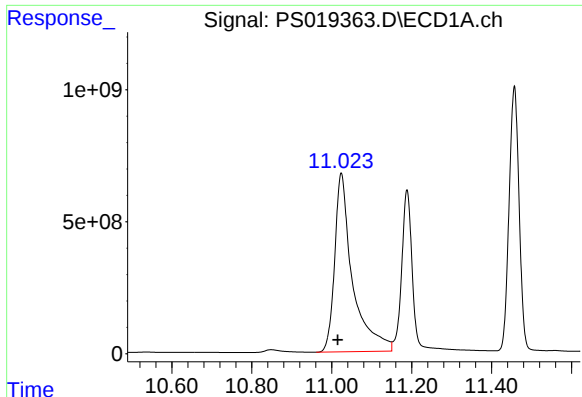

#15 Picloram


R.T.: 11.024 min
Delta R.T.: 0.008 min
Response: 21036399411
Conc: 719.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

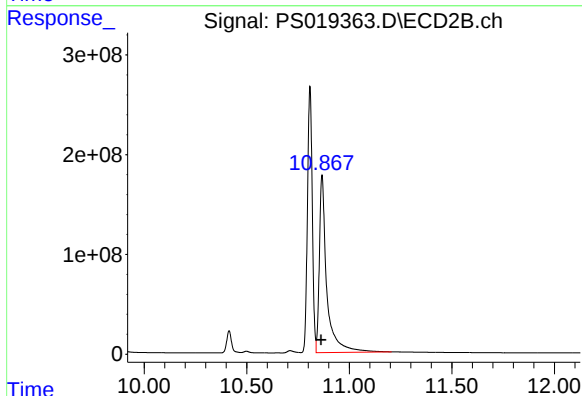


#15 Picloram

R.T.: 10.867 min
Delta R.T.: 0.006 min
Response: 4497492338
Conc: 751.99 ng/ml

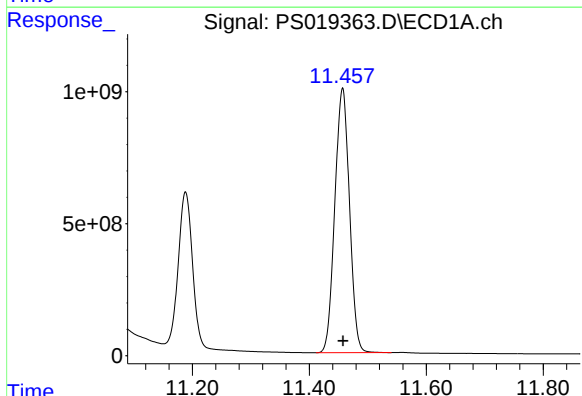

#16 DCPA

R.T.: 11.457 min
Delta R.T.: 0.000 min
Response: 17436376545
Conc: 666.25 ng/ml

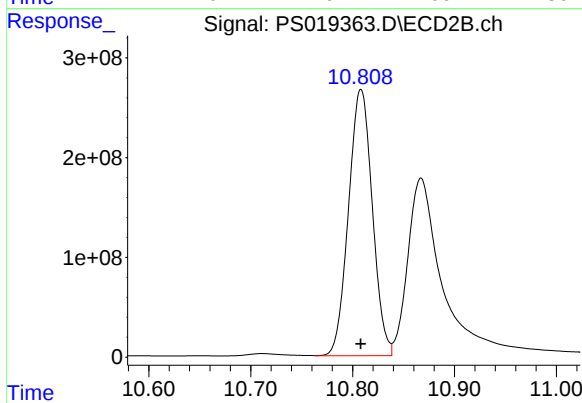

#16 DCPA

R.T.: 10.808 min
Delta R.T.: 0.000 min
Response: 4337553756
Conc: 738.88 ng/ml