

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050924\
 Data File : PS026722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 01:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 05:43:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
 Quant Title : 8080.M
 QLast Update : Mon May 06 13:55:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.268	7.780	1277.7E6	897.0E6	513.761	537.951
Target Compounds							
1) T	Dalapon	2.697f	2.744f	7412885	3252243	2.027	1.109 #
2) T	3,5-DICHL...	6.417f	0.000	21413728	0	6.226	N.D. #
3) T	4-Nitroph...	7.061	7.274f	6234524	1746831	3.870	1.536 #
5) T	DICAMBA	7.472	7.971	36809	1098006	<MDL	<MDL #
6) T	MCP	7.634	8.090	218317	10825494	<MDL	2.106 #
7) T	MCPA	7.809	8.307	410532	4001641	<MDL	<MDL #
8) T	DICHLORPROP	8.202f	8.750f	2339638	18369086	<MDL	9.574 #
9) T	2,4-D	8.410	0.000	59741293	0	18.149	N.D. #
10) T	Pentachlo...	8.696	9.561	1110450	147245	<MDL	<MDL #
11) T	2,4,5-TP ...	9.267	9.923	1181896	475749	<MDL	<MDL #
12) T	2,4,5-T	9.551	10.348	266987	738147	<MDL	<MDL #
13) T	2,4-DB	10.149	10.950f	55374	647943	<MDL	<MDL #
15) T	Picloram	11.182	0.000	703.1E6	0	31.477	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050924\
Data File : PS026722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 01:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 05:43:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
Quant Title : 8080.M
QLast Update : Mon May 06 13:55:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

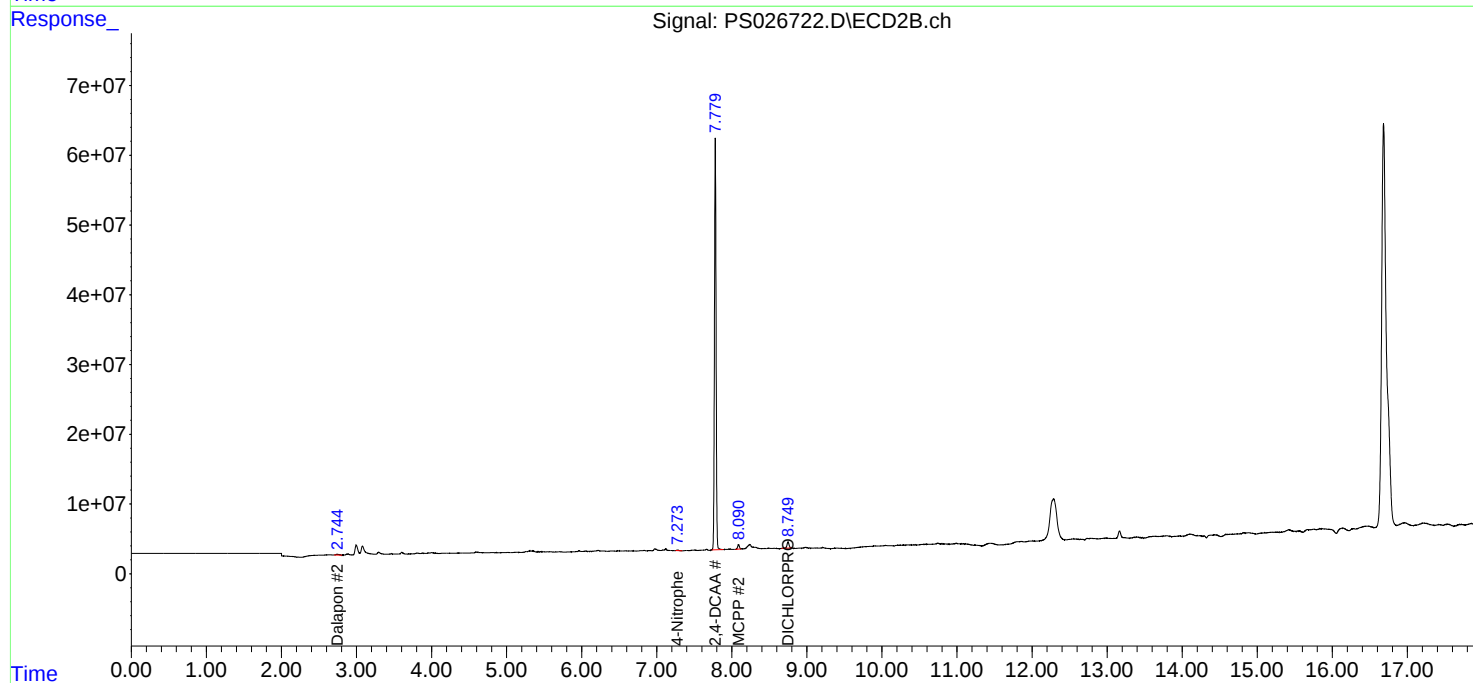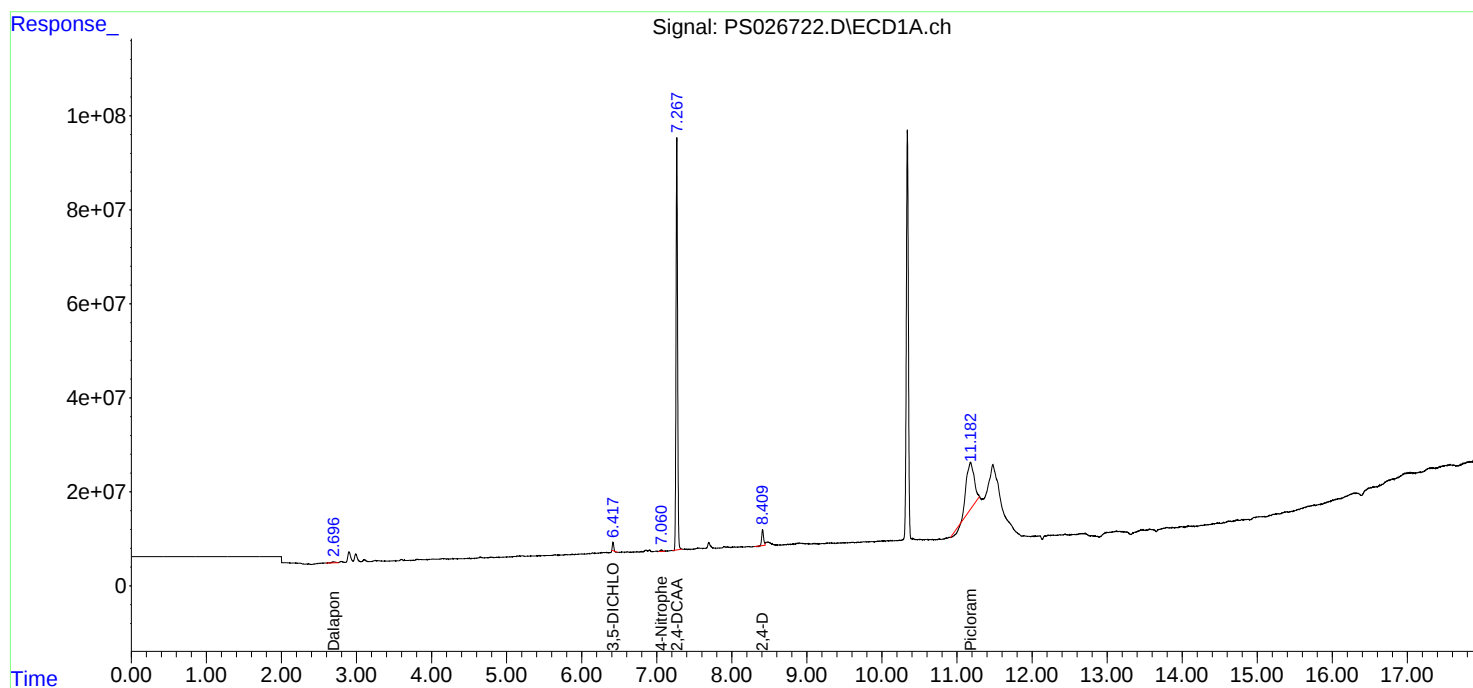


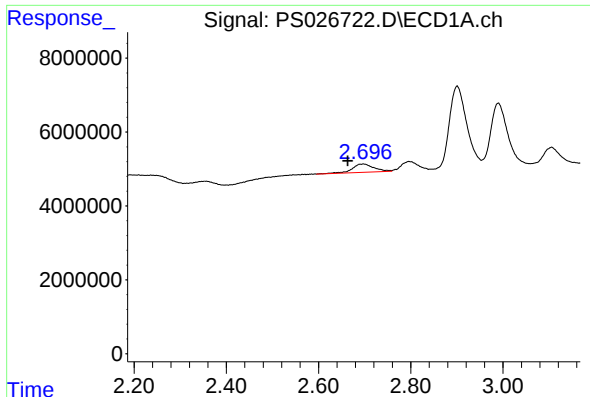

#1 Dalapon


R.T.: 2.697 min
Delta R.T.: 0.034 min
Response: 7412885
Conc: 2.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

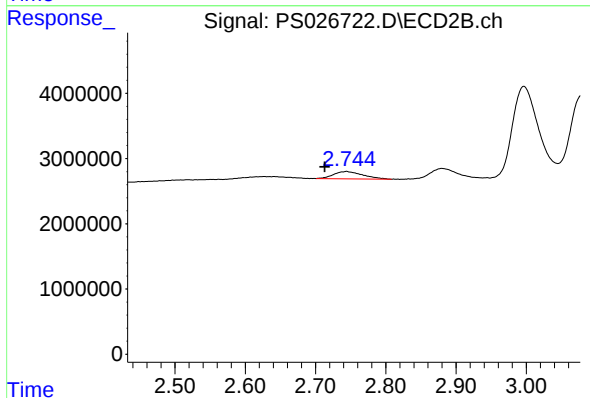


#1 Dalapon

R.T.: 2.744 min
Delta R.T.: 0.031 min
Response: 3252243
Conc: 1.11 ng/ml

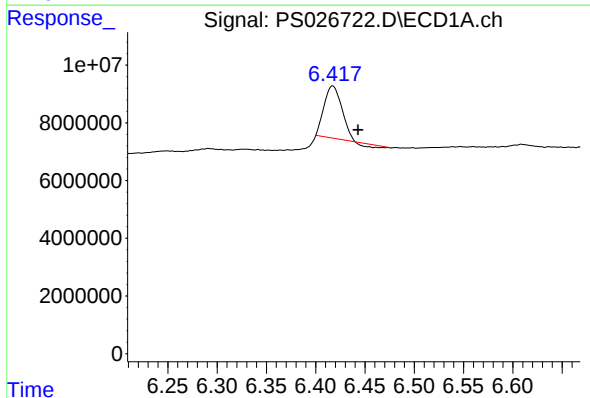


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.417 min
Delta R.T.: -0.026 min
Response: 21413728
Conc: 6.23 ng/ml

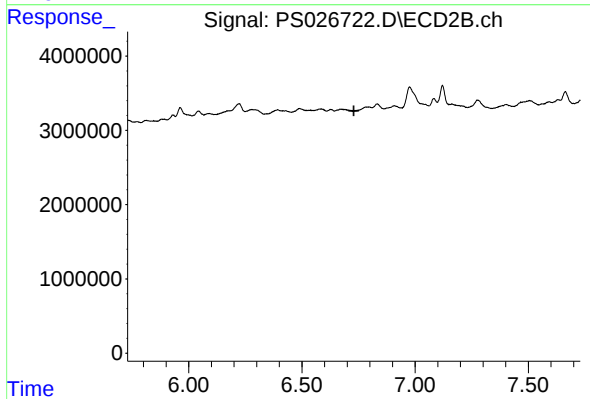

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.730 min
Response: 0
Conc: N.D.

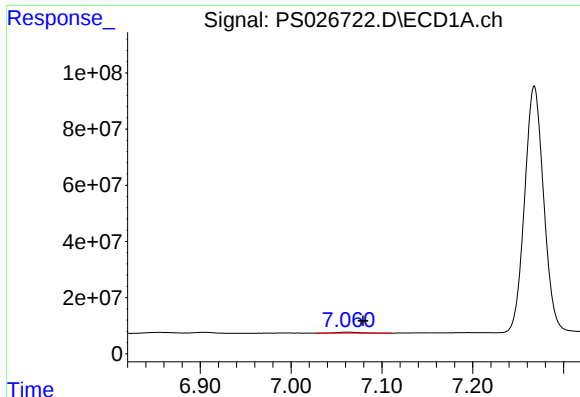

#3 4-Nitrophenol


R.T.: 7.061 min
Delta R.T.: -0.018 min
Response: 6234524
Conc: 3.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

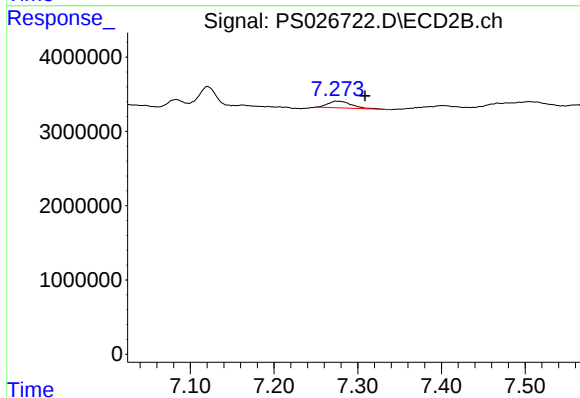


#3 4-Nitrophenol

R.T.: 7.274 min
Delta R.T.: -0.035 min
Response: 1746831
Conc: 1.54 ng/ml

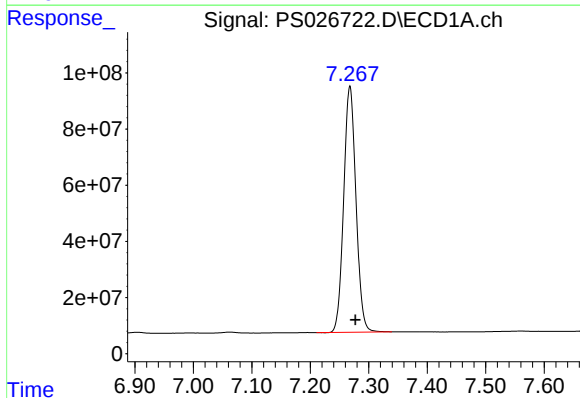


#4 2,4-DCAA

R.T.: 7.268 min
Delta R.T.: -0.010 min
Response: 1277650201
Conc: 513.76 ng/ml

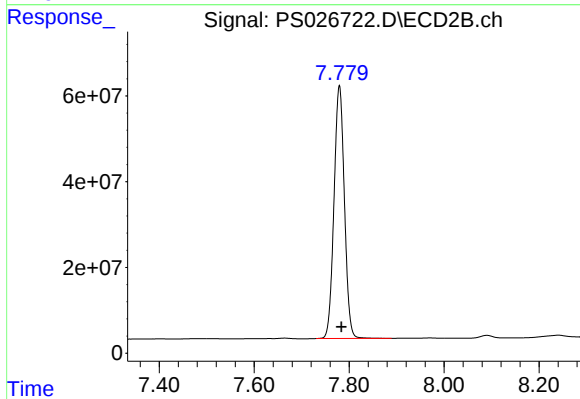

#4 2,4-DCAA


R.T.: 7.780 min
Delta R.T.: -0.004 min
Response: 896988485
Conc: 537.95 ng/ml

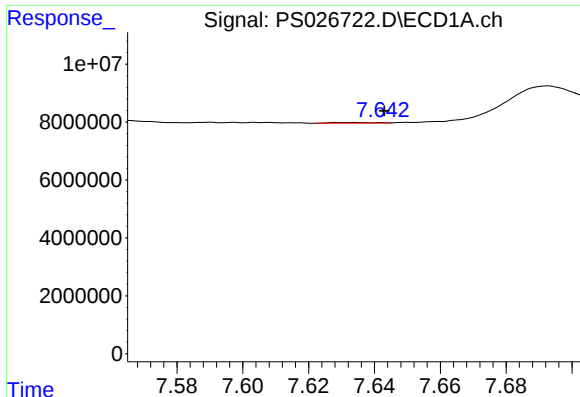

#6 MCPP


R.T.: 7.634 min
Delta R.T.: -0.009 min
Response: 218317
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

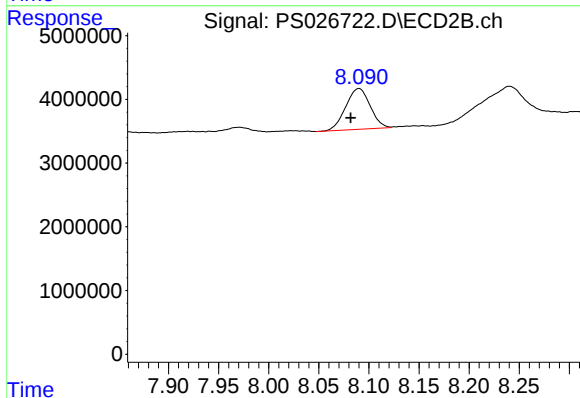


#6 MCPP

R.T.: 8.090 min
Delta R.T.: 0.008 min
Response: 10825494
Conc: 2.11 ug/ml

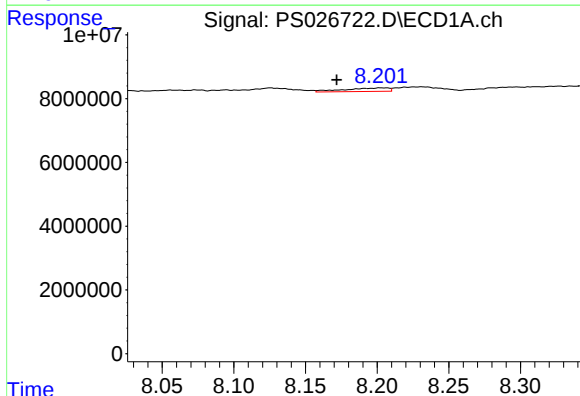


#8 DICHLORPROP

R.T.: 8.202 min
Delta R.T.: 0.031 min
Response: 2339638
Conc: N.D.

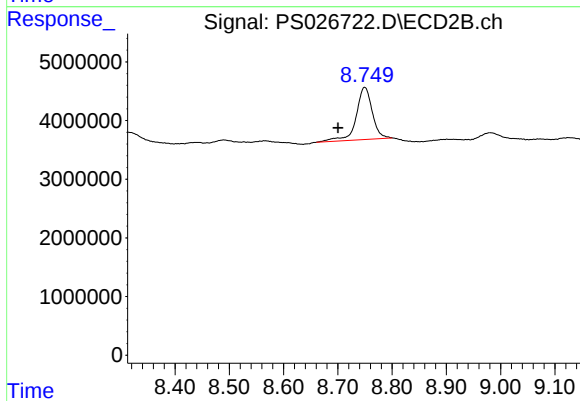

#8 DICHLORPROP


R.T.: 8.750 min
Delta R.T.: 0.049 min
Response: 18369086
Conc: 9.57 ng/ml

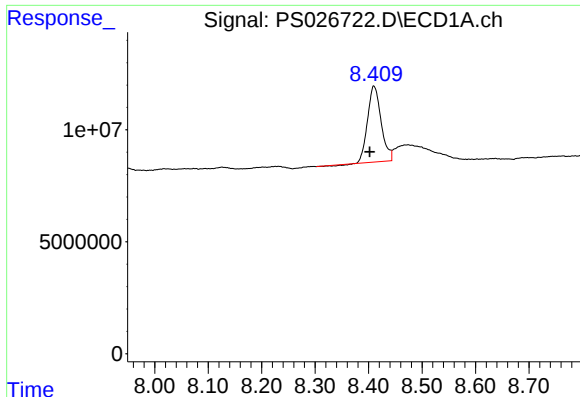

#9 2,4-D


R.T.: 8.410 min
Delta R.T.: 0.007 min
Response: 59741293
Conc: 18.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

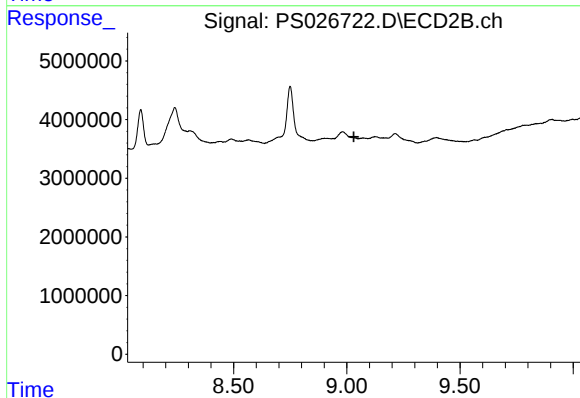


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

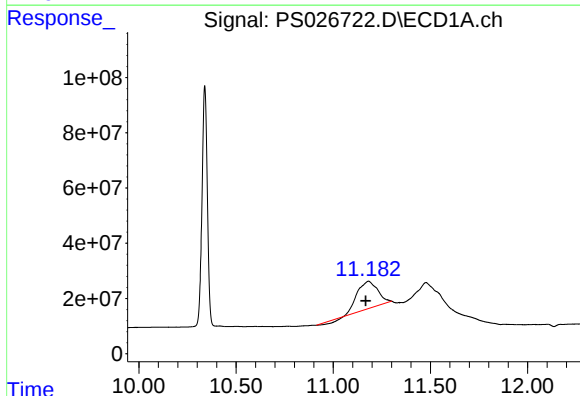

#15 Picloram

R.T.: 11.182 min
Delta R.T.: 0.014 min
Response: 703113423
Conc: 31.48 ng/ml

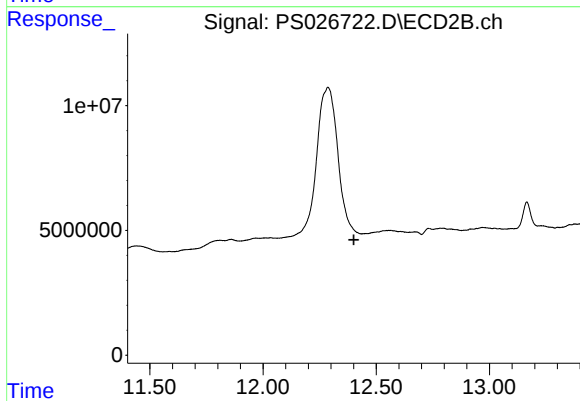

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.401 min
Response: 0
Conc: N.D.