

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050924\
 Data File : PS026719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2024 22:09
 Operator : AR\AJ
 Sample : P2412-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SS-1-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/10/2024
 Supervised By :Ankita Jodhani 05/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 11:46:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
 Quant Title : 8080.M
 QLast Update : Mon May 06 13:55:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.268	7.779	714.5E6	395.7E6	287.325	237.325m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050924\
Data File : PS026719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2024 22:09
Operator : AR\AJ
Sample : P2412-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SS-1-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/10/2024
Supervised By : Ankita Jodhani 05/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 11:46:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
Quant Title : 8080.M
QLast Update : Mon May 06 13:55:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

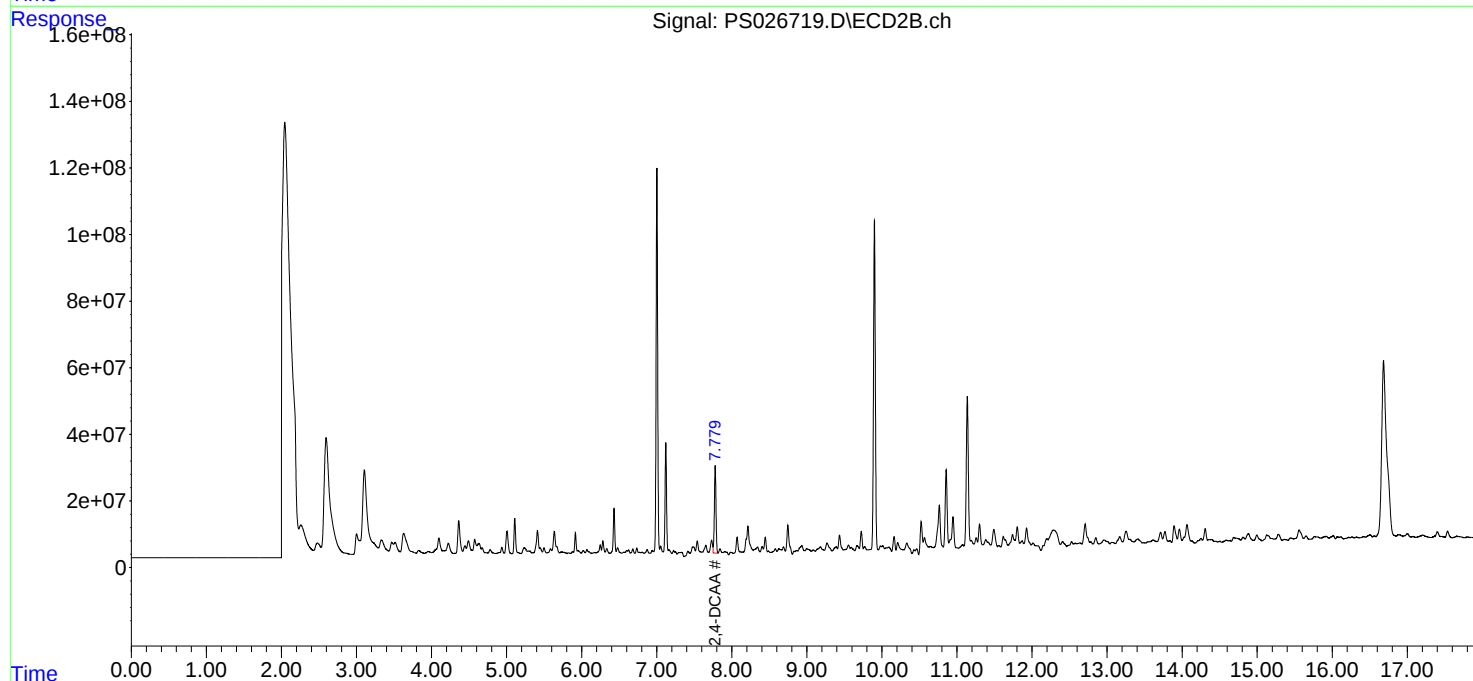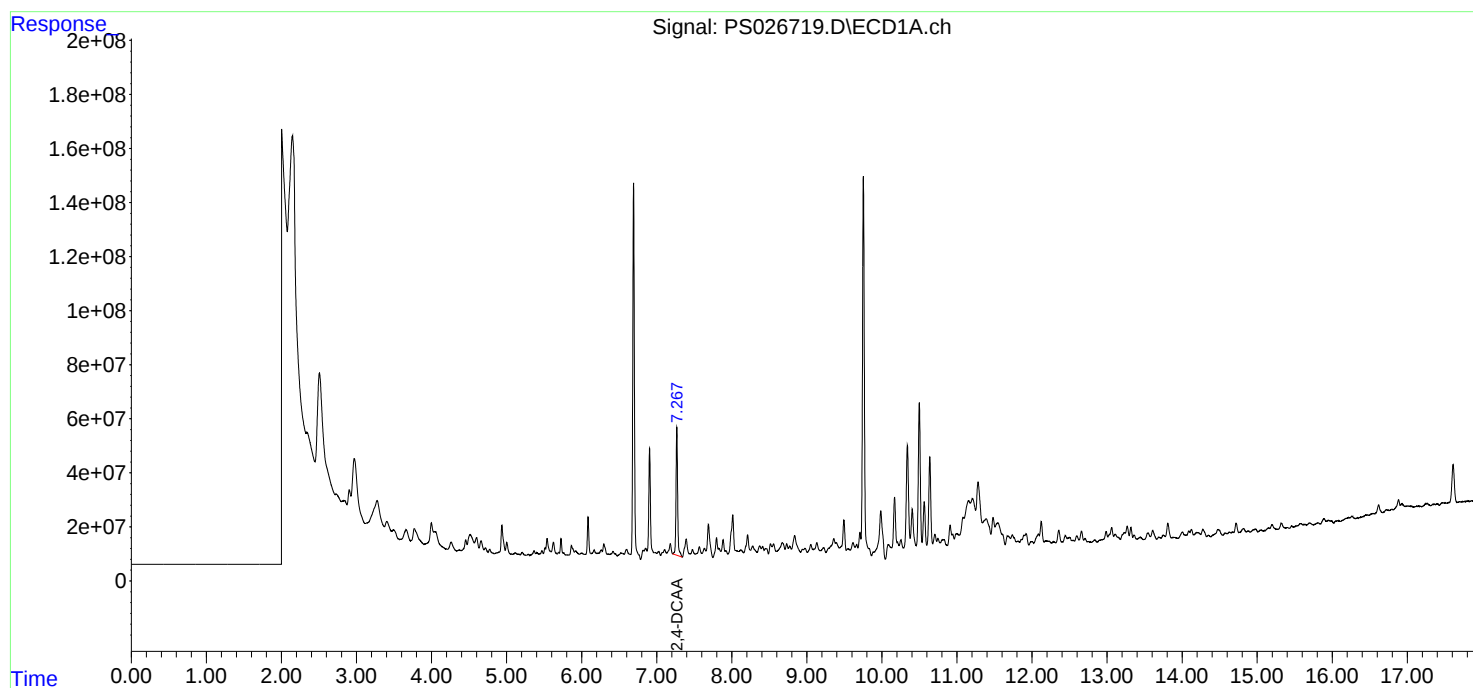

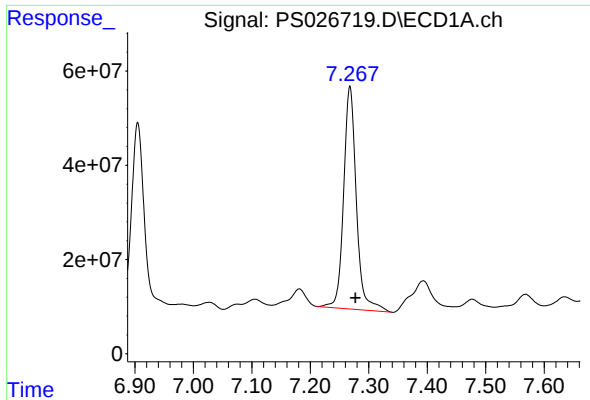


#4 2,4-DCAA

R.T.: 7.268 min
Delta R.T.: -0.010 min
Response: 714535967
Conc: 287.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
SS-1-COMP

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/10/2024
Supervised By :Ankita Jodhani 05/10/2024

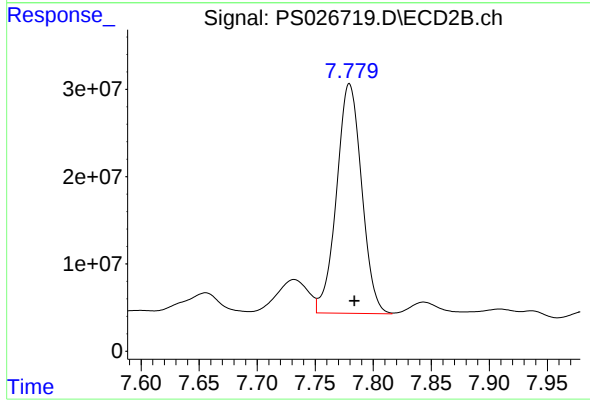

#4 2,4-DCAA

R.T.: 7.779 min
Delta R.T.: -0.005 min
Response: 395719389
Conc: 237.32 ng/ml m