

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051021\
 Data File : PS014961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 19:19
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 00:06:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
9) T	2,4-D	8.324f	0.000	6662295	0	3.744 N.D. #
14) T	DINOSEB	11.024f	0.000	9893727	0	1.380 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051021\
Data File : PS014961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 19:19
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 00:06:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

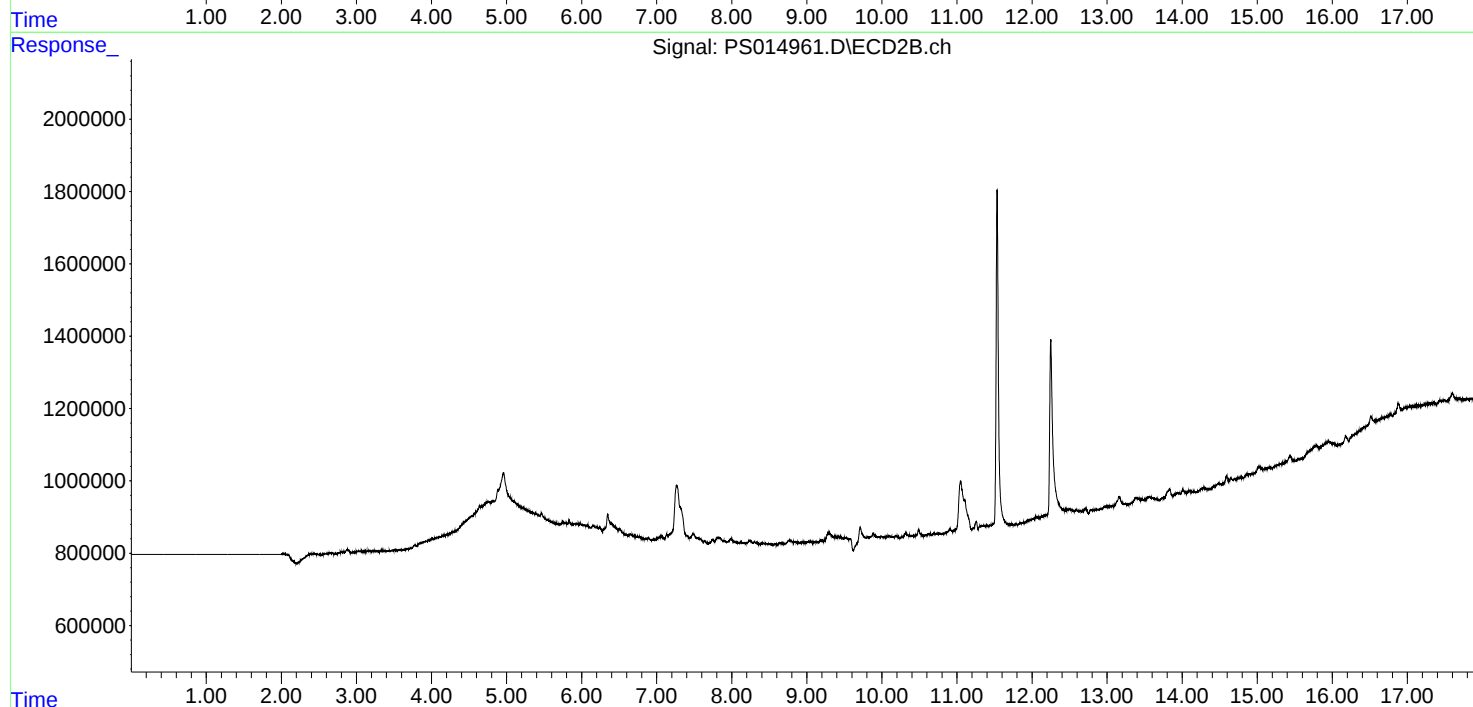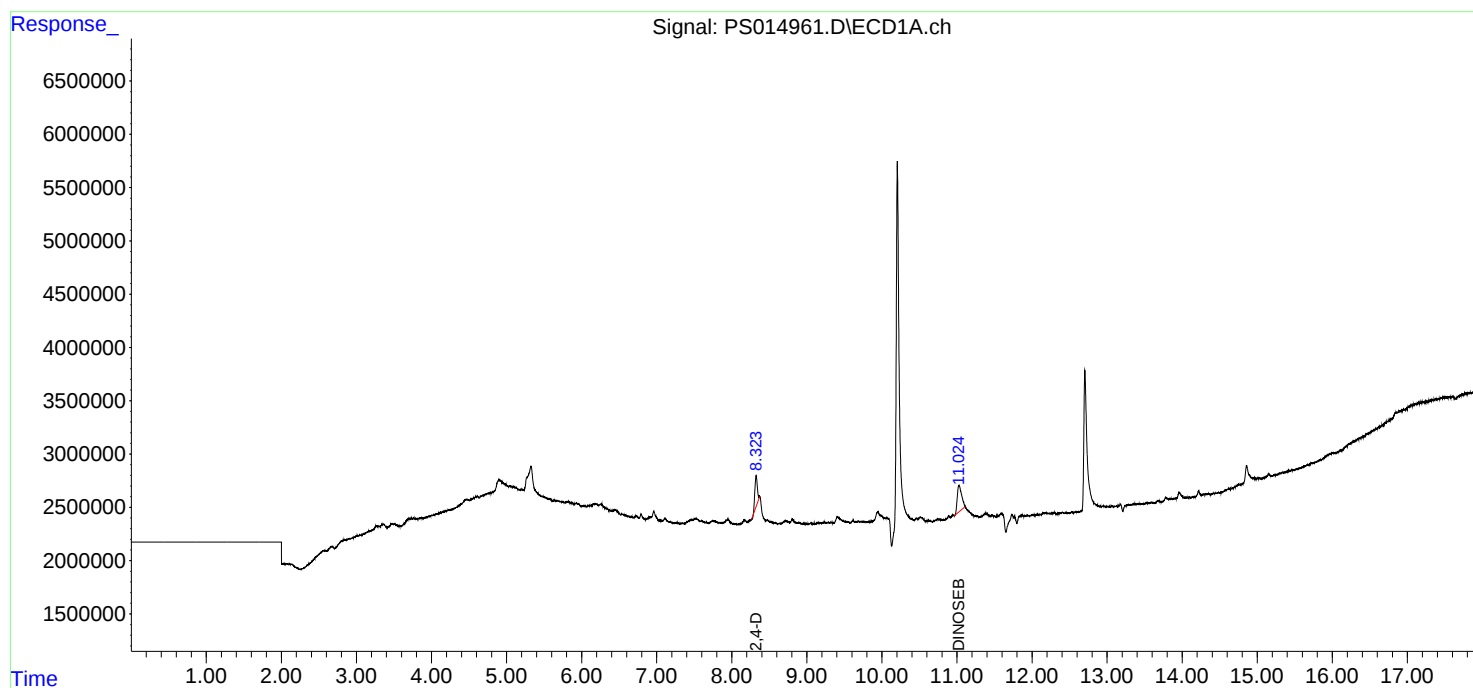


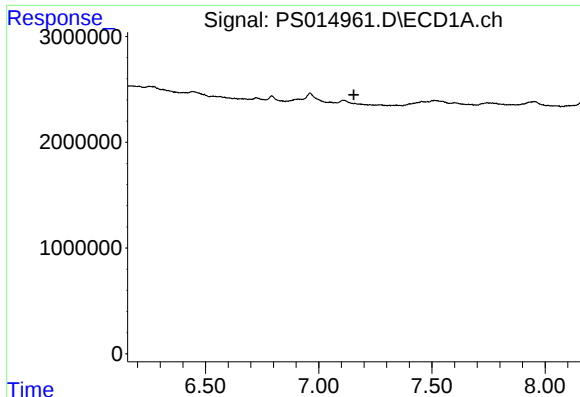

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

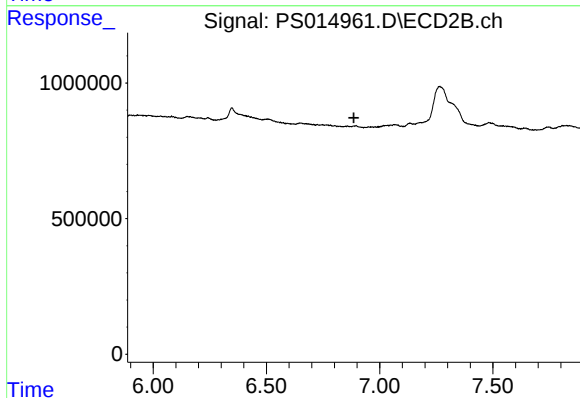


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

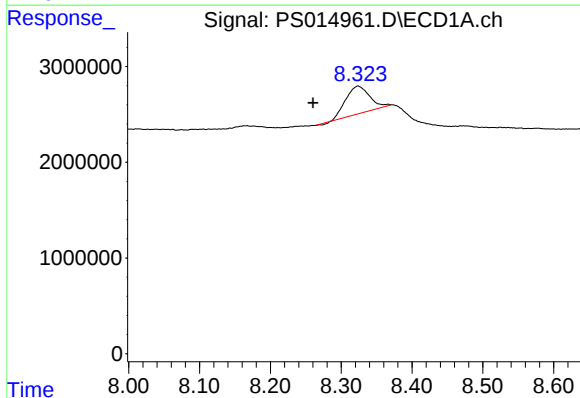


#9 2,4-D

R.T.: 8.324 min
Delta R.T.: 0.064 min
Response: 6662295
Conc: 3.74 ng/ml

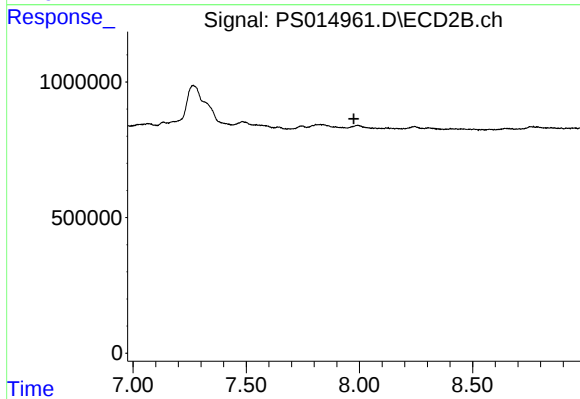

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

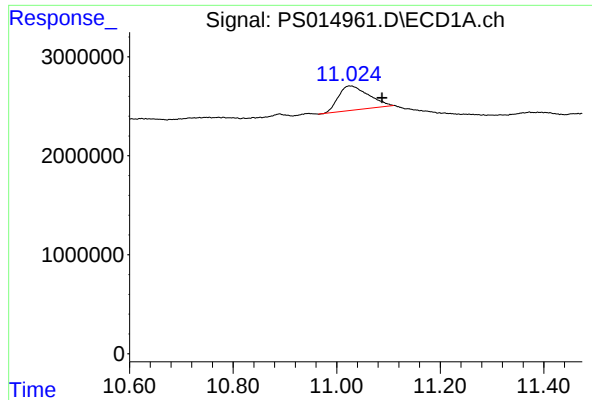

#14 DINOSEB

R.T.: 11.024 min
Delta R.T.: -0.063 min
Response: 9893727
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

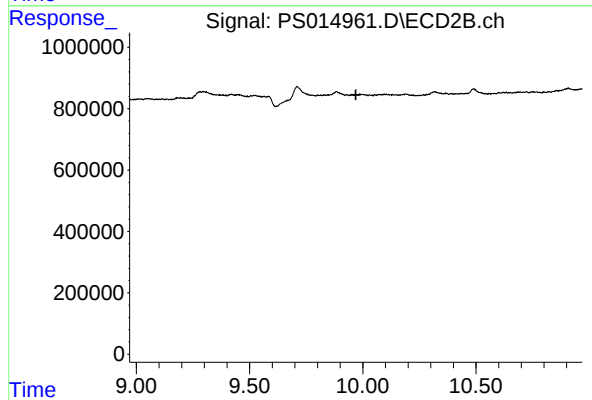

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.970 min
Response: 0
Conc: N.D.