

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051021\
 Data File : PS014969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 22:56
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 00:06:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.890	707.7E6	259.9E6	422.979	537.135 #
Target Compounds							
5) T	DICAMBA	7.352	7.060	6356162	4778097	<MDL	2.231 #
9) T	2,4-D	8.325f	0.000	28006245	0	15.738	N.D. #
10) T	Pentachlo...	8.580	8.411	16659033	5678476	<MDL	<MDL #
11) T	2,4,5-TP ...	9.140	0.000	9206728	0	1.007	N.D. #
12) T	2,4,5-T	9.380	0.000	59247053	0	6.478	N.D. #
14) T	DINOSEB	11.097	0.000	36078695	0	5.031	N.D. #
15) T	Picloram	10.918	11.011f	2616742	90138770	<MDL	22.621 #
16) T	DCPA	11.361	10.902	17966971	7260193	1.315	1.703 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051021\
Data File : PS014969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 22:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 00:06:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

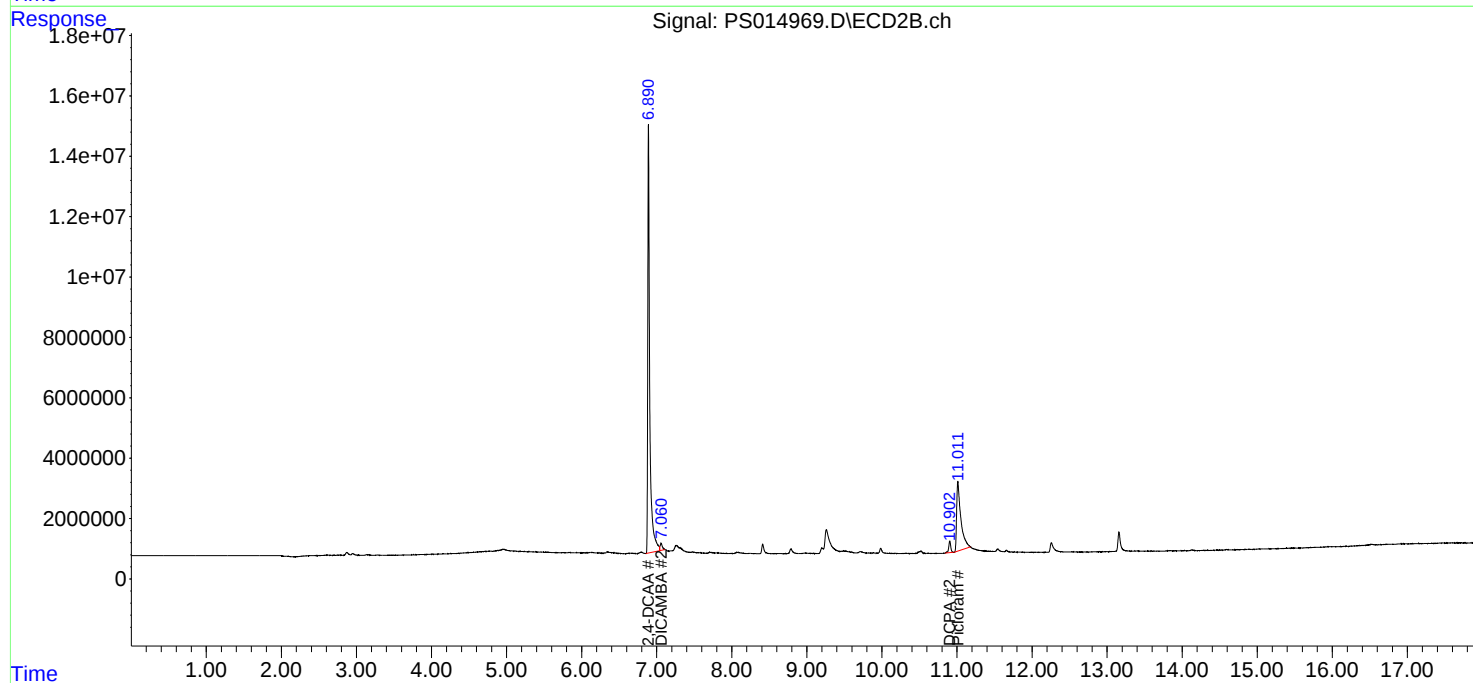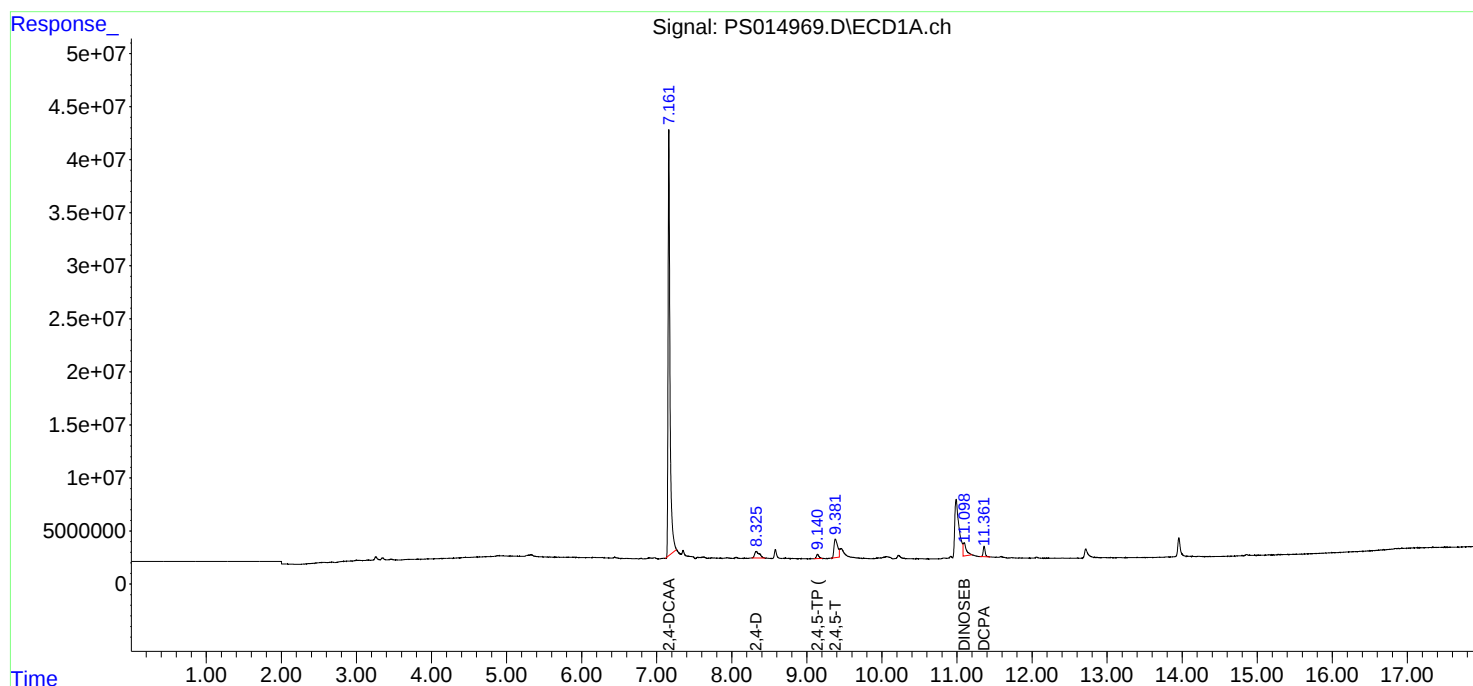


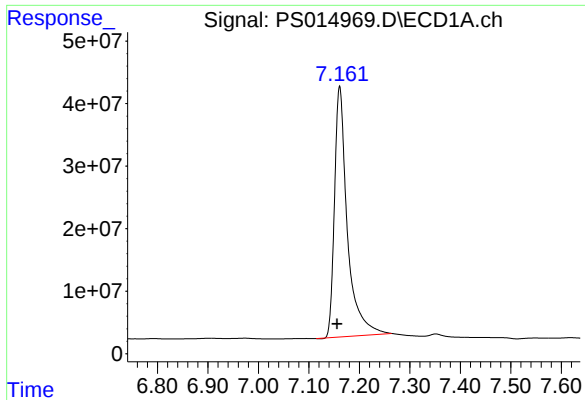

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: 0.005 min
Response: 707748673
Conc: 422.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

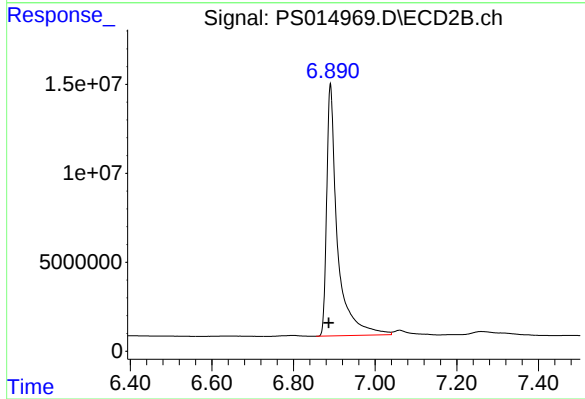


#4 2,4-DCAA

R.T.: 6.890 min
Delta R.T.: 0.004 min
Response: 259926356
Conc: 537.13 ng/ml

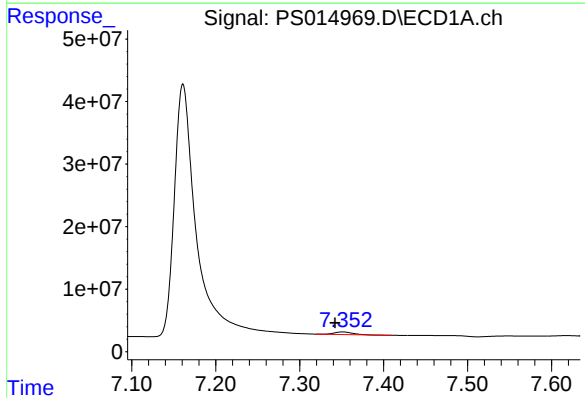


#5 DICAMBA

R.T.: 7.352 min
Delta R.T.: 0.009 min
Response: 6356162
Conc: N.D.

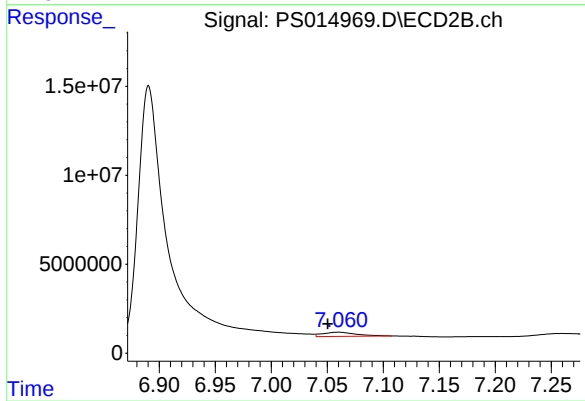

#5 DICAMBA


R.T.: 7.060 min
Delta R.T.: 0.010 min
Response: 4778097
Conc: 2.23 ng/ml

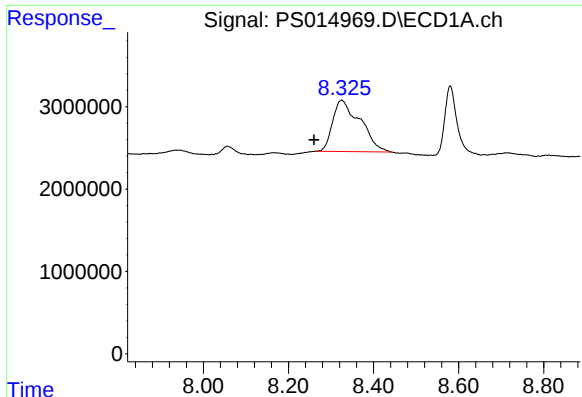

#9 2,4-D


R.T.: 8.325 min
Delta R.T.: 0.065 min
Response: 28006245
Conc: 15.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

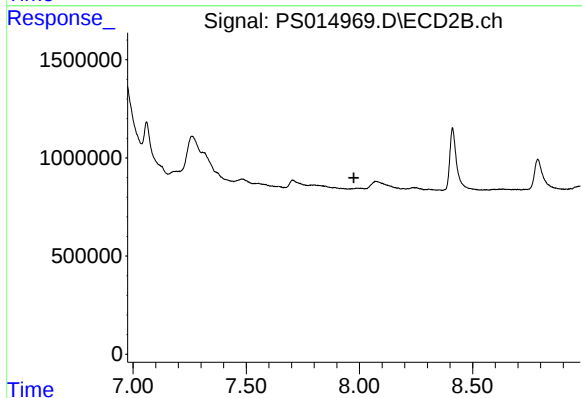


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

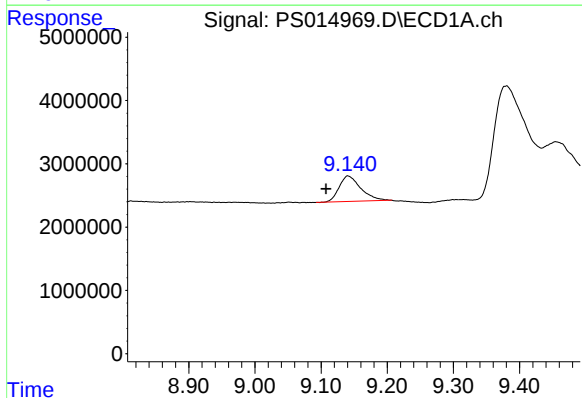


#11 2,4,5-TP (SILVEX)

R.T.: 9.140 min
Delta R.T.: 0.033 min
Response: 9206728
Conc: 1.01 ng/ml

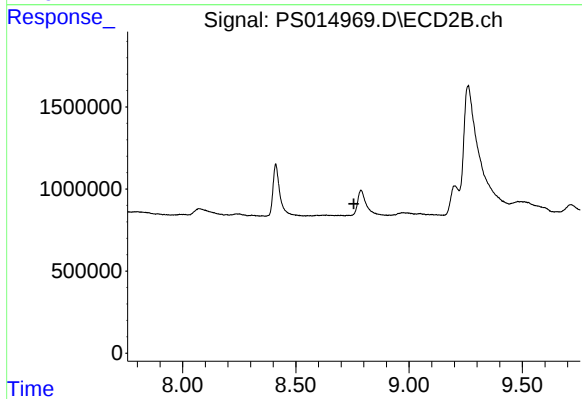

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.756 min
Response: 0
Conc: N.D.

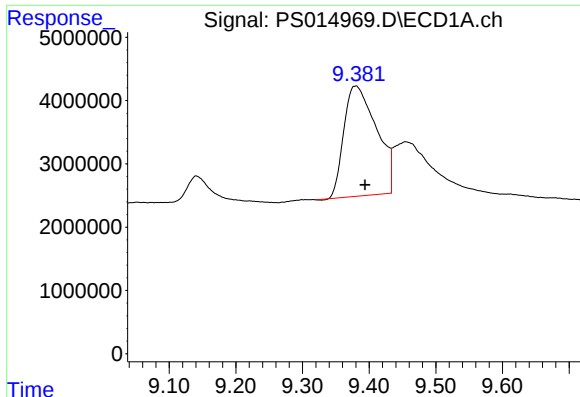

#12 2,4,5-T


R.T.: 9.380 min
Delta R.T.: -0.014 min
Response: 59247053
Conc: 6.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

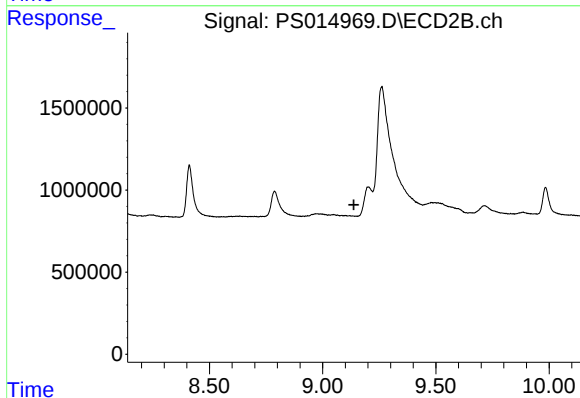


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.138 min
Response: 0
Conc: N.D.

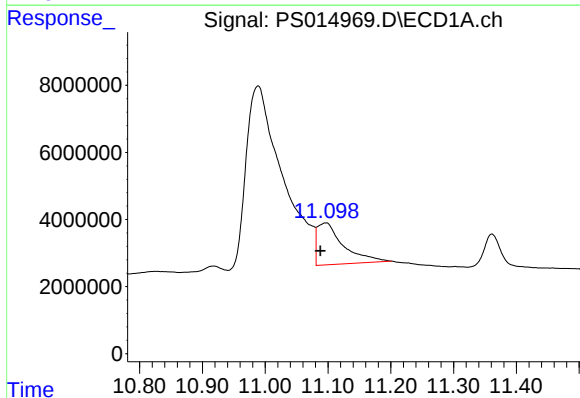


#14 DINOSEB

R.T.: 11.097 min
Delta R.T.: 0.009 min
Response: 36078695
Conc: 5.03 ng/ml

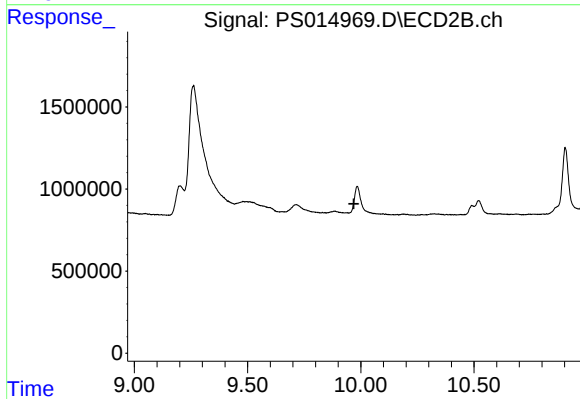

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.970 min
Response: 0
Conc: N.D.

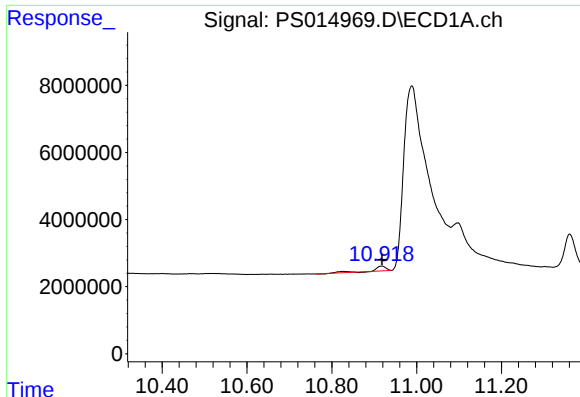

#15 Picloram


R.T.: 10.918 min
Delta R.T.: 0.000 min
Response: 2616742
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

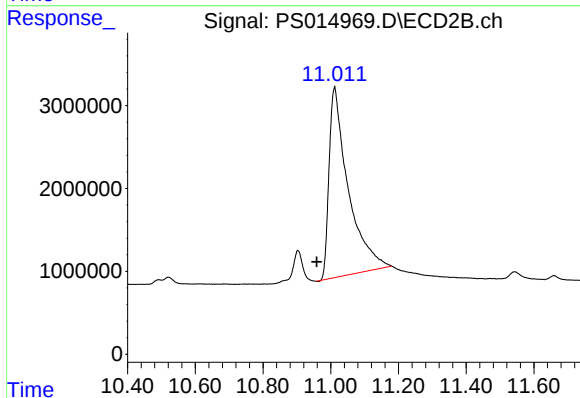


#15 Picloram

R.T.: 11.011 min
Delta R.T.: 0.053 min
Response: 90138770
Conc: 22.62 ng/ml

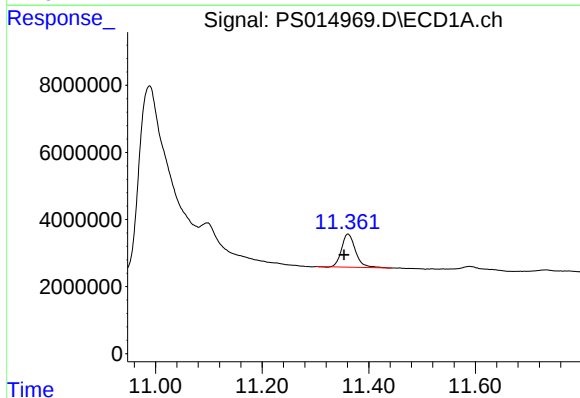

#16 DCPA

R.T.: 11.361 min
Delta R.T.: 0.007 min
Response: 17966971
Conc: 1.32 ng/ml

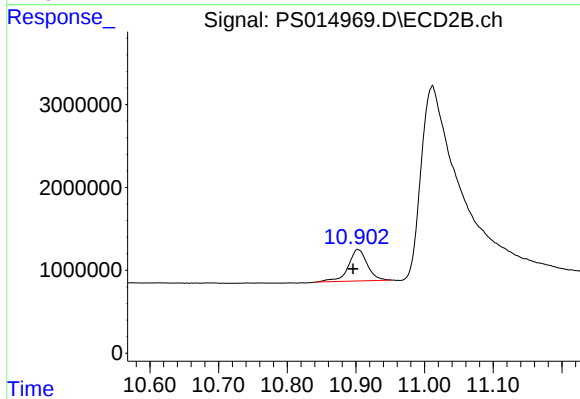

#16 DCPA

R.T.: 10.902 min
Delta R.T.: 0.006 min
Response: 7260193
Conc: 1.70 ng/ml