

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051022\
 Data File : PS019364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2022 09:51
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 17:49:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.192	6.806	139433	254960	<MDL	<MDL	#
Target Compounds								
2) T	3,5-DICHL...	6.437	5.930f	542835	87492	<MDL	<MDL	#
3) T	4-Nitroph...	7.012	0.000	4222701	0	4.357	N.D.	#
5) T	DICAMBA	7.416	6.964	2397096	669619	<MDL	<MDL	#
6) T	MCP	7.619	7.026f	92376	3692389	<MDL	1.388	#
7) T	MCPA	7.690f	0.000	520160	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.126	7.619	852587	3880496	<MDL	4.528	#
9) T	2,4-D	8.335	7.919f	515618	303544	<MDL	<MDL	#
10) T	Pentachlo...	8.651	8.306	7182039	1996445	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.207	8.672	2676270	1093991	<MDL	<MDL	#
12) T	2,4,5-T	9.502	9.059	9556729	1308339	<MDL	<MDL	#
13) T	2,4-DB	10.074f	9.570	2569189	265367	<MDL	<MDL	#
14) T	DINOSEB	0.000	9.880	0	709965	N.D.	<MDL	
15) T	Picloram	10.993	10.893	308.4E6	50328359	10.550	8.415	
16) T	DCPA	11.466	10.812	5188031	9328248	<MDL	1.589	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051022\
Data File : PS019364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2022 09:51
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 17:49:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

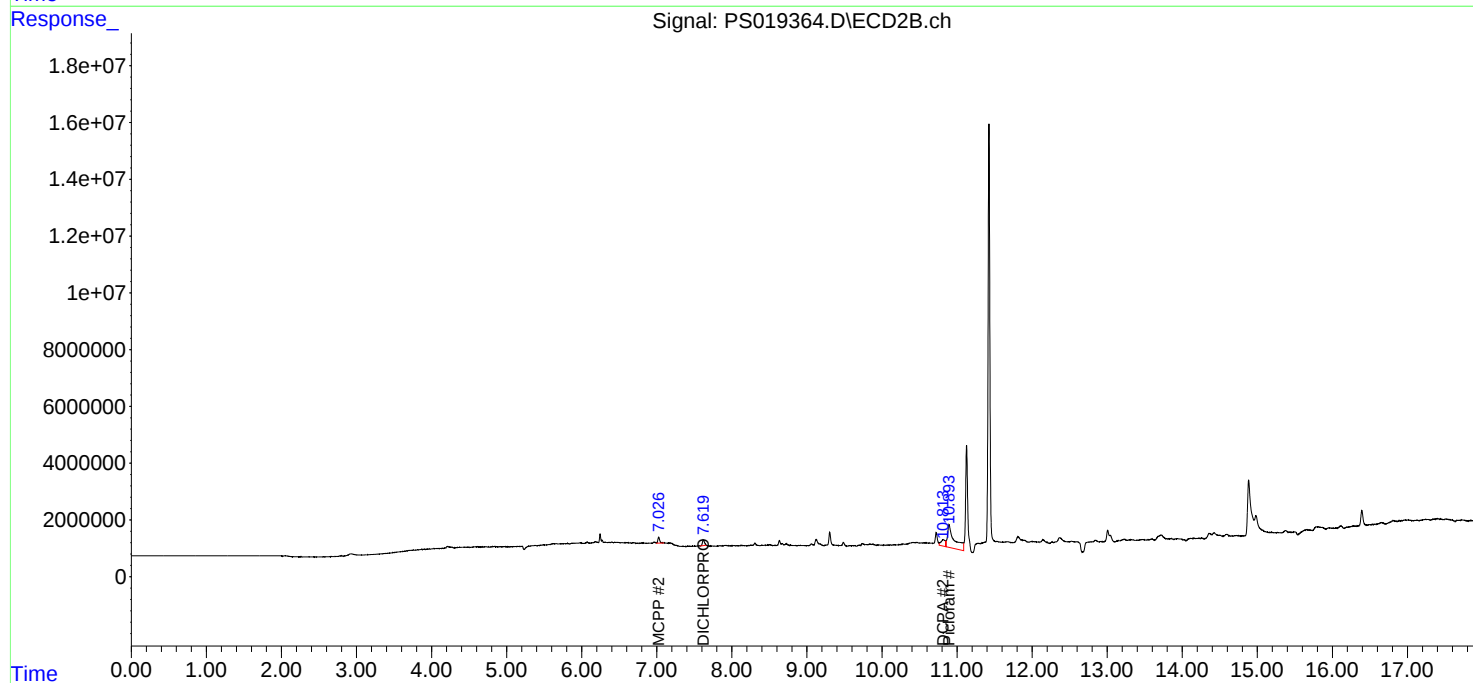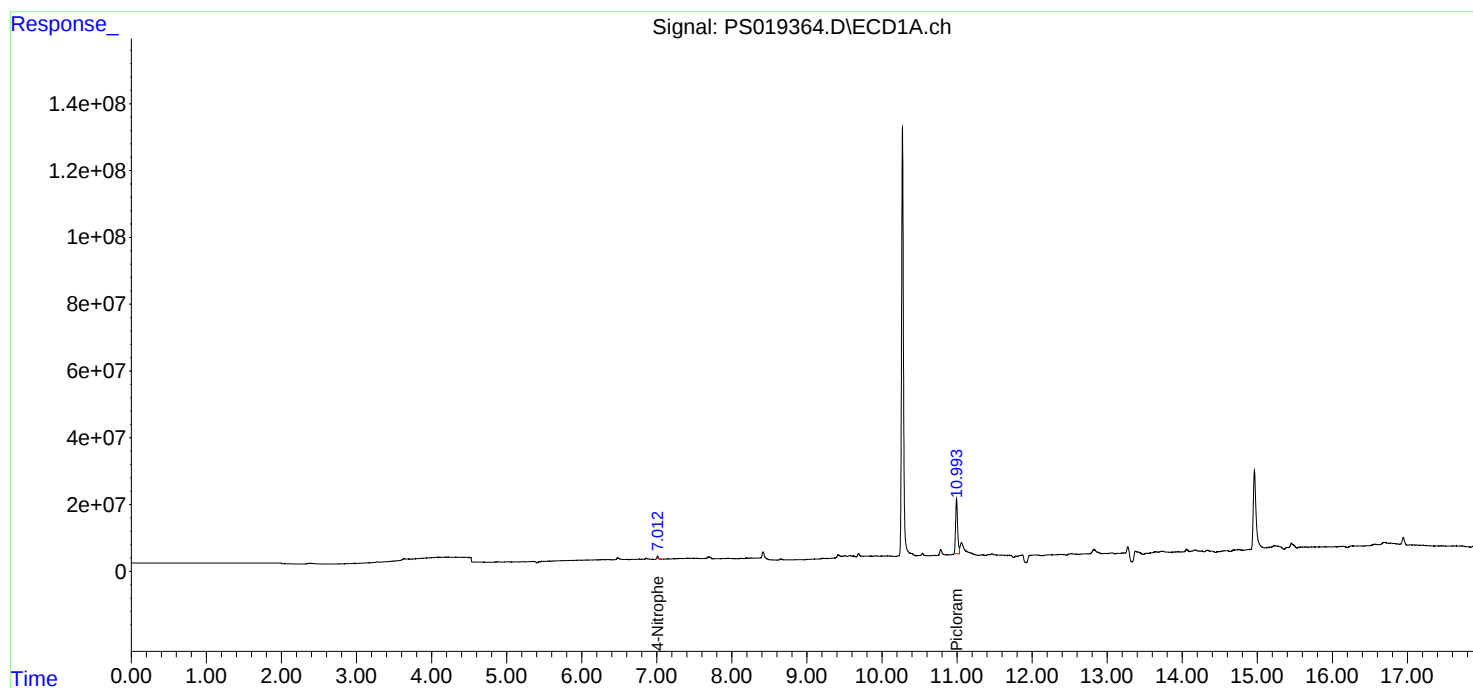


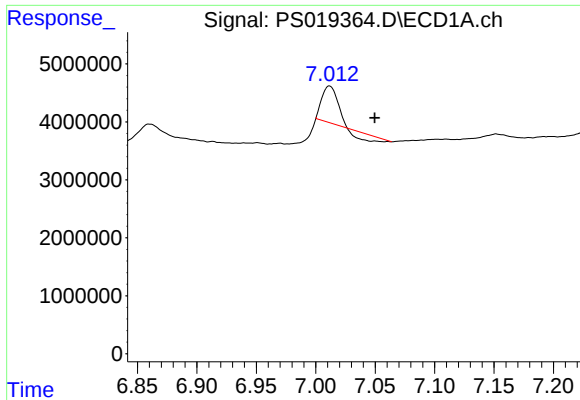

#3 4-Nitrophenol


R.T.: 7.012 min
Delta R.T.: -0.038 min
Response: 4222701
Conc: 4.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

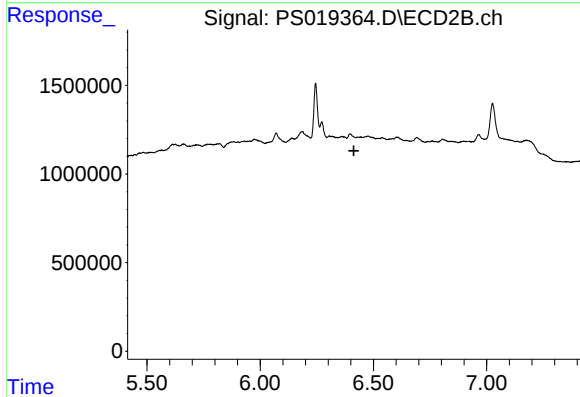


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

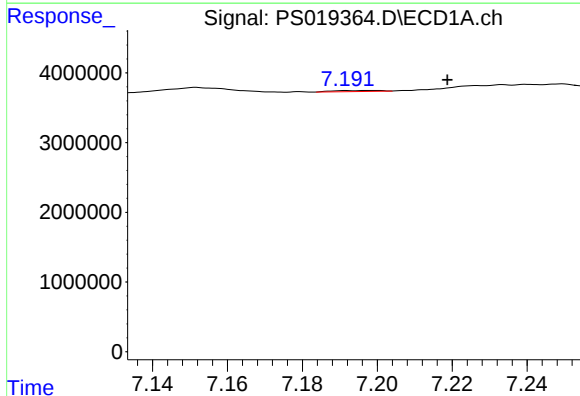


#4 2,4-DCAA

R.T.: 7.192 min
Delta R.T.: -0.027 min
Response: 139433
Conc: N.D.

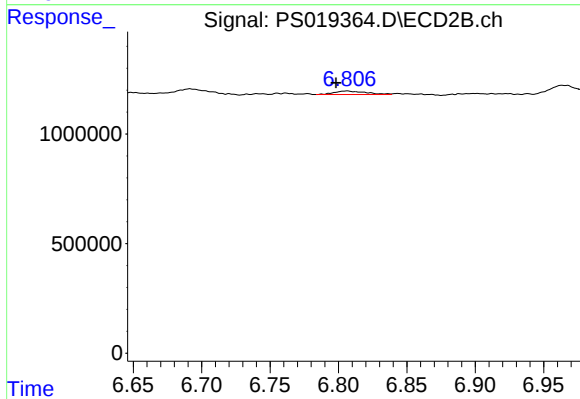

#4 2,4-DCAA


R.T.: 6.806 min
Delta R.T.: 0.008 min
Response: 254960
Conc: N.D.

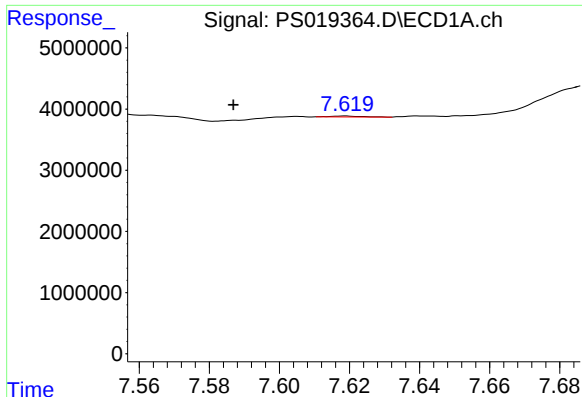

#6 MCP


R.T.: 7.619 min
Delta R.T.: 0.032 min
Response: 92376
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

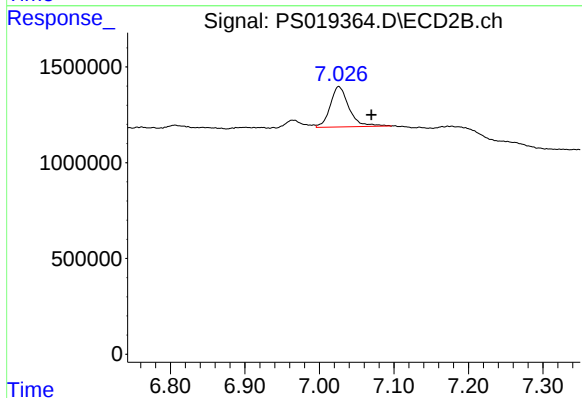


#6 MCP

R.T.: 7.026 min
Delta R.T.: -0.044 min
Response: 3692389
Conc: 1.39 ug/ml

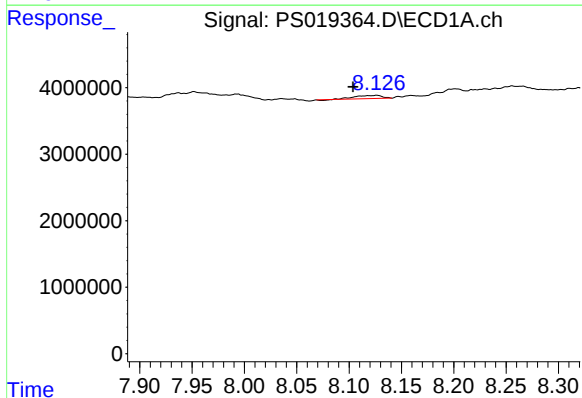


#8 DICHLORPROP

R.T.: 8.126 min
Delta R.T.: 0.023 min
Response: 852587
Conc: N.D.

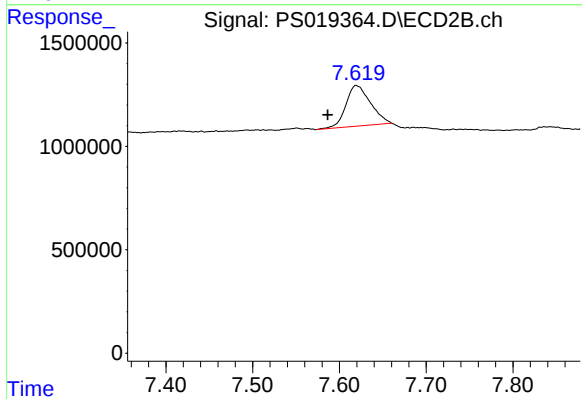

#8 DICHLORPROP


R.T.: 7.619 min
Delta R.T.: 0.033 min
Response: 3880496
Conc: 4.53 ng/ml

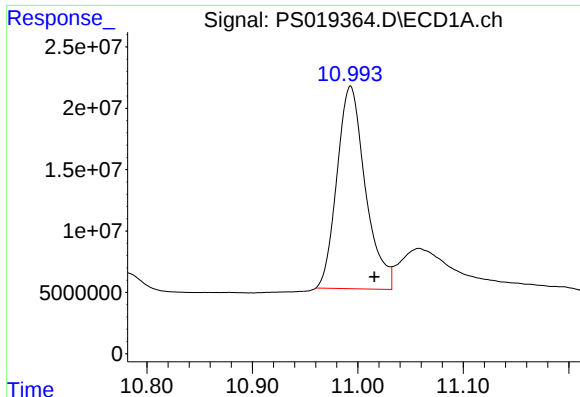

#15 Picloram


R.T.: 10.993 min
Delta R.T.: -0.023 min
Response: 308375975
Conc: 10.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

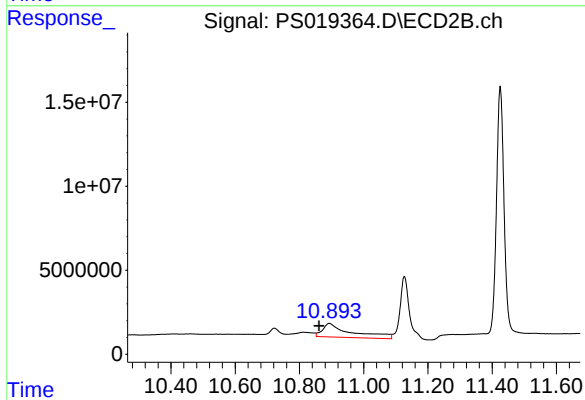


#15 Picloram

R.T.: 10.893 min
Delta R.T.: 0.032 min
Response: 50328359
Conc: 8.41 ng/ml

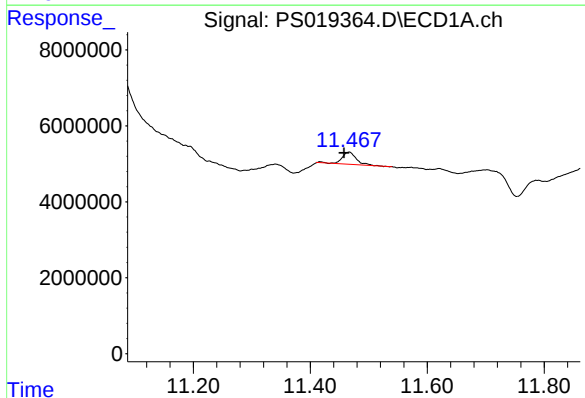

#16 DCPA

R.T.: 11.466 min
Delta R.T.: 0.008 min
Response: 5188031
Conc: N.D.

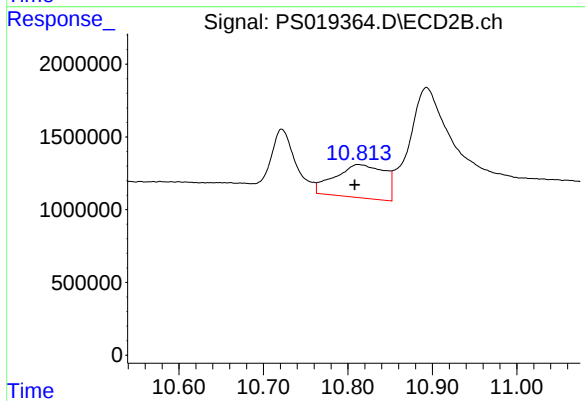

#16 DCPA

R.T.: 10.812 min
Delta R.T.: 0.004 min
Response: 9328248
Conc: 1.59 ng/ml