

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051023\
 Data File : PS022963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2023 17:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 03:56:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.497	6.856	793.2E6	290.3E6	521.529	517.285
Target Compounds							
1) T	Dalapon	2.586	0.000	1719243	0	1.063	N.D. #
3) T	4-Nitroph...	6.330	0.000	4729278	0	4.492	N.D. #
5) T	DICAMBA	6.644	7.009	396837	190762	<MDL	<MDL #
6) T	MCP	6.733f	0.000	1253684	0	<MDL	N.D. #
8) T	DICHLORPROP	7.249	7.662	109.9E6	1412073	58.633	2.282 #
9) T	2,4-D	7.450	0.000	49962524	0	21.589	N.D. #
10) T	Pentachlo...	7.696	8.363	1101081	996106	<MDL	<MDL #
11) T	2,4,5-TP ...	8.237	0.000	3780024	0	<MDL	N.D. #
12) T	2,4,5-T	8.501	9.145f	4193634	2982105	<MDL	<MDL #
13) T	2,4-DB	9.003	0.000	26545735	0	11.315	N.D. #
14) T	DINOSEB	10.092	0.000	1635095	0	<MDL	N.D. #
15) T	Picloram	9.915	10.903	62615971	10112063	3.651	2.374 #
16) T	DCPA	10.359	10.852	2635504	6516108	<MDL	1.744 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051023\
Data File : PS022963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2023 17:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 03:56:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

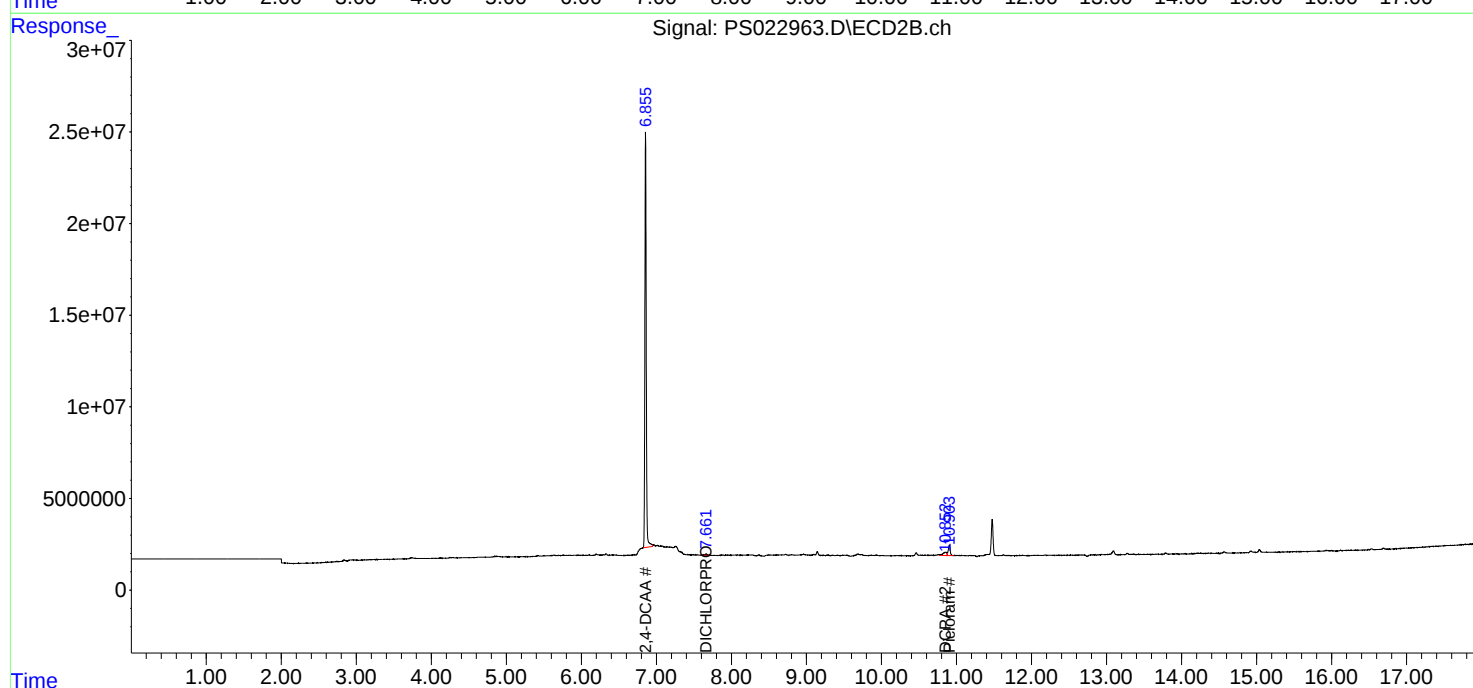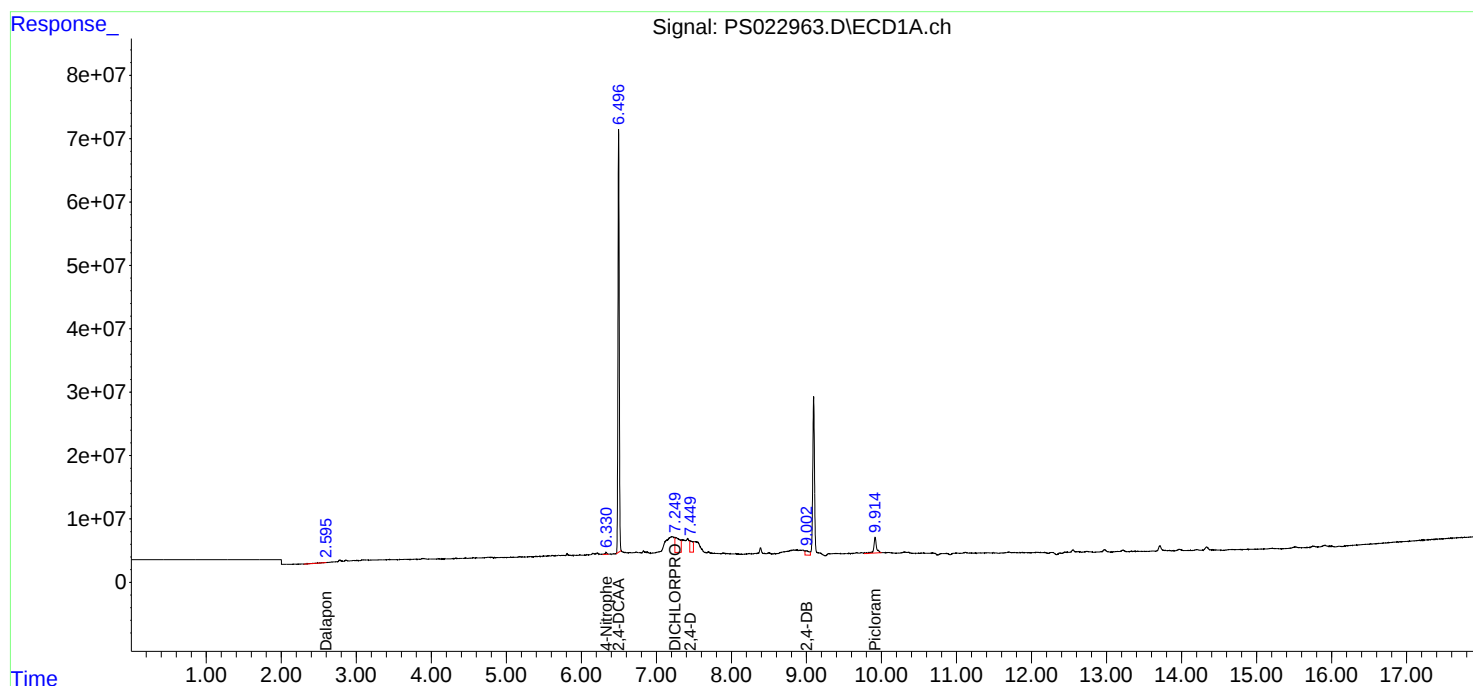


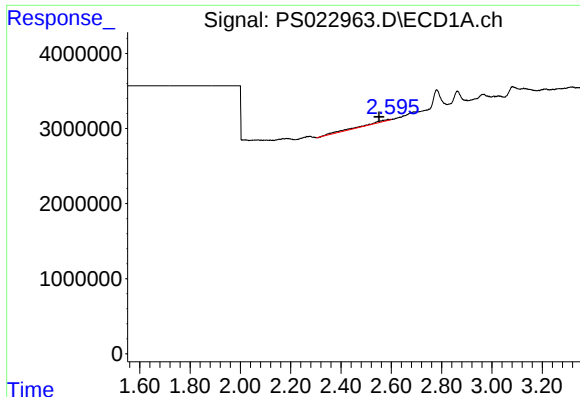

#1 Dalapon


R.T.: 2.586 min
Delta R.T.: 0.035 min
Response: 1719243
Conc: 1.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

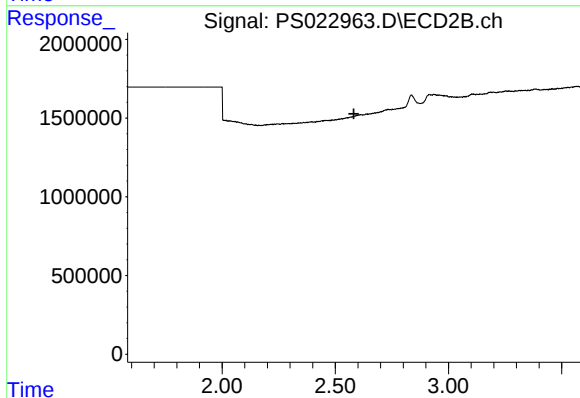


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.582 min
Response: 0
Conc: N.D.

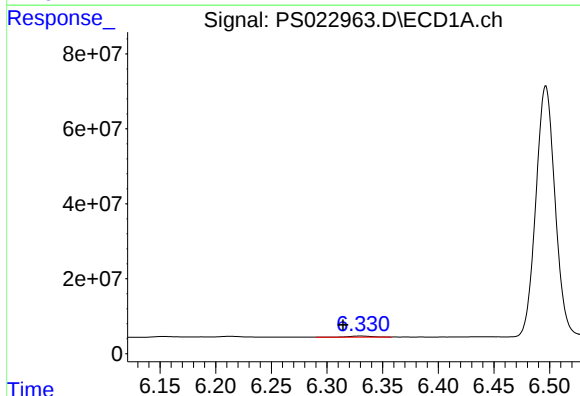


#3 4-Nitrophenol

R.T.: 6.330 min
Delta R.T.: 0.016 min
Response: 4729278
Conc: 4.49 ng/ml

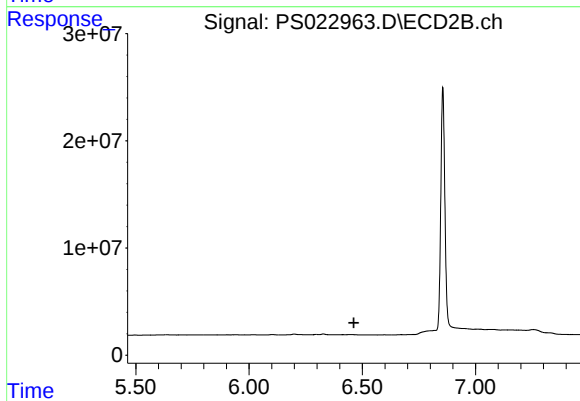

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

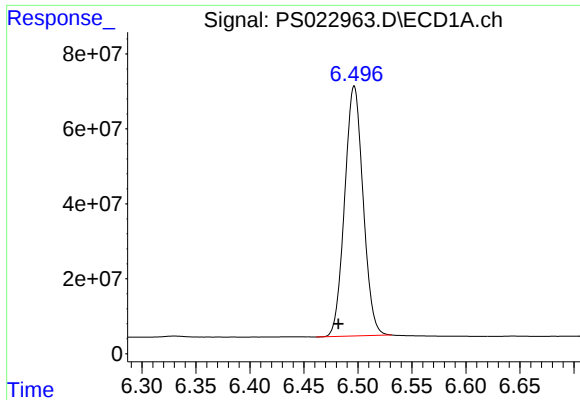

#4 2,4-DCAA


R.T.: 6.497 min
Delta R.T.: 0.015 min
Response: 793242915
Conc: 521.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

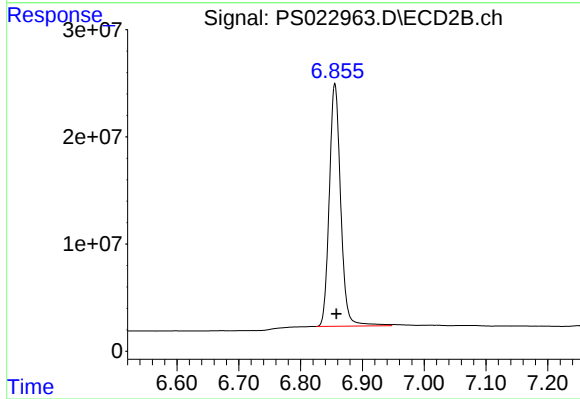


#4 2,4-DCAA

R.T.: 6.856 min
Delta R.T.: -0.002 min
Response: 290256505
Conc: 517.28 ng/ml

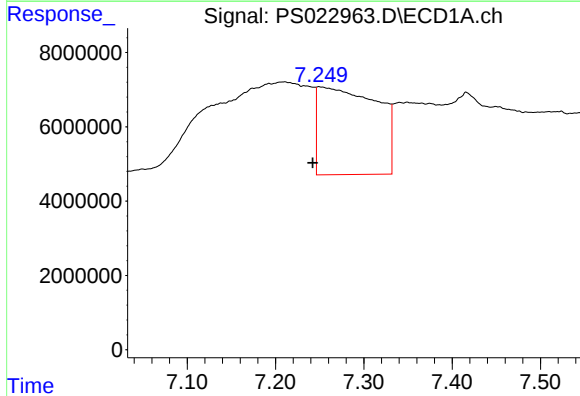


#8 DICHLORPROP

R.T.: 7.249 min
Delta R.T.: 0.007 min
Response: 109885573
Conc: 58.63 ng/ml

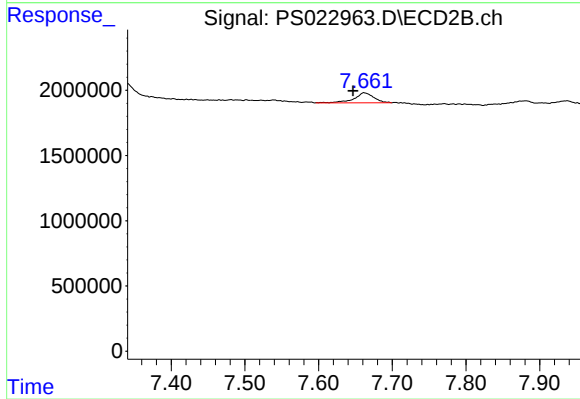

#8 DICHLORPROP


R.T.: 7.662 min
Delta R.T.: 0.015 min
Response: 1412073
Conc: 2.28 ng/ml

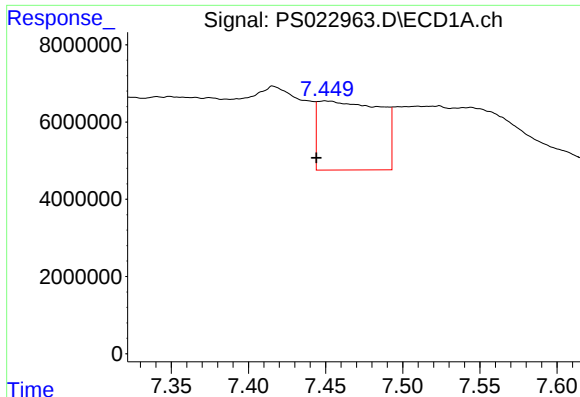

#9 2,4-D


R.T.: 7.450 min
Delta R.T.: 0.006 min
Response: 49962524
Conc: 21.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

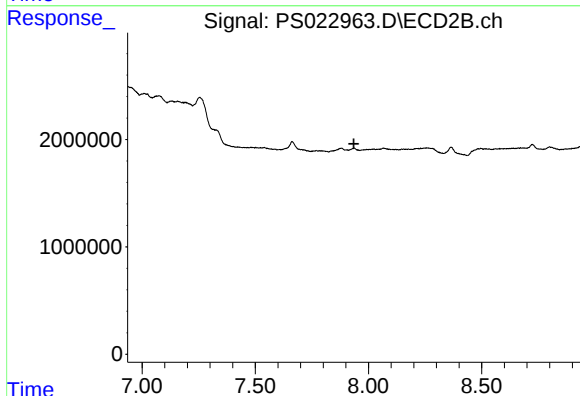


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.935 min
Response: 0
Conc: N.D.

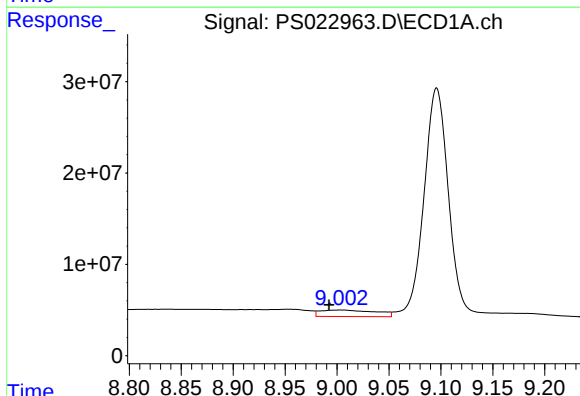


#13 2,4-DB

R.T.: 9.003 min
Delta R.T.: 0.011 min
Response: 26545735
Conc: 11.32 ng/ml

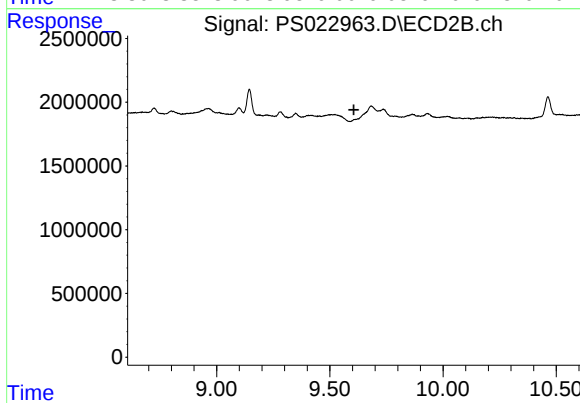

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

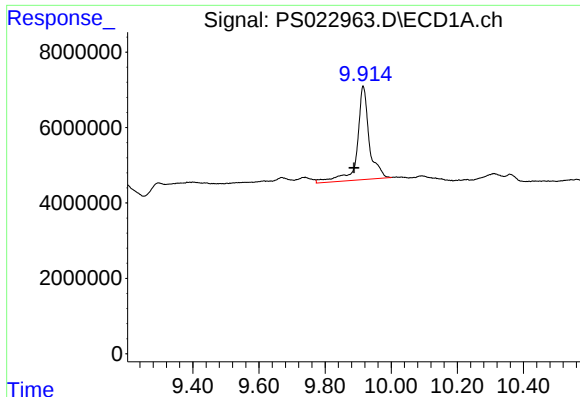

#15 Picloram


R.T.: 9.915 min
Delta R.T.: 0.027 min
Response: 62615971
Conc: 3.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

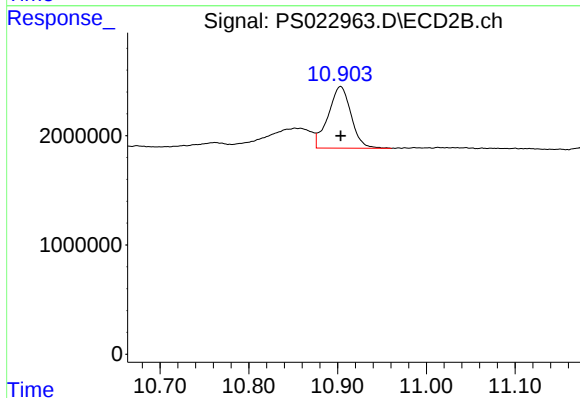


#15 Picloram

R.T.: 10.903 min
Delta R.T.: 0.000 min
Response: 10112063
Conc: 2.37 ng/ml

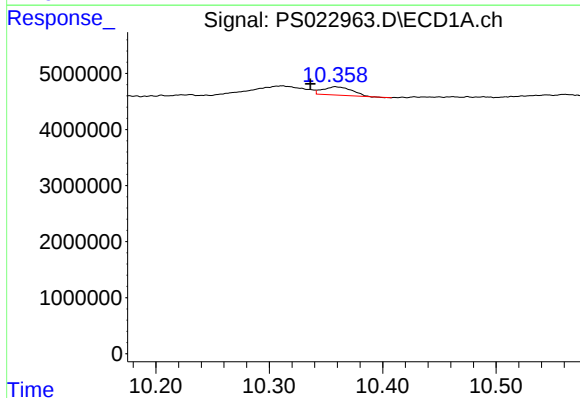

#16 DCPA

R.T.: 10.359 min
Delta R.T.: 0.023 min
Response: 2635504
Conc: N.D.

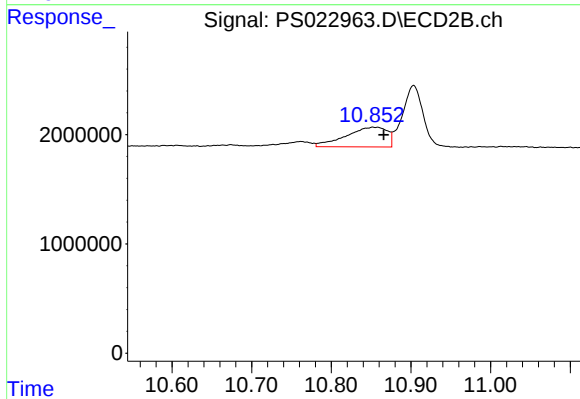

#16 DCPA

R.T.: 10.852 min
Delta R.T.: -0.014 min
Response: 6516108
Conc: 1.74 ng/ml