

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051023\
 Data File : PS022985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 03:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 04:08:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.481	6.857	772.9E6	289.2E6	508.128	515.377
Target Compounds							
1) T	Dalapon	2.560	0.000	1154615	0	<MDL	N.D. #
3) T	4-Nitroph...	6.313	6.447	16284475	1368448	15.468	4.124 #
6) T	MCP	6.816	0.000	12444656	0	2.663	N.D. #
8) T	DICHLORPROP	7.258	7.664	4300133	9386624	2.294	15.168 #
9) T	2,4-D	7.451	7.879f	4061156	3387581	1.755	4.735 #
10) T	Pentachlo...	7.674	8.364	2687951	3253814	<MDL	<MDL #
11) T	2,4,5-TP ...	8.211	8.724	7570362	1497304	<MDL	<MDL #
12) T	2,4,5-T	8.476	9.098	12165420	2090280	1.053	<MDL #
13) T	2,4-DB	8.982	0.000	32455977	0	13.834	N.D. #
14) T	DINOSEB	10.070	0.000	1126399	0	<MDL	N.D. #
15) T	Picloram	9.888	10.902	25814064	3814361	1.505	<MDL #
16) T	DCPA	10.335	10.865	3427845	995547	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051023\
Data File : PS022985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 03:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 04:08:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

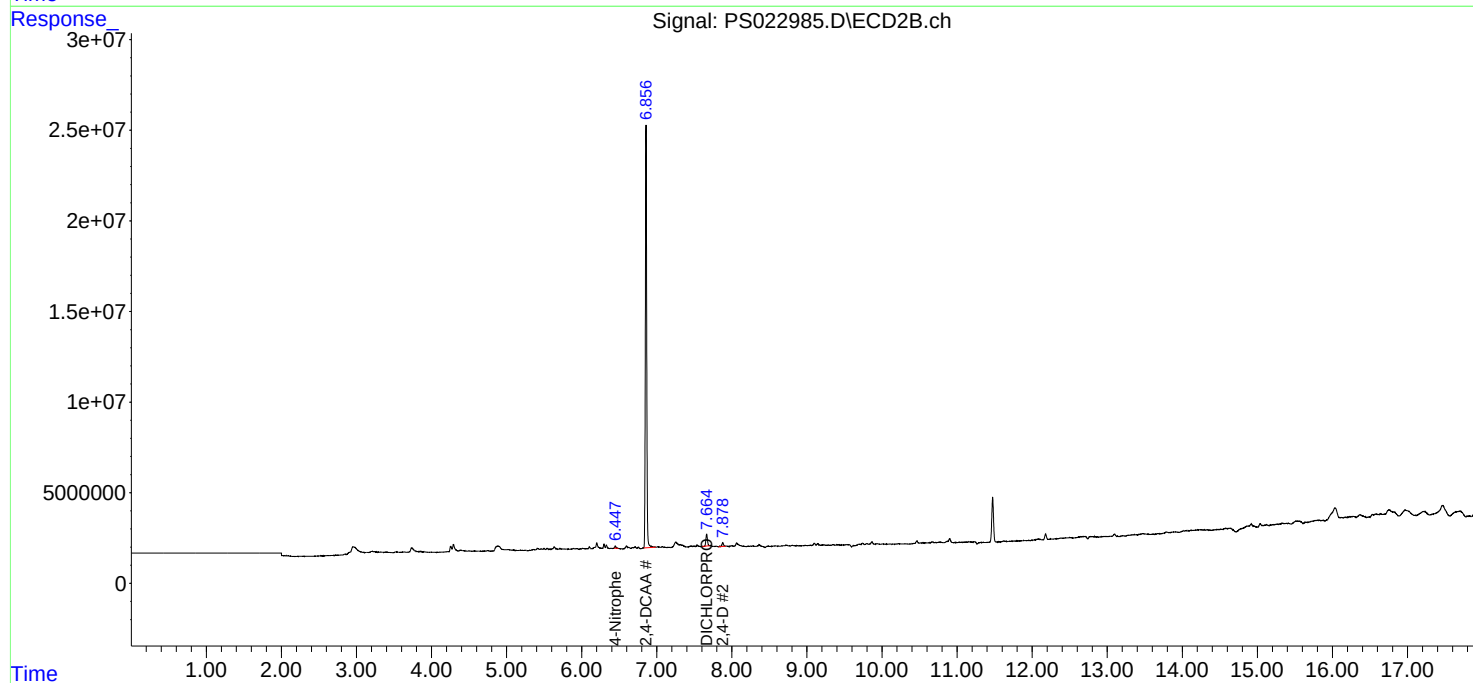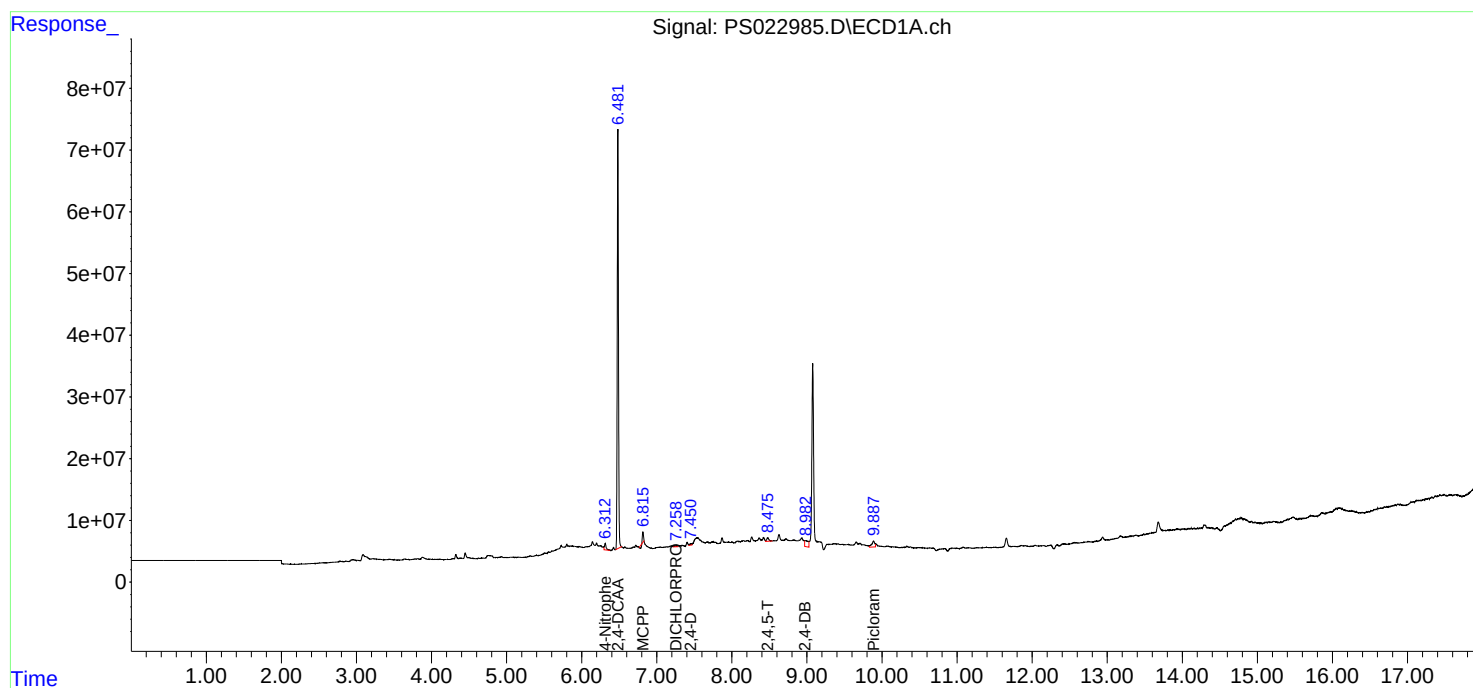


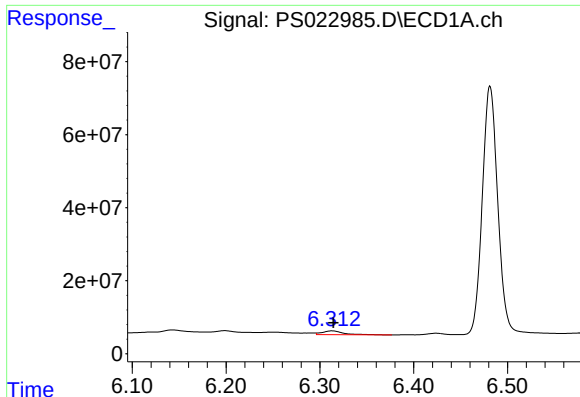

#3 4-Nitrophenol


R.T.: 6.313 min
Delta R.T.: -0.001 min
Response: 16284475
Conc: 15.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

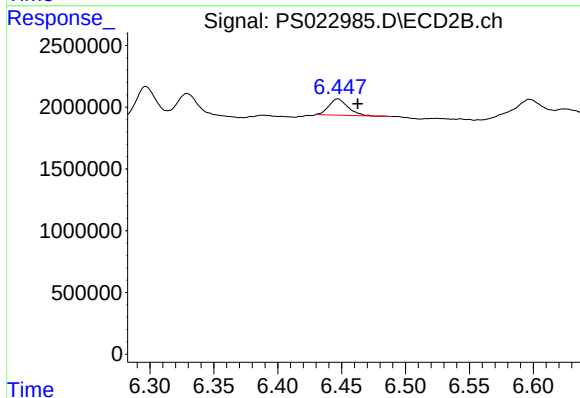


#3 4-Nitrophenol

R.T.: 6.447 min
Delta R.T.: -0.016 min
Response: 1368448
Conc: 4.12 ng/ml

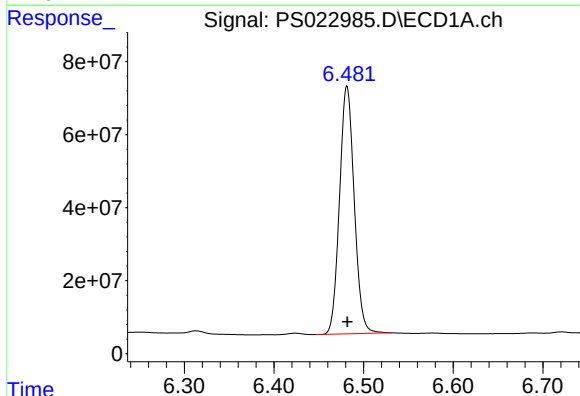


#4 2,4-DCAA

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 772860359
Conc: 508.13 ng/ml

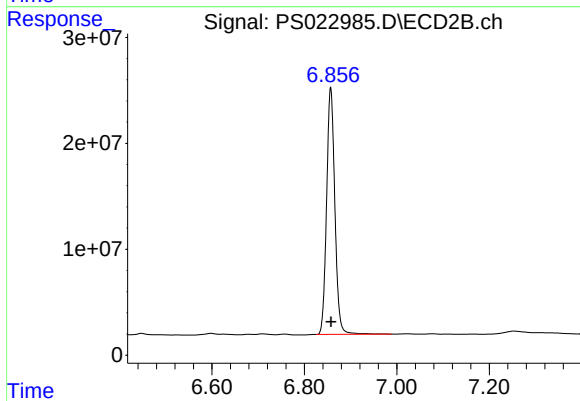

#4 2,4-DCAA


R.T.: 6.857 min
Delta R.T.: -0.001 min
Response: 289186018
Conc: 515.38 ng/ml

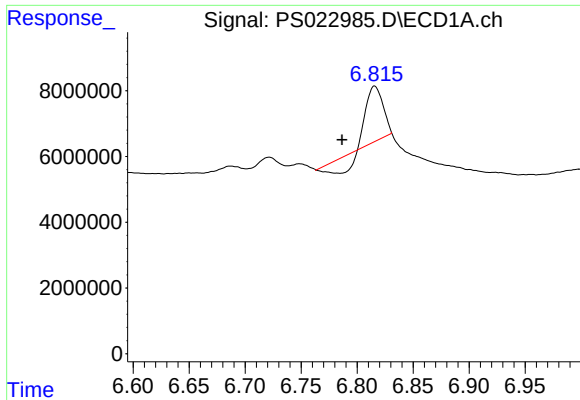

#6 MCP


R.T.: 6.816 min
Delta R.T.: 0.029 min
Response: 12444656
Conc: 2.66 ug/ml

Instrument :
ECD_S
ClientSampleId :

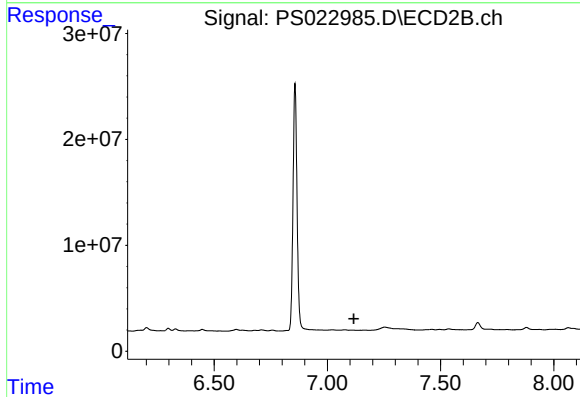


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

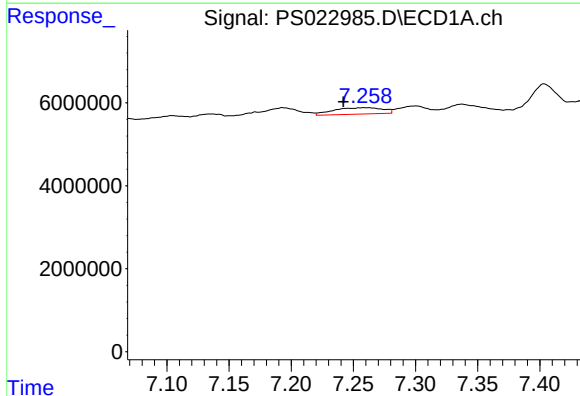


#8 DICHLORPROP

R.T.: 7.258 min
Delta R.T.: 0.016 min
Response: 4300133
Conc: 2.29 ng/ml

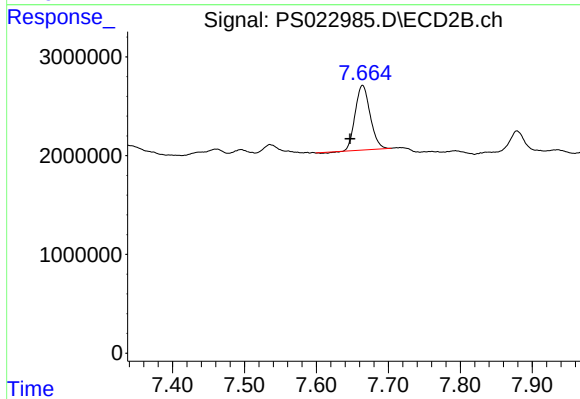

#8 DICHLORPROP


R.T.: 7.664 min
Delta R.T.: 0.017 min
Response: 9386624
Conc: 15.17 ng/ml

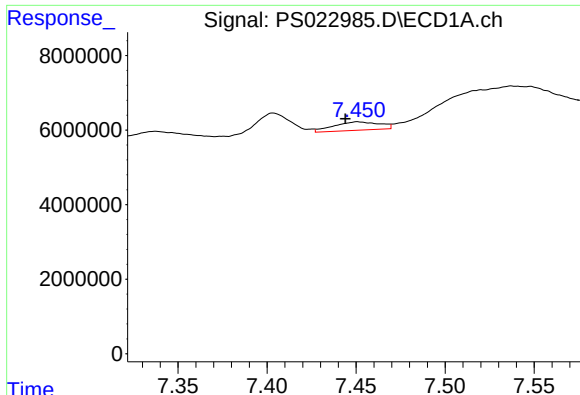

#9 2,4-D


R.T.: 7.451 min
Delta R.T.: 0.007 min
Response: 4061156
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

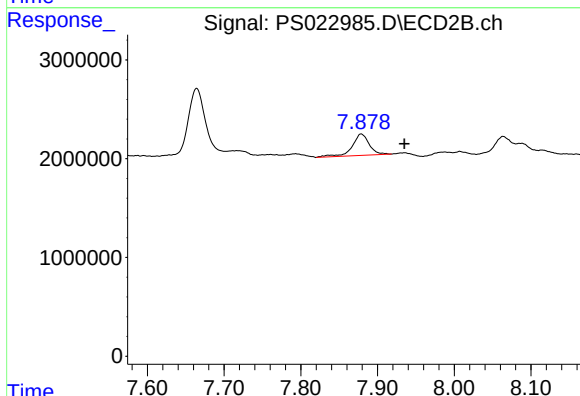


#9 2,4-D

R.T.: 7.879 min
Delta R.T.: -0.056 min
Response: 3387581
Conc: 4.74 ng/ml

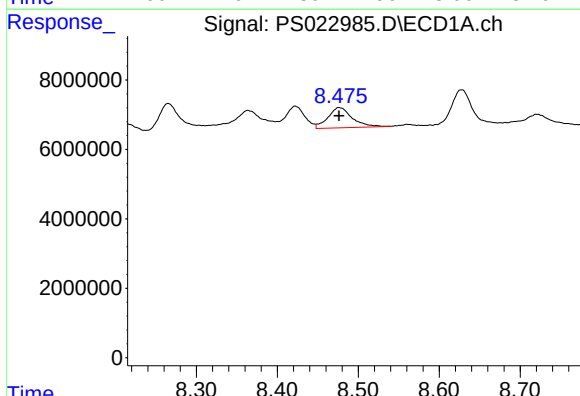


#12 2,4,5-T

R.T.: 8.476 min
Delta R.T.: 0.000 min
Response: 12165420
Conc: 1.05 ng/ml

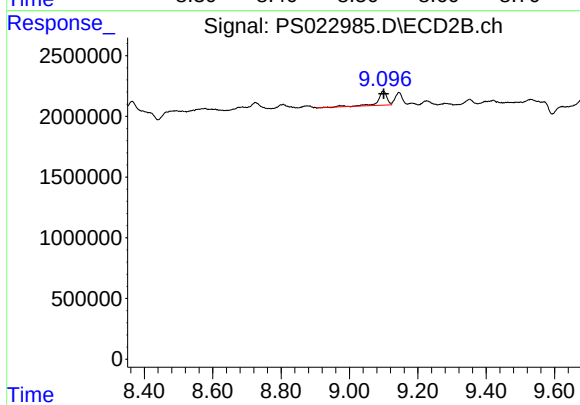

#12 2,4,5-T


R.T.: 9.098 min
Delta R.T.: -0.001 min
Response: 2090280
Conc: N.D.

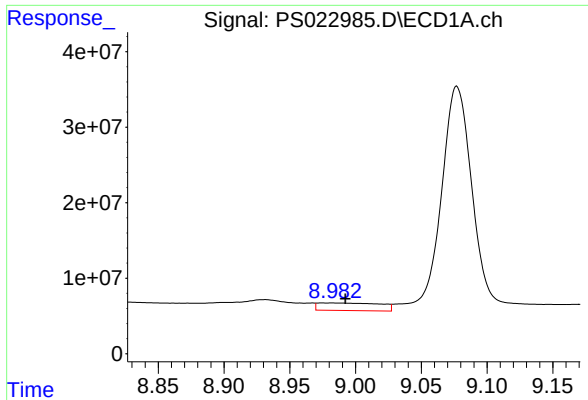

#13 2,4-DB


R.T.: 8.982 min
Delta R.T.: -0.010 min
Response: 32455977
Conc: 13.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

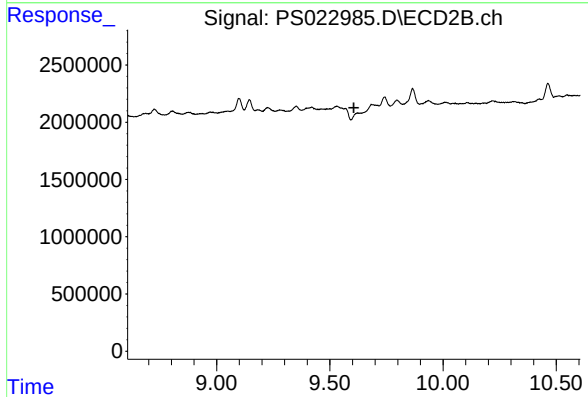


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

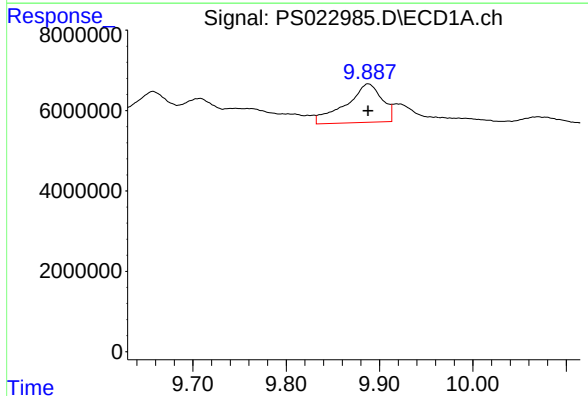

#15 Picloram

R.T.: 9.888 min
Delta R.T.: 0.000 min
Response: 25814064
Conc: 1.51 ng/ml

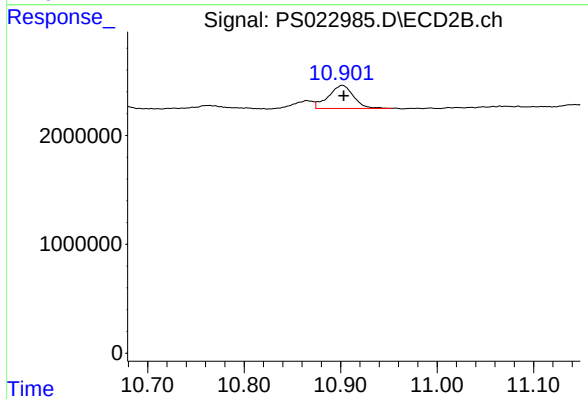

#15 Picloram

R.T.: 10.902 min
Delta R.T.: -0.002 min
Response: 3814361
Conc: N.D.