

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051024\
 Data File : PS026732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 19:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 01:09:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
 Quant Title : 8080.M
 QLast Update : Mon May 06 13:55:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.266	7.778	1226.5E6	859.1E6	493.201	515.224
Target Compounds							
1) T	Dalapon	2.694f	2.740f	22120848	5366011	6.048	1.830 #
2) T	3,5-DICHL...	6.416f	0.000	19084660	0	5.549	N.D. #
3) T	4-Nitroph...	7.061	7.275f	6917675	1394678	4.294	1.226 #
5) T	DICAMBA	7.452	7.972	916699	2253183	<MDL	<MDL #
6) T	MCP	7.604f	8.089	273833	12145786	<MDL	2.363 #
7) T	MCPA	7.800	0.000	385514	0	<MDL	N.D. #
8) T	DICHLORPROP	8.194	8.748f	2640662	17421529	<MDL	9.080 #
9) T	2,4-D	8.408	0.000	69104800	0	20.993	N.D. #
10) T	Pentachlo...	8.689	9.556	2070798	4033002	<MDL	<MDL #
11) T	2,4,5-TP ...	9.268	9.929	5568272	3521471	<MDL	<MDL #
12) T	2,4,5-T	9.559	10.352	3076816	2775639	<MDL	<MDL #
13) T	2,4-DB	10.153	10.951f	174537	1014469	<MDL	<MDL #
14) T	DINOSEB	0.000	11.298	0	1090252	N.D.	<MDL
15) T	Picloram	11.156	12.389	958.8E6	7535964	42.924	<MDL #
16) T	DCPA	11.684f	12.389f	-1001247	7535964	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051024\
Data File : PS026732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 19:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 01:09:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050624.M
Quant Title : 8080.M
QLast Update : Mon May 06 13:55:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

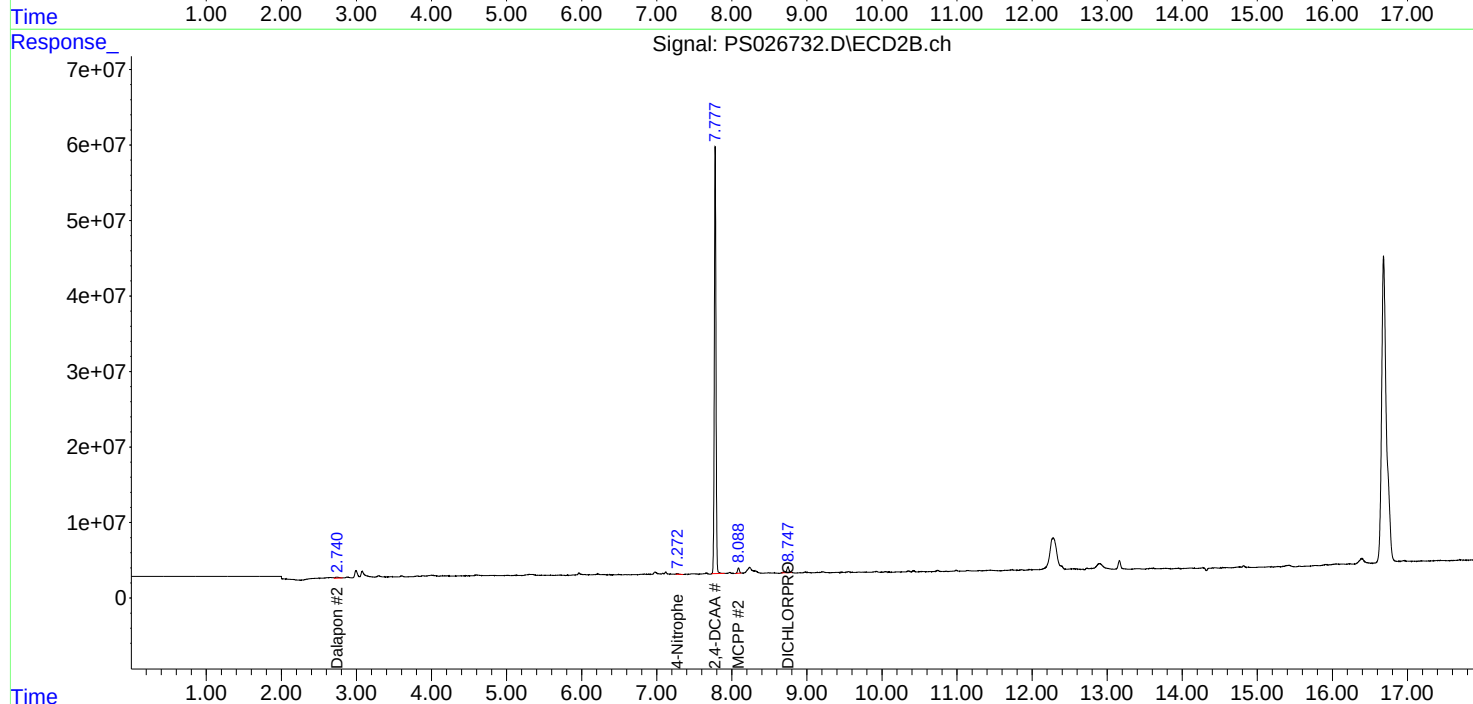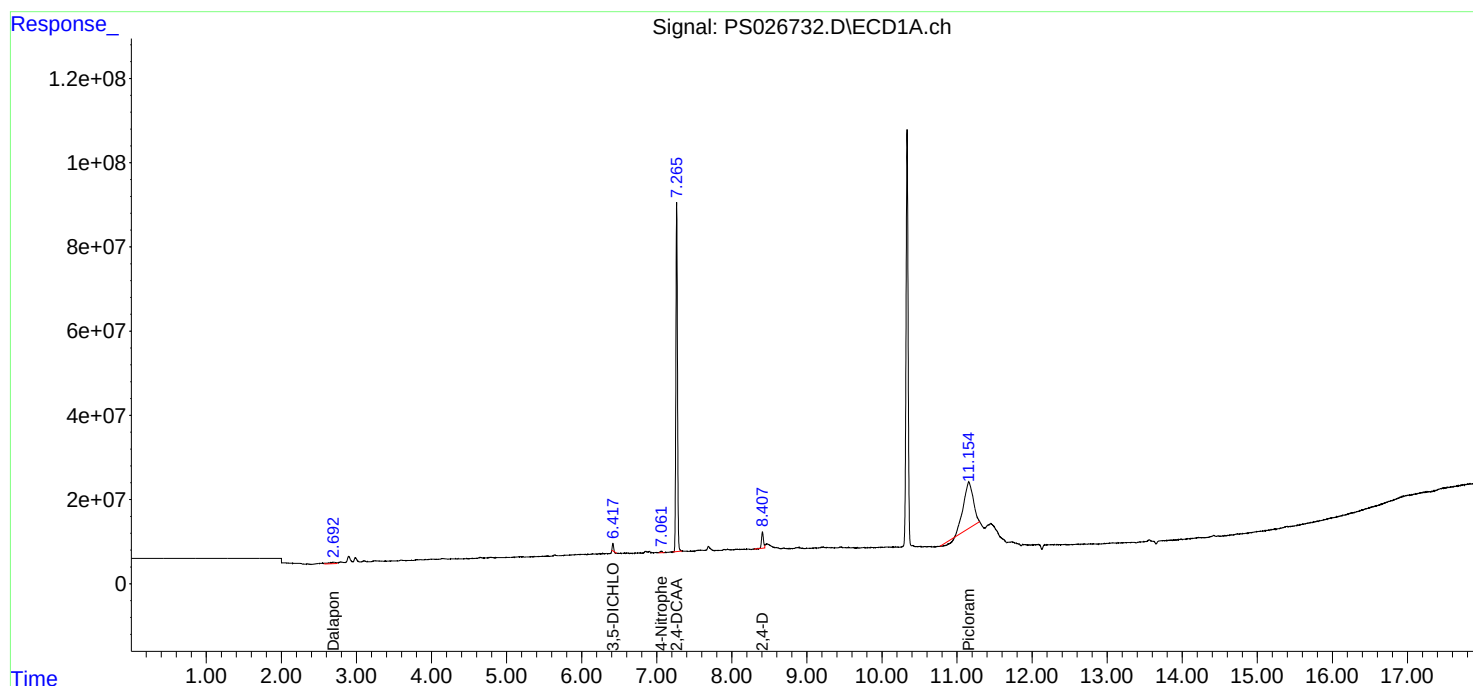


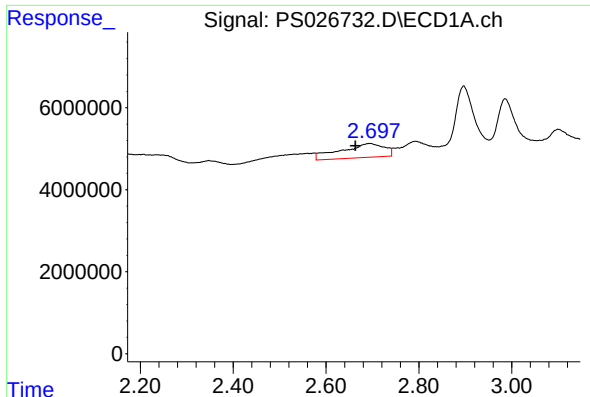

#1 Dalapon


R.T.: 2.694 min
Delta R.T.: 0.031 min
Response: 22120848
Conc: 6.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

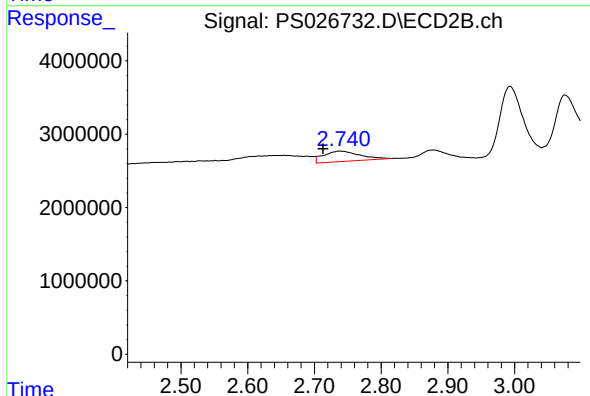


#1 Dalapon

R.T.: 2.740 min
Delta R.T.: 0.027 min
Response: 5366011
Conc: 1.83 ng/ml

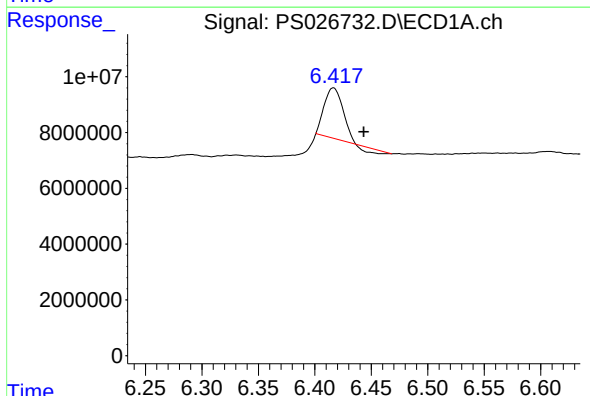


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.416 min
Delta R.T.: -0.027 min
Response: 19084660
Conc: 5.55 ng/ml

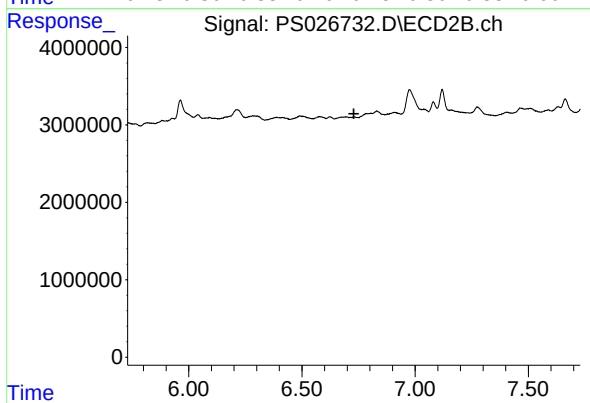

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.730 min
Response: 0
Conc: N.D.

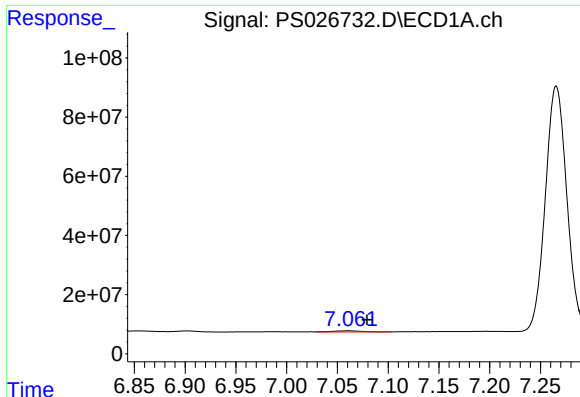

#3 4-Nitrophenol


R.T.: 7.061 min
Delta R.T.: -0.019 min
Response: 6917675
Conc: 4.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

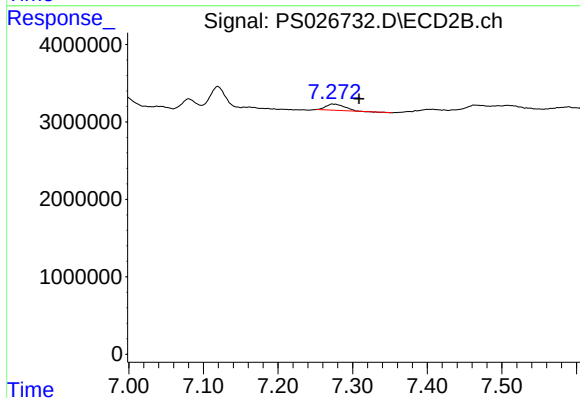


#3 4-Nitrophenol

R.T.: 7.275 min
Delta R.T.: -0.034 min
Response: 1394678
Conc: 1.23 ng/ml

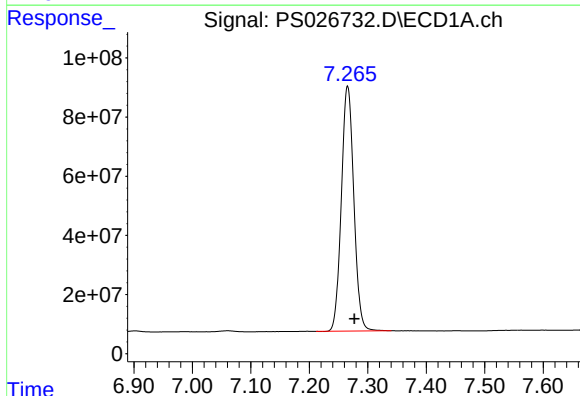


#4 2,4-DCAA

R.T.: 7.266 min
Delta R.T.: -0.012 min
Response: 1226519545
Conc: 493.20 ng/ml

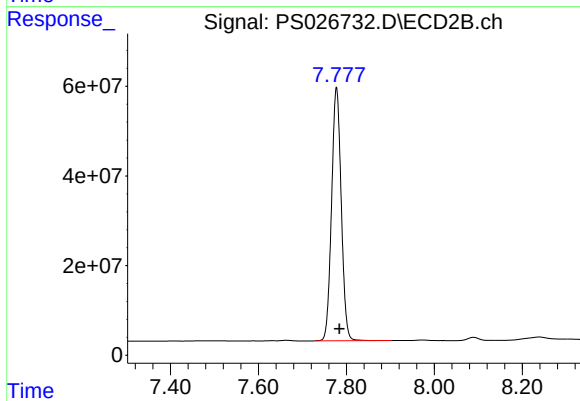

#4 2,4-DCAA


R.T.: 7.778 min
Delta R.T.: -0.006 min
Response: 859092018
Conc: 515.22 ng/ml

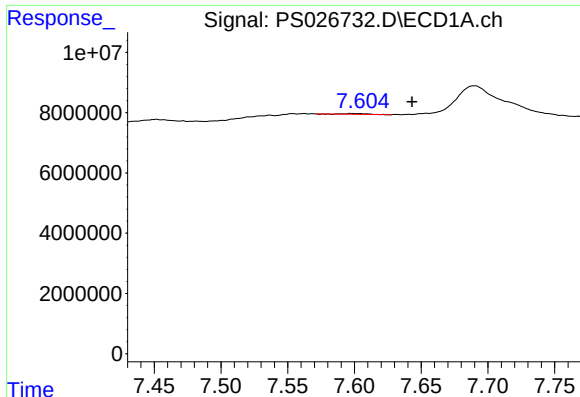

#6 MCP


R.T.: 7.604 min
Delta R.T.: -0.039 min
Response: 273833
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

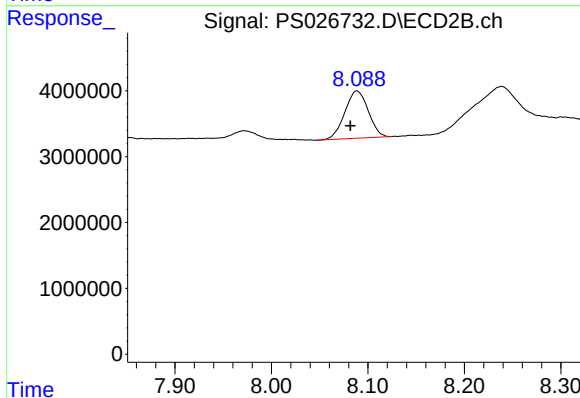


#6 MCP

R.T.: 8.089 min
Delta R.T.: 0.007 min
Response: 12145786
Conc: 2.36 ug/ml

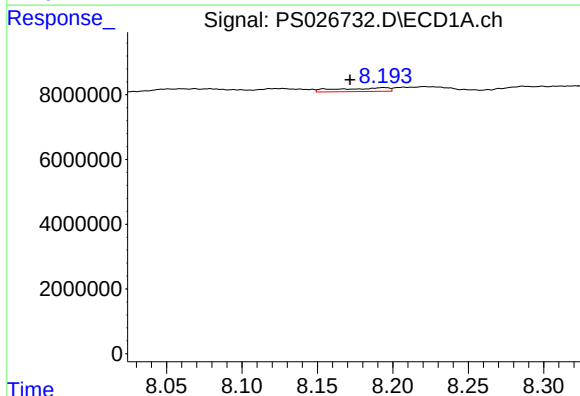


#8 DICHLORPROP

R.T.: 8.194 min
Delta R.T.: 0.022 min
Response: 2640662
Conc: N.D.

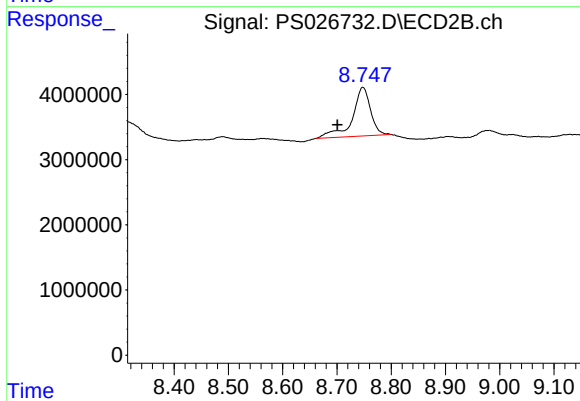

#8 DICHLORPROP


R.T.: 8.748 min
Delta R.T.: 0.047 min
Response: 17421529
Conc: 9.08 ng/ml

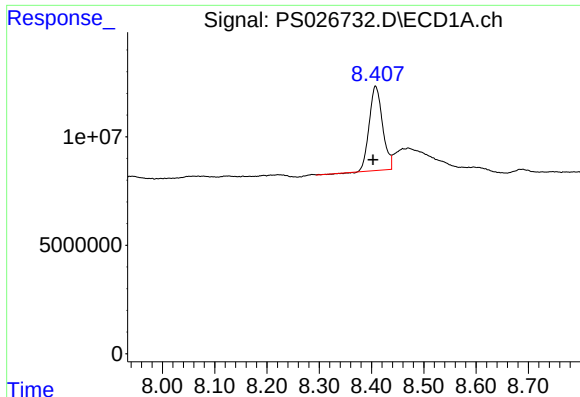

#9 2,4-D


R.T.: 8.408 min
Delta R.T.: 0.005 min
Response: 69104800
Conc: 20.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

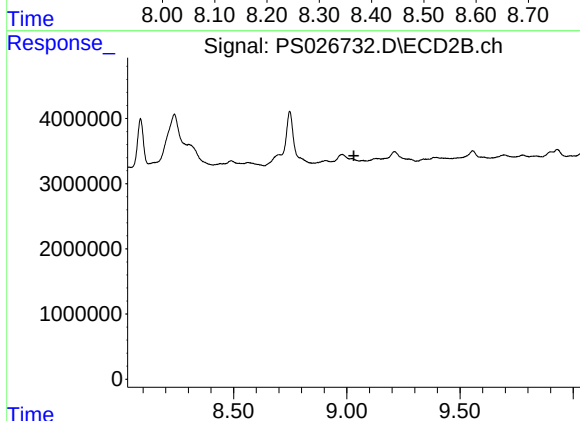


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 9.031 min
Response: 0
Conc: N.D.

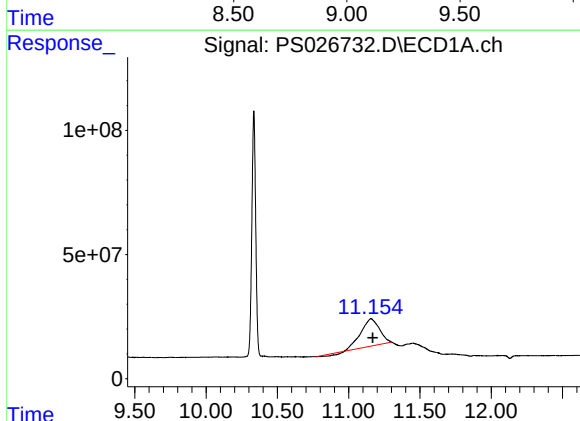

#15 Picloram

R.T.: 11.156 min
Delta R.T.: -0.012 min
Response: 958799300
Conc: 42.92 ng/ml

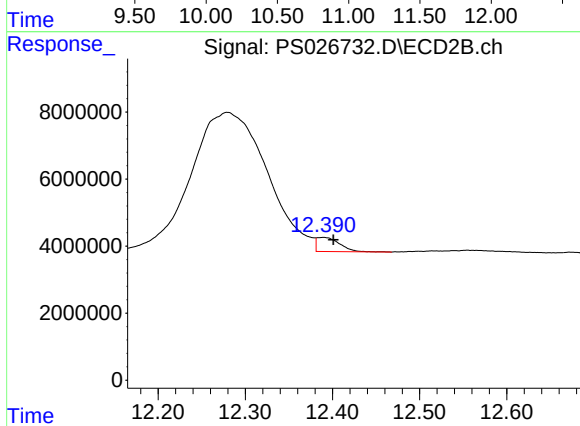

#15 Picloram

R.T.: 12.389 min
Delta R.T.: -0.012 min
Response: 7535964
Conc: N.D.