

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051119\
 Data File : PS004559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2019 16:33
 Operator : EI\SJ
 Sample : K2750-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 72-11995

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:12:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051019.M
 Quant Title : 8080.M
 QLast Update : Sat May 11 04:17:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.999	5.694	248.1E6	191.5E6	391.340	404.767
Target Compounds							
1) T	Dalapon	2.364	2.028	158.4E6	50350383	178.068	81.091 #
2) T	3,5-DICHL...	5.417	5.006	2908891	175.7E6	3.477	278.976 #
3) T	4-Nitroph...	5.894	5.355	8432338	24691269	39.195	119.898 #
5) T	DICAMBA	6.189	5.801	3636565	11169374	1.424	5.755 #
8) T	DICHLORPROP	0.000	6.392	0	9686666	N.D.	20.786
10) T	Pentachlo...	7.364	7.044	5183306	3442556	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	7.352	0	111.0E6	N.D.	42.195
12) T	2,4,5-T	0.000	7.827	0	7010687	N.D.	3.010
15) T	Picloram	9.630	9.528	25483640	16378723	6.209	4.648 #
16) T	DCPA	0.000	9.528	0	16378723	N.D.	4.851



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051119\
Data File : PS004559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2019 16:33
Operator : EI\SJ
Sample : K2750-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
72-11995

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:12:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051019.M
Quant Title : 8080.M
QLast Update : Sat May 11 04:17:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

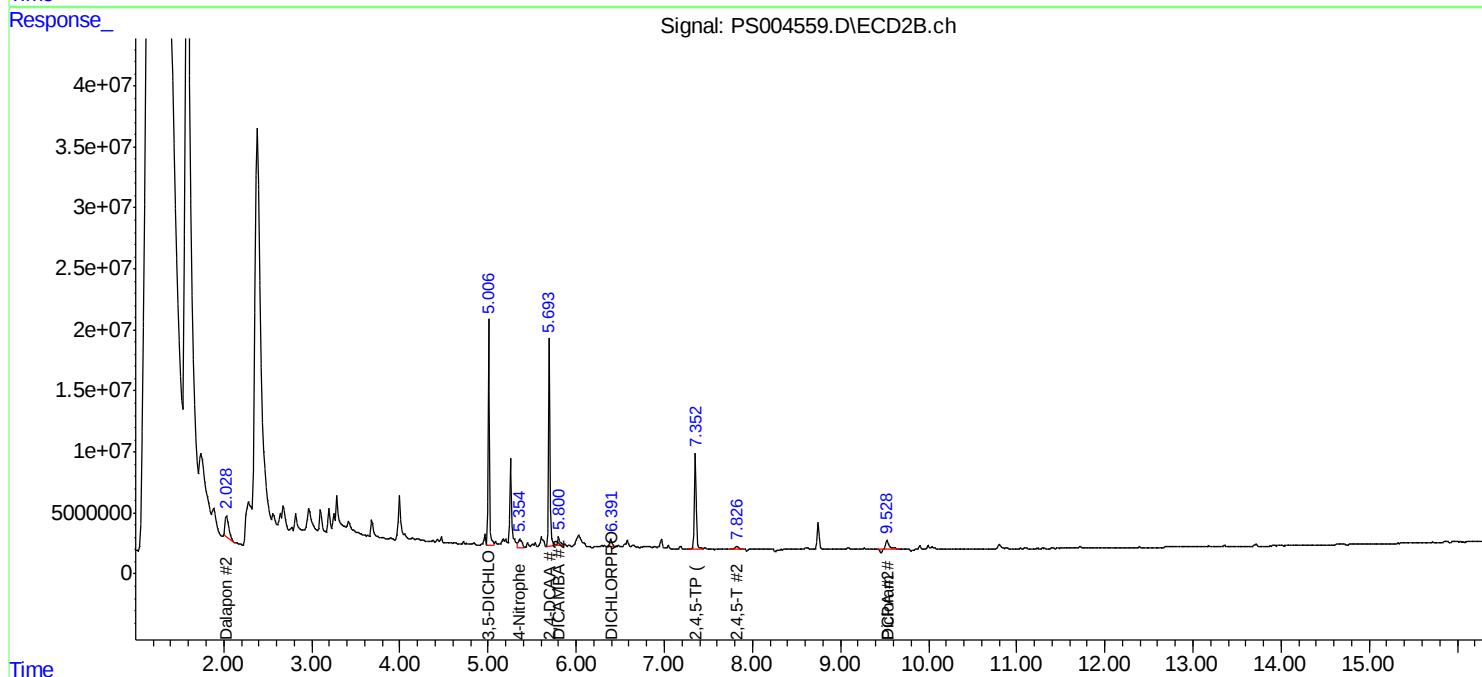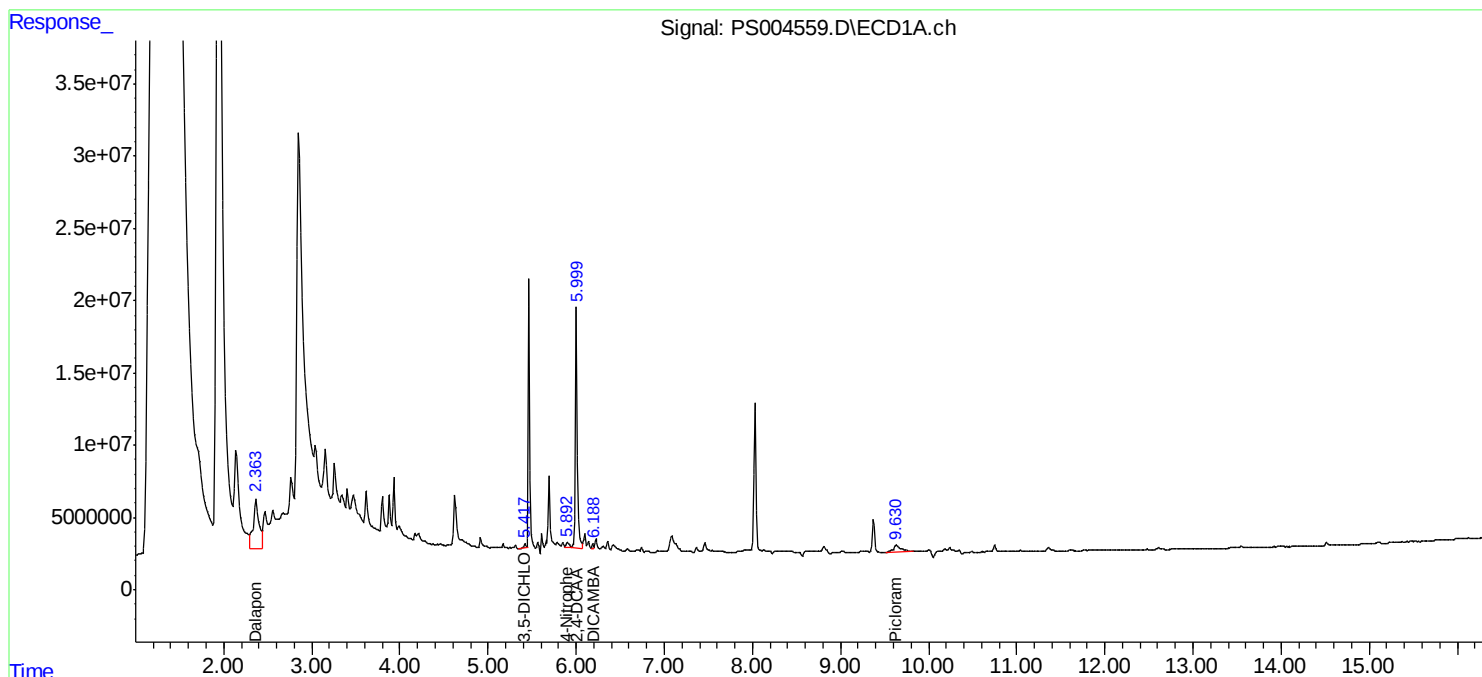


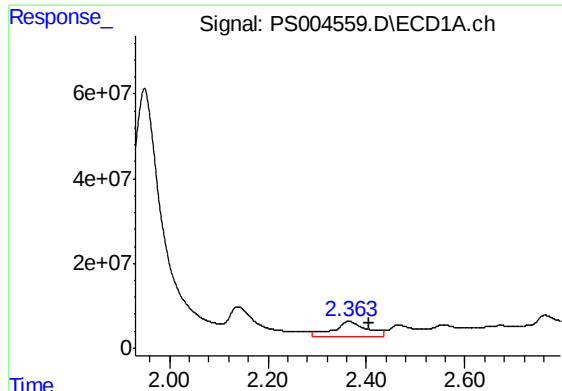

#1 Dalapon


R.T.: 2.364 min
Delta R.T.: -0.042 min
Response: 158442534
Conc: 178.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11995

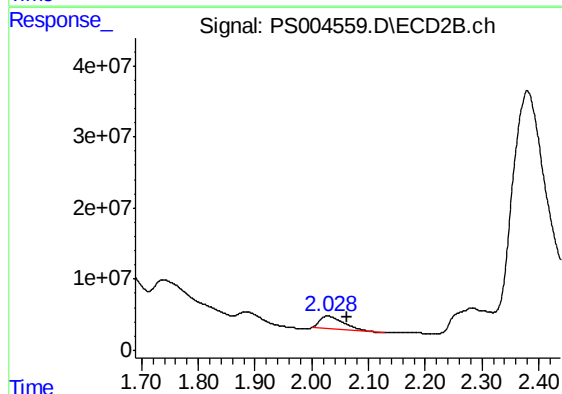


#1 Dalapon

R.T.: 2.028 min
Delta R.T.: -0.036 min
Response: 50350383
Conc: 81.09 ng/ml

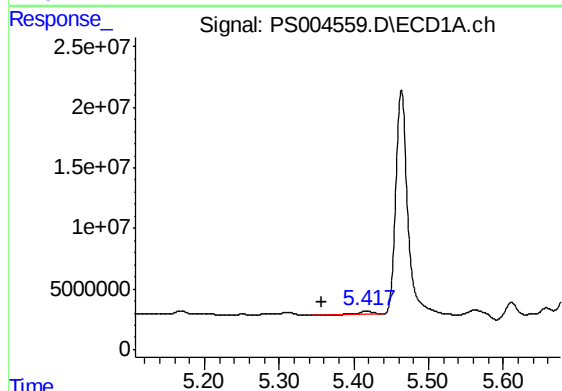


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.417 min
Delta R.T.: 0.060 min
Response: 2908891
Conc: 3.48 ng/ml

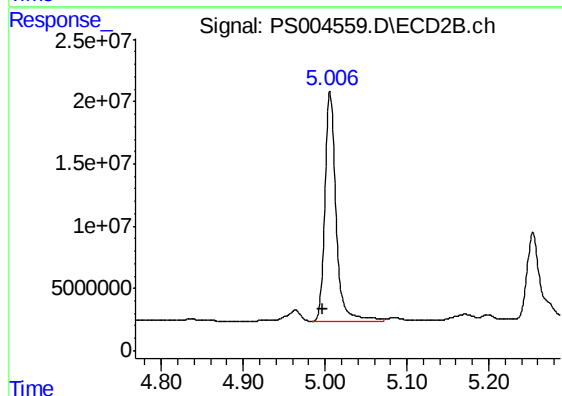

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.006 min
Delta R.T.: 0.010 min
Response: 175716663
Conc: 278.98 ng/ml

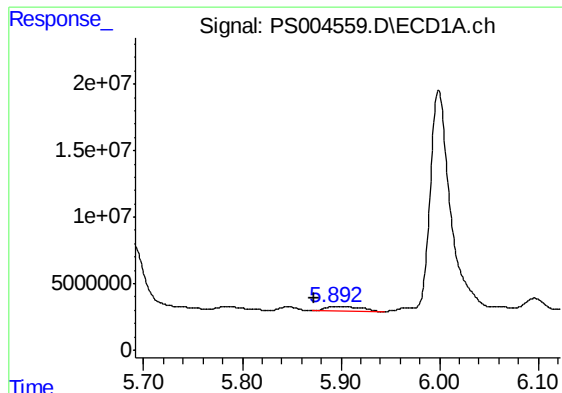

#3 4-Nitrophenol


R.T.: 5.894 min
Delta R.T.: 0.021 min
Response: 8432338
Conc: 39.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11995

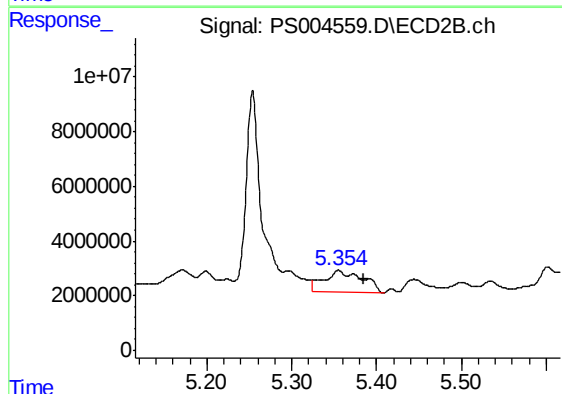


#3 4-Nitrophenol

R.T.: 5.355 min
Delta R.T.: -0.030 min
Response: 24691269
Conc: 119.90 ng/ml

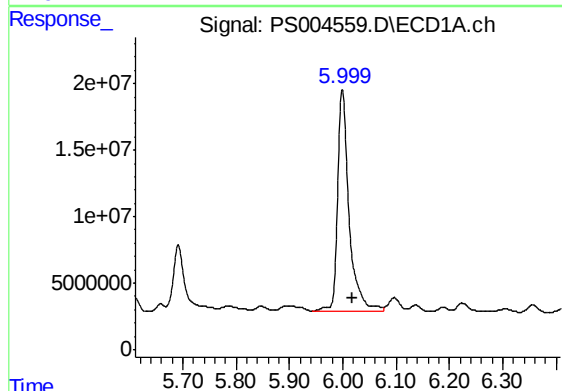


#4 2,4-DCAA

R.T.: 5.999 min
Delta R.T.: -0.019 min
Response: 248078620
Conc: 391.34 ng/ml

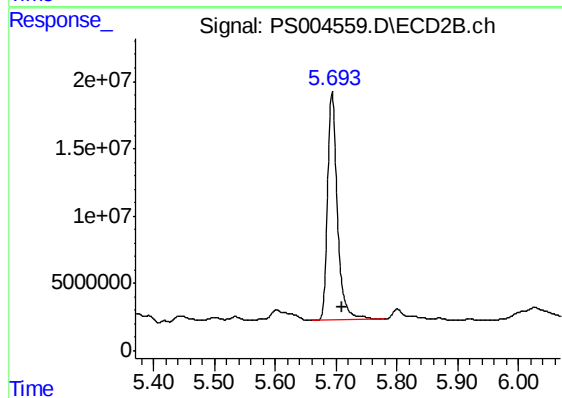

#4 2,4-DCAA


R.T.: 5.694 min
Delta R.T.: -0.017 min
Response: 191477152
Conc: 404.77 ng/ml

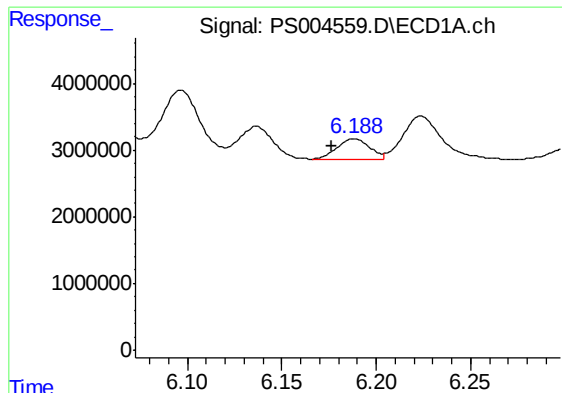

#5 DICAMBA


R.T.: 6.189 min
Delta R.T.: 0.012 min
Response: 3636565
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11995

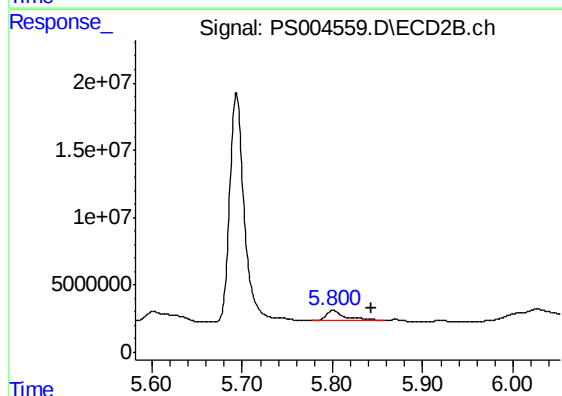


#5 DICAMBA

R.T.: 5.801 min
Delta R.T.: -0.043 min
Response: 11169374
Conc: 5.75 ng/ml

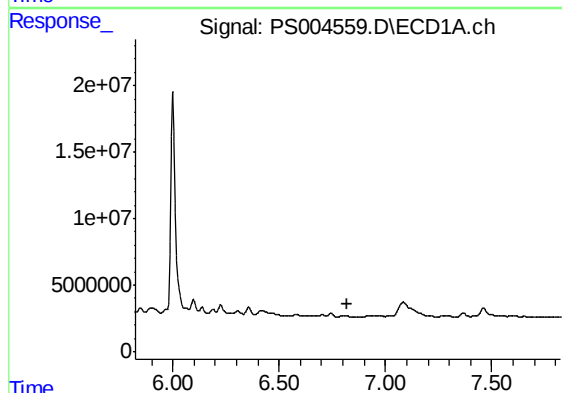


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.824 min
Response: 0
Conc: N.D.

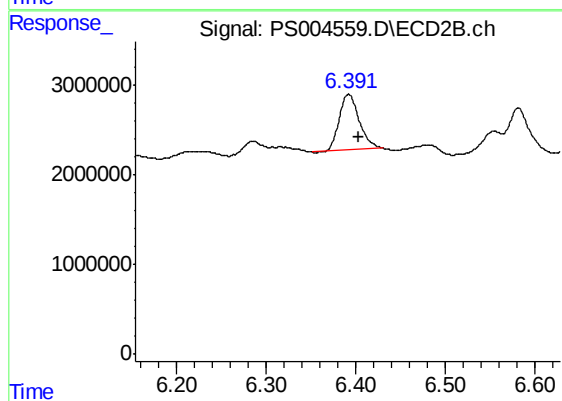

#8 DICHLORPROP


R.T.: 6.392 min
Delta R.T.: -0.012 min
Response: 9686666
Conc: 20.79 ng/ml

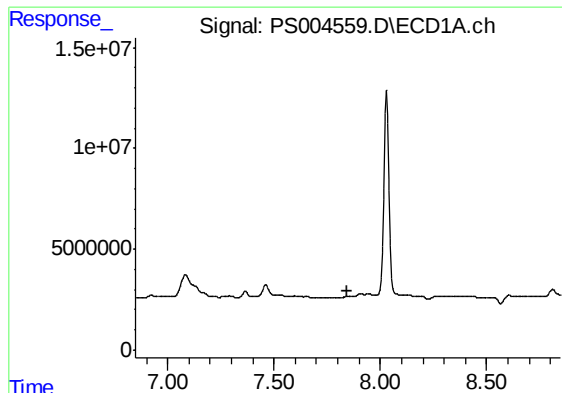

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.848 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
72-11995

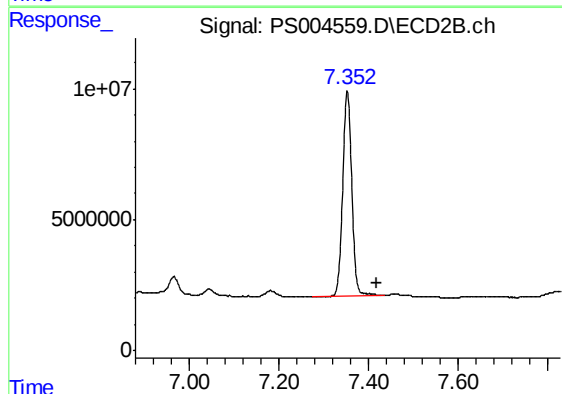


#11 2,4,5-TP (SILVEX)

R.T.: 7.352 min
Delta R.T.: -0.065 min
Response: 111041367
Conc: 42.19 ng/ml

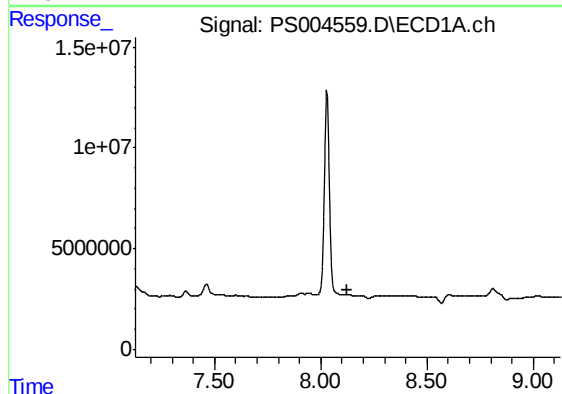


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.128 min
Response: 0
Conc: N.D.

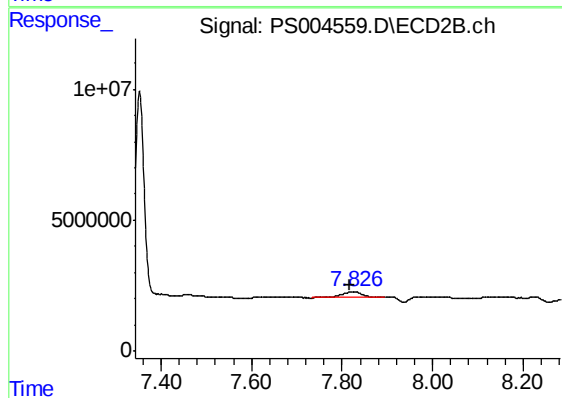

#12 2,4,5-T


R.T.: 7.827 min
Delta R.T.: 0.011 min
Response: 7010687
Conc: 3.01 ng/ml

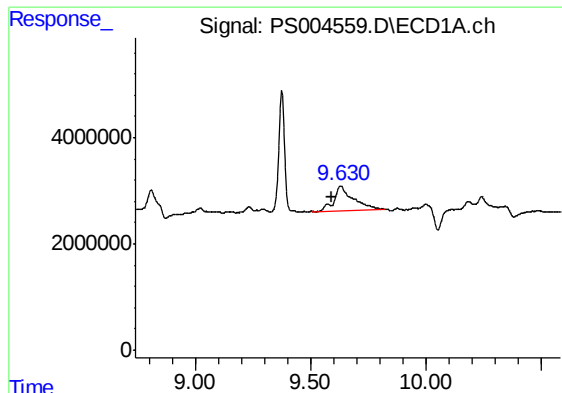

#15 Picloram


R.T.: 9.630 min
Delta R.T.: 0.035 min
Response: 25483640
Conc: 6.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11995

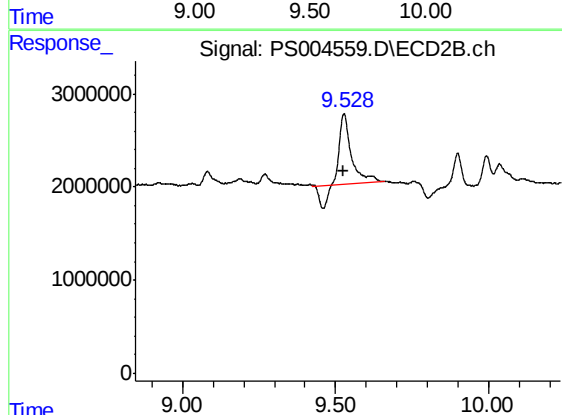


#15 Picloram

R.T.: 9.528 min
Delta R.T.: 0.001 min
Response: 16378723
Conc: 4.65 ng/ml

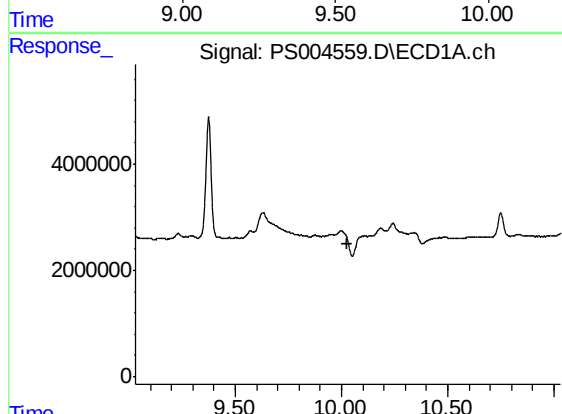

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.030 min
Response: 0
Conc: N.D.

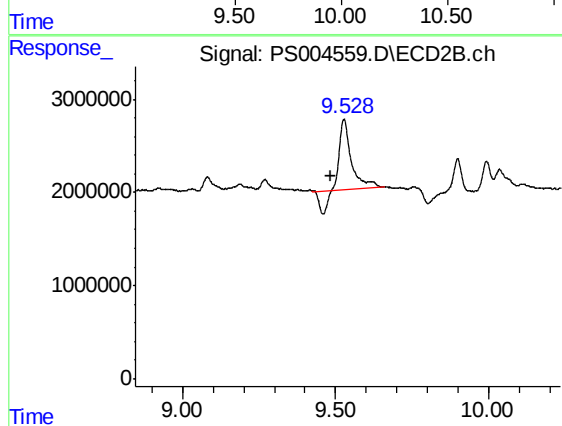

#16 DCPA

R.T.: 9.528 min
Delta R.T.: 0.044 min
Response: 16378723
Conc: 4.85 ng/ml