

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
 Data File : PS010201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2020 11:52
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 17:08:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.925	0	266438	N.D.	<MDL
Target Compounds							
1) T	Dalapon	0.000	2.638	0	433609	N.D.	<MDL
5) T	DICAMBA	0.000	7.093	0	862350	N.D.	<MDL
6) T	MCPD	0.000	7.215	0	260291	N.D.	<MDL
7) T	MCPA	0.000	7.371	0	3307975	N.D.	1.216
8) T	DICHLORPROP	0.000	7.746	0	1496742	N.D.	2.651
11) T	2,4,5-TP ...	0.000	8.802	0	1331967	N.D.	<MDL
12) T	2,4,5-T	0.000	9.186	0	2468811	N.D.	<MDL
13) T	2,4-DB	0.000	9.694	0	966569	N.D.	2.425
14) T	DINOSEB	0.000	10.025	0	566491	N.D.	<MDL
15) T	Picloram	11.032	11.007	30108811	39998664	6.567	9.474 #
16) T	DCPA	0.000	10.953	0	1829847	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
Data File : PS010201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2020 11:52
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 17:08:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

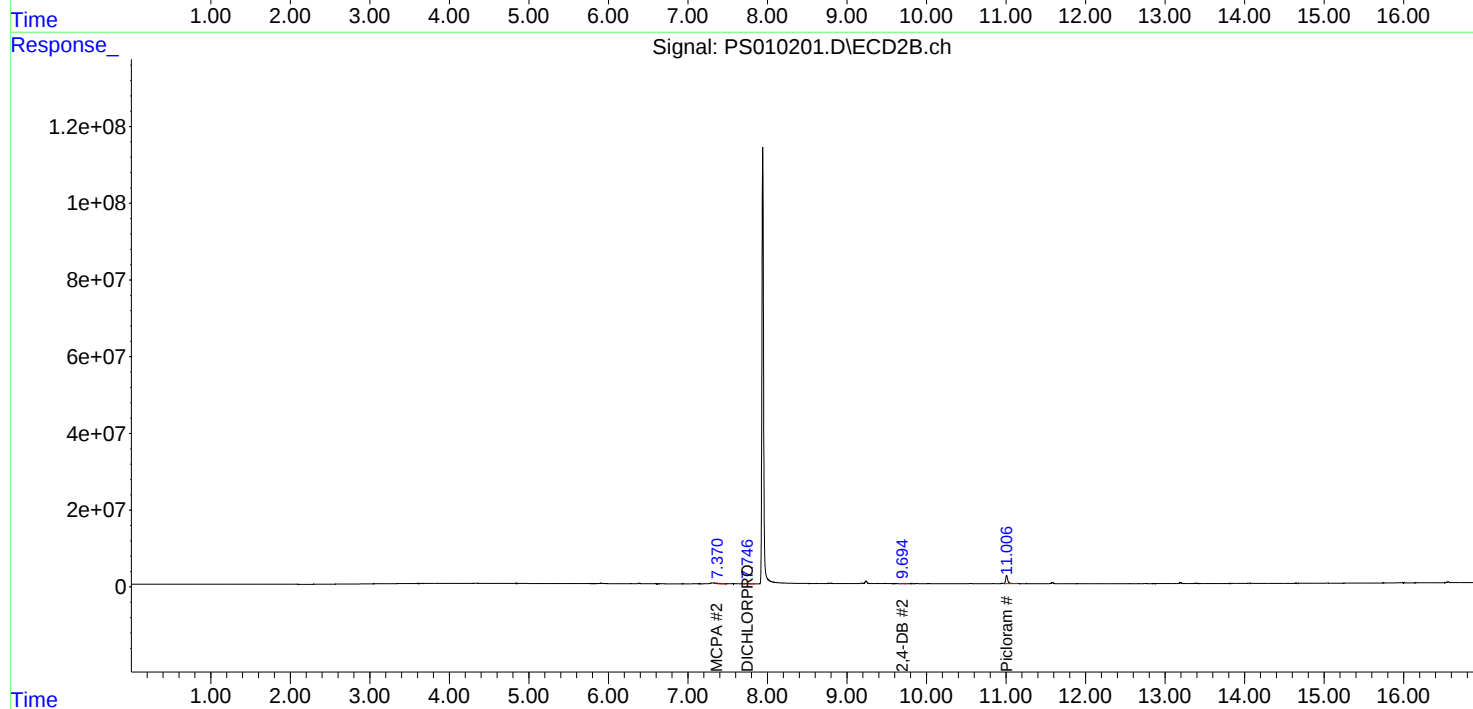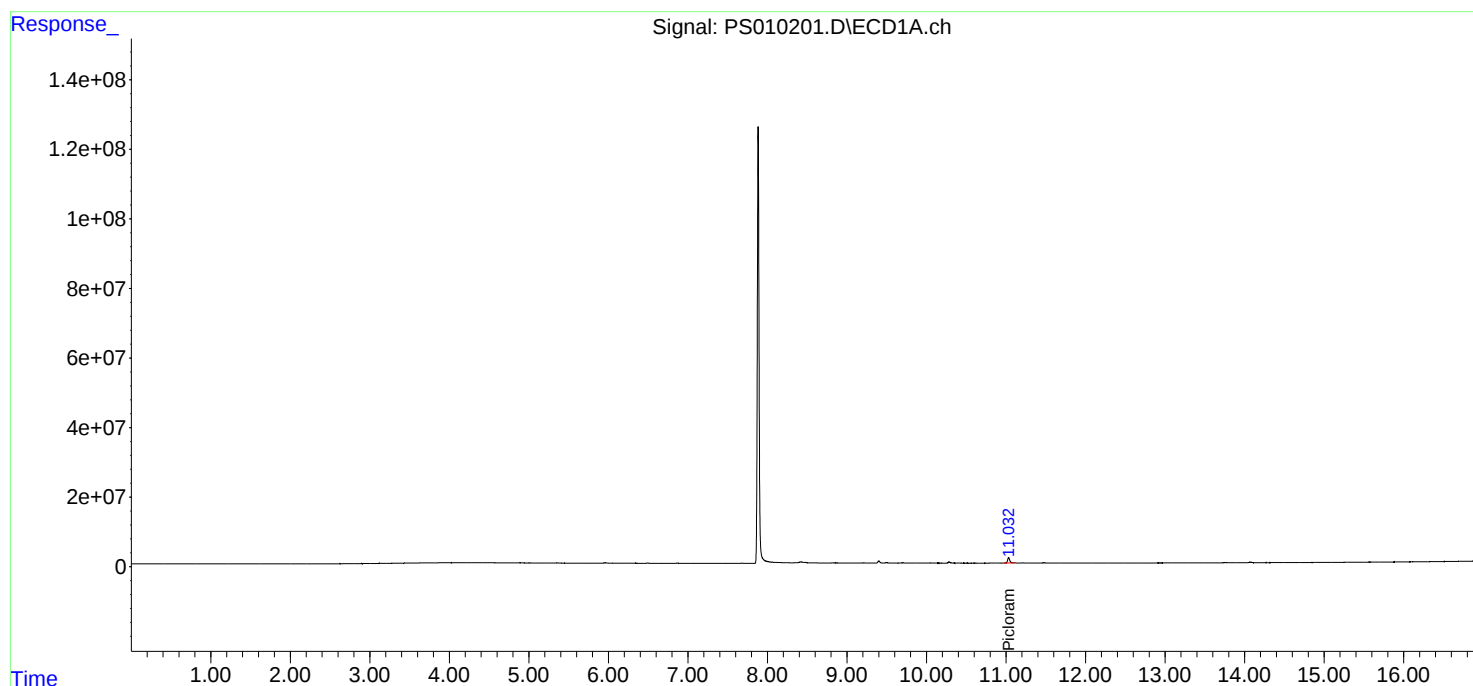


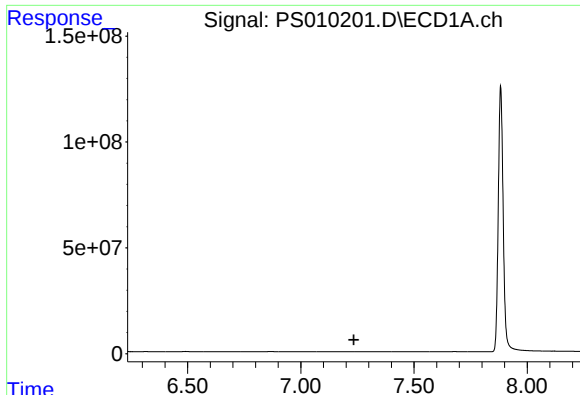

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

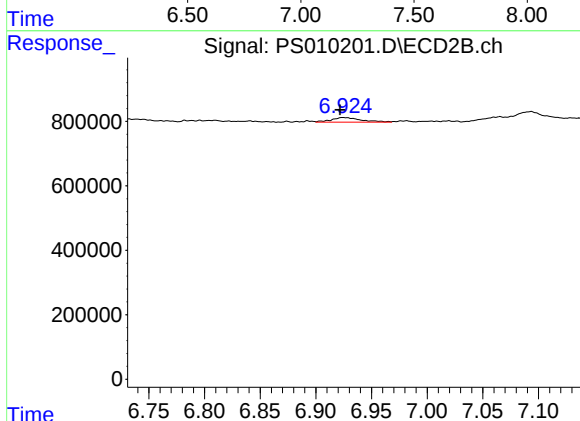


#4 2,4-DCAA

R.T.: 6.925 min
Delta R.T.: 0.003 min
Response: 266438
Conc: N.D.

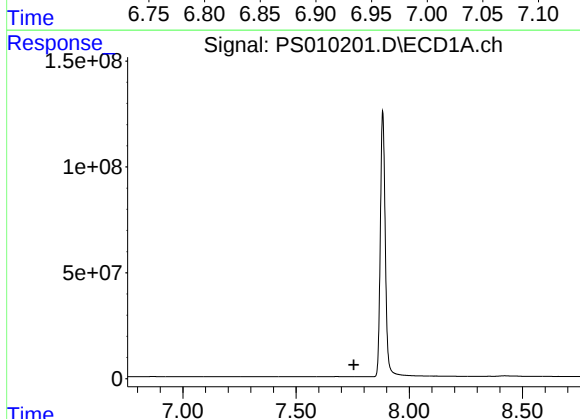


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

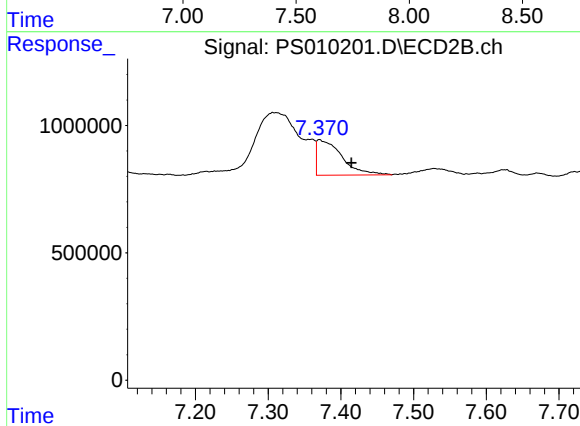

#7 MCPA


R.T.: 7.371 min
Delta R.T.: -0.044 min
Response: 3307975
Conc: 1.22 ug/ml

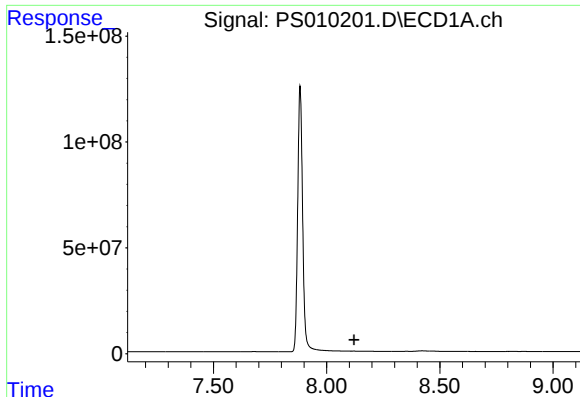

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

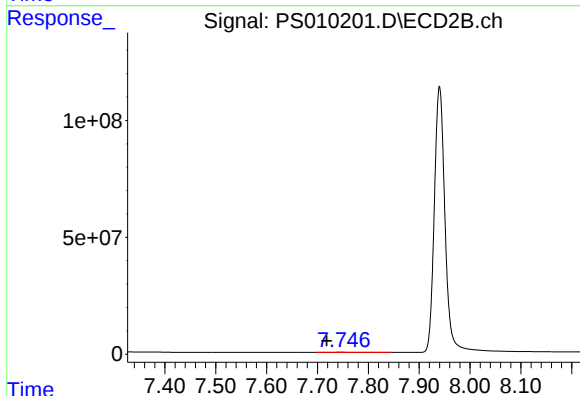


#8 DICHLORPROP

R.T.: 7.746 min
Delta R.T.: 0.028 min
Response: 1496742
Conc: 2.65 ng/ml

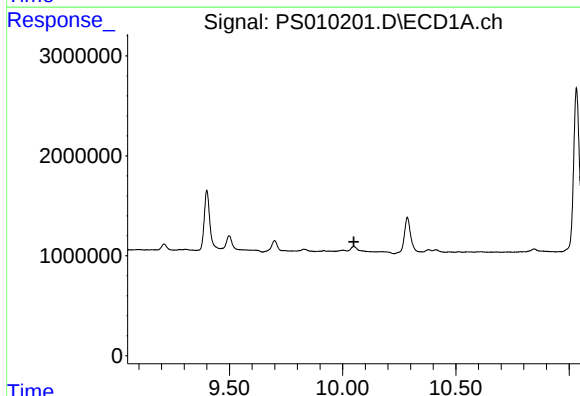


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

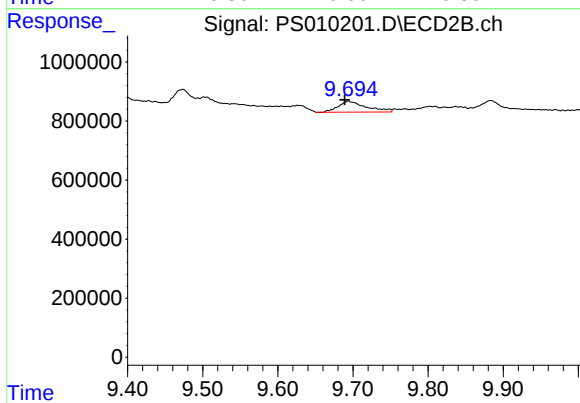

#13 2,4-DB


R.T.: 9.694 min
Delta R.T.: 0.005 min
Response: 966569
Conc: 2.43 ng/ml

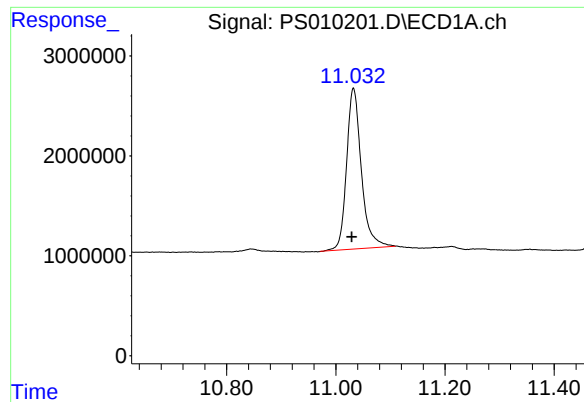

#15 Picloram

R.T.: 11.032 min
Delta R.T.: 0.003 min
Response: 30108811
Conc: 6.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

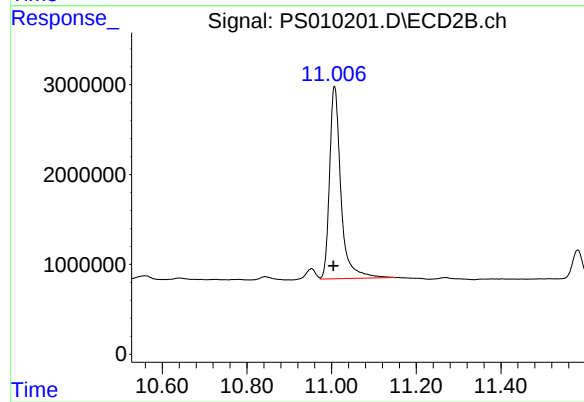

#15 Picloram

R.T.: 11.007 min
Delta R.T.: 0.003 min
Response: 39998664
Conc: 9.47 ng/ml