

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
 Data File : PS010220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2020 19:32
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 00:06:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.921	303.2E6	264.1E6	431.293	492.406
Target Compounds							
1) T	Dalapon	0.000	2.633	0	16542	N.D.	<MDL
2) T	3,5-DICHL...	0.000	6.076	0	372201	N.D.	<MDL
5) T	DICAMBA	0.000	7.090	0	2630981	N.D.	1.202
6) T	MCP	0.000	7.154	0	388267	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.743	0	4862336	N.D.	8.612
9) T	2,4-D	0.000	8.015	0	662900	N.D.	<MDL
10) T	Pentachlo...	0.000	8.441	0	1291124	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.802	0	2507533	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	2568002	N.D.	<MDL
13) T	2,4-DB	0.000	9.695	0	654538	N.D.	1.642
14) T	DINOSEB	0.000	10.024	0	1655090	N.D.	<MDL
15) T	Picloram	0.000	11.008	0	3815844	N.D.	<MDL
16) T	DCPA	0.000	10.951	0	3402534	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
Data File : PS010220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2020 19:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 00:06:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

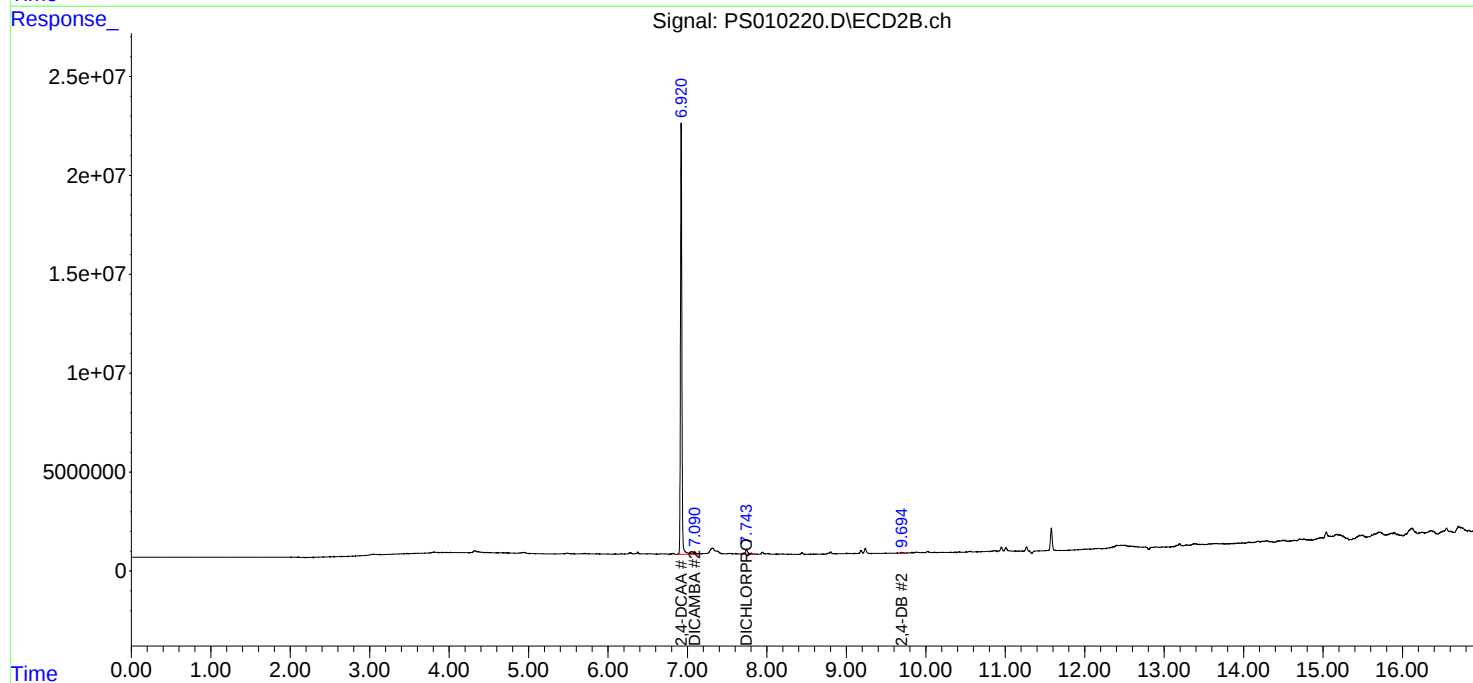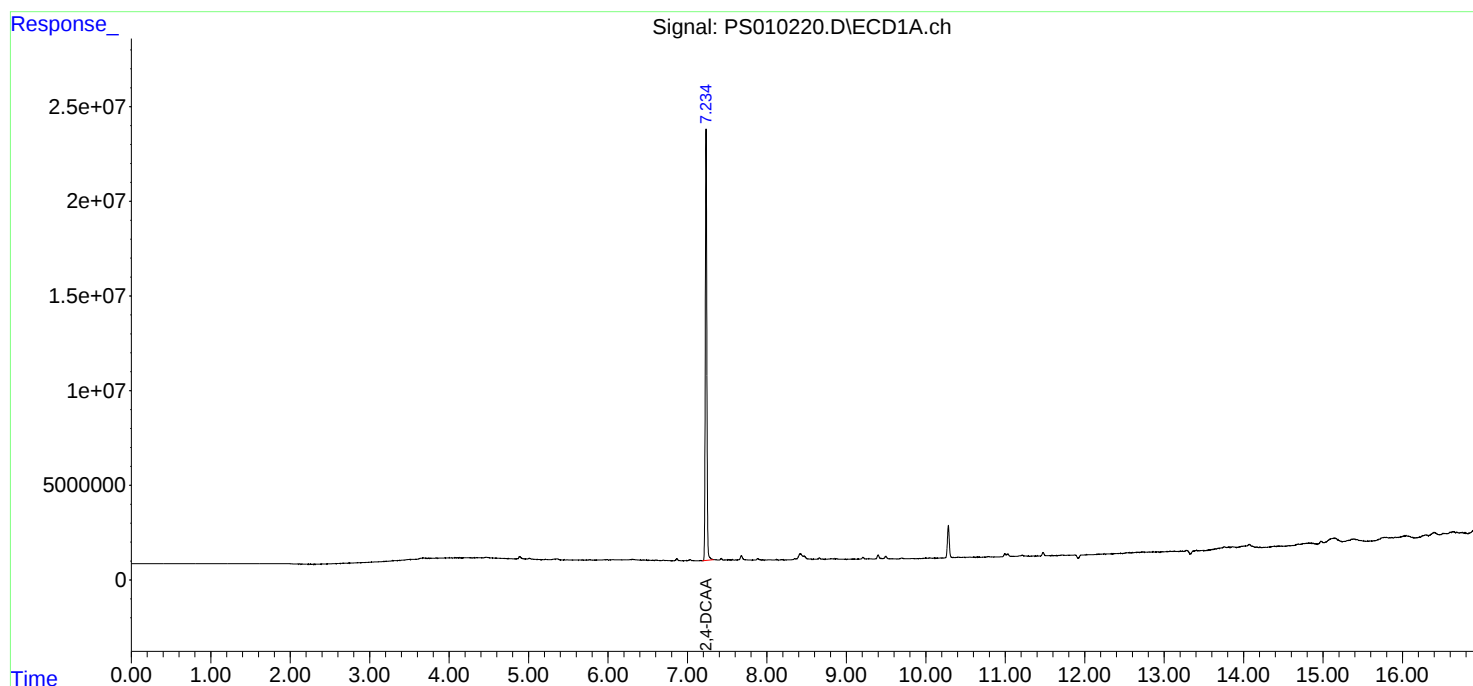


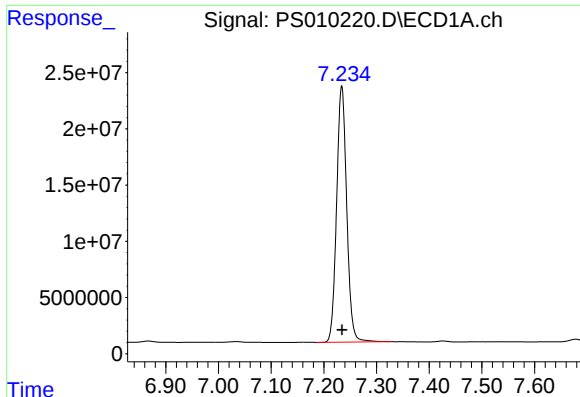

#4 2,4-DCAA


R.T.: 7.234 min
Delta R.T.: 0.000 min
Response: 303240143
Conc: 431.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

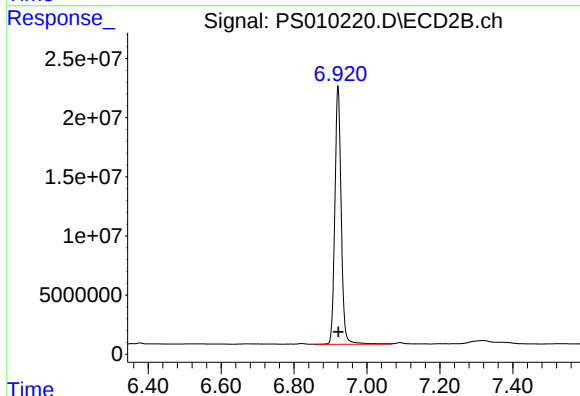


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 264072884
Conc: 492.41 ng/ml

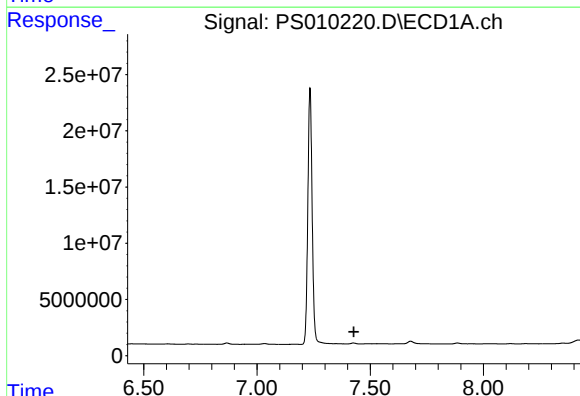


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

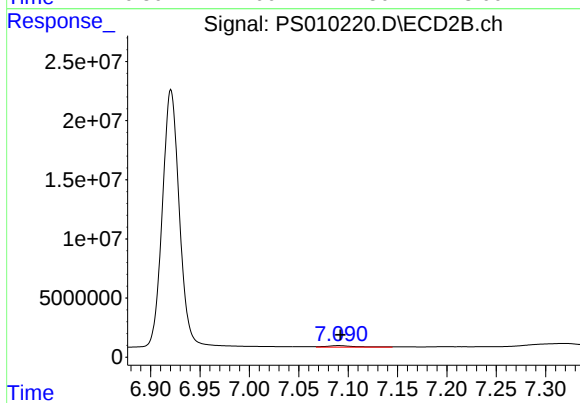

#5 DICAMBA


R.T.: 7.090 min
Delta R.T.: -0.002 min
Response: 2630981
Conc: 1.20 ng/ml

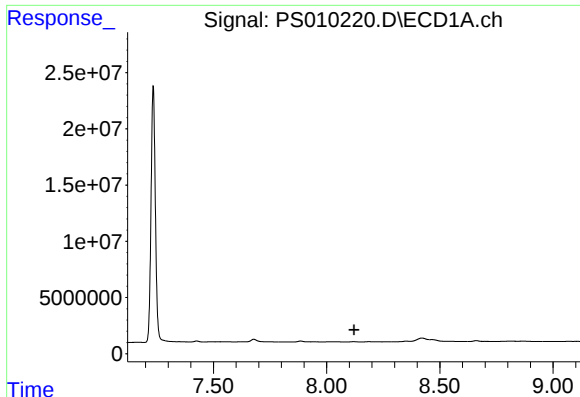

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

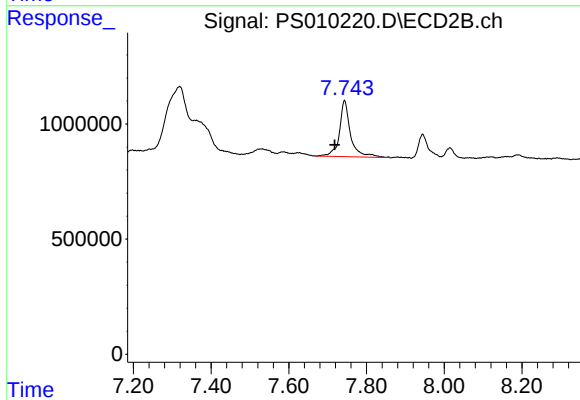


#8 DICHLORPROP

R.T.: 7.743 min
Delta R.T.: 0.025 min
Response: 4862336
Conc: 8.61 ng/ml

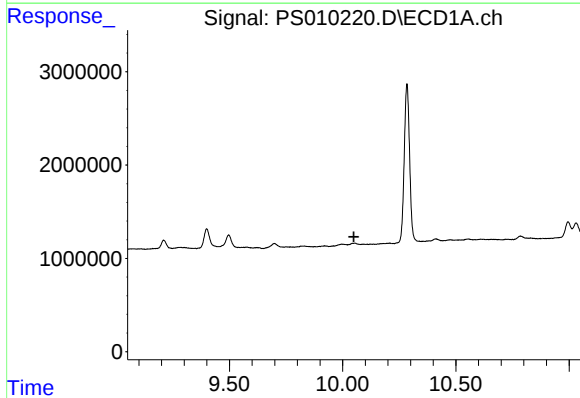

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

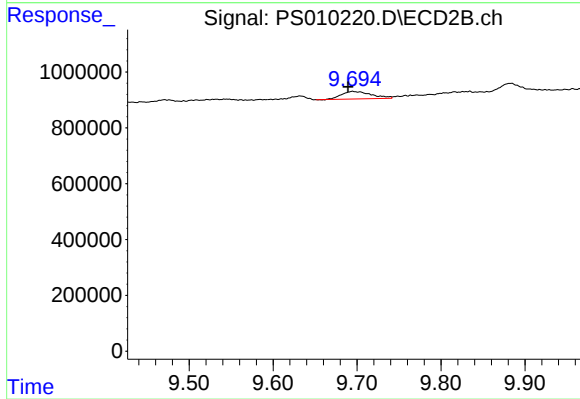

#13 2,4-DB

R.T.: 9.695 min
Delta R.T.: 0.006 min
Response: 654538
Conc: 1.64 ng/ml