

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
 Data File : PS010205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2020 13:24
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 17:01:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:00:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.922	525.7E6	399.4E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.045	2.628	611.5E6	550.7E6	682.500	682.500
2) T	3,5-DICHL...	6.445	6.070	674.5E6	568.6E6	697.500	697.500
3) T	4-Nitroph...	7.063	6.526	225.1E6	225.7E6	682.500	682.500
5) T	DICAMBA	7.427	7.091	1946.2E6	1550.9E6	705.000	705.000
6) T	MCPD	7.596	7.189	155.0E6	129.1E6	70.500	70.500
7) T	MCPA	7.747	7.405	217.2E6	186.0E6	69.750	69.750
8) T	DICHLORPROP	8.119	7.717	470.3E6	392.0E6	705.000	705.000
9) T	2,4-D	8.348	8.011	504.7E6	480.6E6	705.000	705.000
10) T	Pentachlo...	8.662	8.443	6493.8E6	4800.7E6	712.500	712.500
11) T	2,4,5-TP ...	9.211	8.803	2648.7E6	2073.3E6	712.500	712.500
12) T	2,4,5-T	9.495	9.182	2539.7E6	2089.1E6	712.500	712.500
13) T	2,4-DB	10.049	9.689	361.1E6	282.2E6	712.500	712.500
14) T	DINOSEB	11.213	10.023	1948.2E6	1511.7E6	705.000	705.000
15) T	Picloram	11.028	11.003	3330.5E6	3048.6E6	712.500	712.500
16) T	DCPA	11.477	10.952	3275.9E6	2573.6E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
Data File : PS010205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2020 13:24
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 17:01:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:00:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

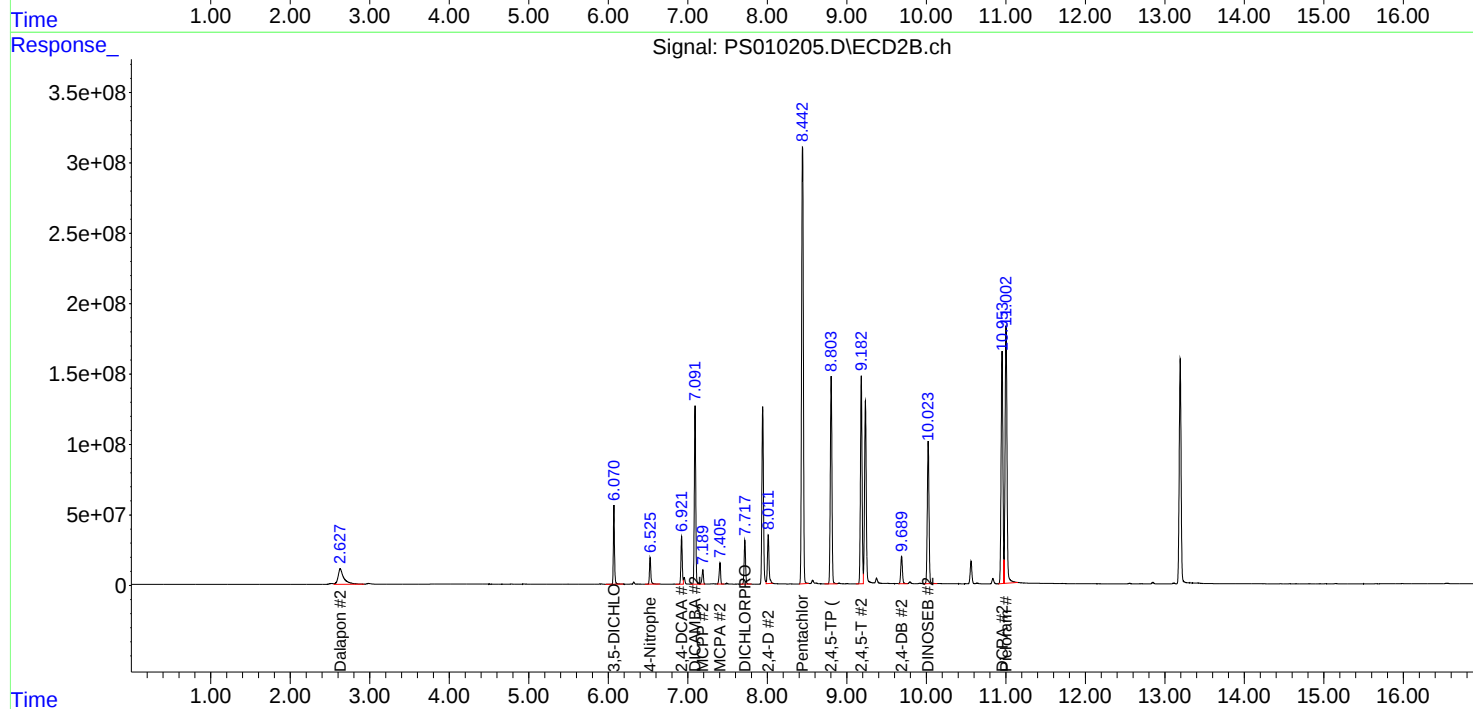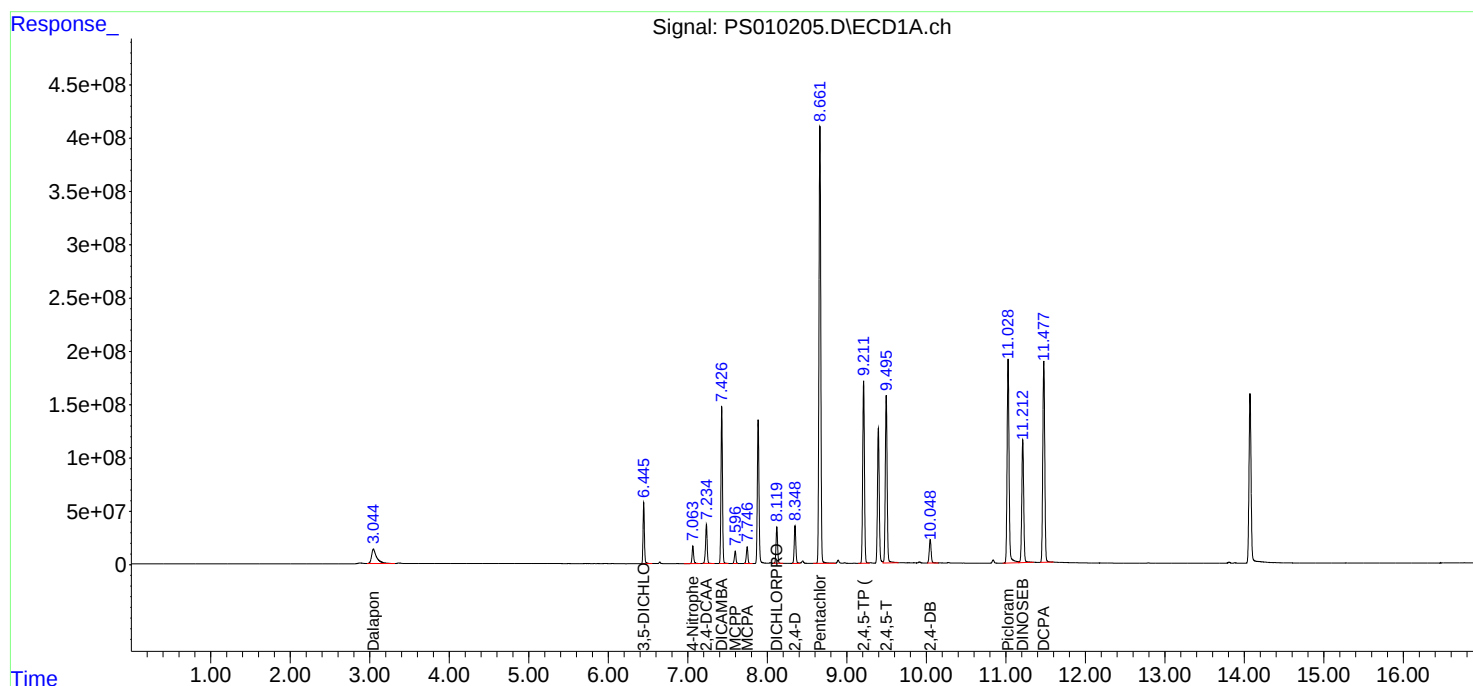


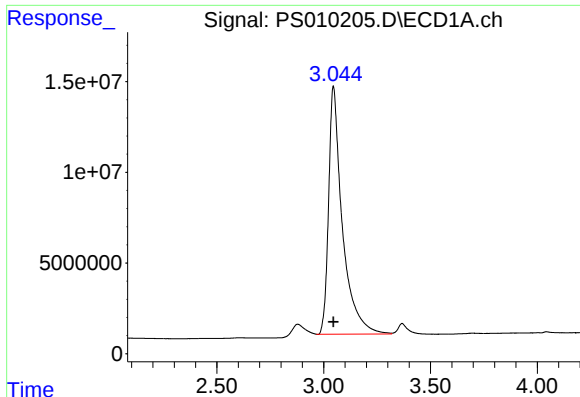

#1 Dalapon


R.T.: 3.045 min
Delta R.T.: 0.000 min
Response: 611538922
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

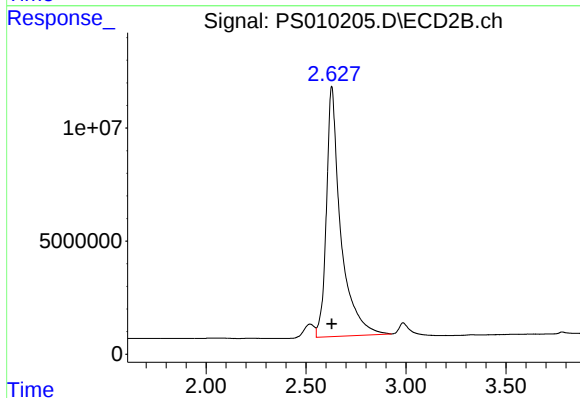


#1 Dalapon

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 550658040
Conc: 682.50 ng/ml

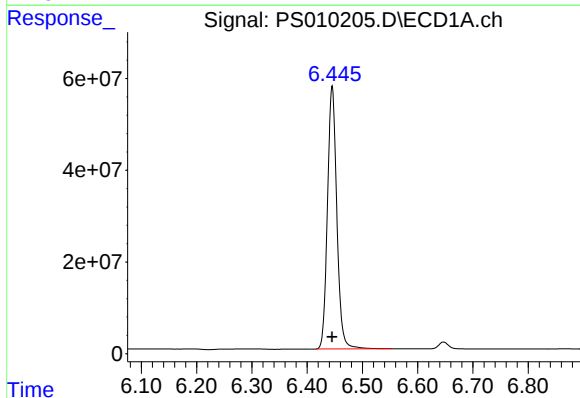


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.445 min
Delta R.T.: 0.000 min
Response: 674485384
Conc: 697.50 ng/ml

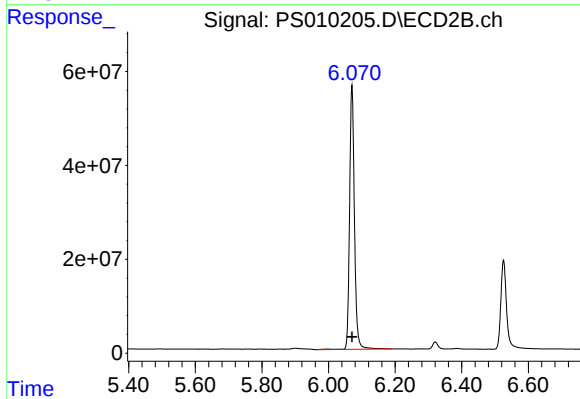

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 568583408
Conc: 697.50 ng/ml

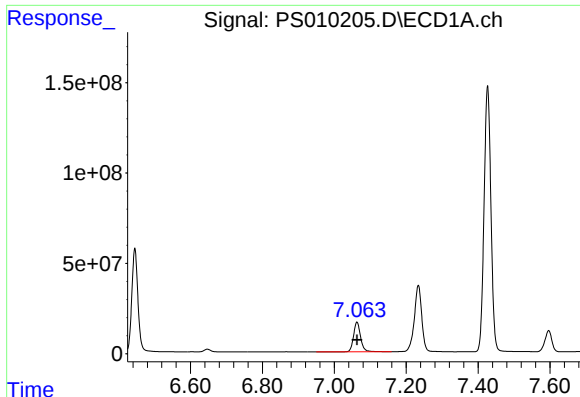

#3 4-Nitrophenol


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 225123957
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

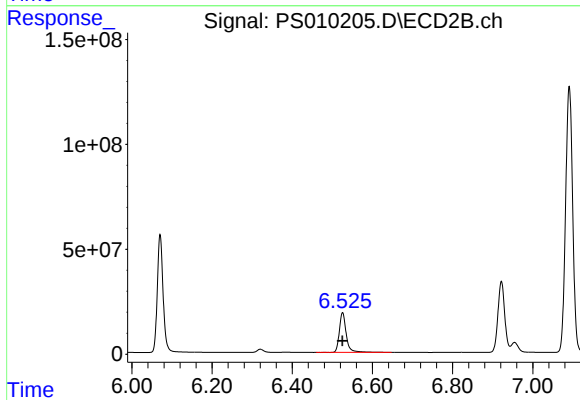


#3 4-Nitrophenol

R.T.: 6.526 min
Delta R.T.: 0.000 min
Response: 225685255
Conc: 682.50 ng/ml

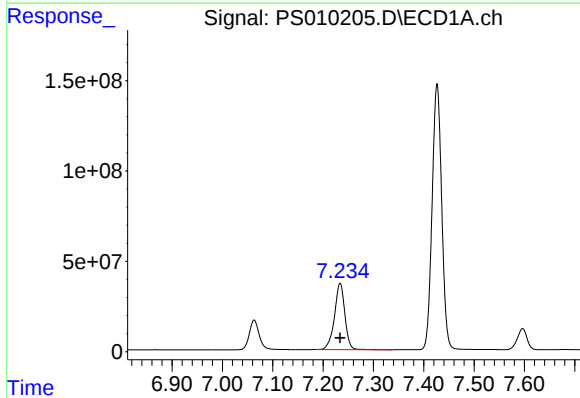


#4 2,4-DCAA

R.T.: 7.234 min
Delta R.T.: 0.000 min
Response: 525716171
Conc: 750.00 ng/ml

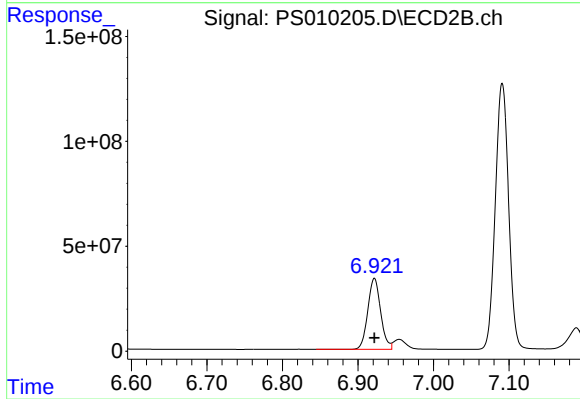

#4 2,4-DCAA


R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 399387530
Conc: 750.00 ng/ml

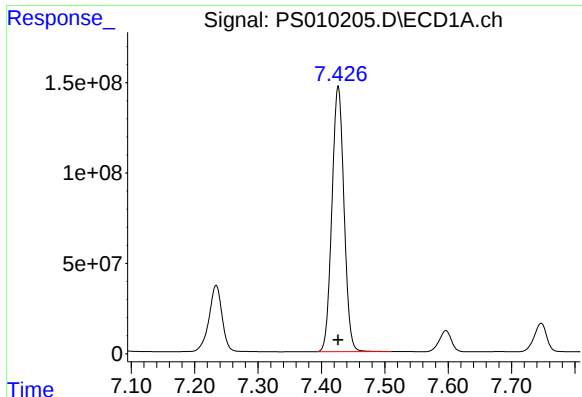

#5 DICAMBA


R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 1946162035
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

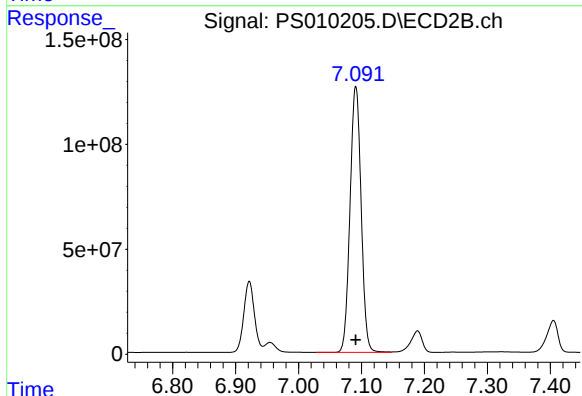


#5 DICAMBA

R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 1550861657
Conc: 705.00 ng/ml

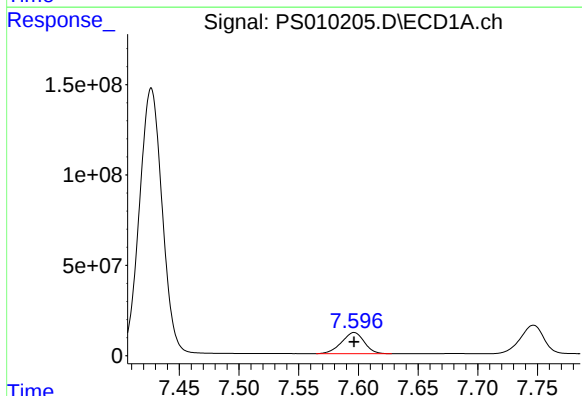


#6 MCP

R.T.: 7.596 min
Delta R.T.: 0.000 min
Response: 155006512
Conc: 70.50 ug/ml

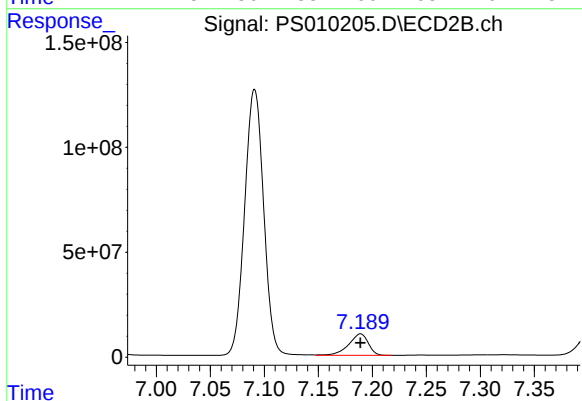

#6 MCP


R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 129141005
Conc: 70.50 ug/ml

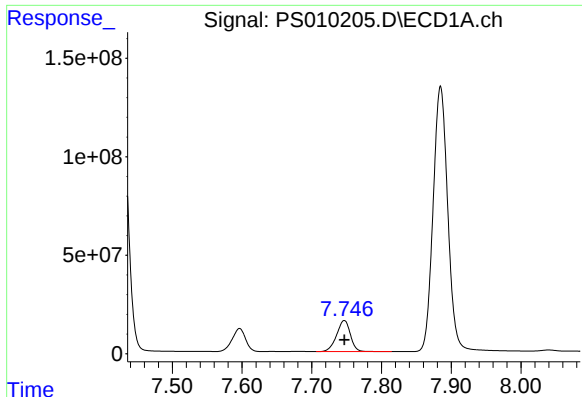

#7 MCPA


R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 217247594
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

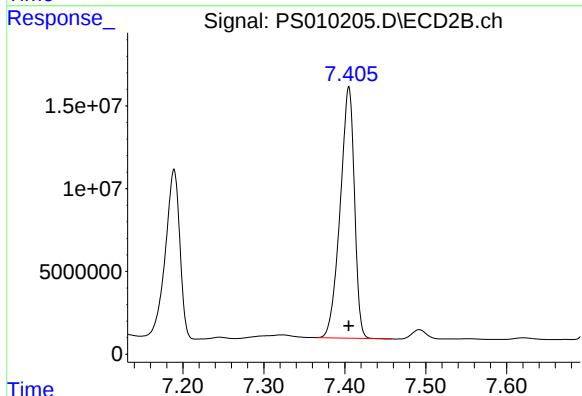


#7 MCPA

R.T.: 7.405 min
Delta R.T.: 0.000 min
Response: 186037242
Conc: 69.75 ug/ml

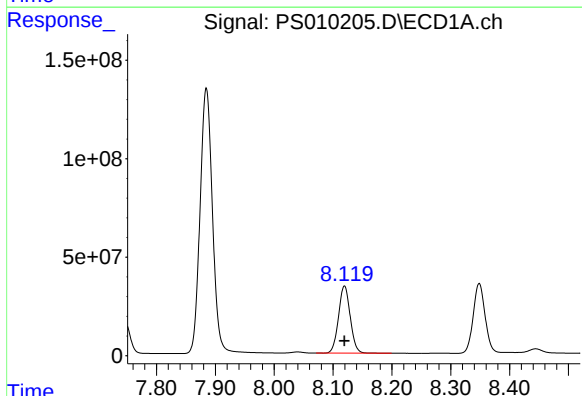


#8 DICHLORPROP

R.T.: 8.119 min
Delta R.T.: 0.000 min
Response: 470301202
Conc: 705.00 ng/ml

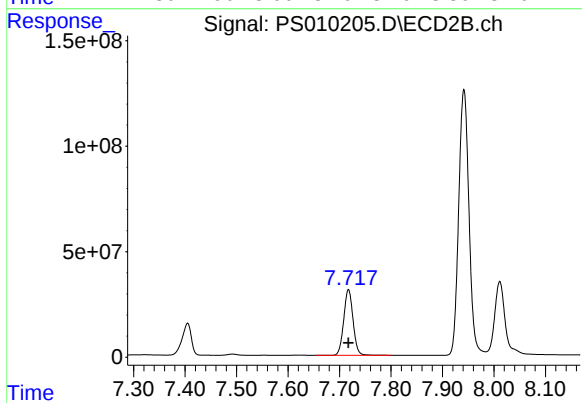

#8 DICHLORPROP


R.T.: 7.717 min
Delta R.T.: 0.000 min
Response: 391987678
Conc: 705.00 ng/ml

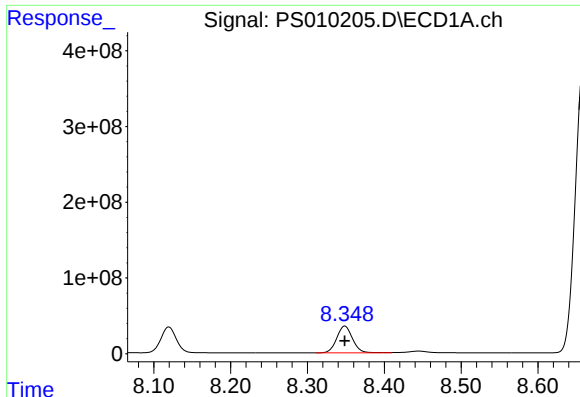

#9 2,4-D


R.T.: 8.348 min
Delta R.T.: 0.000 min
Response: 504668255
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

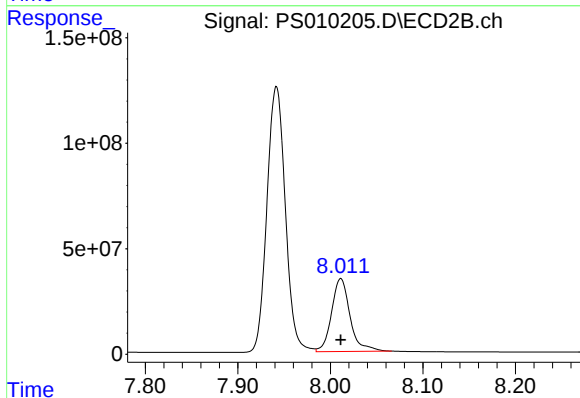


#9 2,4-D

R.T.: 8.011 min
Delta R.T.: 0.000 min
Response: 480633262
Conc: 705.00 ng/ml

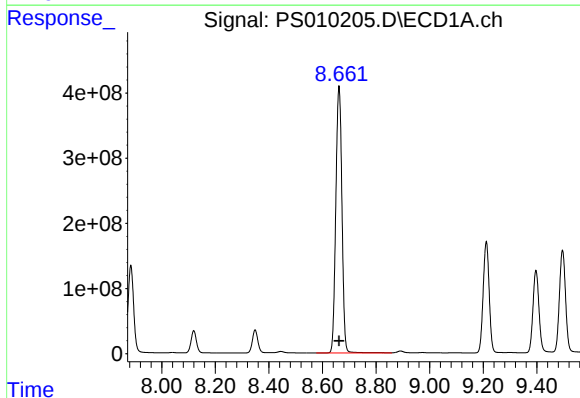


#10 Pentachlorophenol

R.T.: 8.662 min
Delta R.T.: 0.000 min
Response: 6493756279
Conc: 712.50 ng/ml

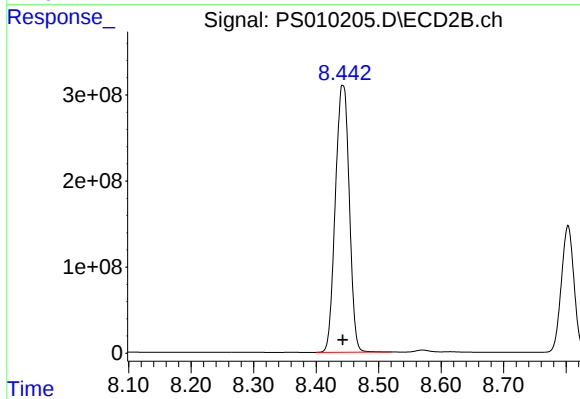

#10 Pentachlorophenol


R.T.: 8.443 min
Delta R.T.: 0.000 min
Response: 4800654852
Conc: 712.50 ng/ml

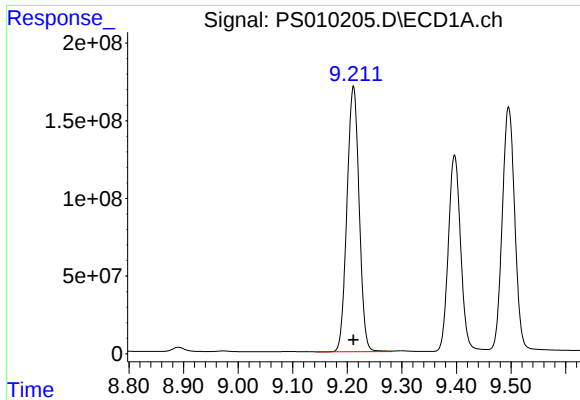

#11 2,4,5-TP (SILVEX)


R.T.: 9.211 min
Delta R.T.: 0.000 min
Response: 2648680039
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

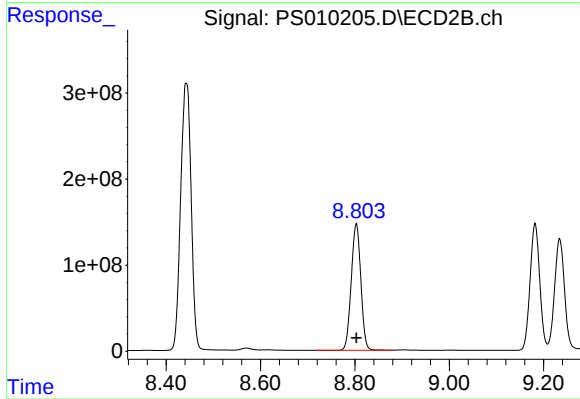


#11 2,4,5-TP (SILVEX)

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 2073342230
Conc: 712.50 ng/ml

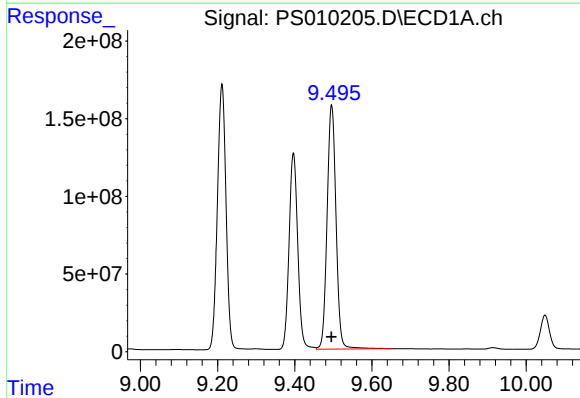


#12 2,4,5-T

R.T.: 9.495 min
Delta R.T.: 0.000 min
Response: 2539700948
Conc: 712.50 ng/ml

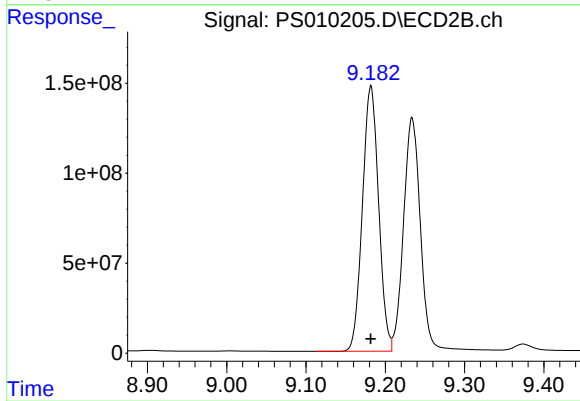

#12 2,4,5-T


R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 2089062985
Conc: 712.50 ng/ml

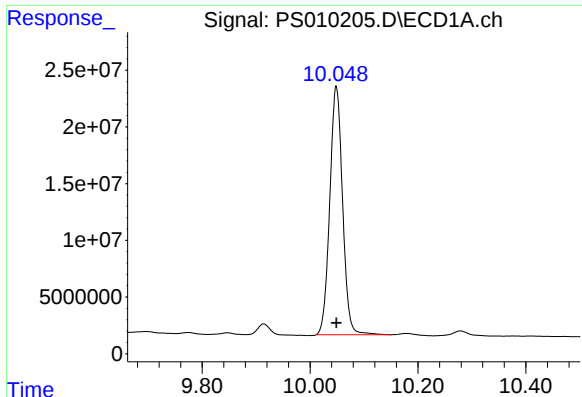

#13 2,4-DB


R.T.: 10.049 min
Delta R.T.: 0.000 min
Response: 361077774
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

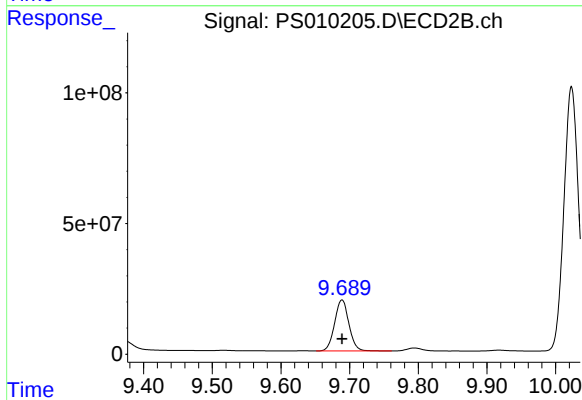


#13 2,4-DB

R.T.: 9.689 min
Delta R.T.: 0.000 min
Response: 282170720
Conc: 712.50 ng/ml

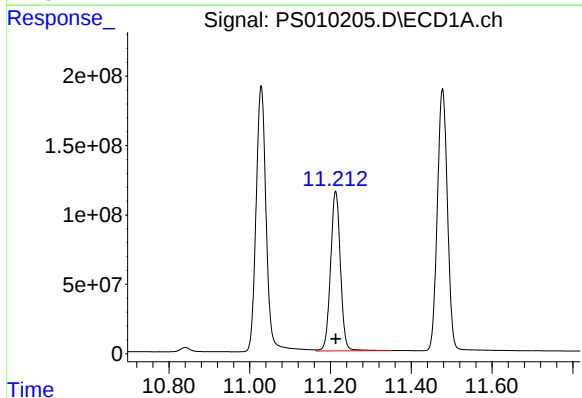


#14 DINOSEB

R.T.: 11.213 min
Delta R.T.: 0.000 min
Response: 1948163901
Conc: 705.00 ng/ml

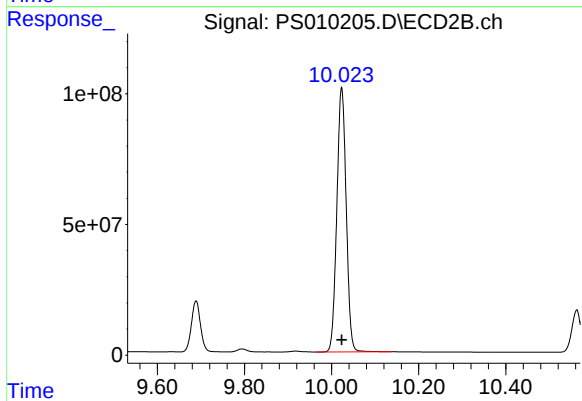

#14 DINOSEB


R.T.: 10.023 min
Delta R.T.: 0.000 min
Response: 1511653628
Conc: 705.00 ng/ml

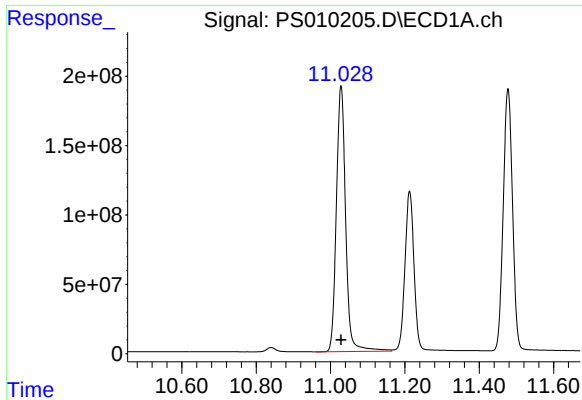

#15 Picloram


R.T.: 11.028 min
Delta R.T.: 0.000 min
Response: 3330510614
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

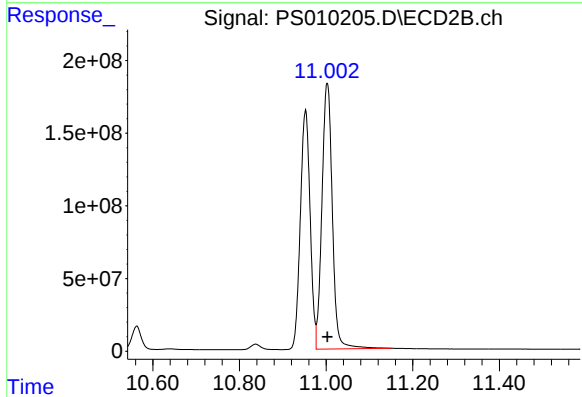


#15 Picloram

R.T.: 11.003 min
Delta R.T.: 0.000 min
Response: 3048608359
Conc: 712.50 ng/ml

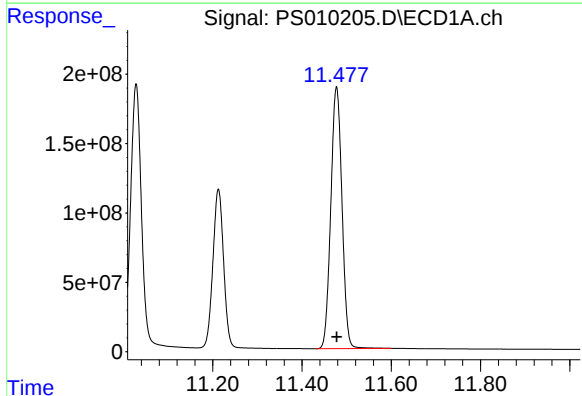

#16 DCPA

R.T.: 11.477 min
Delta R.T.: 0.000 min
Response: 3275879108
Conc: 720.00 ng/ml

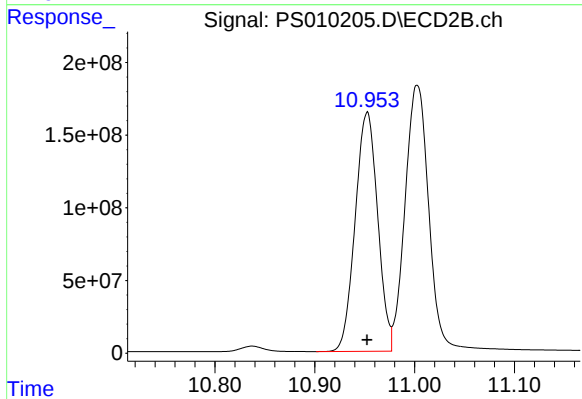

#16 DCPA

R.T.: 10.952 min
Delta R.T.: 0.000 min
Response: 2573593834
Conc: 720.00 ng/ml