

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051121\
 Data File : PS014986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 07:48
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 15:08:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.431f	0.000	8300463	0	3.541	N.D. #
5) T	DICAMBA	7.348	0.000	7605208	0	1.161	N.D. #
7) T	MCPA	7.666	0.000	822797	0	<MDL	N.D. #
9) T	2,4-D	8.300f	0.000	10754919	0	6.044	N.D. #
10) T	Pentachlo...	8.568	8.399	11209949	4310219	<MDL	<MDL #
11) T	2,4,5-TP ...	9.117	8.765	10126095	3789027	1.108	1.315
12) T	2,4,5-T	9.420	9.167	25218368	4971730	2.757	1.863 #
13) T	2,4-DB	9.986f	0.000	8424771	0	4.855	N.D. #
14) T	DINOSEB	11.091	0.000	23526997	0	3.281	N.D. #
15) T	Picloram	10.898	10.984	37851295	90707859	3.116	22.764 #
16) T	DCPA	11.356	10.898	18506562	6517037	1.355	1.529



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051121\
Data File : PS014986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 07:48
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 15:08:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

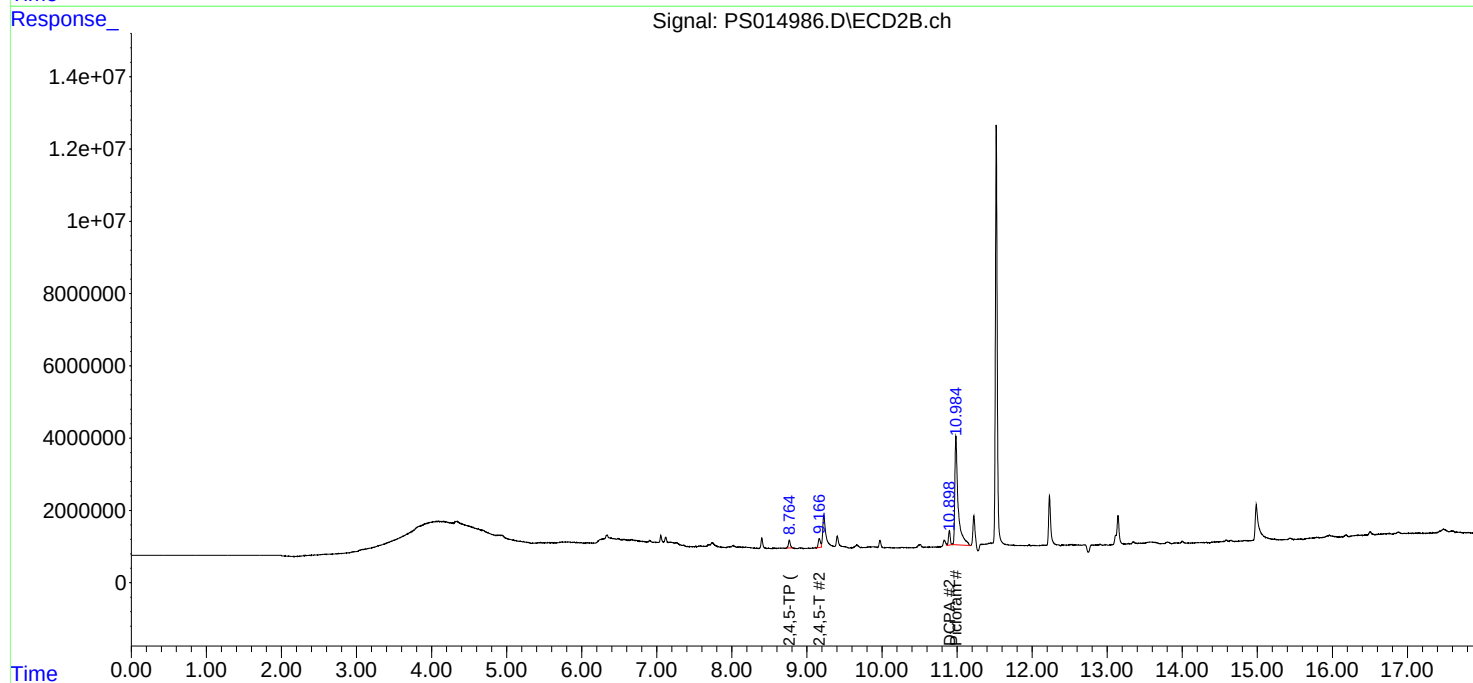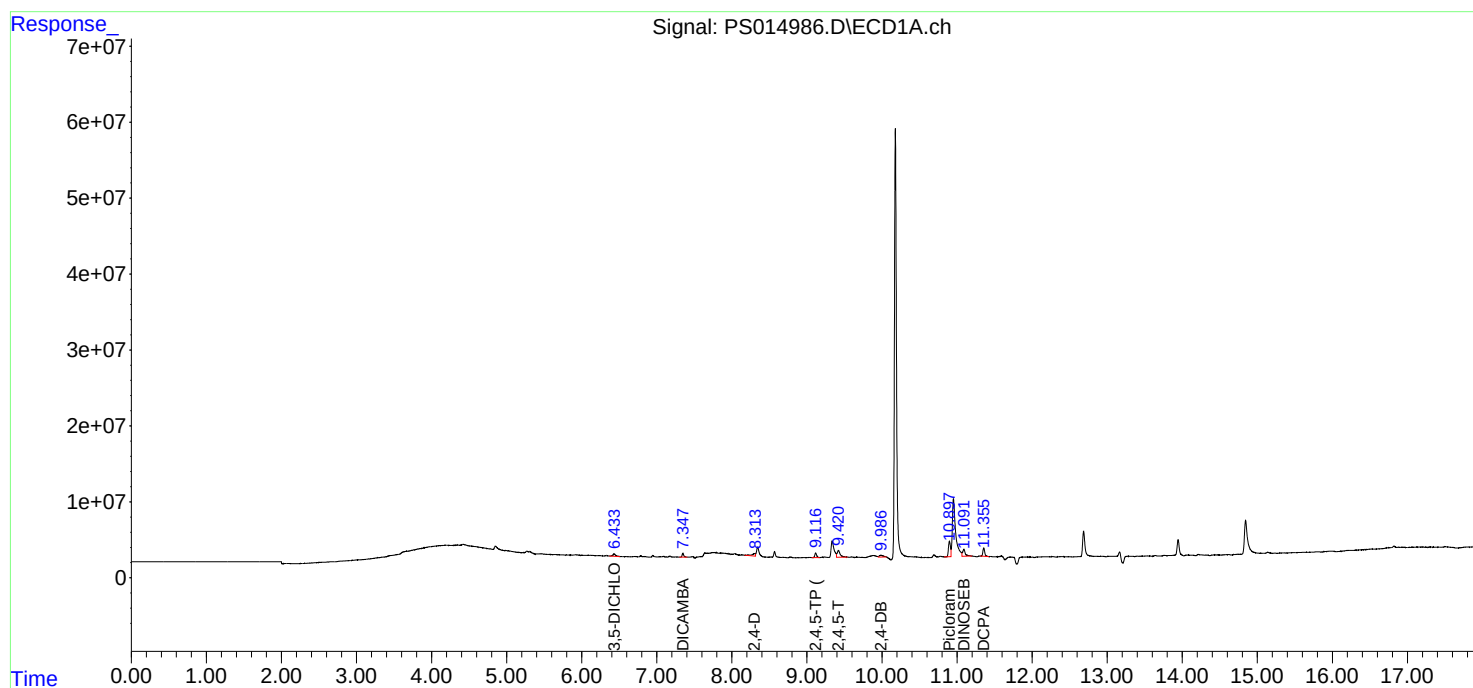


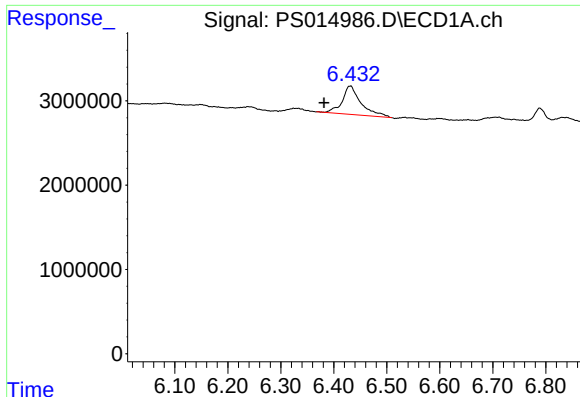

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.431 min
Delta R.T.: 0.050 min
Response: 8300463
Conc: 3.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

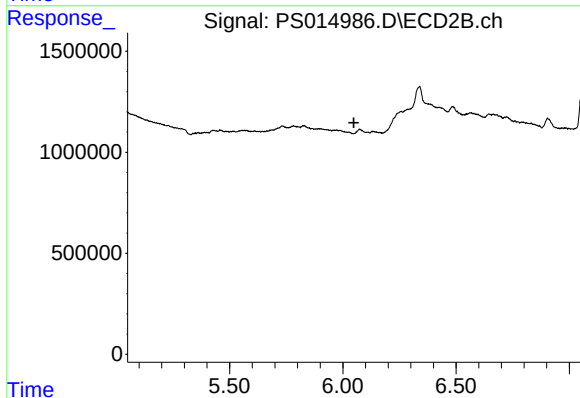


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

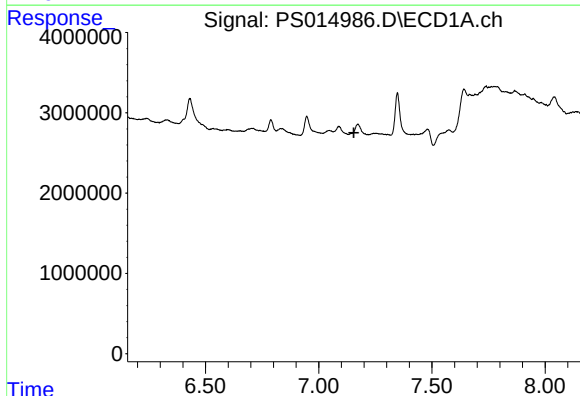


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.156 min
Response: 0
Conc: N.D.

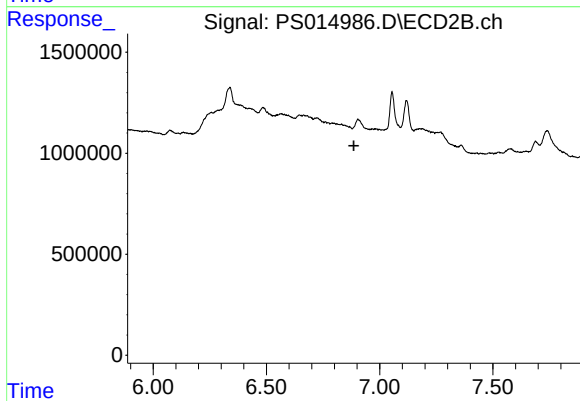

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

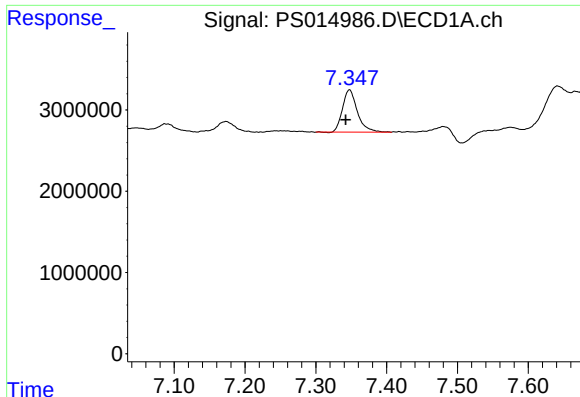

#5 DICAMBA


R.T.: 7.348 min
Delta R.T.: 0.005 min
Response: 7605208
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

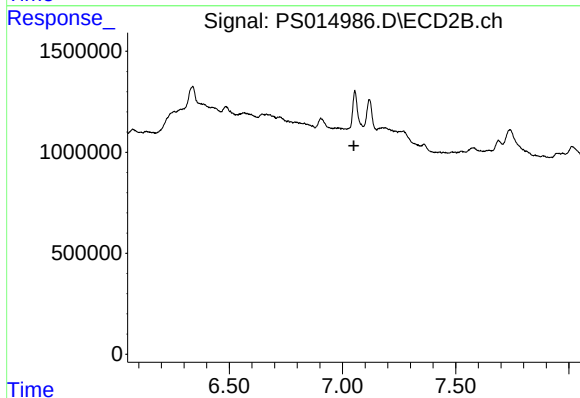


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.051 min
Response: 0
Conc: N.D.

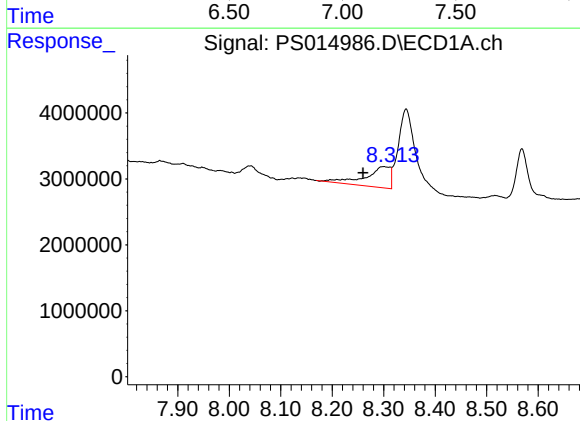


#9 2,4-D

R.T.: 8.300 min
Delta R.T.: 0.040 min
Response: 10754919
Conc: 6.04 ng/ml

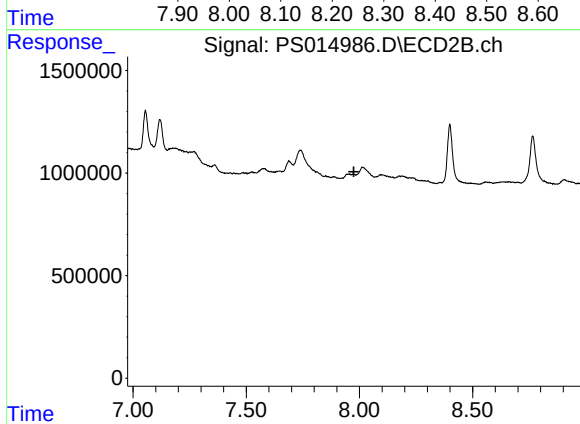

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

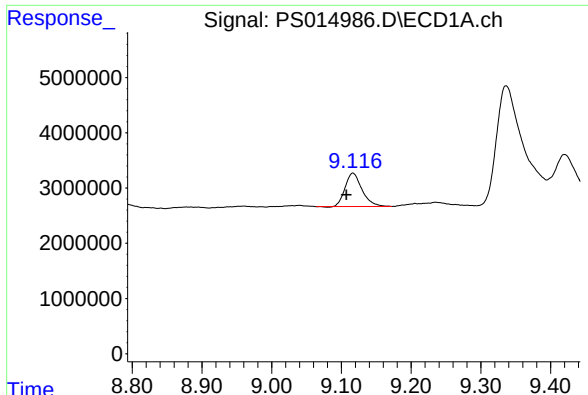

#11 2,4,5-TP (SILVEX)


R.T.: 9.117 min
Delta R.T.: 0.009 min
Response: 10126095
Conc: 1.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

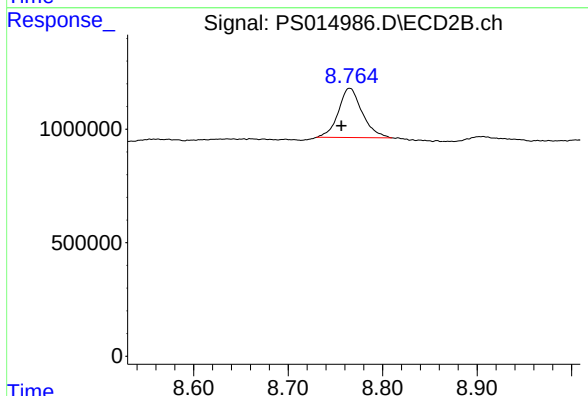


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: 0.009 min
Response: 3789027
Conc: 1.31 ng/ml

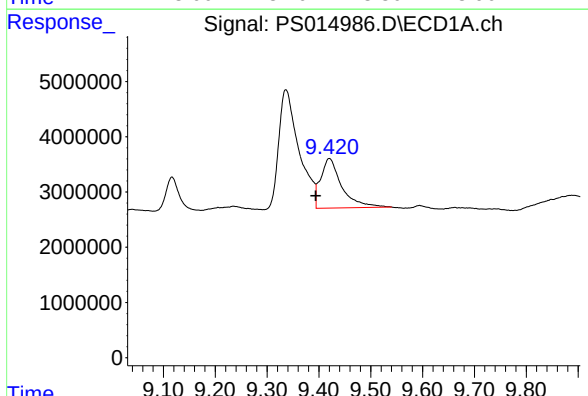


#12 2,4,5-T

R.T.: 9.420 min
Delta R.T.: 0.026 min
Response: 25218368
Conc: 2.76 ng/ml

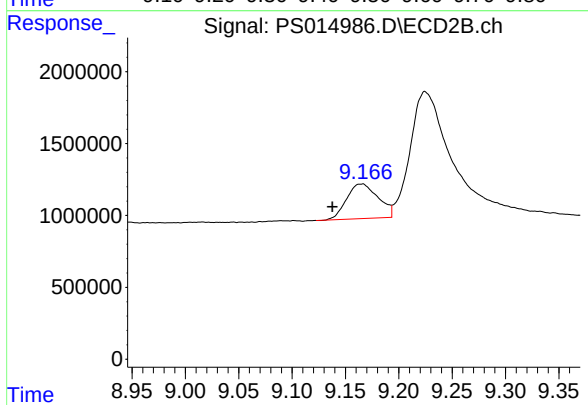

#12 2,4,5-T


R.T.: 9.167 min
Delta R.T.: 0.029 min
Response: 4971730
Conc: 1.86 ng/ml

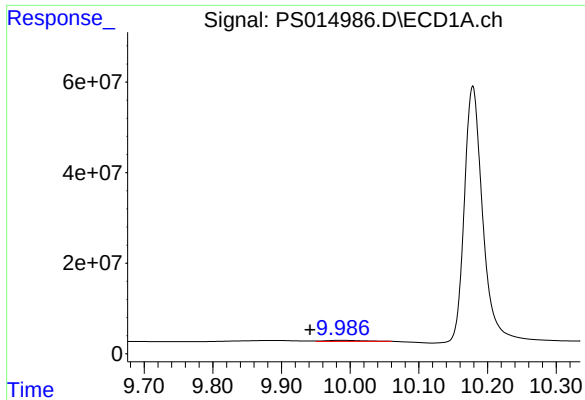

#13 2,4-DB


R.T.: 9.986 min
Delta R.T.: 0.044 min
Response: 8424771
Conc: 4.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

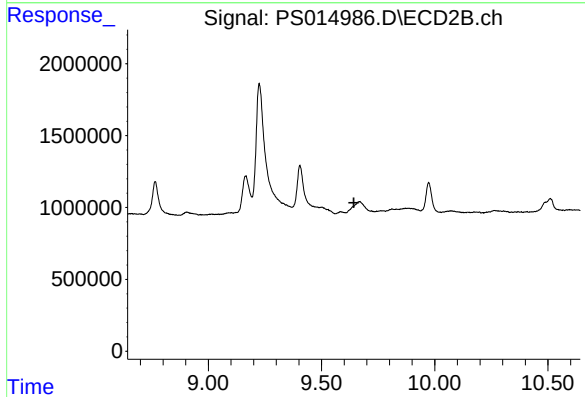


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.643 min
Response: 0
Conc: N.D.

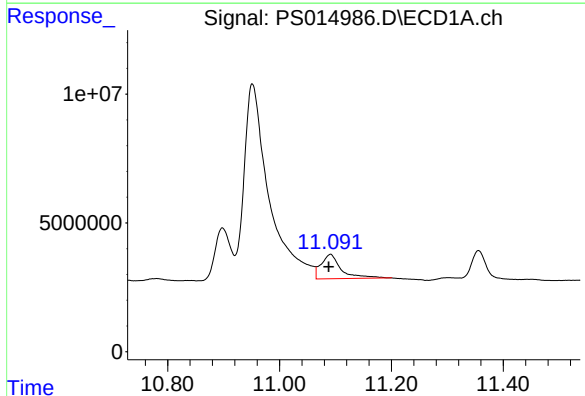


#14 DINOSEB

R.T.: 11.091 min
Delta R.T.: 0.003 min
Response: 23526997
Conc: 3.28 ng/ml

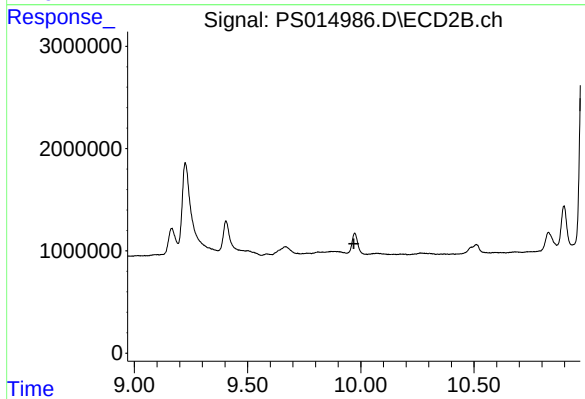

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.970 min
Response: 0
Conc: N.D.

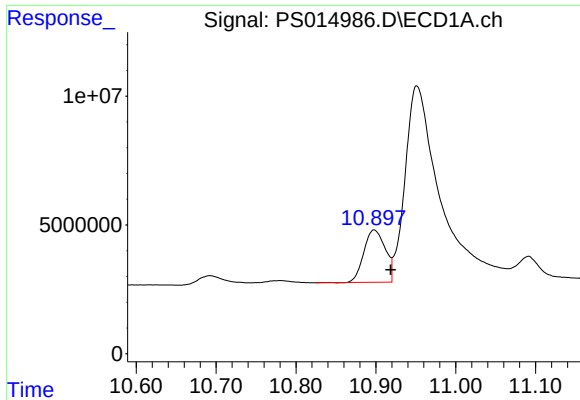

#15 Picloram


R.T.: 10.898 min
Delta R.T.: -0.021 min
Response: 37851295
Conc: 3.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

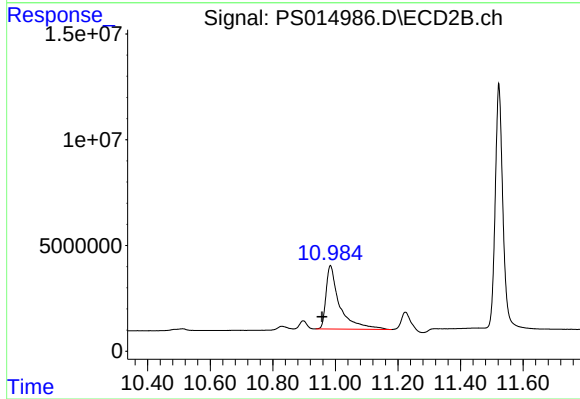


#15 Picloram

R.T.: 10.984 min
Delta R.T.: 0.026 min
Response: 90707859
Conc: 22.76 ng/ml

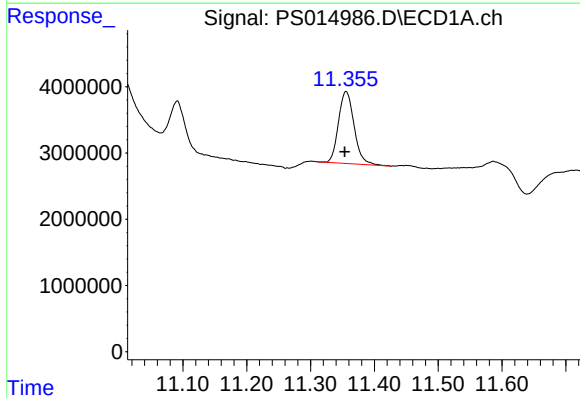

#16 DCPA

R.T.: 11.356 min
Delta R.T.: 0.002 min
Response: 18506562
Conc: 1.35 ng/ml

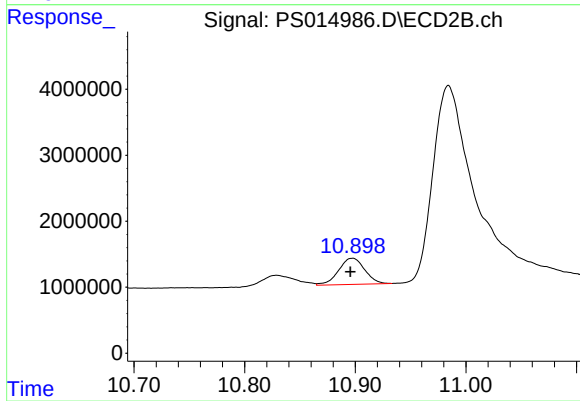

#16 DCPA

R.T.: 10.898 min
Delta R.T.: 0.002 min
Response: 6517037
Conc: 1.53 ng/ml