

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051121\
 Data File : PS014991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 12:59
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 15:11:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.888	694.3E6	264.1E6	414.915	545.660 #
Target Compounds							
5) T	DICAMBA	7.351	7.056	3387672	2655618	<MDL	1.240 #
9) T	2,4-D	8.325f	0.000	61083216	0	34.325	N.D. #
10) T	Pentachlo...	8.579	0.000	5277014	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.133	0.000	5502740	0	<MDL	N.D. #
12) T	2,4,5-T	9.360	0.000	67075635	0	7.334	N.D. #
14) T	DINOSEB	11.092	0.000	25236623	0	3.519	N.D. #
15) T	Picloram	10.920	10.996	4444574	107.5E6	<MDL	26.967 #
16) T	DCPA	11.362	10.901	12939424	6349622	<MDL	1.490 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051121\
Data File : PS014991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 12:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 15:11:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

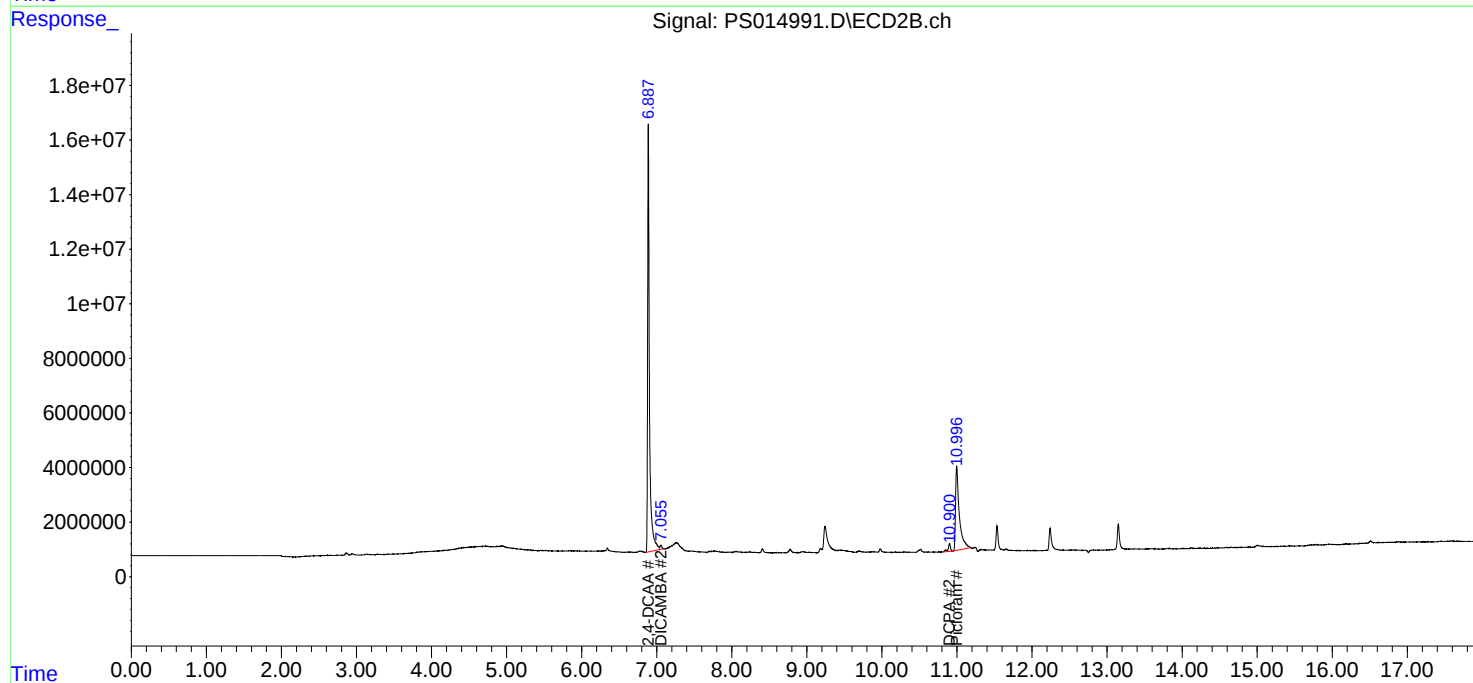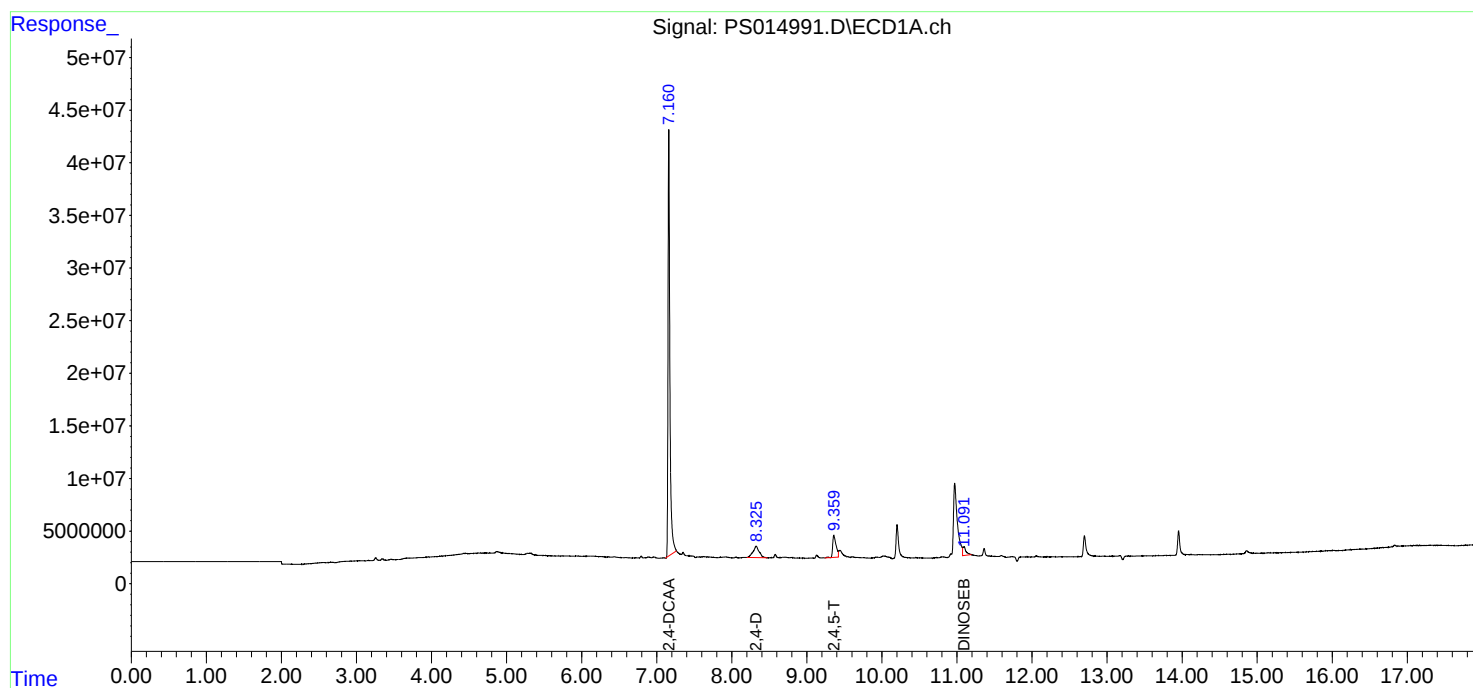


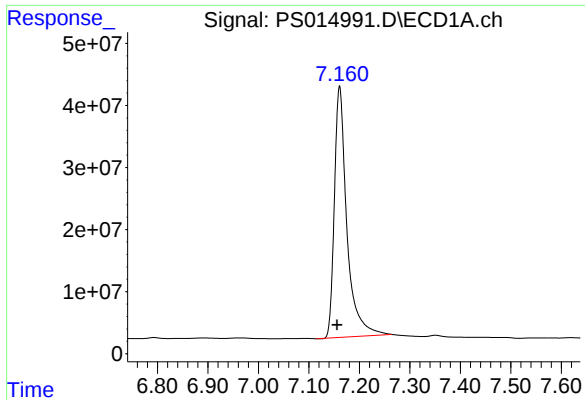

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: 0.005 min
Response: 694256871
Conc: 414.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

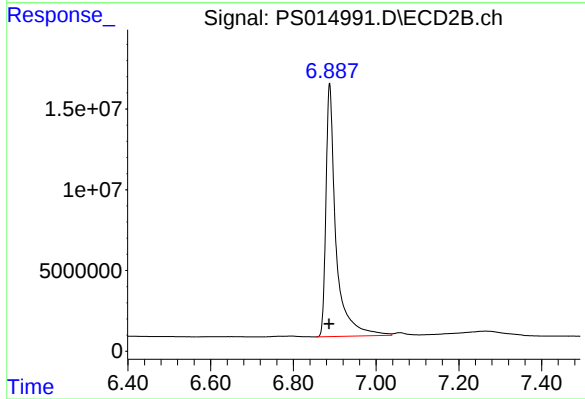


#4 2,4-DCAA

R.T.: 6.888 min
Delta R.T.: 0.001 min
Response: 264051898
Conc: 545.66 ng/ml

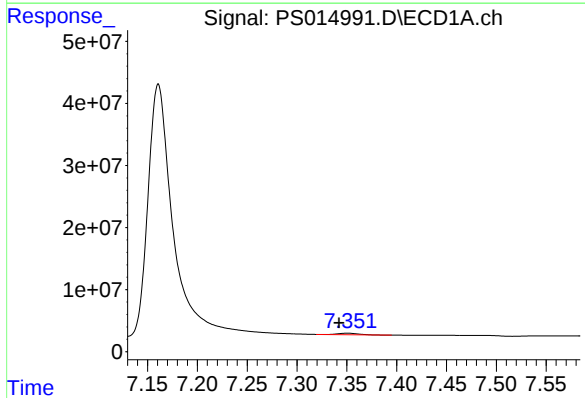


#5 DICAMBA

R.T.: 7.351 min
Delta R.T.: 0.008 min
Response: 3387672
Conc: N.D.

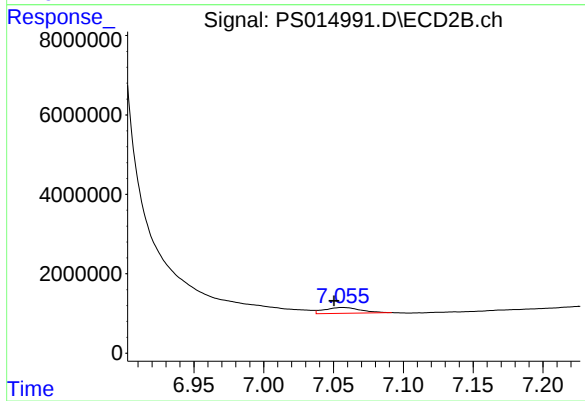

#5 DICAMBA


R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 2655618
Conc: 1.24 ng/ml

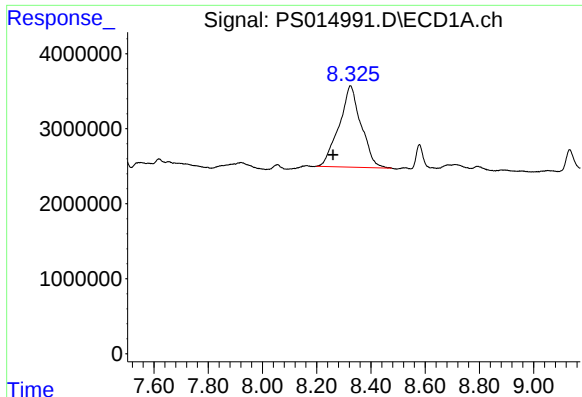

#9 2,4-D


R.T.: 8.325 min
Delta R.T.: 0.064 min
Response: 61083216
Conc: 34.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

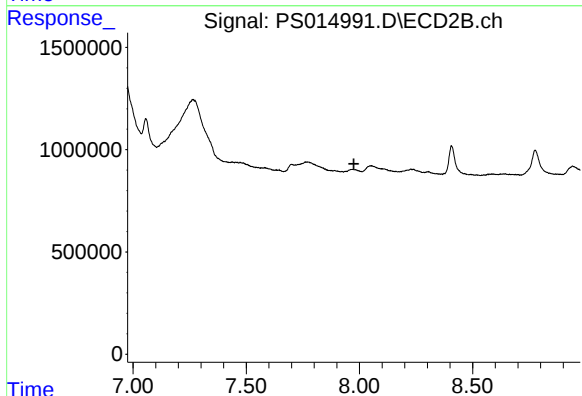


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

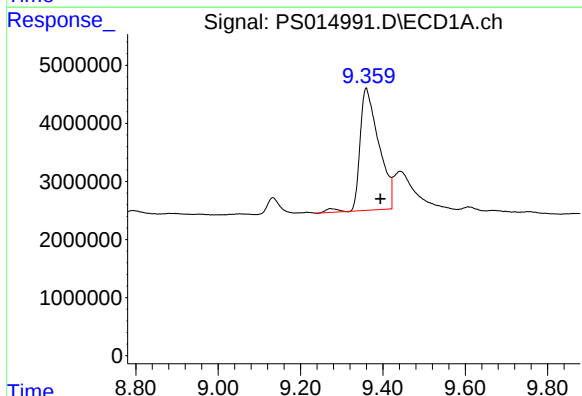


#12 2,4,5-T

R.T.: 9.360 min
Delta R.T.: -0.034 min
Response: 67075635
Conc: 7.33 ng/ml

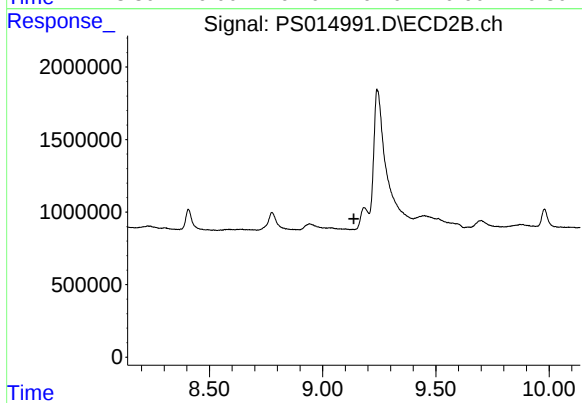

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.138 min
Response: 0
Conc: N.D.

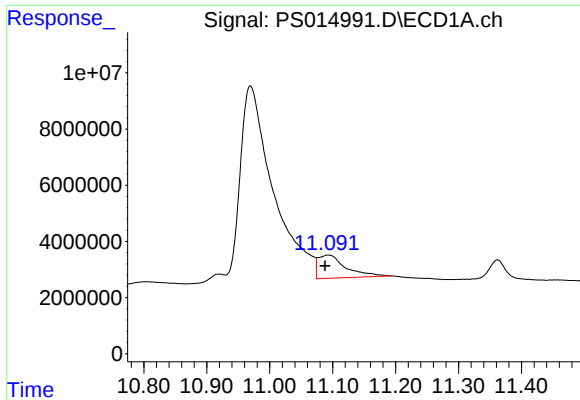

#14 DINOSEB


R.T.: 11.092 min
Delta R.T.: 0.004 min
Response: 25236623
Conc: 3.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

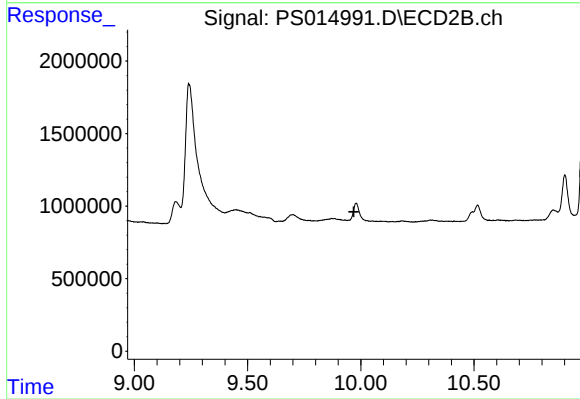


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.970 min
Response: 0
Conc: N.D.

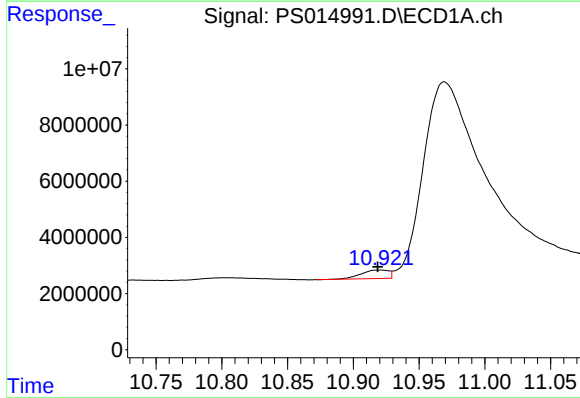


#15 Picloram

R.T.: 10.920 min
Delta R.T.: 0.002 min
Response: 4444574
Conc: N.D.

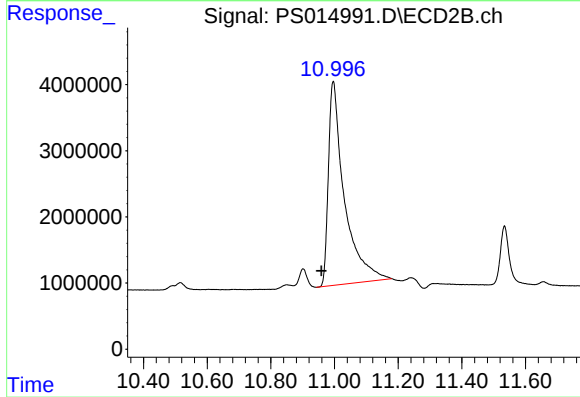

#15 Picloram


R.T.: 10.996 min
Delta R.T.: 0.038 min
Response: 107455594
Conc: 26.97 ng/ml

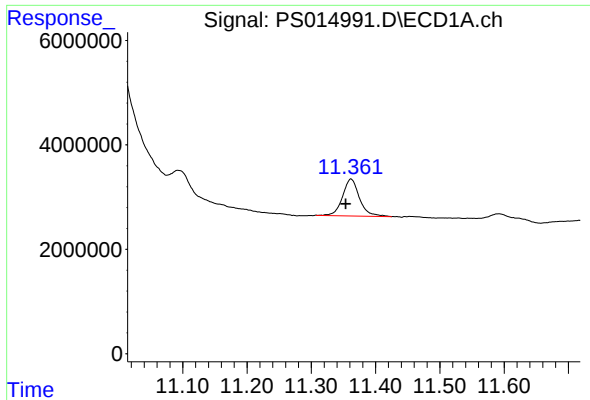

#16 DCPA

R.T.: 11.362 min
Delta R.T.: 0.008 min
Response: 12939424
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

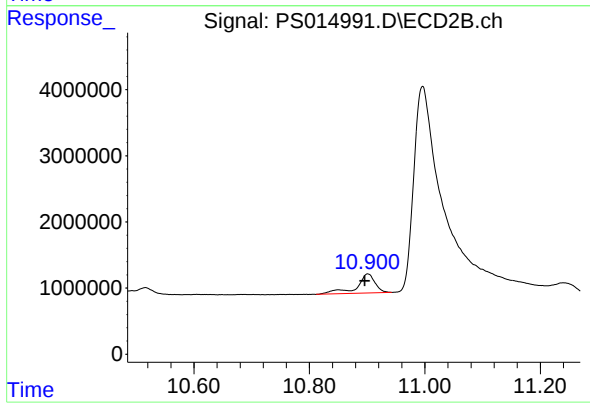

#16 DCPA

R.T.: 10.901 min
Delta R.T.: 0.005 min
Response: 6349622
Conc: 1.49 ng/ml