

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051123\
 Data File : PS022991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 14:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 21:15:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.483	6.857	733.7E6	295.7E6	482.357	527.008
Target Compounds							
1) T	Dalapon	2.579	0.000	1289010	0	<MDL	N.D. #
5) T	DICAMBA	6.630	7.078f	-1248131	716411	N.D.	<MDL
6) T	MCP	6.817	7.078	3377477	716411	<MDL	<MDL #
7) T	MCPA	6.857f	7.312	-1347028	6590532	N.D.	2.489
8) T	DICHLORPROP	7.245	7.664	1745666	4913314	<MDL	7.939 #
9) T	2,4-D	7.405	0.000	10051852	0	4.343	N.D. #
10) T	Pentachlo...	7.678	8.365	4466976	3074994	<MDL	<MDL #
11) T	2,4,5-TP ...	8.217	8.727	16854542	732160	1.443	<MDL #
12) T	2,4,5-T	8.479	9.099	16382821	2694783	1.418	<MDL #
13) T	2,4-DB	8.975	0.000	12569582	0	5.358	N.D. #
15) T	Picloram	9.891	10.902	53623700	10711420	3.127	2.515
16) T	DCPA	10.336	10.902	1302814	10711420	<MDL	2.867 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051123\
Data File : PS022991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 14:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 21:15:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

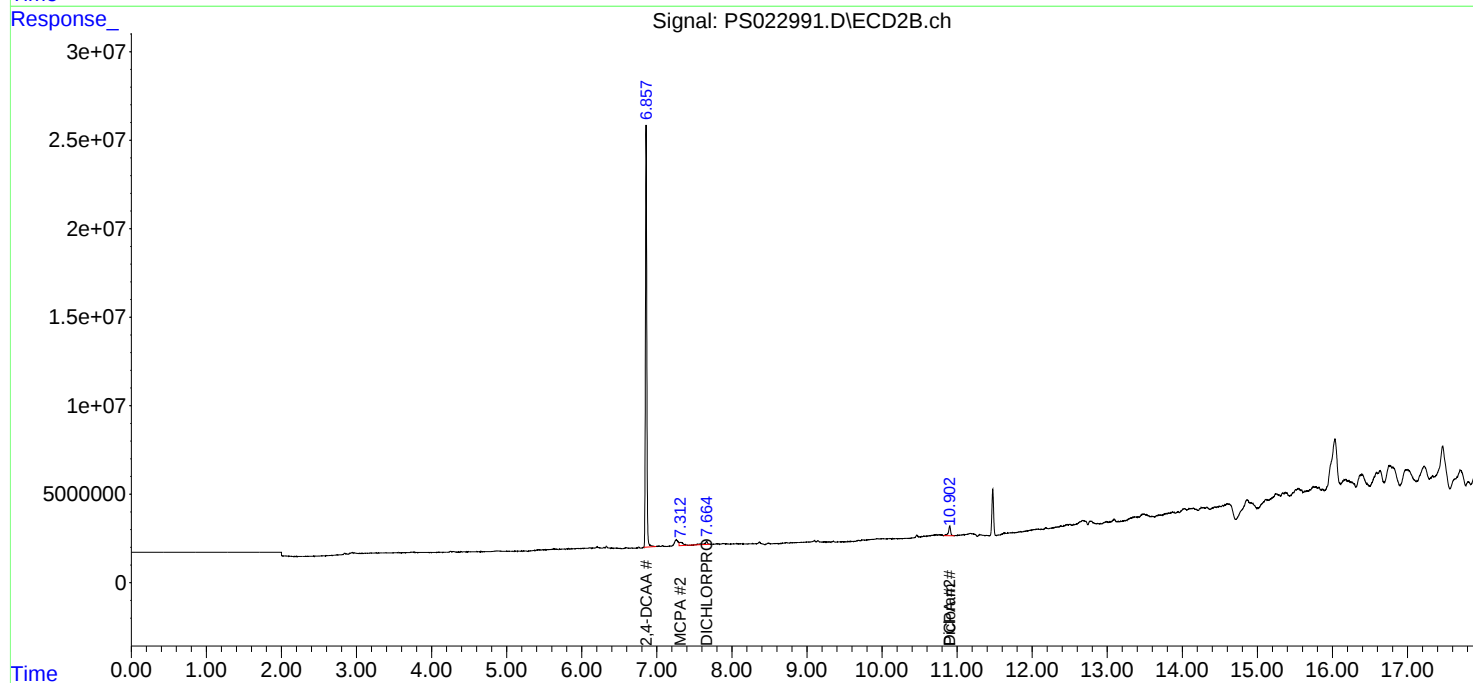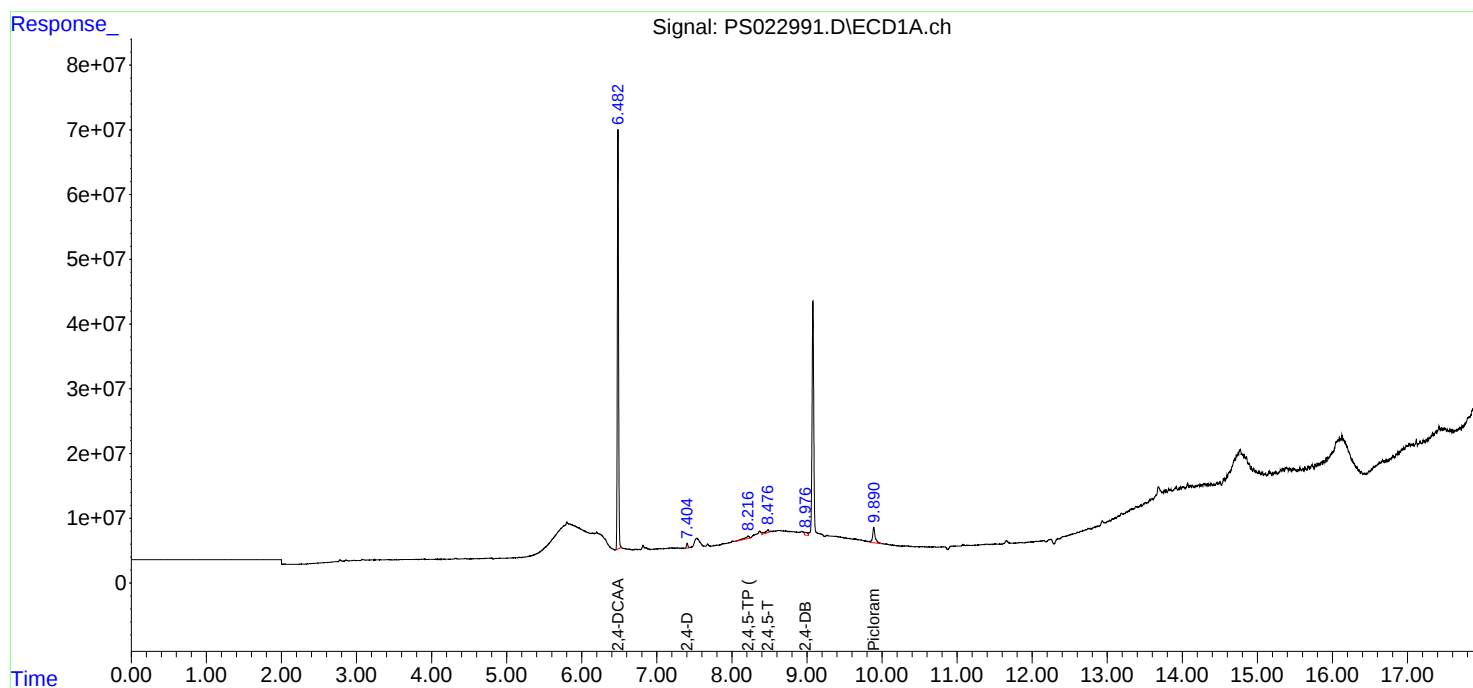


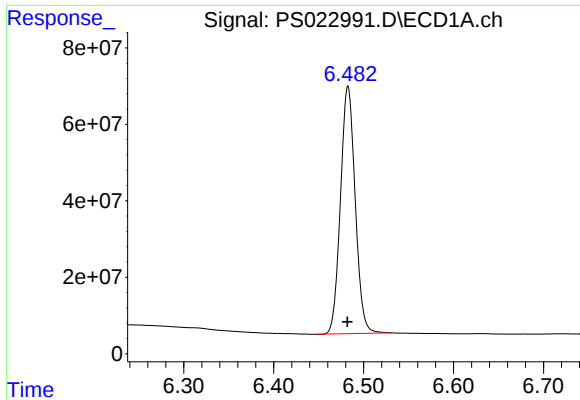

#4 2,4-DCAA


R.T.: 6.483 min
Delta R.T.: 0.000 min
Response: 733662344
Conc: 482.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

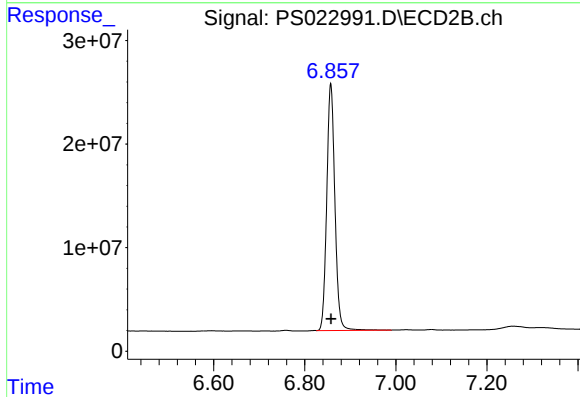


#4 2,4-DCAA

R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 295712446
Conc: 527.01 ng/ml

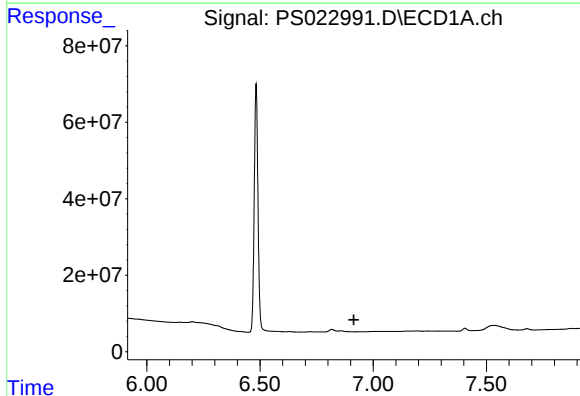


#7 MCPA

R.T.: 6.857 min
Delta R.T.: -0.058 min
Response: -1347028
Conc: N.D.

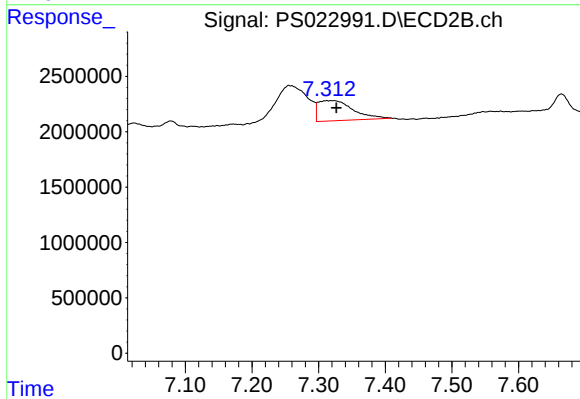

#7 MCPA


R.T.: 7.312 min
Delta R.T.: -0.014 min
Response: 6590532
Conc: 2.49 ug/ml

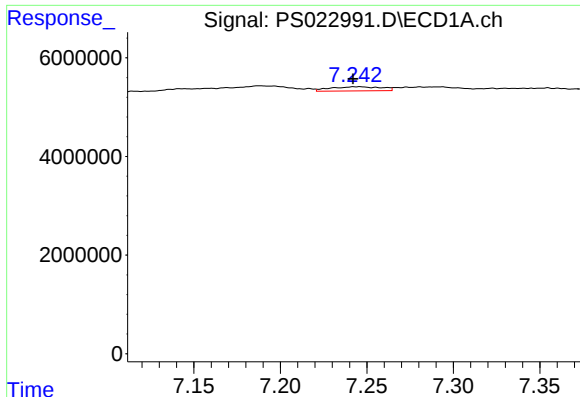

#8 DICHLORPROP


R.T.: 7.245 min
Delta R.T.: 0.003 min
Response: 1745666
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

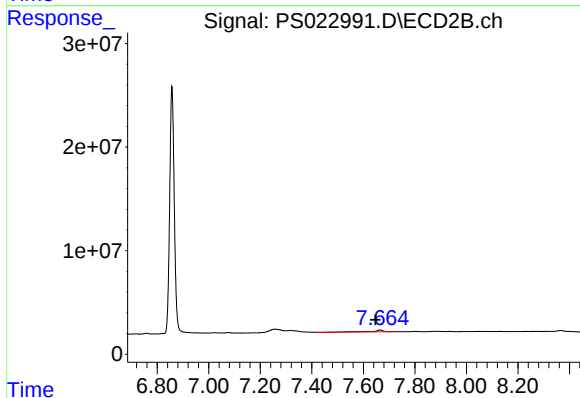


#8 DICHLORPROP

R.T.: 7.664 min
Delta R.T.: 0.018 min
Response: 4913314
Conc: 7.94 ng/ml

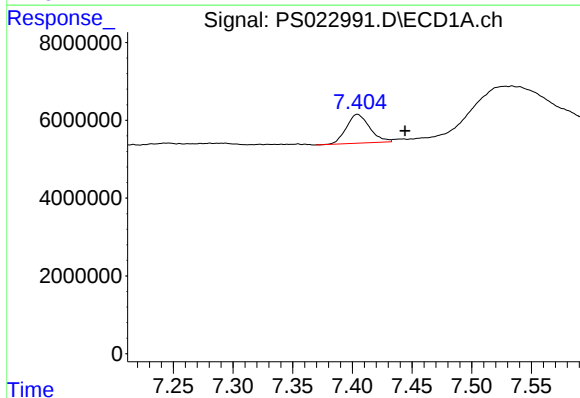


#9 2,4-D

R.T.: 7.405 min
Delta R.T.: -0.040 min
Response: 10051852
Conc: 4.34 ng/ml

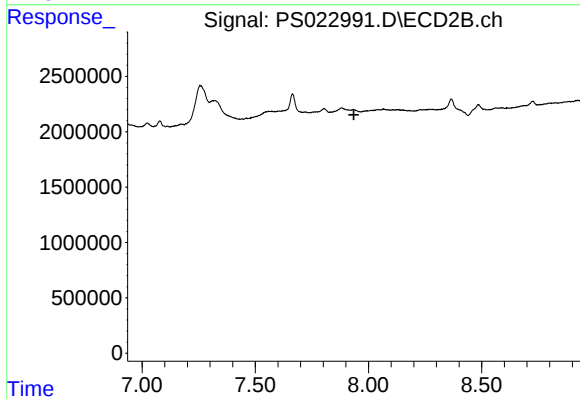

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.935 min
Response: 0
Conc: N.D.

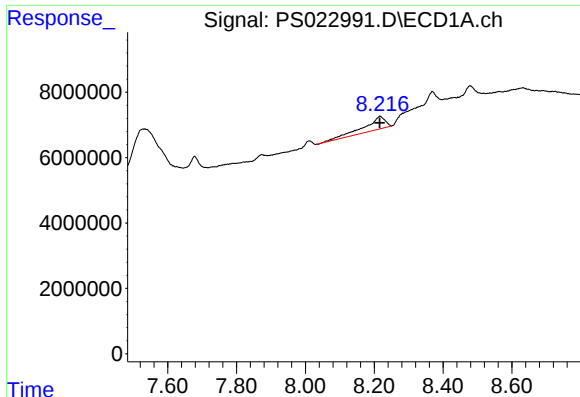

#11 2,4,5-TP (SILVEX)


R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 16854542
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

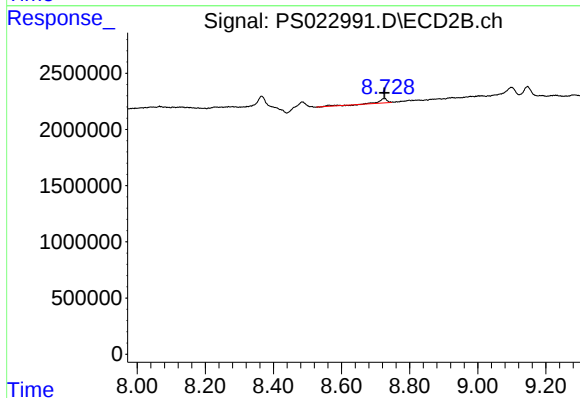


#11 2,4,5-TP (SILVEX)

R.T.: 8.727 min
Delta R.T.: 0.002 min
Response: 732160
Conc: N.D.

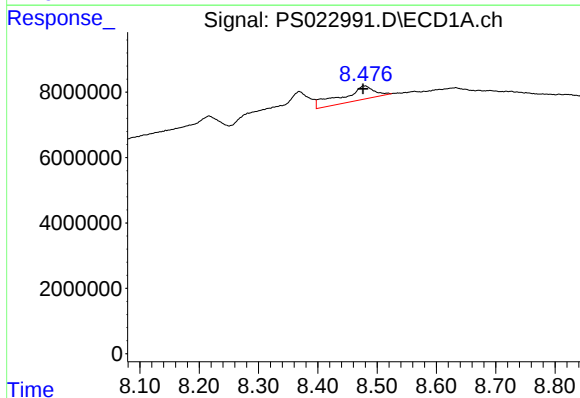


#12 2,4,5-T

R.T.: 8.479 min
Delta R.T.: 0.002 min
Response: 16382821
Conc: 1.42 ng/ml

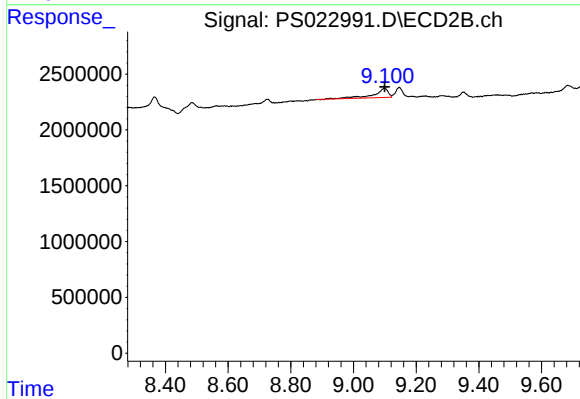

#12 2,4,5-T


R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 2694783
Conc: N.D.

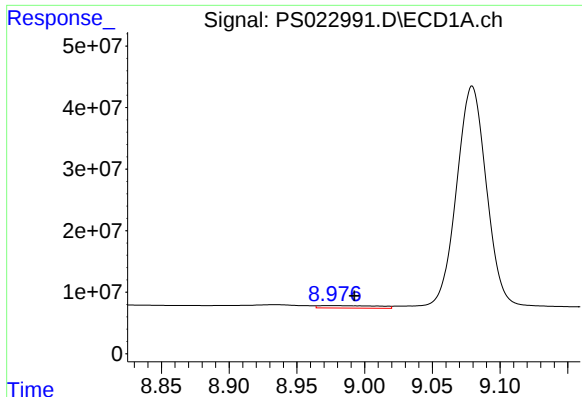

#13 2,4-DB


R.T.: 8.975 min
Delta R.T.: -0.017 min
Response: 12569582
Conc: 5.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

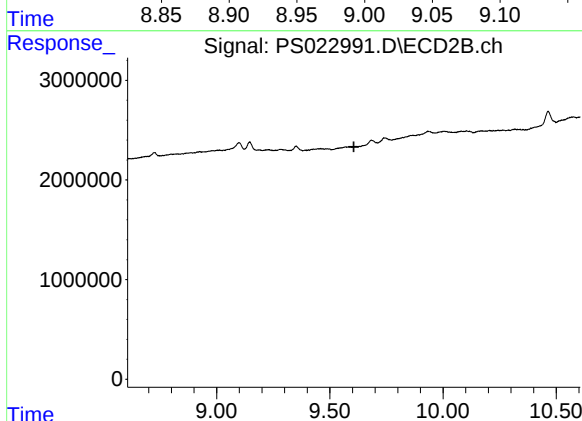


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

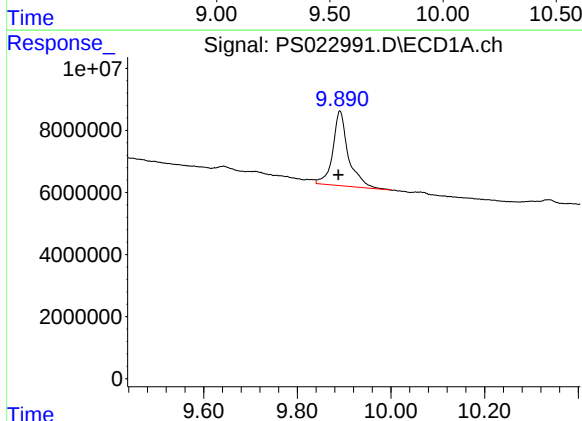


#15 Picloram

R.T.: 9.891 min
Delta R.T.: 0.003 min
Response: 53623700
Conc: 3.13 ng/ml

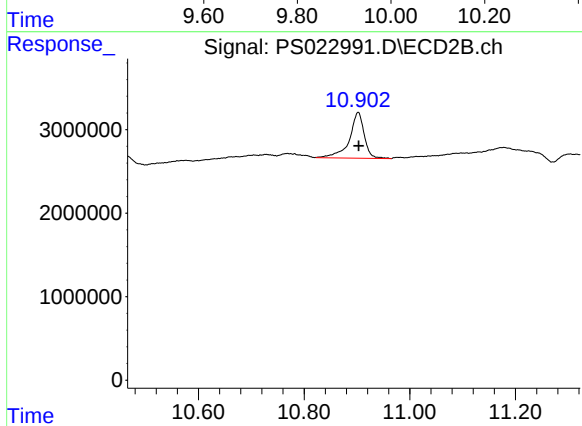

#15 Picloram


R.T.: 10.902 min
Delta R.T.: -0.001 min
Response: 10711420
Conc: 2.52 ng/ml

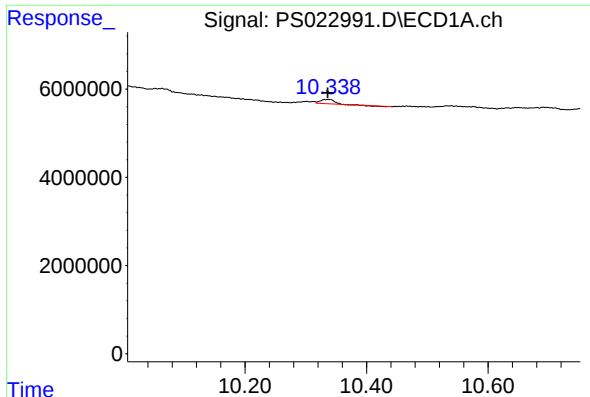

#16 DCPA

R.T.: 10.336 min
Delta R.T.: 0.000 min
Response: 1302814
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

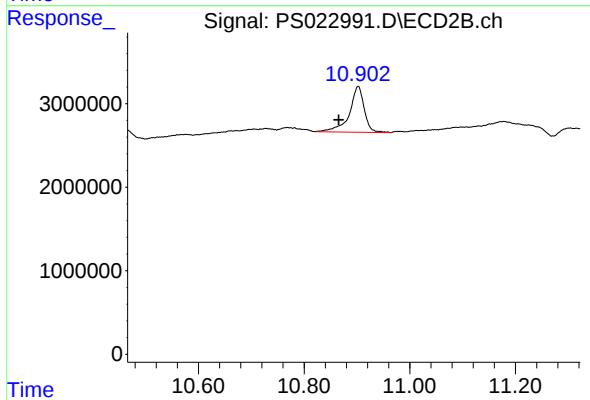

#16 DCPA

R.T.: 10.902 min
Delta R.T.: 0.037 min
Response: 10711420
Conc: 2.87 ng/ml